
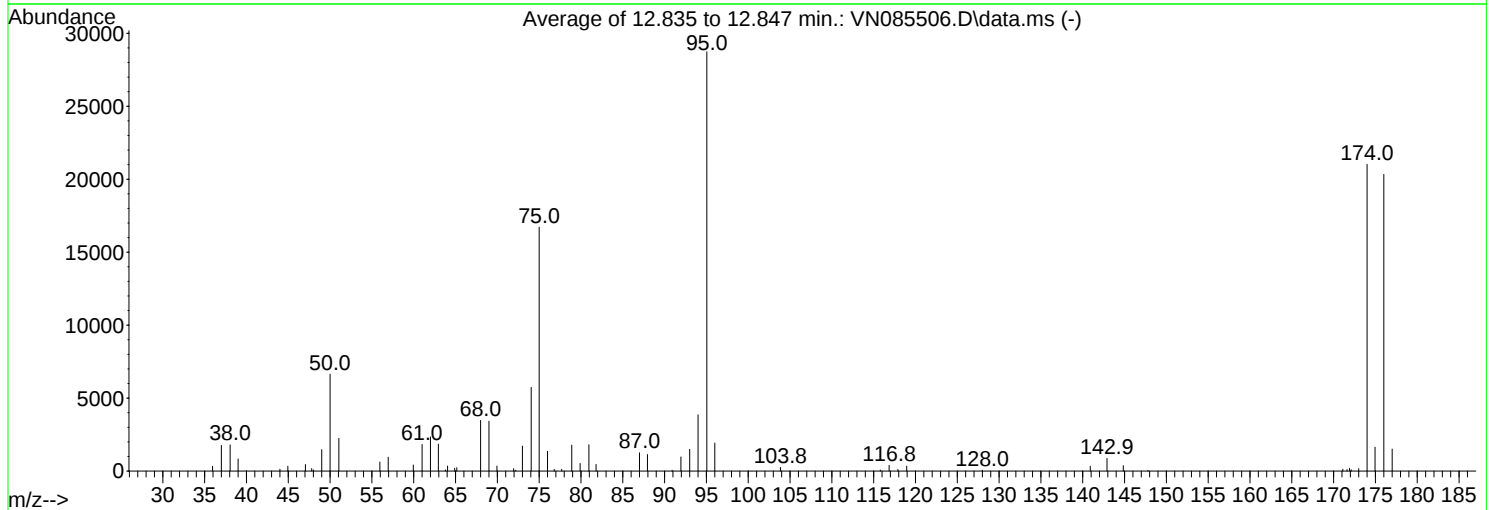


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012125\
Data File : VN085506.D
Acq On : 21 Jan 2025 10:13
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
Title : SW846 8260
Last Update : Wed Jan 15 02:16:08 2025

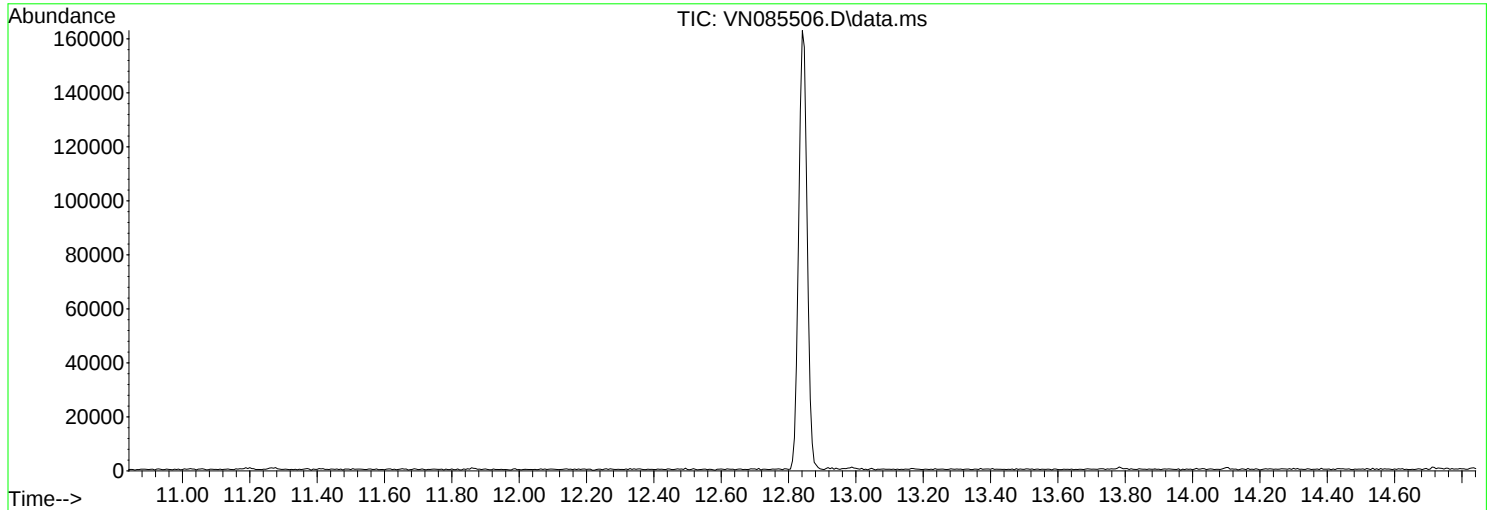

AutoFind: Scans 1850, 1851, 1852; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	6638	PASS
75	95	30	60	58.1	16709	PASS
95	95	100	100	100.0	28736	PASS
96	95	5	9	6.7	1922	PASS
173	174	0.00	2	0.8	163	PASS
174	95	50	100	73.2	21027	PASS
175	174	5	9	7.8	1638	PASS
176	174	95	101	96.7	20328	PASS
177	176	5	9	7.4	1505	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	330	50.00	6638	65.15	233	77.70	123
37.00	1760	51.05	2241	68.00	3469	78.90	1780
38.05	1797	55.95	624	69.00	3420	79.90	522
39.00	828	56.95	953	69.95	342	80.95	1808
40.00	12	59.95	419	71.95	165	81.80	462
44.00	128	61.00	1822	72.20	57	87.00	1253
44.95	330	62.00	2345	73.00	1714	87.95	1131
47.05	451	62.95	1849	74.05	5732	90.90	57
47.80	170	63.80	81	75.00	16709	91.95	966
48.00	78	64.05	348	76.00	1358	93.00	1490
49.00	1472	64.90	186	76.80	118	94.00	3856

Average of 12.835 to 12.847 min.: VN085506.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.05	28736	147.80	50				
96.00	1922	171.10	128				
103.85	251	171.60	102				
115.80	73	171.90	188				
116.85	400	172.10	91				
117.90	113	173.00	163				
118.95	336	174.00	21027				
128.00	58	174.95	1638				
140.90	337	176.00	20328				
142.90	867	177.00	1505				
144.85	375						

Instrument :

MSVOA_N

ClientSampleId :

BFB