


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN012220\
Data File : VN059820.D
Acq On : 22 Jan 2020 9:12
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011320W.M
Title : SW846 8260
Last Update : Sat Jan 18 03:09:32 2020

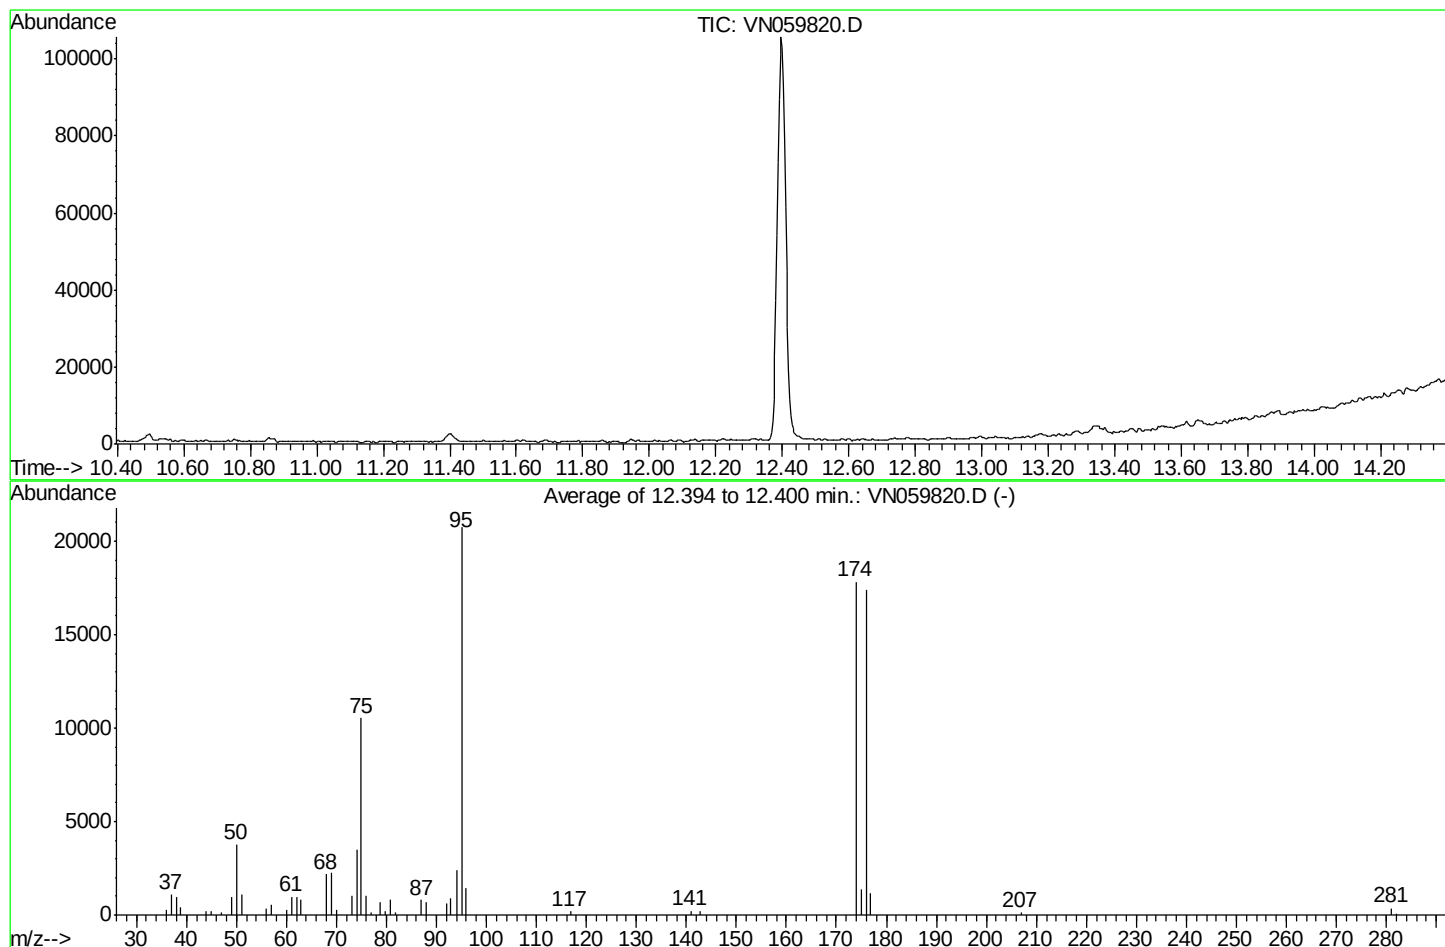

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	3739	PASS
75	95	30	60	50.7	10520	PASS
95	95	100	100	100.0	20738	PASS
96	95	5	9	7.0	1451	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	85.9	17808	PASS
175	174	5	9	7.9	1403	PASS
176	174	95	101	97.5	17362	PASS
177	176	5	9	6.8	1177	PASS