

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012224\
 Data File : VN080746.D
 Acq On : 22 Jan 2024 19:21
 Operator : JC\MD
 Sample : P1179-13 50X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 S-6

Quant Time: Jan 23 03:58:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011024W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 11 06:34:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	124509	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	296628	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	302150	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	122070	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	100788	46.095	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	92.200%
35) Dibromofluoromethane	8.165	113	84045	49.867	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.740%
50) Toluene-d8	10.565	98	338822	52.723	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	105.440%
62) 4-Bromofluorobenzene	12.853	95	133909	54.338	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	108.680%
Target Compounds						
					Qvalue	
40) Benzene	8.606	78	395273	40.728	ug/l	100
52) Toluene	10.629	92	131437	23.637	ug/l	100
68) m/p-Xylenes	12.071	106	20453	4.615	ug/l	85
69) o-Xylene	12.400	106	12831	2.961	ug/l	93
95) Naphthalene	15.641	128	70673	8.309	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012224\
Data File : VN080746.D
Acq On : 22 Jan 2024 19:21
Operator : JC\MD
Sample : P1179-13 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
S-6

Quant Time: Jan 23 03:58:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011024W.M
Quant Title : SW846 8260
QLast Update : Thu Jan 11 06:34:36 2024
Response via : Initial Calibration




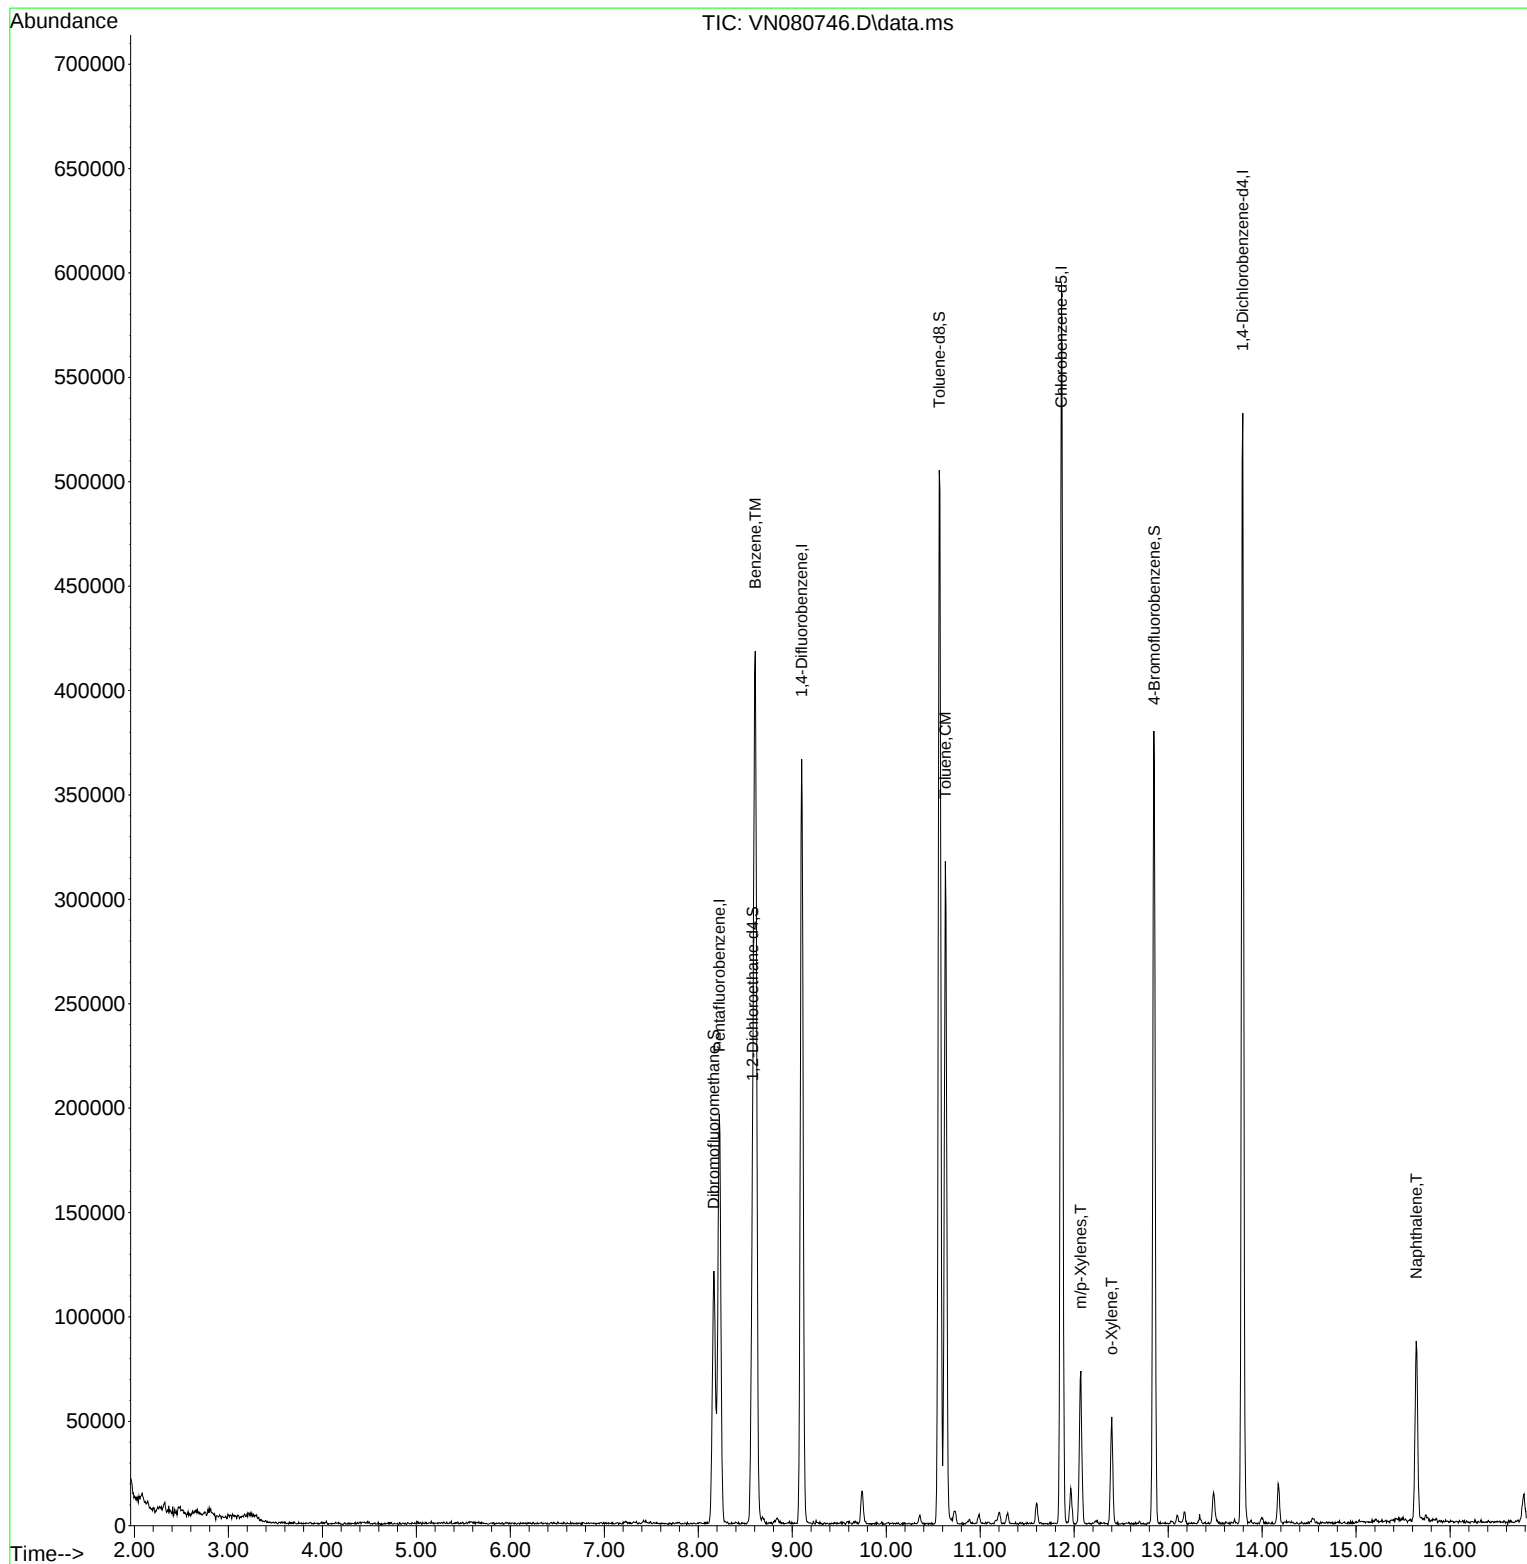


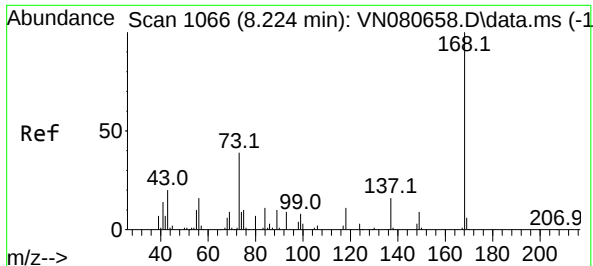

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN080746.D
Acq: 22 Jan 2024 19:21




Instrument :
MSVOA_N
ClientSampleId :
S-6


Tgt Ion:168 Resp: 124509
Ion Ratio Lower Upper
168 100
99 65.9 53.0 79.6

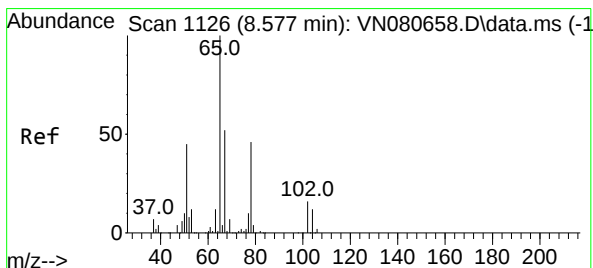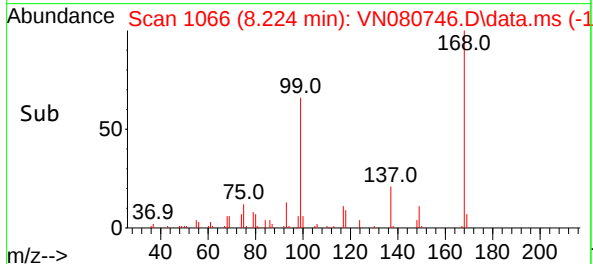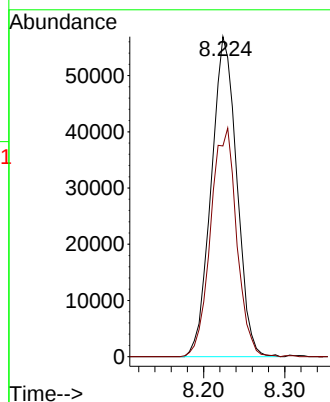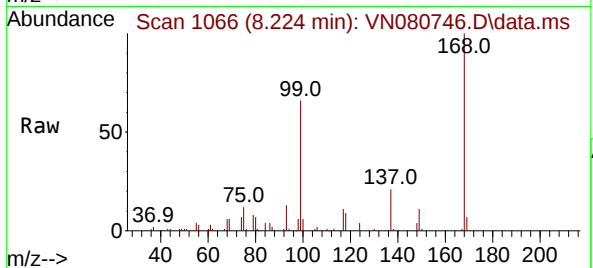

#33
1,2-Dichloroethane-d4
Concen: 46.095 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.000 min
Lab File: VN080746.D
Acq: 22 Jan 2024 19:21

Tgt Ion: 65 Resp: 100788
Ion Ratio Lower Upper
65 100
67 53.6 0.0 106.6

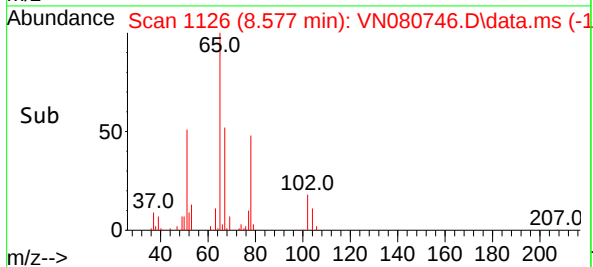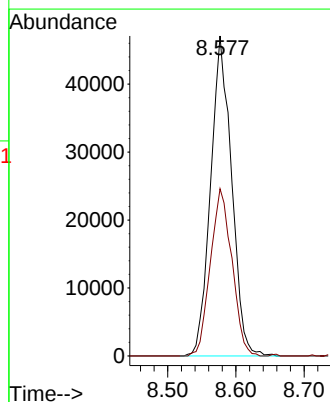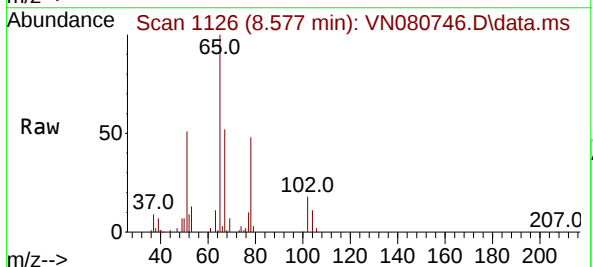

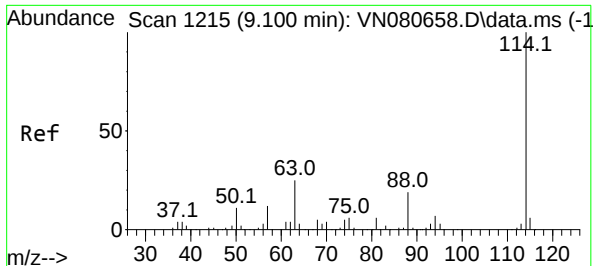

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 11

Delta R.T. 0.000 min

Lab File: VN080746.D

Acq: 22 Jan 2024 19:21

Instrument :

MSVOA_N

ClientSampleId :

S-6





Tgt Ion:114 Resp: 296628

Ion Ratio Lower Upper

114 100

63 26.1 0.0 36.4

88 17.9 0.0 30.6

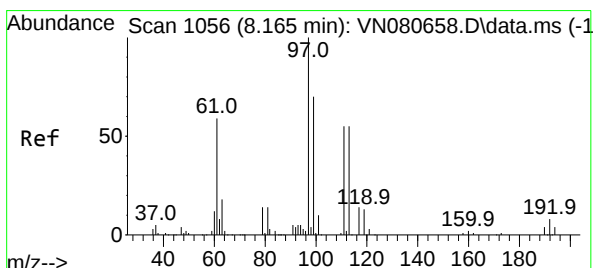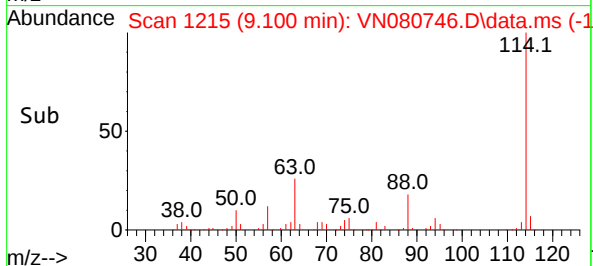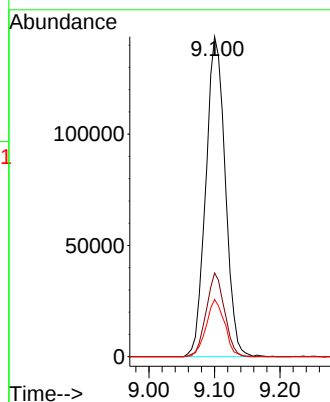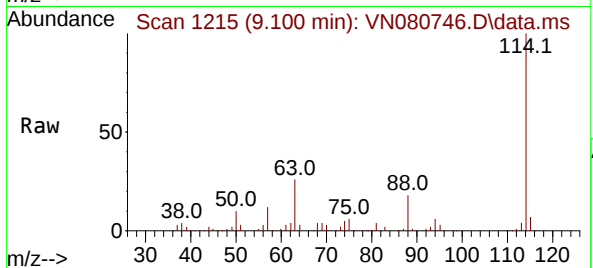

#35

Dibromofluoromethane

Concen: 49.867 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.000 min

Lab File: VN080746.D

Acq: 22 Jan 2024 19:21




Tgt Ion:113 Resp: 84045


Ion Ratio Lower Upper

113 100

111 104.7 82.6 123.8

192 15.5 12.7 19.1


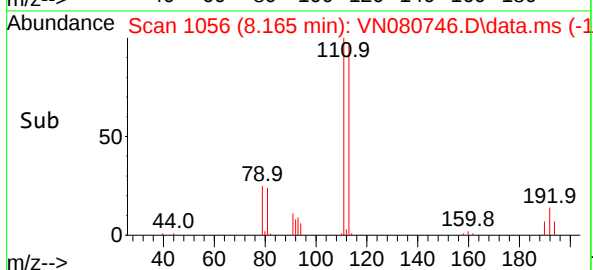
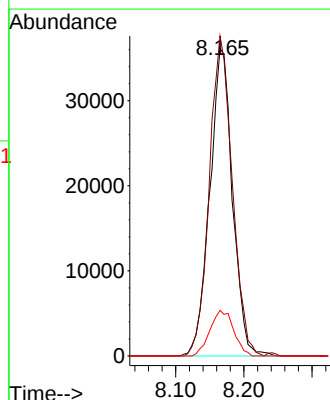
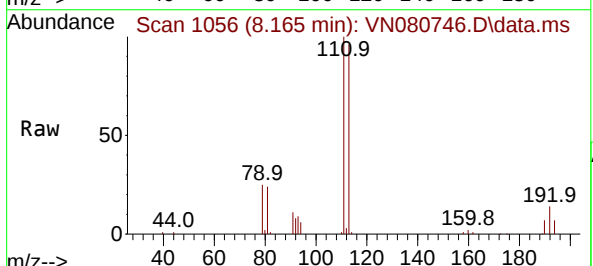


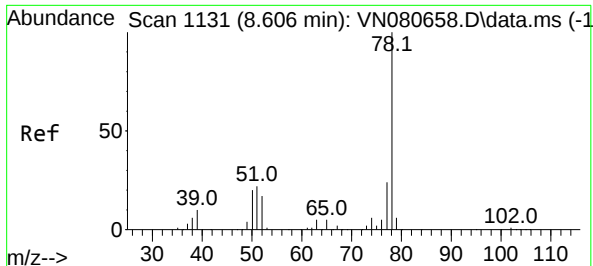

#40
Benzene
Concen: 40.728 ug/l
RT: 8.606 min Scan# 1131
Delta R.T. 0.000 min
Lab File: VN080746.D
Acq: 22 Jan 2024 19:21




Instrument :
MSVOA_N
ClientSampleId :
S-6


Tgt Ion: 78 Resp: 395273
Ion Ratio Lower Upper
78 100
77 23.8 19.0 28.6

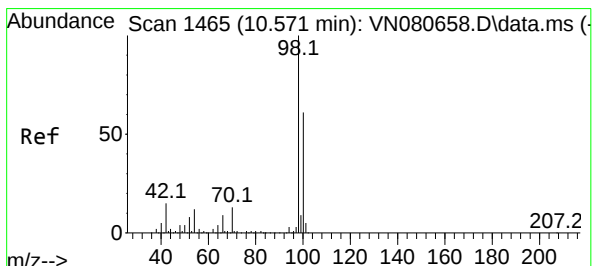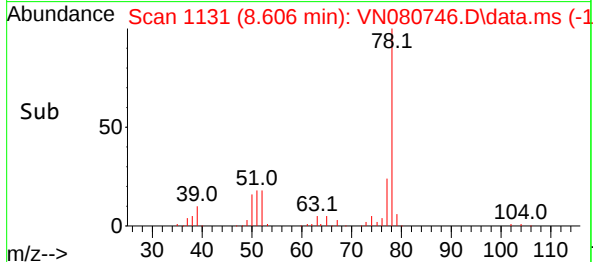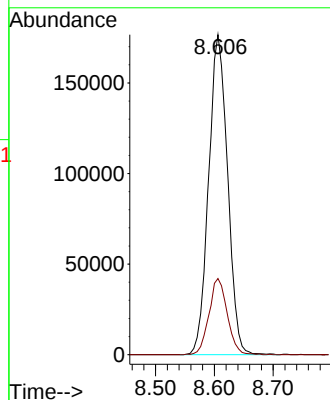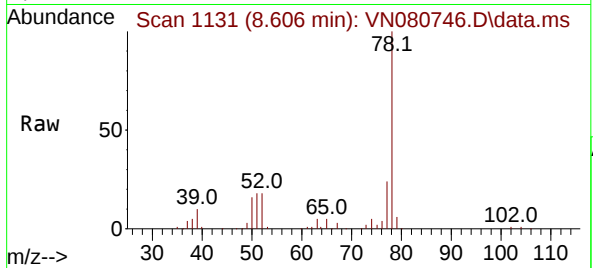

#50
Toluene-d8
Concen: 52.723 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.006 min
Lab File: VN080746.D
Acq: 22 Jan 2024 19:21

Tgt Ion: 98 Resp: 338822
Ion Ratio Lower Upper
98 100
100 65.5 52.0 78.0

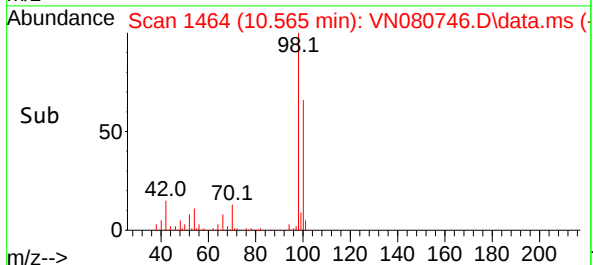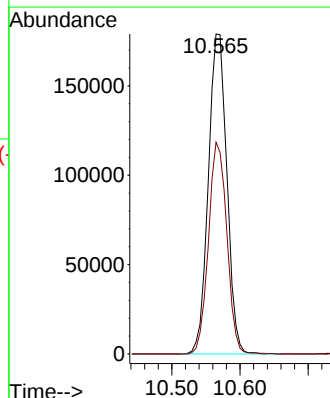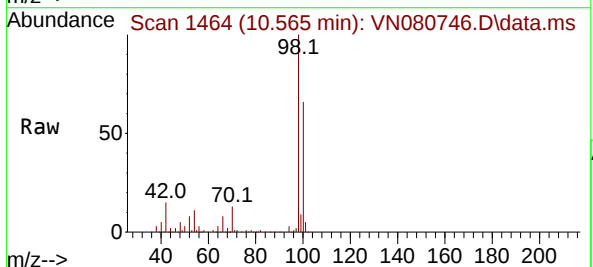

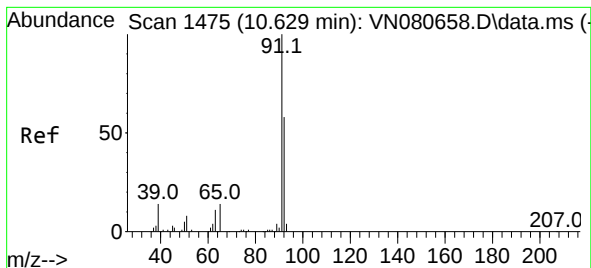

#52

Toluene

Concen: 23.637 ug/l

RT: 10.629 min Scan# 1475

Delta R.T. 0.000 min

Lab File: VN080746.D

Acq: 22 Jan 2024 19:21

Instrument :

MSVOA_N

ClientSampleId :





S-6

Tgt Ion: 92 Resp: 131437

Ion Ratio Lower Upper

92 100

91 171.6 137.4 206.0

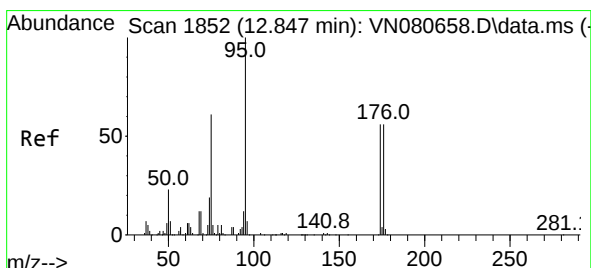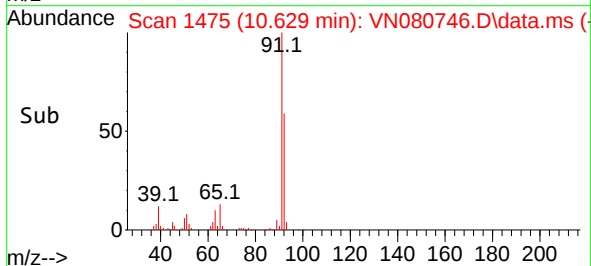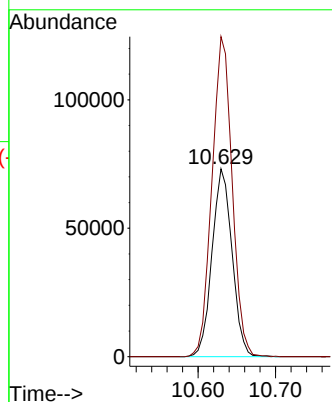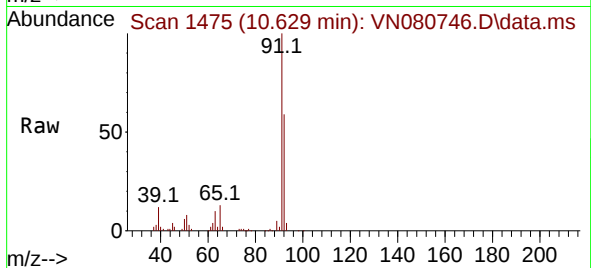

#62

4-Bromofluorobenzene

Concen: 54.338 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. 0.006 min

Lab File: VN080746.D

Acq: 22 Jan 2024 19:21




Tgt Ion: 95 Resp: 133909


Ion Ratio Lower Upper

95 100

174 61.8 0.0 143.8

176 58.6 0.0 135.8


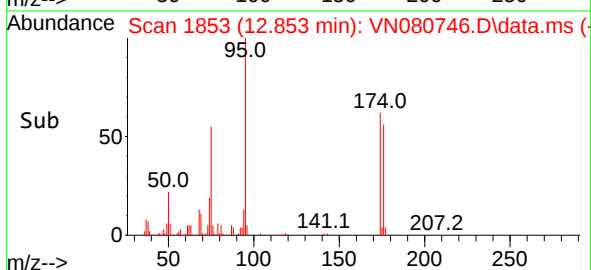
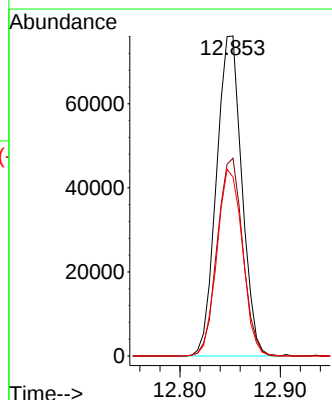
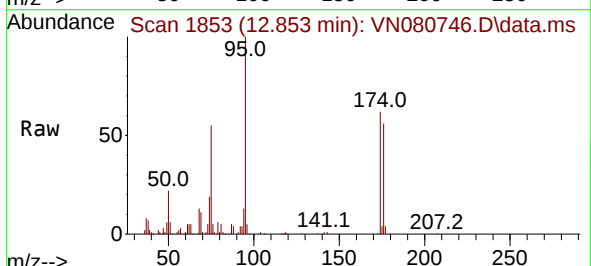


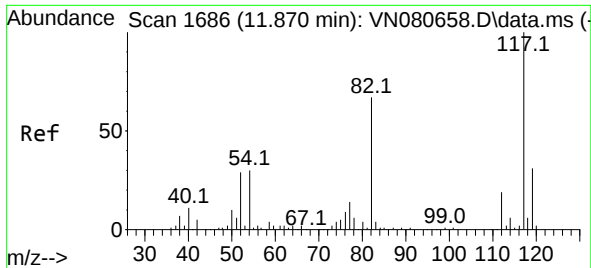

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN080746.D
Acq: 22 Jan 2024 19:21




Instrument :
MSVOA_N
ClientSampleId :
S-6


Tgt Ion:117 Resp: 302150
Ion Ratio Lower Upper
117 100
82 64.4 44.0 66.0
119 33.6 25.6 38.4

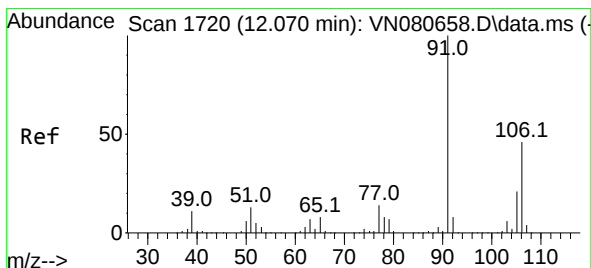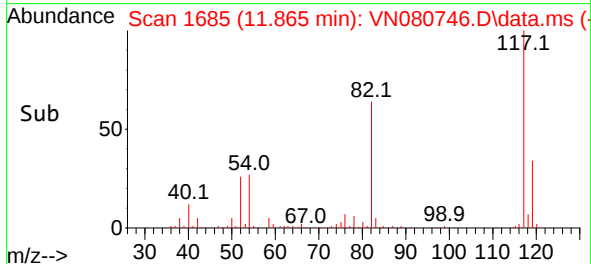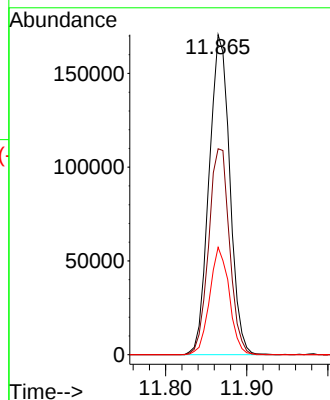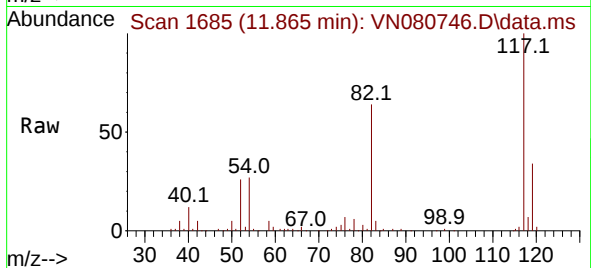

#68
m/p-Xylenes
Concen: 4.615 ug/l
RT: 12.071 min Scan# 1720
Delta R.T. 0.000 min
Lab File: VN080746.D
Acq: 22 Jan 2024 19:21

Tgt Ion:106 Resp: 20453
Ion Ratio Lower Upper
106 100
91 222.0 159.6 239.4


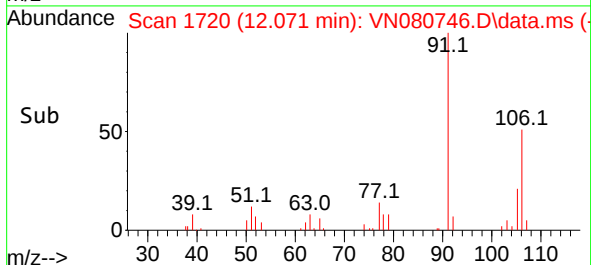
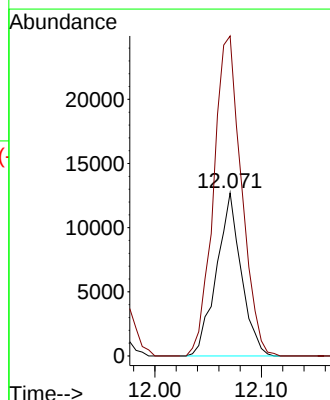
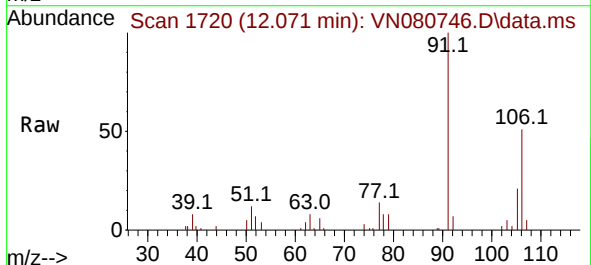


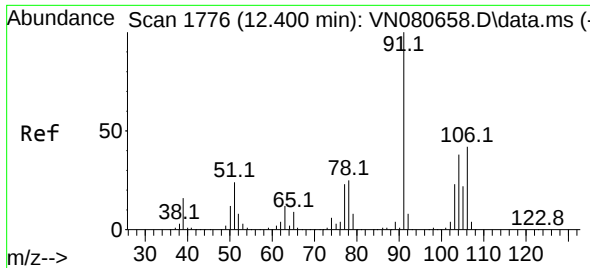

#69
o-Xylene
Concen: 2.961 ug/l
RT: 12.400 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN080746.D
Acq: 22 Jan 2024 19:21




Instrument :
MSVOA_N
ClientSampleId :
S-6


Tgt Ion:106 Resp: 12831
Ion Ratio Lower Upper
106 100
91 221.6 105.2 315.5

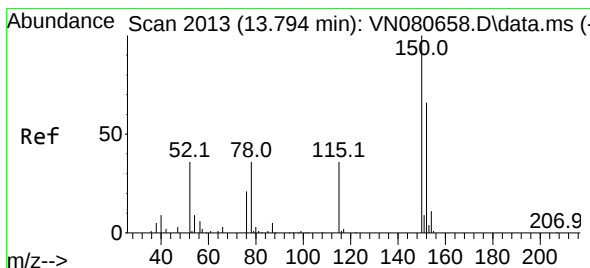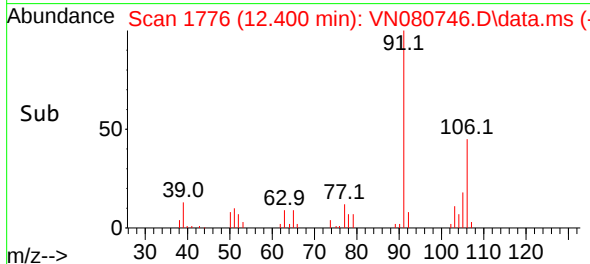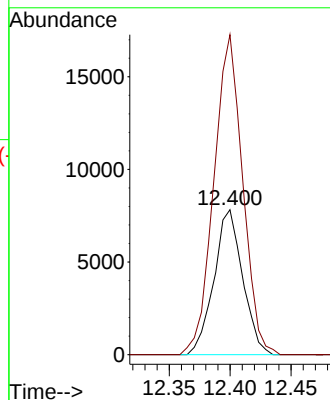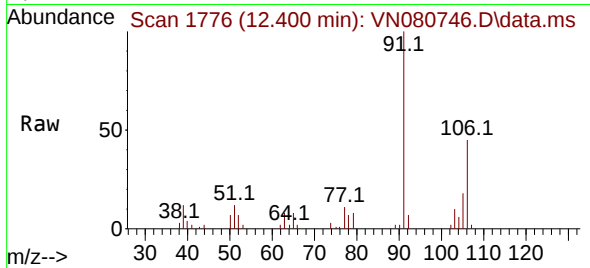

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.000 min
Lab File: VN080746.D
Acq: 22 Jan 2024 19:21

Tgt Ion:152 Resp: 122070
Ion Ratio Lower Upper
152 100
115 68.5 32.3 96.8
150 158.5 0.0 355.8

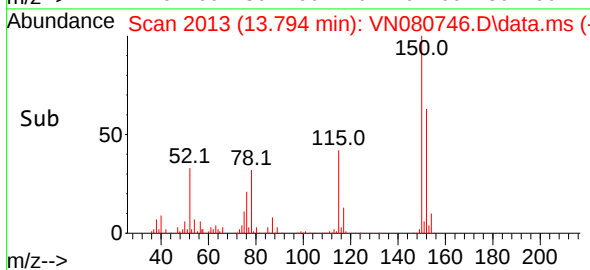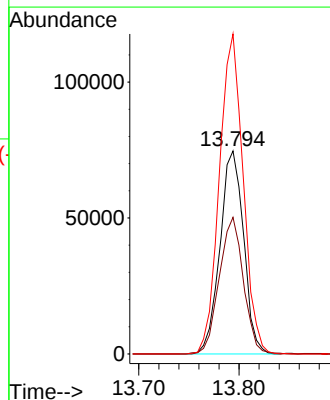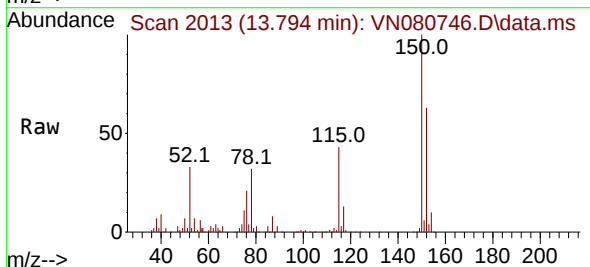

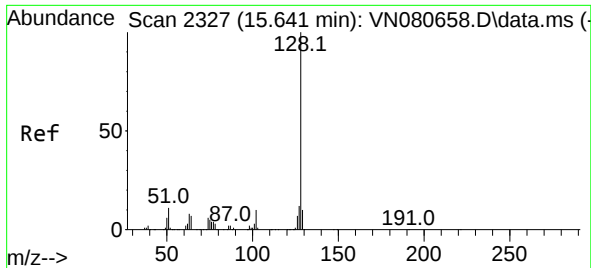

#95
Naphthalene
Concen: 8.309 ug/l
RT: 15.641 min Scan# 21
Delta R.T. 0.000 min
Lab File: VN080746.D
Acq: 22 Jan 2024 19:21

Instrument :
MSVOA_N
ClientSampleId :
S-6

Tgt Ion:128 Resp: 70673
Ion Ratio Lower Upper
128 100
127 13.6 10.0 15.0
129 11.4 8.7 13.1

