
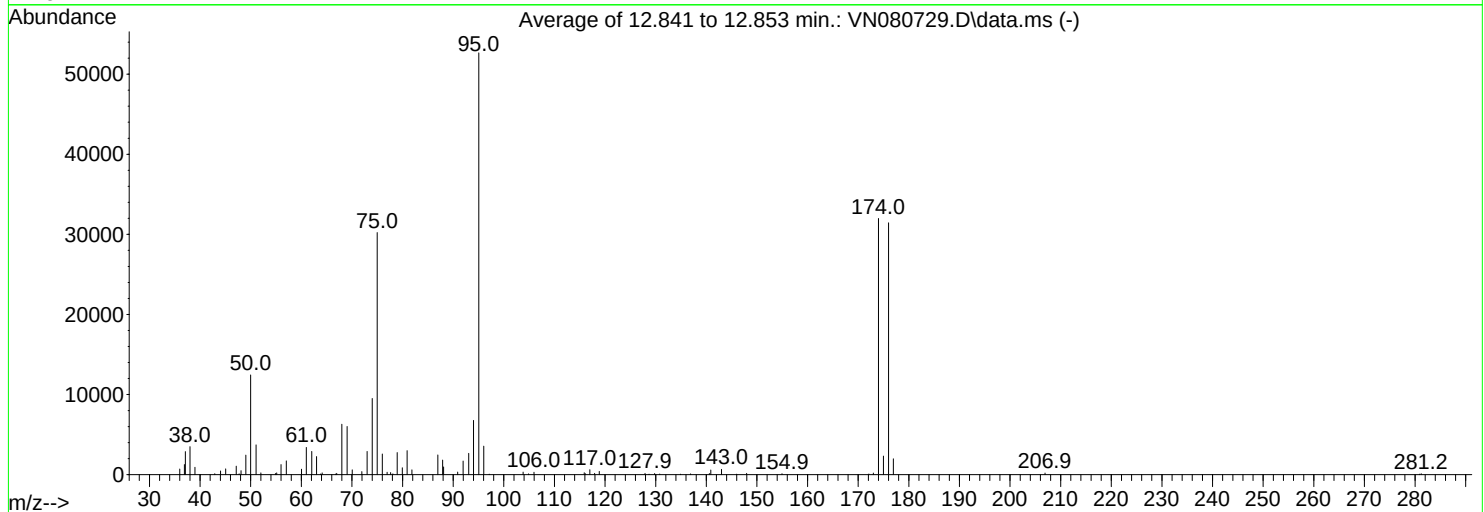


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012224\
Data File : VN080729.D
Acq On : 22 Jan 2024 09:14
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011024W.M
Title : SW846 8260
Last Update : Thu Jan 11 06:34:36 2024

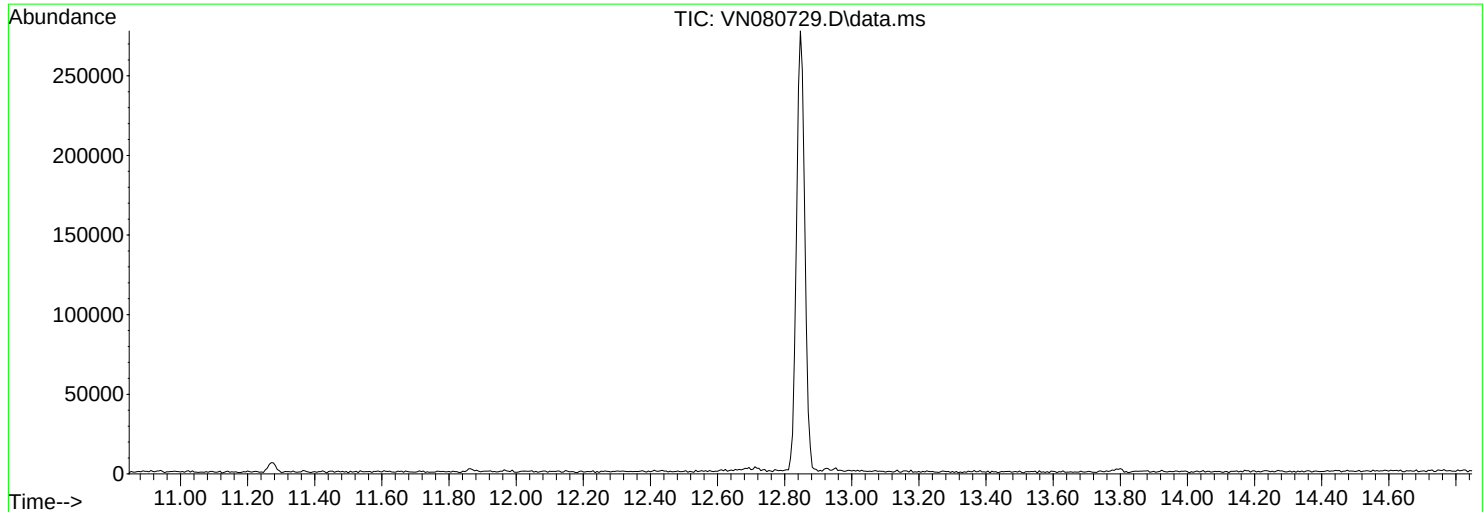

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.6	12450	PASS
75	95	30	60	57.4	30235	PASS
95	95	100	100	100.0	52664	PASS
96	95	5	9	6.8	3560	PASS
173	174	0.00	2	0.6	197	PASS
174	95	50	100	60.7	31984	PASS
175	174	5	9	7.2	2312	PASS
176	174	95	101	98.3	31440	PASS
177	176	5	9	6.3	1978	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	706	48.10	511	62.05	2904	74.00	951
36.90	1269	49.05	2433	63.00	2259	75.00	3023
37.10	2872	50.00	12450	63.80	80	76.00	258
38.00	3500	51.05	3721	64.10	218	76.95	30
39.00	915	52.00	228	66.80	72	77.65	267
40.00	12	54.90	141	67.00	156	78.10	95
42.90	113	55.15	223	68.00	6284	78.95	2764
44.05	460	56.00	1251	69.05	6020	79.95	856
45.05	725	57.05	1717	70.05	594	80.90	2990
47.15	1060	60.05	673	71.95	378	81.85	608
47.70	106	61.00	3400	73.00	2900	86.95	2458

Average of 12.841 to 12.853 min.: VN080729.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.90	1811	105.95	299	136.90	111	176.00	31440
88.10	956	115.90	243	140.60	136	176.95	1978
90.90	316	116.10	122	140.90	578	206.90	195
91.95	1691	117.00	624	143.00	669	280.90	71
93.05	2652	117.95	171	146.00	63	281.20	130
94.00	6780	118.85	397	147.95	167		
95.05	52664	127.90	165	154.95	119		
96.05	3560	128.70	59	172.10	76		
97.10	64	129.80	137	173.00	197		
103.80	331	130.80	74	174.00	31984		
104.90	92	134.90	64	175.00	2312		

Instrument :

MSVOA_N

ClientSampleId :

BFB