



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012323\
Data File : VN076354.D
Acq On : 23 Jan 2023 09:44
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Title : SW846 8260
Last Update : Tue Jan 17 03:59:22 2023

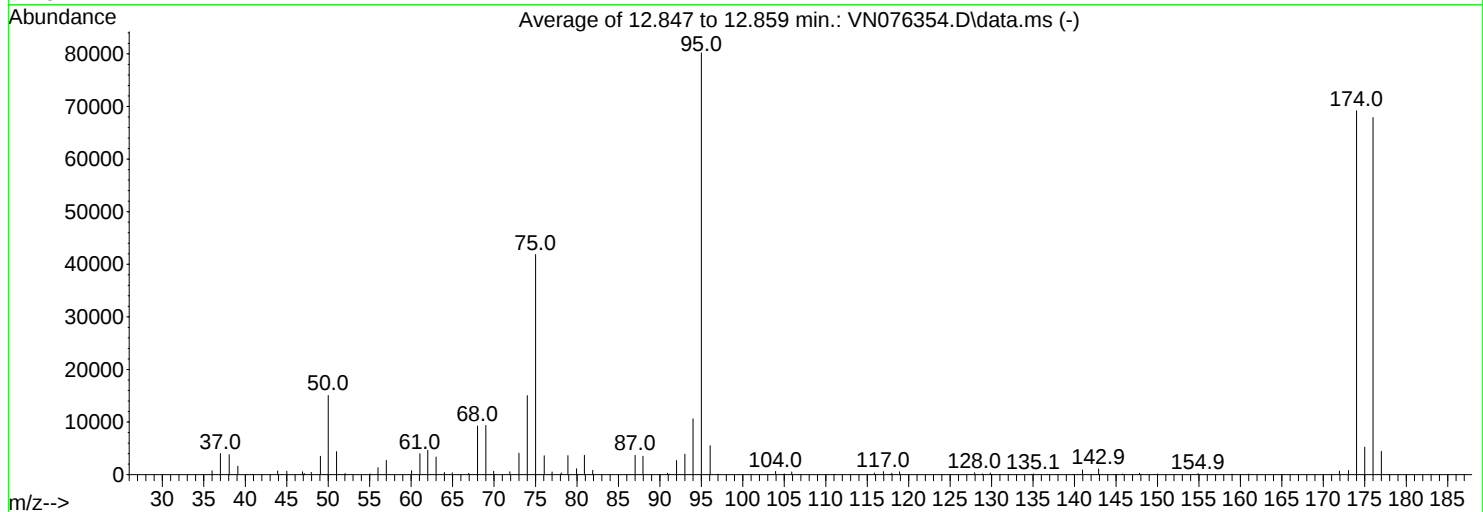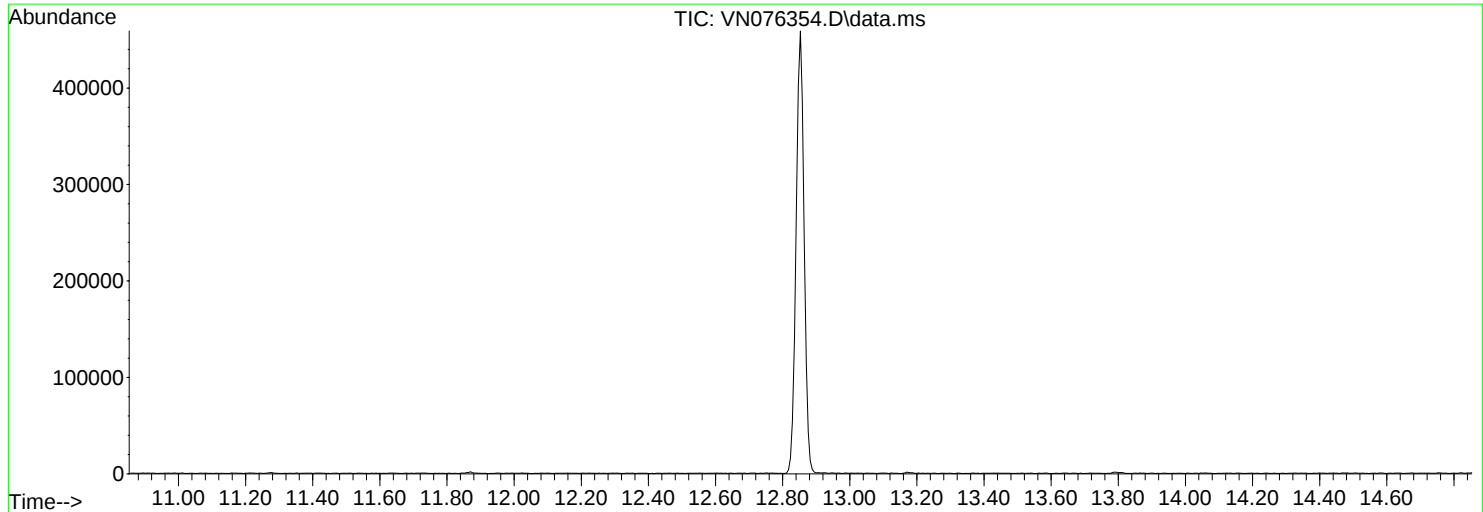

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	15072	PASS
75	95	30	60	52.2	41859	PASS
95	95	100	100	100.0	80203	PASS
96	95	5	9	6.9	5523	PASS
173	174	0.00	2	1.1	792	PASS
174	95	50	100	86.3	69195	PASS
175	174	5	9	7.6	5238	PASS
176	174	95	101	98.1	67901	PASS
177	176	5	9	6.5	4444	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	730	49.05	3510	64.00	426	77.00	531
37.00	4015	50.00	15072	64.95	364	78.10	344
38.05	3793	51.00	4385	66.95	237	78.90	361
39.10	1612	52.05	208	68.00	9242	79.95	112
40.20	77	55.05	169	69.00	9383	80.90	3685
40.90	54	56.00	1342	69.95	633	81.90	821
43.90	699	57.00	2722	71.90	537	86.00	75
45.00	686	60.05	763	73.00	4081	87.00	3694
46.90	542	61.05	3976	74.00	15021	87.95	3502
47.10	220	62.00	4637	75.00	41859	90.90	272
47.95	426	63.00	3358	76.05	3579	91.10	128

Average of 12.847 to 12.859 min.: VN076354.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.00	2683	115.85	323	139.90	61	171.00	51
93.00	3907	116.95	583	140.95	888	171.95	670
94.00	10632	117.80	79	142.90	1101	173.05	792
95.00	80203	117.95	274	145.00	75	174.00	69195
96.05	5523	118.90	554	145.80	114	175.00	5238
97.00	98	127.95	374	147.85	272	176.00	67901
103.95	604	128.90	148	150.00	153	177.00	4444
105.00	156	129.85	308	154.90	209	177.90	55
105.90	524	134.80	69	157.00	53		
111.10	57	135.05	162	159.00	90		
113.00	52	136.70	56	161.00	121		

Instrument :

MSVOA_N

ClientSampleId :

BFB