

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012324\
 Data File : VN080759.D
 Acq On : 23 Jan 2024 13:48
 Operator : JC\MD
 Sample : P1183-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MR-305-0-2

Quant Time: Jan 24 01:59:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011024W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 11 06:34:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	117328	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	280951	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	296274	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	121729	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	97345	47.246	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	94.500%		
35) Dibromofluoromethane	8.165	113	75692	47.417	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	94.840%		
50) Toluene-d8	10.571	98	321475	52.815	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	105.640%		
62) 4-Bromofluorobenzene	12.853	95	126157	54.049	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	108.100%		
Target Compounds						
					Qvalue	
3) Chloromethane	2.365	50	2331	0.433	ug/l #	81
6) Chloroethane	3.124	64	128	Below Cal	#	43
11) Tert butyl alcohol	5.489	59	272	0.781	ug/l #	69
13) Acrolein	4.236	56	61	0.210	ug/l #	1
16) Acetone	4.430	43	17560	25.959	ug/l	95
18) Methyl Acetate	5.018	43	3184	1.581	ug/l	98
20) Methylene Chloride	5.277	84	6982	3.536	ug/l #	86
25) 2-Butanone	7.483	43	9466	7.742	ug/l #	76
29) Tetrahydrofuran	7.841	42	1007	1.222	ug/l #	50
31) Cyclohexane	8.224	56	3958	1.243	ug/l #	17
36) 1,1-Dichloropropene	8.218	75	12779	3.908	ug/l #	49
37) Ethyl Acetate	7.559	43	4574	1.443	ug/l #	66
38) Carbon Tetrachloride	8.224	117	13741	4.680	ug/l #	16
41) Methacrylonitrile	7.841	41	554	0.301	ug/l #	29
42) 1,2-Dichloroethane	8.688	62	825	0.234	ug/l #	73
43) Isopropyl Acetate	8.688	43	117960	20.239	ug/l #	81
45) 1,2-Dichloropropane	9.741	63	1203	0.494	ug/l #	45
48) Methyl methacrylate	9.671	41	3594	1.302	ug/l #	31
51) 4-Methyl-2-Pentanone	10.447	43	5002	1.591	ug/l	93
52) Toluene	10.635	92	2248	0.427	ug/l	85
53) t-1,3-Dichloropropene	10.735	75	772	0.203	ug/l #	43
54) cis-1,3-Dichloropropene	10.359	75	40326	10.011	ug/l #	69
56) Ethyl methacrylate	10.982	69	1064	0.293	ug/l #	1
57) 1,3-Dichloropropane	11.200	76	4086	1.104	ug/l #	42
59) 2-Hexanone	11.171	43	117436	50.593	ug/l #	19
71) Bromoform	12.841	173	439	0.278	ug/l #	1
74) N-amyl acetate	12.482	43	2797	0.403	ug/l #	36
76) 1,2,3-Trichloropropane	12.847	75	73661	19.624	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.847	75	73661	46.262	ug/l #	15
92) 1,2-Dibromo-3-Chloropr...	14.570	75	61	Below Cal	#	19
95) Naphthalene	15.635	128	7168	0.845	ug/l #	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012324\
Data File : VN080759.D
Acq On : 23 Jan 2024 13:48
Operator : JC\MD
Sample : P1183-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MR-305-0-2

Quant Time: Jan 24 01:59:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011024W.M
Quant Title : SW846 8260
QLast Update : Thu Jan 11 06:34:36 2024
Response via : Initial Calibration




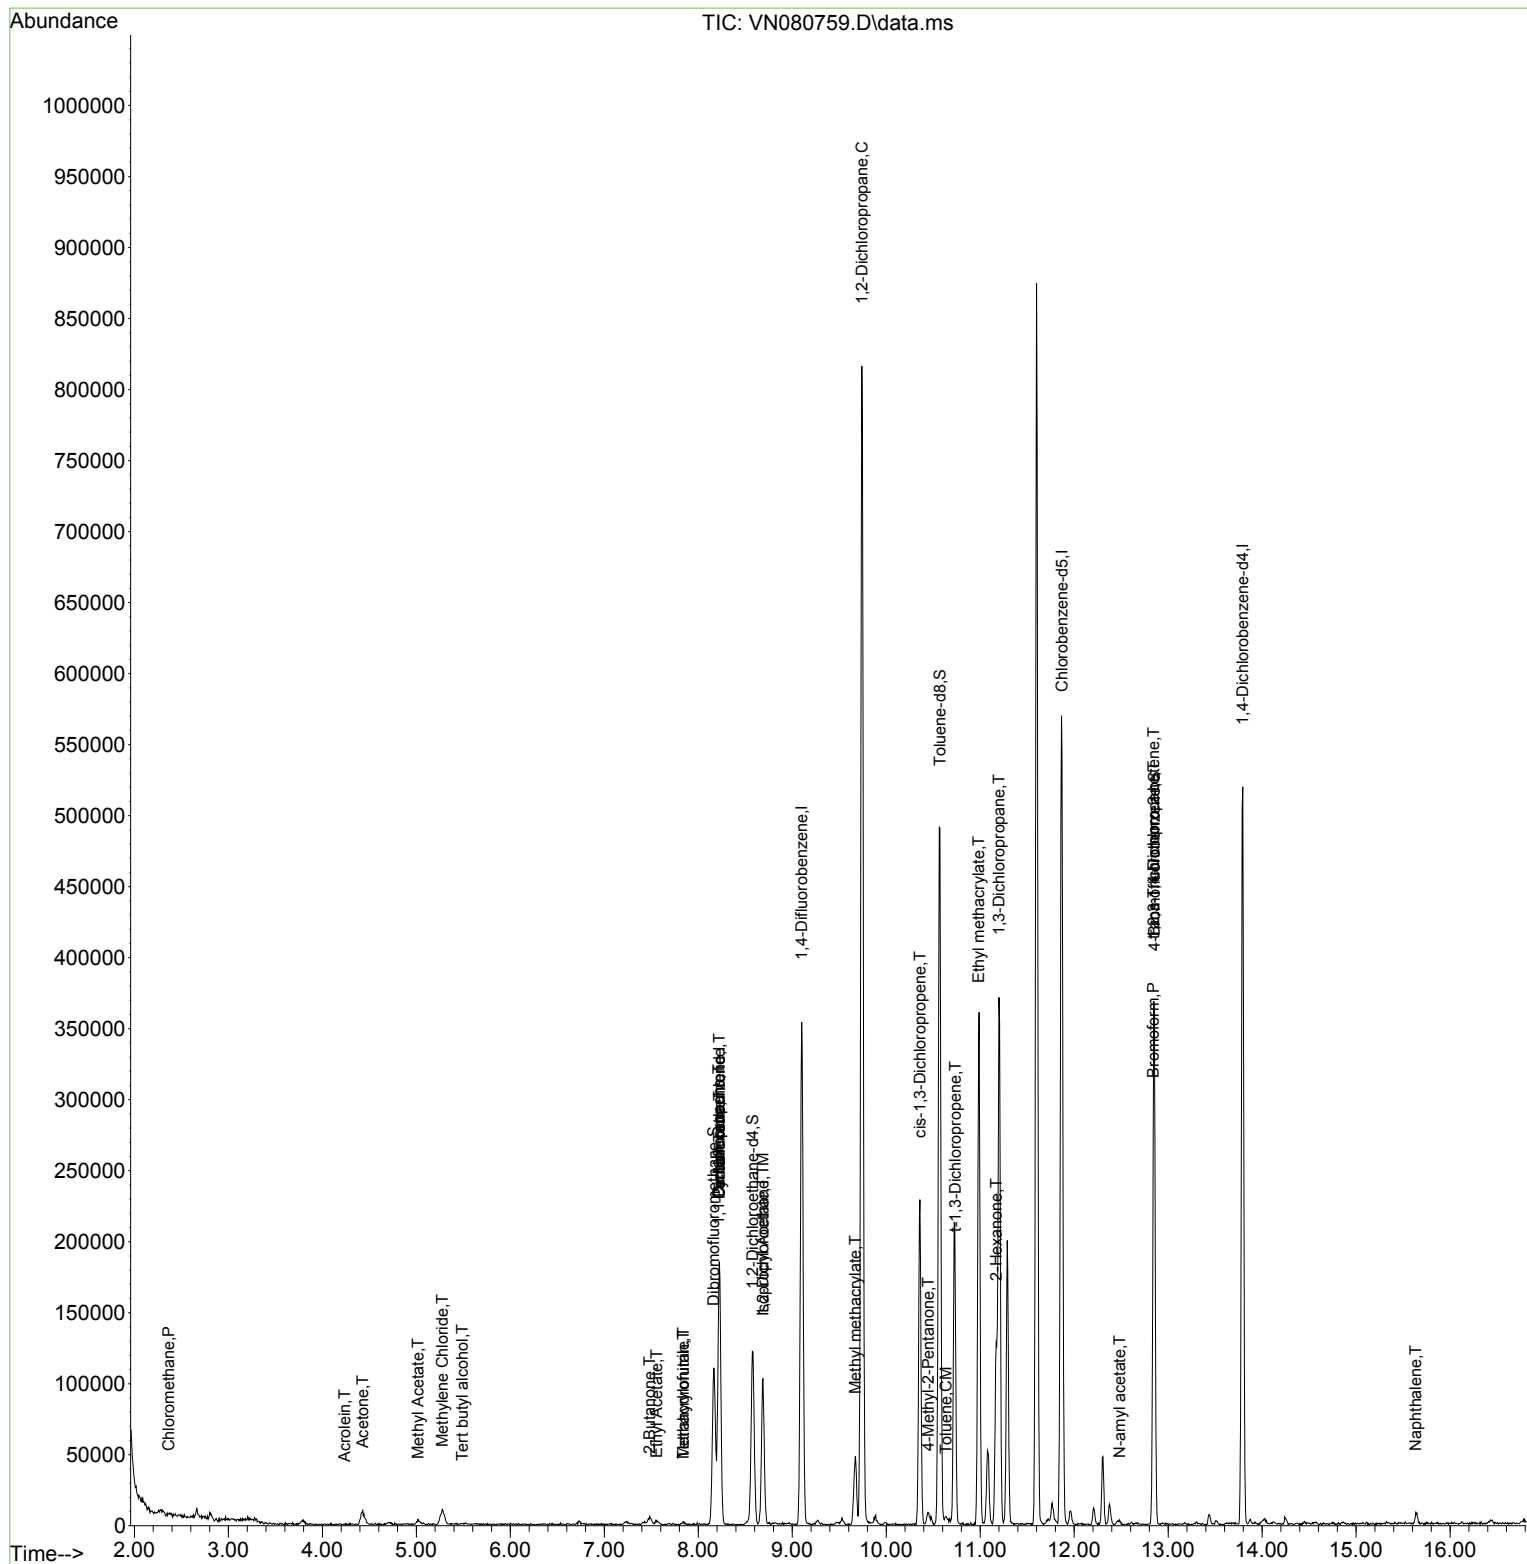




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1
Delta R.T. -0.000 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48




Instrument :
MSVOA_N
ClientSampleId :
MR-305-0-2


Tgt Ion:168 Resp: 117328
Ion Ratio Lower Upper
168 100
99 77.4 53.0 79.6

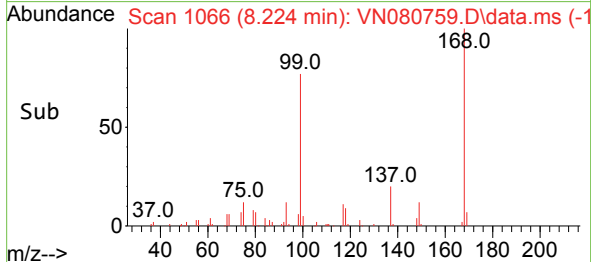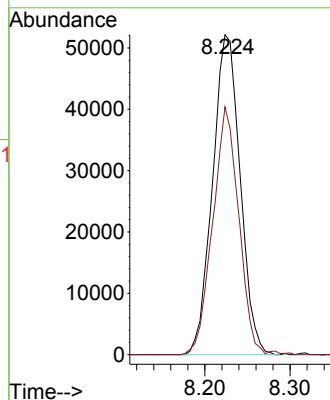

#3
Chloromethane
Concen: 0.433 ug/l
RT: 2.365 min Scan# 70
Delta R.T. 0.006 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48

Tgt Ion: 50 Resp: 2331
Ion Ratio Lower Upper
50 100
52 44.0 26.5 39.7#



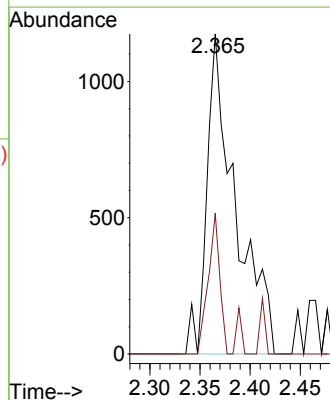
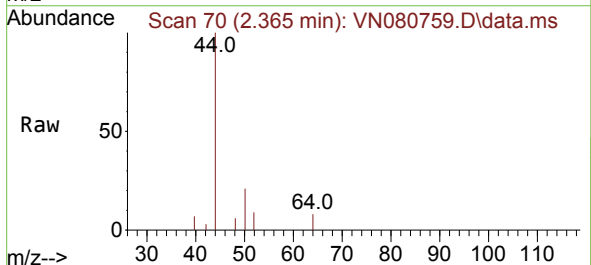




#11
Tert butyl alcohol
Concen: 0.781 ug/l
RT: 5.489 min Scan# 605
Delta R.T. -0.023 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48




Instrument :
MSVOA_N
ClientSampleId :
MR-305-0-2


Tgt Ion: 59 Resp: 272
Ion Ratio Lower Upper
59 100
57 21.7 8.2 12.4#



#13
Acrolein
Concen: 0.210 ug/l
RT: 4.236 min Scan# 388
Delta R.T. 0.065 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48

Tgt Ion: 56 Resp: 61
Ion Ratio Lower Upper
56 100
55 260.7 54.5 81.7#

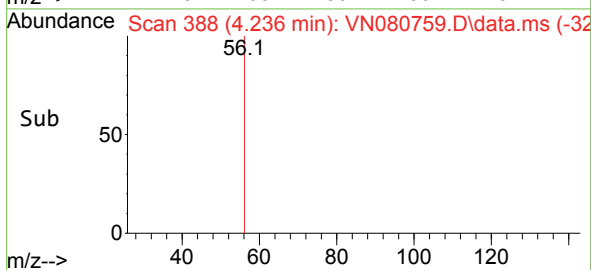



#16

Acetone

Concen: 25.959 ug/l

RT: 4.430 min Scan# 41

Delta R.T. 0.006 min

Lab File: VN080759.D

Acq: 23 Jan 2024 13:48

Instrument :

MSVOA_N

ClientSampleId :





MR-305-0-2

Tgt Ion: 43 Resp: 17560

Ion Ratio Lower Upper

43 100

58 37.7 28.0 42.0

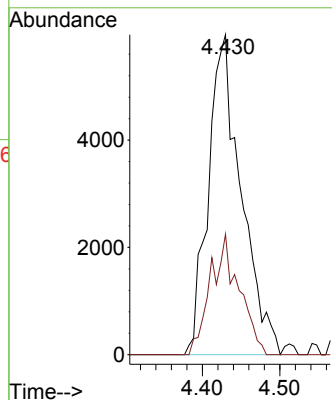

#18

Methyl Acetate

Concen: 1.581 ug/l

RT: 5.018 min Scan# 521

Delta R.T. -0.000 min

Lab File: VN080759.D




Acq: 23 Jan 2024 13:48


Tgt Ion: 43 Resp: 3184

Ion Ratio Lower Upper

43 100

74 31.4 26.2 39.4



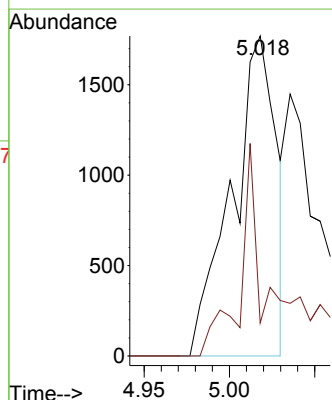





#20
Methylene Chloride
Concen: 3.536 ug/l
RT: 5.277 min Scan# 51
Delta R.T. 0.006 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48




Instrument :
MSVOA_N
ClientSampleId :
MR-305-0-2


Tgt Ion: 84	Resp: 6982
Ion Ratio	Lower Upper
84 100	
49 109.0	79.7 119.5
51 22.1	25.2 37.8#
86 50.1	53.3 79.9#

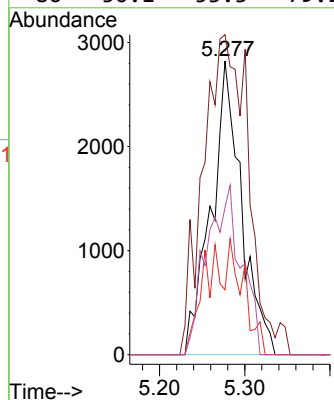

#25
2-Butanone
Concen: 7.742 ug/l
RT: 7.483 min Scan# 940
Delta R.T. 0.006 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48

Tgt Ion: 43	Resp: 9466
Ion Ratio	Lower Upper
43 100	
72 23.0	30.2 45.2#

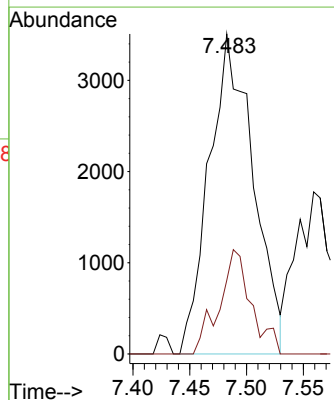



#29

Tetrahydrofuran

Concen: 1.222 ug/l

RT: 7.841 min Scan# 1000

Delta R.T. 0.006 min

Lab File: VN080759.D

Acq: 23 Jan 2024 13:48

Instrument :

MSVOA_N

ClientSampleId :

MR-305-0-2





Tgt Ion: 42 Resp: 1007

Ion Ratio Lower Upper

42 100

72 25.5 49.8 74.6#

71 20.5 47.4 71.2#

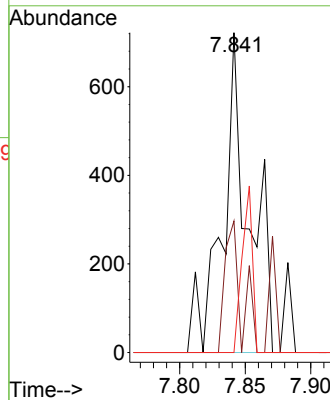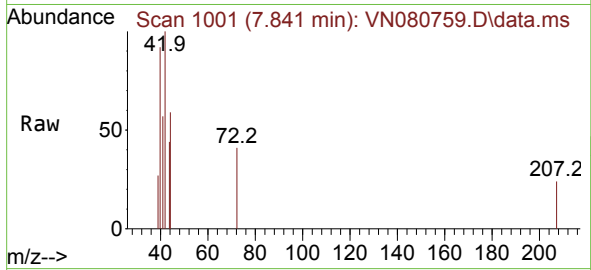

#31

Cyclohexane

Concen: 1.243 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.035 min

Lab File: VN080759.D

Acq: 23 Jan 2024 13:48




Tgt Ion: 56 Resp: 3958


Ion Ratio Lower Upper

56 100

69 181.5 26.8 40.2#

84 128.1 81.8 122.6#

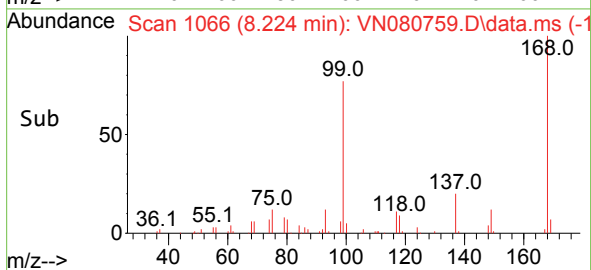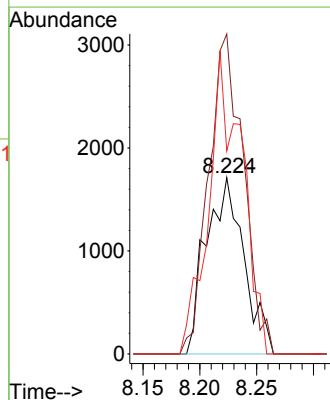



#33

1,2-Dichloroethane-d4

Concen: 47.246 ug/l

RT: 8.577 min Scan# 1126

Delta R.T. -0.000 min

Lab File: VN080759.D

Acq: 23 Jan 2024 13:48

Instrument :

MSVOA_N

ClientSampleId :





MR-305-0-2

Tgt Ion: 65 Resp: 97345

Ion Ratio Lower Upper

65 100

67 53.0 0.0 106.6

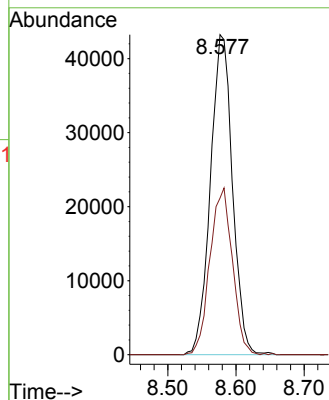

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1215

Delta R.T. 0.000 min

Lab File: VN080759.D

Acq: 23 Jan 2024 13:48




Tgt Ion: 114 Resp: 280951


Ion Ratio Lower Upper

114 100

63 24.5 0.0 36.4

88 17.2 0.0 30.6



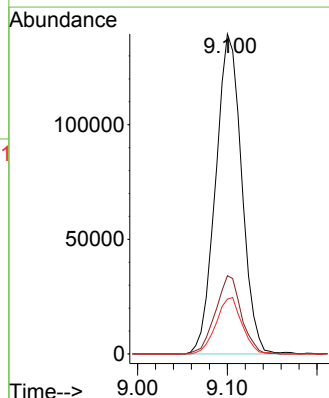





#35
Dibromofluoromethane
Concen: 47.417 ug/l
RT: 8.165 min Scan# 1056
Delta R.T. 0.000 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48




Instrument :
MSVOA_N
ClientSampleId :
MR-305-0-2


Tgt Ion:113 Resp: 75692
Ion Ratio Lower Upper
113 100
111 106.3 82.6 123.8
192 16.3 12.7 19.1

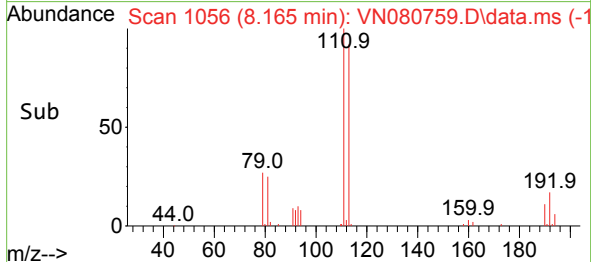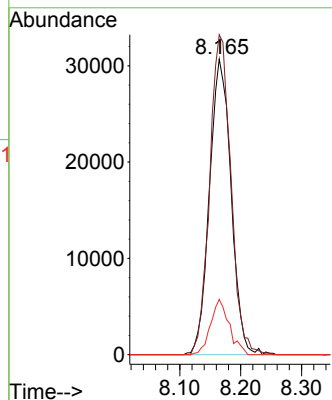

#36
1,1-Dichloropropene
Concen: 3.908 ug/l
RT: 8.218 min Scan# 1065
Delta R.T. -0.159 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48

Tgt Ion: 75 Resp: 12779
Ion Ratio Lower Upper
75 100
110 9.7 19.1 57.3#
77 0.0 25.0 37.4#

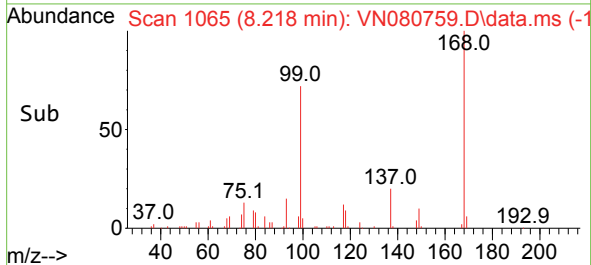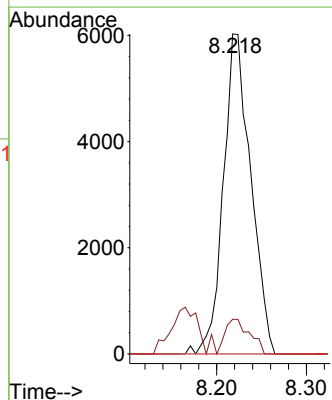



#37

Ethyl Acetate

Concen: 1.443 ug/l

RT: 7.559 min Scan# 91

Delta R.T. 0.006 min

Lab File: VN080759.D

Acq: 23 Jan 2024 13:48

Instrument :

MSVOA_N

ClientSampleId :

MR-305-0-2





Tgt Ion: 43 Resp: 4574

Ion Ratio Lower Upper

43 100

61 0.0 13.2 19.8#

70 2.6 11.3 16.9#

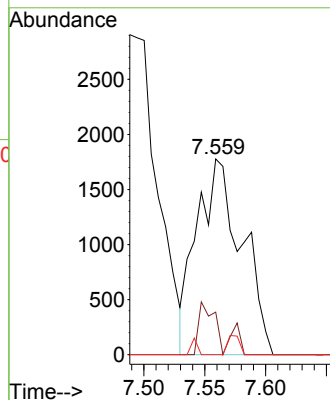

#38

Carbon Tetrachloride

Concen: 4.680 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.141 min

Lab File: VN080759.D

Acq: 23 Jan 2024 13:48




Tgt Ion: 117 Resp: 13741


Ion Ratio Lower Upper

117 100

119 4.9 77.3 115.9#

121 0.0 23.3 34.9#



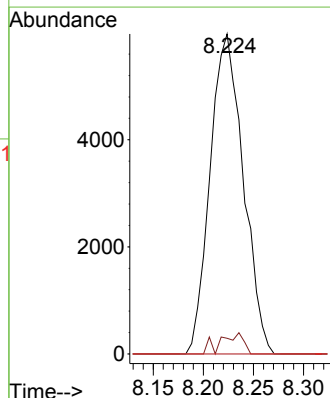





#41
Methacrylonitrile
Concen: 0.301 ug/l
RT: 7.841 min Scan# 1101
Delta R.T. 0.065 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48




Instrument :
MSVOA_N
ClientSampleId :
MR-305-0-2


Tgt Ion:	41	Resp:	554
Ion	Ratio	Lower	Upper
41	100		
39	33.4	42.6	64.0#
67	0.0	77.5	116.3#
52	0.0	28.9	43.3#

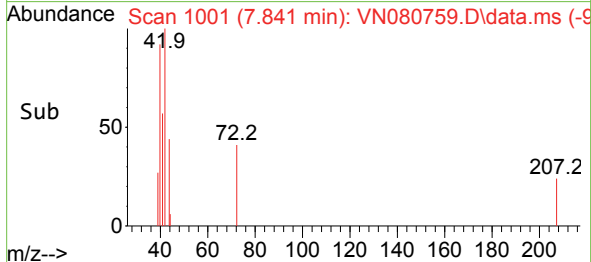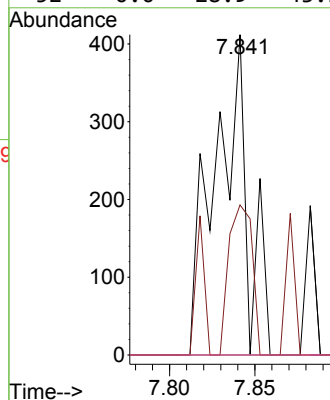

#42
1,2-Dichloroethane
Concen: 0.234 ug/l
RT: 8.688 min Scan# 1145
Delta R.T. 0.018 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48

Tgt Ion:	62	Resp:	825
Ion	Ratio	Lower	Upper
62	100		
98	0.0	0.0	19.8


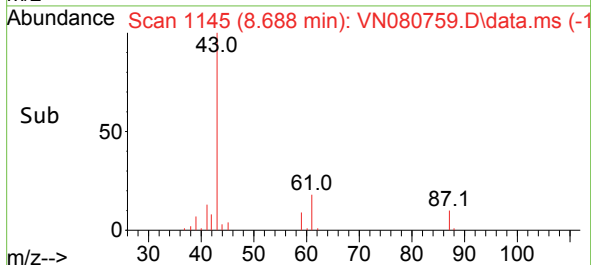
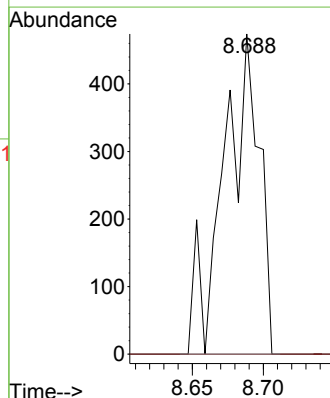
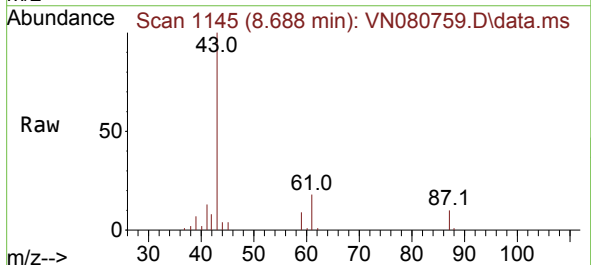




#43
Isopropyl Acetate
Concen: 20.239 ug/l
RT: 8.688 min Scan# 1145
Delta R.T. 0.000 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48




Instrument :
MSVOA_N
ClientSampleId :
MR-305-0-2


Tgt Ion: 43 Resp: 117960
Ion Ratio Lower Upper
43 100
61 18.8 24.7 37.1#
87 11.5 14.6 21.8#

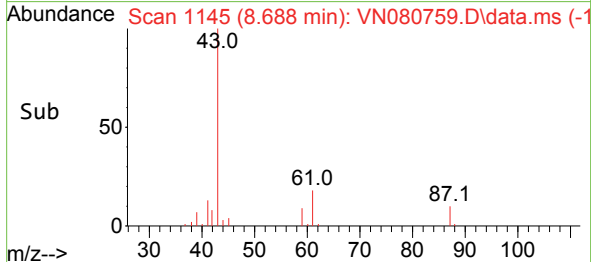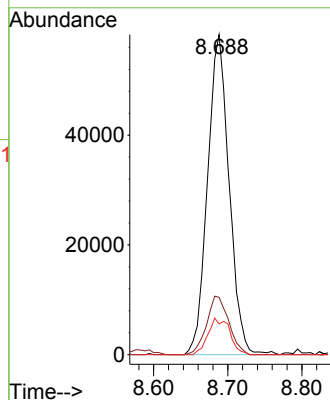

#45
1,2-Dichloropropane
Concen: 0.494 ug/l
RT: 9.741 min Scan# 1324
Delta R.T. 0.118 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48

Tgt Ion: 63 Resp: 1203
Ion Ratio Lower Upper
63 100
65 0.0 23.9 35.9#



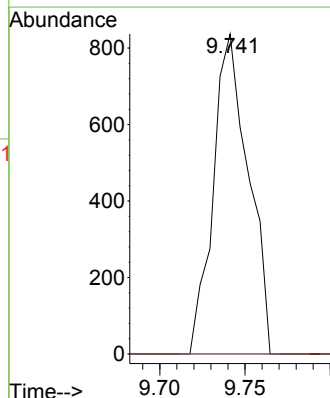





#48
Methyl methacrylate
Concen: 1.302 ug/l
RT: 9.671 min Scan# 11
Delta R.T. -0.012 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48




Instrument :
MSVOA_N
ClientSampleId :
MR-305-0-2


Tgt Ion: 41 Resp: 3594
Ion Ratio Lower Upper
41 100
69 0.0 90.4 135.6#
39 60.4 54.6 81.8

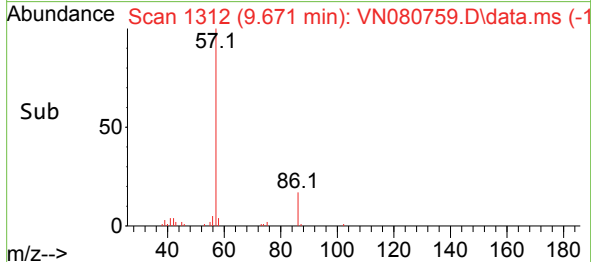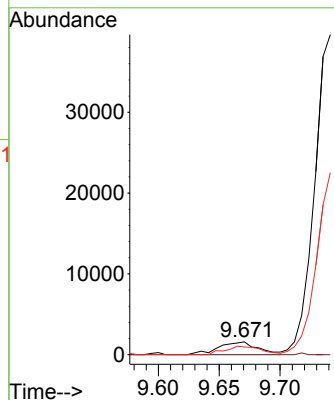

#50
Toluene-d8
Concen: 52.815 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.000 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48

Tgt Ion: 98 Resp: 321475
Ion Ratio Lower Upper
98 100
100 65.8 52.0 78.0

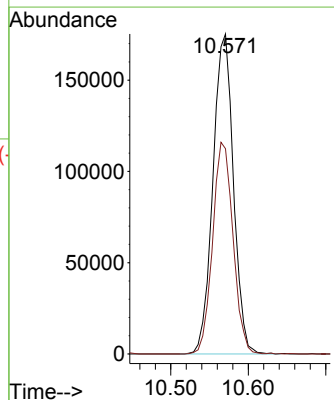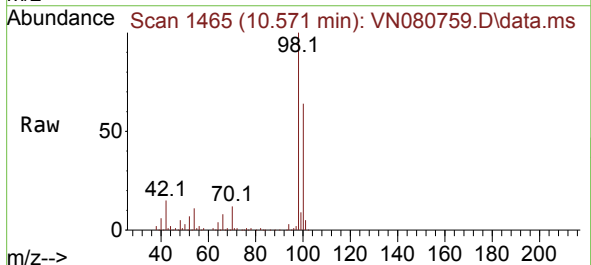

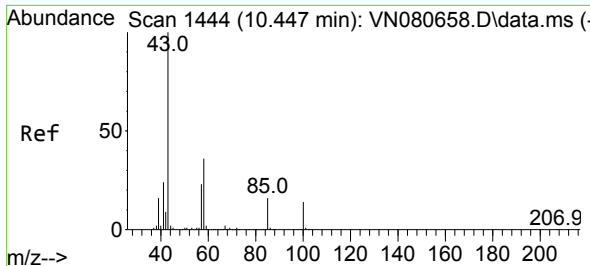

#51

4-Methyl-2-Pentanone

Concen: 1.591 ug/l

RT: 10.447 min Scan# 1444

Delta R.T. 0.000 min

Lab File: VN080759.D

Acq: 23 Jan 2024 13:48

Instrument :

MSVOA_N

ClientSampleId :





MR-305-0-2

Tgt Ion: 43 Resp: 5002

Ion Ratio Lower Upper

43 100

58 50.3 36.6 54.8

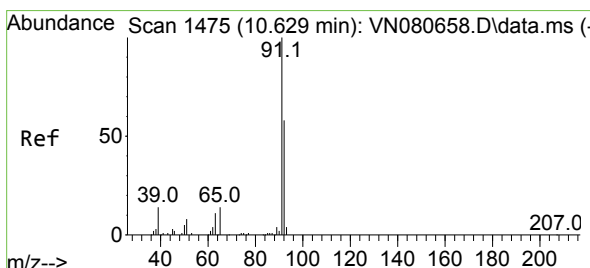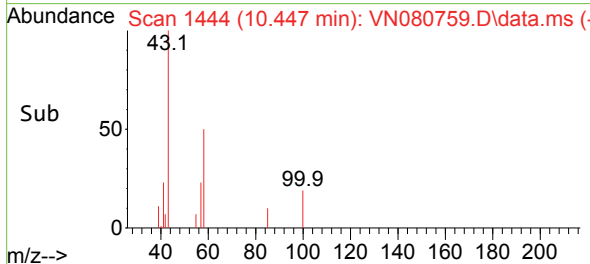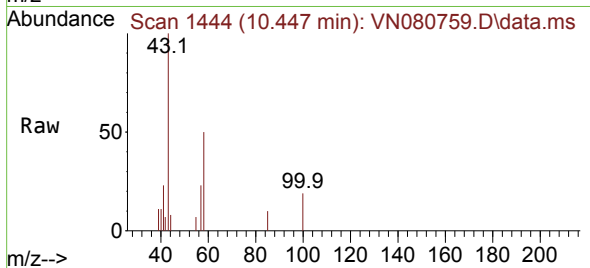

#52

Toluene

Concen: 0.427 ug/l

RT: 10.635 min Scan# 1476

Delta R.T. 0.006 min

Lab File: VN080759.D




Acq: 23 Jan 2024 13:48


Tgt Ion: 92 Resp: 2248

Ion Ratio Lower Upper

92 100

91 150.8 137.4 206.0


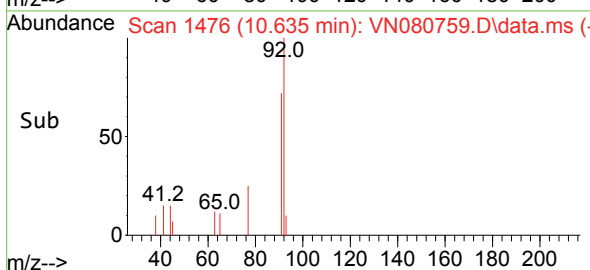
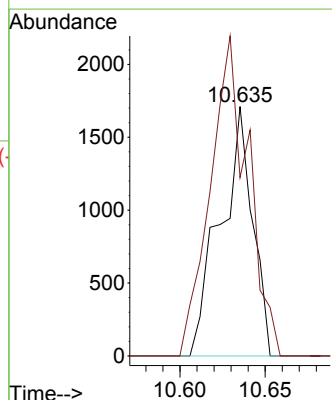
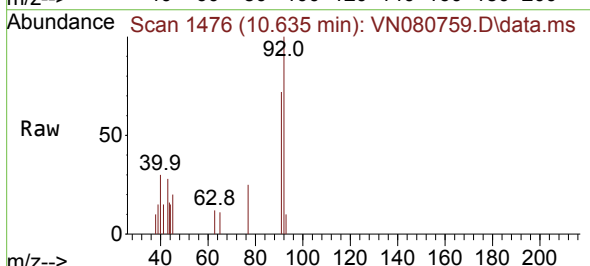




#53
t-1,3-Dichloropropene
Concen: 0.203 ug/l
RT: 10.735 min Scan# 1493
Delta R.T. -0.100 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48




Instrument :
MSVOA_N
ClientSampleId :
MR-305-0-2


Tgt Ion: 75 Resp: 772
Ion Ratio Lower Upper
75 100
77 0.0 25.4 38.0#

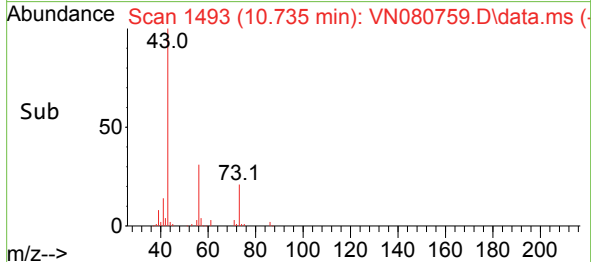

#54
cis-1,3-Dichloropropene
Concen: 10.011 ug/l
RT: 10.359 min Scan# 1429
Delta R.T. 0.047 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48

Tgt Ion: 75 Resp: 40326
Ion Ratio Lower Upper
75 100
77 0.0 26.1 39.1#
39 34.3 31.6 47.4



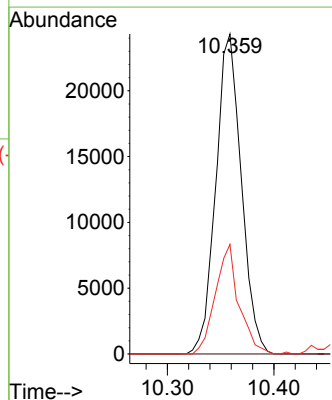





#56
Ethyl methacrylate
Concen: 0.293 ug/l
RT: 10.982 min Scan# 11
Delta R.T. 0.106 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48




Instrument :
MSVOA_N
ClientSampleId :
MR-305-0-2


Tgt Ion: 69 Resp: 1064
Ion Ratio Lower Upper
69 100
41 6279.7 39.6 59.4#
39 2558.3 28.6 43.0#



#57
1,3-Dichloropropane
Concen: 1.104 ug/l
RT: 11.200 min Scan# 1572
Delta R.T. 0.035 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48

Tgt Ion: 76 Resp: 4086
Ion Ratio Lower Upper
76 100
78 0.0 26.1 39.1#


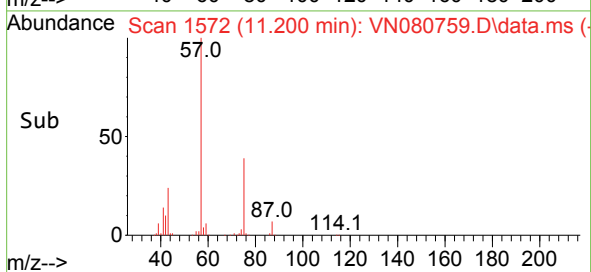

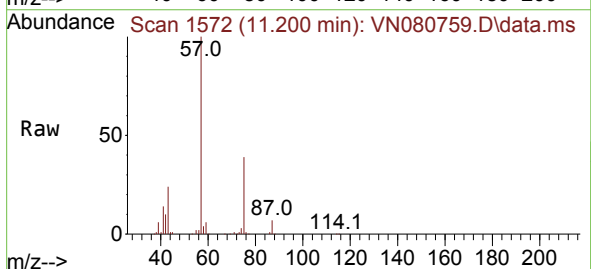




#59
2-Hexanone
Concen: 50.593 ug/l
RT: 11.171 min Scan# 1174
Delta R.T. -0.024 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48




Instrument :
MSVOA_N
ClientSampleId :
MR-305-0-2


Tgt Ion: 43 Resp: 117436
Ion Ratio Lower Upper
43 100
58 0.0 31.7 95.1#

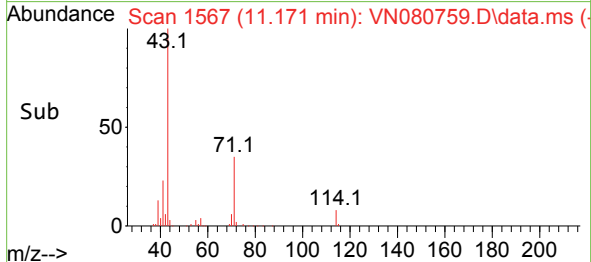

#62
4-Bromofluorobenzene
Concen: 54.049 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48

Tgt Ion: 95 Resp: 126157
Ion Ratio Lower Upper
95 100
174 62.0 0.0 143.8
176 61.9 0.0 135.8









#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48




Instrument :
MSVOA_N
ClientSampleId :
MR-305-0-2


Tgt Ion:117 Resp: 296274
Ion Ratio Lower Upper
117 100
82 64.3 44.0 66.0
119 32.7 25.6 38.4

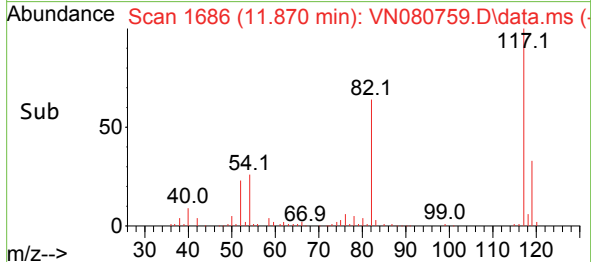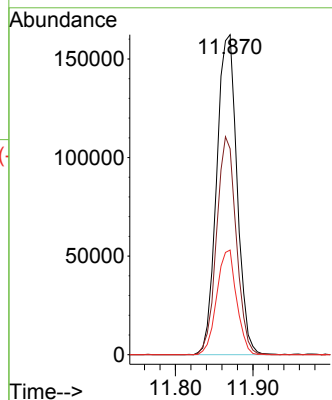

#71
Bromoform
Concen: 0.278 ug/l
RT: 12.841 min Scan# 1851
Delta R.T. 0.259 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48

Tgt Ion:173 Resp: 439
Ion Ratio Lower Upper
173 100
175 1202.5 24.3 73.0#
254 0.0 0.0 0.0

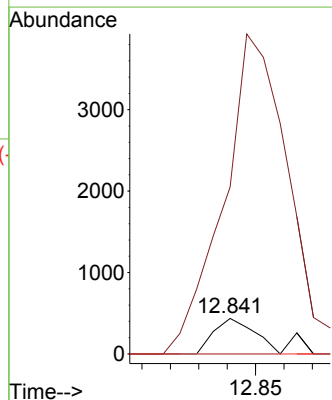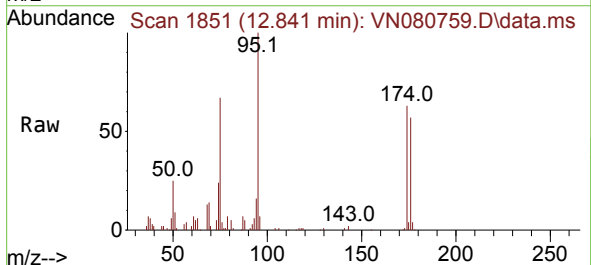

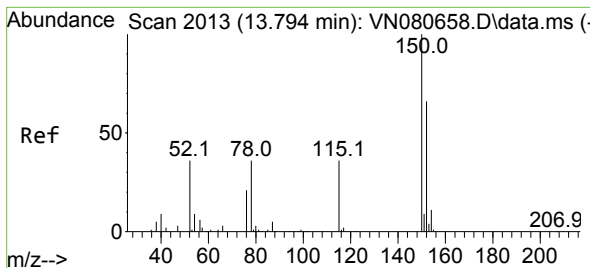

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 2013

Delta R.T. 0.000 min

Lab File: VN080759.D

Acq: 23 Jan 2024 13:48

Instrument :

MSVOA_N

ClientSampleId :

MR-305-0-2





Tgt Ion:152 Resp: 121729

Ion Ratio Lower Upper

152 100

115 68.9 32.3 96.8

150 158.1 0.0 355.8

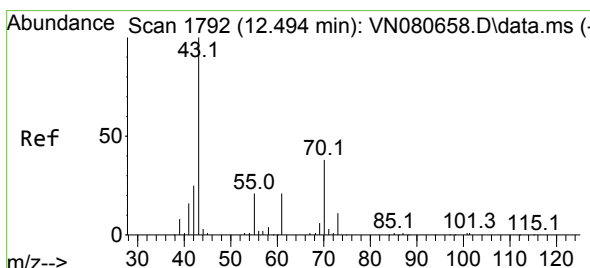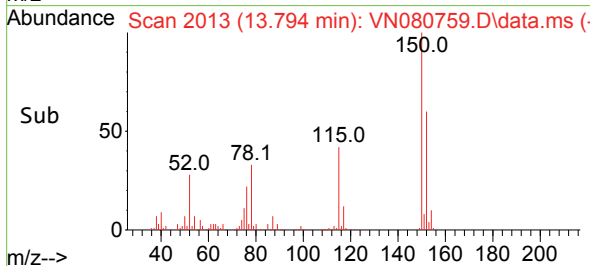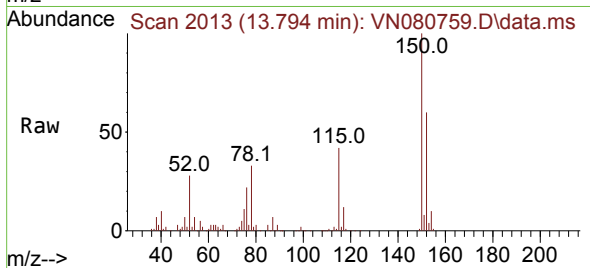

#74

N-ethyl acetate

Concen: 0.403 ug/l

RT: 12.482 min Scan# 1790

Delta R.T. -0.012 min

Lab File: VN080759.D

Acq: 23 Jan 2024 13:48

Tgt Ion: 43 Resp: 2797




Ion Ratio Lower Upper


43 100

70 0.0 43.4 65.2#

55 0.0 21.4 32.0#

61 0.0 22.8 34.2#


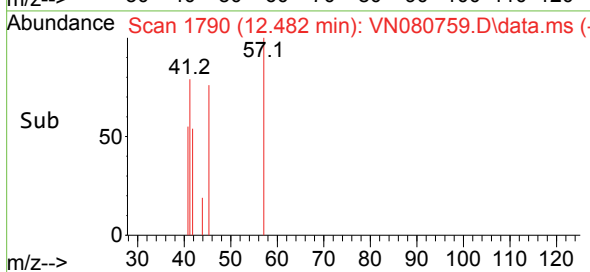
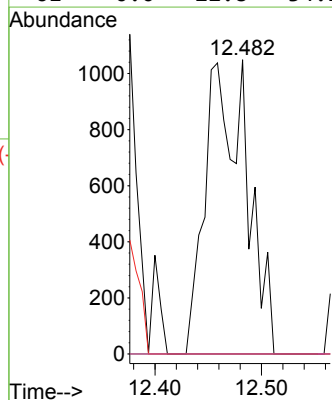
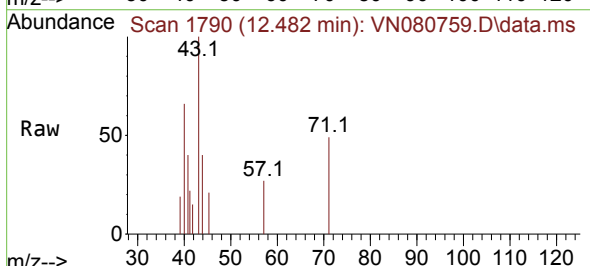




#76
1,2,3-Trichloropropane
Concen: 19.624 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.147 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48




Instrument :
MSVOA_N
ClientSampleId :
MR-305-0-2


Tgt Ion: 75 Resp: 73661
Ion Ratio Lower Upper
75 100
77 1.7 84.5 253.5#

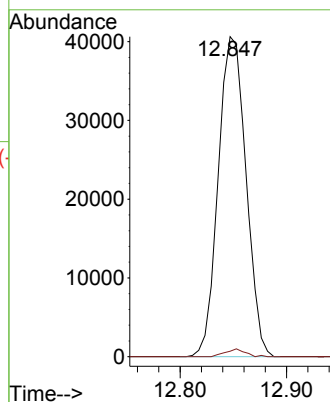

#81
trans-1,4-Dichloro-2-butene
Concen: 46.262 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.112 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48

Tgt Ion: 75 Resp: 73661
Ion Ratio Lower Upper
75 100
53 0.0 67.4 101.2#
89 0.2 38.8 58.2#


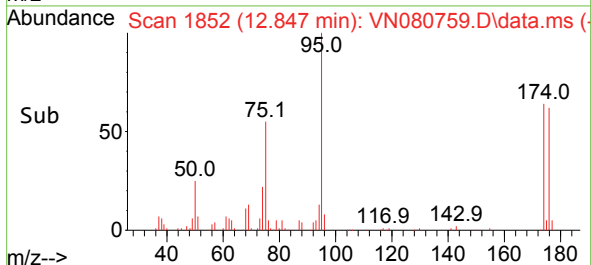
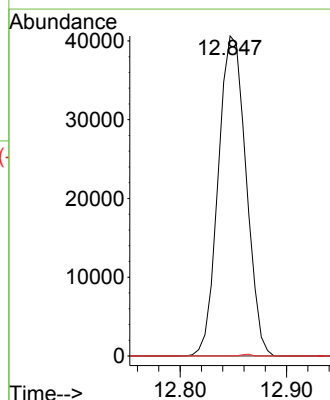



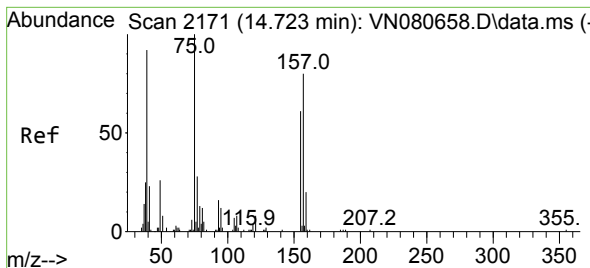

#92
1,2-Dibromo-3-Chloropropane
Concen: Below Cal
RT: 14.570 min Scan# 2171
Delta R.T. -0.153 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48

Instrument :
MSVOA_N
ClientSampleId :
MR-305-0-2

Tgt Ion: 75 Resp: 61
Ion Ratio Lower Upper
75 100
155 127.9 39.1 117.2#
157 0.0 50.3 150.9#

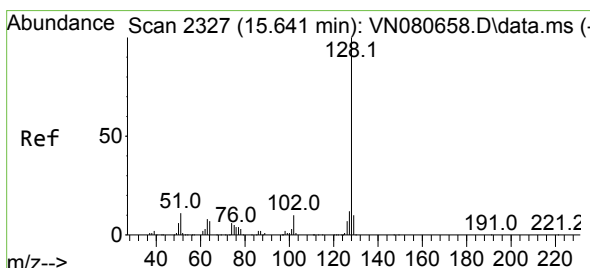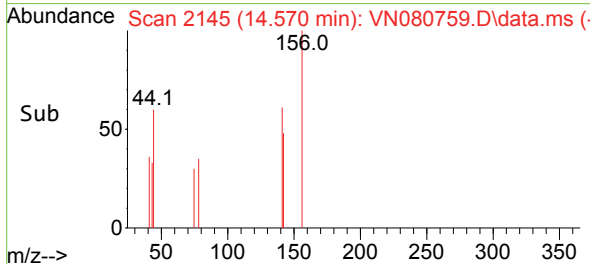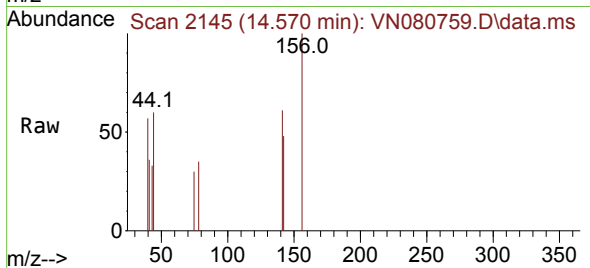

#95
Naphthalene
Concen: 0.845 ug/l
RT: 15.635 min Scan# 2326
Delta R.T. -0.006 min
Lab File: VN080759.D
Acq: 23 Jan 2024 13:48

Tgt Ion:128 Resp: 7168
Ion Ratio Lower Upper
128 100
127 10.2 10.0 15.0
129 6.8 8.7 13.1#

