

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012324\
 Data File : VN080754.D
 Acq On : 23 Jan 2024 10:55
 Operator : JC\MD
 Sample : VN0123WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0123WBL01

Quant Time: Jan 24 01:54:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011024W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 11 06:34:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	125743	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	295558	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	312699	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	122356	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	97346	44.084	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	88.160%
35) Dibromofluoromethane	8.165	113	82892	49.361	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.720%
50) Toluene-d8	10.565	98	341575	53.344	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	106.680%
62) 4-Bromofluorobenzene	12.847	95	133770	54.478	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	108.960%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012324\
Data File : VN080754.D
Acq On : 23 Jan 2024 10:55
Operator : JC\MD
Sample : VN0123WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0123WBL01


Quant Time: Jan 24 01:54:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011024W.M
Quant Title : SW846 8260
QLast Update : Thu Jan 11 06:34:36 2024
Response via : Initial Calibration

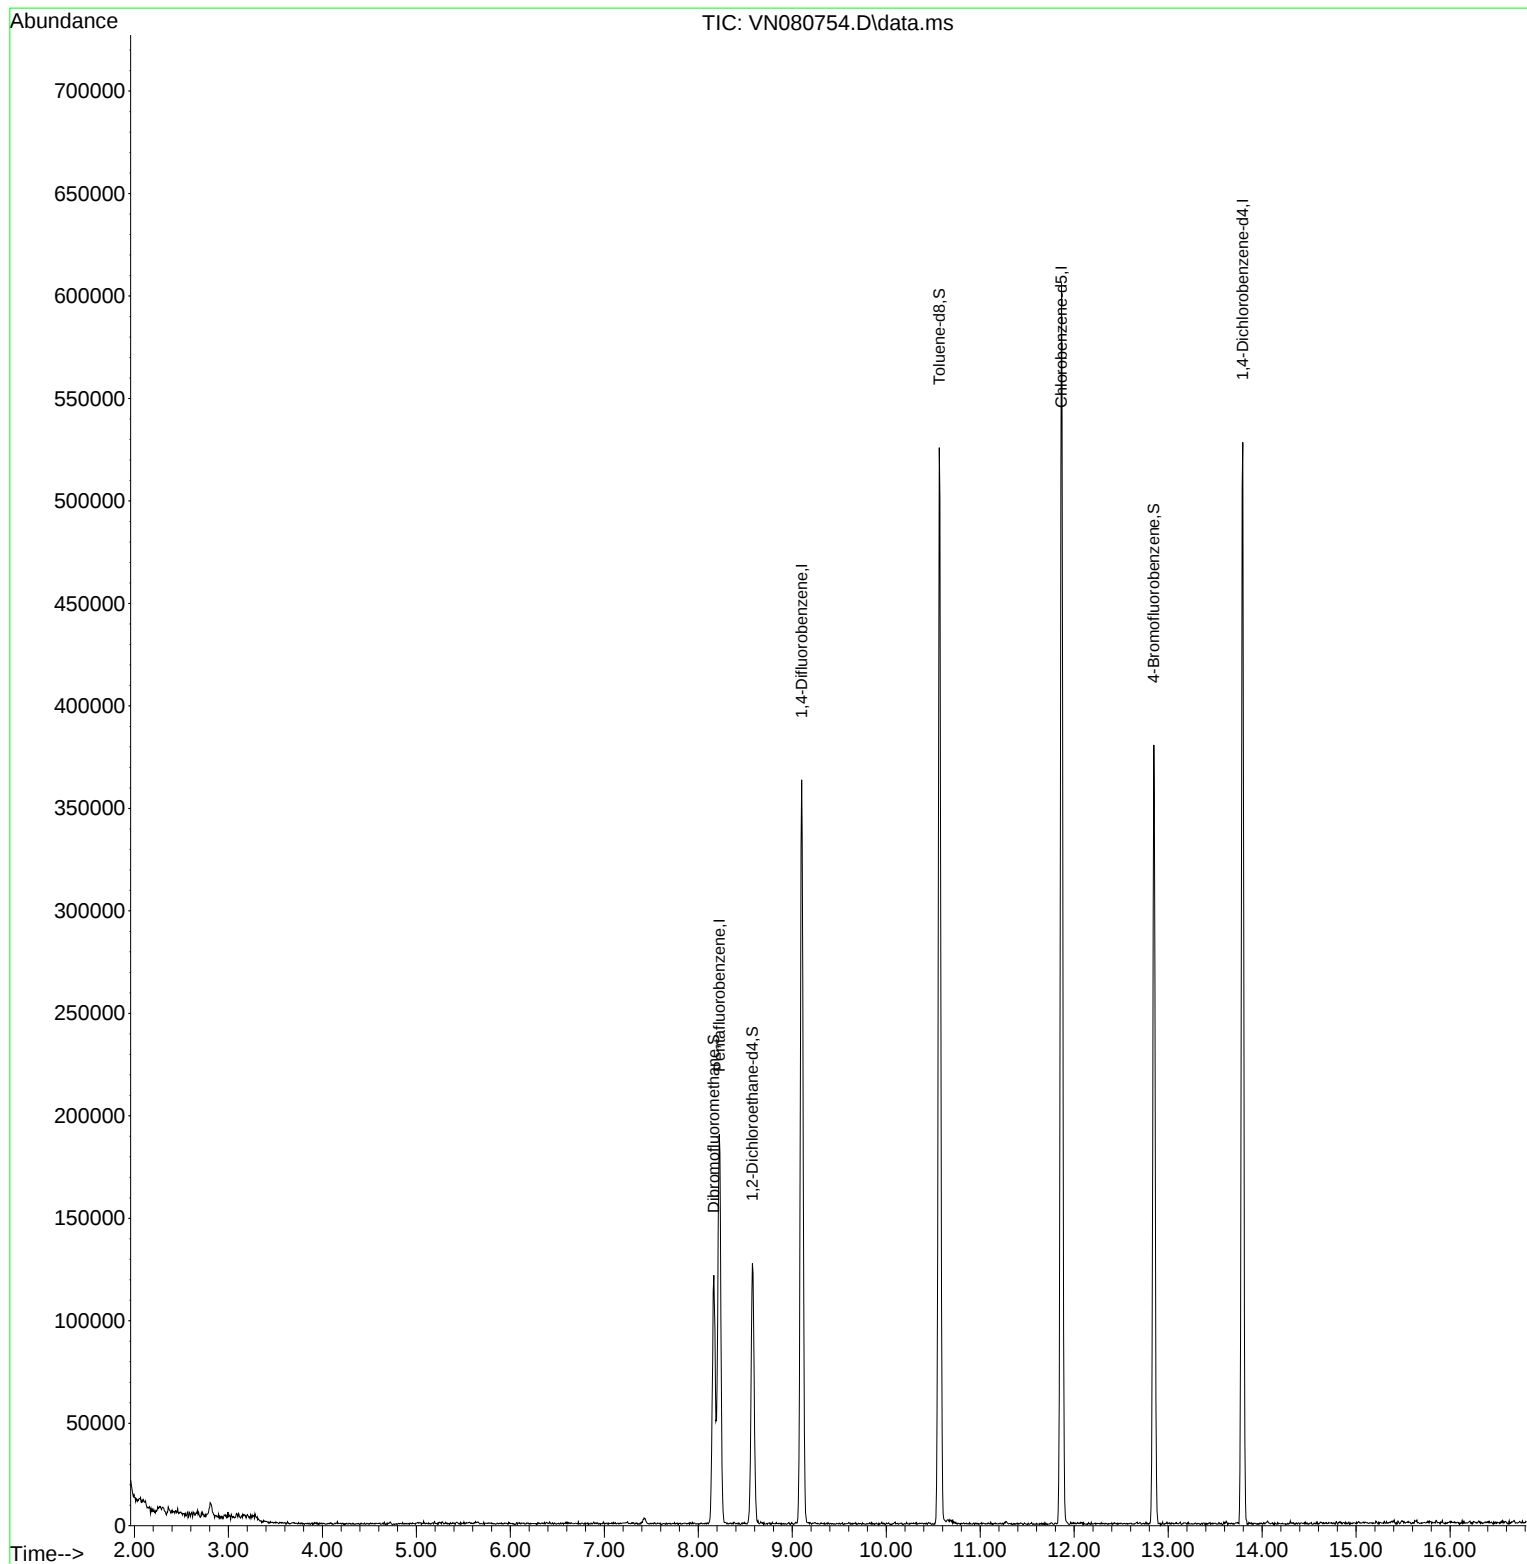



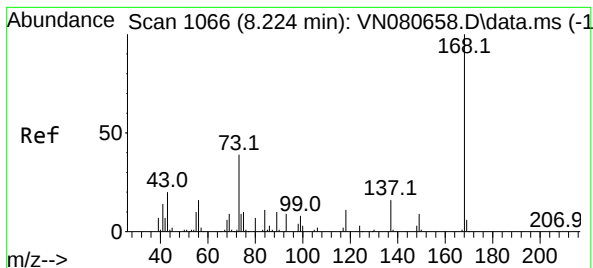


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN080754.D
Acq: 23 Jan 2024 10:55

Instrument :
MSVOA_N
ClientSampleId :
VN0123WBL01



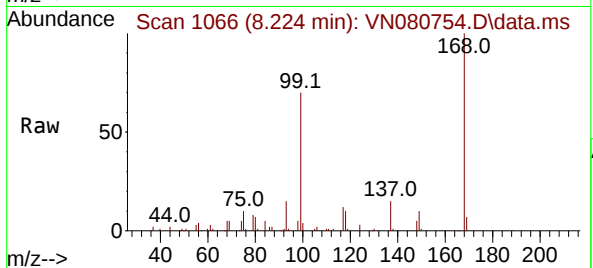



Tgt Ion:168 Resp: 125743
Ion Ratio Lower Upper
168 100
99 69.9 53.0 79.6

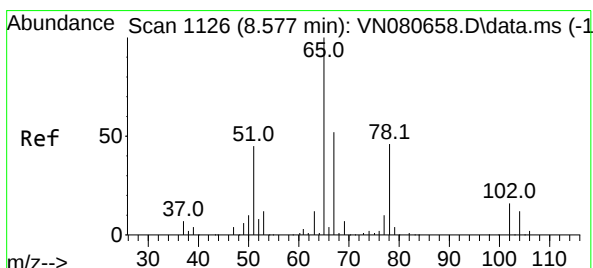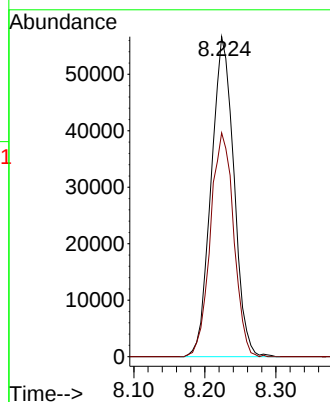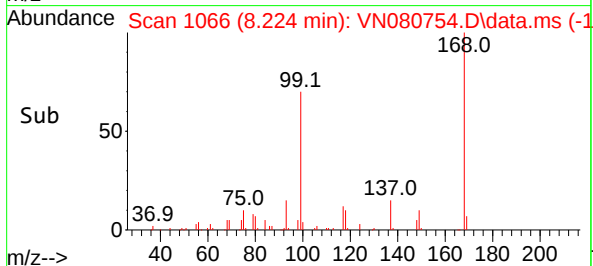

#33
1,2-Dichloroethane-d4
Concen: 44.084 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.000 min
Lab File: VN080754.D
Acq: 23 Jan 2024 10:55

Tgt Ion: 65 Resp: 97346
Ion Ratio Lower Upper
65 100
67 55.6 0.0 106.6

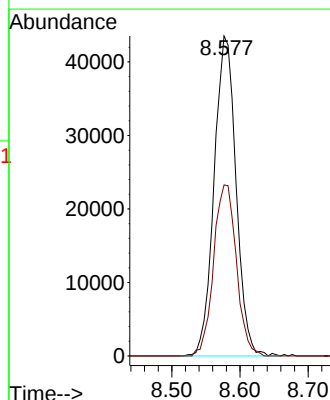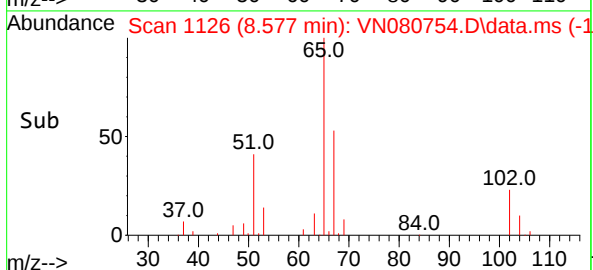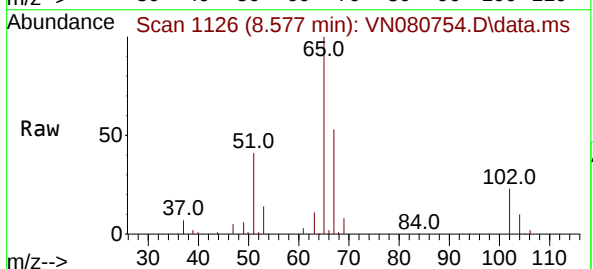

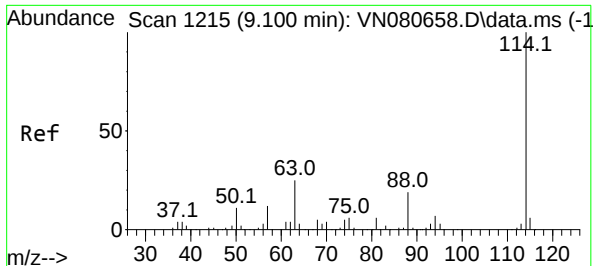

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN080754.D

Acq: 23 Jan 2024 10:55

Instrument :

MSVOA_N

ClientSampleId :

VN0123WBL01





Tgt Ion:114 Resp: 295558

Ion Ratio Lower Upper

114 100

63 24.5 0.0 36.4

88 16.3 0.0 30.6

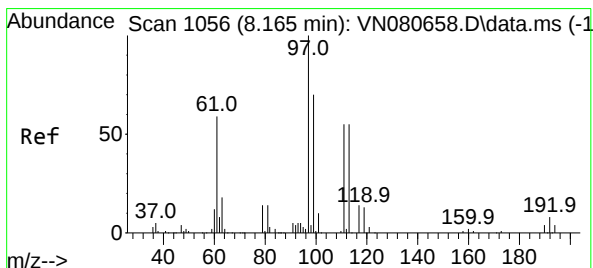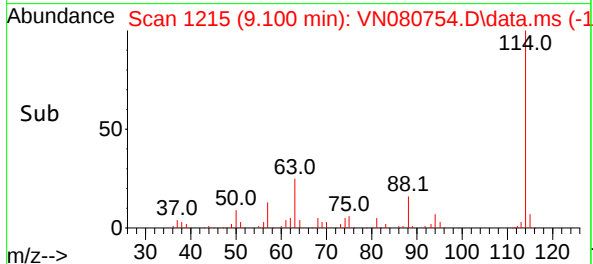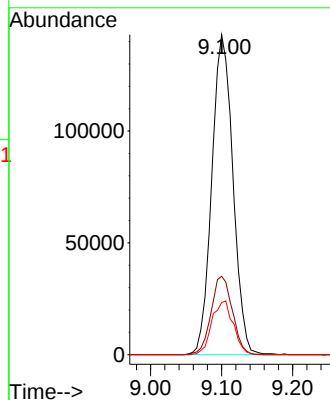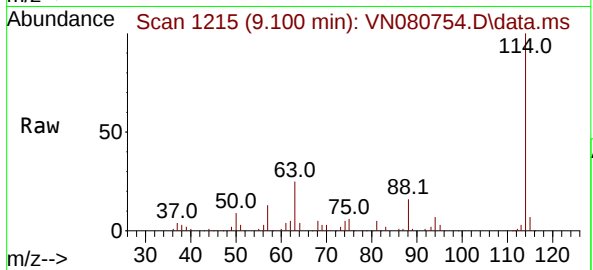

#35

Dibromofluoromethane

Concen: 49.361 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.000 min

Lab File: VN080754.D

Acq: 23 Jan 2024 10:55




Tgt Ion:113 Resp: 82892


Ion Ratio Lower Upper

113 100

111 101.5 82.6 123.8

192 15.8 12.7 19.1


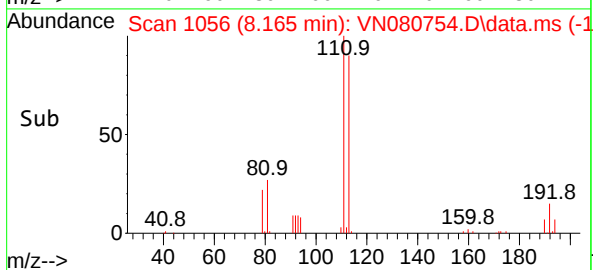
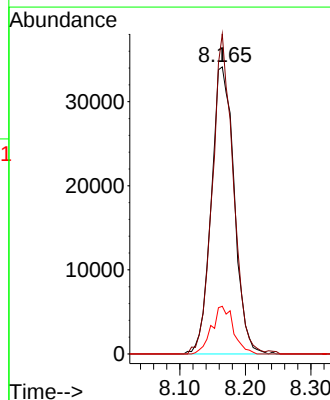
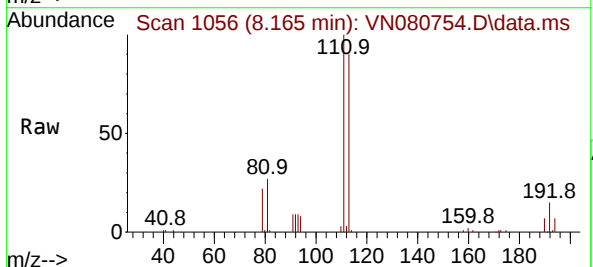


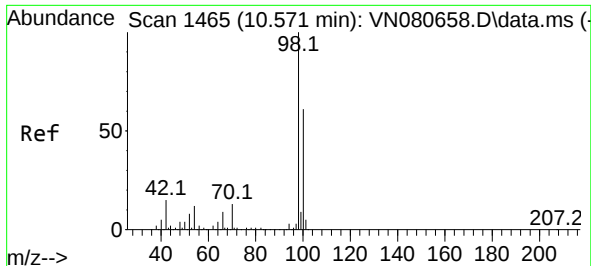

#50
Toluene-d8
Concen: 53.344 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.006 min
Lab File: VN080754.D
Acq: 23 Jan 2024 10:55




Instrument :
MSVOA_N
ClientSampleId :
VN0123WBL01


Tgt Ion: 98 Resp: 341575
Ion Ratio Lower Upper
98 100
100 63.8 52.0 78.0

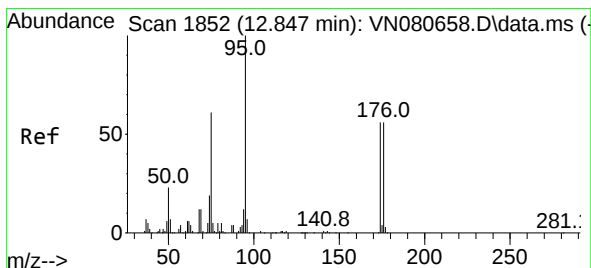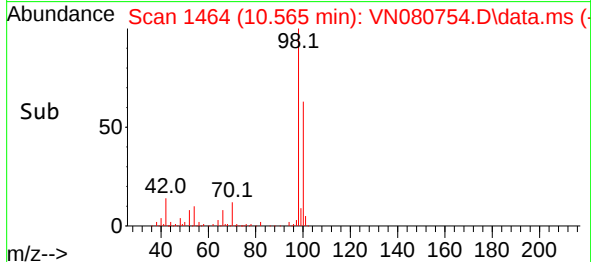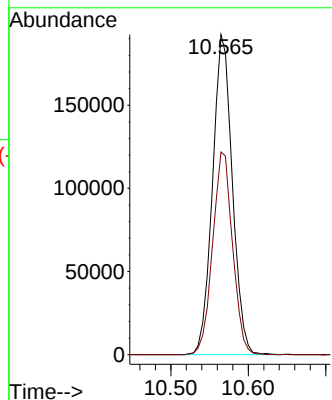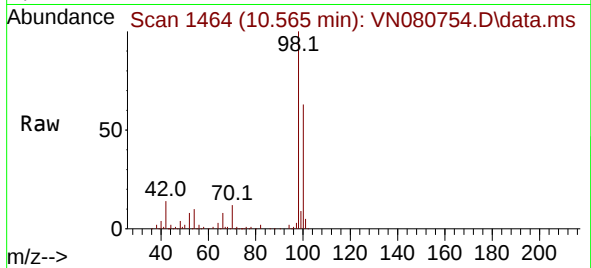

#62
4-Bromofluorobenzene
Concen: 54.478 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN080754.D
Acq: 23 Jan 2024 10:55

Tgt Ion: 95 Resp: 133770
Ion Ratio Lower Upper
95 100
174 62.1 0.0 143.8
176 59.0 0.0 135.8


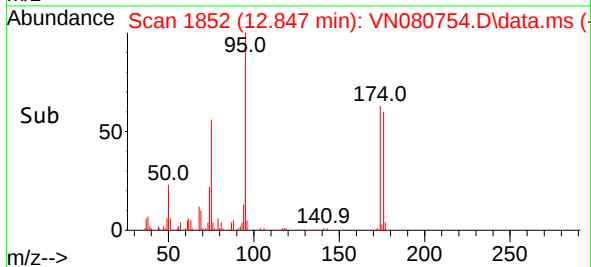
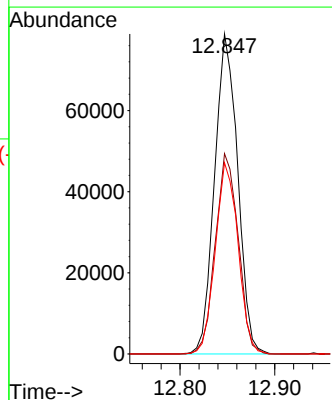
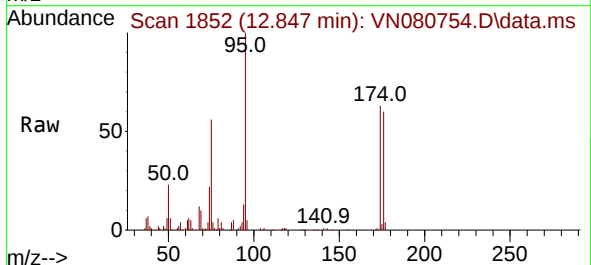


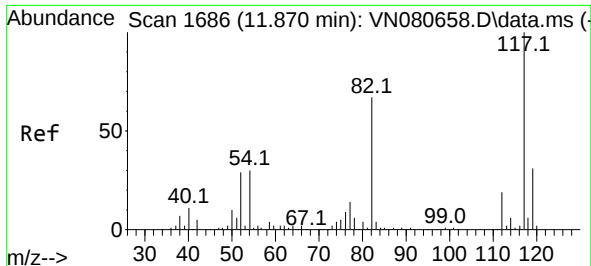

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.006 min
Lab File: VN080754.D
Acq: 23 Jan 2024 10:55

Instrument :
MSVOA_N
ClientSampleId :
VN0123WBL01

Tgt Ion:117 Resp: 312699
Ion Ratio Lower Upper
117 100
82 63.9 44.0 66.0
119 31.6 25.6 38.4

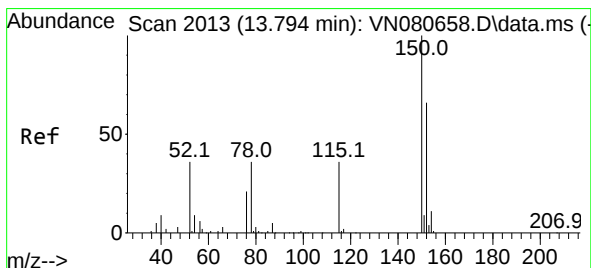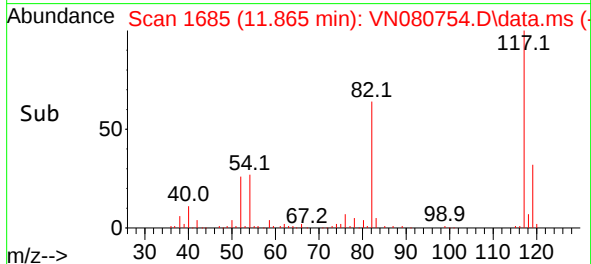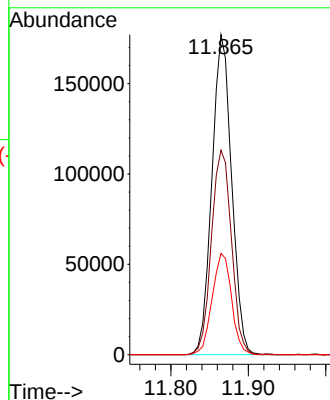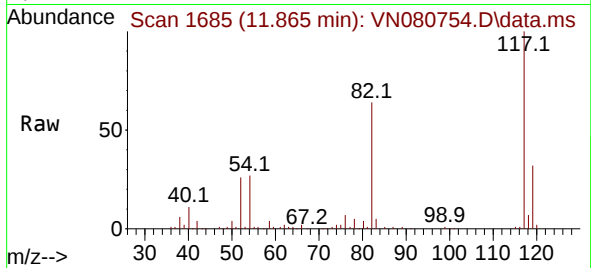

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.000 min
Lab File: VN080754.D
Acq: 23 Jan 2024 10:55

Tgt Ion:152 Resp: 122356
Ion Ratio Lower Upper
152 100
115 67.7 32.3 96.8
150 157.5 0.0 355.8

