
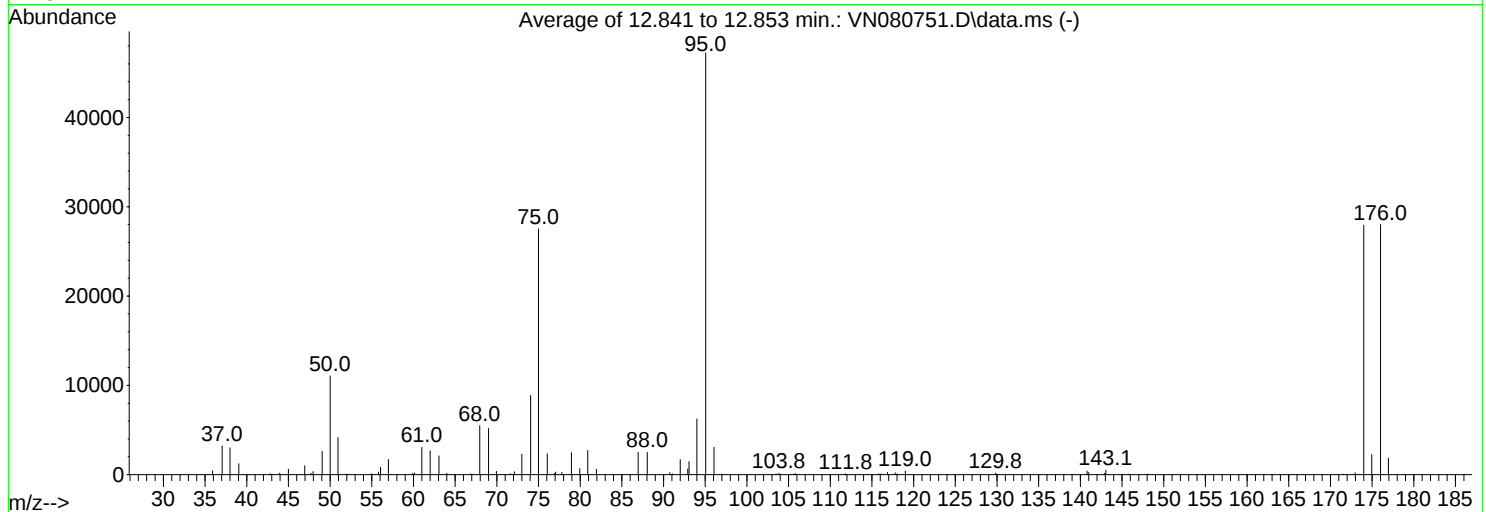


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012324\
Data File : VN080751.D
Acq On : 23 Jan 2024 09:20
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011024W.M
Title : SW846 8260
Last Update : Thu Jan 11 06:34:36 2024

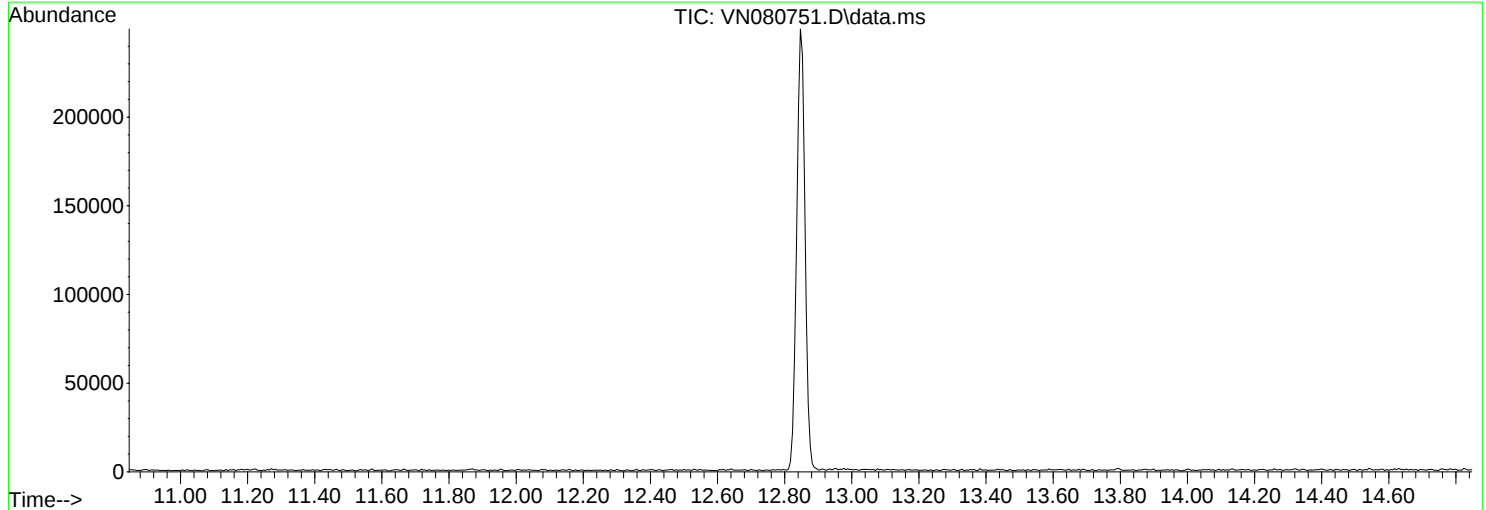

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.4	11050	PASS
75	95	30	60	58.3	27520	PASS
95	95	100	100	100.0	47235	PASS
96	95	5	9	6.5	3063	PASS
173	174	0.00	2	0.8	210	PASS
174	95	50	100	59.2	27941	PASS
175	174	5	9	8.1	2260	PASS
176	174	95	101	100.2	28003	PASS
177	176	5	9	6.6	1852	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	432	50.00	11050	62.00	2678	75.00	2752
37.05	3226	50.95	4161	63.05	2094	76.05	2341
38.00	3015	51.90	71	64.00	156	76.90	15
39.05	1213	52.10	61	66.90	83	77.05	28
42.80	105	55.00	112	67.95	5488	77.80	275
43.95	169	55.80	289	69.00	5163	78.95	2450
45.00	619	56.05	828	69.95	368	79.95	679
46.95	1013	57.00	1679	71.60	82	80.90	2703
47.70	137	59.90	135	72.10	317	81.95	619
47.95	349	60.10	191	73.00	2297	86.95	2514
49.05	2623	61.00	3055	74.05	8875	88.05	2516

Average of 12.841 to 12.853 min.: VN080751.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.75	235	105.60	52	141.00	259		
91.10	86	105.80	123	142.90	139		
92.00	1683	111.85	111	143.05	507		
92.90	628	115.80	94	145.80	59		
93.05	1470	116.10	92	148.10	75		
94.00	6235	116.85	249	171.60	60		
95.05	47235	117.80	197	172.95	210		
96.05	3063	118.00	84	174.00	27941		
97.00	68	119.00	395	174.95	2260		
103.50	84	129.85	185	176.00	28003		
103.85	154	140.80	394	176.95	1852		

Instrument :

MSVOA_N

ClientSampleId :

BFB