

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012422\
 Data File : VN070749.D
 Acq On : 24 Jan 2022 12:22
 Operator : JC/MD
 Sample : N1217-06ME
 Misc : 5.01g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 72-72017ME

Quant Time: Jan 24 23:29:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 18 13:32:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.078	168	931760	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1494395	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	1230839	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	494283	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.432	65	626240	46.897	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	93.800%		
35) Dibromofluoromethane	8.016	113	420726	45.387	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	90.780%		
50) Toluene-d8	10.438	98	1821378	46.641	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	93.280%		
62) 4-Bromofluorobenzene	12.731	95	584387	41.995	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	83.980%		
Target Compounds						Qvalue
11) Tert butyl alcohol	5.294	59	3490	1.449	ug/l #	71
13) Acrolein	4.033	56	1244	0.360	ug/l	86
16) Acetone	4.296	43	20615	2.224	ug/l	96
18) Methyl Acetate	4.854	43	17377	0.953	ug/l #	77
25) 2-Butanone	7.351	43	30293	2.597	ug/l #	83
29) Tetrahydrofuran	7.697	42	7981	1.118	ug/l #	72
30) Chloroform	7.807	83	3935	Below Cal		96
31) Cyclohexane	8.078	56	21628	0.920	ug/l #	11
36) 1,1-Dichloropropene	8.078	75	78347	5.020	ug/l #	48
37) Ethyl Acetate	7.351	43	30293	1.462	ug/l #	69
38) Carbon Tetrachloride	8.078	117	94279	6.791	ug/l #	16
43) Isopropyl Acetate	8.582	43	9565	0.302	ug/l #	55
49) 1,4-Dioxane	9.574	88	307	1.356	ug/l #	77
51) 4-Methyl-2-Pentanone	10.336	43	10601	0.525	ug/l	94
53) t-1,3-Dichloropropene	10.714	75	450	2.426	ug/l #	77
56) Ethyl methacrylate	10.765	69	1900	2.386	ug/l #	81
58) 2-Chloroethyl Vinyl ether	10.035	63	217	21.273	ug/l #	45
59) 2-Hexanone	11.089	43	20817	1.419	ug/l	95
74) N-amyl acetate	12.390	43	12122	0.634	ug/l	93
76) 1,2,3-Trichloropropane	12.731	75	309539	23.611	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.731	75	309539	70.343	ug/l #	5
84) 1,2,4-Trimethylbenzene	13.366	105	9970	0.274	ug/l	95
87) 1,3-Dichlorobenzene	13.616	146	4626	0.265	ug/l	93
88) 1,4-Dichlorobenzene	13.616	146	4626	0.267	ug/l	92
89) n-Butylbenzene	13.943	91	13753	0.474	ug/l	97
91) 1,2-Dichlorobenzene	13.983	146	4934	0.286	ug/l	93
92) 1,2-Dibromo-3-Chloropr...	14.600	75	1196	0.446	ug/l	62
93) 1,2,4-Trichlorobenzene	15.263	180	8891	4.332	ug/l	96
94) Hexachlorobutadiene	15.370	225	1328	0.260	ug/l #	57
95) Naphthalene	15.504	128	30651	6.026	ug/l	97
96) 1,2,3-Trichlorobenzene	15.694	180	9732	4.259	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012422\
 Data File : VN070749.D
 Acq On : 24 Jan 2022 12:22
 Operator : JC/MD
 Sample : N1217-06ME
 Misc : 5.01g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 72-72017ME

Quant Time: Jan 24 23:29:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 18 13:32:07 2022
 Response via : Initial Calibration

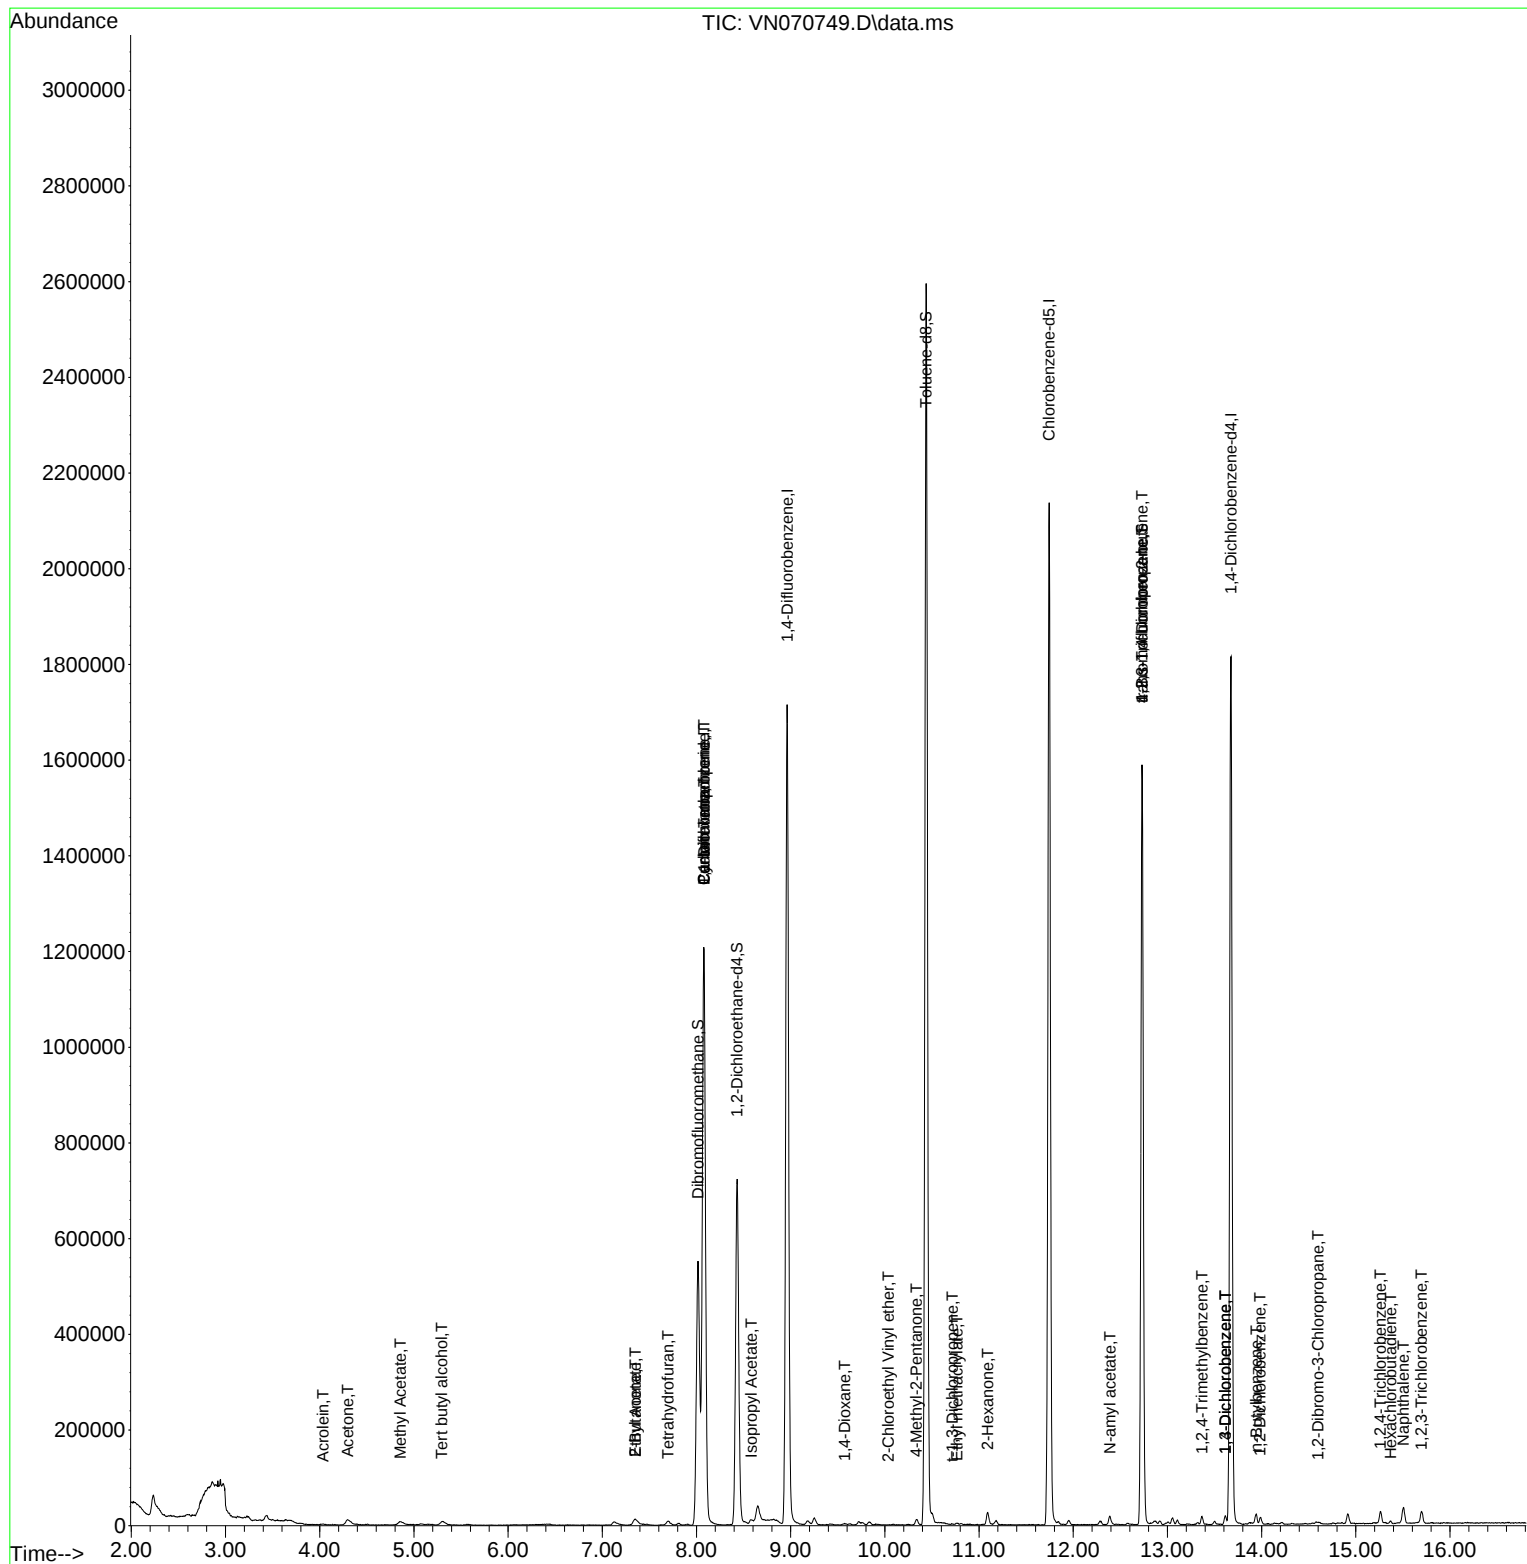



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.078 min Scan# 21

Delta R.T. -0.005 min

Lab File: VN070749.D

Acq: 24 Jan 2022 12:22

Instrument :

MSVOA_N

ClientSampleId :





72-72017ME

Tgt Ion:168 Resp: 931760

Ion Ratio Lower Upper

168 100

99 60.8 41.3 61.9

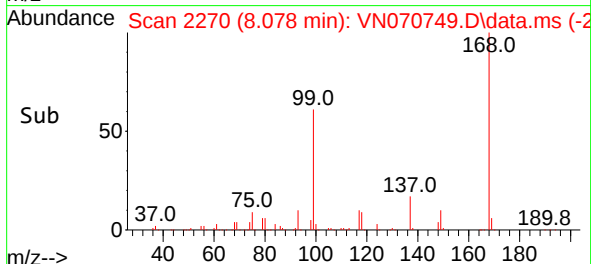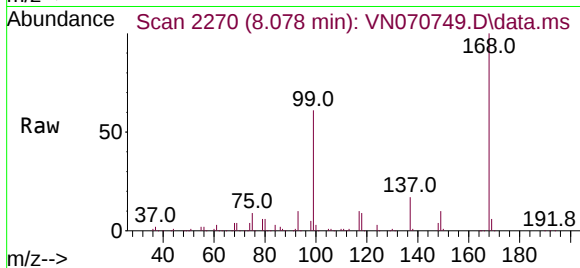

#11

Tert butyl alcohol

Concen: 1.449 ug/l

RT: 5.294 min Scan# 1232

Delta R.T. -0.083 min

Lab File: VN070749.D




Acq: 24 Jan 2022 12:22


Tgt Ion: 59 Resp: 3490

Ion Ratio Lower Upper

59 100

57 0.0 8.7 13.1#


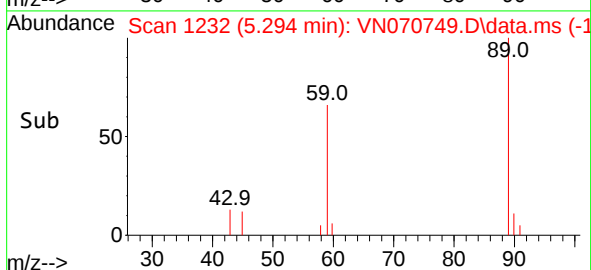

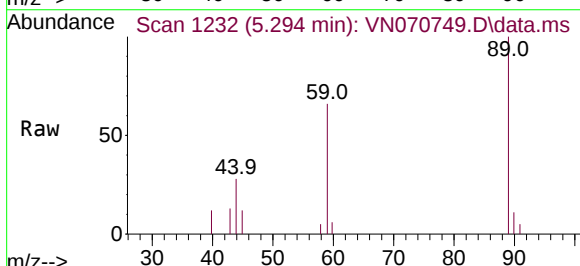




#13
Acrolein
Concen: 0.360 ug/l
RT: 4.033 min Scan# 762
Delta R.T. -0.006 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22




Instrument :
MSVOA_N
ClientSampleId :
72-72017ME


Tgt Ion: 56 Resp: 1244
Ion Ratio Lower Upper
56 100
55 82.2 56.6 85.0

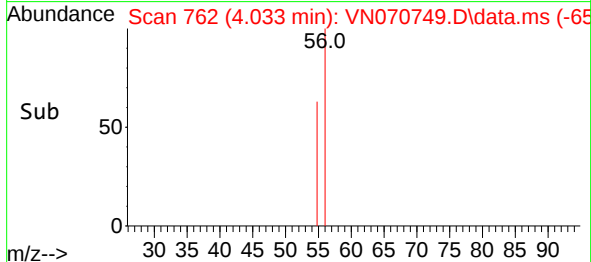

#16
Acetone
Concen: 2.224 ug/l
RT: 4.296 min Scan# 860
Delta R.T. 0.011 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22

Tgt Ion: 43 Resp: 20615
Ion Ratio Lower Upper
43 100
58 26.8 23.1 34.7


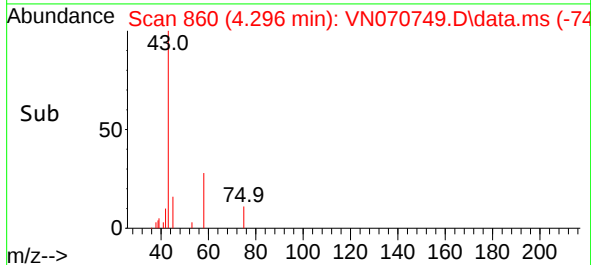

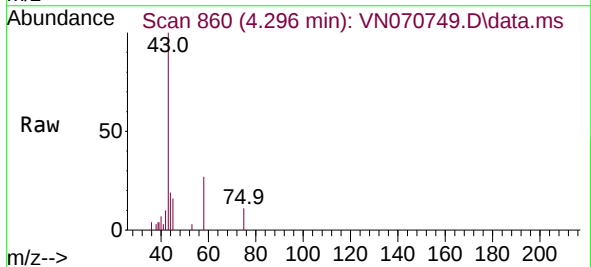


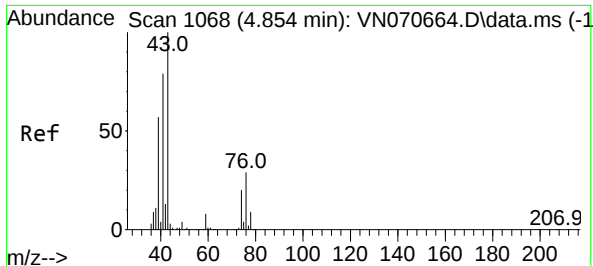

#18
Methyl Acetate
Concen: 0.953 ug/l
RT: 4.854 min Scan# 1068
Delta R.T. -0.000 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22




Instrument :
MSVOA_N
ClientSampleId :
72-72017ME


Tgt Ion: 43 Resp: 17377
Ion Ratio Lower Upper
43 100
74 12.8 19.4 29.2#

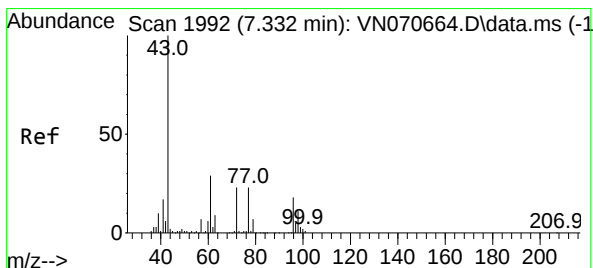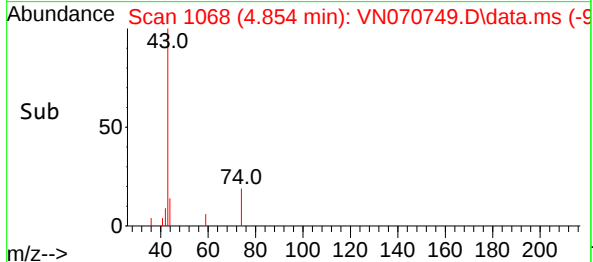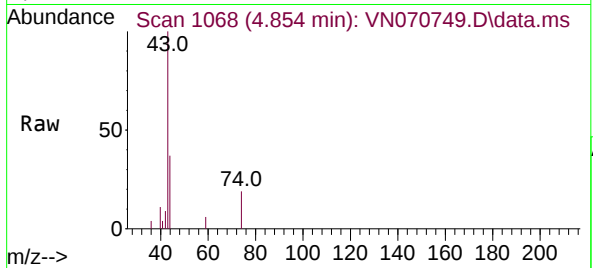

#25
2-Butanone
Concen: 2.597 ug/l
RT: 7.351 min Scan# 1999
Delta R.T. 0.019 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22

Tgt Ion: 43 Resp: 30293
Ion Ratio Lower Upper
43 100
72 18.1 21.7 32.5#

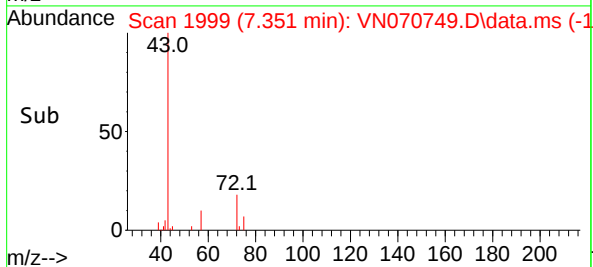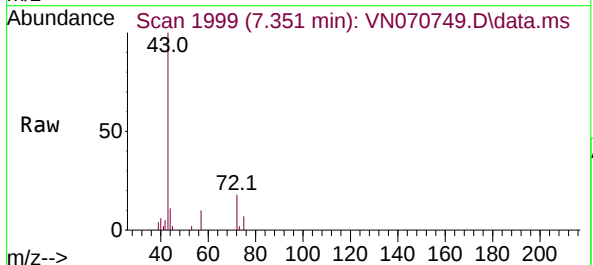



#29

Tetrahydrofuran

Concen: 1.118 ug/l

RT: 7.697 min Scan# 2123

Delta R.T. 0.014 min

Lab File: VN070749.D

Acq: 24 Jan 2022 12:22

Instrument :

MSVOA_N

ClientSampleId :

72-72017ME





Tgt Ion: 42 Resp: 7981

Ion Ratio Lower Upper

42 100

72 21.4 36.3 54.5#

71 31.3 34.7 52.1#

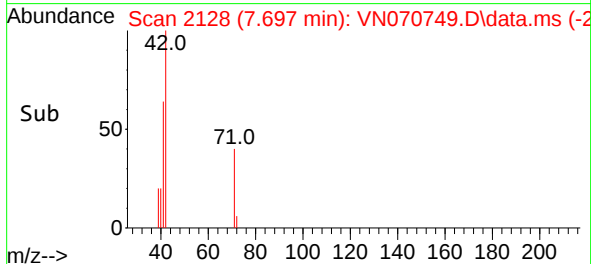

#30

Chloroform

Concen: Below Cal

RT: 7.807 min Scan# 2169

Delta R.T. -0.011 min

Lab File: VN070749.D




Acq: 24 Jan 2022 12:22


Tgt Ion: 83 Resp: 3935

Ion Ratio Lower Upper

83 100

85 68.2 51.9 77.9


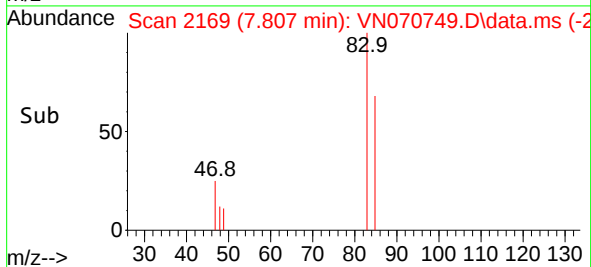

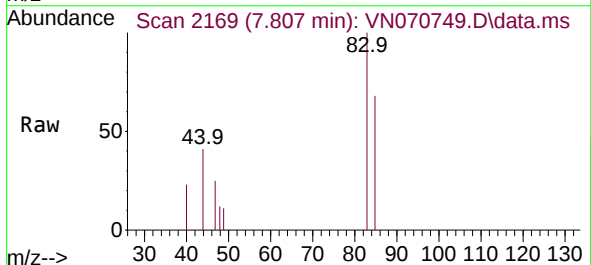




#31
Cyclohexane
Concen: 0.920 ug/l
RT: 8.078 min Scan# 21
Delta R.T. -0.016 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22




Instrument :
MSVOA_N
ClientSampleId :
72-72017ME


Tgt Ion: 56 Resp: 21628
Ion Ratio Lower Upper
56 100
69 161.6 27.1 40.7#
84 129.2 73.4 110.0#

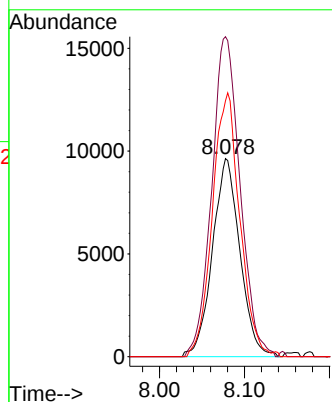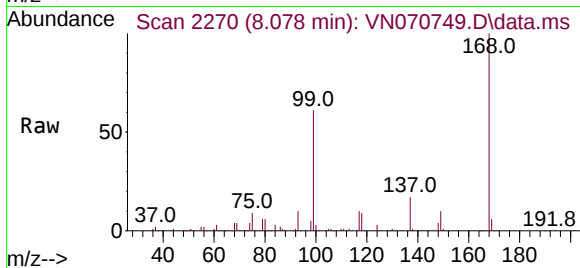

#33
1,2-Dichloroethane-d4
Concen: 46.897 ug/l
RT: 8.432 min Scan# 2402
Delta R.T. -0.002 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22

Tgt Ion: 65 Resp: 626240
Ion Ratio Lower Upper
65 100
67 52.2 0.0 103.0


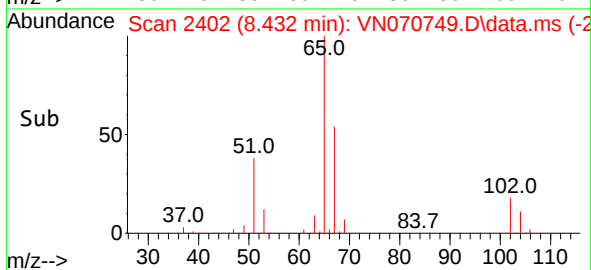
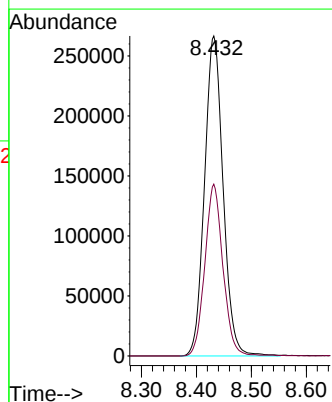
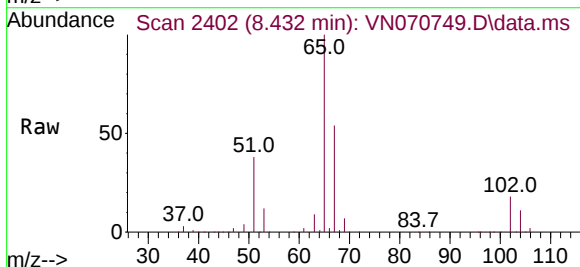




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.963 min Scan# 2600
Delta R.T. -0.002 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22




Instrument :
MSVOA_N
ClientSampleId :
72-72017ME


Tgt Ion:114 Resp: 1494395
Ion Ratio Lower Upper
114 100
63 23.8 0.0 37.8
88 16.6 0.0 27.4

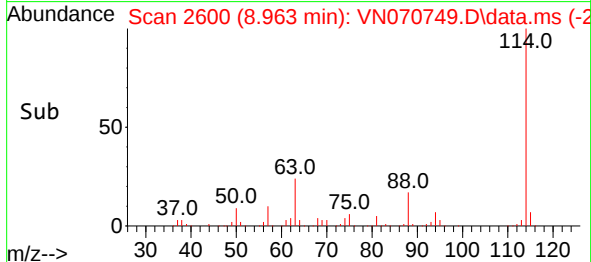

#35
Dibromofluoromethane
Concen: 45.387 ug/l
RT: 8.016 min Scan# 2247
Delta R.T. -0.003 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22

Tgt Ion:113 Resp: 420726
Ion Ratio Lower Upper
113 100
111 103.0 82.2 123.2
192 19.5 16.9 25.3

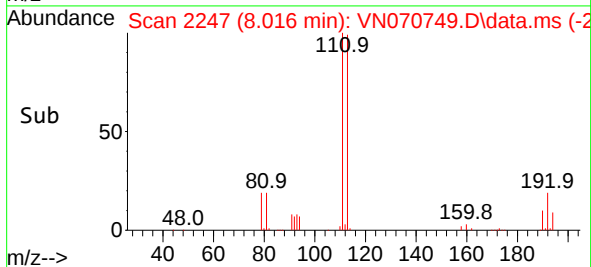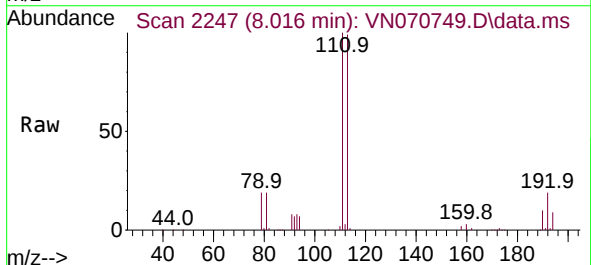



#36

1,1-Dichloropropene

Concen: 5.020 ug/l

RT: 8.078 min Scan# 21

Delta R.T. -0.142 min

Lab File: VN070749.D

Acq: 24 Jan 2022 12:22

Instrument :

MSVOA_N

ClientSampleId :

72-72017ME





Tgt Ion: 75 Resp: 78347

Ion Ratio Lower Upper

75 100

110 7.7 18.4 55.2#

77 0.0 24.4 36.6#

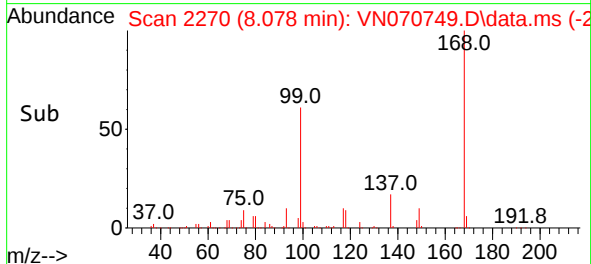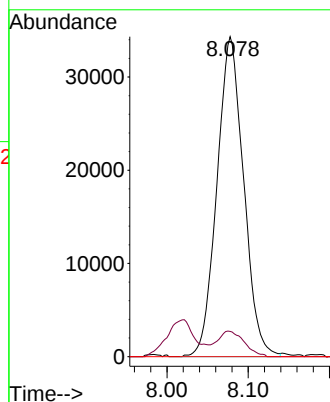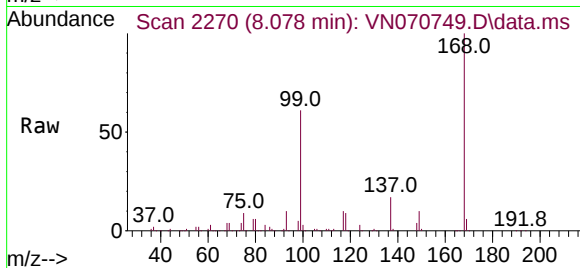

#37

Ethyl Acetate

Concen: 1.462 ug/l

RT: 7.351 min Scan# 1999

Delta R.T. -0.059 min

Lab File: VN070749.D

Acq: 24 Jan 2022 12:22




Tgt Ion: 43 Resp: 30293


Ion Ratio Lower Upper

43 100

61 0.5 11.5 17.3#

70 0.0 7.9 11.9#


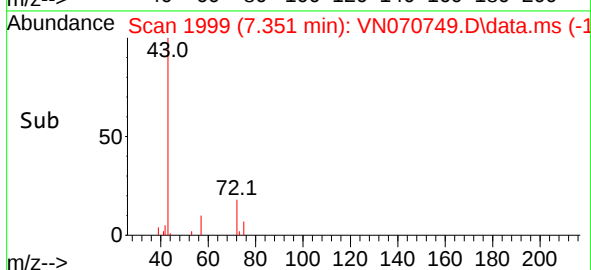

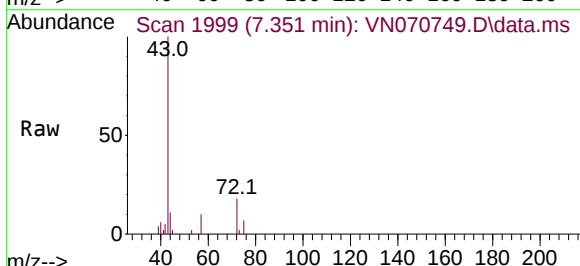




#38
Carbon Tetrachloride
Concen: 6.791 ug/l
RT: 8.078 min Scan# 21
Delta R.T. -0.128 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22




Instrument :
MSVOA_N
ClientSampleId :
72-72017ME


Tgt Ion:117 Resp: 94279
Ion Ratio Lower Upper
117 100
119 4.5 76.1 114.1#
121 0.0 24.2 36.2#

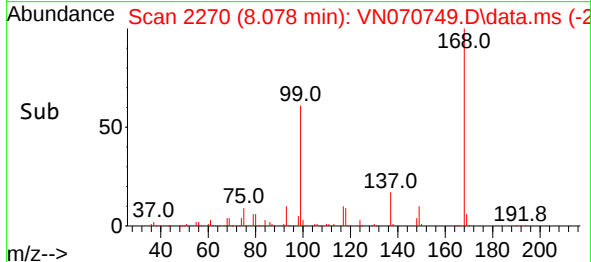

#43
Isopropyl Acetate
Concen: 0.302 ug/l
RT: 8.582 min Scan# 2458
Delta R.T. 0.022 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22

Tgt Ion: 43 Resp: 9565
Ion Ratio Lower Upper
43 100
61 0.0 20.4 30.6#
87 0.0 11.2 16.8#

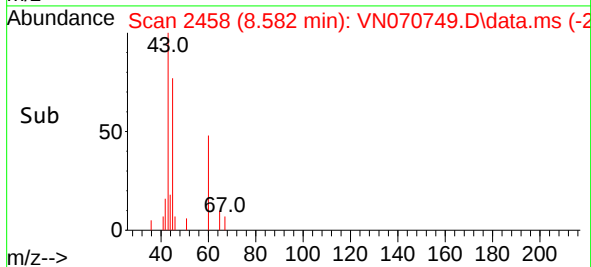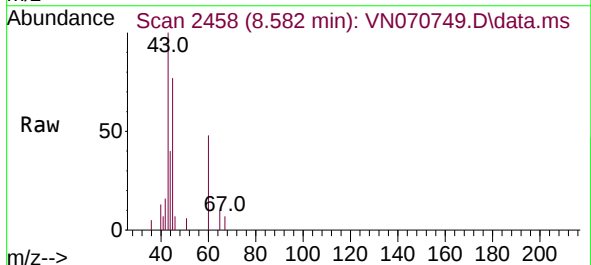



#49

1,4-Dioxane

Concen: 1.356 ug/l

RT: 9.574 min Scan# 21

Delta R.T. 0.005 min

Lab File: VN070749.D

Acq: 24 Jan 2022 12:22

Instrument :

MSVOA_N

ClientSampleId :

72-72017ME





Tgt Ion: 88 Resp: 307

Ion Ratio Lower Upper

88 100

43 42.0 23.4 35.2#

58 45.6 50.6 75.8#

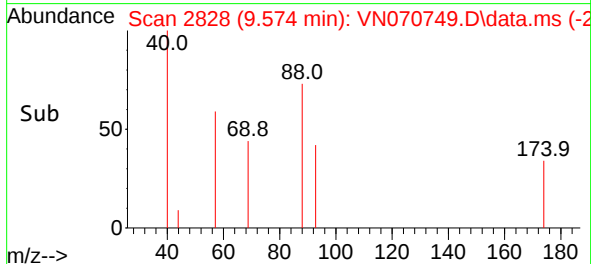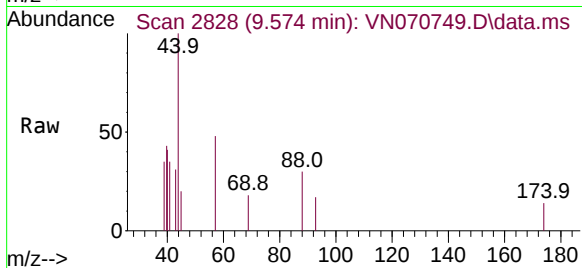

#50

Toluene-d8

Concen: 46.641 ug/l

RT: 10.438 min Scan# 3150

Delta R.T. -0.000 min

Lab File: VN070749.D




Acq: 24 Jan 2022 12:22


Tgt Ion: 98 Resp: 1821378

Ion Ratio Lower Upper

98 100

100 64.2 50.4 75.6

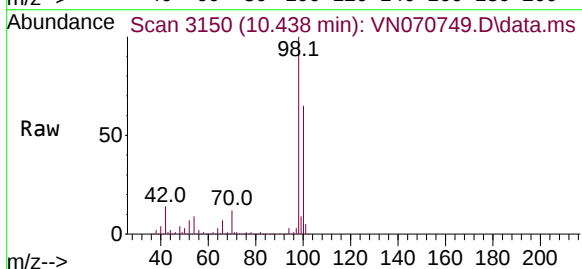

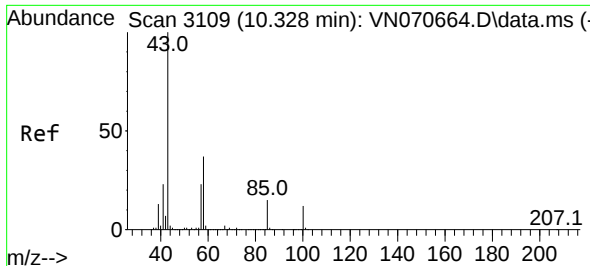

#51

4-Methyl-2-Pentanone

Concen: 0.525 ug/l

RT: 10.336 min Scan# 3112

Delta R.T. 0.008 min

Lab File: VN070749.D

Acq: 24 Jan 2022 12:22

Instrument :

MSVOA_N

ClientSampleId :





72-72017ME

Tgt Ion: 43 Resp: 10601

Ion Ratio Lower Upper

43 100

58 34.3 30.4 45.6

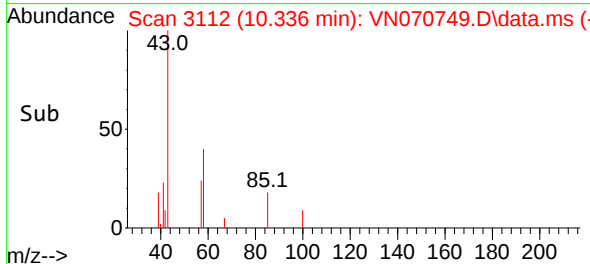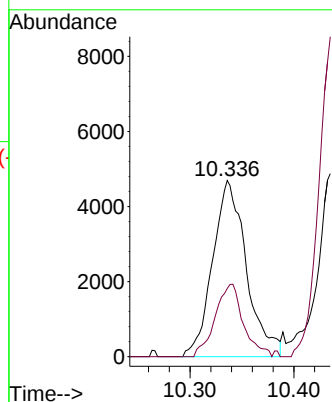

#53

t-1,3-Dichloropropene

Concen: 2.426 ug/l

RT: 10.714 min Scan# 3253

Delta R.T. -0.003 min

Lab File: VN070749.D




Acq: 24 Jan 2022 12:22


Tgt Ion: 75 Resp: 450

Ion Ratio Lower Upper

75 100

77 19.0 25.6 38.4#


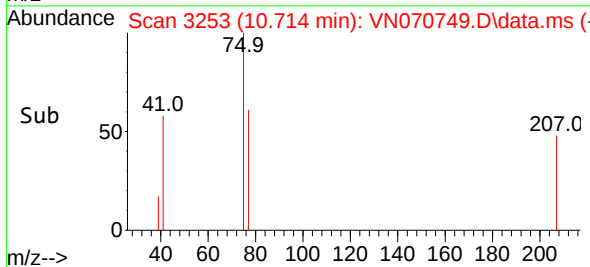
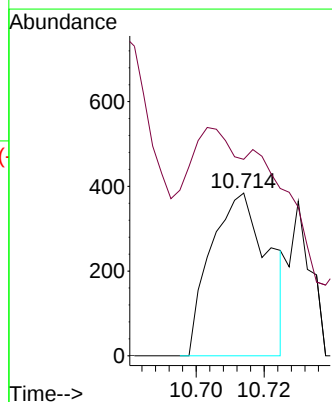
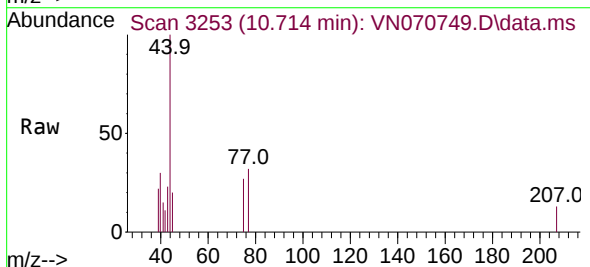




#56
Ethyl methacrylate
Concen: 2.386 ug/l
RT: 10.765 min Scan# 31
Delta R.T. 0.005 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22




Instrument :
MSVOA_N
ClientSampleId :
72-72017ME


Tgt Ion: 69 Resp: 1900
Ion Ratio Lower Upper
69 100
41 86.8 51.4 77.0#
39 46.1 34.6 52.0

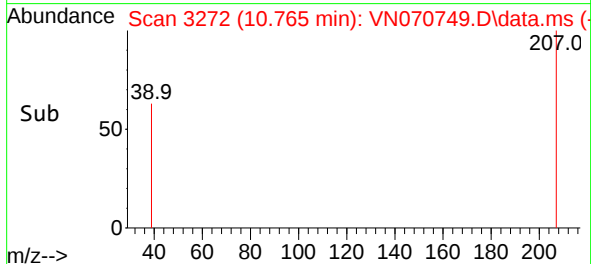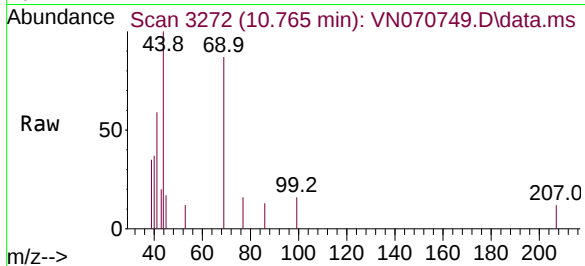

#58
2-Chloroethyl Vinyl ether
Concen: 21.273 ug/l
RT: 10.035 min Scan# 3000
Delta R.T. -0.003 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22

Tgt Ion: 63 Resp: 217
Ion Ratio Lower Upper
63 100
106 0.0 23.9 35.9#


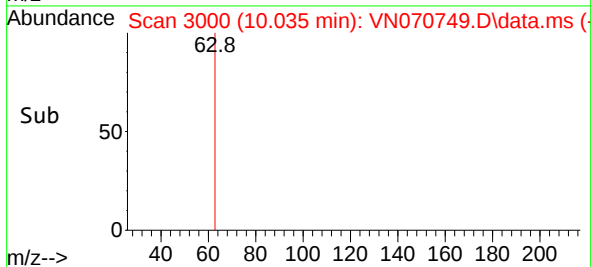

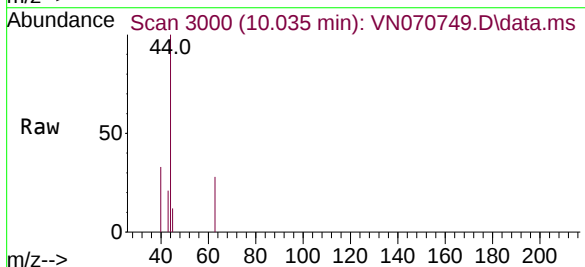


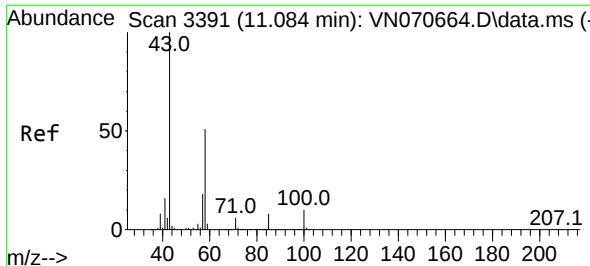

#59
2-Hexanone
Concen: 1.419 ug/l
RT: 11.089 min Scan# 31
Delta R.T. 0.005 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22




Instrument :
MSVOA_N
ClientSampleId :
72-72017ME


Tgt Ion: 43 Resp: 20817
Ion Ratio Lower Upper
43 100
58 50.4 26.9 80.7

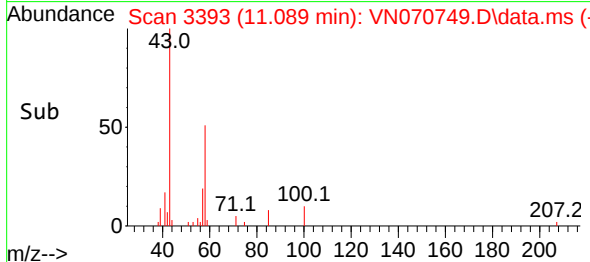

#62
4-Bromofluorobenzene
Concen: 41.995 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.003 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22

Tgt Ion: 95 Resp: 584387
Ion Ratio Lower Upper
95 100
174 74.1 0.0 187.2
176 71.4 0.0 181.4


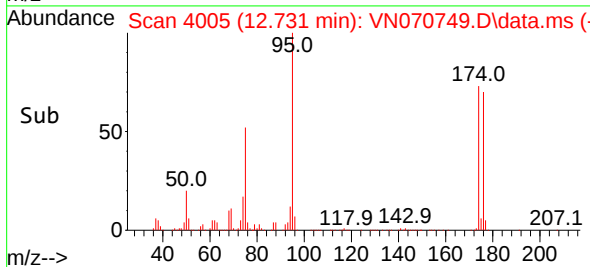

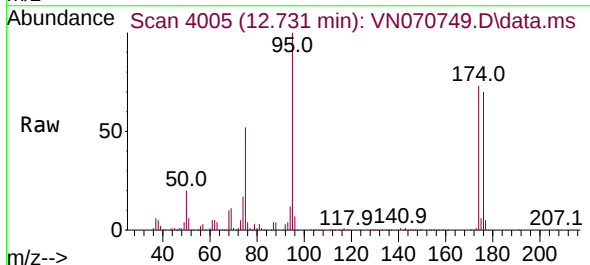


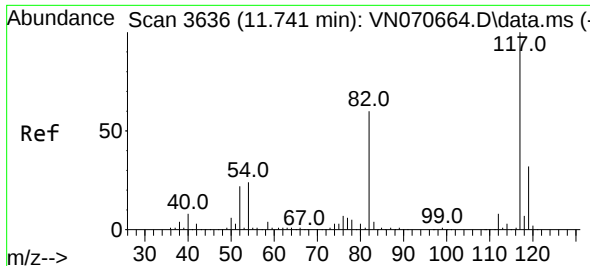

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 30
Delta R.T. 0.003 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22




Instrument :
MSVOA_N
ClientSampleId :
72-72017ME


Tgt Ion:117 Resp: 1230839
Ion Ratio Lower Upper
117 100
82 61.1 42.4 63.6
119 31.8 25.4 38.2

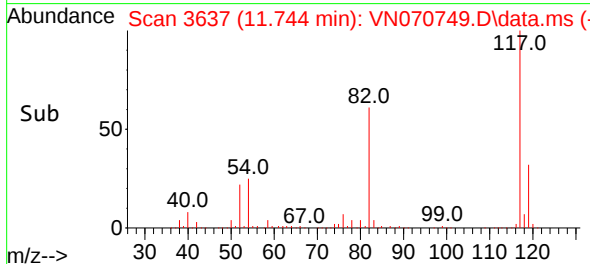

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 4357
Delta R.T. 0.003 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22

Tgt Ion:152 Resp: 494283
Ion Ratio Lower Upper
152 100
115 63.2 27.5 82.5
150 158.6 0.0 344.4


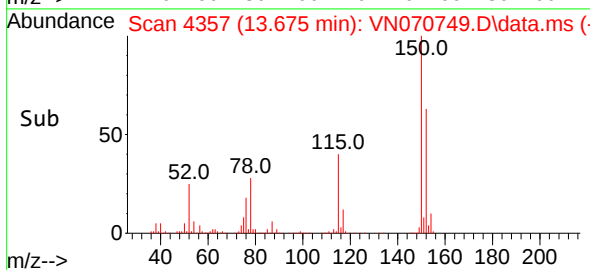

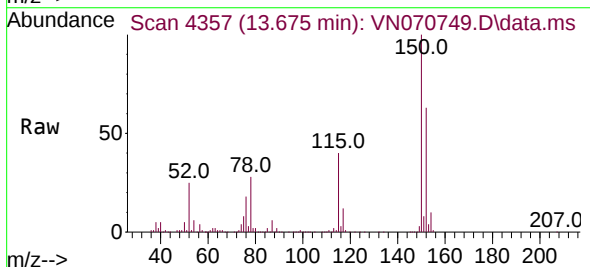




#74
N-amy1 acetate
Concen: 0.634 ug/l
RT: 12.390 min Scan# 31
Delta R.T. 0.005 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22




Instrument :
MSVOA_N
ClientSampleId :
72-72017ME


Tgt Ion: 43	Resp: 12122
Ion Ratio	Lower Upper
43 100	
70 35.8	33.4 50.0
55 27.3	19.3 28.9
61 21.2	18.5 27.7

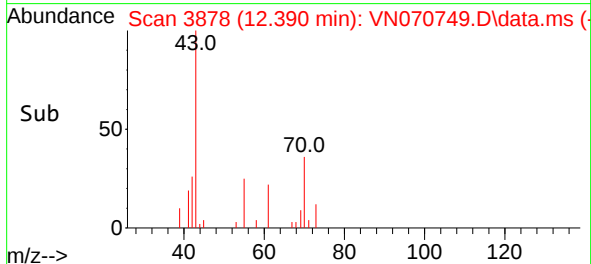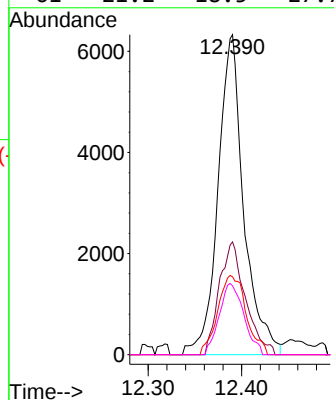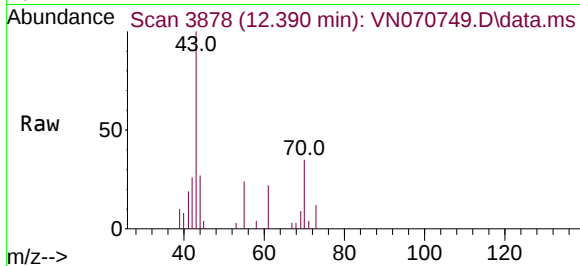

#76
1,2,3-Trichloropropane
Concen: 23.611 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.147 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22

Tgt Ion: 75	Resp: 309539
Ion Ratio	Lower Upper
75 100	
77 1.2	82.6 247.8#


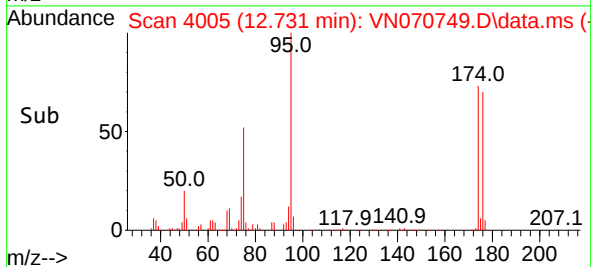
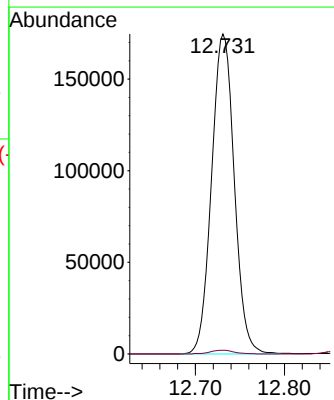
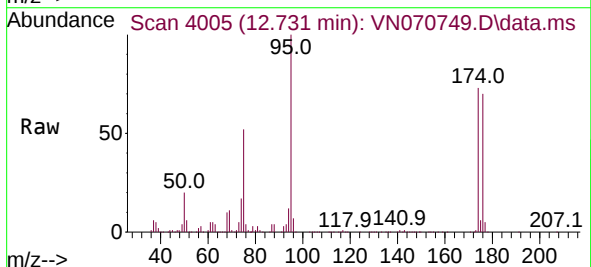


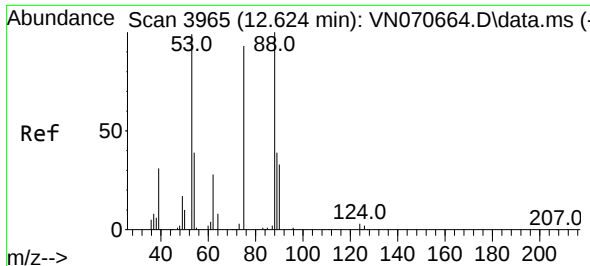

#81
trans-1,4-Dichloro-2-butene
Concen: 70.343 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.107 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22




Instrument :
MSVOA_N
ClientSampleId :
72-72017ME


Tgt Ion: 75 Resp: 309539
Ion Ratio Lower Upper
75 100
53 0.1 90.5 135.7#
89 0.0 38.2 57.4#

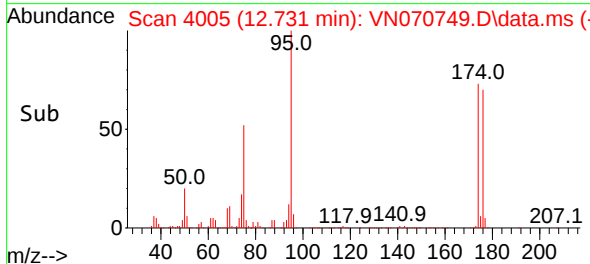

#84
1,2,4-Trimethylbenzene
Concen: 0.274 ug/l
RT: 13.366 min Scan# 4242
Delta R.T. -0.001 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22

Tgt Ion: 105 Resp: 9970
Ion Ratio Lower Upper
105 100
120 42.0 22.8 68.4


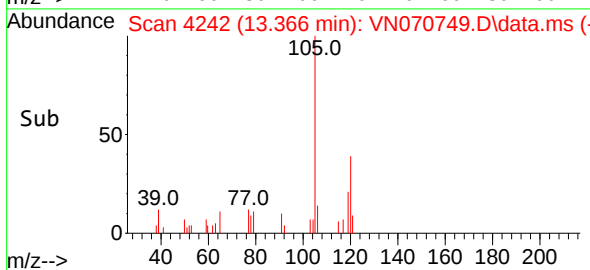

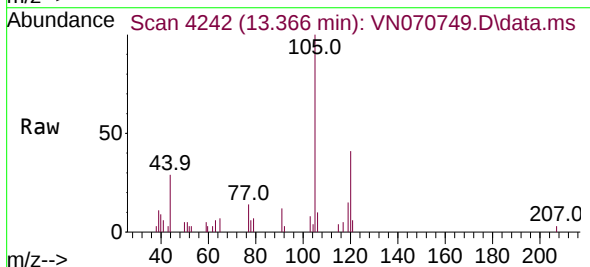


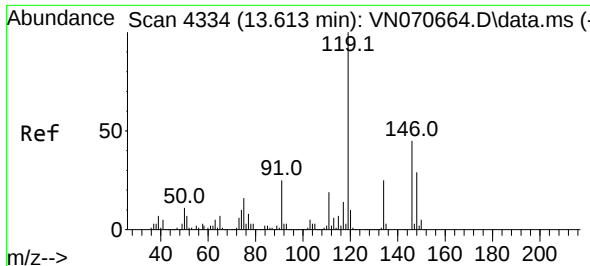

#87
1,3-Dichlorobenzene
Concen: 0.265 ug/l
RT: 13.616 min Scan# 4335
Delta R.T. 0.003 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22




Instrument :
MSVOA_N
ClientSampleId :
72-72017ME


Tgt Ion:146 Resp: 4626
Ion Ratio Lower Upper
146 100
111 43.5 18.6 55.6
148 59.3 31.6 95.0

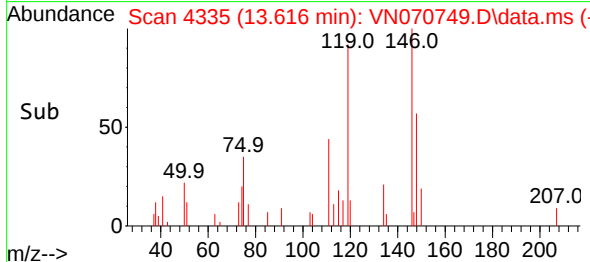

#88
1,4-Dichlorobenzene
Concen: 0.267 ug/l
RT: 13.616 min Scan# 4335
Delta R.T. -0.075 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22

Tgt Ion:146 Resp: 4626
Ion Ratio Lower Upper
146 100
111 43.5 18.3 54.8
148 59.3 31.8 95.4


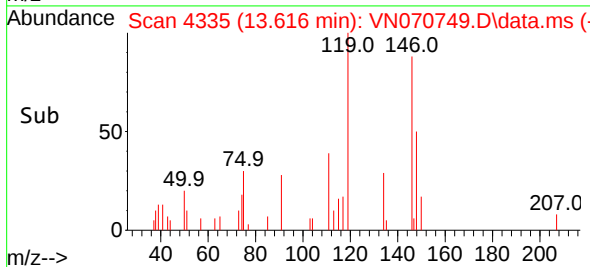

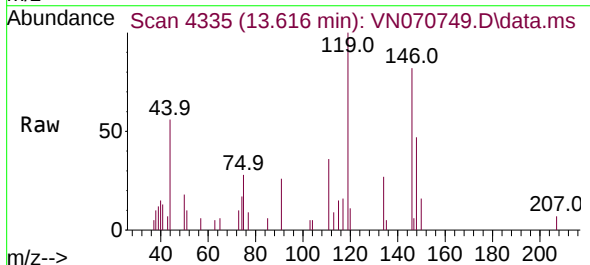




#89
n-Butylbenzene
Concen: 0.474 ug/l
RT: 13.943 min Scan# 4456
Delta R.T. 0.003 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22




Instrument :
MSVOA_N
ClientSampleId :
72-72017ME


Tgt Ion: 91 Resp: 13753
Ion Ratio Lower Upper
91 100
92 49.3 25.4 76.0
134 24.8 13.6 40.8

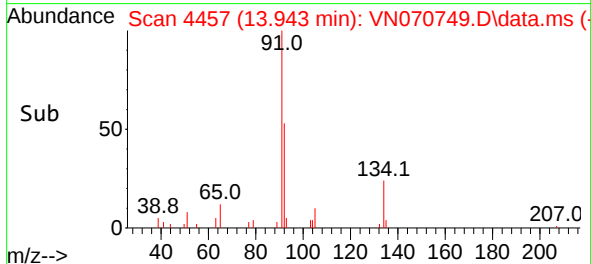

#91
1,2-Dichlorobenzene
Concen: 0.286 ug/l
RT: 13.983 min Scan# 4472
Delta R.T. -0.003 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22

Tgt Ion: 146 Resp: 4934
Ion Ratio Lower Upper
146 100
111 42.9 19.1 57.3
148 59.1 32.1 96.3

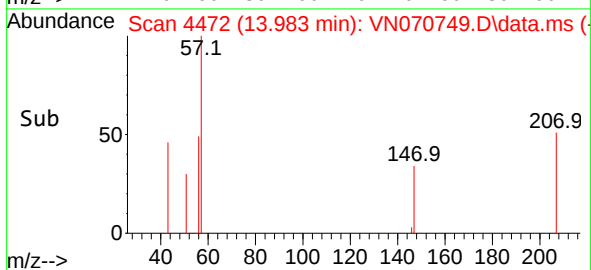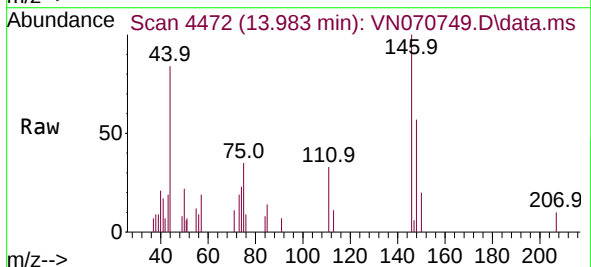

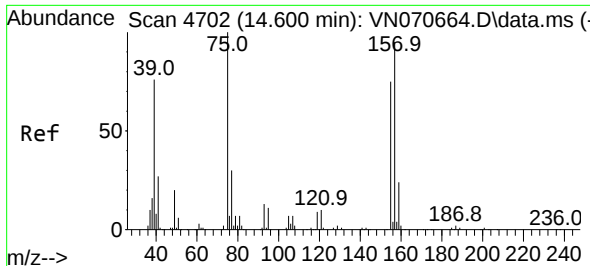

#92

1,2-Dibromo-3-Chloropropane

Concen: 0.446 ug/l

RT: 14.600 min Scan# 41

Delta R.T. 0.000 min

Lab File: VN070749.D

Acq: 24 Jan 2022 12:22

Instrument :

MSVOA_N

ClientSampleId :

72-72017ME





Tgt Ion: 75 Resp: 1196

Ion Ratio Lower Upper

75 100

155 59.9 46.9 140.7

157 76.5 60.6 181.7

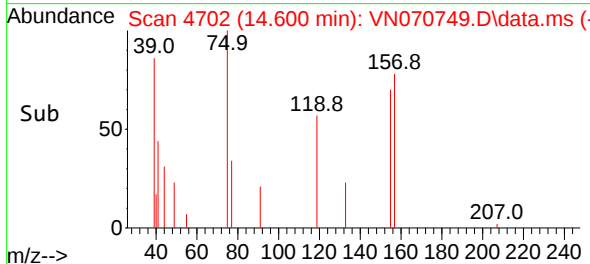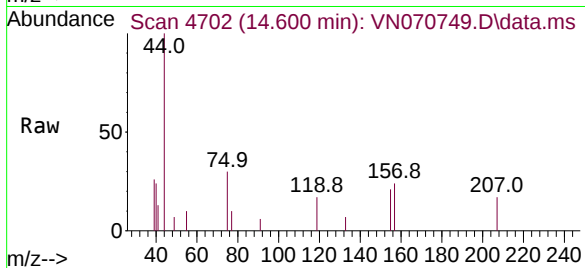

#93

1,2,4-Trichlorobenzene

Concen: 4.332 ug/l

RT: 15.263 min Scan# 4949

Delta R.T. -0.000 min

Lab File: VN070749.D

Acq: 24 Jan 2022 12:22




Tgt Ion: 180 Resp: 8891


Ion Ratio Lower Upper

180 100

182 91.1 48.3 144.9

145 28.8 14.5 43.5


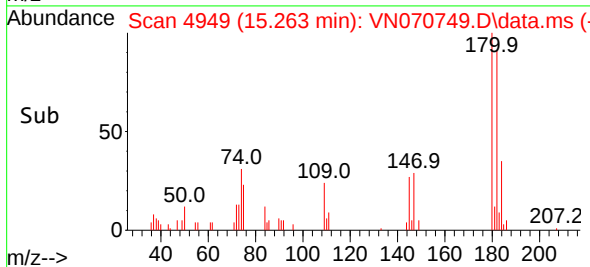

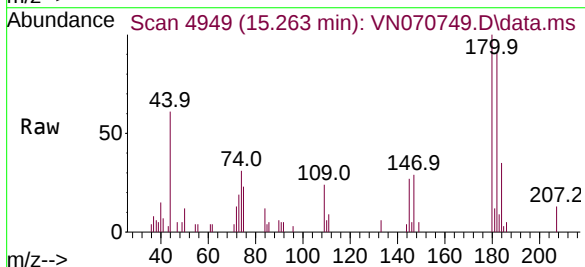




#94
Hexachlorobutadiene
Concen: 0.260 ug/l
RT: 15.370 min Scan# 4989
Delta R.T. 0.003 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22




Instrument :
MSVOA_N
ClientSampleId :
72-72017ME


Tgt Ion:225 Resp: 1328
Ion Ratio Lower Upper
225 100
223 32.5 31.9 95.7
227 27.8 32.1 96.3#

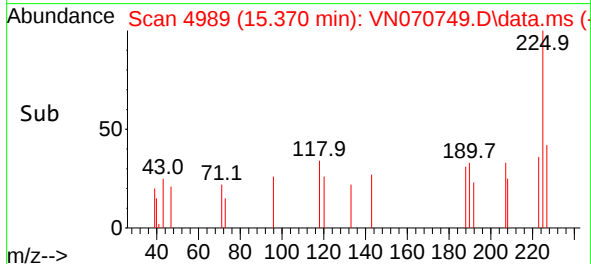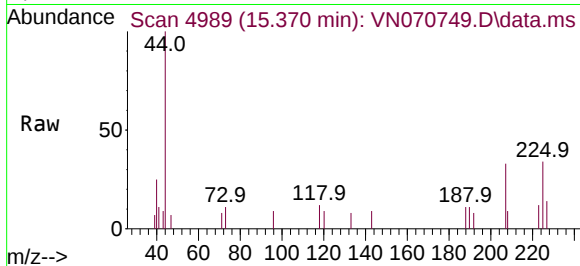

#95
Naphthalene
Concen: 6.026 ug/l
RT: 15.504 min Scan# 5039
Delta R.T. -0.000 min
Lab File: VN070749.D
Acq: 24 Jan 2022 12:22


Tgt Ion:128 Resp: 30651
Ion Ratio Lower Upper
128 100
127 14.9 10.5 15.7
129 10.5 8.7 13.1

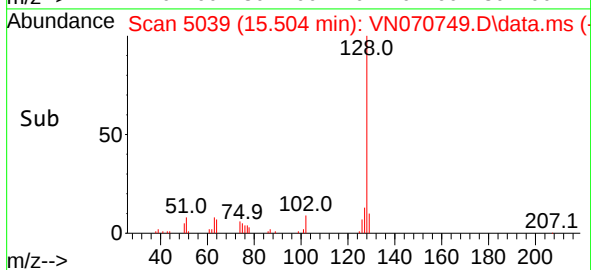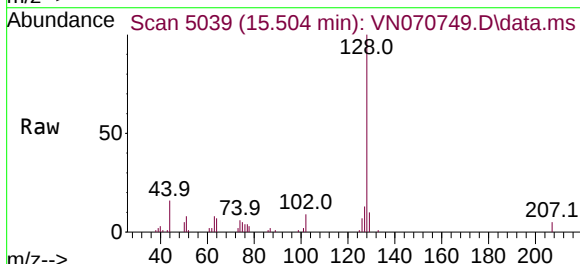



#96
 1,2,3-Trichlorobenzene
 Concen: 4.259 ug/l
 RT: 15.694 min Scan# 51
 Delta R.T. -0.003 min
 Lab File: VN070749.D
 Acq: 24 Jan 2022 12:22

Instrument :
 MSVOA_N
 ClientSampleId :
 72-72017ME

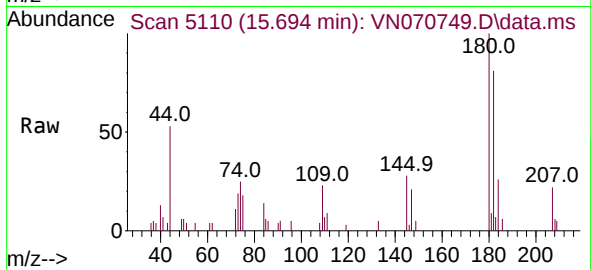

Tgt Ion:	180	Resp:	9732
Ion Ratio	Lower	Upper	
180	100		
182	91.7	47.4	142.2
145	16.5	15.0	45.1

