

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012422\
 Data File : VN070758.D
 Acq On : 24 Jan 2022 16:20
 Operator : JC/MD
 Sample : N1224-20
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 AREA-1-B-2@4-BGS

Quant Time: Jan 24 23:33:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 18 13:32:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.086	168	1002233	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.965	114	1627653	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	1453975	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	538415	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	684198	47.634	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	95.260%		
35) Dibromofluoromethane	8.021	113	467712	46.325	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	92.640%		
50) Toluene-d8	10.440	98	2016182	47.402	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	94.800%		
62) 4-Bromofluorobenzene	12.731	95	665514	43.909	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	87.820%		
Target Compounds						Qvalue
8) Diethyl Ether	3.829	74	2265	0.282	ug/l	90
13) Acrolein	4.036	56	1804	0.485	ug/l #	44
16) Acetone	4.291	43	167788	16.830	ug/l	99
18) Methyl Acetate	4.865	43	28322	1.445	ug/l #	81
20) Methylene Chloride	5.095	84	46363	3.531	ug/l	89
25) 2-Butanone	7.340	43	25058	1.997	ug/l #	87
29) Tetrahydrofuran	7.699	42	2631	0.343	ug/l #	46
31) Cyclohexane	8.083	56	22997	0.909	ug/l #	1
36) 1,1-Dichloropropene	8.083	75	82818	4.872	ug/l #	49
37) Ethyl Acetate	7.340	43	25058	1.110	ug/l #	68
38) Carbon Tetrachloride	8.086	117	101691	6.725	ug/l #	17
43) Isopropyl Acetate	8.563	43	139037	4.034	ug/l #	81
48) Methyl methacrylate	9.542	41	28509	1.736	ug/l #	8
51) 4-Methyl-2-Pentanone	10.330	43	21450	0.975	ug/l	95
53) t-1,3-Dichloropropene	10.620	75	137	2.410	ug/l #	43
54) cis-1,3-Dichloropropene	10.242	75	151752	7.430	ug/l #	62
55) 1,1,2-Trichloroethane	10.878	97	5265	0.425	ug/l #	19
56) Ethyl methacrylate	10.784	69	2571	2.406	ug/l #	31
57) 1,3-Dichloropropane	11.089	76	83391	3.806	ug/l #	43
59) 2-Hexanone	11.089	43	1404277	87.894	ug/l #	49
73) Isopropylbenzene	12.578	105	36937	0.725	ug/l	99
76) 1,2,3-Trichloropropane	12.728	75	351842	24.638	ug/l #	1
78) n-propylbenzene	12.919	91	14372	0.252	ug/l	92
79) 2-Chlorotoluene	12.919	91	14372	0.399	ug/l #	38
81) trans-1,4-Dichloro-2-b...	12.728	75	351842	73.402	ug/l #	5
90) Hexachloroethane	14.217	117	4649	0.695	ug/l #	6
93) 1,2,4-Trichlorobenzene	15.271	180	491	3.471	ug/l #	1
95) Naphthalene	15.509	128	3592	5.064	ug/l #	87
96) 1,2,3-Trichlorobenzene	15.694	180	196	3.235	ug/l #	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012422\
Data File : VN070758.D
Acq On : 24 Jan 2022 16:20
Operator : JC/MD
Sample : N1224-20
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-BGS

Quant Time: Jan 24 23:33:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 18 13:32:07 2022
Response via : Initial Calibration




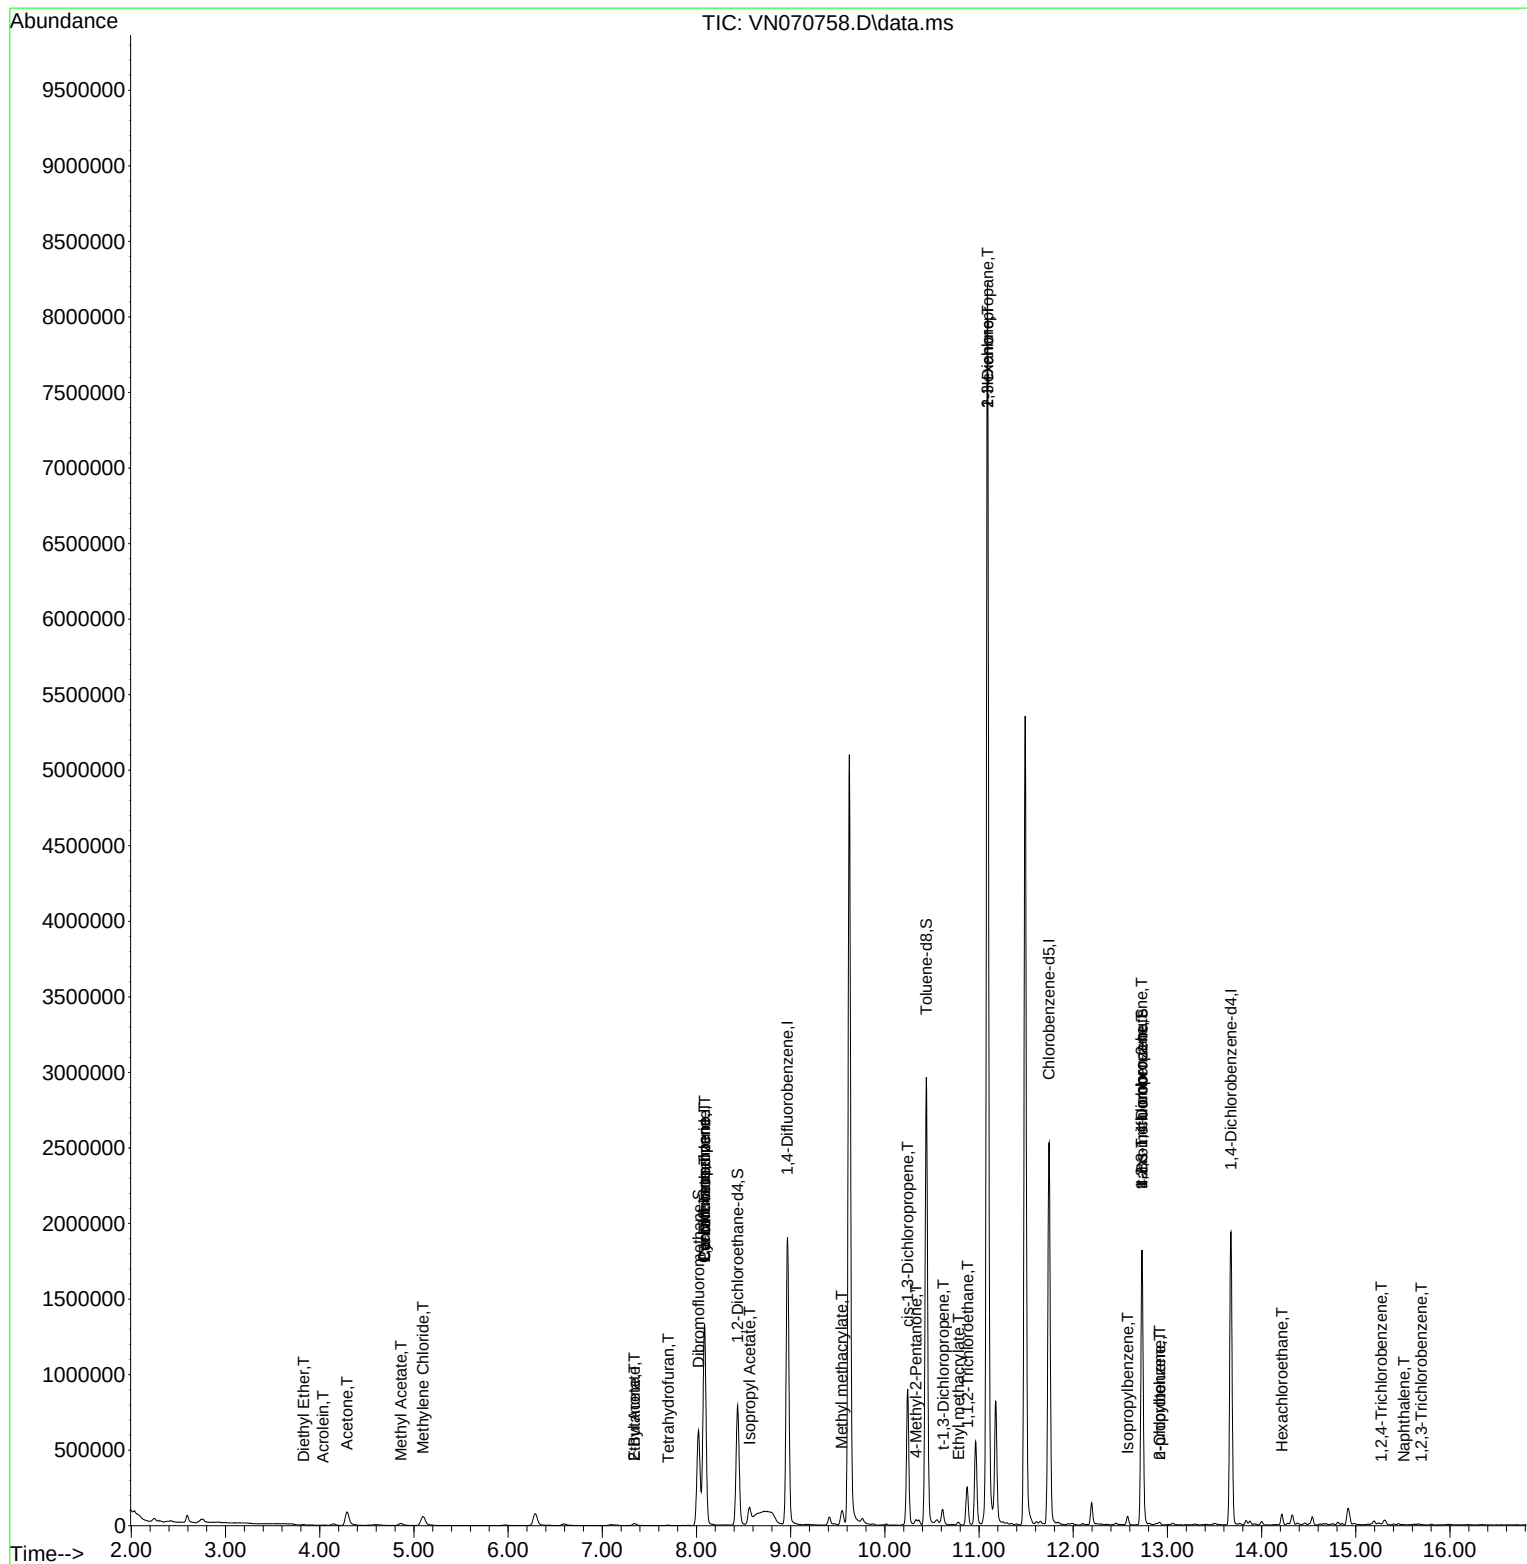




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 21
Delta R.T. 0.003 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-BGS


Tgt Ion:168 Resp: 1002233
Ion Ratio Lower Upper
168 100
99 60.4 41.3 61.9

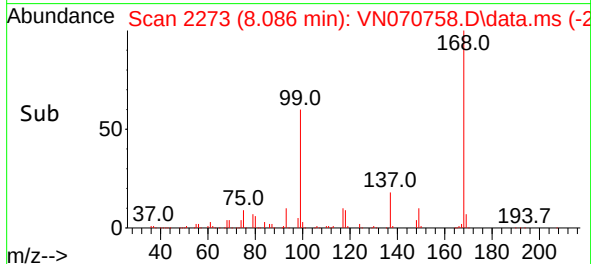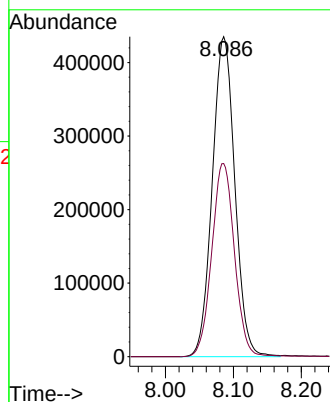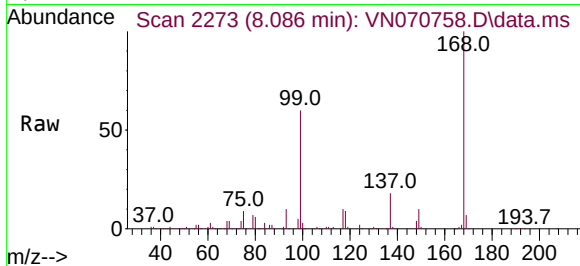

#8
Diethyl Ether
Concen: 0.282 ug/l
RT: 3.829 min Scan# 686
Delta R.T. 0.005 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20

Tgt Ion: 74 Resp: 2265
Ion Ratio Lower Upper
74 100
45 84.6 47.0 141.2


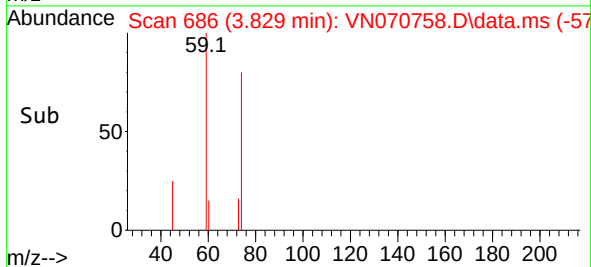
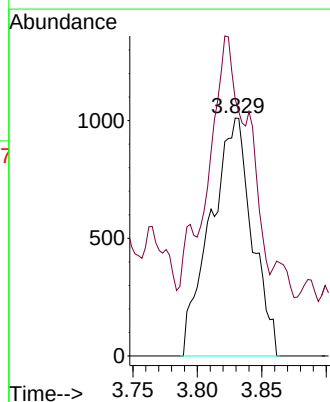
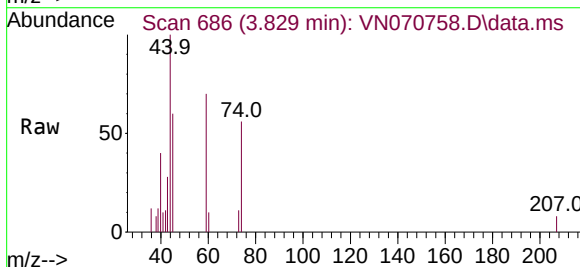




#13
Acrolein
Concen: 0.485 ug/l
RT: 4.036 min Scan# 763
Delta R.T. -0.003 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-BGS


Tgt Ion: 56 Resp: 1804
Ion Ratio Lower Upper
56 100
55 24.8 56.6 85.0#

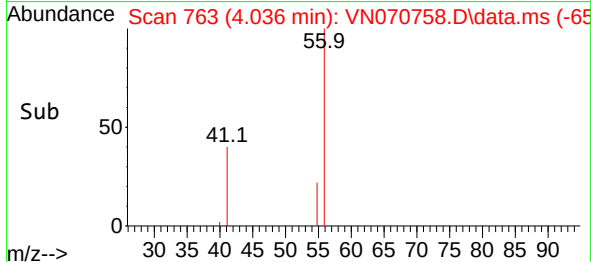

#16
Acetone
Concen: 16.830 ug/l
RT: 4.291 min Scan# 858
Delta R.T. 0.006 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20

Tgt Ion: 43 Resp: 167788
Ion Ratio Lower Upper
43 100
58 28.5 23.1 34.7

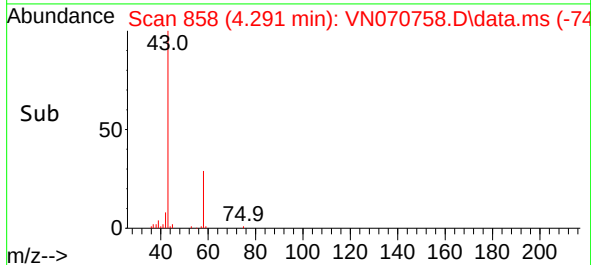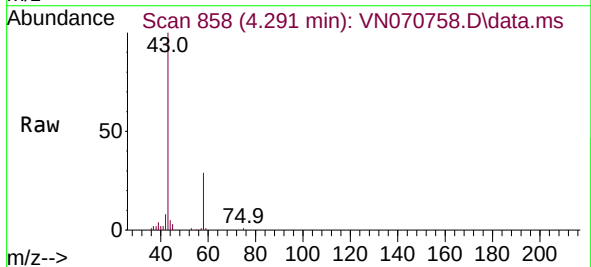



#18

Methyl Acetate

Concen: 1.445 ug/l

RT: 4.865 min Scan# 1107

Delta R.T. 0.011 min

Lab File: VN070758.D

Acq: 24 Jan 2022 16:20

Instrument :

MSVOA_N

ClientSampleId :





AREA-1-B-2@4-BGS

Tgt Ion: 43 Resp: 28322

Ion Ratio Lower Upper

43 100

74 14.7 19.4 29.2#

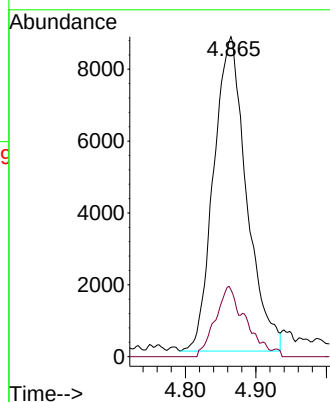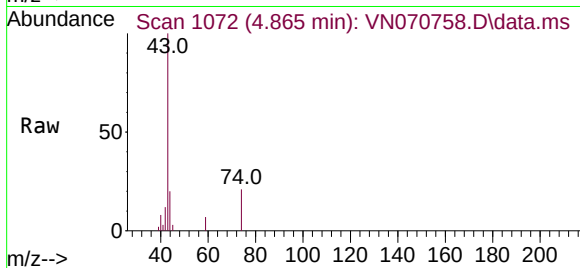

#20

Methylene Chloride

Concen: 3.531 ug/l

RT: 5.095 min Scan# 1158

Delta R.T. 0.000 min

Lab File: VN070758.D

Acq: 24 Jan 2022 16:20

Tgt Ion: 84 Resp: 46363




Ion Ratio Lower Upper


84 100

49 136.3 93.5 140.3

51 40.6 29.4 44.2

86 64.7 53.0 79.4

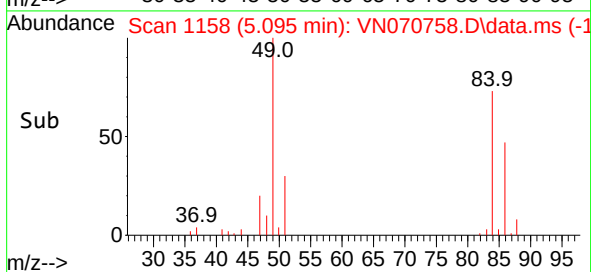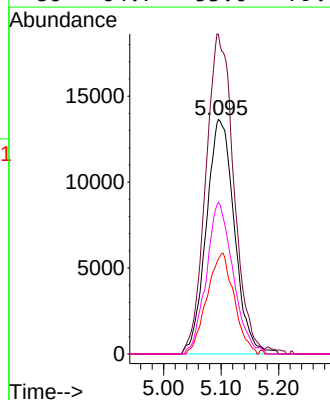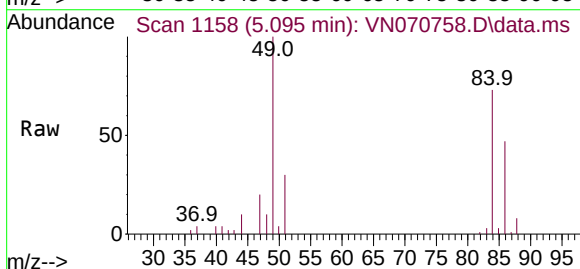

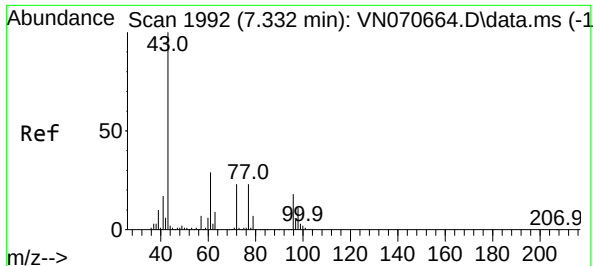

#25

2-Butanone

Concen: 1.997 ug/l

RT: 7.340 min Scan# 1992

Delta R.T. 0.008 min

Lab File: VN070758.D

Acq: 24 Jan 2022 16:20

Instrument :

MSVOA_N

ClientSampleId :





AREA-1-B-2@4-BGS

Tgt Ion: 43 Resp: 25058

Ion Ratio Lower Upper

43 100

72 20.5 21.7 32.5#

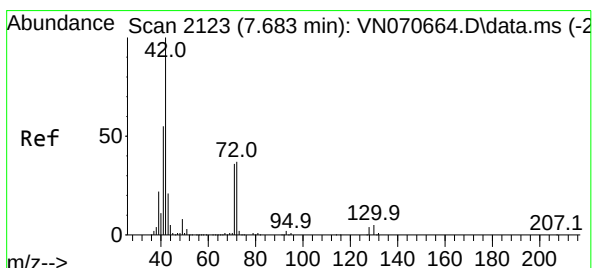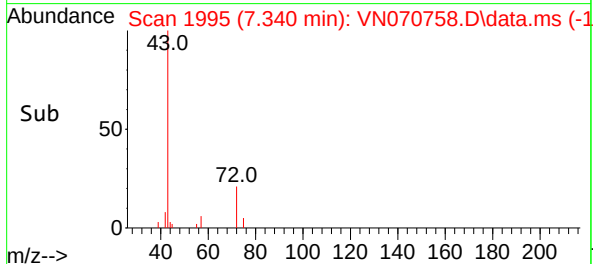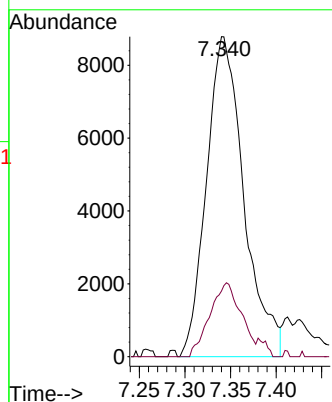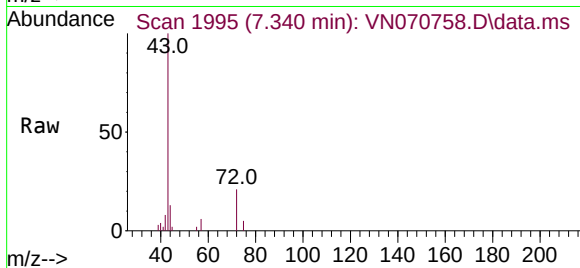

#29

Tetrahydrofuran

Concen: 0.343 ug/l

RT: 7.699 min Scan# 2129

Delta R.T. 0.016 min

Lab File: VN070758.D

Acq: 24 Jan 2022 16:20




Tgt Ion: 42 Resp: 2631


Ion Ratio Lower Upper

42 100

72 5.3 36.3 54.5#

71 13.5 34.7 52.1#


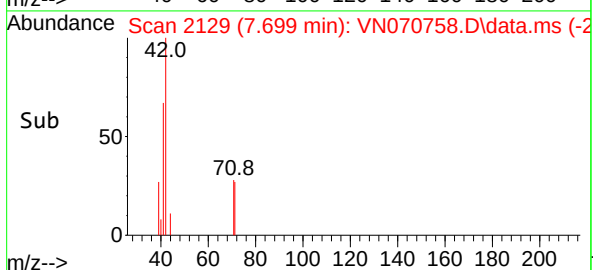

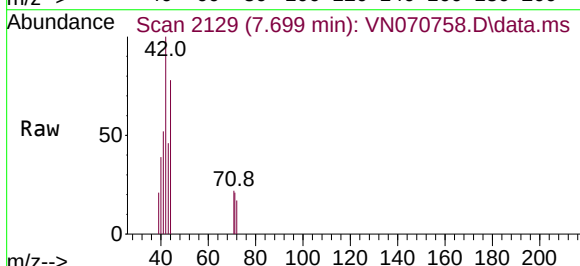




#31
Cyclohexane
Concen: 0.909 ug/l
RT: 8.083 min Scan# 21
Delta R.T. -0.011 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-BGS


Tgt Ion: 56 Resp: 22997
Ion Ratio Lower Upper
56 100
69 184.2 27.1 40.7#
84 143.9 73.4 110.0#

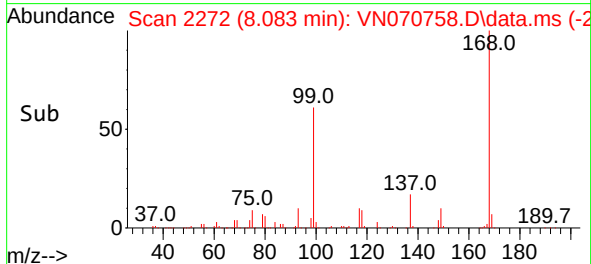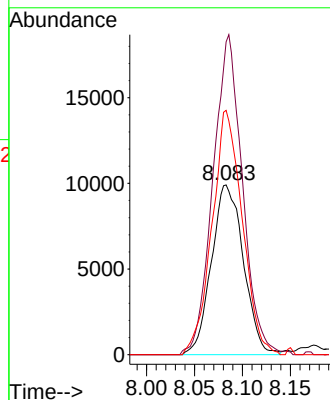

#33
1,2-Dichloroethane-d4
Concen: 47.634 ug/l
RT: 8.437 min Scan# 2404
Delta R.T. 0.003 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20

Tgt Ion: 65 Resp: 684198
Ion Ratio Lower Upper
65 100
67 52.0 0.0 103.0

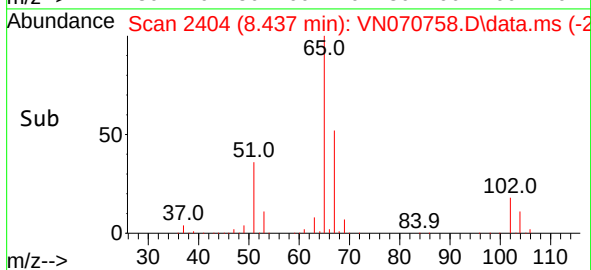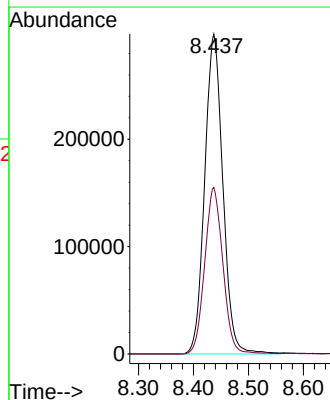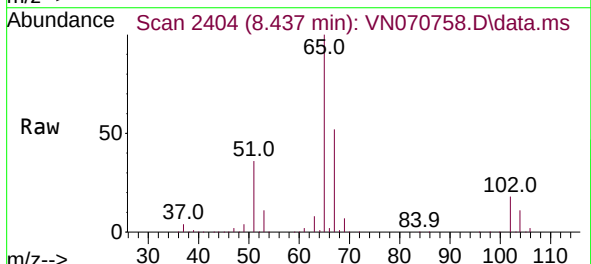



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.965 min Scan# 2601

Delta R.T. 0.000 min

Lab File: VN070758.D

Acq: 24 Jan 2022 16:20

Instrument :

MSVOA_N

ClientSampleId :

AREA-1-B-2@4-BGS





Tgt Ion:114 Resp: 1627653

Ion Ratio Lower Upper

114 100

63 23.5 0.0 37.8

88 16.6 0.0 27.4

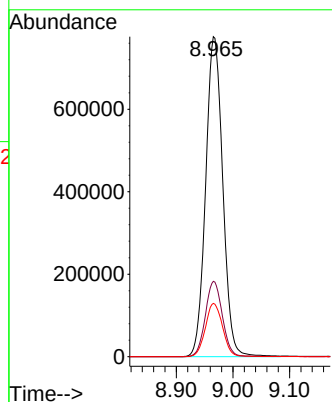

#35

Dibromofluoromethane

Concen: 46.325 ug/l

RT: 8.021 min Scan# 2249

Delta R.T. 0.002 min

Lab File: VN070758.D

Acq: 24 Jan 2022 16:20




Tgt Ion:113 Resp: 467712


Ion Ratio Lower Upper

113 100

111 102.6 82.2 123.2

192 19.1 16.9 25.3


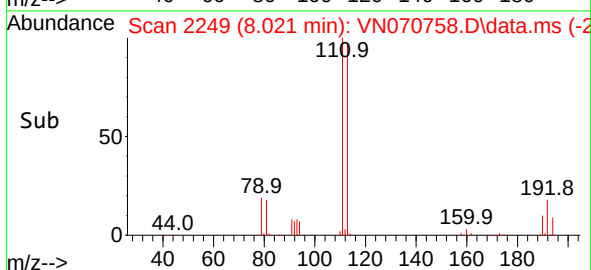






#36
 1,1-Dichloropropene
 Concen: 4.872 ug/l
 RT: 8.083 min Scan# 21
 Delta R.T. -0.137 min
 Lab File: VN070758.D
 Acq: 24 Jan 2022 16:20




Instrument :
 MSVOA_N
 ClientSampleId :
 AREA-1-B-2@4-BGS


Tgt Ion: 75 Resp: 82818
 Ion Ratio Lower Upper
 75 100
 110 8.7 18.4 55.2#
 77 0.0 24.4 36.6#

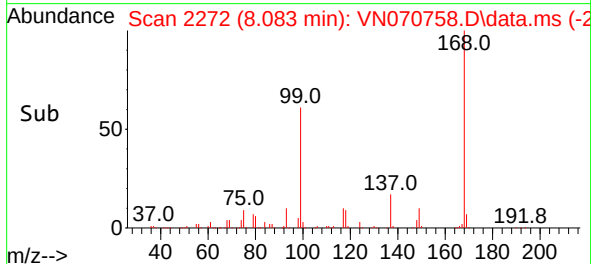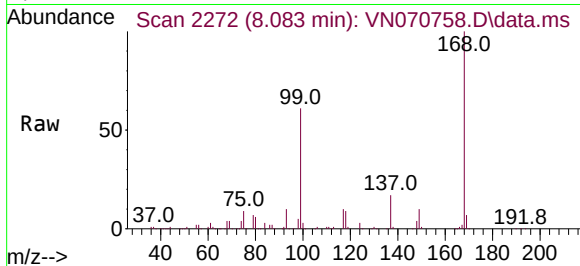

#37
 Ethyl Acetate
 Concen: 1.110 ug/l
 RT: 7.340 min Scan# 1995
 Delta R.T. -0.070 min
 Lab File: VN070758.D
 Acq: 24 Jan 2022 16:20

Tgt Ion: 43 Resp: 25058
 Ion Ratio Lower Upper
 43 100
 61 0.0 11.5 17.3#
 70 0.1 7.9 11.9#


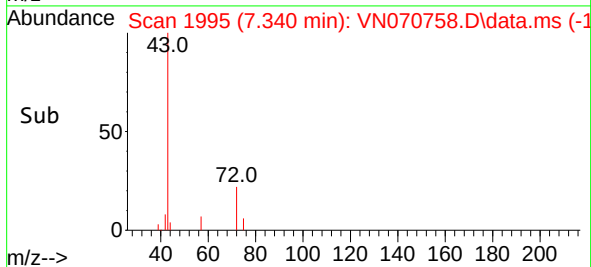

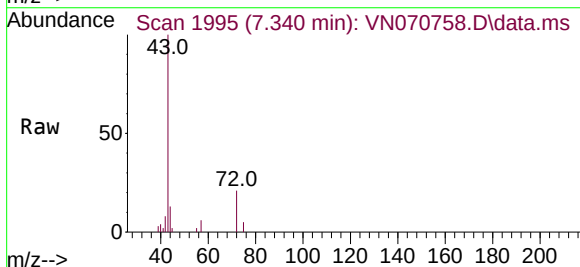




#38
Carbon Tetrachloride
Concen: 6.725 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.120 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-BGS


Tgt Ion:117 Resp: 101691
Ion Ratio Lower Upper
117 100
119 5.5 76.1 114.1#
121 0.0 24.2 36.2#

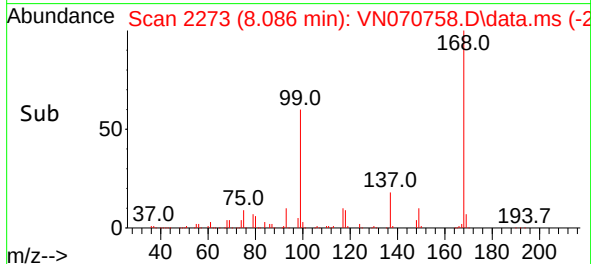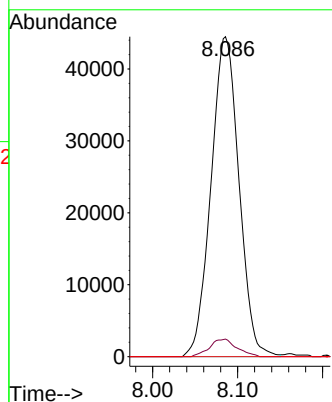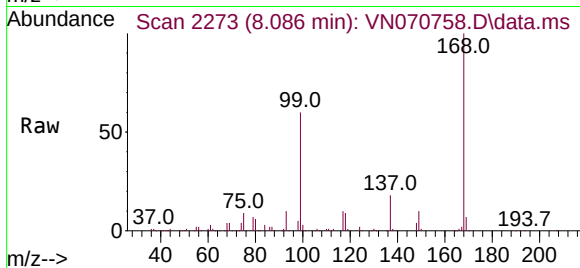

#43
Isopropyl Acetate
Concen: 4.034 ug/l
RT: 8.563 min Scan# 2451
Delta R.T. 0.003 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20

Tgt Ion: 43 Resp: 139037
Ion Ratio Lower Upper
43 100
61 14.4 20.4 30.6#
87 8.8 11.2 16.8#


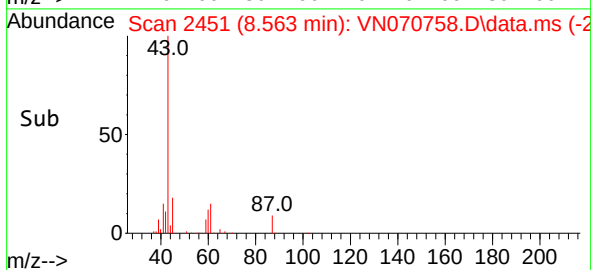
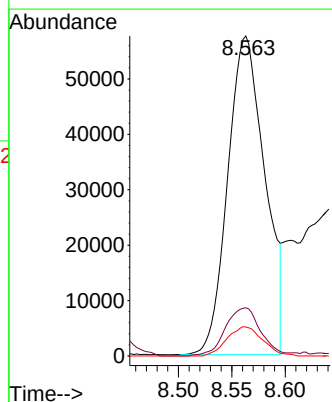
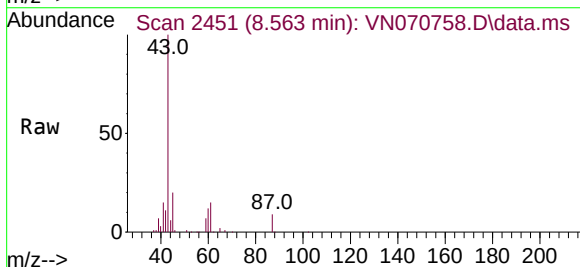




#48
Methyl methacrylate
Concen: 1.736 ug/l
RT: 9.542 min Scan# 21
Delta R.T. -0.016 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-BGS


Tgt Ion: 41 Resp: 28509
Ion Ratio Lower Upper
41 100
69 0.0 72.4 108.6#
39 0.0 58.4 87.6#

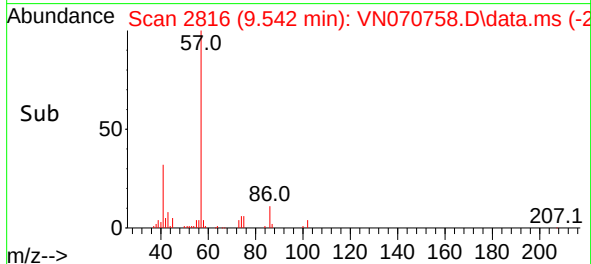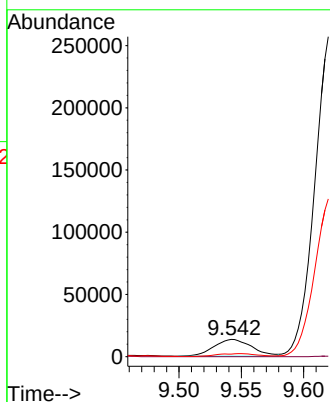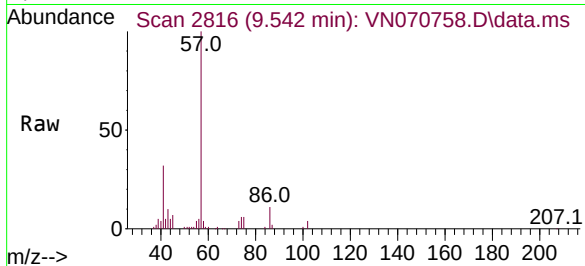

#50
Toluene-d8
Concen: 47.402 ug/l
RT: 10.440 min Scan# 3151
Delta R.T. 0.002 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20

Tgt Ion: 98 Resp: 2016182
Ion Ratio Lower Upper
98 100
100 64.5 50.4 75.6


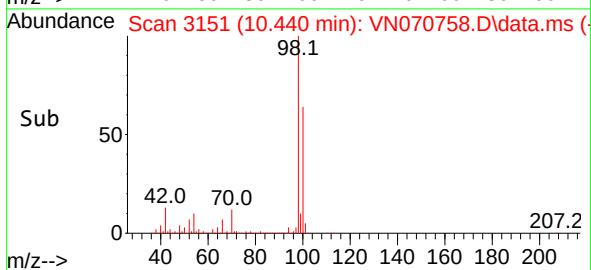
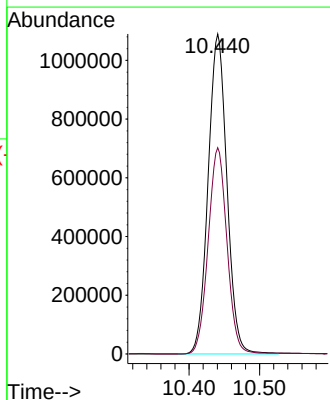
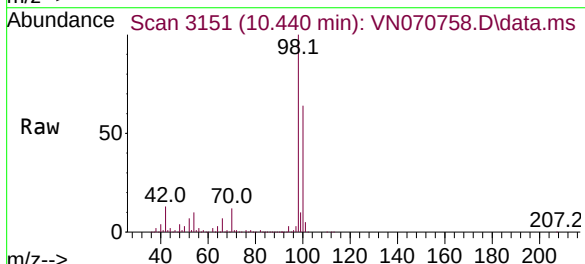


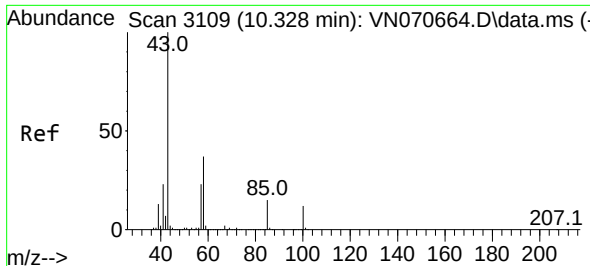

#51
4-Methyl-2-Pentanone
Concen: 0.975 ug/l
RT: 10.330 min Scan# 3109
Delta R.T. 0.002 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-BGS


Tgt Ion: 43 Resp: 21450
Ion Ratio Lower Upper
43 100
58 41.0 30.4 45.6

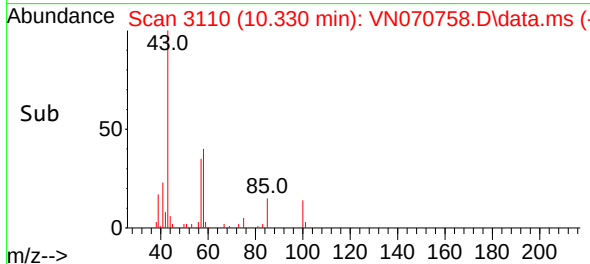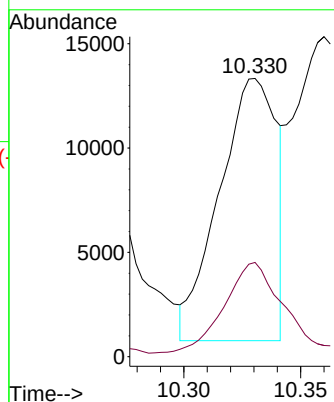

#53
t-1,3-Dichloropropene
Concen: 2.410 ug/l
RT: 10.620 min Scan# 3218
Delta R.T. -0.097 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20

Tgt Ion: 75 Resp: 137
Ion Ratio Lower Upper
75 100
77 0.0 25.6 38.4#


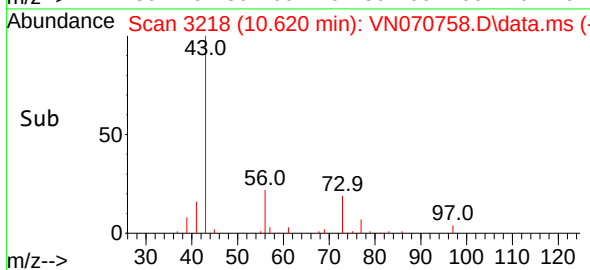
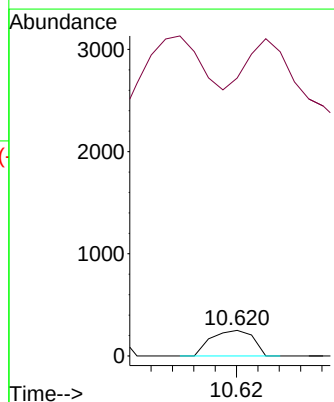
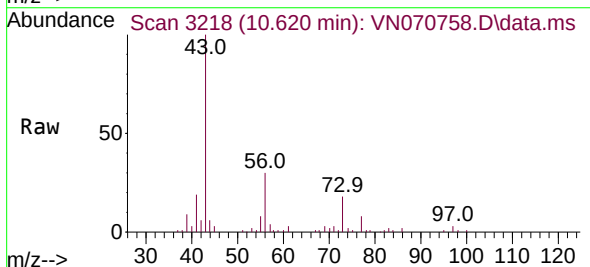


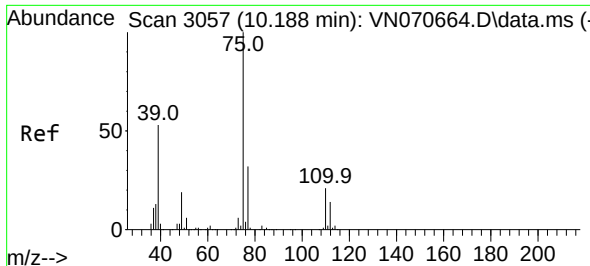

#54
 cis-1,3-Dichloropropene
 Concen: 7.430 ug/l
 RT: 10.242 min Scan# 3057
 Delta R.T. 0.054 min
 Lab File: VN070758.D
 Acq: 24 Jan 2022 16:20




Instrument :
 MSVOA_N
 ClientSampleId :
 AREA-1-B-2@4-BGS


Tgt Ion: 75 Resp: 151752
 Ion Ratio Lower Upper
 75 100
 77 0.6 26.4 39.6#
 39 35.0 42.5 63.7#

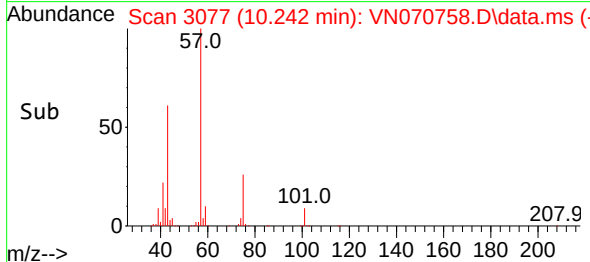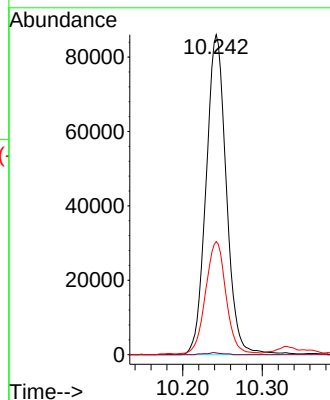

#55
 1,1,2-Trichloroethane
 Concen: 0.425 ug/l
 RT: 10.878 min Scan# 3314
 Delta R.T. -0.018 min
 Lab File: VN070758.D
 Acq: 24 Jan 2022 16:20

Tgt Ion: 97 Resp: 5265
 Ion Ratio Lower Upper
 97 100
 83 7.5 67.8 101.6#
 85 0.0 45.4 68.2#
 99 0.0 49.4 74.0#


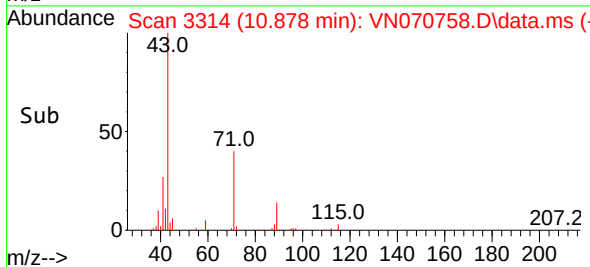
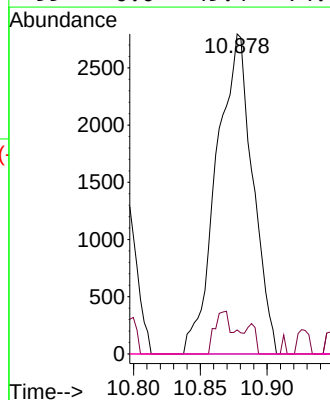
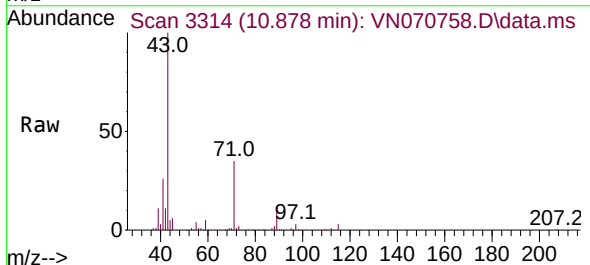




#56
Ethyl methacrylate
Concen: 2.406 ug/l
RT: 10.784 min Scan# 31
Delta R.T. 0.024 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-BGS


Tgt Ion: 69 Resp: 2571
Ion Ratio Lower Upper
69 100
41 119.1 51.4 77.0#
39 0.0 34.6 52.0#

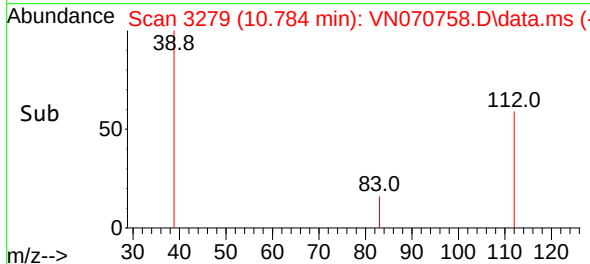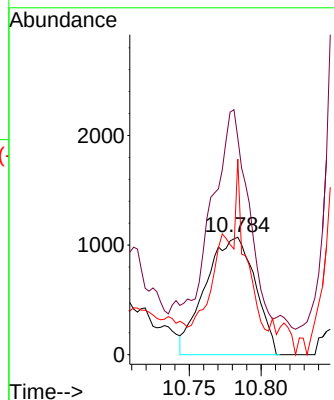

#57
1,3-Dichloropropane
Concen: 3.806 ug/l
RT: 11.089 min Scan# 3393
Delta R.T. 0.045 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20

Tgt Ion: 76 Resp: 83391
Ion Ratio Lower Upper
76 100
78 0.4 25.7 38.5#


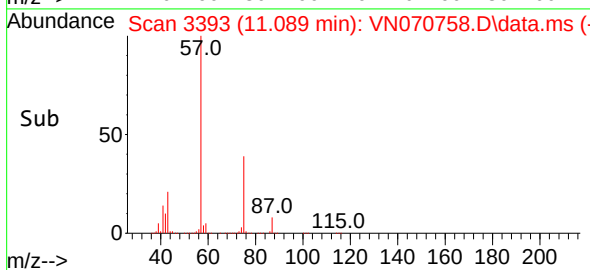
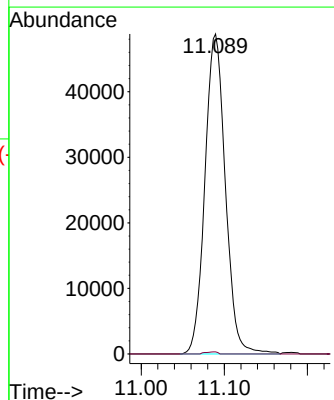
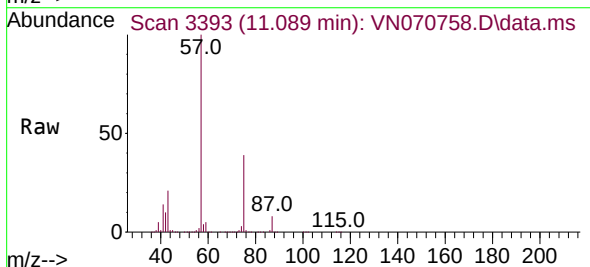


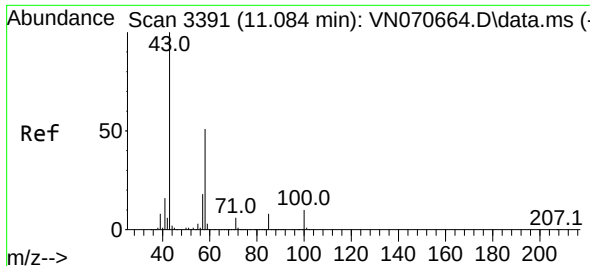

#59
2-Hexanone
Concen: 87.894 ug/l
RT: 11.089 min Scan# 311
Delta R.T. 0.005 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-BGS


Tgt Ion: 43 Resp: 1404277
Ion Ratio Lower Upper
43 100
58 17.0 26.9 80.7#

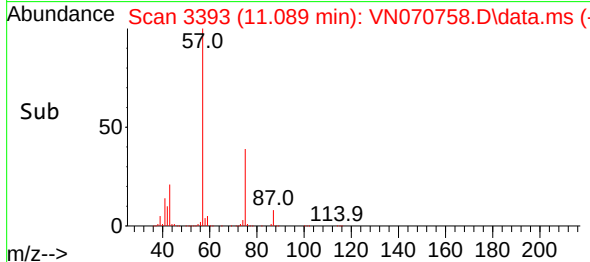

#62
4-Bromofluorobenzene
Concen: 43.909 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.003 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20

Tgt Ion: 95 Resp: 665514
Ion Ratio Lower Upper
95 100
174 74.9 0.0 187.2
176 71.2 0.0 181.4


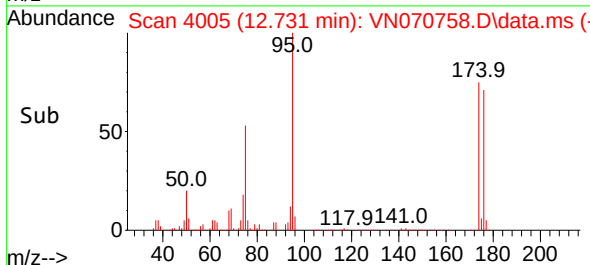
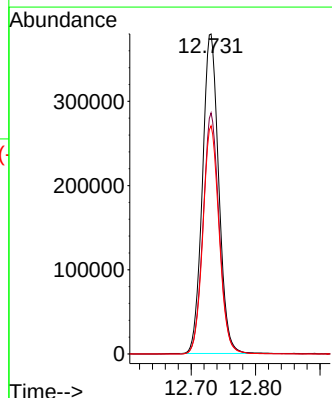
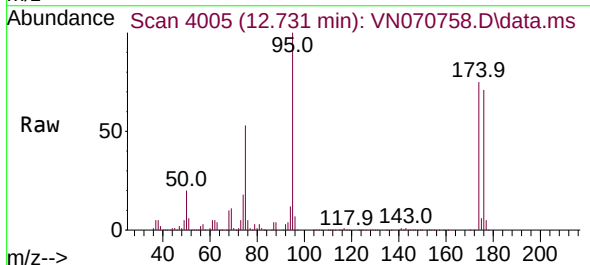


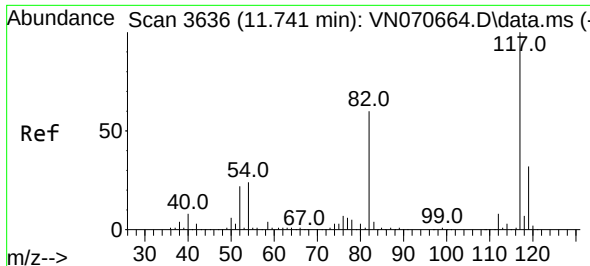

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3636
Delta R.T. 0.003 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-BGS


Tgt Ion:117 Resp: 1453975
Ion Ratio Lower Upper
117 100
82 60.4 42.4 63.6
119 32.0 25.4 38.2

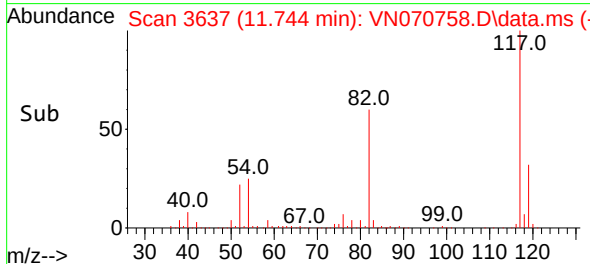

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 4357
Delta R.T. 0.003 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20

Tgt Ion:152 Resp: 538415
Ion Ratio Lower Upper
152 100
115 62.1 27.5 82.5
150 157.1 0.0 344.4


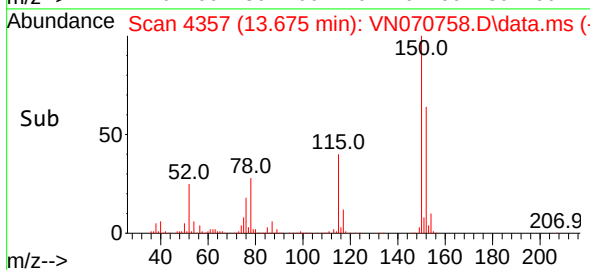

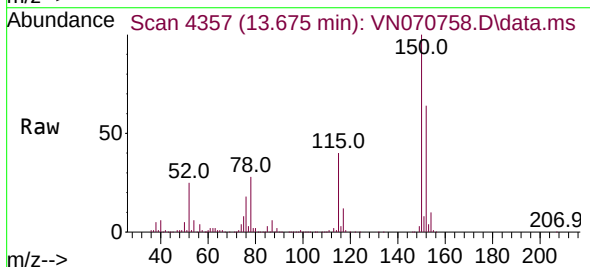


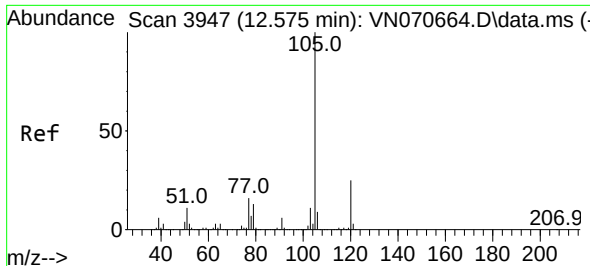

#73
Isopropylbenzene
Concen: 0.725 ug/l
RT: 12.578 min Scan# 3947
Delta R.T. 0.003 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-BGS


Tgt Ion:105 Resp: 36937
Ion Ratio Lower Upper
105 100
120 26.0 13.4 40.1

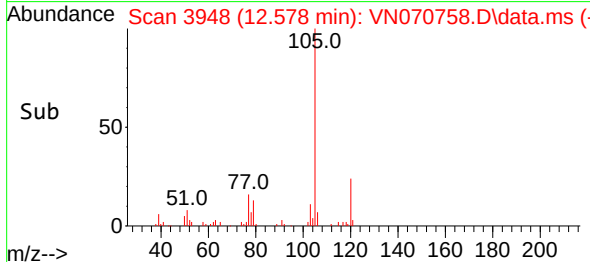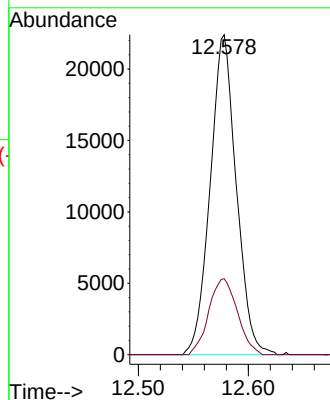

#76
1,2,3-Trichloropropane
Concen: 24.638 ug/l
RT: 12.728 min Scan# 4004
Delta R.T. -0.150 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20

Tgt Ion: 75 Resp: 351842
Ion Ratio Lower Upper
75 100
77 1.2 82.6 247.8#


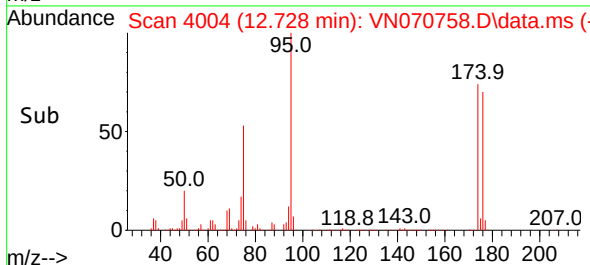
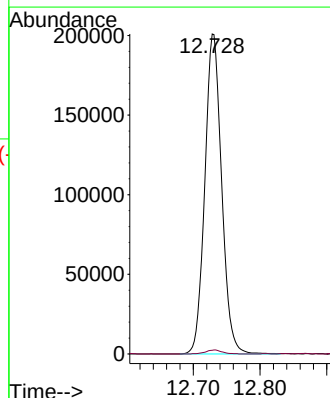
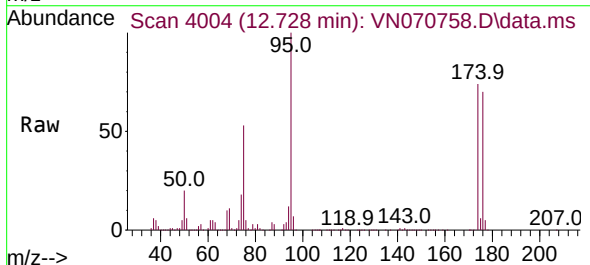




#78
n-propylbenzene
Concen: 0.252 ug/l
RT: 12.919 min Scan# 4075
Delta R.T. -0.000 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-BGS


Tgt Ion: 91 Resp: 14372
Ion Ratio Lower Upper
91 100
120 20.1 11.9 35.9

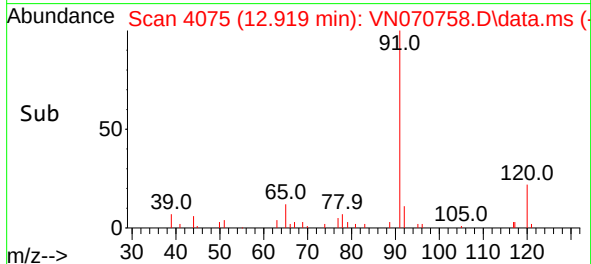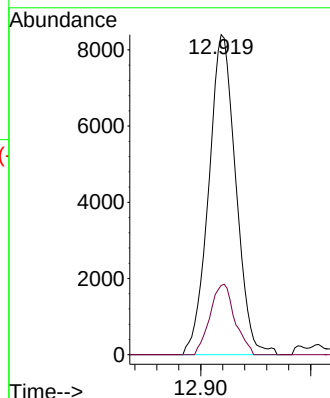

#79
2-Chlorotoluene
Concen: 0.399 ug/l
RT: 12.919 min Scan# 4075
Delta R.T. -0.085 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20

Tgt Ion: 91 Resp: 14372
Ion Ratio Lower Upper
91 100
126 0.0 18.3 54.8#



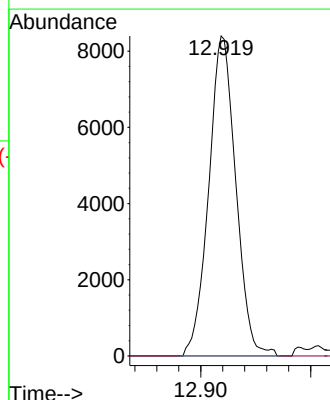
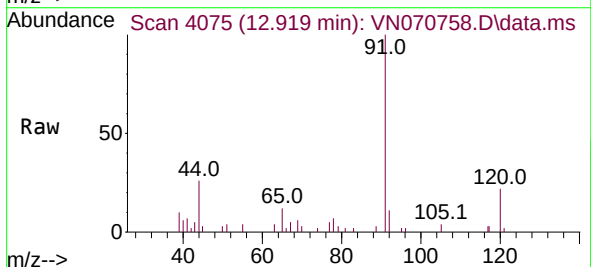


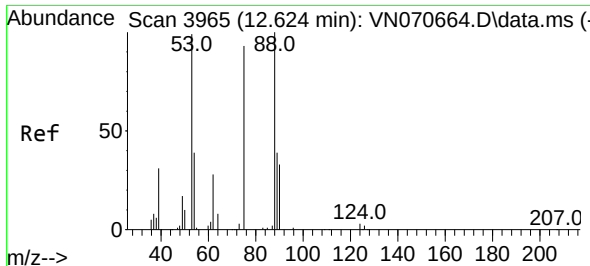

#81
trans-1,4-Dichloro-2-butene
Concen: 73.402 ug/l
RT: 12.728 min Scan# 4004
Delta R.T. 0.104 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-BGS


Tgt Ion: 75 Resp: 351842
Ion Ratio Lower Upper
75 100
53 0.1 90.5 135.7#
89 0.0 38.2 57.4#

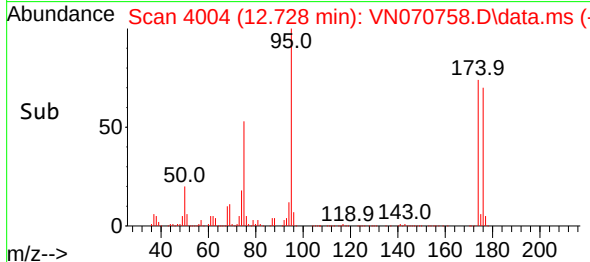

#90
Hexachloroethane
Concen: 0.695 ug/l
RT: 14.217 min Scan# 4559
Delta R.T. 0.008 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20

Tgt Ion: 117 Resp: 4649
Ion Ratio Lower Upper
117 100
201 0.0 43.9 131.6#


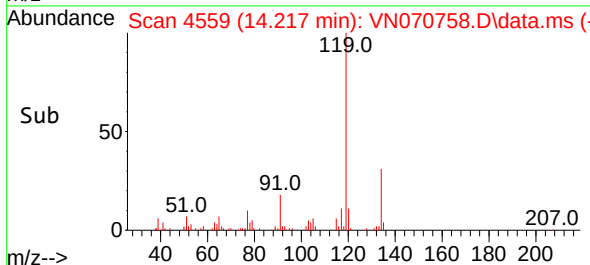
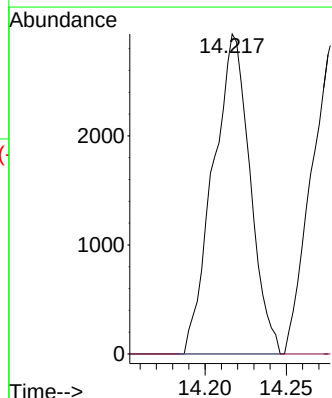
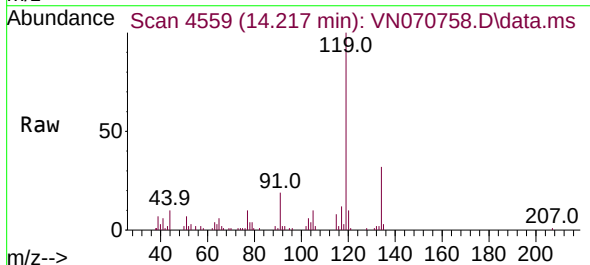


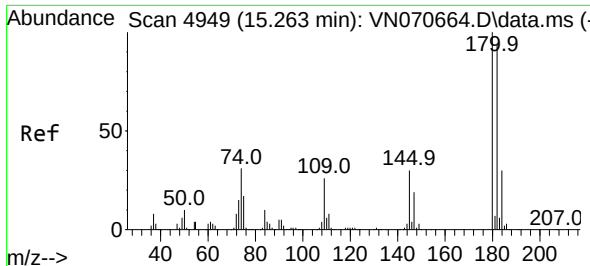

#93
1,2,4-Trichlorobenzene
Concen: 3.471 ug/l
RT: 15.271 min Scan# 4949
Delta R.T. 0.008 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-BGS


Tgt Ion:180 Resp: 491
Ion Ratio Lower Upper
180 100
182 120.2 48.3 144.9
145 723.0 14.5 43.5#

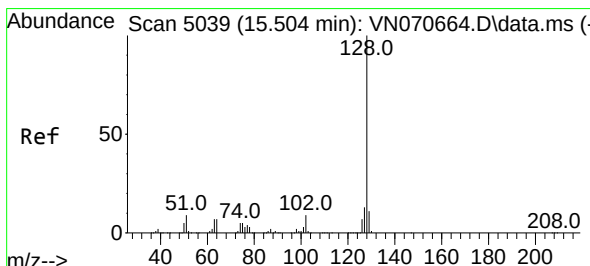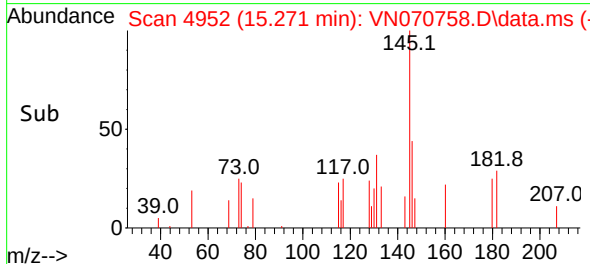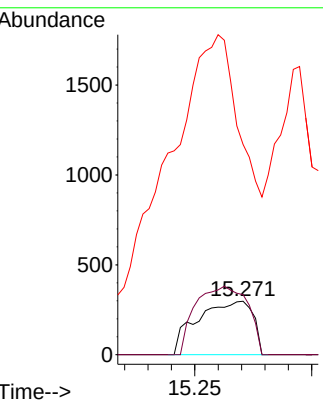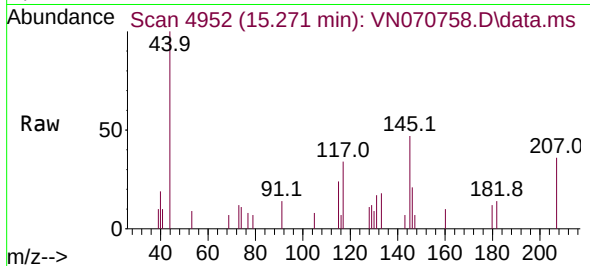

#95
Naphthalene
Concen: 5.064 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.005 min
Lab File: VN070758.D
Acq: 24 Jan 2022 16:20


Tgt Ion:128 Resp: 3592
Ion Ratio Lower Upper
128 100
127 6.4 10.5 15.7#
129 7.8 8.7 13.1#

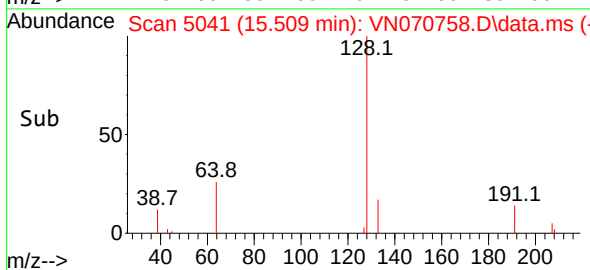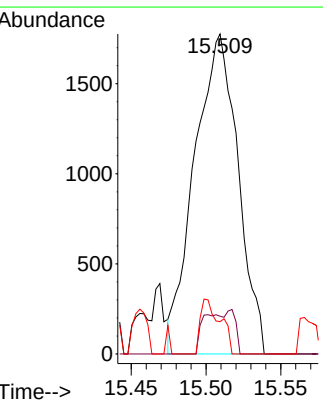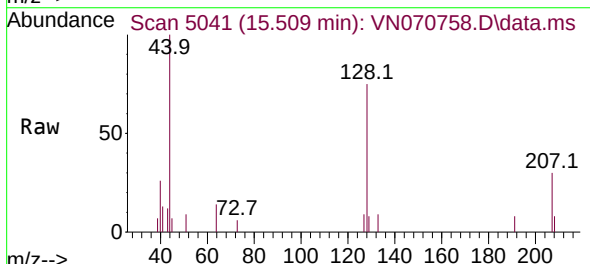



#96
 1,2,3-Trichlorobenzene
 Concen: 3.235 ug/l
 RT: 15.694 min Scan# 51
 Delta R.T. -0.003 min
 Lab File: VN070758.D
 Acq: 24 Jan 2022 16:20

Instrument :
 MSVOA_N
 ClientSampleId :
 AREA-1-B-2@4-BGS

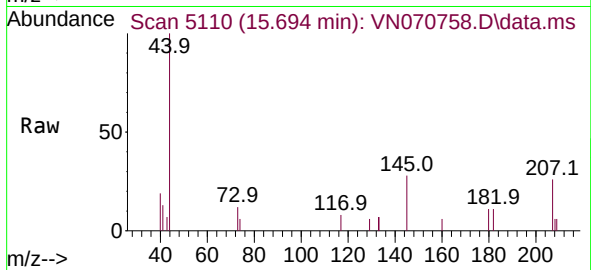

Tgt Ion:180 Resp: 196
 Ion Ratio Lower Upper
 180 100
 182 0.0 47.4 142.2#
 145 0.0 15.0 45.1#

