

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012423\
 Data File : VN076372.D
 Acq On : 24 Jan 2023 10:40
 Operator : JC\MD
 Sample : VN0124MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0124MBL01

Quant Time: Jan 25 00:33:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 17 03:59:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	349339	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	551653	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	459537	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	178892	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	194669	49.768	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	99.540%
35) Dibromofluoromethane	8.177	113	166815	48.341	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.680%
50) Toluene-d8	10.571	98	631407	49.544	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	99.080%
62) 4-Bromofluorobenzene	12.853	95	187936	45.172	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	90.340%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012423\
Data File : VN076372.D
Acq On : 24 Jan 2023 10:40
Operator : JC\MD
Sample : VN0124MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0124MBL01

Quant Time: Jan 25 00:33:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 17 03:59:22 2023
Response via : Initial Calibration




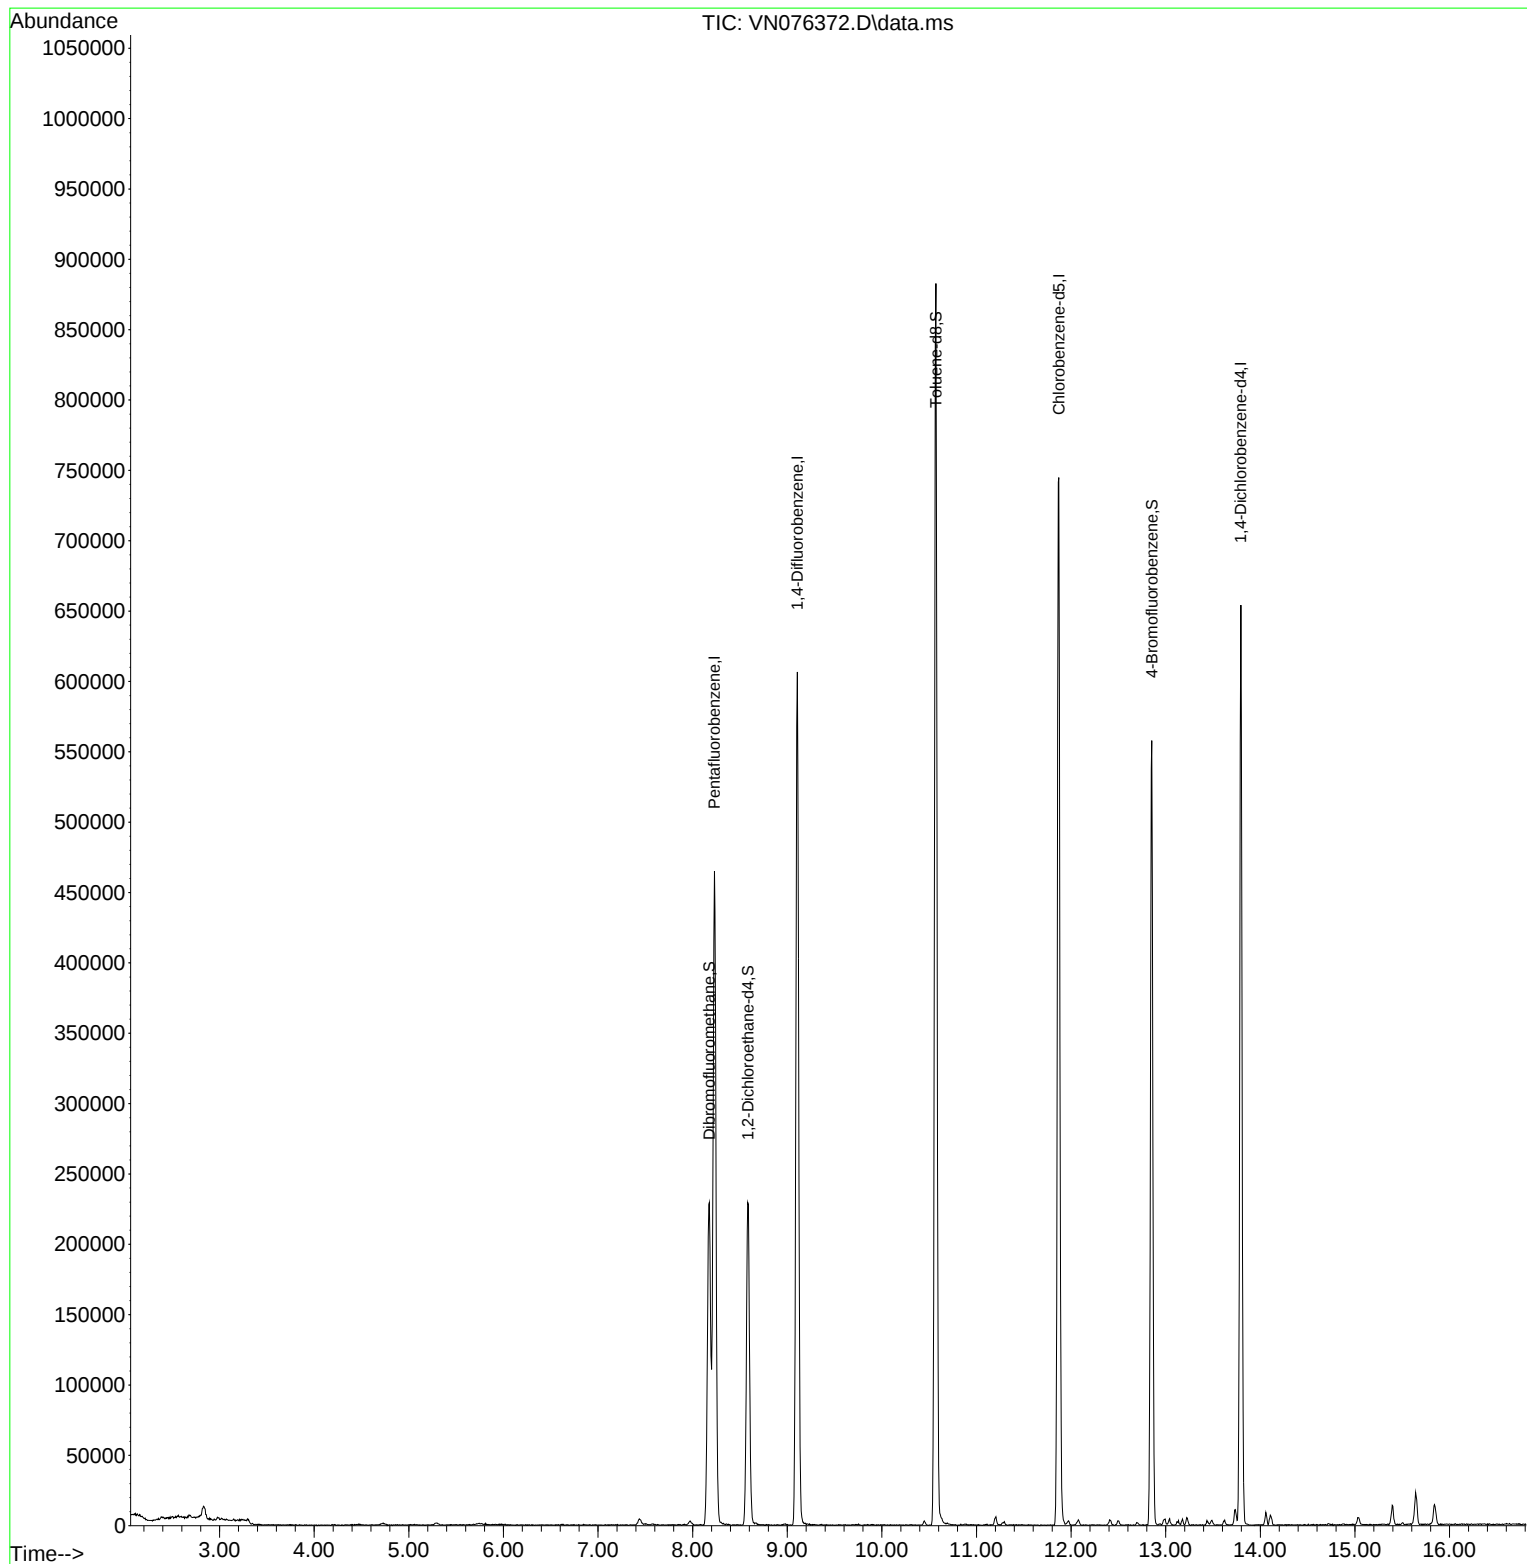


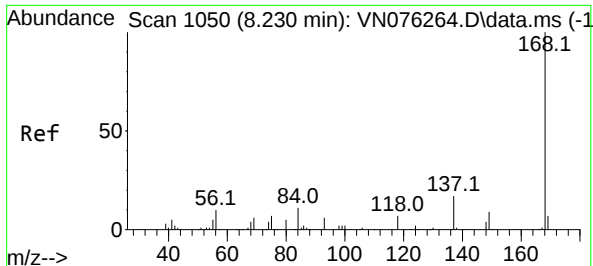

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.000 min
Lab File: VN076372.D
Acq: 24 Jan 2023 10:40




Instrument :
MSVOA_N
ClientSampleId :
VN0124MBL01

Tgt Ion:168 Resp: 349339
Ion Ratio Lower Upper
168 100
99 57.6 41.6 62.4

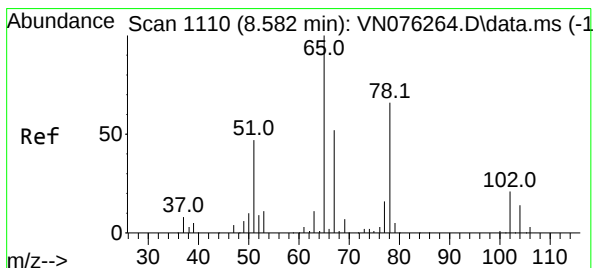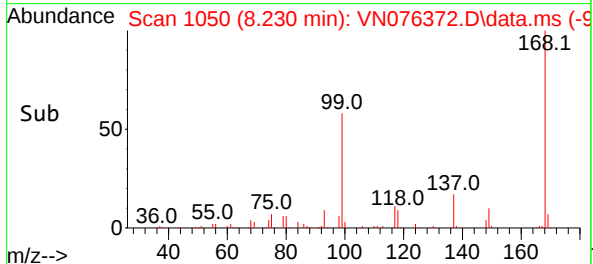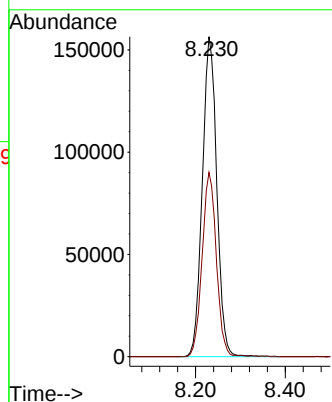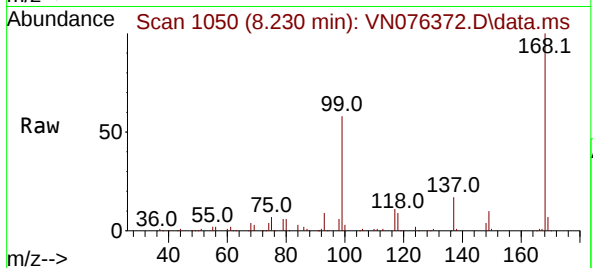

#33
1,2-Dichloroethane-d4
Concen: 49.768 ug/l
RT: 8.583 min Scan# 1110
Delta R.T. 0.001 min
Lab File: VN076372.D
Acq: 24 Jan 2023 10:40

Tgt Ion: 65 Resp: 194669
Ion Ratio Lower Upper
65 100
67 50.4 0.0 104.6

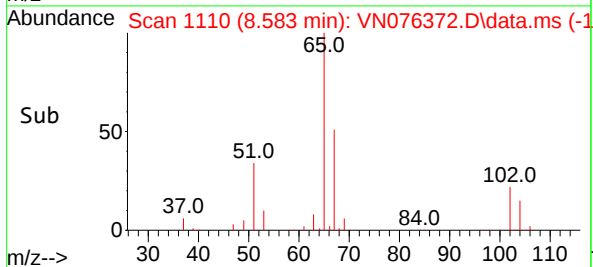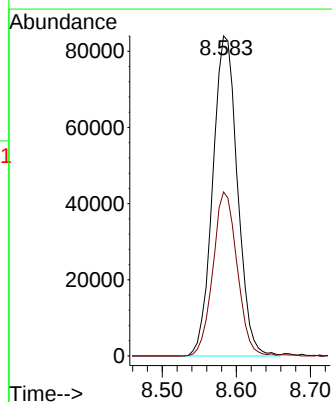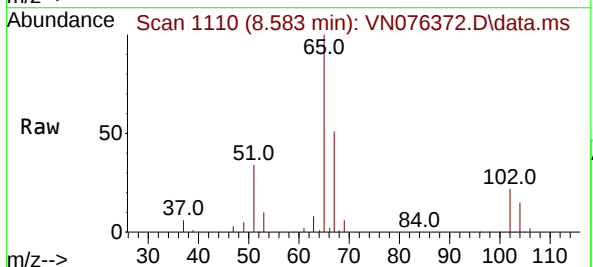



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. 0.000 min

Lab File: VN076372.D

Acq: 24 Jan 2023 10:40

Instrument :

MSVOA_N

ClientSampleId :

VN0124MBL01




Tgt Ion:114 Resp: 551653

Ion Ratio Lower Upper

114 100

63 18.9 0.0 35.8

88 15.0 0.0 28.0

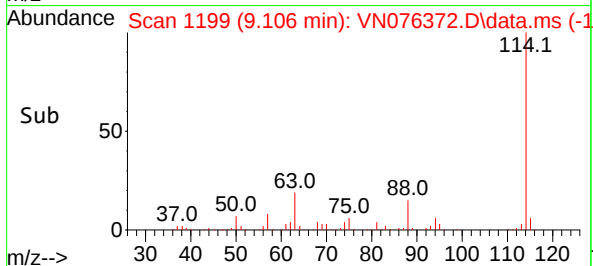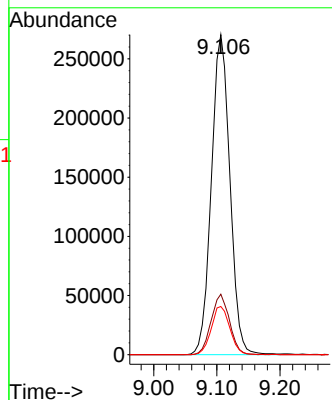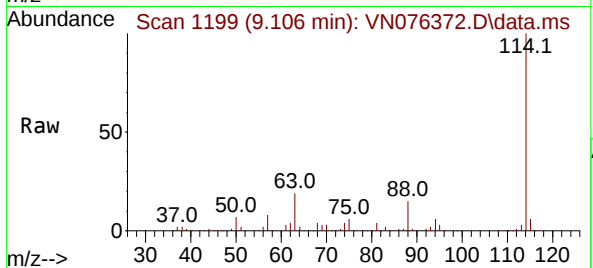

#35

Dibromofluoromethane

Concen: 48.341 ug/l

RT: 8.177 min Scan# 1041

Delta R.T. 0.006 min

Lab File: VN076372.D

Acq: 24 Jan 2023 10:40




Tgt Ion:113 Resp: 166815

Ion Ratio Lower Upper

113 100

111 103.6 82.7 124.1

192 19.4 15.6 23.4


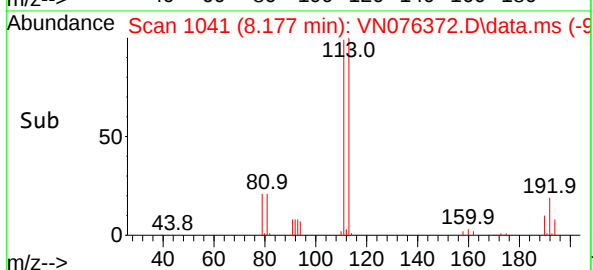
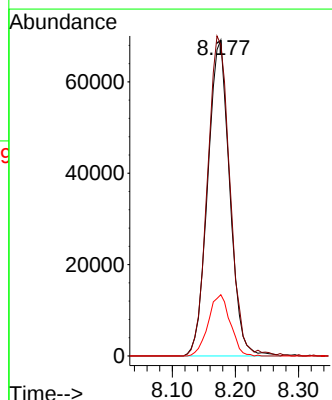
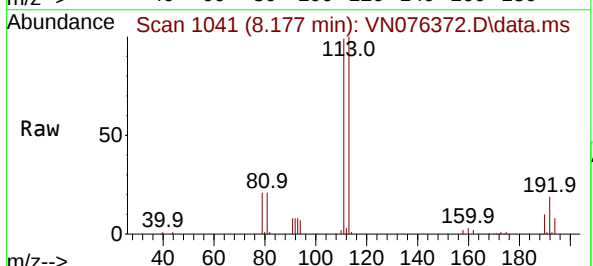




#50
Toluene-d8
Concen: 49.544 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN076372.D
Acq: 24 Jan 2023 10:40




Instrument :
MSVOA_N
ClientSampleId :
VN0124MBL01


Tgt Ion: 98 Resp: 631407
Ion Ratio Lower Upper
98 100
100 64.8 52.2 78.4

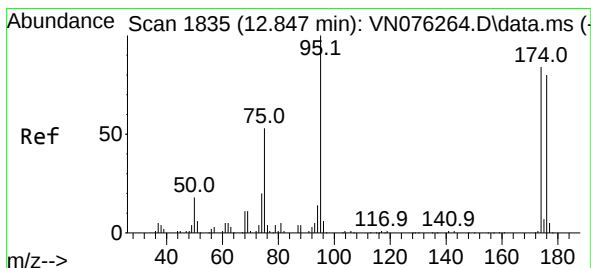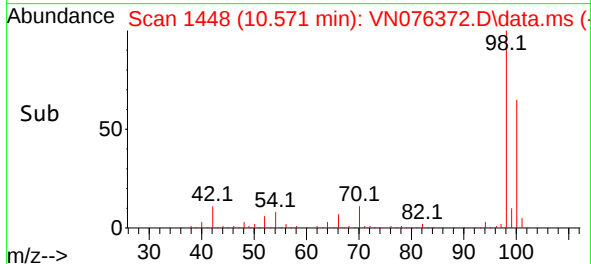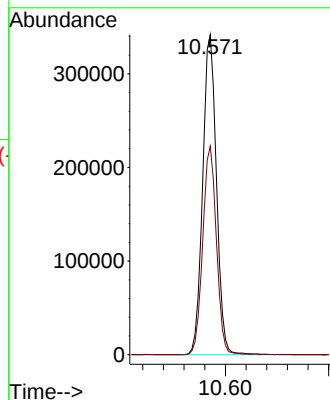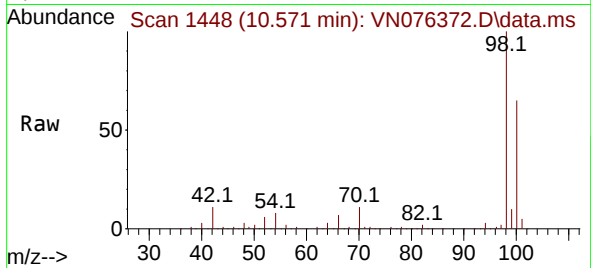

#62
4-Bromofluorobenzene
Concen: 45.172 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.006 min
Lab File: VN076372.D
Acq: 24 Jan 2023 10:40

Tgt Ion: 95 Resp: 187936
Ion Ratio Lower Upper
95 100
174 84.2 0.0 174.6
176 80.6 0.0 167.8


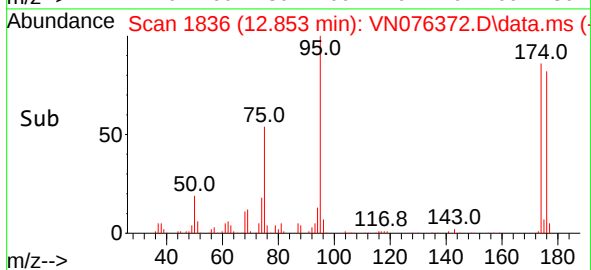
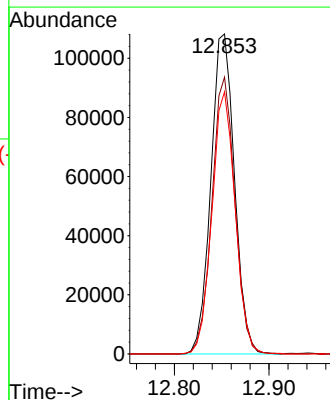
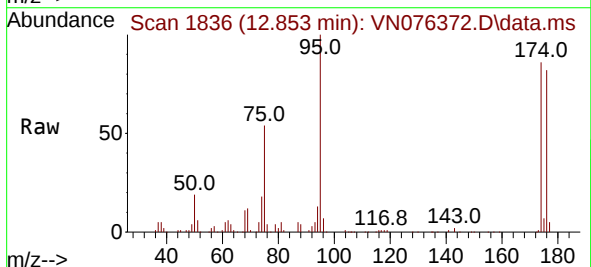


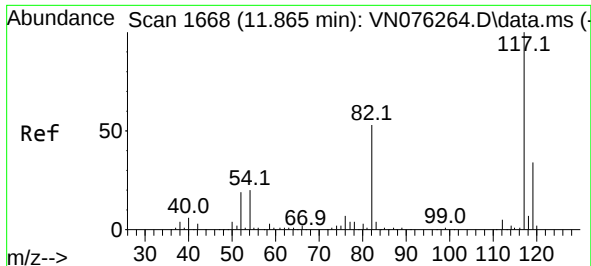

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 117
Delta R.T. 0.006 min
Lab File: VN076372.D
Acq: 24 Jan 2023 10:40

Instrument :
MSVOA_N
ClientSampleId :
VN0124MBL01

Tgt Ion:117 Resp: 459537
Ion Ratio Lower Upper
117 100
82 52.7 42.2 63.2
119 31.7 26.9 40.3

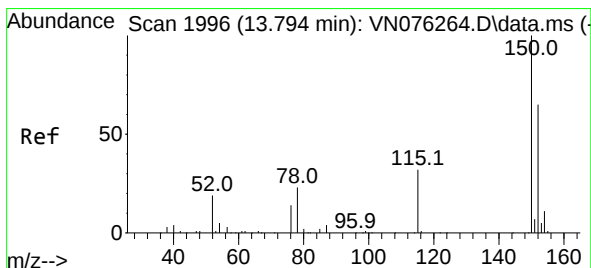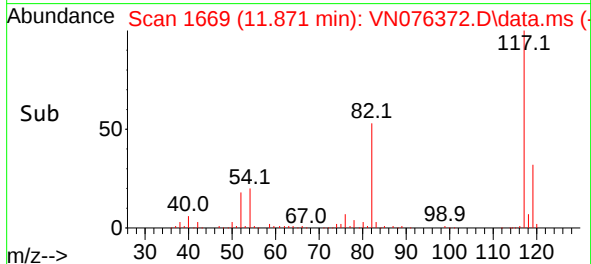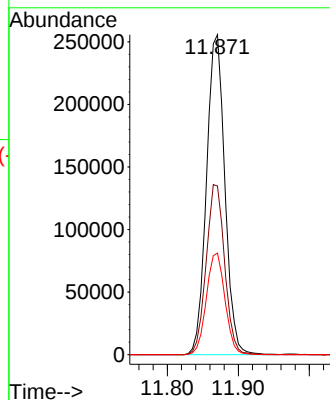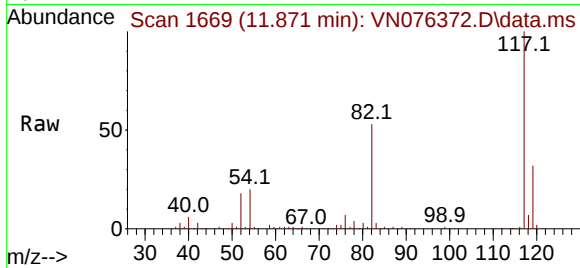

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. 0.000 min
Lab File: VN076372.D
Acq: 24 Jan 2023 10:40

Tgt Ion:152 Resp: 178892
Ion Ratio Lower Upper
152 100
115 58.1 29.6 88.9
150 158.0 0.0 351.4

