
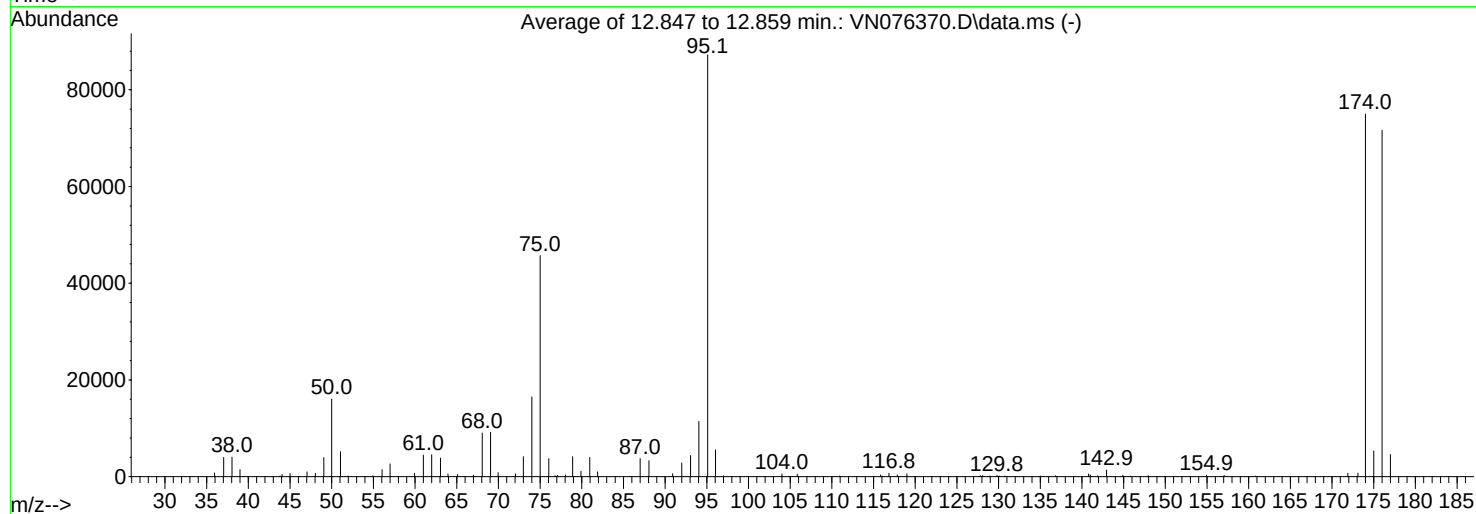


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012423\
Data File : VN076370.D
Acq On : 24 Jan 2023 08:49
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Title : SW846 8260
Last Update : Tue Jan 17 03:59:22 2023

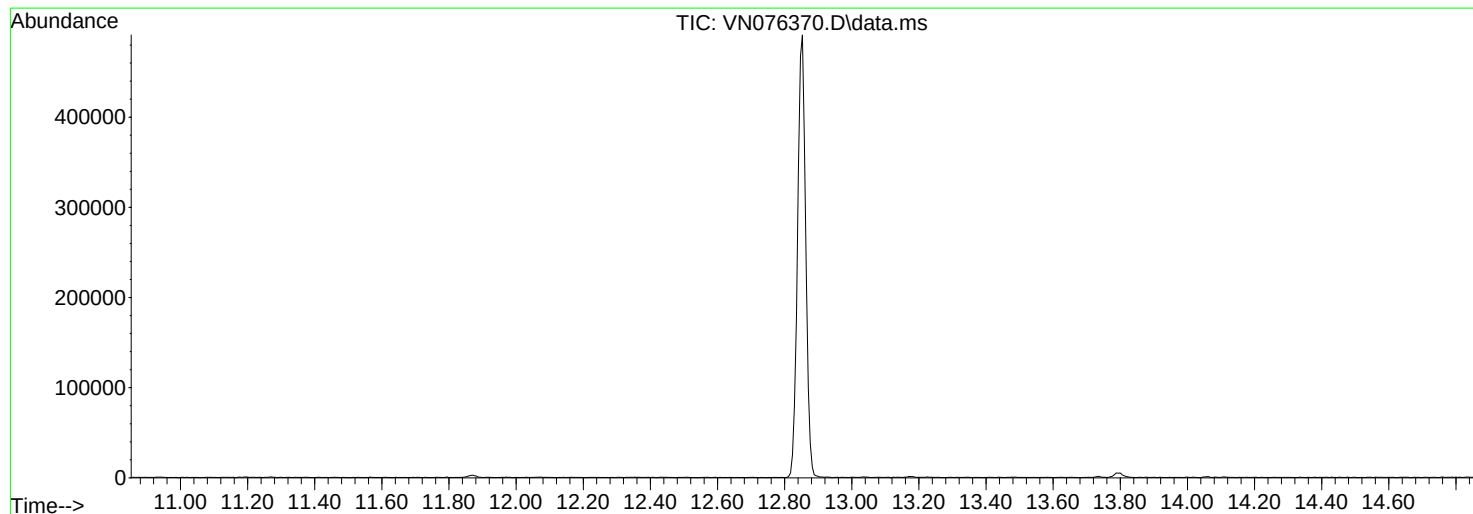

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1826

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.4	16061	PASS
75	95	30	60	52.4	45747	PASS
95	95	100	100	100.0	87232	PASS
96	95	5	9	6.4	5542	PASS
173	174	0.00	2	1.0	731	PASS
174	95	50	100	86.0	74981	PASS
175	174	5	9	7.1	5337	PASS
176	174	95	101	95.6	71648	PASS
177	176	5	9	6.4	4558	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	753	49.05	3933	63.95	558	76.80	19
37.05	3968	50.00	16061	65.10	482	77.10	25
38.05	4051	51.05	5159	67.00	291	78.05	35
39.00	1469	51.95	143	68.05	9032	78.90	412
39.90	62	54.95	198	69.05	9166	79.90	1125
43.80	151	56.05	1455	69.95	839	80.95	3970
44.05	430	57.00	2647	72.05	583	81.90	986
45.00	677	59.95	703	73.00	4143	85.70	58
46.10	61	61.00	4485	74.00	16485	87.00	3729
47.05	987	62.00	4541	75.00	45747	88.05	3313
48.05	684	63.05	3844	76.05	3727	90.90	608

Average of 12.847 to 12.859 min.: VN076370.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.00	2850	115.85	368	130.75	134	154.95	286
93.05	4387	116.10	103	135.05	130	157.05	272
94.05	11425	116.85	698	136.85	209	160.80	123
95.10	87232	117.85	365	140.80	576	171.00	64
96.05	5542	119.00	601	141.00	353	171.90	703
97.00	161	127.80	184	141.85	159	173.10	731
104.00	554	128.10	220	142.95	1349	174.00	74981
104.80	51	128.70	70	144.90	298	175.00	5337
105.00	69	128.95	126	145.85	126	176.00	71648
105.85	543	129.80	264	147.95	216	177.00	4558
110.90	133	130.10	151	149.90	61		

Instrument :

MSVOA_N

ClientSampleId :

BFB