


Acrolein

Response Ratio

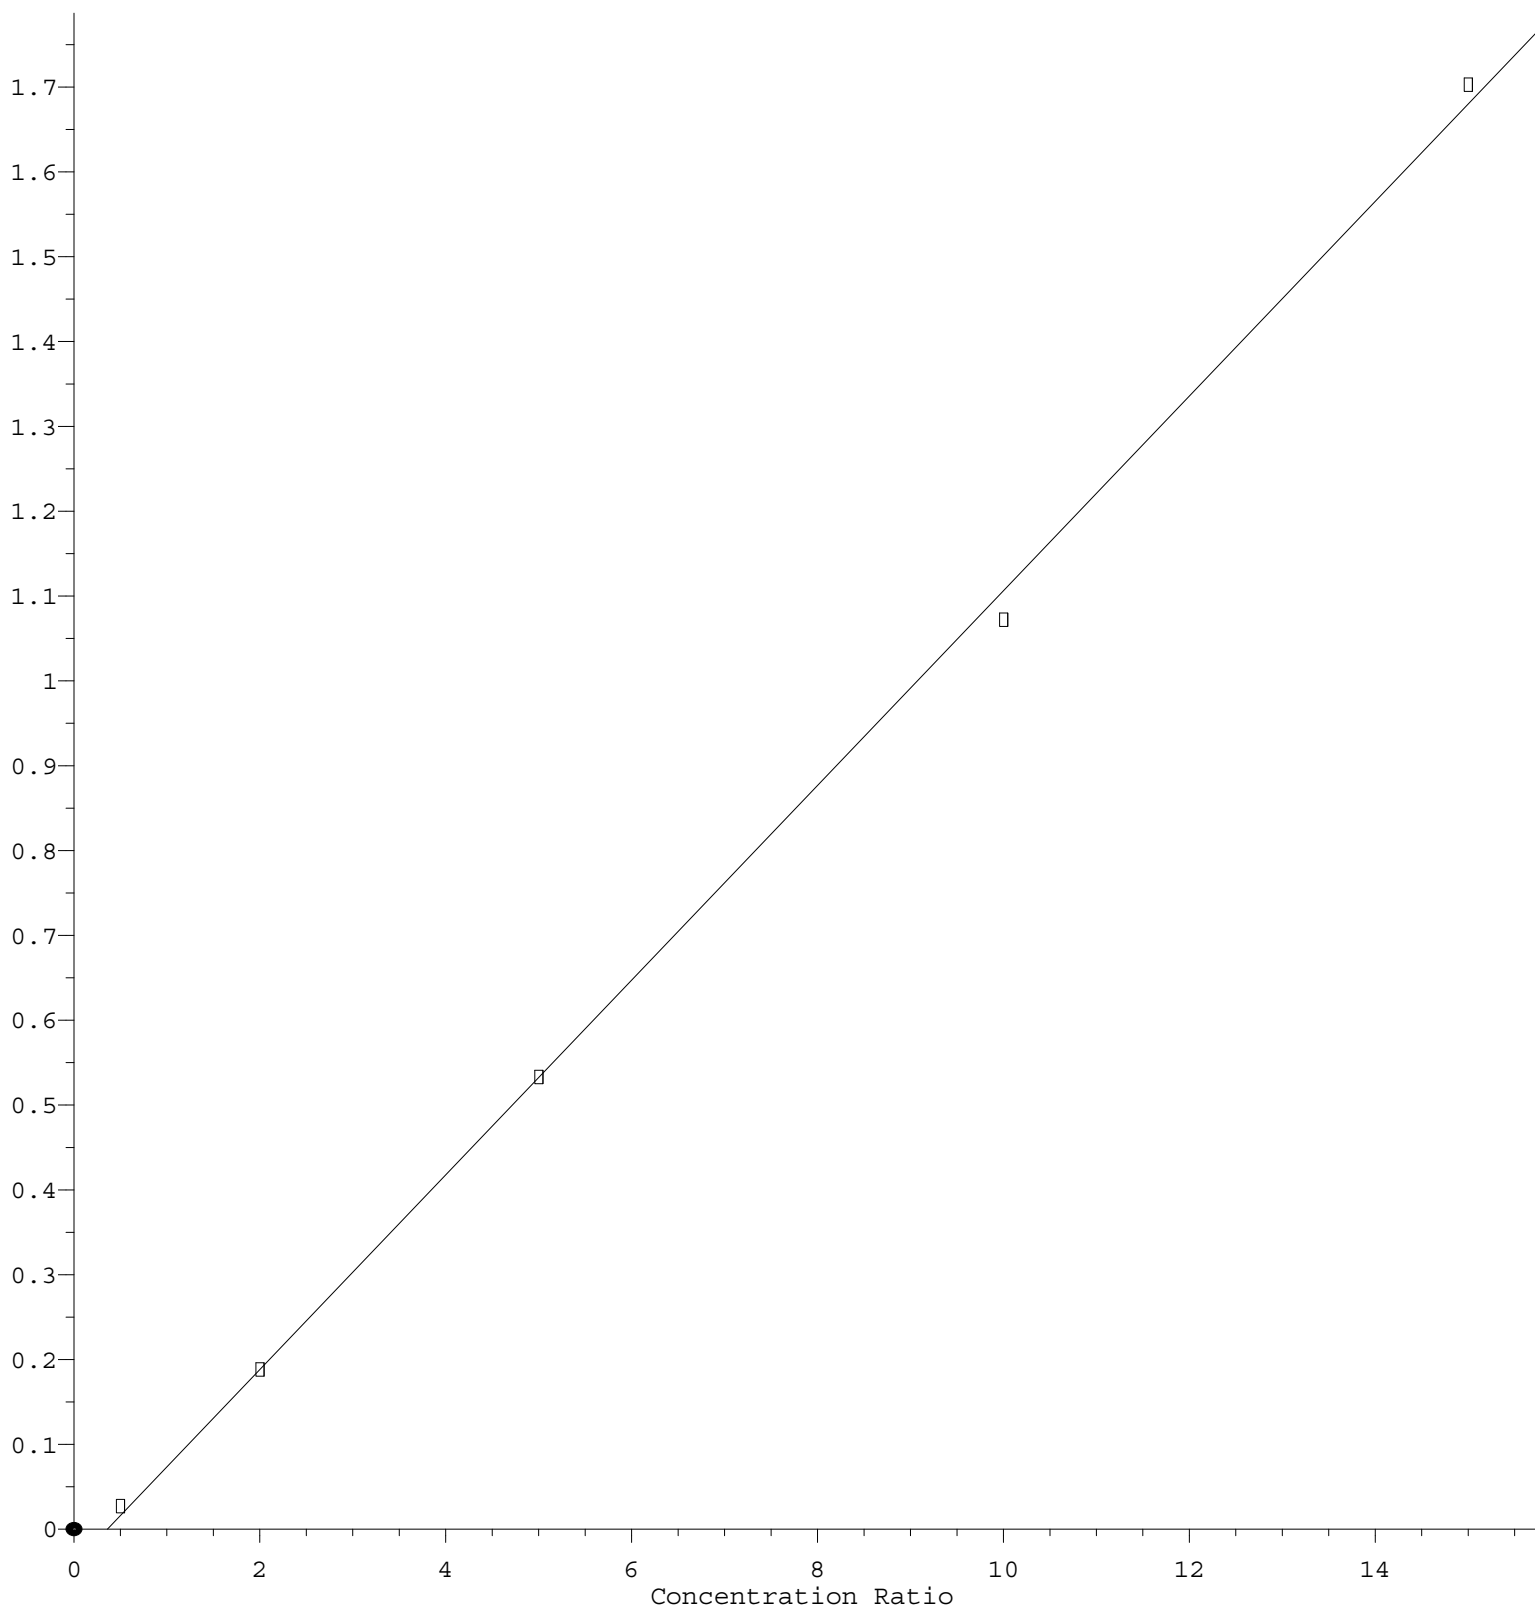

$$\text{Response} = 1.148\text{e-}001 * \text{Amt} - 4.152\text{e-}002$$


Coef of Det (r^2) = 0.999037 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N012521W.M

Calibration Table Last Updated: Mon Jan 25 13:47:28 2021

Hexachlorobutadiene

Response Ratio

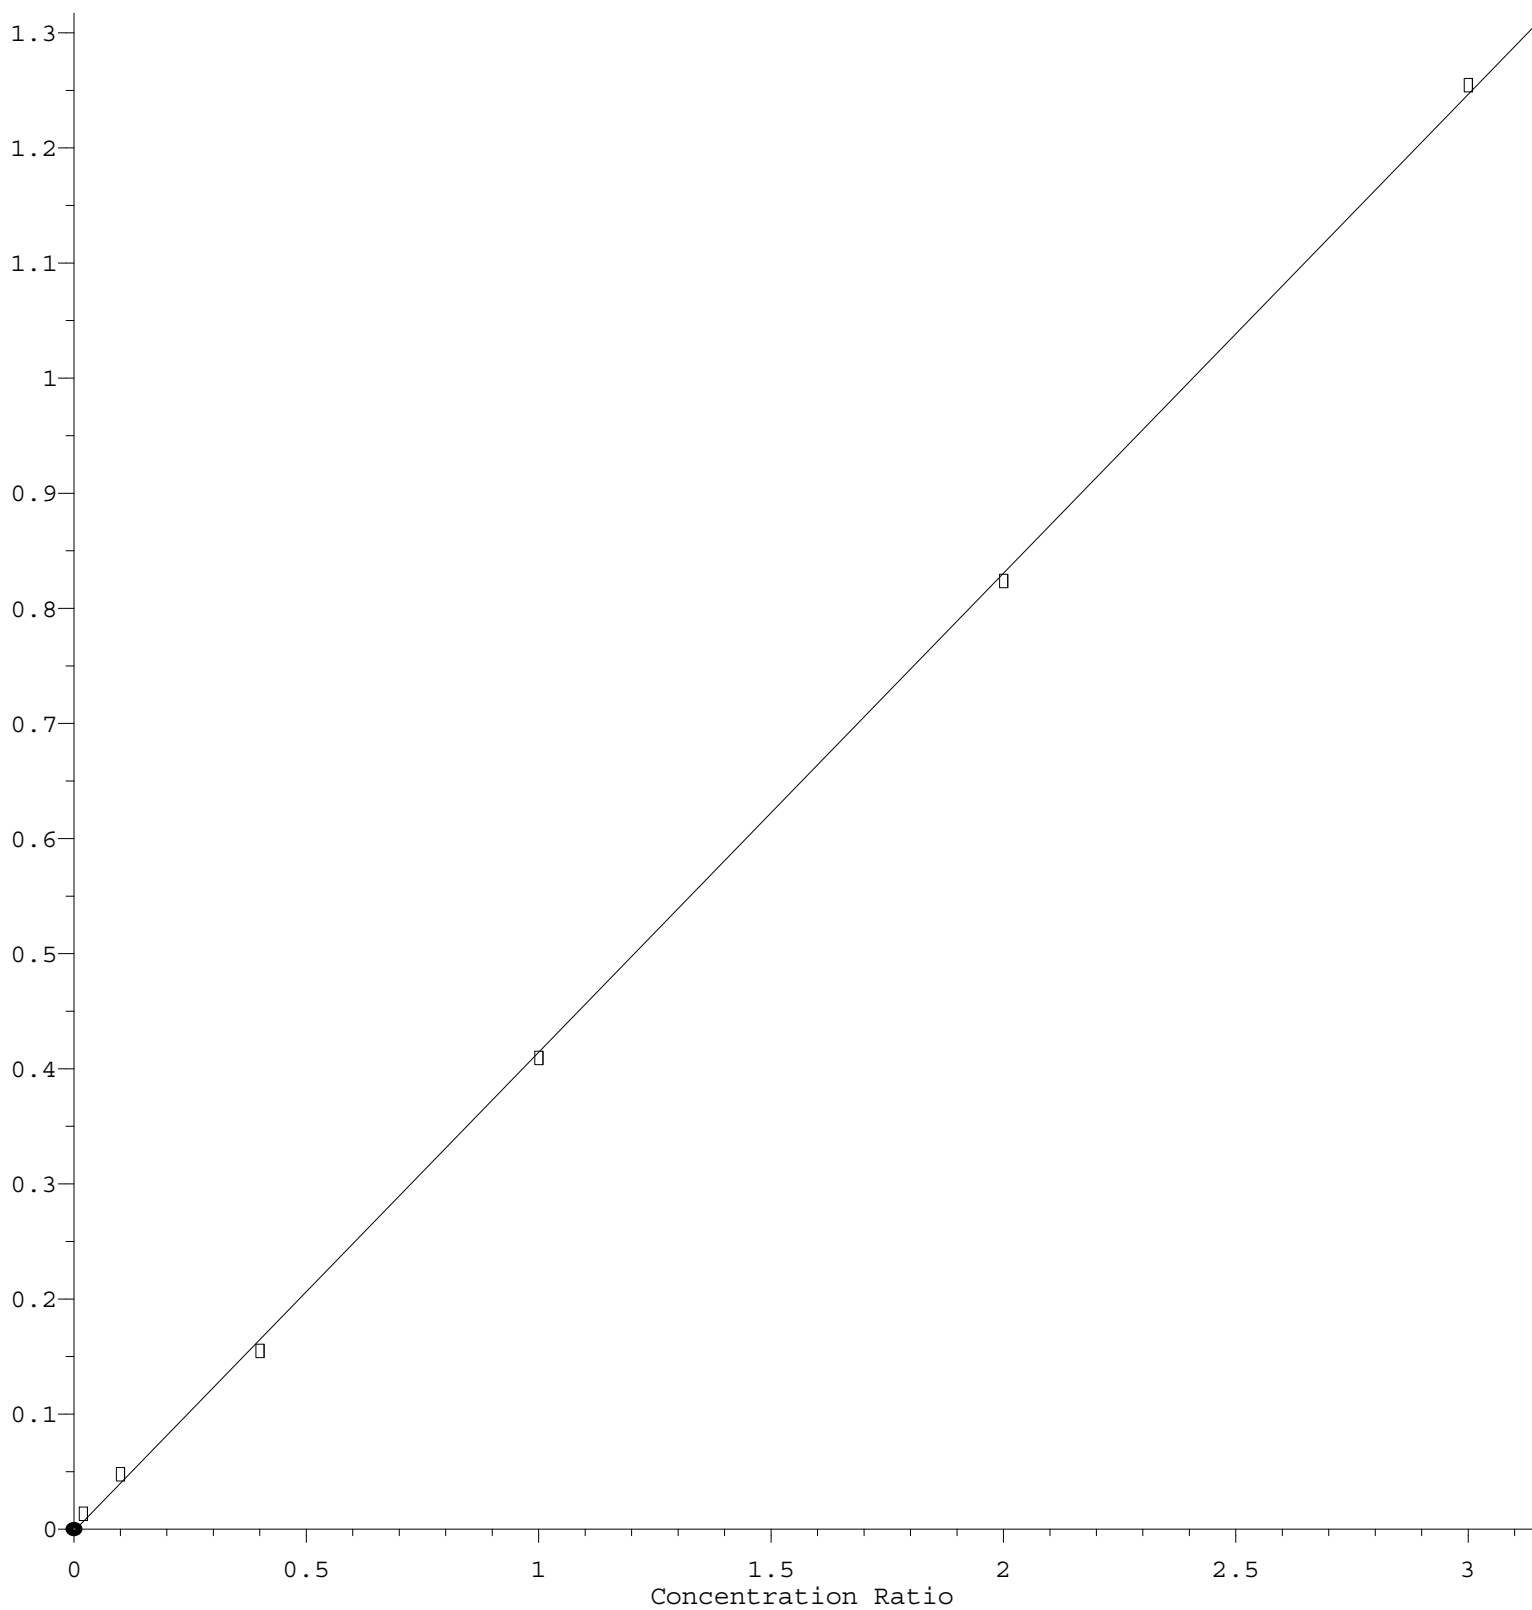

$$\text{Response} = 4.163\text{e-}001 * \text{Amt} - 1.807\text{e-}003$$


Coef of Det (r^2) = 0.999728 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N012521W.M

Calibration Table Last Updated: Mon Jan 25 13:47:28 2021

Naphthalene


Response Ratio

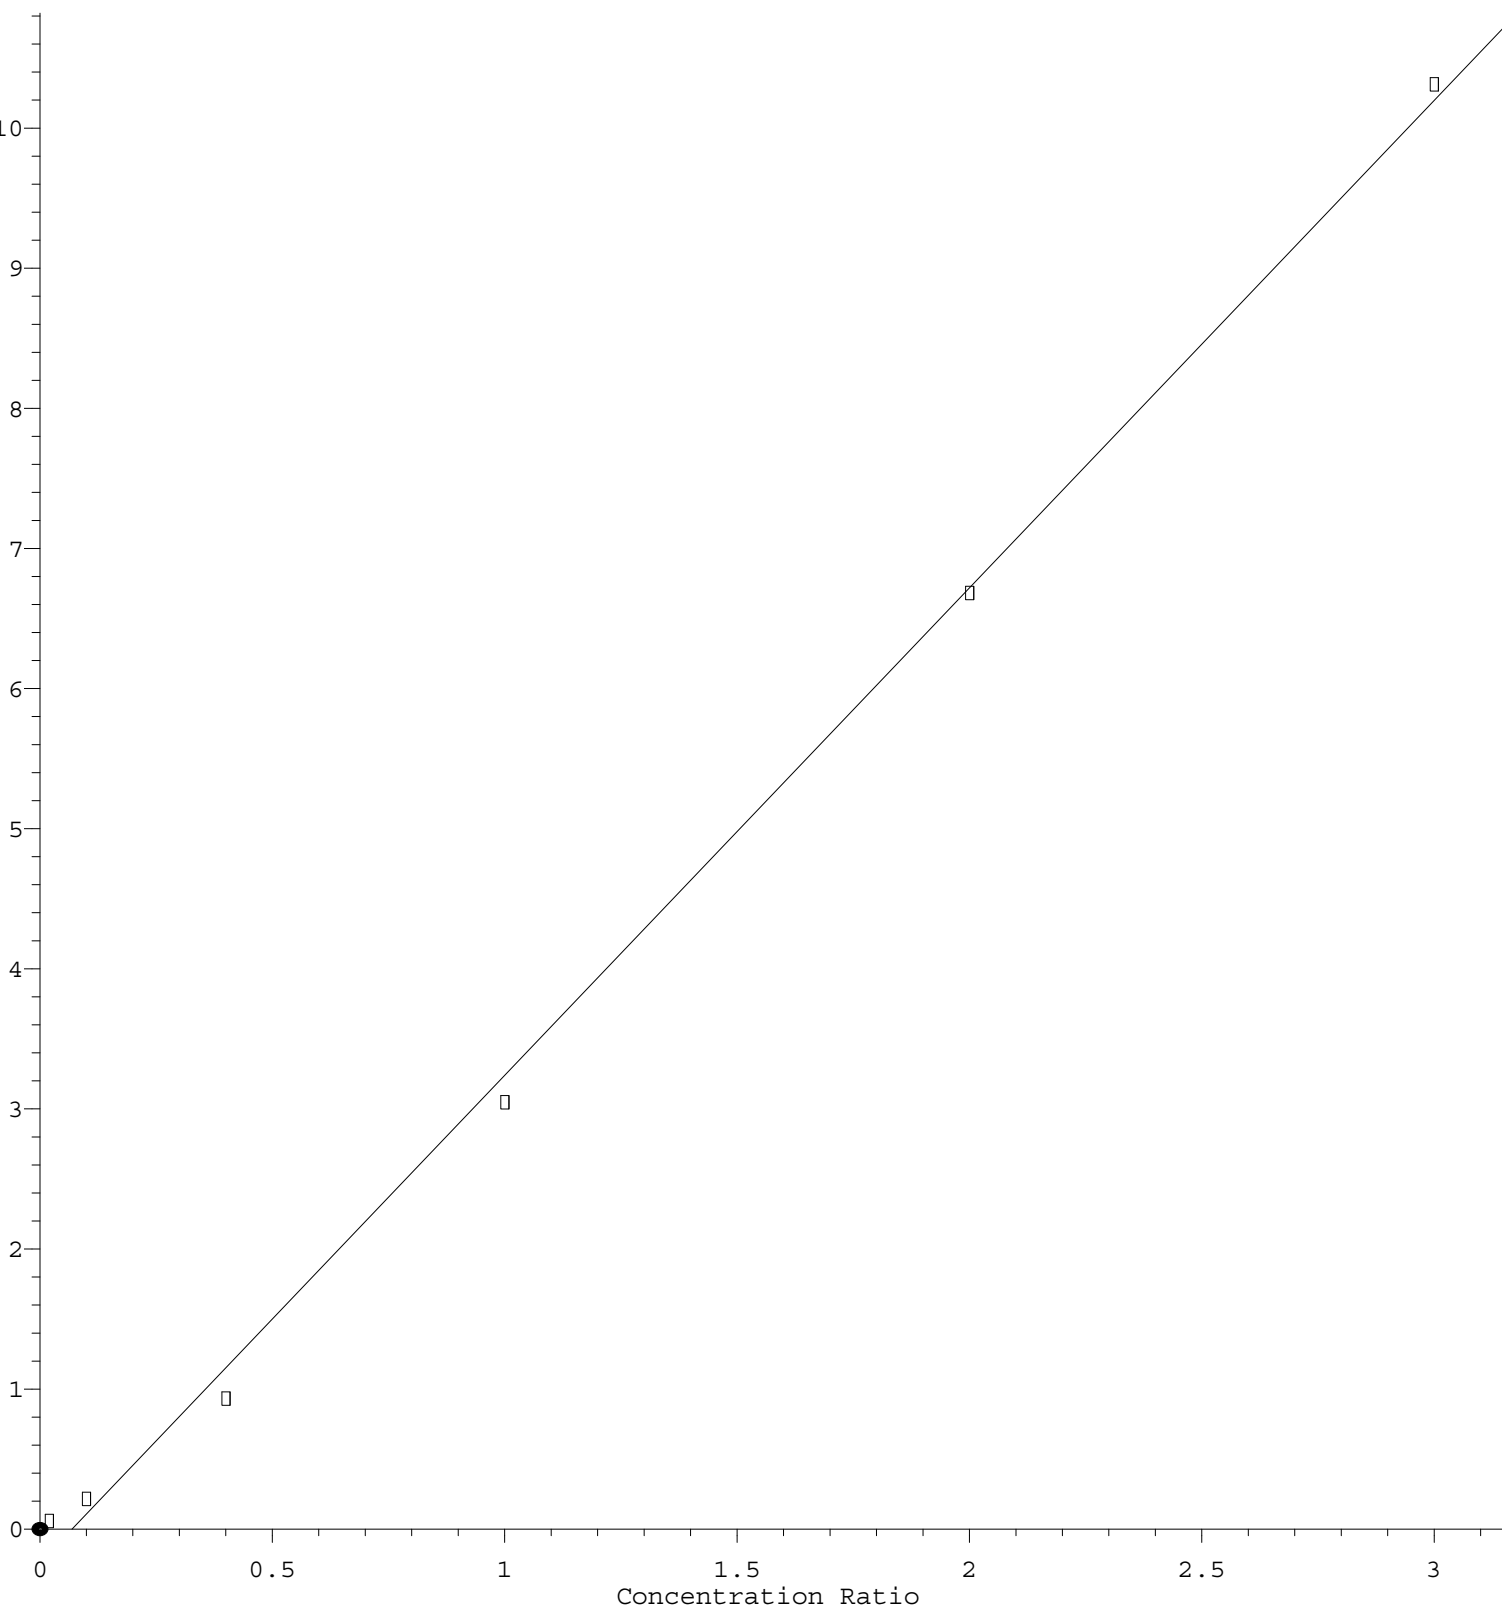

$\text{Response} = 3.480\text{e}+000 * \text{Amt} - 2.402\text{e}-001$
 Coef of Det (r^2) = 0.998098 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N012521W.M
 Calibration Table Last Updated: Mon Jan 25 13:47:28 2021

1,2,3-Trichlorobenzene

Response Ratio

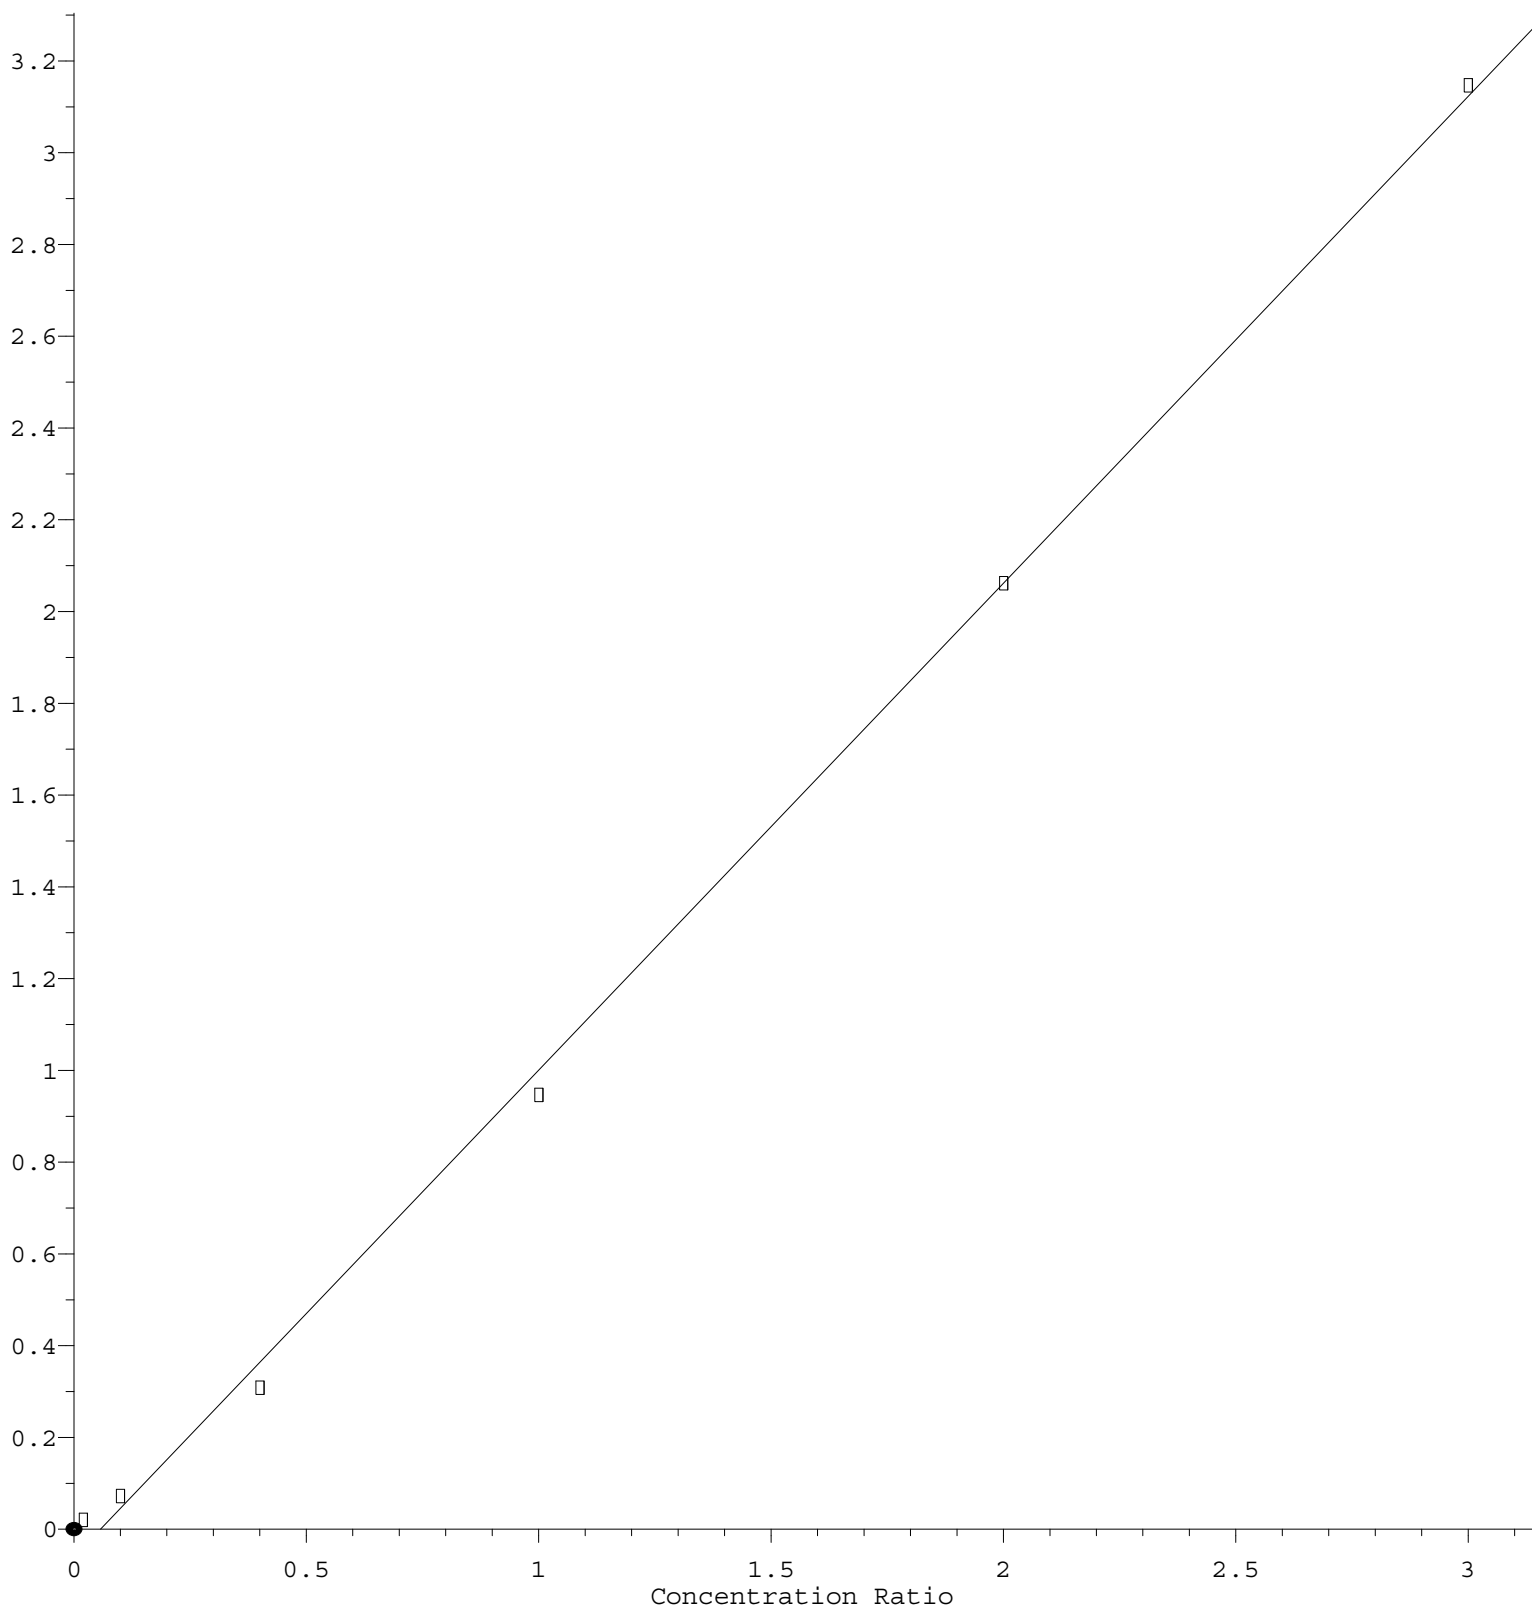

$$\text{Response} = 1.061\text{e}+000 * \text{Amt} - 6.036\text{e}-002$$


Coef of Det (r^2) = 0.998635 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N012521W.M

Calibration Table Last Updated: Mon Jan 25 13:47:28 2021

1,2,4-Trichlorobenzene

Response Ratio

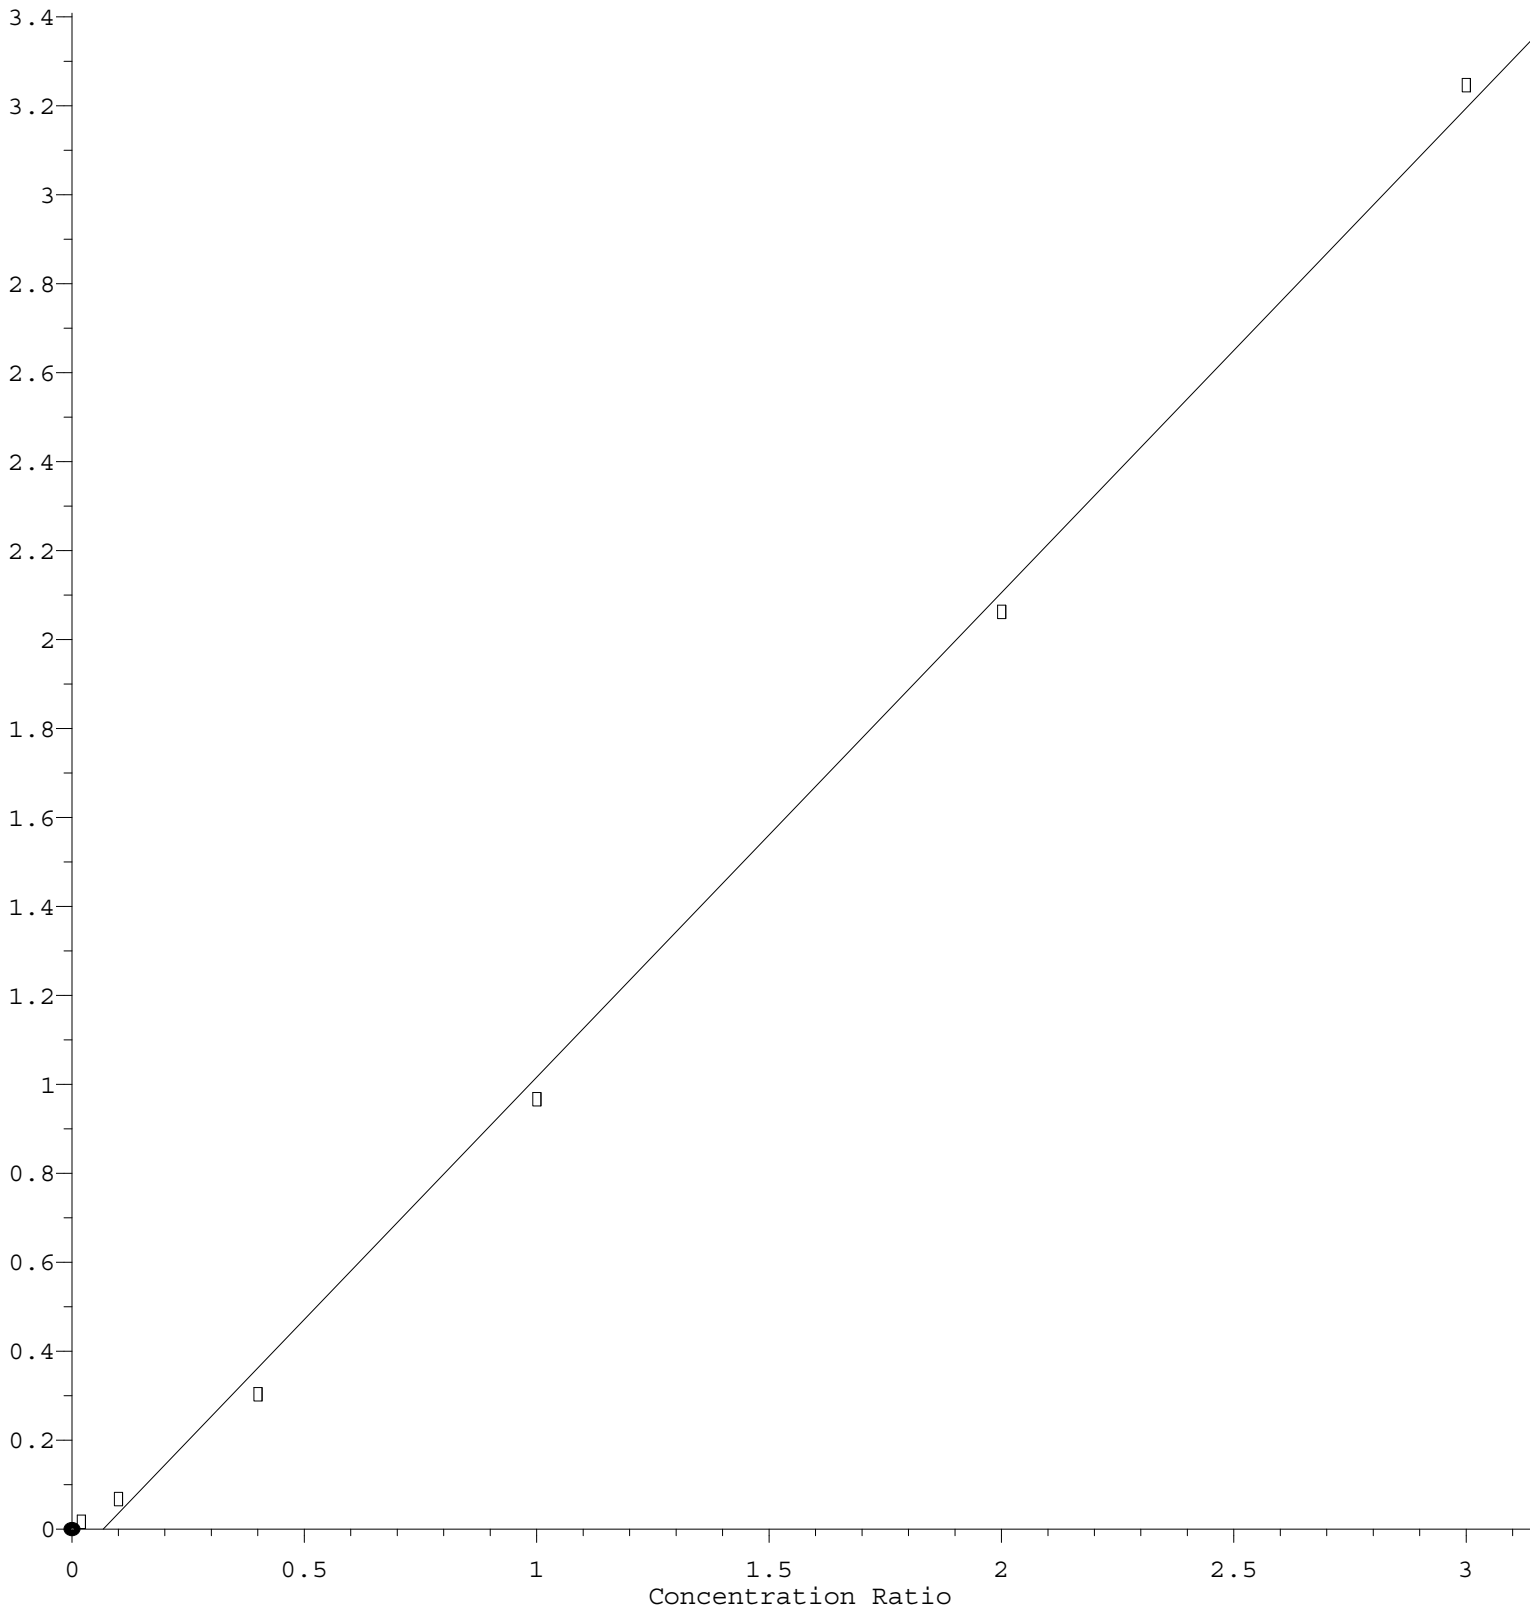

$$\text{Response} = 1.089\text{e}+000 * \text{Amt} - 7.334\text{e}-002$$

Coef of Det (r^2) = 0.998081 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N012521W.M

Calibration Table Last Updated: Mon Jan 25 13:47:28 2021