


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012522\
 Data File : VN070766.D
 Acq On : 25 Jan 2022 10:51
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
 Title : SW846 8260
 Last Update : Tue Jan 18 13:32:07 2022

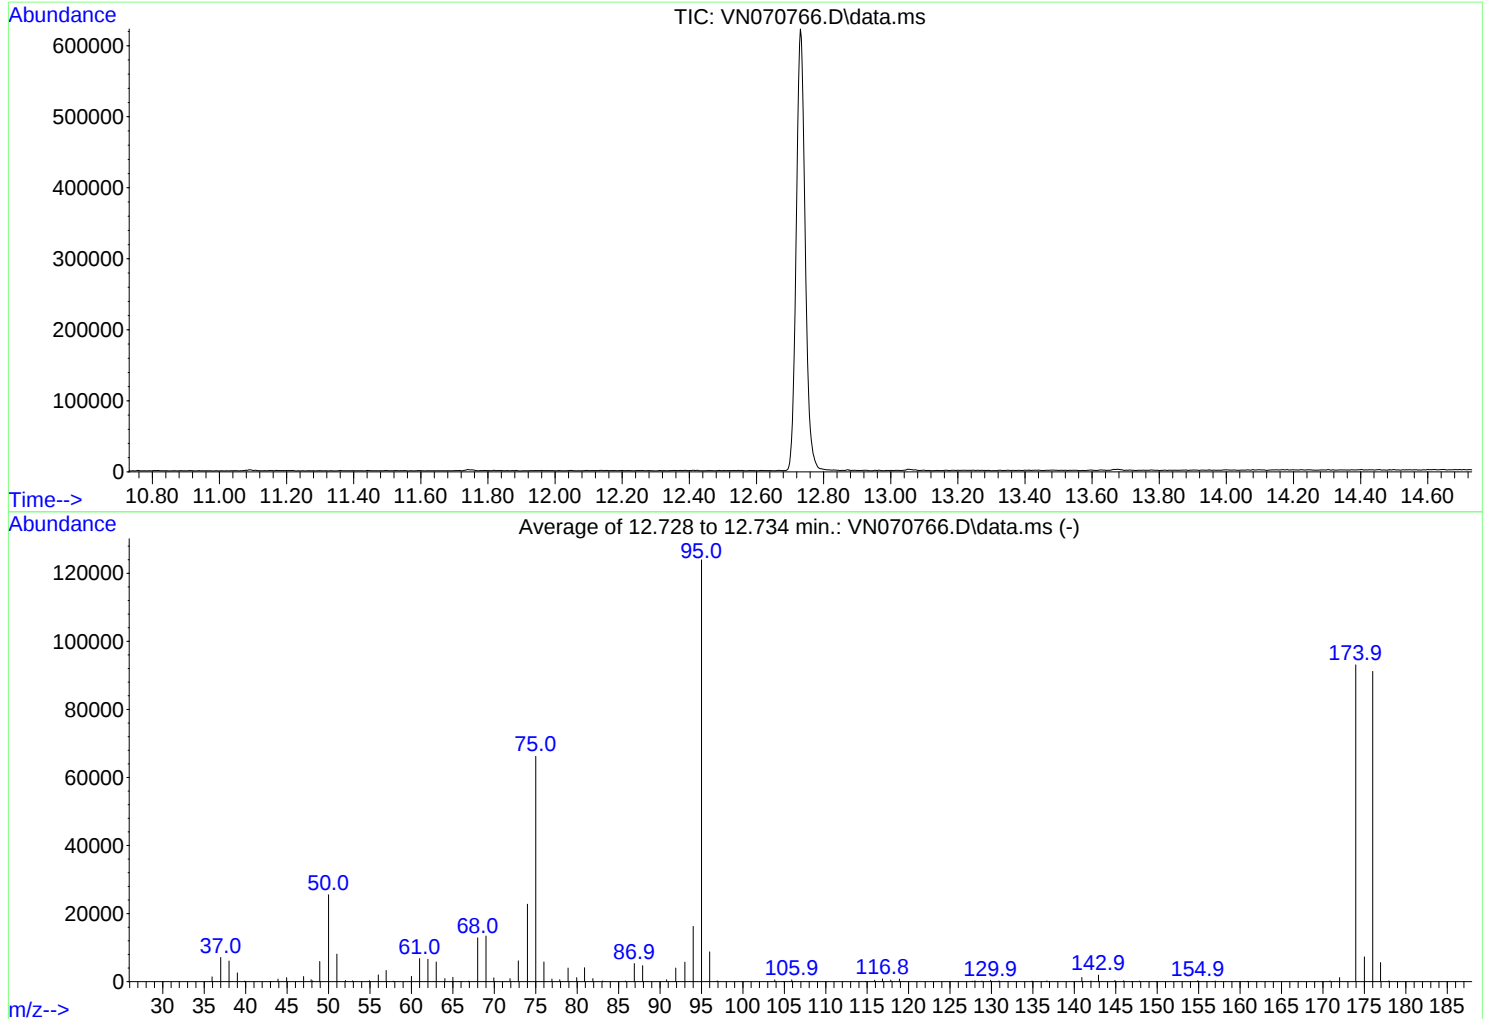

AutoFind: Scans 4004, 4005, 4006; Background Corrected with Scan 3986

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	25552	PASS
75	95	30	60	53.4	66213	PASS
95	95	100	100	100.0	123949	PASS
96	95	5	9	7.1	8752	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	75.1	93109	PASS
175	174	5	9	7.8	7301	PASS
176	174	95	101	97.9	91171	PASS
177	176	5	9	6.1	5606	PASS