

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012523\
 Data File : VN076391.D
 Acq On : 25 Jan 2023 10:47
 Operator : JC\MD
 Sample : VN0125MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0125MBL01

Quant Time: Jan 26 07:13:23 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 17 03:59:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	339771	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	545791	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	459842	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	171641	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	201096	52.859	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	105.720%
35) Dibromofluoromethane	8.177	113	169103	49.530	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.060%
50) Toluene-d8	10.571	98	630586	50.011	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	100.020%
62) 4-Bromofluorobenzene	12.853	95	185504	45.067	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	90.140%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012523\
Data File : VN076391.D
Acq On : 25 Jan 2023 10:47
Operator : JC\MD
Sample : VN0125MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0125MBL01

Quant Time: Jan 26 07:13:23 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 17 03:59:22 2023
Response via : Initial Calibration




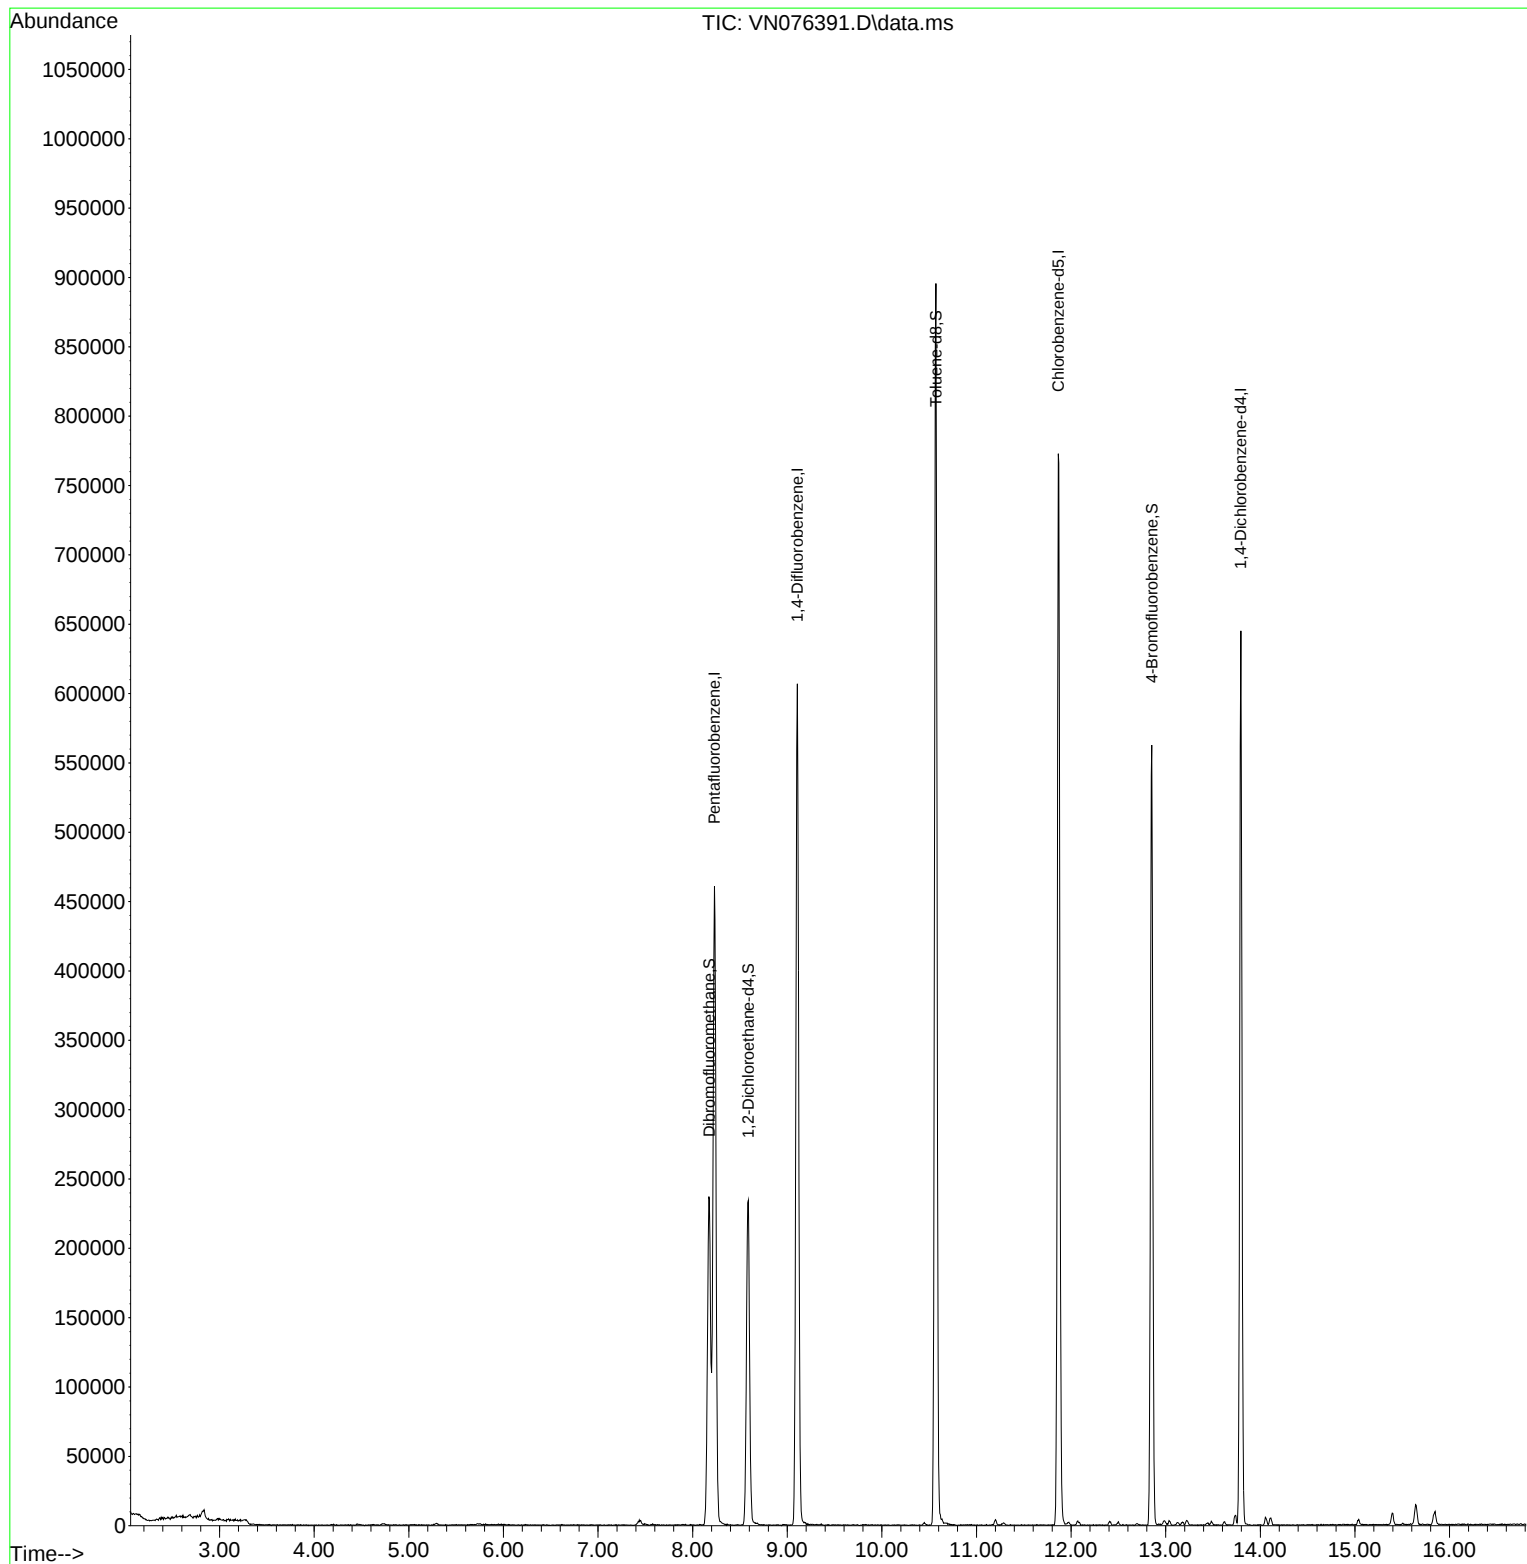


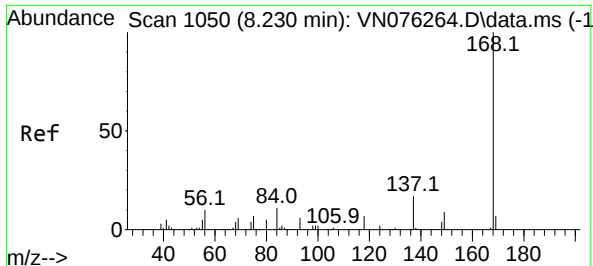

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.000 min
Lab File: VN076391.D
Acq: 25 Jan 2023 10:47




Instrument :
MSVOA_N
ClientSampleId :
VN0125MBL01


Tgt Ion:168 Resp: 339771
Ion Ratio Lower Upper
168 100
99 56.7 41.6 62.4

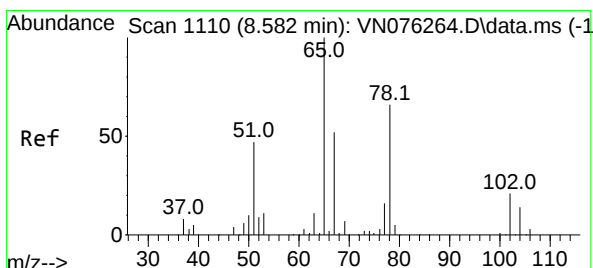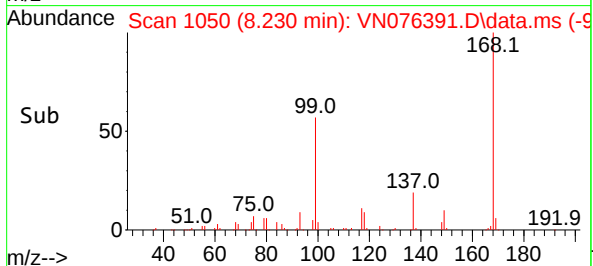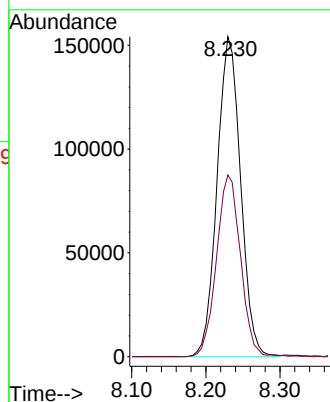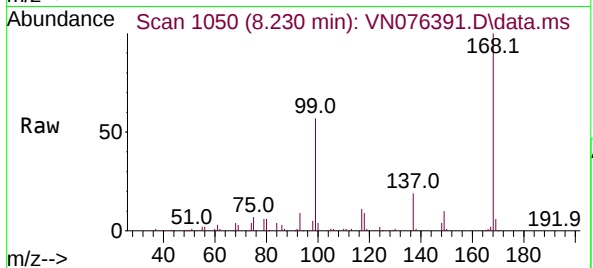

#33
1,2-Dichloroethane-d4
Concen: 52.859 ug/l
RT: 8.588 min Scan# 1111
Delta R.T. 0.006 min
Lab File: VN076391.D
Acq: 25 Jan 2023 10:47

Tgt Ion: 65 Resp: 201096
Ion Ratio Lower Upper
65 100
67 50.4 0.0 104.6

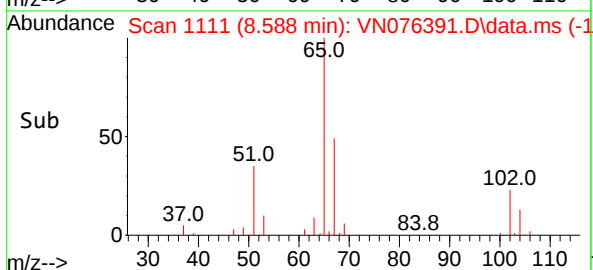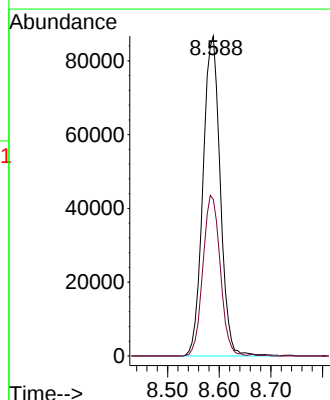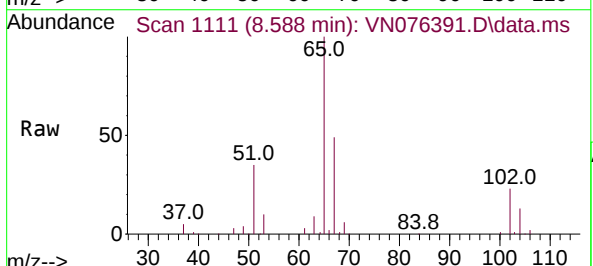

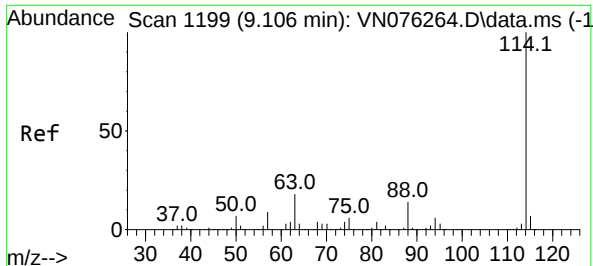

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. 0.000 min

Lab File: VN076391.D

Acq: 25 Jan 2023 10:47

Instrument :

MSVOA_N

ClientSampleId :

VN0125MBL01





Tgt Ion:114 Resp: 545791

Ion Ratio Lower Upper

114 100

63 18.5 0.0 35.8

88 14.9 0.0 28.0

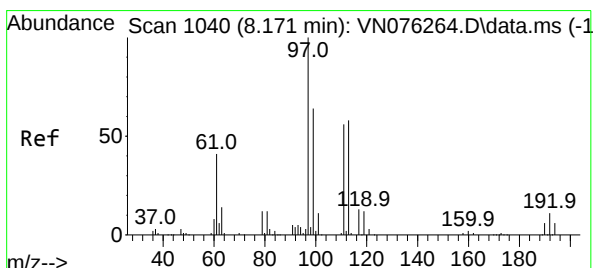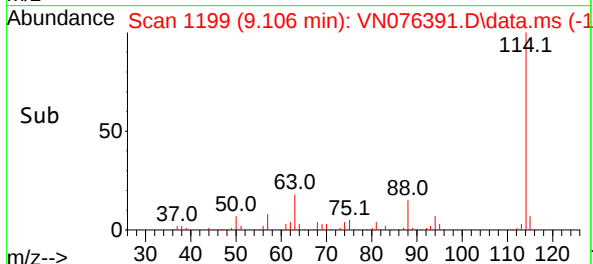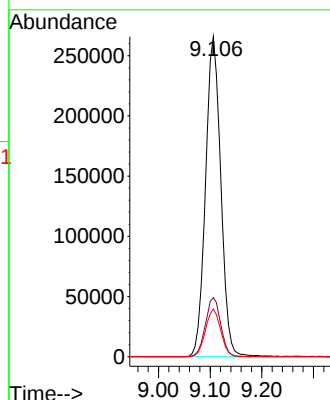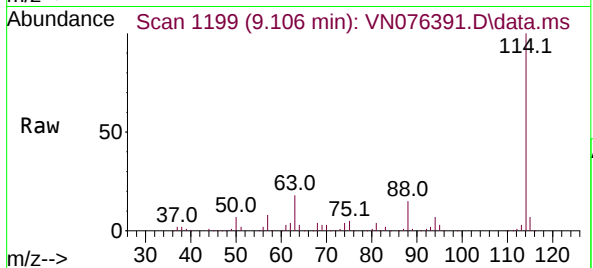

#35

Dibromofluoromethane

Concen: 49.530 ug/l

RT: 8.177 min Scan# 1041

Delta R.T. 0.006 min

Lab File: VN076391.D

Acq: 25 Jan 2023 10:47




Tgt Ion:113 Resp: 169103


Ion Ratio Lower Upper

113 100

111 102.6 82.7 124.1

192 19.1 15.6 23.4


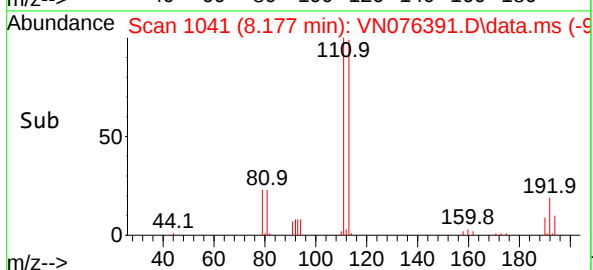
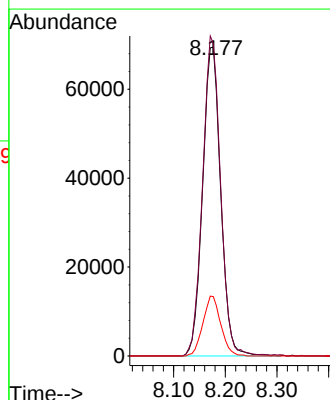
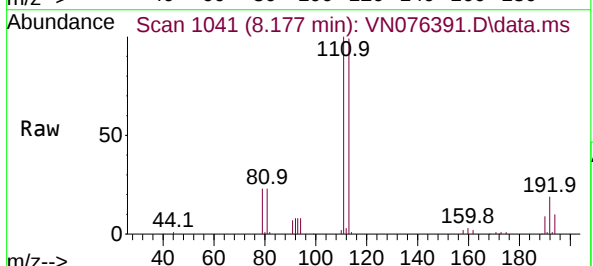


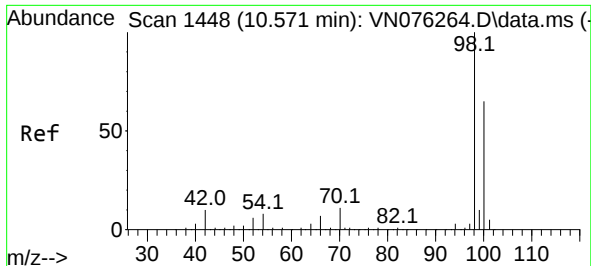

#50
Toluene-d8
Concen: 50.011 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN076391.D
Acq: 25 Jan 2023 10:47




Instrument :
MSVOA_N
ClientSampleId :
VN0125MBL01


Tgt Ion: 98 Resp: 630586
Ion Ratio Lower Upper
98 100
100 65.4 52.2 78.4

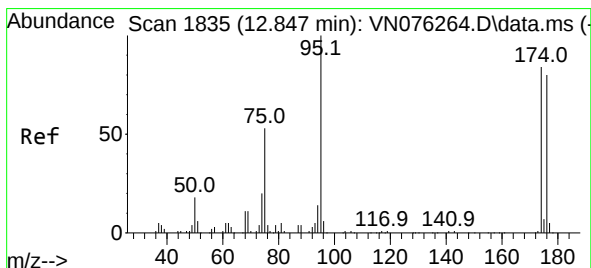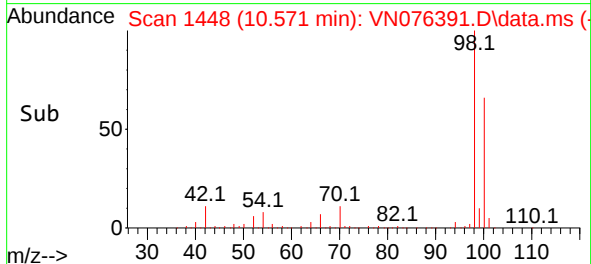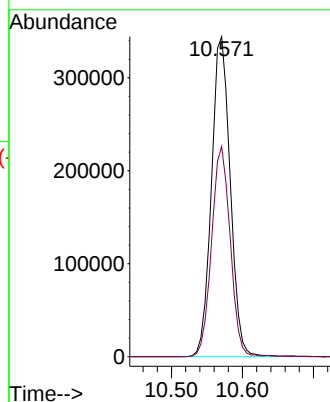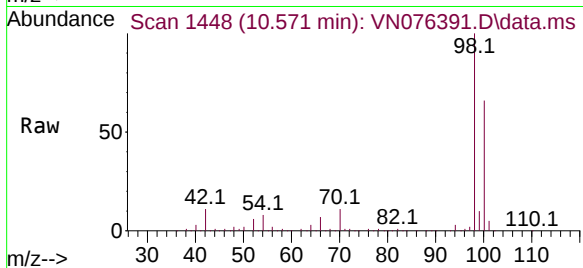

#62
4-Bromofluorobenzene
Concen: 45.067 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.006 min
Lab File: VN076391.D
Acq: 25 Jan 2023 10:47

Tgt Ion: 95 Resp: 185504
Ion Ratio Lower Upper
95 100
174 85.0 0.0 174.6
176 78.9 0.0 167.8


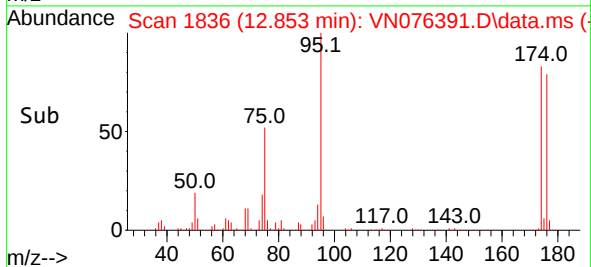
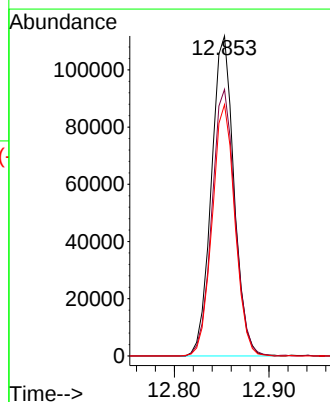
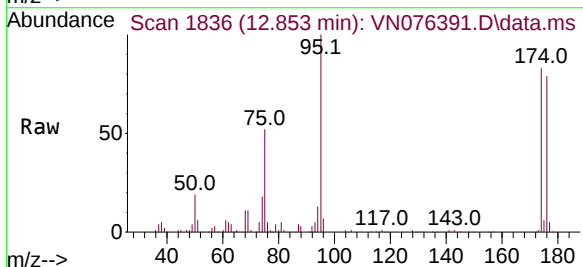


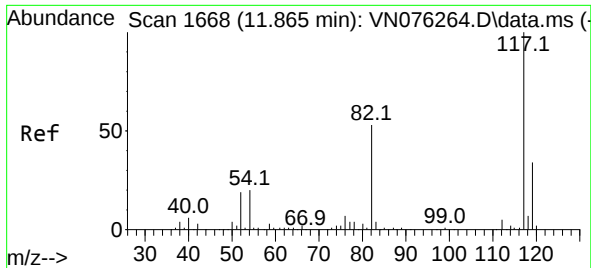

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN076391.D
Acq: 25 Jan 2023 10:47

Instrument :
MSVOA_N
ClientSampleId :
VN0125MBL01

Tgt Ion:117 Resp: 459842
Ion Ratio Lower Upper
117 100
82 54.7 42.2 63.2
119 31.5 26.9 40.3

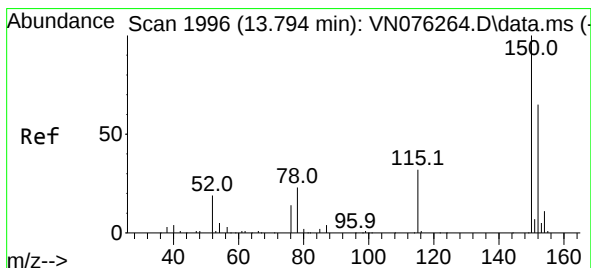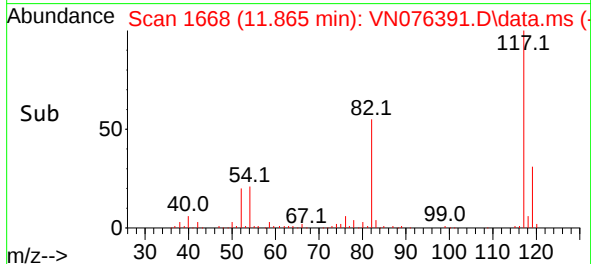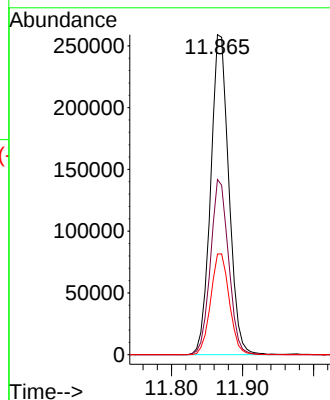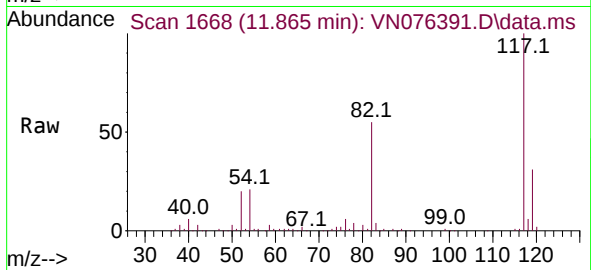

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. 0.000 min
Lab File: VN076391.D
Acq: 25 Jan 2023 10:47

Tgt Ion:152 Resp: 171641
Ion Ratio Lower Upper
152 100
115 59.5 29.6 88.9
150 159.1 0.0 351.4

