
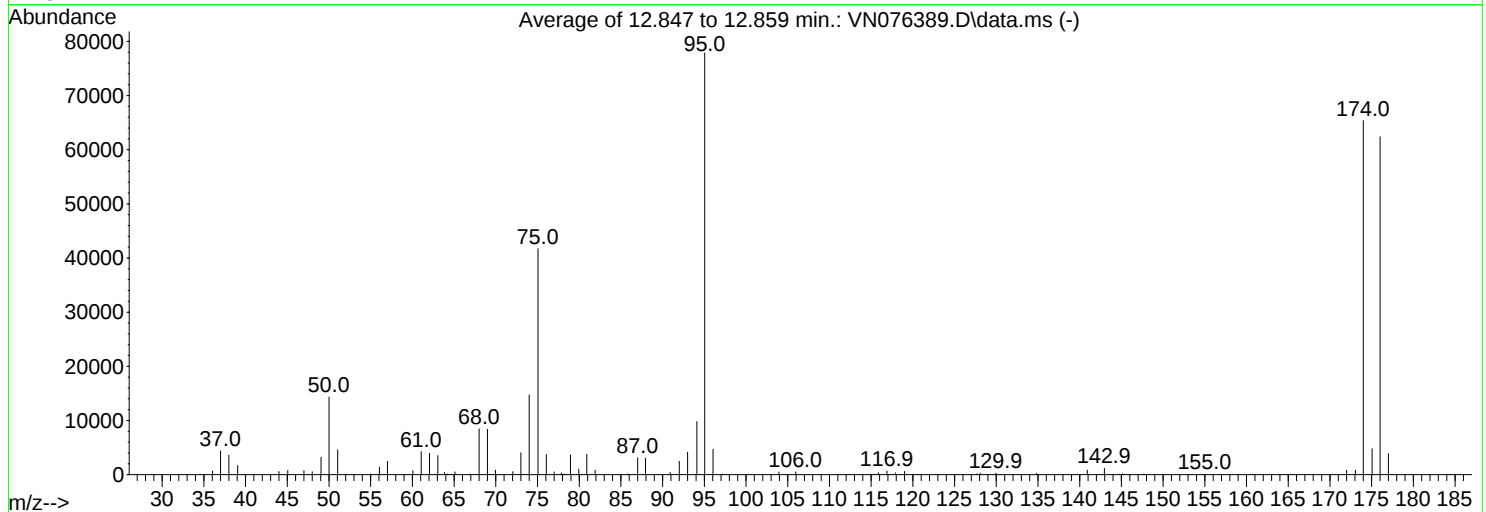


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012523\
Data File : VN076389.D
Acq On : 25 Jan 2023 09:41
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Title : SW846 8260
Last Update : Tue Jan 17 03:59:22 2023

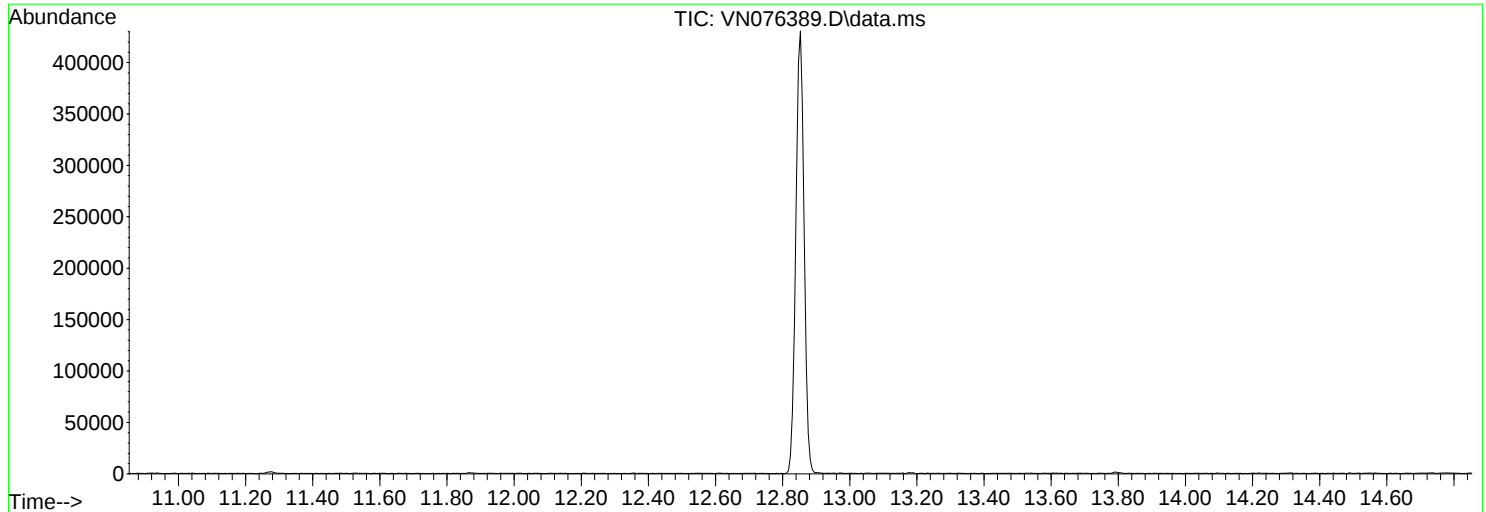

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	14326	PASS
75	95	30	60	53.6	41712	PASS
95	95	100	100	100.0	77885	PASS
96	95	5	9	6.0	4699	PASS
173	174	0.00	2	1.2	785	PASS
174	95	50	100	83.9	65373	PASS
175	174	5	9	7.3	4792	PASS
176	174	95	101	95.4	62384	PASS
177	176	5	9	6.2	3873	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	686	51.05	4581	63.85	419	75.05	4171
37.00	4360	51.90	51	64.20	114	76.05	371
38.00	3613	52.10	94	65.10	500	77.00	51
39.05	1681	55.00	141	66.80	86	77.85	30
39.85	12	56.05	1404	67.00	79	78.20	109
44.00	574	57.00	2463	68.00	8457	78.95	3635
45.05	775	57.90	64	69.00	8371	79.95	1015
47.00	742	60.05	745	69.95	817	80.90	3759
48.00	534	61.05	4248	72.05	566	81.90	820
49.05	3226	62.05	3942	73.00	4056	83.00	54
50.00	14326	63.05	3528	74.00	14732	85.85	159

Average of 12.847 to 12.859 min.: VN076389.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.00	3135	105.95	512	129.95	290	156.80	62
87.95	3053	112.90	65	134.85	265	157.00	52
90.90	419	114.90	50	140.90	871	158.90	62
92.00	2452	115.85	370	142.10	53	160.80	53
93.00	4129	116.90	683	142.95	1163	172.00	839
94.10	9803	117.60	75	144.80	62	173.05	785
95.05	77885	117.90	320	145.15	164	174.00	65373
96.05	4699	119.00	595	145.90	59	175.05	4792
97.20	83	127.70	150	147.70	134	176.00	62384
103.95	490	128.05	269	154.80	57	177.00	3873
104.80	56	128.90	93	155.00	73		

Instrument :

MSVOA_N

ClientSampleId :

BFB