

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012621\
 Data File : VN065610.D
 Acq On : 26 Jan 2021 17:40
 Operator : JC/MD
 Sample : M1229-01 50X
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TRE-1125

Quant Time: Jan 27 03:30:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012521W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jan 25 13:47:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.624	168	207625	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.550	114	365101	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.376	117	324256	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.315	152	120008	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.987	65	134881	49.38	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	98.76%		
35) Dibromofluoromethane	7.550	113	106822	49.37	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	98.74%		
50) Toluene-d8	10.058	98	456153	53.64	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	107.28%		
62) 4-Bromofluorobenzene	12.373	95	155244	50.69	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	101.38%		
Target Compounds						Qvalue
16) Acetone	3.785	43	17021	16.01	ug/l	96
52) Toluene	10.122	92	39828	5.99	ug/l	97
67) Ethyl Benzene	11.479	91	9594	0.75	ug/l	100
68) m/p-Xylenes	11.588	106	13633	2.96	ug/l	92
69) o-Xylene	11.916	106	7821	1.75	ug/l	91
84) 1,2,4-Trimethylbenzene	13.009	105	10580	1.19	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012621\
Data File : VN065610.D
Acq On : 26 Jan 2021 17:40
Operator : JC/MD
Sample : M1229-01 50X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TRE-1125

Quant Time: Jan 27 03:30:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012521W.M
Quant Title : SW846 8260
QLast Update : Mon Jan 25 13:47:28 2021
Response via : Initial Calibration




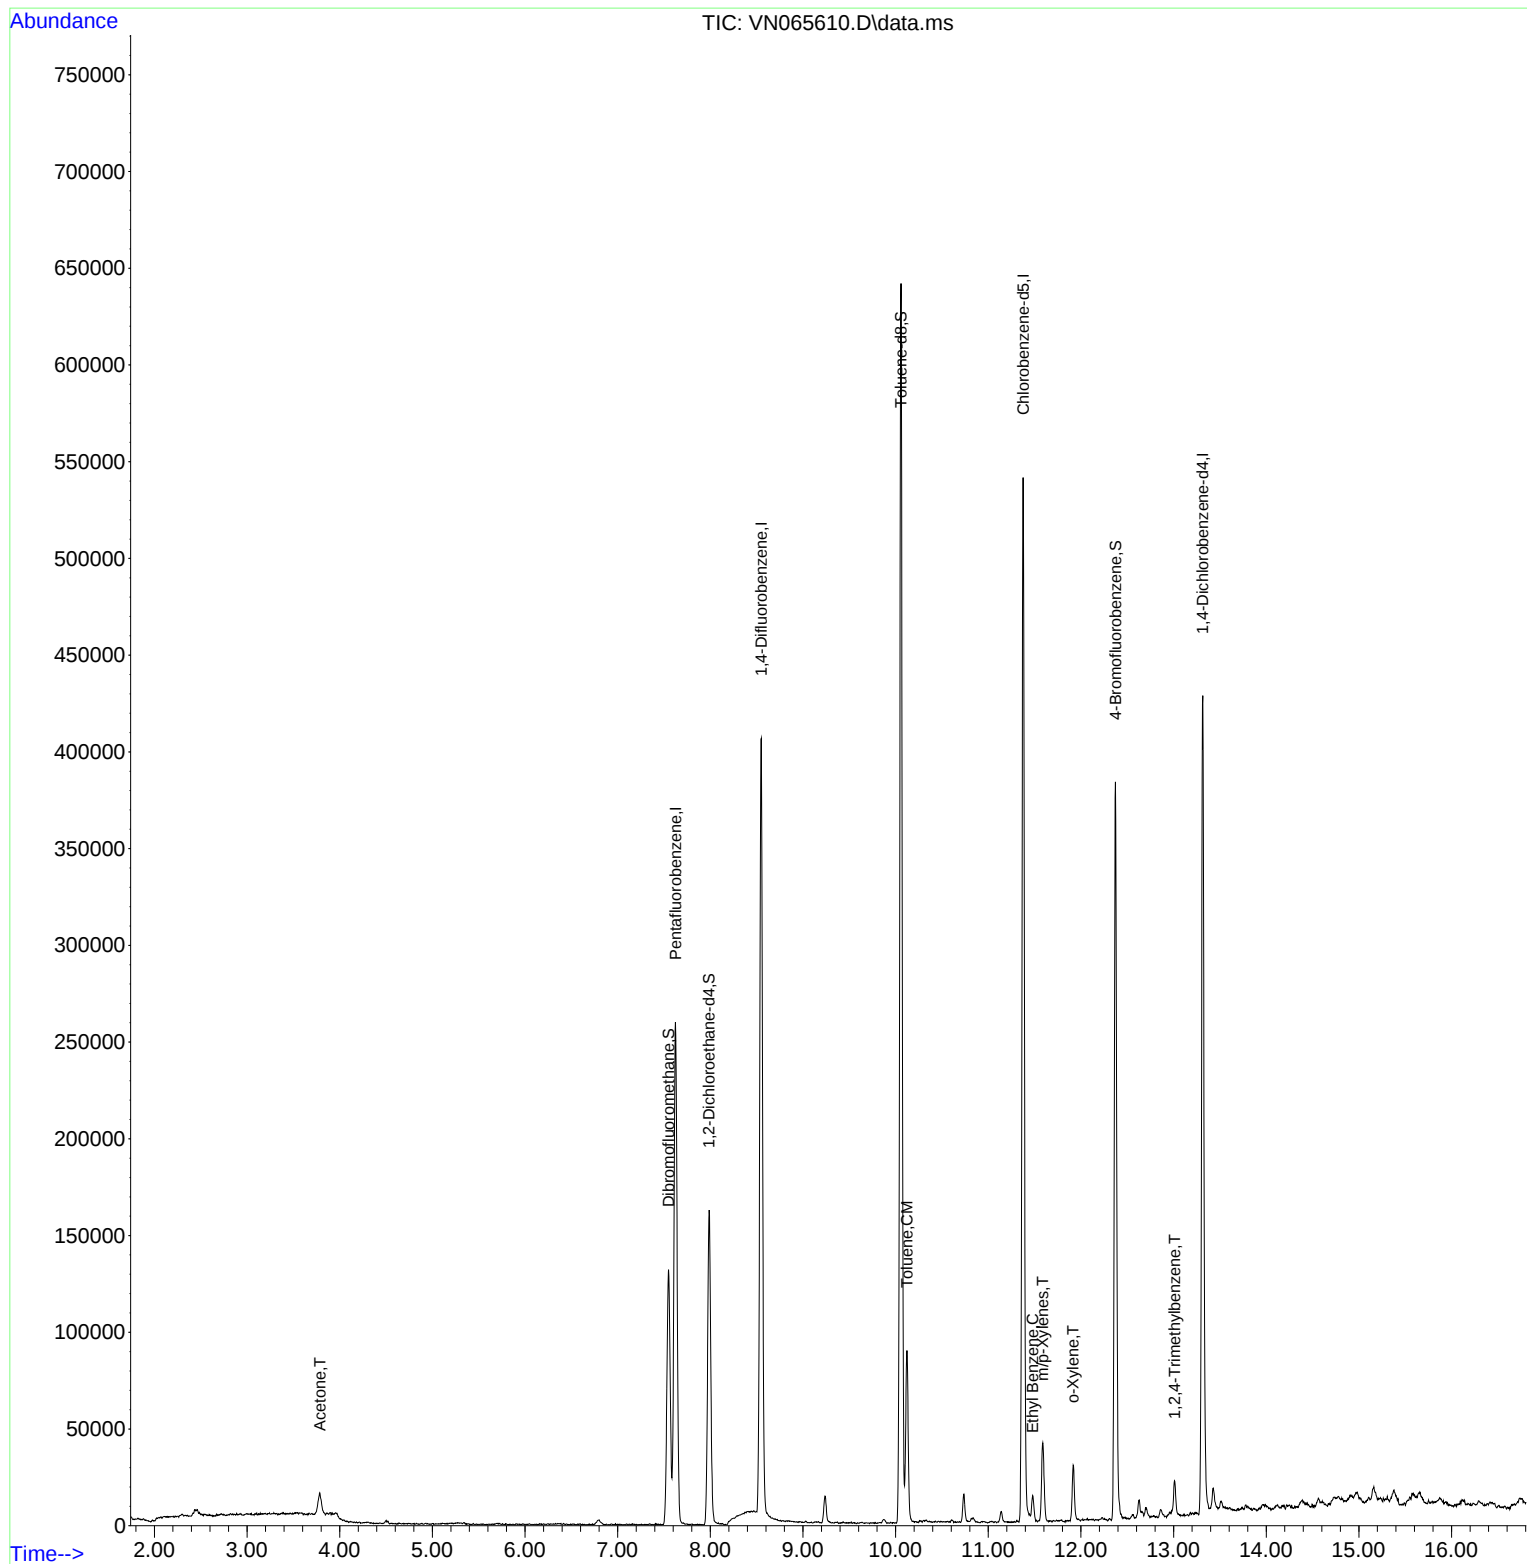


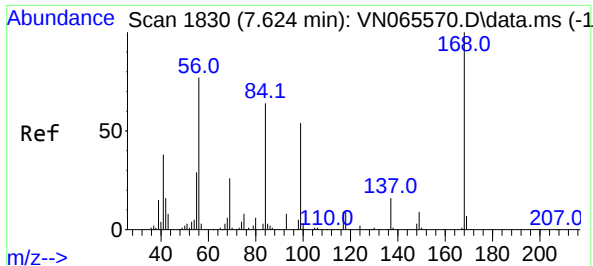

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.624 min Scan# 1830
Delta R.T. -0.000 min
Lab File: VN065610.D
Acq: 26 Jan 2021 17:40




Instrument :
MSVOA_N
ClientSampleId :
TRE-1125


Tgt Ion:168 Resp: 207625
Ion Ratio Lower Upper
168 100
99 61.4 42.6 63.8

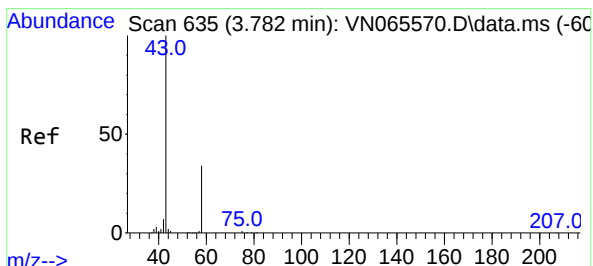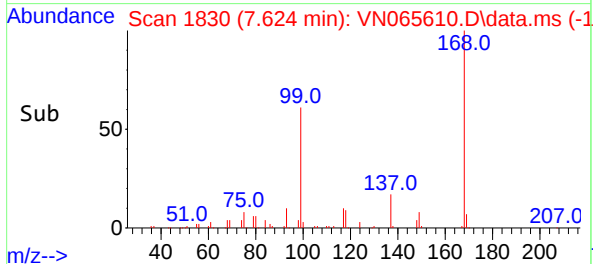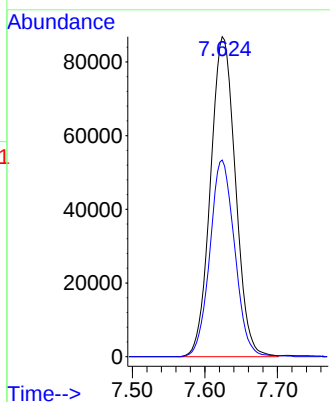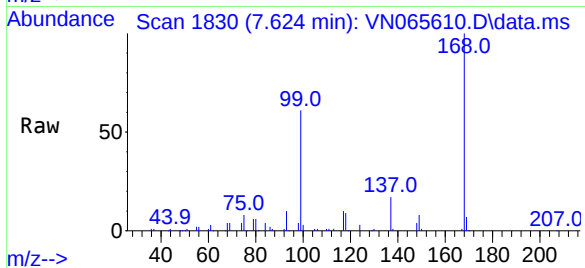

#16
Acetone
Concen: 16.01 ug/l
RT: 3.785 min Scan# 636
Delta R.T. 0.003 min
Lab File: VN065610.D
Acq: 26 Jan 2021 17:40

Tgt Ion: 43 Resp: 17021
Ion Ratio Lower Upper
43 100
58 36.1 27.0 40.6

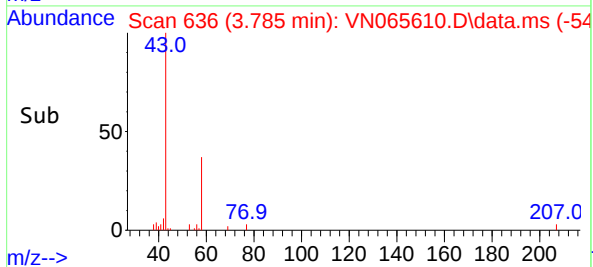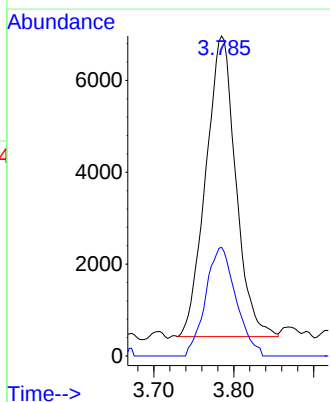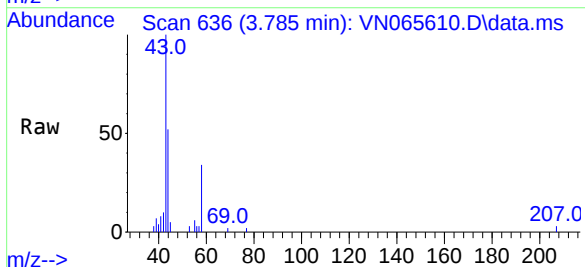




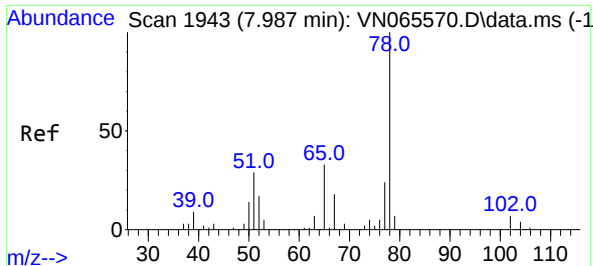


#33

1,2-Dichloroethane-d4
Concen: 49.38 ug/l
RT: 7.987 min Scan# 1943
Delta R.T. 0.000 min
Lab File: VN065610.D
Acq: 26 Jan 2021 17:40

Instrument :
MSVOA_N
ClientSampleId :
TRE-1125




Tgt Ion: 65 Resp: 134881
Ion Ratio Lower Upper
65 100
67 55.5 0.0 107.2

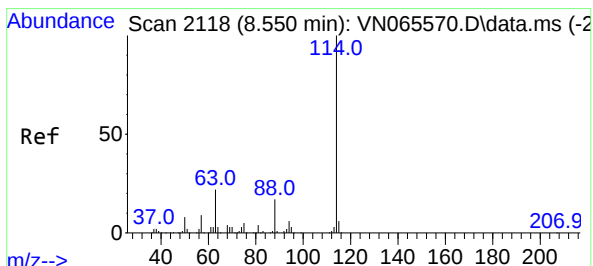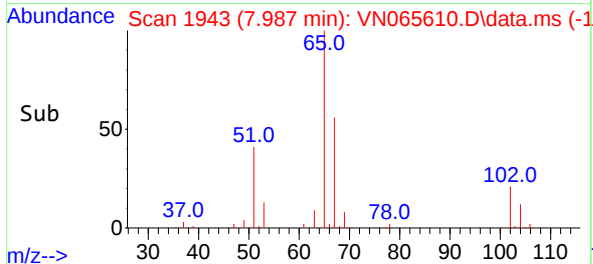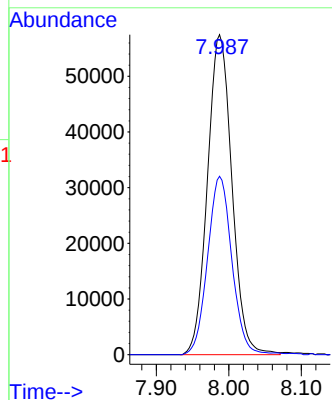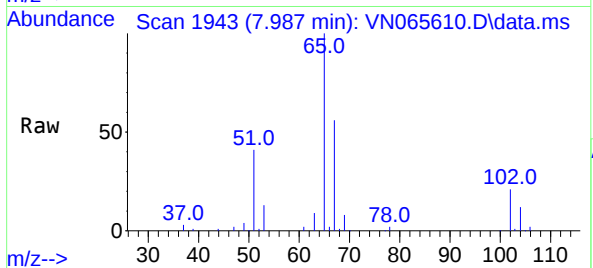


#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.550 min Scan# 2118
Delta R.T. -0.000 min
Lab File: VN065610.D
Acq: 26 Jan 2021 17:40

Tgt Ion: 114 Resp: 365101
Ion Ratio Lower Upper
114 100
63 22.5 0.0 38.6
88 16.8 0.0 30.6


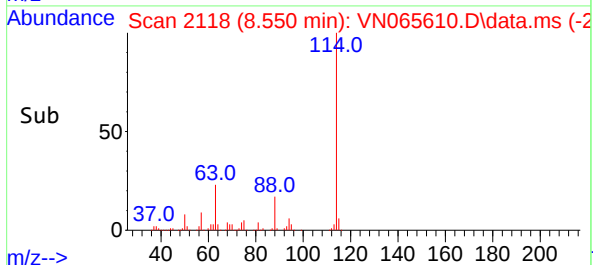
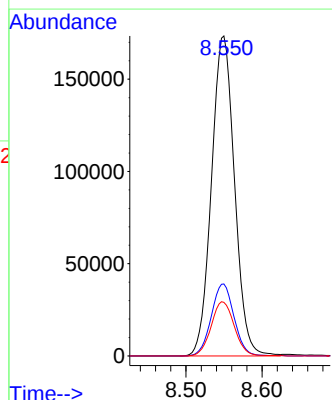
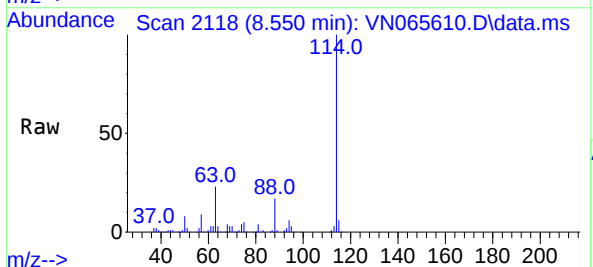


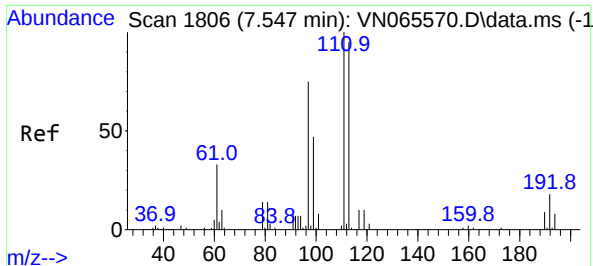

#35
Dibromofluoromethane
Concen: 49.37 ug/l
RT: 7.550 min Scan# 1807
Delta R.T. 0.003 min
Lab File: VN065610.D
Acq: 26 Jan 2021 17:40




Instrument :
MSVOA_N
ClientSampleId :
TRE-1125


Tgt Ion:113 Resp: 106822
Ion Ratio Lower Upper
113 100
111 104.4 82.2 123.2
192 17.4 15.4 23.0

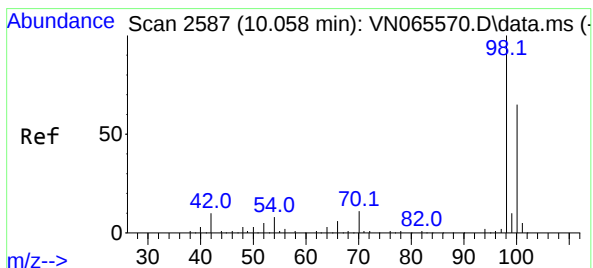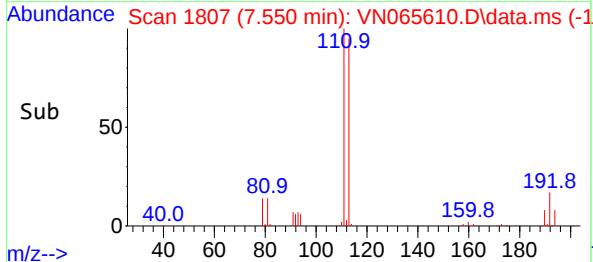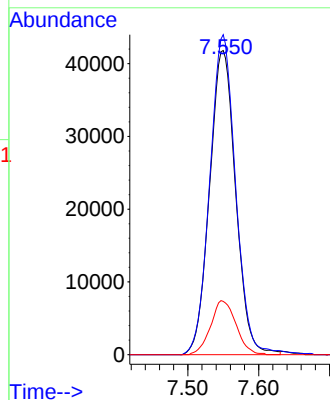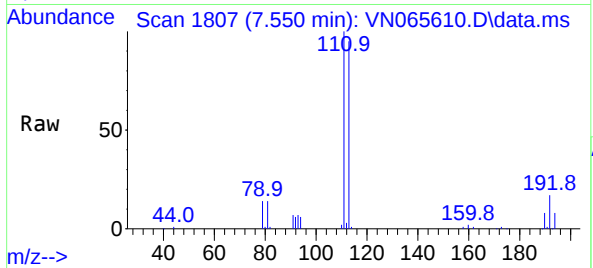

#50
Toluene-d8
Concen: 53.64 ug/l
RT: 10.058 min Scan# 2587
Delta R.T. -0.000 min
Lab File: VN065610.D
Acq: 26 Jan 2021 17:40

Tgt Ion: 98 Resp: 456153
Ion Ratio Lower Upper
98 100
100 64.7 50.5 75.7


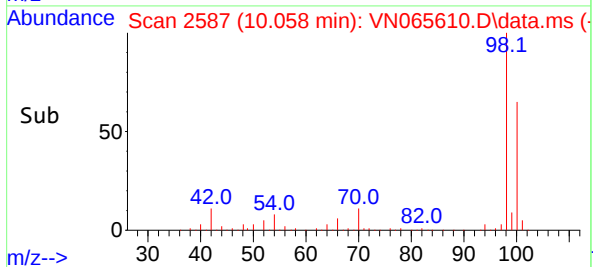
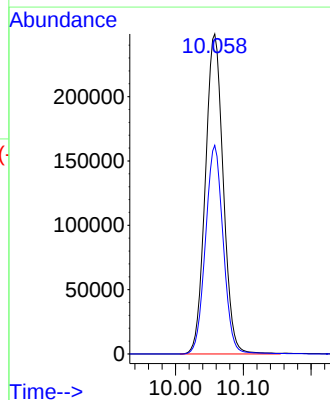
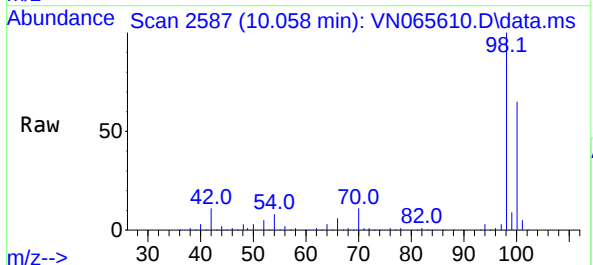


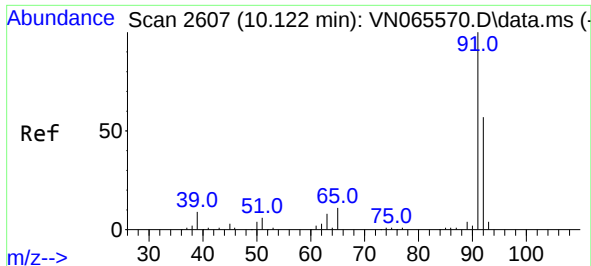

#52
Toluene
Concen: 5.99 ug/l
RT: 10.122 min Scan# 2607
Delta R.T. 0.000 min
Lab File: VN065610.D
Acq: 26 Jan 2021 17:40




Instrument :
MSVOA_N
ClientSampled :
TRE-1125


Tgt Ion: 92 Resp: 39828
Ion Ratio Lower Upper
92 100
91 171.9 140.7 211.1

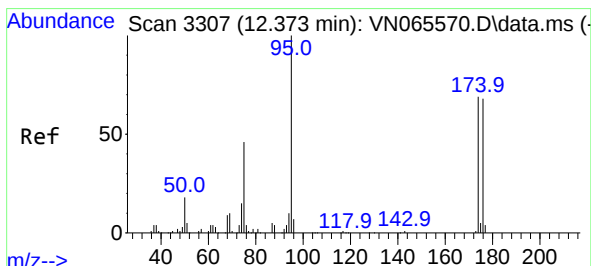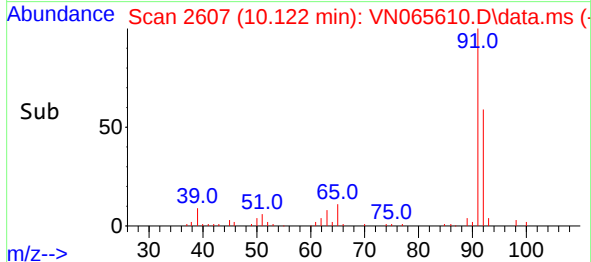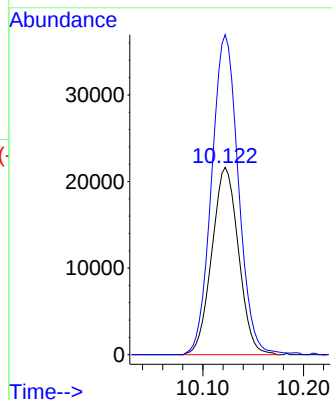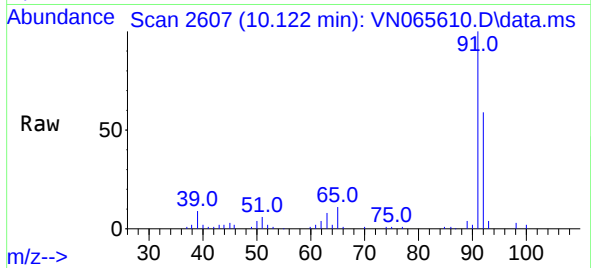

#62
4-Bromofluorobenzene
Concen: 50.69 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. -0.000 min
Lab File: VN065610.D
Acq: 26 Jan 2021 17:40

Tgt Ion: 95 Resp: 155244
Ion Ratio Lower Upper
95 100
174 67.5 0.0 169.0
176 64.8 0.0 162.4


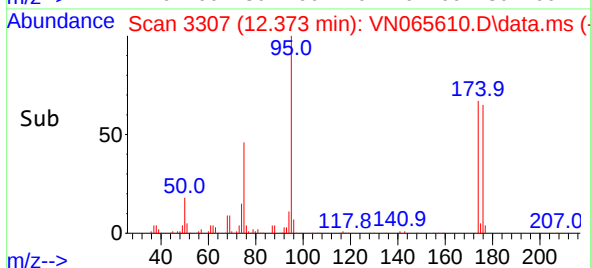
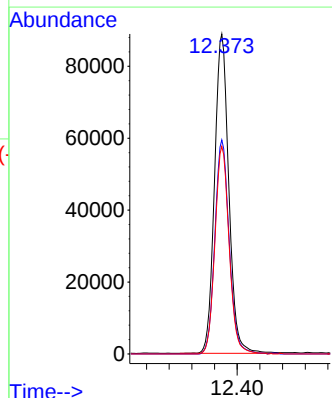
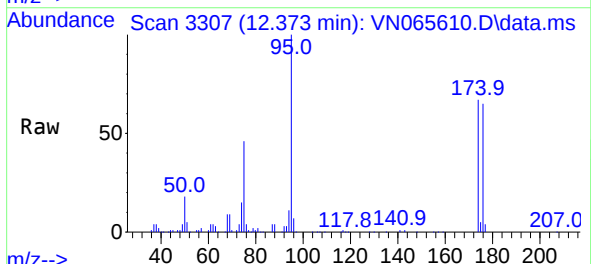


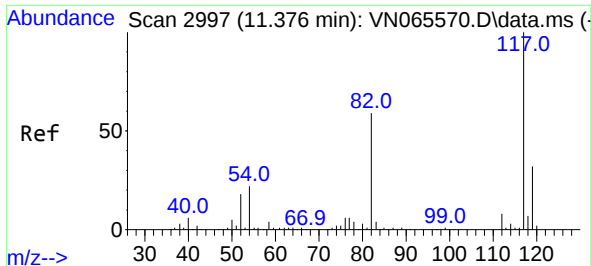

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.376 min Scan# 2997
Delta R.T. 0.000 min
Lab File: VN065610.D
Acq: 26 Jan 2021 17:40




Instrument :
MSVOA_N
ClientSampleId :
TRE-1125


Tgt Ion:117 Resp: 324256
Ion Ratio Lower Upper
117 100
82 58.4 43.7 65.5
119 31.5 26.1 39.1

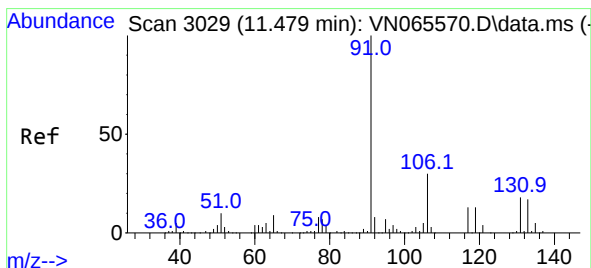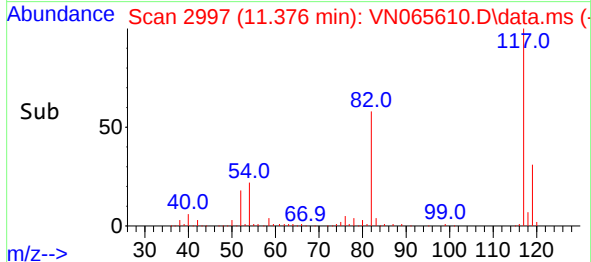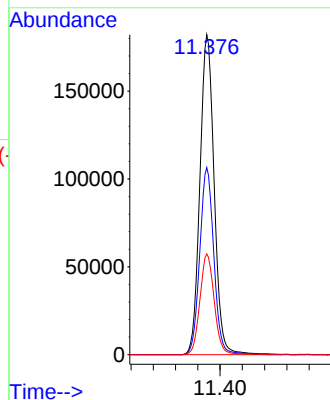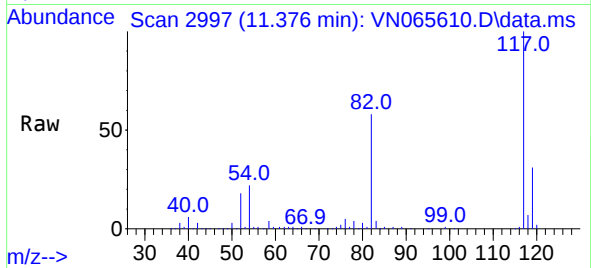

#67
Ethyl Benzene
Concen: 0.75 ug/l
RT: 11.479 min Scan# 3029
Delta R.T. -0.000 min
Lab File: VN065610.D
Acq: 26 Jan 2021 17:40

Tgt Ion: 91 Resp: 9594
Ion Ratio Lower Upper
91 100
106 31.8 25.5 38.3


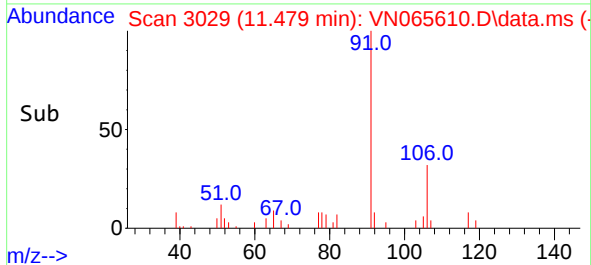
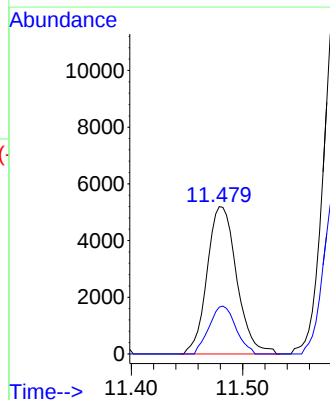
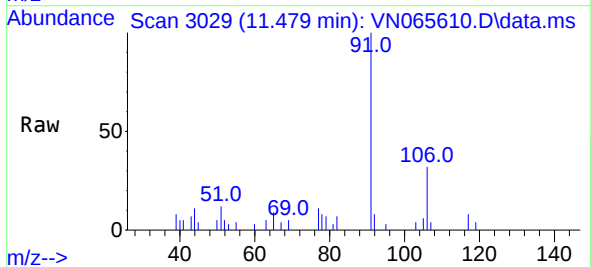


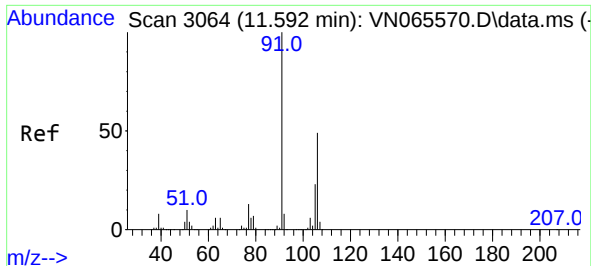

#68
m/p-Xylenes
Concen: 2.96 ug/l
RT: 11.588 min Scan# 3063
Delta R.T. -0.004 min
Lab File: VN065610.D
Acq: 26 Jan 2021 17:40




Instrument :
MSVOA_N
ClientSampleId :
TRE-1125


Tgt Ion:106 Resp: 13633
Ion Ratio Lower Upper
106 100
91 214.0 161.4 242.0

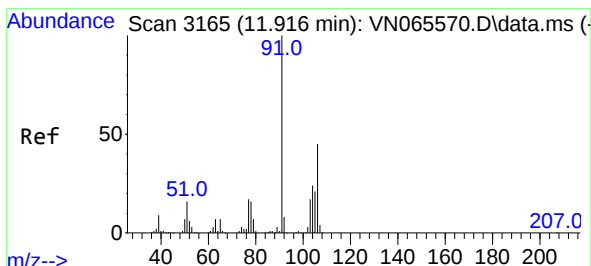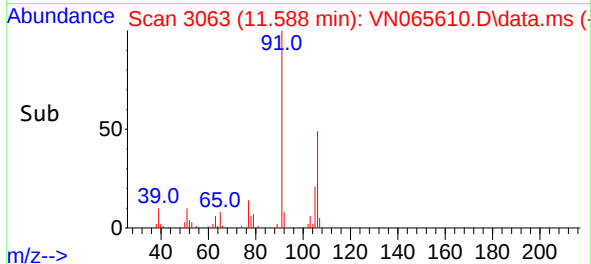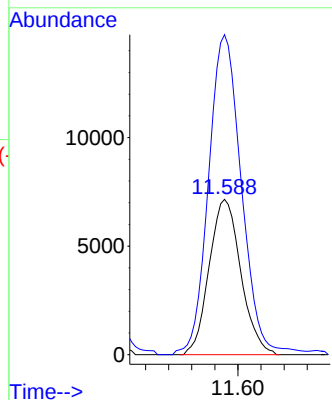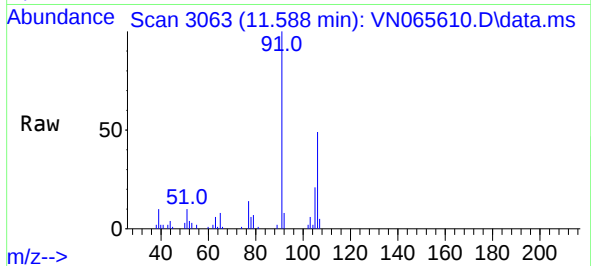

#69
o-Xylene
Concen: 1.75 ug/l
RT: 11.916 min Scan# 3165
Delta R.T. 0.000 min
Lab File: VN065610.D
Acq: 26 Jan 2021 17:40

Tgt Ion:106 Resp: 7821
Ion Ratio Lower Upper
106 100
91 227.6 106.8 320.4


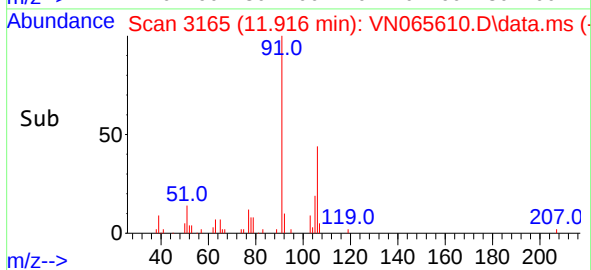
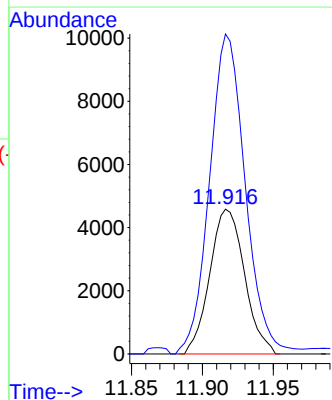
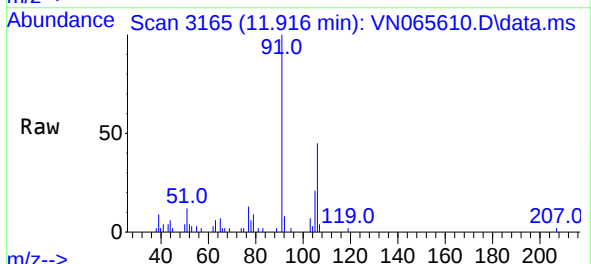


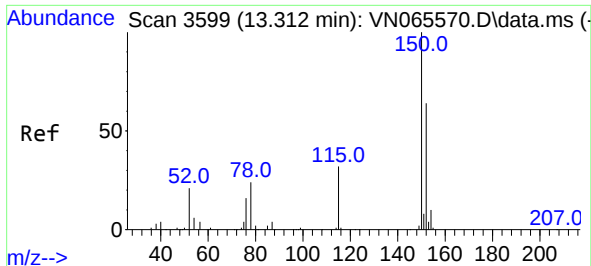

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.315 min Scan# 3600
Delta R.T. 0.003 min
Lab File: VN065610.D
Acq: 26 Jan 2021 17:40

Instrument :
MSVOA_N
ClientSampleId :
TRE-1125

Tgt Ion:152 Resp: 120008
Ion Ratio Lower Upper
152 100
115 62.8 28.5 85.6
150 158.9 0.0 347.6

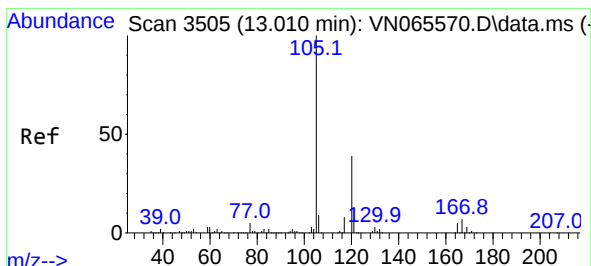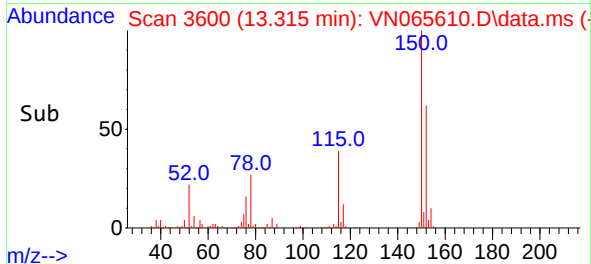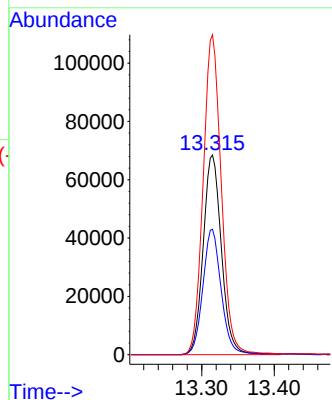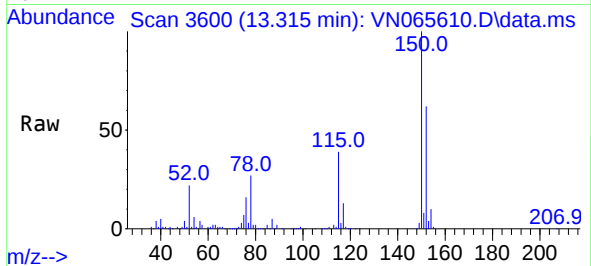

#84
1,2,4-Trimethylbenzene
Concen: 1.19 ug/l
RT: 13.009 min Scan# 3505
Delta R.T. -0.001 min
Lab File: VN065610.D
Acq: 26 Jan 2021 17:40

Tgt Ion:105 Resp: 10580
Ion Ratio Lower Upper
105 100
120 40.9 22.4 67.0

