

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012622\
 Data File : VN070794.D
 Acq On : 26 Jan 2022 17:04
 Operator : JC/MD
 Sample : N1267-17
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BASEMENT-WALLS

Quant Time: Jan 27 03:33:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 18 13:32:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.086	168	842238	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	1340293	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	1215313	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	479123	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	579386	48.000	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	96.000%		
35) Dibromofluoromethane	8.021	113	397037	47.756	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	95.520%		
50) Toluene-d8	10.440	98	1691714	48.301	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	96.600%		
62) 4-Bromofluorobenzene	12.728	95	597372	47.864	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	95.720%		
Target Compounds					Qvalue	
11) Tert butyl alcohol	5.374	59	934	0.429	ug/l #	78
16) Acetone	4.288	43	114005	13.608	ug/l	100
18) Methyl Acetate	4.859	43	10916	0.663	ug/l #	63
20) Methylene Chloride	5.101	84	18890	1.712	ug/l	95
25) 2-Butanone	7.337	43	24032	2.280	ug/l #	86
29) Tetrahydrofuran	7.697	42	2836	0.439	ug/l #	42
30) Chloroform	8.075	83	140	Below Cal	#	18
31) Cyclohexane	8.088	56	20362	0.958	ug/l #	20
36) 1,1-Dichloropropene	8.086	75	69241	4.947	ug/l #	49
37) Ethyl Acetate	7.337	43	24032	1.293	ug/l #	68
38) Carbon Tetrachloride	8.086	117	86593	6.955	ug/l #	16
43) Isopropyl Acetate	8.563	43	85748	3.021	ug/l #	86
45) 1,2-Dichloropropane	9.622	63	5070	0.430	ug/l #	44
48) Methyl methacrylate	9.539	41	21083	1.559	ug/l #	8
49) 1,4-Dioxane	9.617	88	517	2.546	ug/l #	1
51) 4-Methyl-2-Pentanone	10.328	43	10444	0.577	ug/l #	73
53) t-1,3-Dichloropropene	10.639	75	27	2.405	ug/l #	1
54) cis-1,3-Dichloropropene	10.242	75	109218	6.494	ug/l #	64
56) Ethyl methacrylate	10.872	69	1028	2.352	ug/l #	1
57) 1,3-Dichloropropane	11.089	76	61838	3.428	ug/l #	43
59) 2-Hexanone	11.089	43	1025452	77.944	ug/l #	49
71) Bromoform	12.733	173	3618	0.528	ug/l #	1
74) N-amyl acetate	12.358	43	4552	0.246	ug/l #	45
76) 1,2,3-Trichloropropane	12.731	75	317280	24.968	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.731	75	317280	74.383	ug/l #	5
93) 1,2,4-Trichlorobenzene	15.257	180	413	3.469	ug/l #	47
95) Naphthalene	15.507	128	2389	5.035	ug/l #	76
96) 1,2,3-Trichlorobenzene	15.700	180	568	3.279	ug/l #	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012622\
Data File : VN070794.D
Acq On : 26 Jan 2022 17:04
Operator : JC/MD
Sample : N1267-17
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BASEMENT-WALLS

Quant Time: Jan 27 03:33:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 18 13:32:07 2022
Response via : Initial Calibration




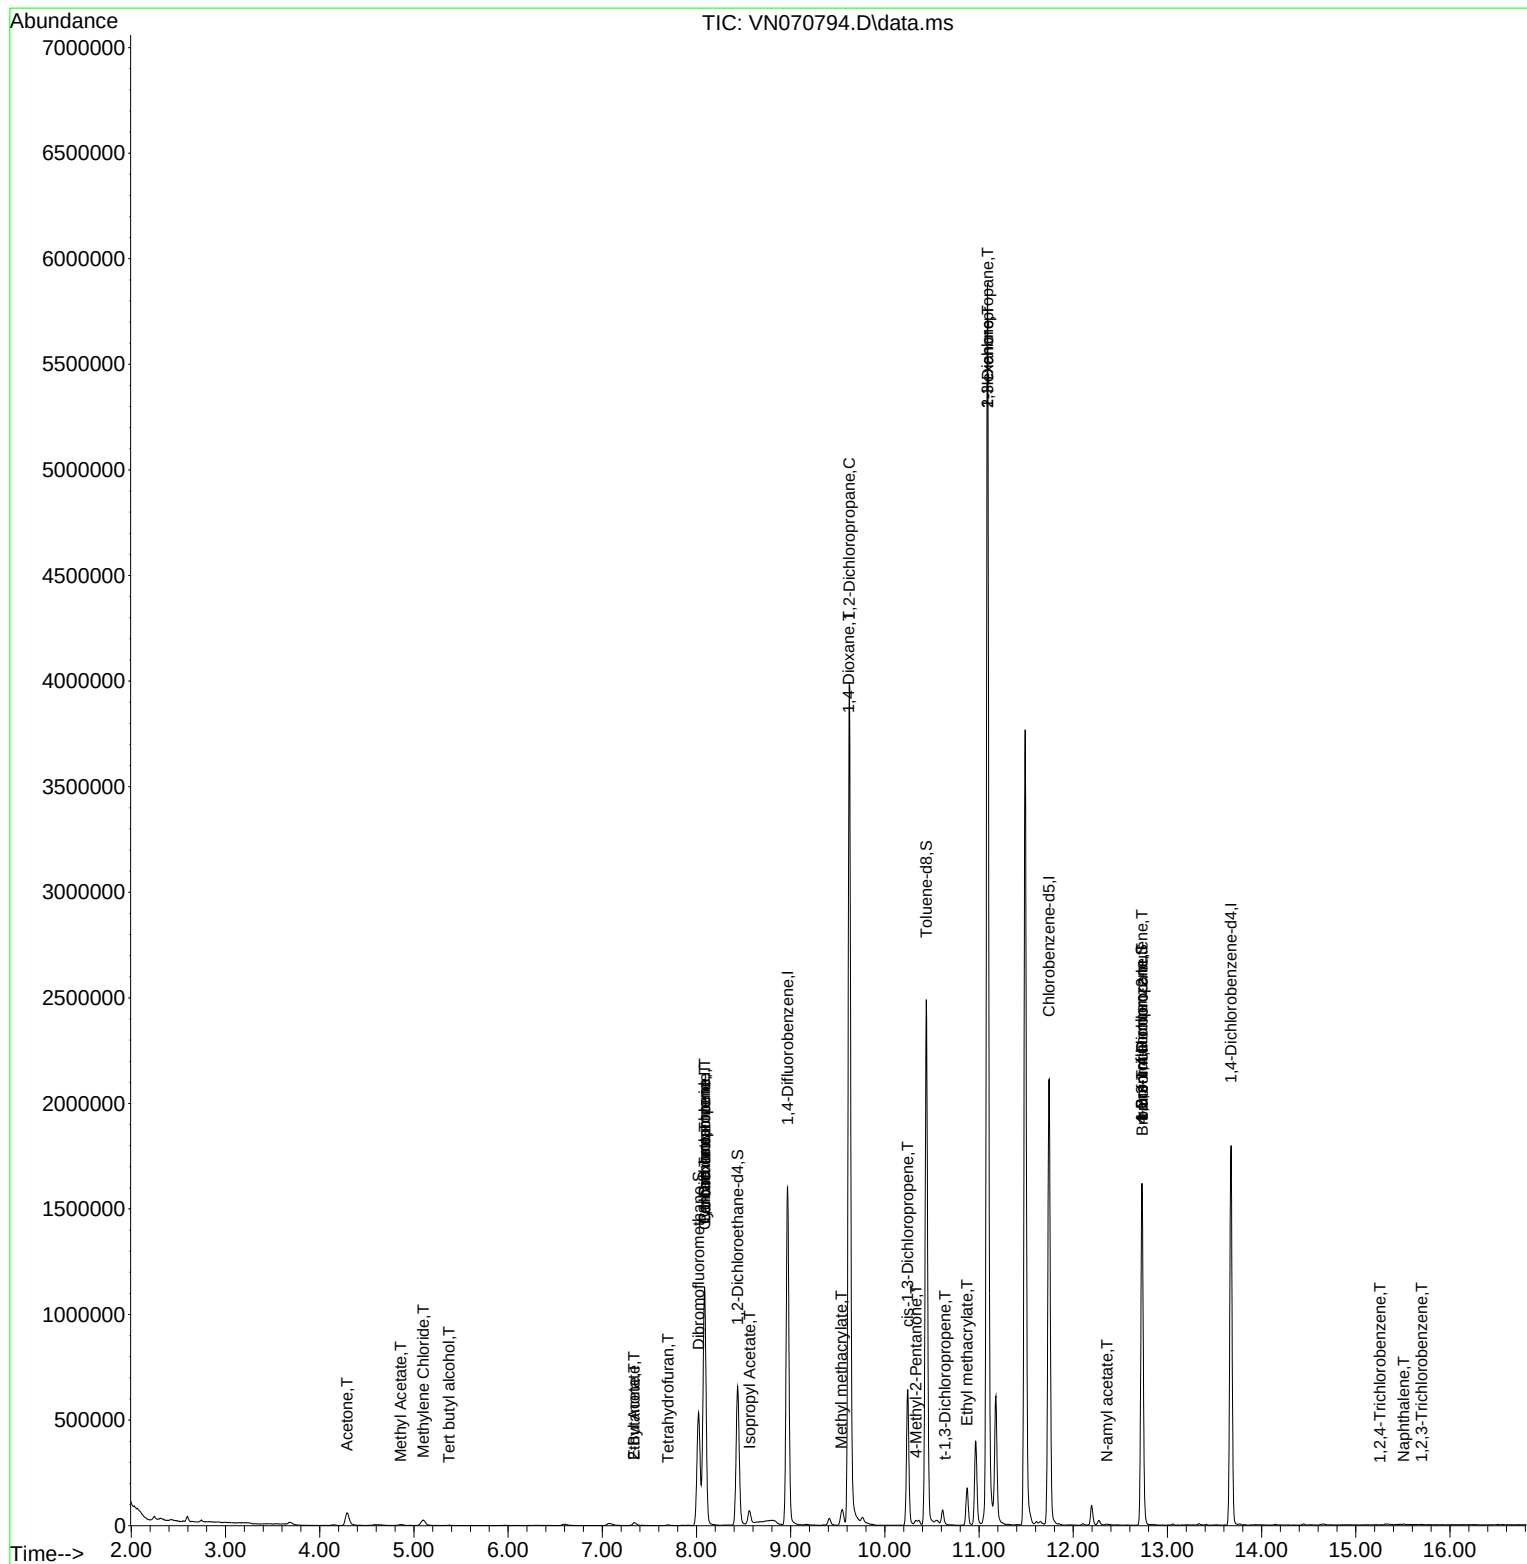


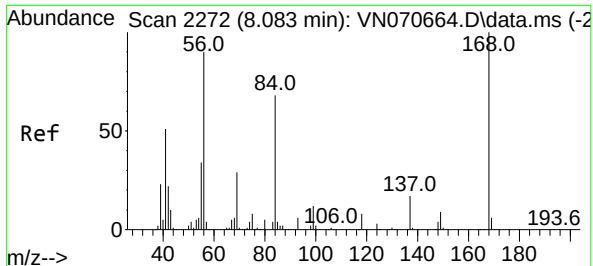

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 21
Delta R.T. 0.003 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04




Instrument :
MSVOA_N
ClientSampleId :
BASEMENT-WALLS


Tgt Ion:168 Resp: 842238
Ion Ratio Lower Upper
168 100
99 61.8 41.3 61.9

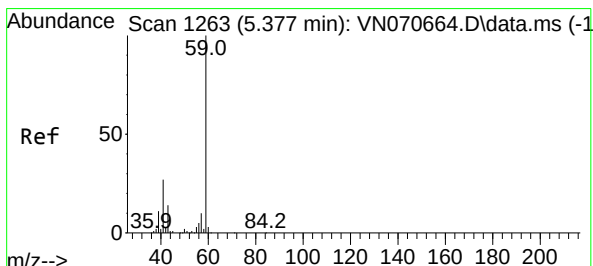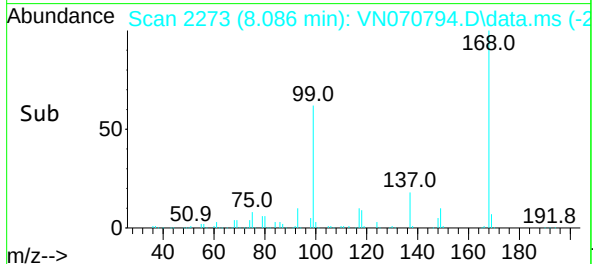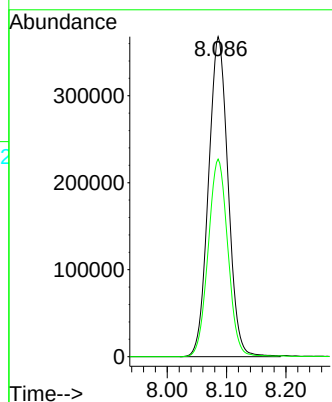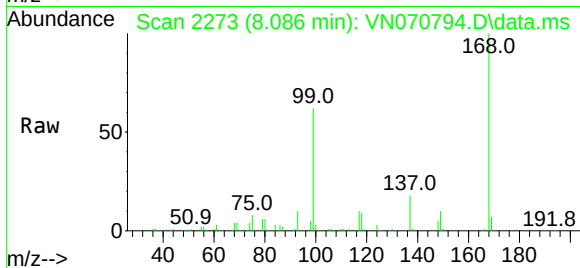

#11
Tert butyl alcohol
Concen: 0.429 ug/l
RT: 5.374 min Scan# 1262
Delta R.T. -0.003 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04

Tgt Ion: 59 Resp: 934
Ion Ratio Lower Upper
59 100
57 2.7 8.7 13.1#


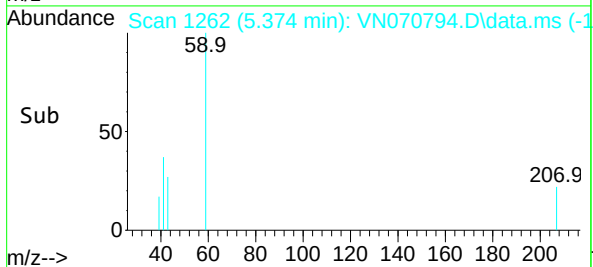
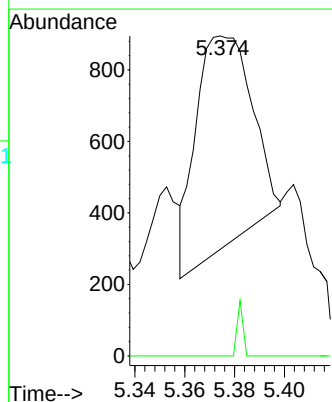
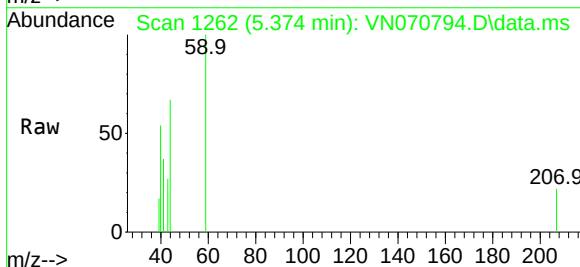




#16
Acetone
Concen: 13.608 ug/l
RT: 4.288 min Scan# 856
Delta R.T. 0.003 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04




Instrument :
MSVOA_N
ClientSampleId :
BASEMENT-WALLS


Tgt Ion: 43 Resp: 114005
Ion Ratio Lower Upper
43 100
58 28.9 23.1 34.7

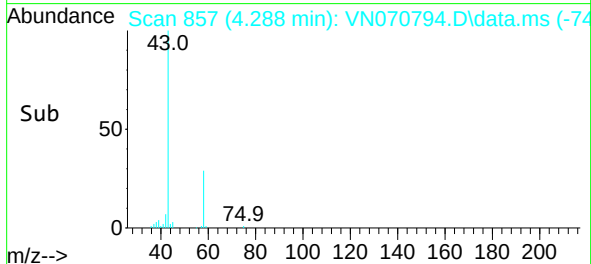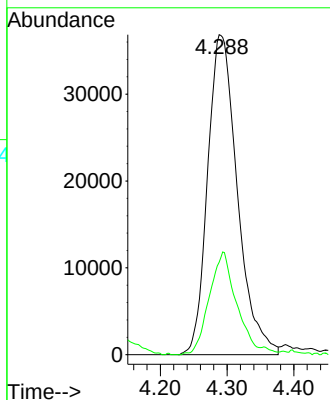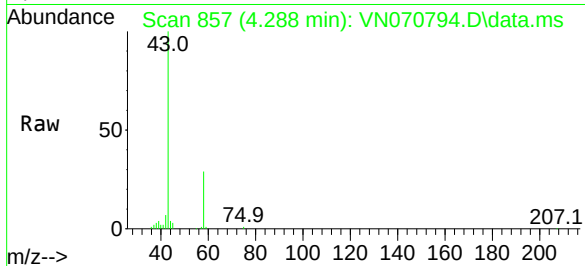

#18
Methyl Acetate
Concen: 0.663 ug/l
RT: 4.859 min Scan# 1070
Delta R.T. 0.005 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04


Tgt Ion: 43 Resp: 10916
Ion Ratio Lower Upper
43 100
74 6.0 19.4 29.2#

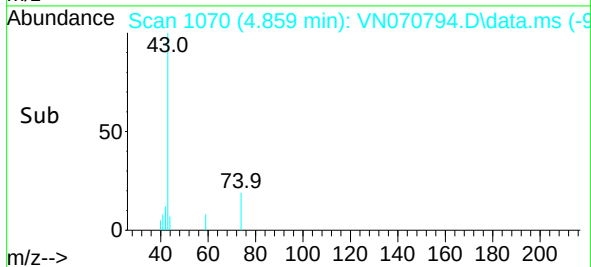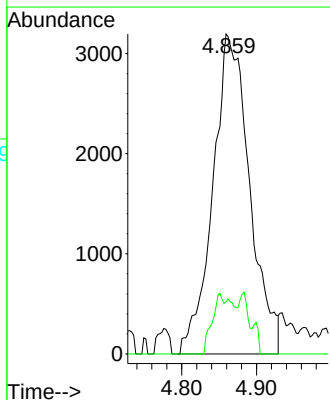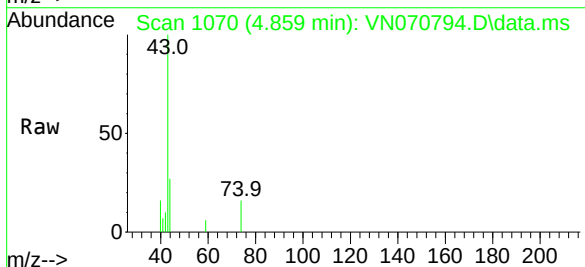



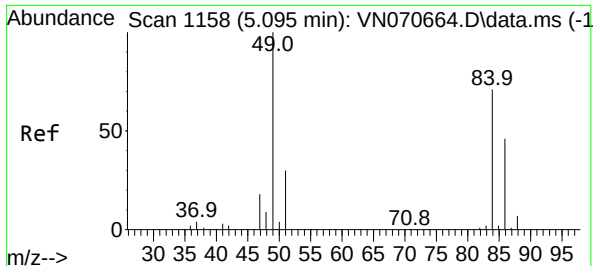


#20
Methylene Chloride
Concen: 1.712 ug/l
RT: 5.101 min Scan# 1158
Delta R.T. 0.006 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04

Instrument :
MSVOA_N
ClientSampleId :
BASEMENT-WALLS



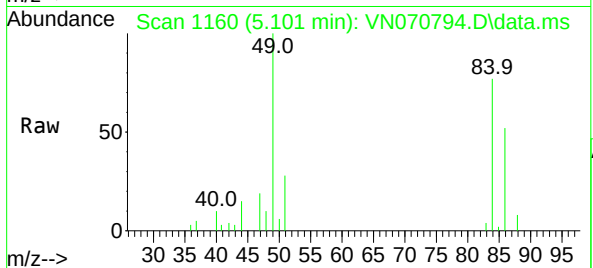



Tgt Ion: 84	Resp: 18890
Ion Ratio	Lower Upper
84 100	
49 126.1	93.5 140.3
51 36.4	29.4 44.2
86 67.0	53.0 79.4

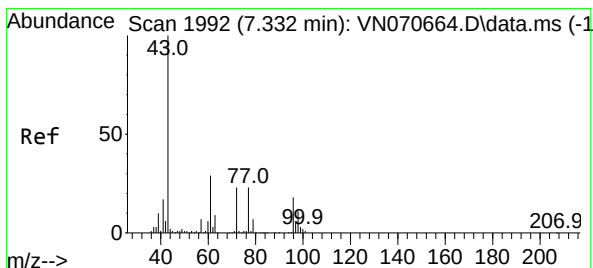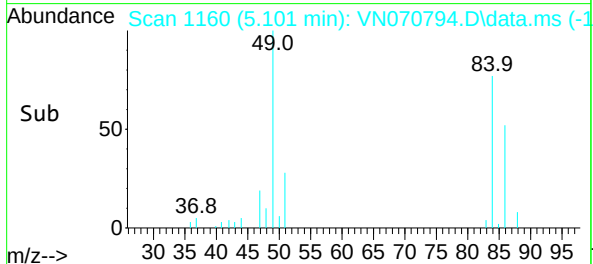

#25
2-Butanone
Concen: 2.280 ug/l
RT: 7.337 min Scan# 1994
Delta R.T. 0.005 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04

Tgt Ion: 43	Resp: 24032		
Ion Ratio	Lower	Upper	
43	100		
72	19.7	21.7	32.5#

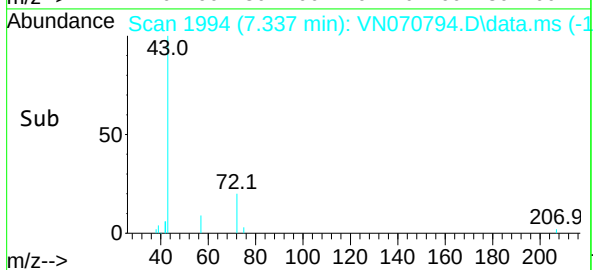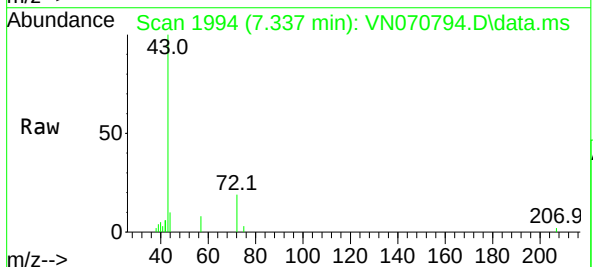



#29

Tetrahydrofuran

Concen: 0.439 ug/l

RT: 7.697 min Scan# 2123

Delta R.T. 0.014 min

Lab File: VN070794.D


Acq: 26 Jan 2022 17:04

Instrument :




MSVOA_N

ClientSampleId :

BASEMENT-WALLS

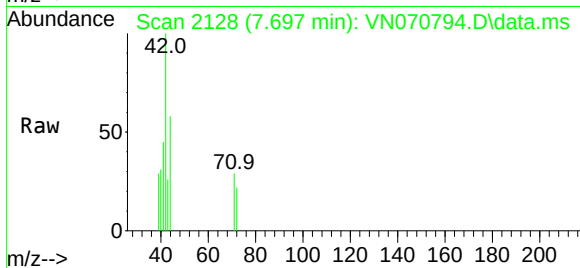

Tgt Ion:	42	Resp:	2836
Ion	Ratio	Lower	Upper
42	100		
72	9.6	36.3	54.5#
71	4.4	34.7	52.1#

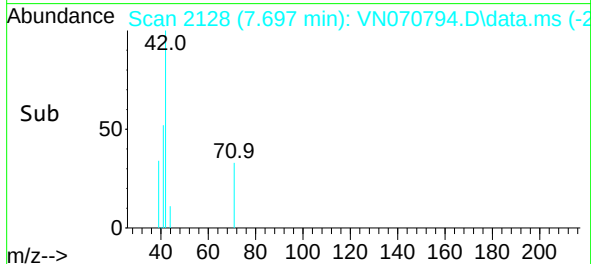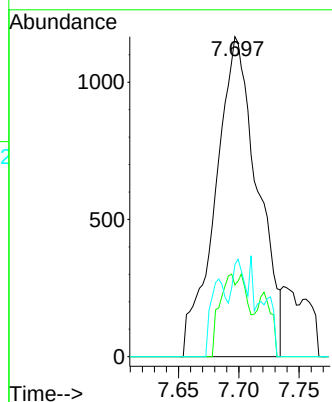

#30

Chloroform

Concen: Below Cal




RT: 8.075 min Scan# 2269


Delta R.T. 0.257 min

Lab File: VN070794.D

Acq: 26 Jan 2022 17:04

Tgt Ion:	83	Resp:	140
Ion	Ratio	Lower	Upper
83	100		
85	0.0	51.9	77.9#


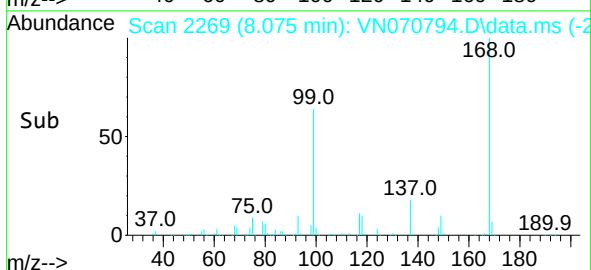

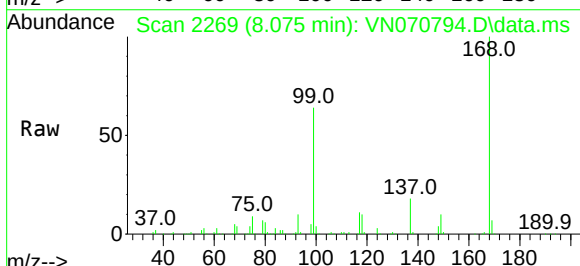




#31
Cyclohexane
Concen: 0.958 ug/l
RT: 8.088 min Scan# 21
Delta R.T. -0.006 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04




Instrument :
MSVOA_N
ClientSampleId :
BASEMENT-WALLS


Tgt Ion: 56 Resp: 20362
Ion Ratio Lower Upper
56 100
69 157.4 27.1 40.7#
84 120.3 73.4 110.0#

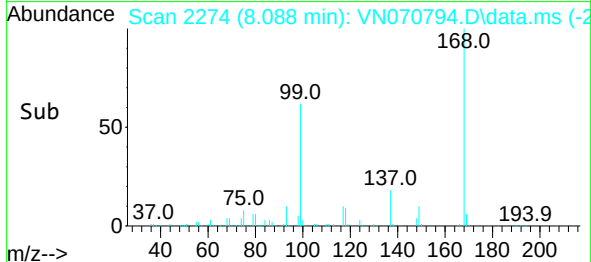

#33
1,2-Dichloroethane-d4
Concen: 48.000 ug/l
RT: 8.437 min Scan# 2404
Delta R.T. 0.003 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04

Tgt Ion: 65 Resp: 579386
Ion Ratio Lower Upper
65 100
67 51.1 0.0 103.0


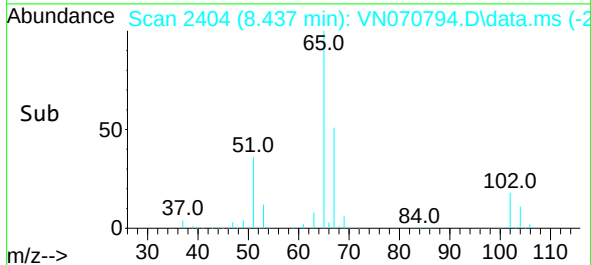

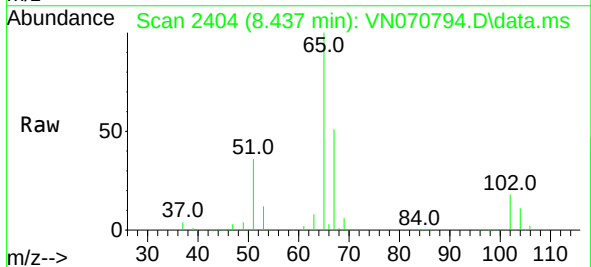




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.968 min Scan# 2601
Delta R.T. 0.003 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04




Instrument :
MSVOA_N
ClientSampleId :
BASEMENT-WALLS


Tgt Ion:114 Resp: 1340293
Ion Ratio Lower Upper
114 100
63 23.4 0.0 37.8
88 17.1 0.0 27.4

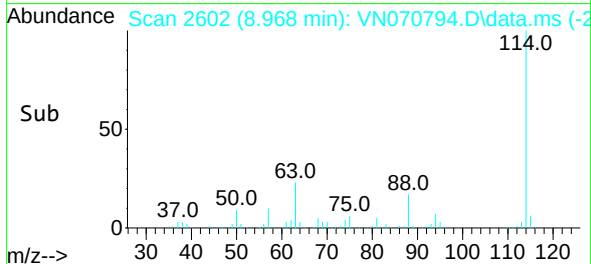

#35
Dibromofluoromethane
Concen: 47.756 ug/l
RT: 8.021 min Scan# 2249
Delta R.T. 0.002 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04

Tgt Ion:113 Resp: 397037
Ion Ratio Lower Upper
113 100
111 102.5 82.2 123.2
192 19.4 16.9 25.3


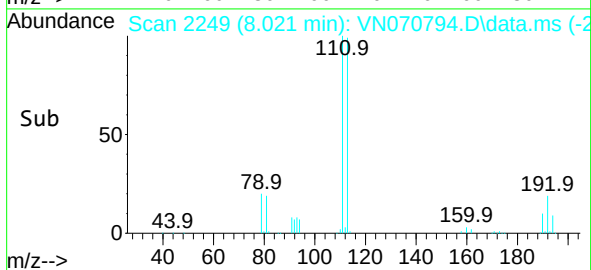

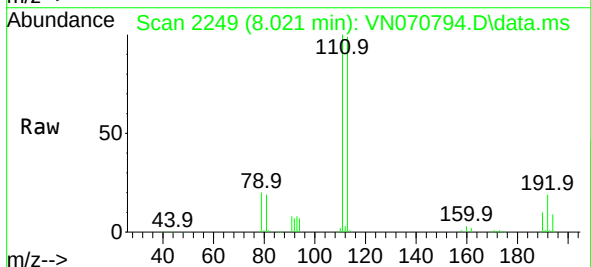




#36
1,1-Dichloropropene
Concen: 4.947 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.134 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04




Instrument :
MSVOA_N
ClientSampleId :
BASEMENT-WALLS


Tgt Ion: 75 Resp: 69241
Ion Ratio Lower Upper
75 100
110 9.1 18.4 55.2#
77 0.0 24.4 36.6#

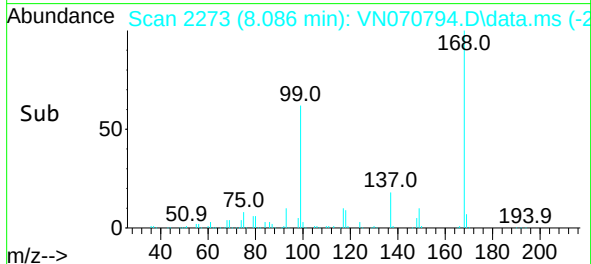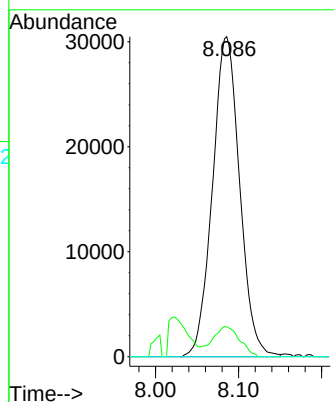

#37
Ethyl Acetate
Concen: 1.293 ug/l
RT: 7.337 min Scan# 1994
Delta R.T. -0.073 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04

Tgt Ion: 43 Resp: 24032
Ion Ratio Lower Upper
43 100
61 0.0 11.5 17.3#
70 0.0 7.9 11.9#


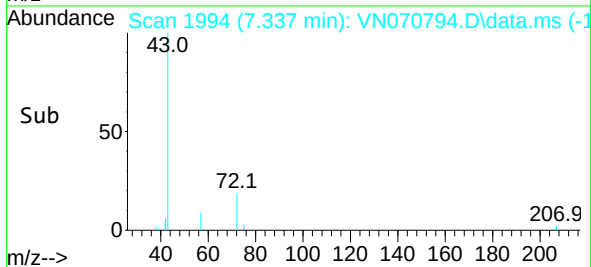
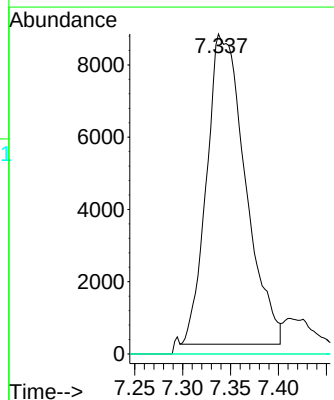
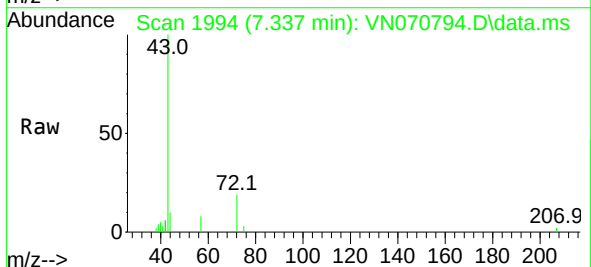




#38
Carbon Tetrachloride
Concen: 6.955 ug/l
RT: 8.086 min Scan# 211
Delta R.T. -0.120 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04




Instrument :
MSVOA_N
ClientSampleId :
BASEMENT-WALLS


Tgt Ion:117 Resp: 86593
Ion Ratio Lower Upper
117 100
119 5.0 76.1 114.1#
121 0.0 24.2 36.2#

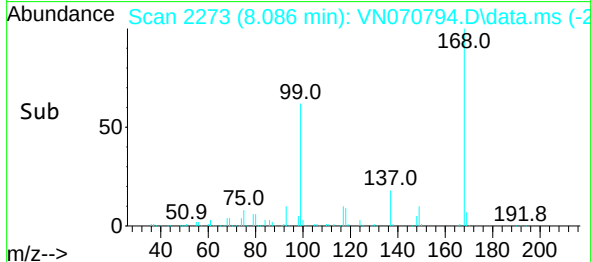

#43
Isopropyl Acetate
Concen: 3.021 ug/l
RT: 8.563 min Scan# 2451
Delta R.T. 0.003 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04

Tgt Ion: 43 Resp: 85748
Ion Ratio Lower Upper
43 100
61 16.6 20.4 30.6#
87 10.5 11.2 16.8#

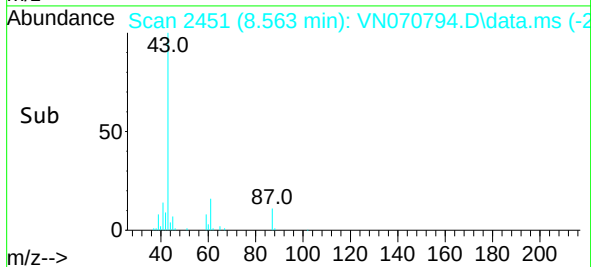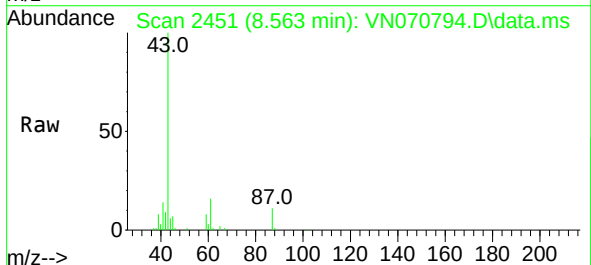



#45

1,2-Dichloropropane

Concen: 0.430 ug/l

RT: 9.622 min Scan# 21

Delta R.T. 0.134 min

Lab File: VN070794.D

Acq: 26 Jan 2022 17:04

Instrument :

MSVOA_N

ClientSampleId :





BASEMENT-WALLS

Tgt Ion: 63 Resp: 5070

Ion Ratio Lower Upper

63 100

65 0.0 24.7 37.1#

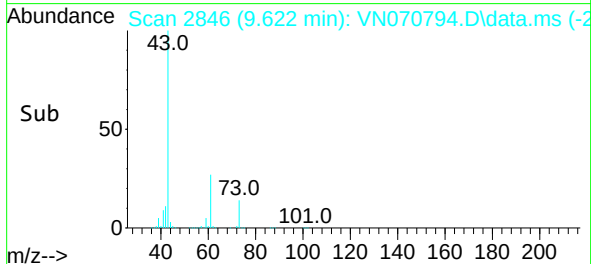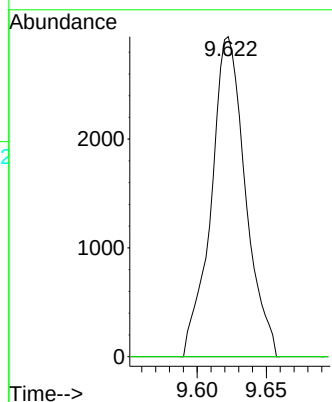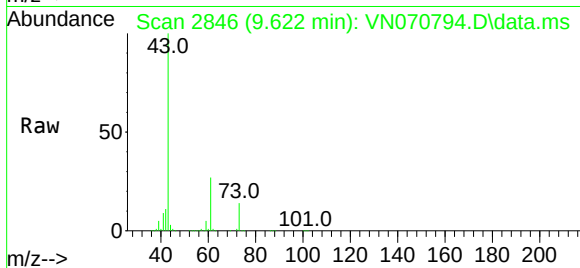

#48

Methyl methacrylate

Concen: 1.559 ug/l

RT: 9.539 min Scan# 2815

Delta R.T. -0.019 min

Lab File: VN070794.D

Acq: 26 Jan 2022 17:04




Tgt Ion: 41 Resp: 21083


Ion Ratio Lower Upper

41 100

69 0.0 72.4 108.6#

39 0.0 58.4 87.6#

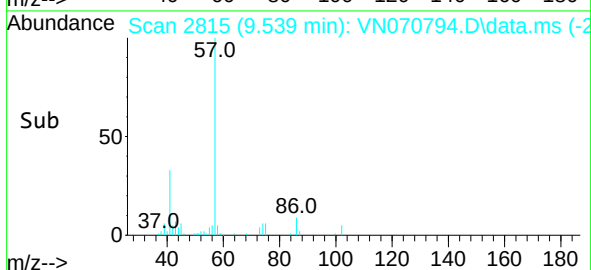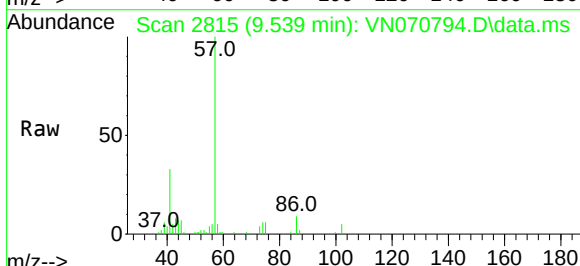



#49

1,4-Dioxane

Concen: 2.546 ug/l

RT: 9.617 min Scan# 21

Delta R.T. 0.048 min

Lab File: VN070794.D

Acq: 26 Jan 2022 17:04

Instrument :

MSVOA_N

ClientSampleId :

BASEMENT-WALLS





Tgt Ion: 88 Resp: 517

Ion Ratio Lower Upper

88 100

43 813261.3 23.4 35.2#

58 3452.8 50.6 75.8#

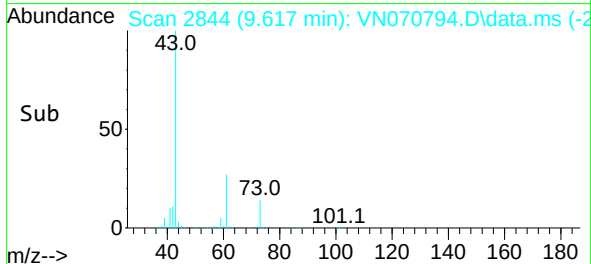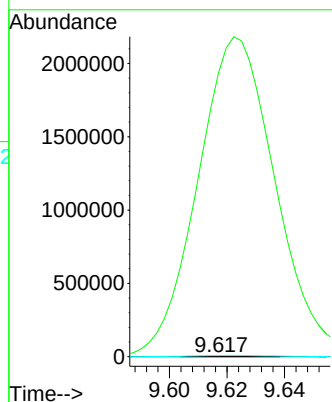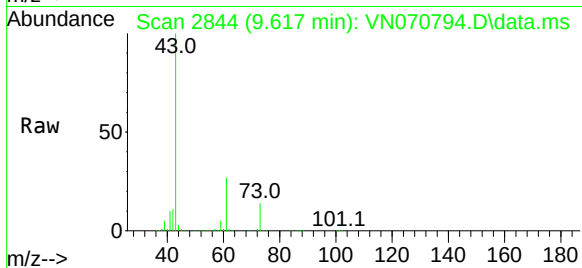

#50

Toluene-d8

Concen: 48.301 ug/l

RT: 10.440 min Scan# 3151

Delta R.T. 0.002 min

Lab File: VN070794.D




Acq: 26 Jan 2022 17:04


Tgt Ion: 98 Resp: 1691714

Ion Ratio Lower Upper

98 100

100 64.0 50.4 75.6




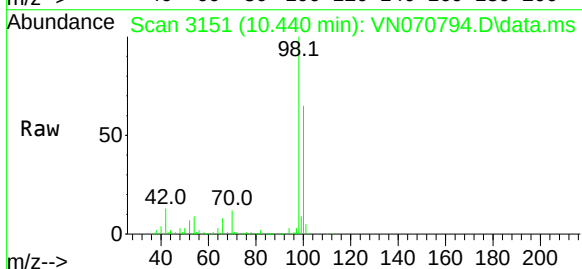




#51
4-Methyl-2-Pentanone
Concen: 0.577 ug/l
RT: 10.328 min Scan# 3109
Delta R.T. -0.000 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04




Instrument :
MSVOA_N
ClientSampleId :
BASEMENT-WALLS


Tgt Ion: 43 Resp: 10444
Ion Ratio Lower Upper
43 100
58 54.4 30.4 45.6#

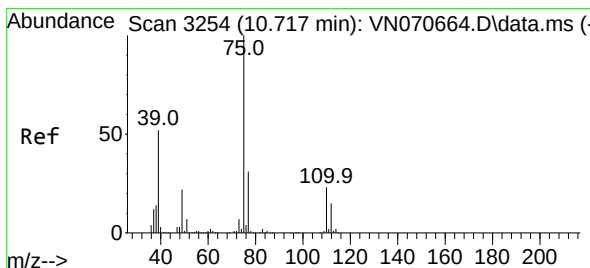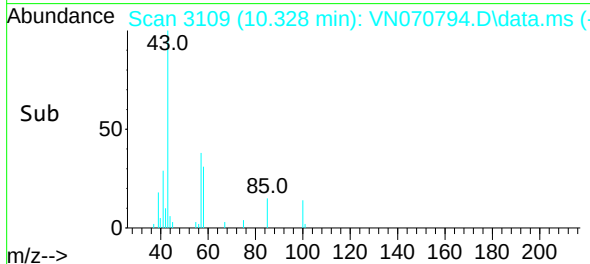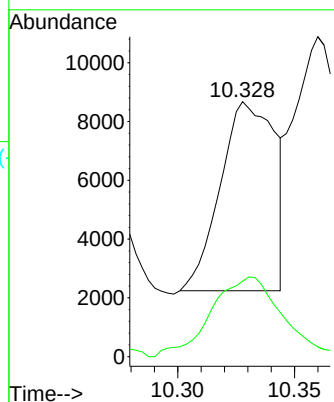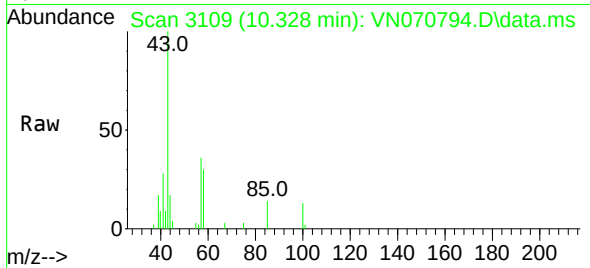

#53
t-1,3-Dichloropropene
Concen: 2.405 ug/l
RT: 10.639 min Scan# 3225
Delta R.T. -0.078 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04

Tgt Ion: 75 Resp: 27
Ion Ratio Lower Upper
75 100
77 374.5 25.6 38.4#


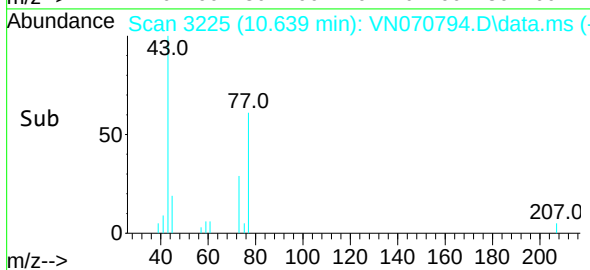
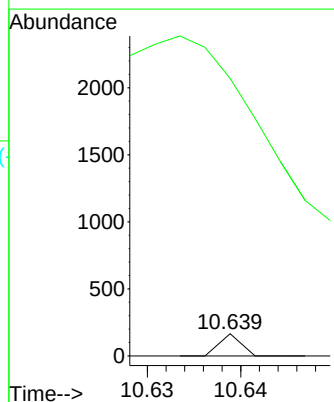
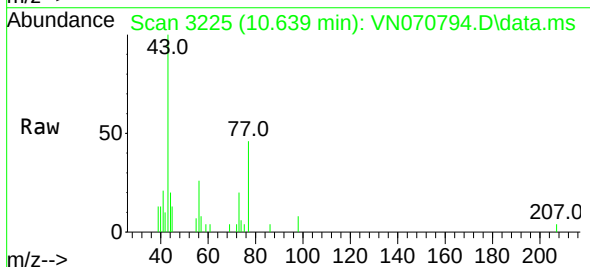


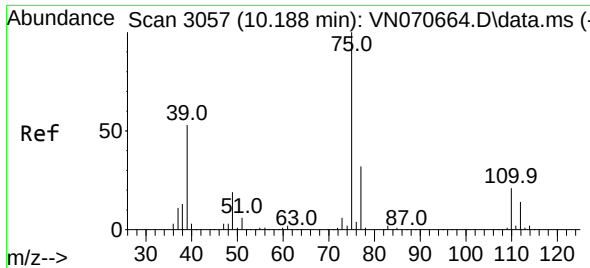

#54
 cis-1,3-Dichloropropene
 Concen: 6.494 ug/l
 RT: 10.242 min Scan# 3057
 Delta R.T. 0.054 min
 Lab File: VN070794.D
 Acq: 26 Jan 2022 17:04




Instrument :
 MSVOA_N
 ClientSampleId :
 BASEMENT-WALLS


Tgt Ion: 75 Resp: 109218
 Ion Ratio Lower Upper
 75 100
 77 0.6 26.4 39.6#
 39 36.8 42.5 63.7#

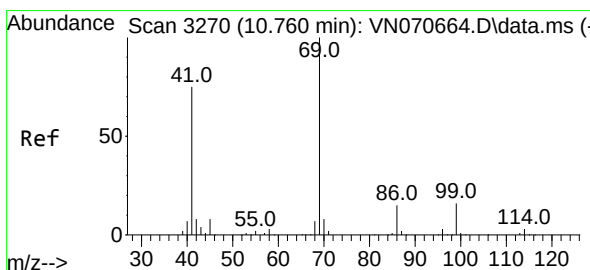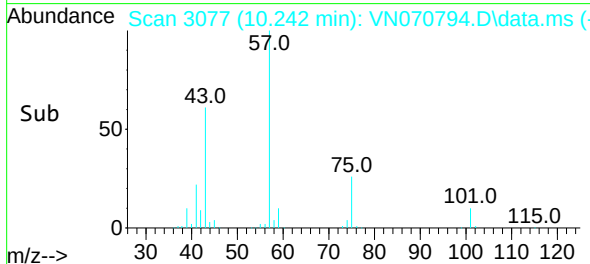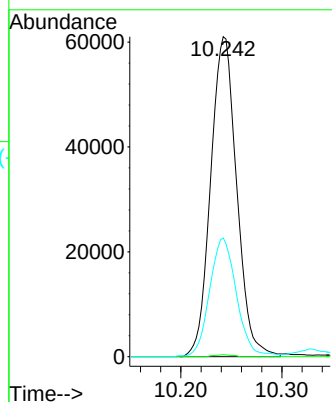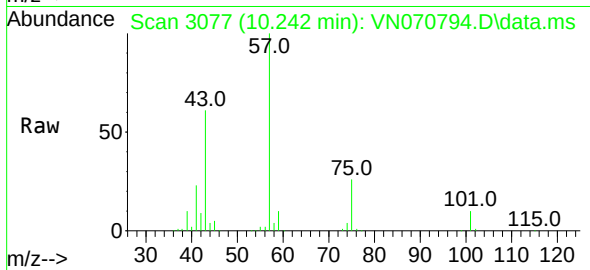

#56
 Ethyl methacrylate
 Concen: 2.352 ug/l
 RT: 10.872 min Scan# 3312
 Delta R.T. 0.112 min
 Lab File: VN070794.D
 Acq: 26 Jan 2022 17:04

Tgt Ion: 69 Resp: 1028
 Ion Ratio Lower Upper
 69 100
 41 3575.5 51.4 77.0#
 39 1556.0 34.6 52.0#

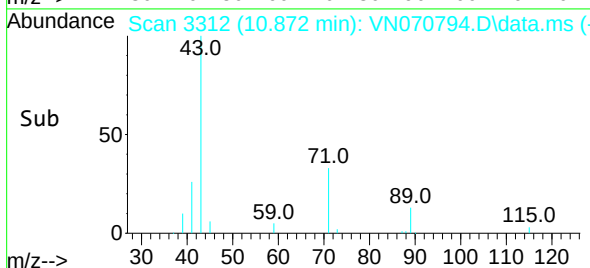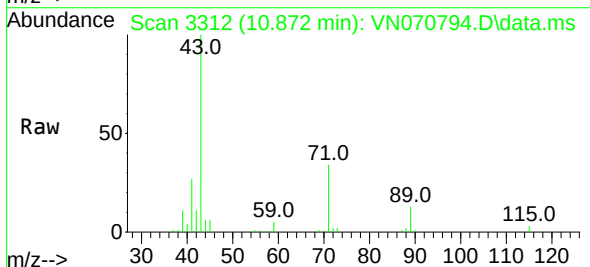



#57

1,3-Dichloropropane

Concen: 3.428 ug/l

RT: 11.089 min Scan# 31

Delta R.T. 0.045 min

Lab File: VN070794.D

Acq: 26 Jan 2022 17:04

Instrument :

MSVOA_N

ClientSampleId :





BASEMENT-WALLS

Tgt Ion: 76 Resp: 61838

Ion Ratio Lower Upper

76 100

78 0.4 25.7 38.5#

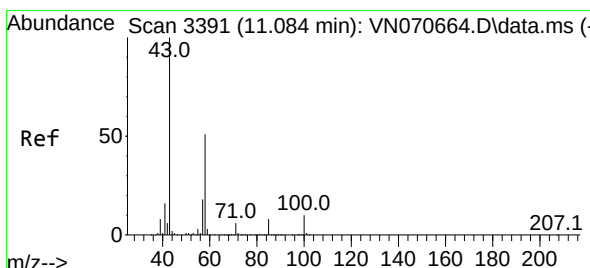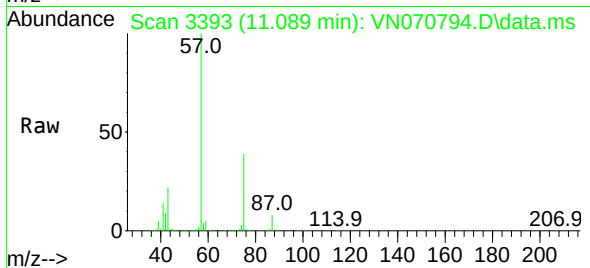

#59

2-Hexanone

Concen: 77.944 ug/l

RT: 11.089 min Scan# 3393

Delta R.T. 0.005 min

Lab File: VN070794.D




Acq: 26 Jan 2022 17:04


Tgt Ion: 43 Resp: 1025452

Ion Ratio Lower Upper

43 100

58 17.2 26.9 80.7#


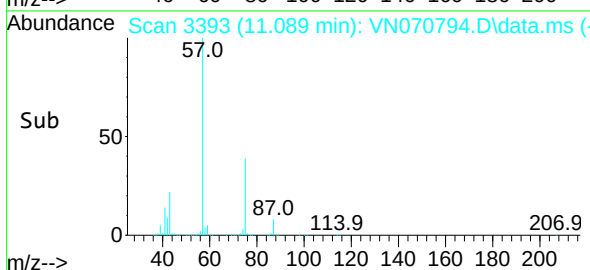






#62
4-Bromofluorobenzene
Concen: 47.864 ug/l
RT: 12.728 min Scan# 4004
Delta R.T. 0.000 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04




Instrument :
MSVOA_N
ClientSampleId :
BASEMENT-WALLS


Tgt Ion: 95 Resp: 597372
Ion Ratio Lower Upper
95 100
174 75.2 0.0 187.2
176 72.2 0.0 181.4

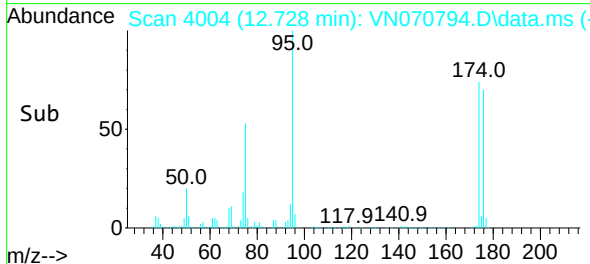

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3637
Delta R.T. 0.003 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04

Tgt Ion: 117 Resp: 1215313
Ion Ratio Lower Upper
117 100
82 60.4 42.4 63.6
119 32.2 25.4 38.2


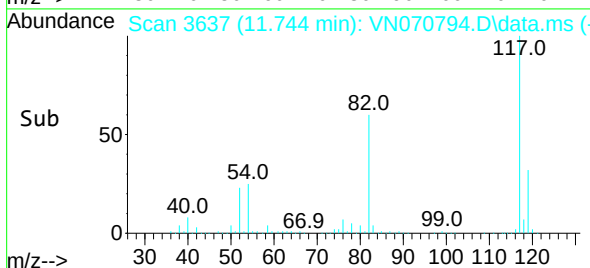
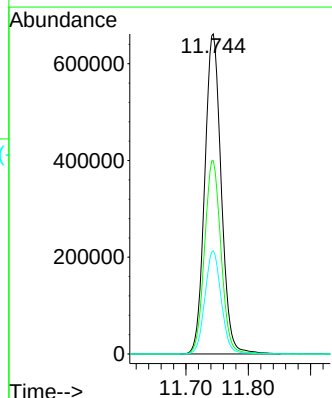
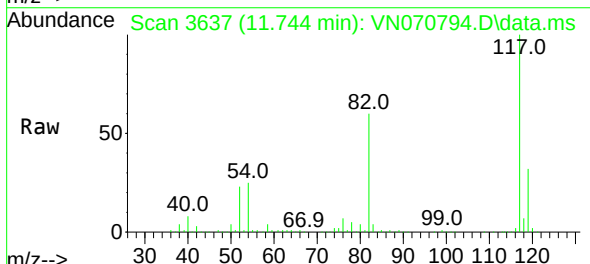


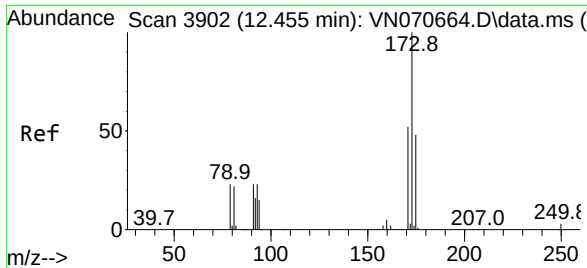

#71
Bromoform
Concen: 0.528 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.278 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04




Instrument :
MSVOA_N
ClientSampleId :
BASEMENT-WALLS


Tgt Ion:173 Resp: 3618
Ion Ratio Lower Upper
173 100
175 817.5 24.2 72.6#
254 0.0 0.0 0.0

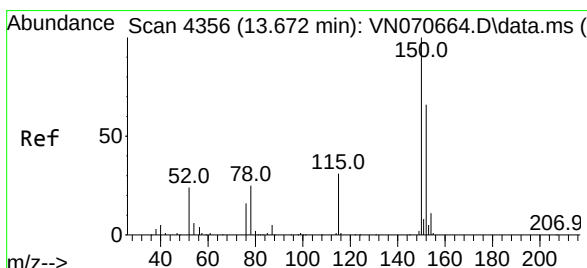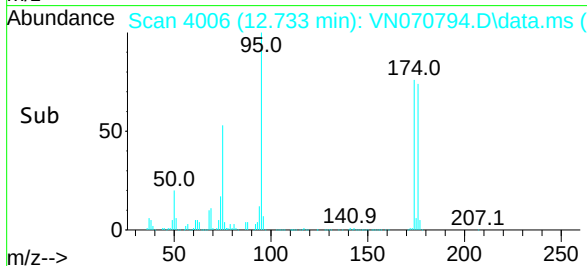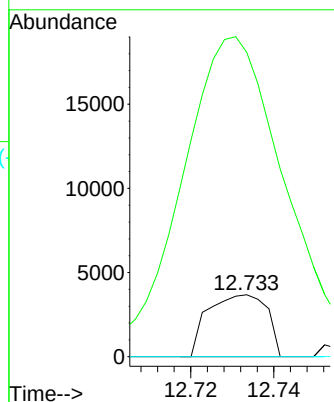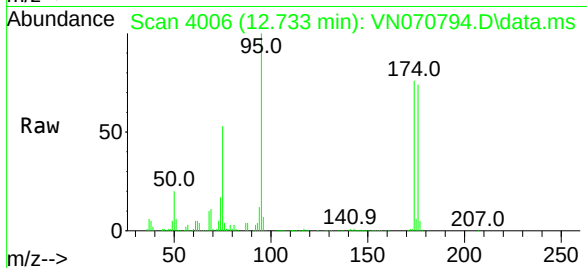

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 4357
Delta R.T. 0.003 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04


Tgt Ion:152 Resp: 479123
Ion Ratio Lower Upper
152 100
115 62.2 27.5 82.5
150 157.4 0.0 344.4

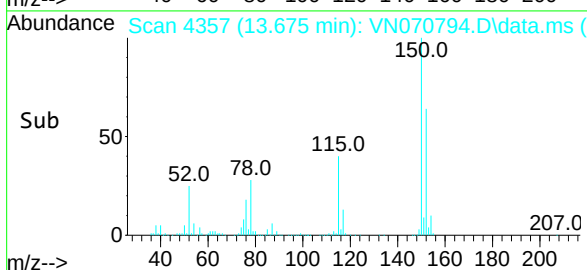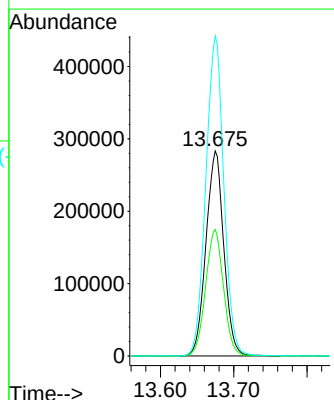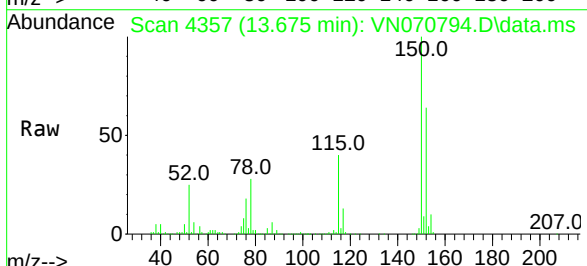






#74
N-amy1 acetate
Concen: 0.246 ug/l
RT: 12.358 min Scan# 31
Delta R.T. -0.027 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04

Instrument :
MSVOA_N
ClientSampleId :
BASEMENT-WALLS







Tgt Ion: 43	Resp: 4552
Ion Ratio	Lower Upper
43 100	
70 0.0	33.4 50.0#
55 2.1	19.3 28.9#
61 0.0	18.5 27.7#

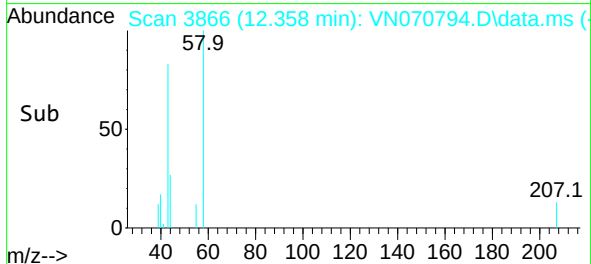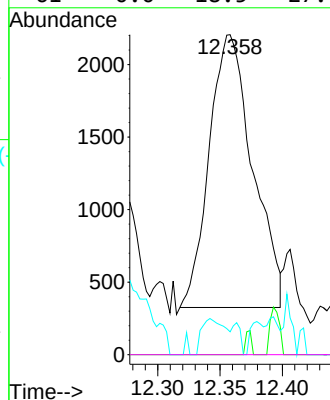

#76
1,2,3-Trichloropropane
Concen: 24.968 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.147 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04

Tgt Ion: 75	Resp: 317280
Ion Ratio	Lower Upper
75 100	
77 1.2	82.6 247.8#


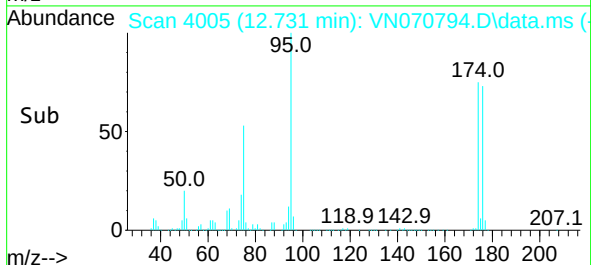
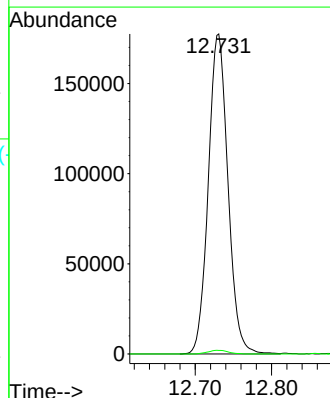
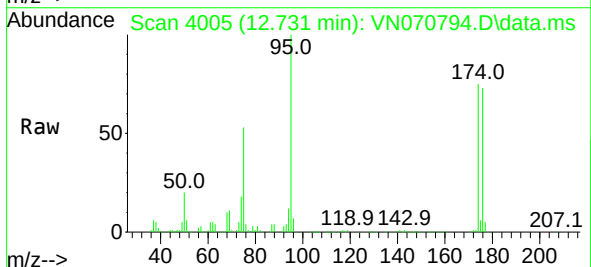




#81
trans-1,4-Dichloro-2-butene
Concen: 74.383 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.107 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04




Instrument :
MSVOA_N
ClientSampleId :
BASEMENT-WALLS


Tgt Ion: 75 Resp: 317280
Ion Ratio Lower Upper
75 100
53 0.1 90.5 135.7#
89 0.0 38.2 57.4#

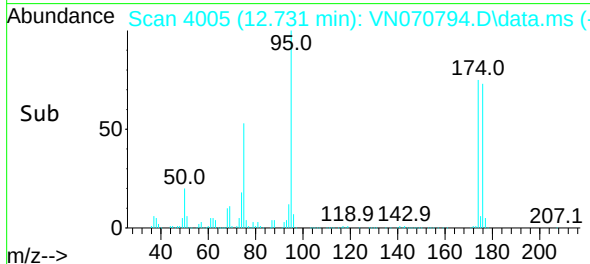

#93
1,2,4-Trichlorobenzene
Concen: 3.469 ug/l
RT: 15.257 min Scan# 4947
Delta R.T. -0.006 min
Lab File: VN070794.D
Acq: 26 Jan 2022 17:04

Tgt Ion: 180 Resp: 413
Ion Ratio Lower Upper
180 100
182 44.6 48.3 144.9#
145 0.0 14.5 43.5#

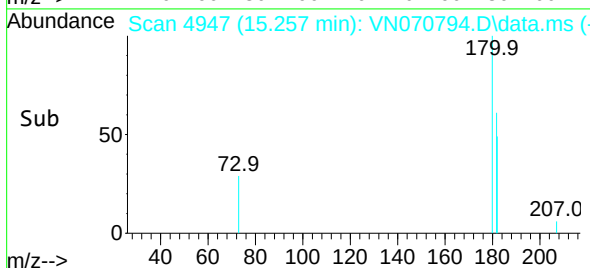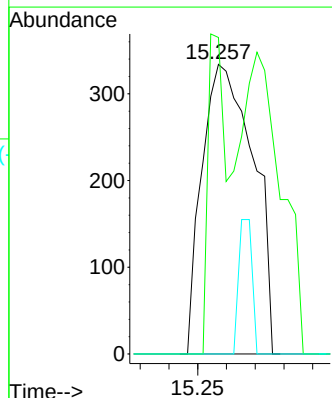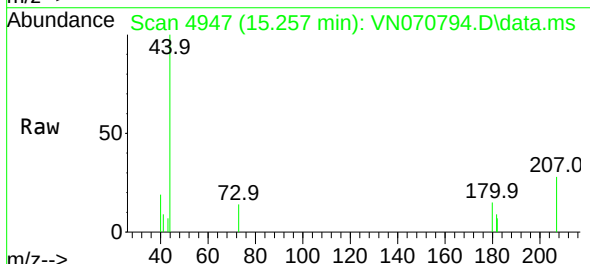



#95

Naphthalene

Concen: 5.035 ug/l

RT: 15.507 min Scan# 5039

Delta R.T. 0.003 min

Lab File: VN070794.D

Acq: 26 Jan 2022 17:04

Instrument :

MSVOA_N

ClientSampleId :

BASEMENT-WALLS





Tgt Ion:128 Resp: 2389

Ion Ratio Lower Upper

128 100

127 5.2 10.5 15.7#

129 0.0 8.7 13.1#

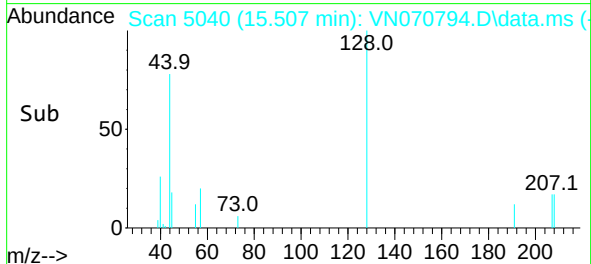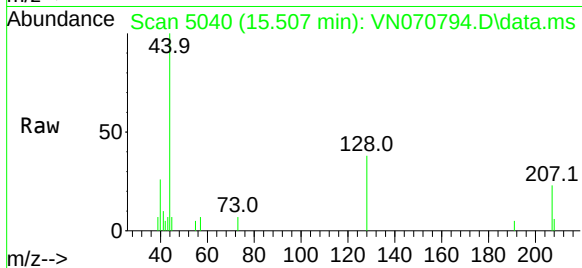

#96

1,2,3-Trichlorobenzene

Concen: 3.279 ug/l

RT: 15.700 min Scan# 5112

Delta R.T. 0.003 min

Lab File: VN070794.D

Acq: 26 Jan 2022 17:04

Tgt Ion:180 Resp: 568

Ion Ratio Lower Upper

180 100

182 49.3 47.4 142.2

145 0.0 15.0 45.1#

