

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012622\
 Data File : VN070795.D
 Acq On : 26 Jan 2022 17:30
 Operator : JC/MD
 Sample : N1267-20
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 2ND-3RD-FLOOR-WALLS-1

Quant Time: Jan 27 03:33:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 18 13:32:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.086	168	820845	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.965	114	1304855	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	1167749	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	430599	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	571743	48.601	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	97.200%
35) Dibromofluoromethane	8.021	113	389422	48.112	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	96.220%
50) Toluene-d8	10.440	98	1646611	48.290	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	96.580%
62) 4-Bromofluorobenzene	12.731	95	529841	43.606	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	87.220%
Target Compounds						
					Qvalue	
16) Acetone	4.291	43	61569	7.541	ug/l	95
20) Methylene Chloride	5.098	84	26561	2.470	ug/l	91
43) Isopropyl Acetate	8.560	43	100005	3.619	ug/l #	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012622\
Data File : VN070795.D
Acq On : 26 Jan 2022 17:30
Operator : JC/MD
Sample : N1267-20
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
2ND-3RD-FLOOR-WALLS-1

Quant Time: Jan 27 03:33:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 18 13:32:07 2022
Response via : Initial Calibration




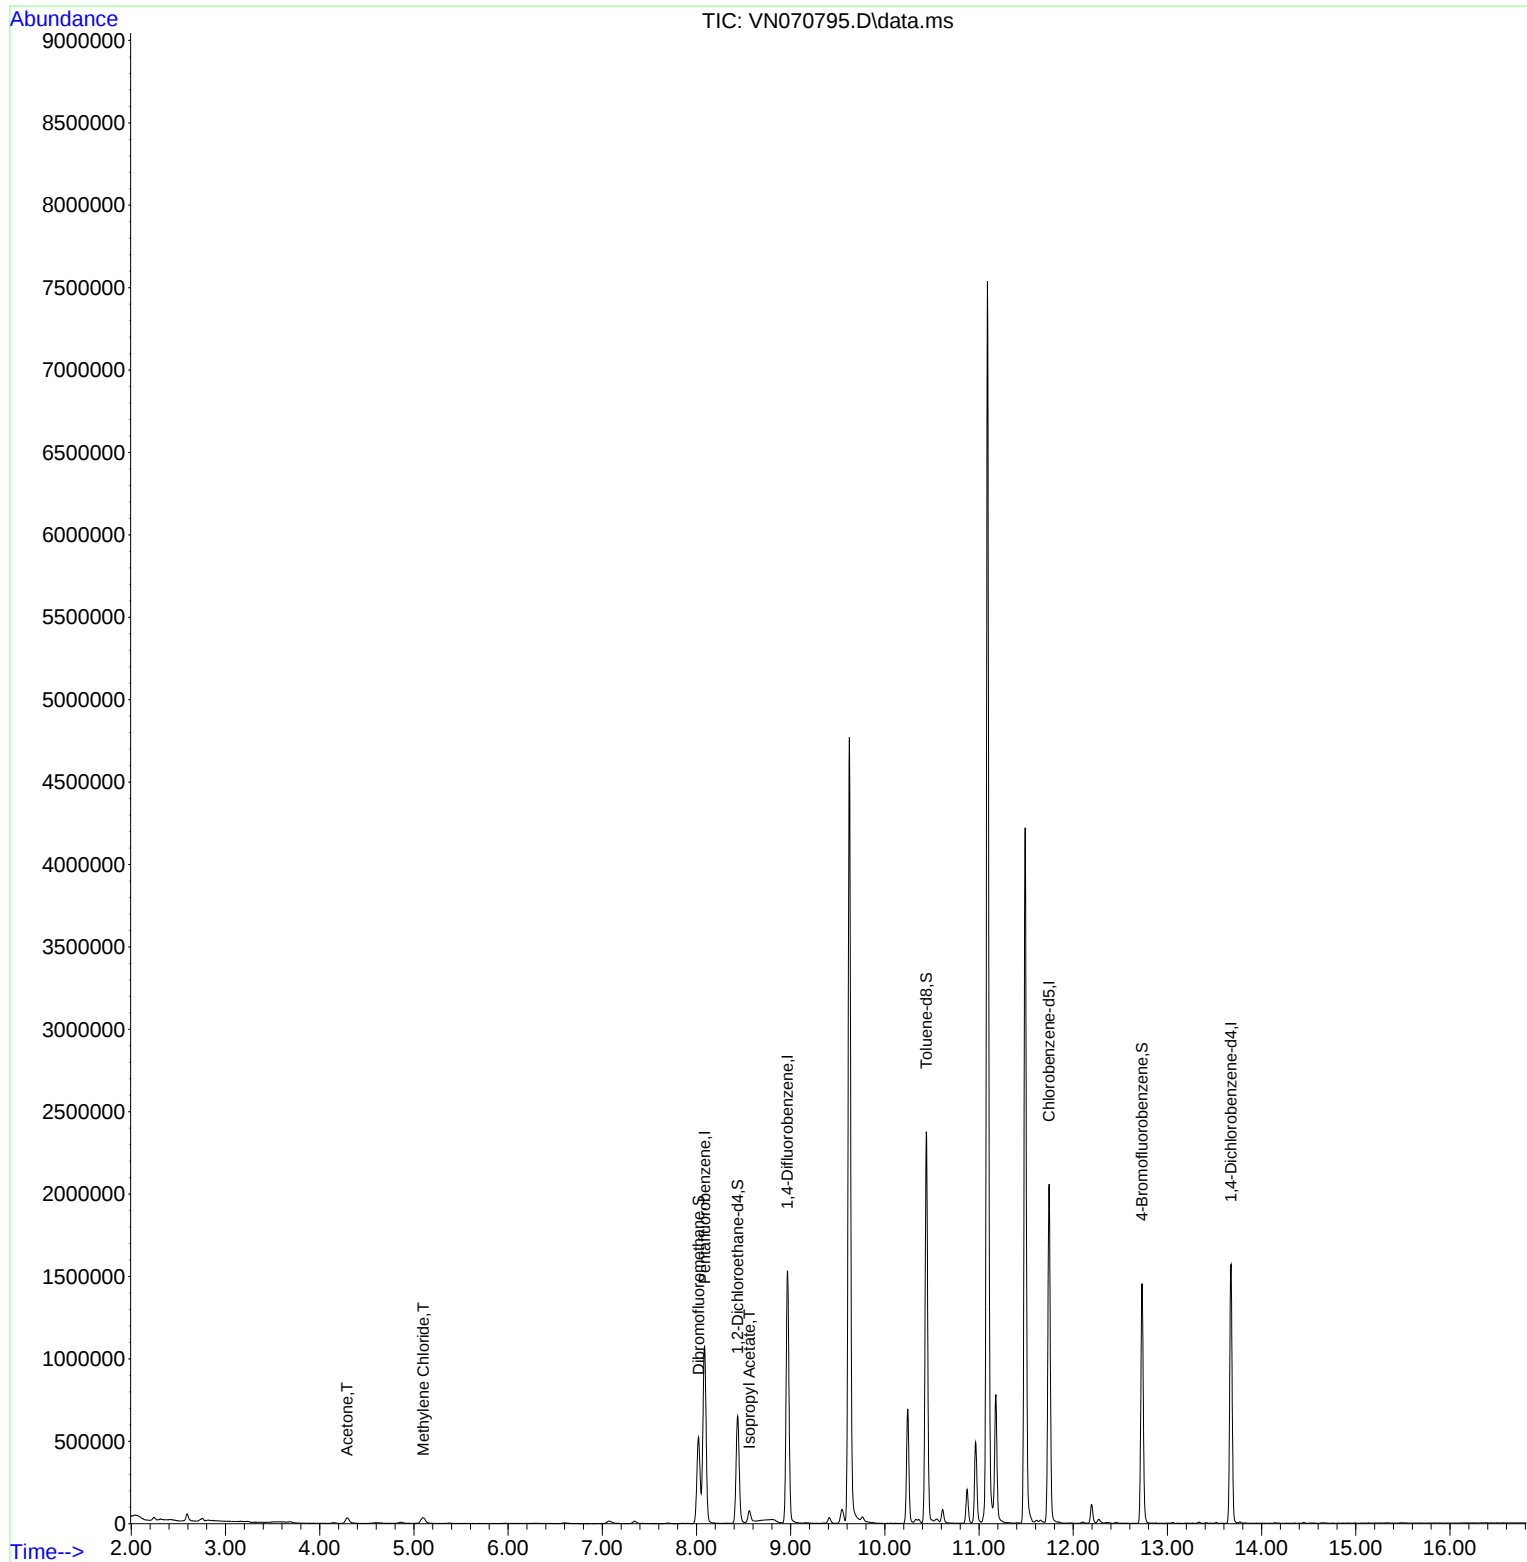


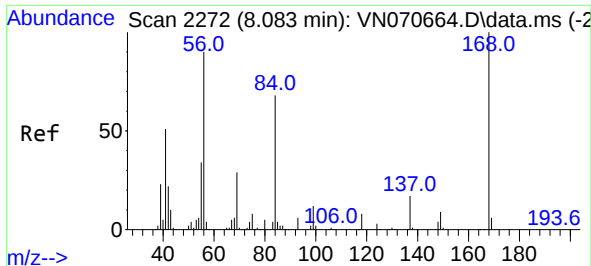

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 21
Delta R.T. 0.003 min
Lab File: VN070795.D
Acq: 26 Jan 2022 17:30




Instrument :
MSVOA_N
ClientSampleId :
2ND-3RD-FLOOR-WALLS-1


Tgt Ion:168 Resp: 820845
Ion Ratio Lower Upper
168 100
99 60.8 41.3 61.9

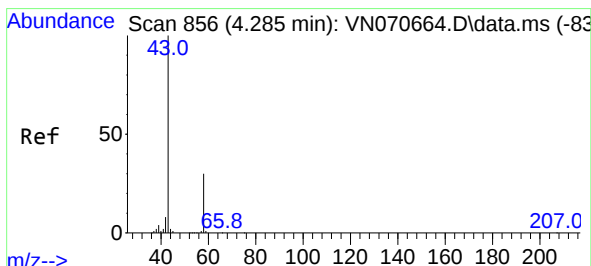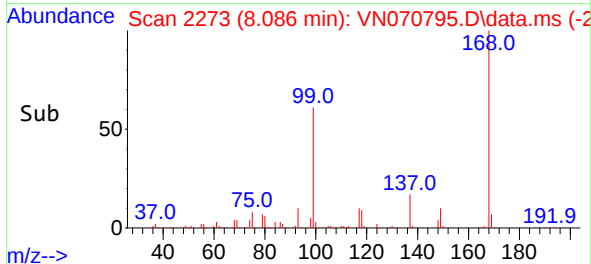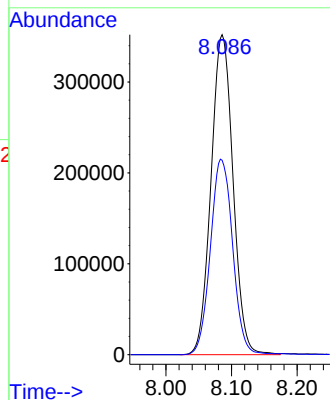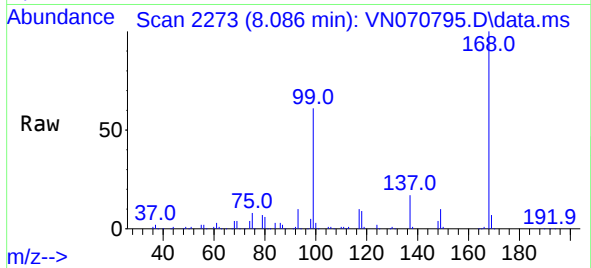

#16
Acetone
Concen: 7.541 ug/l
RT: 4.291 min Scan# 858
Delta R.T. 0.006 min
Lab File: VN070795.D
Acq: 26 Jan 2022 17:30


Tgt Ion: 43 Resp: 61569
Ion Ratio Lower Upper
43 100
58 31.5 23.1 34.7

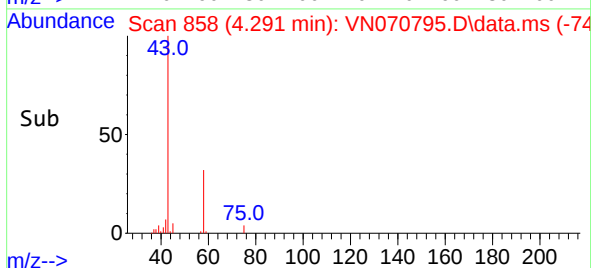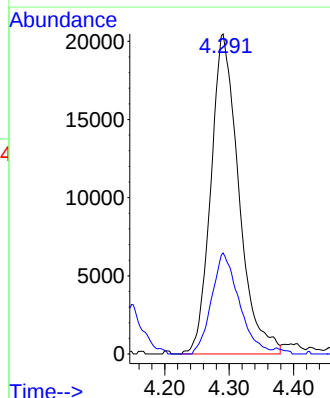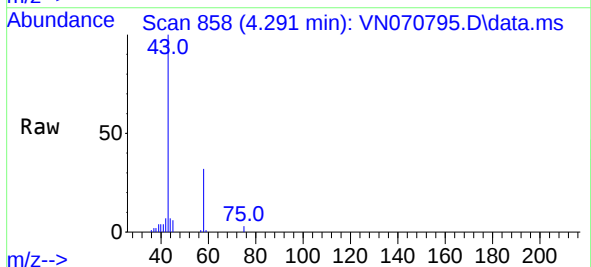

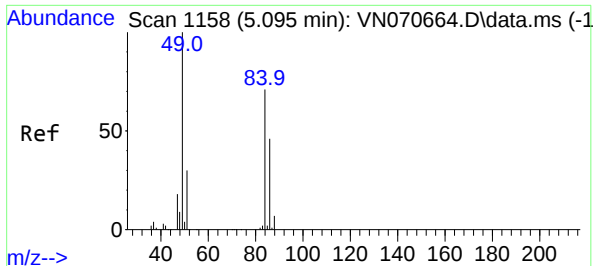




#20
Methylene Chloride
Concen: 2.470 ug/l
RT: 5.098 min Scan# 1158
Delta R.T. 0.003 min
Lab File: VN070795.D
Acq: 26 Jan 2022 17:30

Instrument :
MSVOA_N
ClientSampleId :
2ND-3RD-FLOOR-WALLS-1

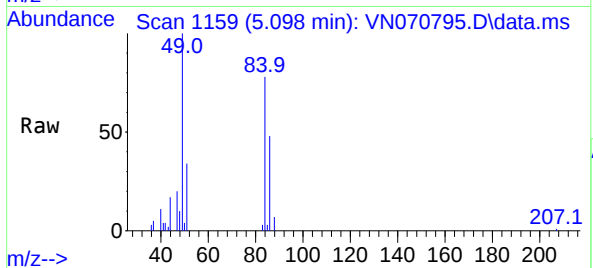

Tgt Ion: 84 Resp: 26561




Ion	Ratio	Lower	Upper
84	100		
49	128.1	93.5	140.3
51	43.0	29.4	44.2
86	60.9	53.0	79.4

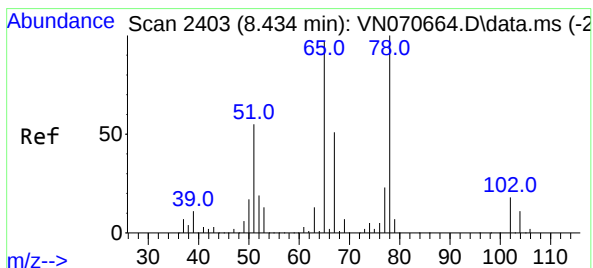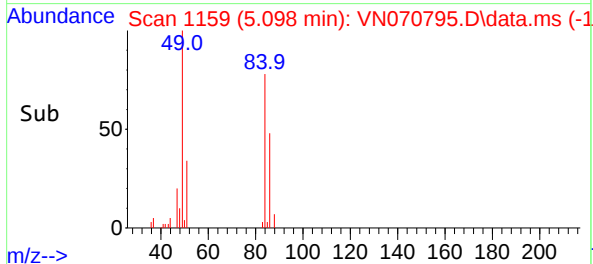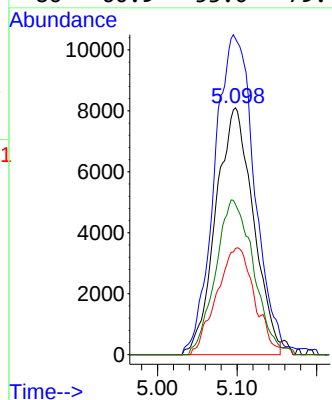


#33
1,2-Dichloroethane-d4
Concen: 48.601 ug/l
RT: 8.437 min Scan# 2404
Delta R.T. 0.003 min
Lab File: VN070795.D
Acq: 26 Jan 2022 17:30

Tgt Ion: 65 Resp: 571743

Ion	Ratio	Lower	Upper
65	100		
67	51.4	0.0	103.0


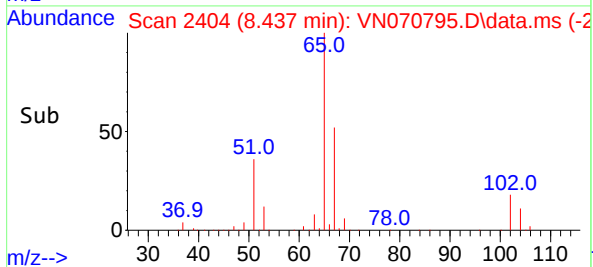
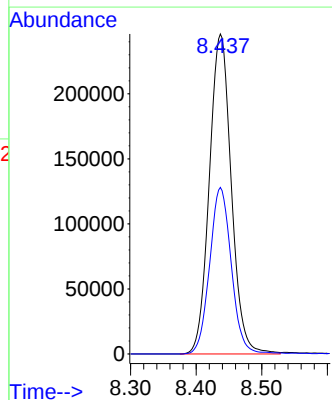
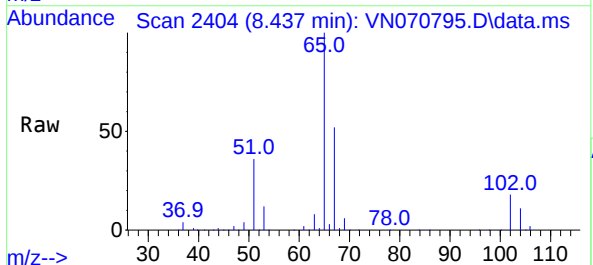


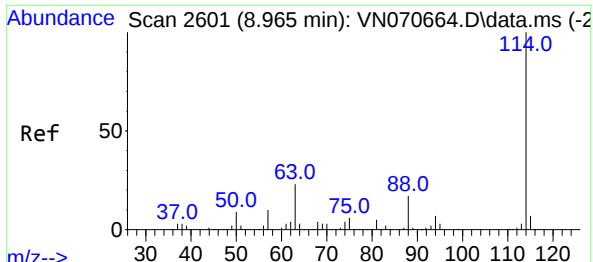

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.965 min Scan# 2601
Delta R.T. 0.000 min
Lab File: VN070795.D
Acq: 26 Jan 2022 17:30




Instrument : MSVOA_N
ClientSampleId : 2ND-3RD-FLOOR-WALLS-1


Tgt Ion:114 Resp: 1304855
Ion Ratio Lower Upper
114 100
63 23.5 0.0 37.8
88 16.9 0.0 27.4

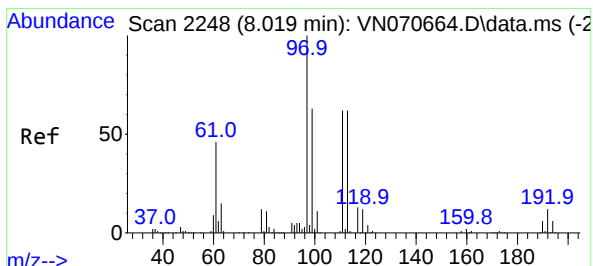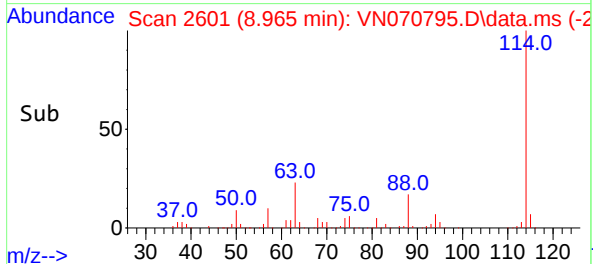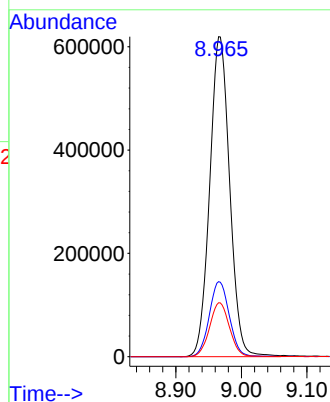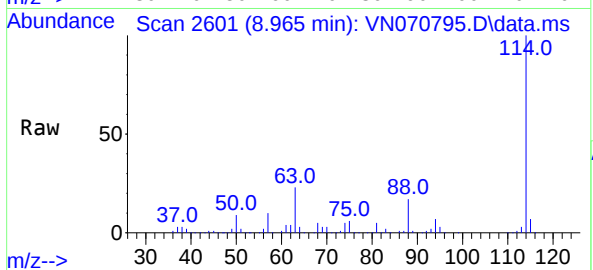

#35
Dibromofluoromethane
Concen: 48.112 ug/l
RT: 8.021 min Scan# 2249
Delta R.T. 0.002 min
Lab File: VN070795.D
Acq: 26 Jan 2022 17:30

Tgt Ion:113 Resp: 389422
Ion Ratio Lower Upper
113 100
111 102.2 82.2 123.2
192 19.4 16.9 25.3


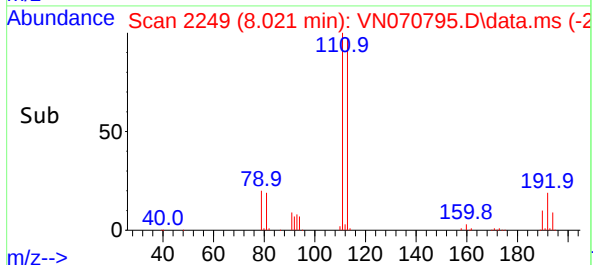
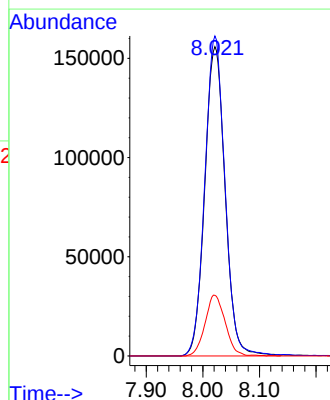
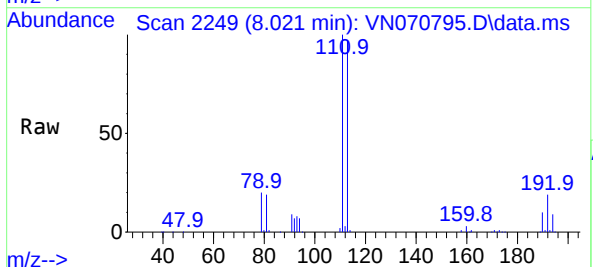


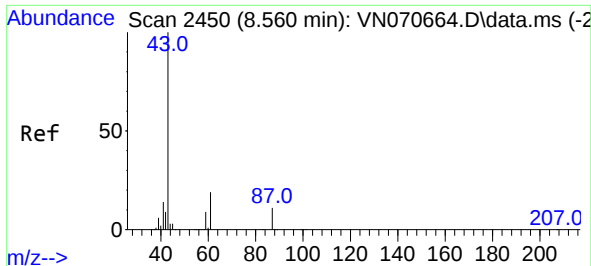

#43
Isopropyl Acetate
Concen: 3.619 ug/l
RT: 8.560 min Scan# 2450
Delta R.T. 0.000 min
Lab File: VN070795.D
Acq: 26 Jan 2022 17:30




Instrument : MSVOA_N
ClientSampleId : 2ND-3RD-FLOOR-WALLS-1


Tgt Ion: 43 Resp: 100005
Ion Ratio Lower Upper
43 100
61 15.6 20.4 30.6#
87 10.1 11.2 16.8#

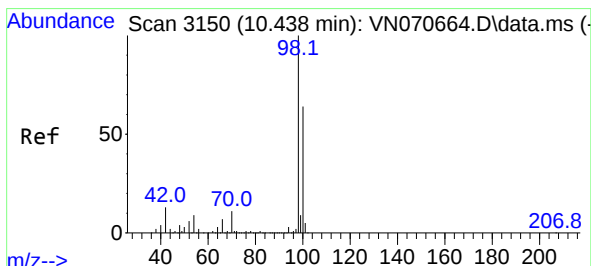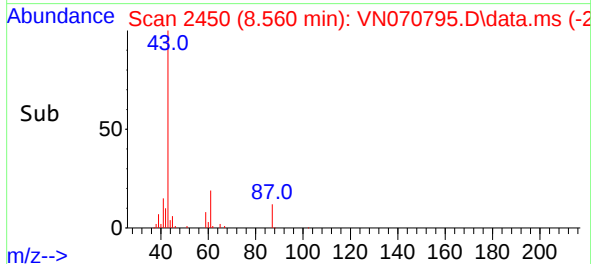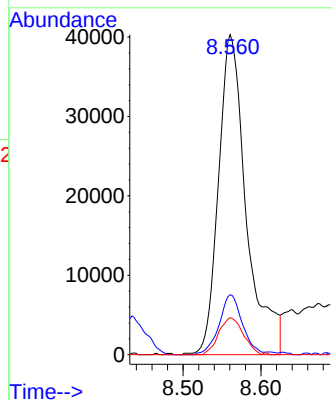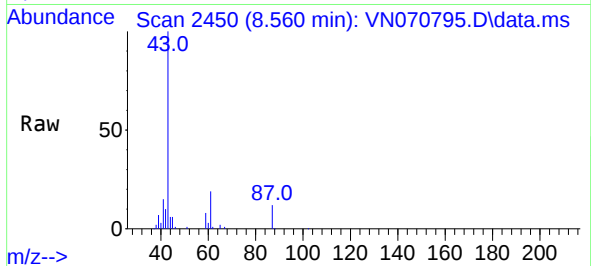

#50
Toluene-d8
Concen: 48.290 ug/l
RT: 10.440 min Scan# 3151
Delta R.T. 0.002 min
Lab File: VN070795.D
Acq: 26 Jan 2022 17:30

Tgt Ion: 98 Resp: 1646611
Ion Ratio Lower Upper
98 100
100 64.1 50.4 75.6


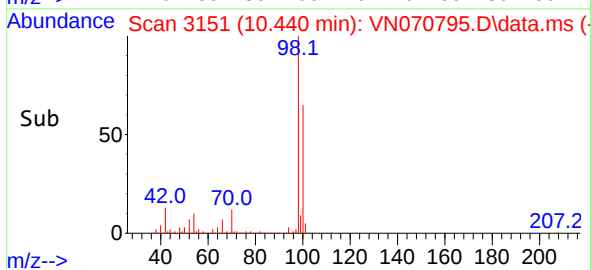
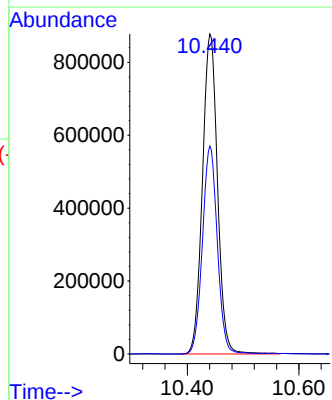
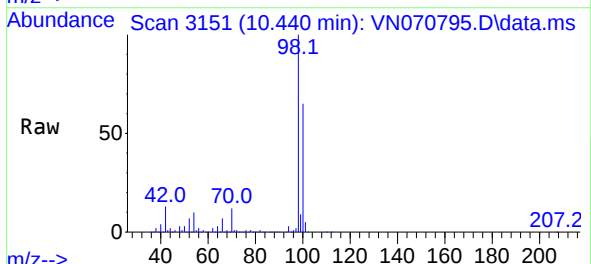


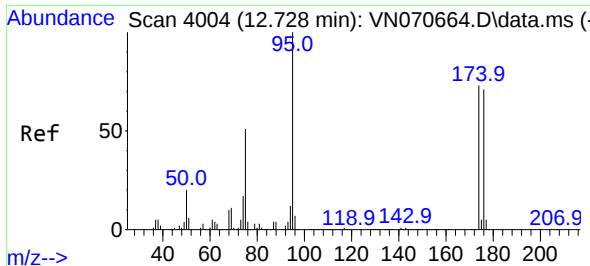

#62
4-Bromofluorobenzene
Concen: 43.606 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.003 min
Lab File: VN070795.D
Acq: 26 Jan 2022 17:30




Instrument :
MSVOA_N
ClientSampleId :
2ND-3RD-FLOOR-WALLS-1


Tgt Ion: 95 Resp: 529841
Ion Ratio Lower Upper
95 100
174 75.1 0.0 187.2
176 72.1 0.0 181.4

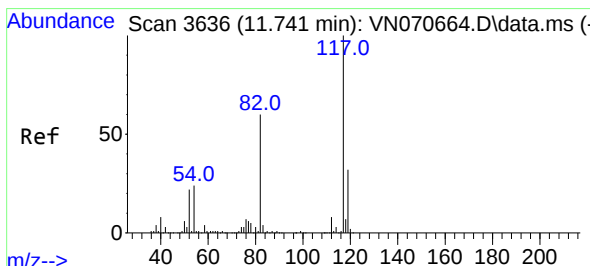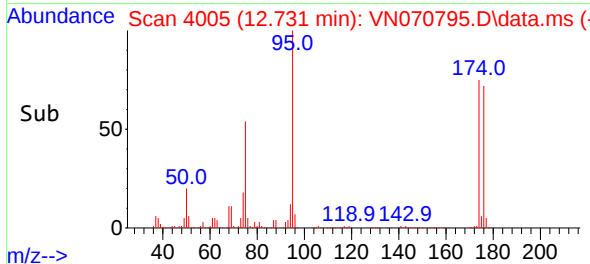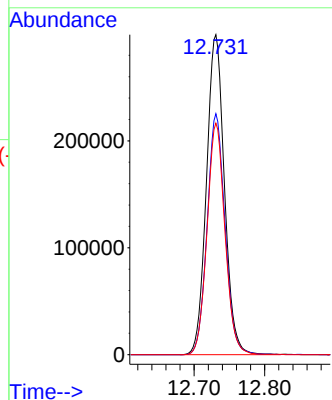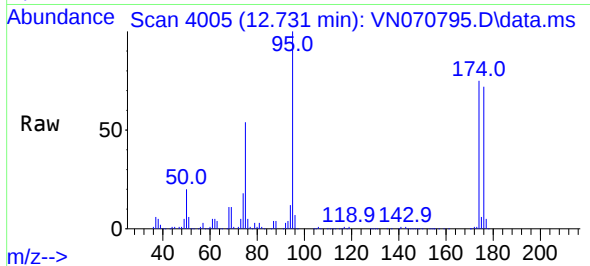

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3637
Delta R.T. 0.003 min
Lab File: VN070795.D
Acq: 26 Jan 2022 17:30


Tgt Ion: 117 Resp: 1167749
Ion Ratio Lower Upper
117 100
82 60.2 42.4 63.6
119 31.7 25.4 38.2

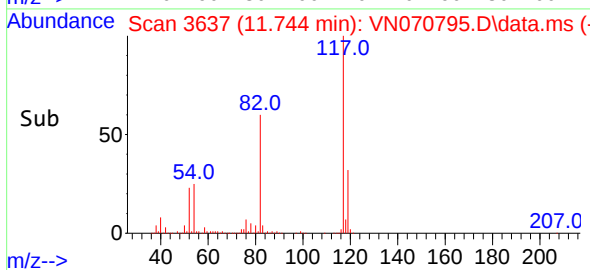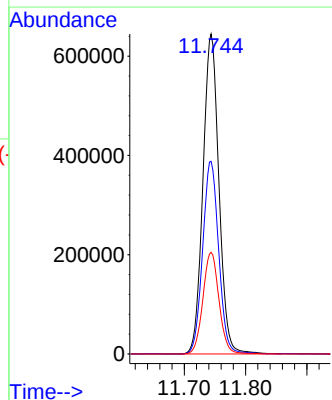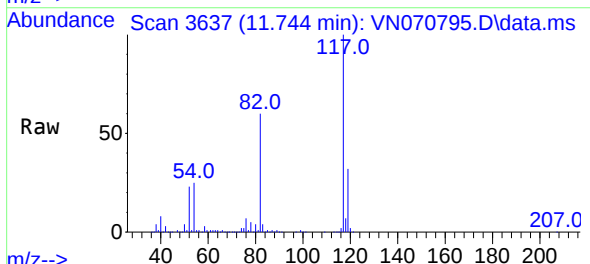

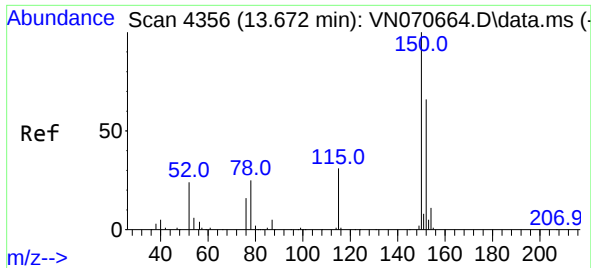

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.675 min Scan# 41
 Delta R.T. 0.003 min
 Lab File: VN070795.D
 Acq: 26 Jan 2022 17:30

Instrument :
 MSVOA_N
 ClientSampleId :
 2ND-3RD-FLOOR-WALLS-1

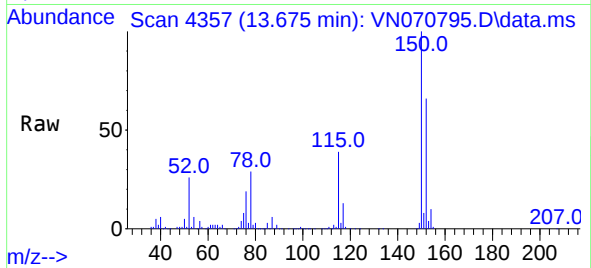

Tgt Ion:152 Resp: 430599
 Ion Ratio Lower Upper
 152 100
 115 62.2 27.5 82.5
 150 157.1 0.0 344.4

