

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012623\
 Data File : VN076415.D
 Acq On : 26 Jan 2023 13:13
 Operator : JC\MD
 Sample : PB150465TB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB150465TB

Quant Time: Jan 27 00:33:57 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 17 03:59:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	434993	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	724752	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	637506	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	237119	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	257649	52.899	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 105.800%	
35) Dibromofluoromethane	8.177	113	218161	48.121	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 96.240%	
50) Toluene-d8	10.571	98	845012	50.469	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 100.940%	
62) 4-Bromofluorobenzene	12.853	95	264632	48.415	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 96.840%	


Target Compounds						Qvalue
11) Tert butyl alcohol	5.530	59	1220	1.873	ug/l #	72
16) Acetone	4.447	43	39337	25.128	ug/l	100
18) Methyl Acetate	5.059	43	3243	0.613	ug/l	91
20) Methylene Chloride	5.295	84	31226	6.231	ug/l	94
25) 2-Butanone	7.506	43	4304	1.805	ug/l	95
31) Cyclohexane	8.230	56	9138	1.221	ug/l #	13
36) 1,1-Dichloropropene	8.235	75	34572	5.367	ug/l #	48
37) Ethyl Acetate	7.571	43	38405	7.464	ug/l	98
38) Carbon Tetrachloride	8.230	117	45030	6.268	ug/l #	17
42) 1,2-Dichloroethane	8.694	62	1675	0.254	ug/l #	73
43) Isopropyl Acetate	8.694	43	220439	26.224	ug/l #	83
45) 1,2-Dichloropropane	9.741	63	2837	0.615	ug/l #	42
48) Methyl methacrylate	9.665	41	5172	1.300	ug/l #	10
49) 1,4-Dioxane	9.688	88	55	0.655	ug/l #	1
51) 4-Methyl-2-Pentanone	10.453	43	17652	3.577	ug/l #	73
54) cis-1,3-Dichloropropene	10.359	75	77833	10.508	ug/l #	64
57) 1,3-Dichloropropane	11.206	76	10863	1.358	ug/l #	42
59) 2-Hexanone	11.171	43	163908	45.836	ug/l #	21
71) Bromoform	12.853	173	1821	0.503	ug/l #	1
74) N-amyl acetate	12.494	43	4235	0.803	ug/l #	63
76) 1,2,3-Trichloropropane	12.853	75	142593	32.682	ug/l #	1
77) Bromobenzene	12.982	156	743	Below Cal		63
81) trans-1,4-Dichloro-2-b...	12.853	75	142593	100.055	ug/l #	11
87) 1,3-Dichlorobenzene	13.741	146	2685	0.311	ug/l	97
88) 1,4-Dichlorobenzene	13.741	146	2685	0.427	ug/l	96
89) n-Butylbenzene	14.059	91	3899	0.315	ug/l	94
91) 1,2-Dichlorobenzene	14.106	146	2580	0.300	ug/l	94
93) 1,2,4-Trichlorobenzene	15.394	180	3175	2.048	ug/l	92
95) Naphthalene	15.641	128	13285	2.878	ug/l	96
96) 1,2,3-Trichlorobenzene	15.847	180	3315	1.970	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012623\
Data File : VN076415.D
Acq On : 26 Jan 2023 13:13
Operator : JC\MD
Sample : PB150465TB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB150465TB

Quant Time: Jan 27 00:33:57 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 17 03:59:22 2023
Response via : Initial Calibration

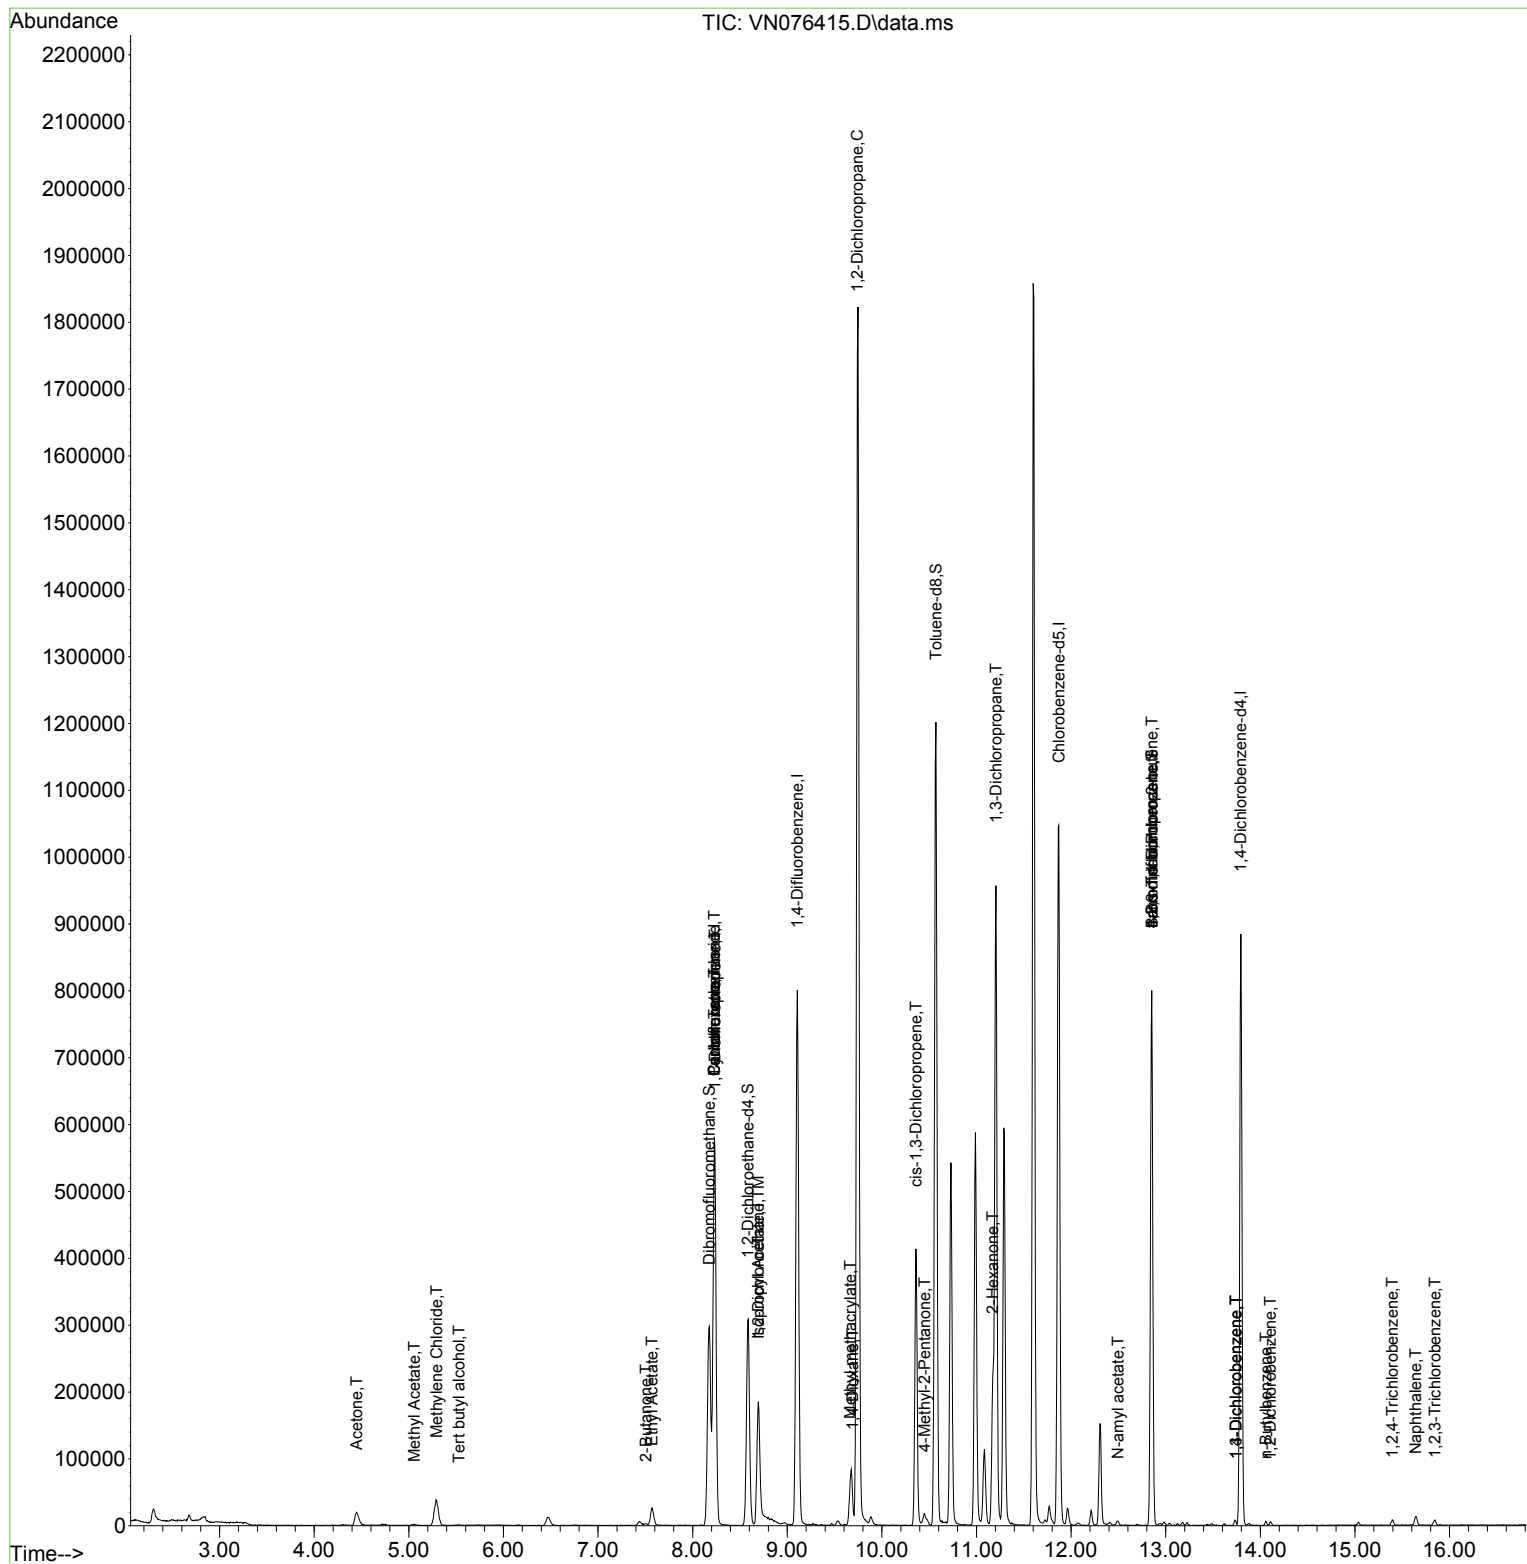



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.230 min Scan# 1050

Delta R.T. -0.000 min

Lab File: VN076415.D

Acq: 26 Jan 2023 13:13

Instrument :

MSVOA_N

ClientSampleId :





PB150465TB

Tgt Ion:168 Resp: 434993

Ion Ratio Lower Upper

168 100

99 58.1 41.6 62.4

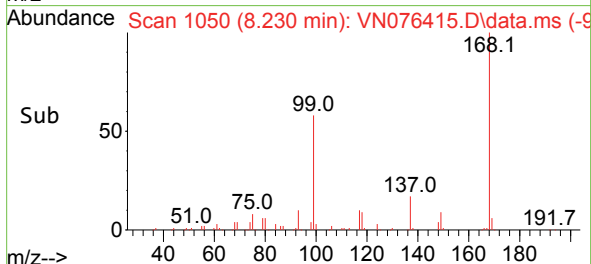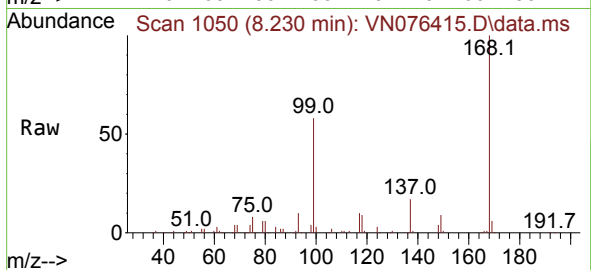

#11

Tert butyl alcohol

Concen: 1.873 ug/l

RT: 5.530 min Scan# 591

Delta R.T. -0.000 min

Lab File: VN076415.D




Acq: 26 Jan 2023 13:13


Tgt Ion: 59 Resp: 1220

Ion Ratio Lower Upper

59 100

57 0.0 8.5 12.7#


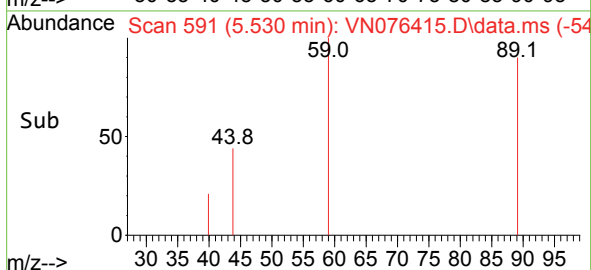






#16
Acetone
Concen: 25.128 ug/l
RT: 4.447 min Scan# 406
Delta R.T. 0.005 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13




Instrument :
MSVOA_N
ClientSampleId :
PB150465TB

Tgt Ion: 43 Resp: 39337
Ion Ratio Lower Upper
43 100
58 33.5 26.7 40.1

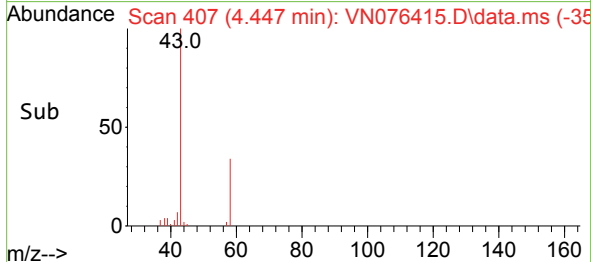

#18
Methyl Acetate
Concen: 0.613 ug/l
RT: 5.059 min Scan# 511
Delta R.T. 0.023 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13

Tgt Ion: 43 Resp: 3243
Ion Ratio Lower Upper
43 100
74 24.5 23.3 34.9




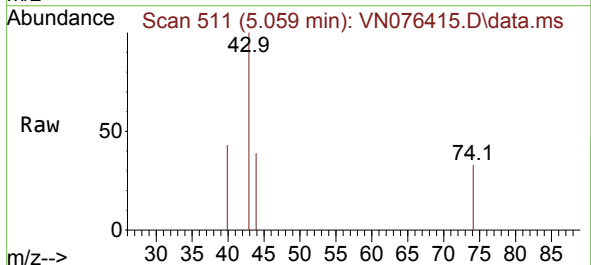




#20
Methylene Chloride
Concen: 6.231 ug/l
RT: 5.295 min Scan# 511
Delta R.T. 0.006 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13




Instrument :
MSVOA_N
ClientSampleId :
PB150465TB


Tgt	Ion: 84	Resp:	31226
Ion	Ratio	Lower	Upper
84	100		
49	102.7	84.5	126.7
51	29.5	26.0	39.0
86	55.7	52.0	78.0

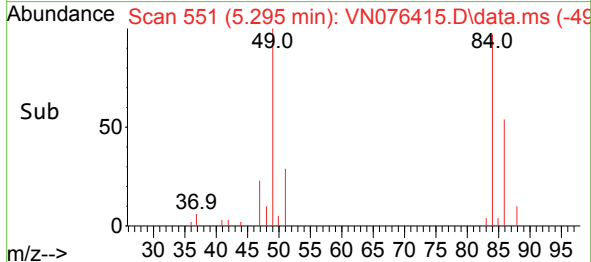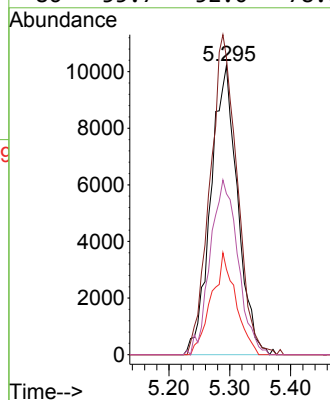

#25
2-Butanone
Concen: 1.805 ug/l
RT: 7.506 min Scan# 927
Delta R.T. 0.018 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13

Tgt Ion: 43	Resp: 4304
Ion Ratio	Lower Upper
43 100	
72 31.3	27.4 41.2


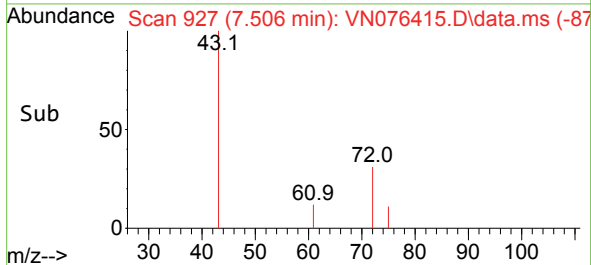
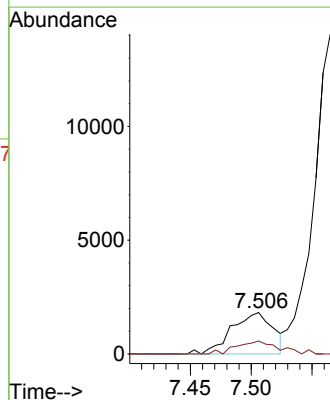





#31
Cyclohexane
Concen: 1.221 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.029 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13




Instrument :
MSVOA_N
ClientSampleId :
PB150465TB


Tgt Ion: 56 Resp: 9138
Ion Ratio Lower Upper
56 100
69 175.0 25.8 38.8#
84 130.3 79.0 118.4#

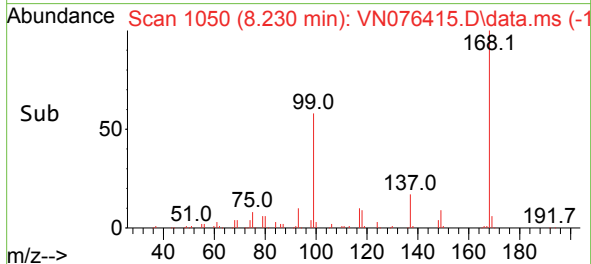

#33
1,2-Dichloroethane-d4
Concen: 52.899 ug/l
RT: 8.583 min Scan# 1110
Delta R.T. 0.001 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13

Tgt Ion: 65 Resp: 257649
Ion Ratio Lower Upper
65 100
67 50.2 0.0 104.6

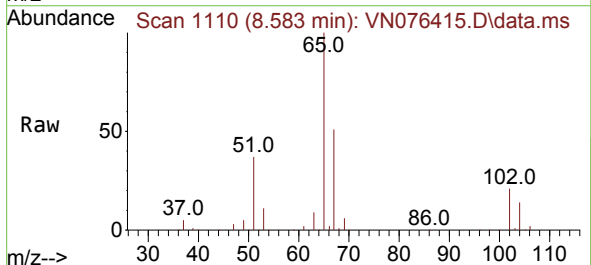



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. 0.000 min

Lab File: VN076415.D

Acq: 26 Jan 2023 13:13

Instrument :

MSVOA_N

ClientSampleId :

PB150465TB





Tgt Ion:114 Resp: 724752

Ion Ratio Lower Upper

114 100

63 18.7 0.0 35.8

88 15.1 0.0 28.0



#35

Dibromofluoromethane

Concen: 48.121 ug/l

RT: 8.177 min Scan# 1041

Delta R.T. 0.006 min

Lab File: VN076415.D

Acq: 26 Jan 2023 13:13




Tgt Ion:113 Resp: 218161


Ion Ratio Lower Upper

113 100

111 103.2 82.7 124.1

192 18.9 15.6 23.4


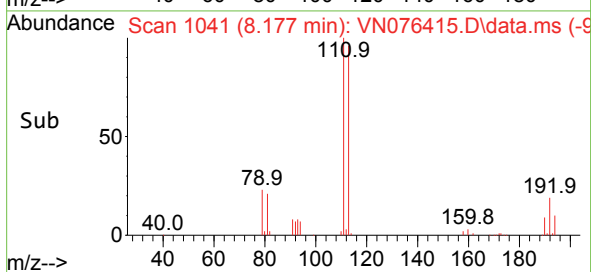






#36
1,1-Dichloropropene
Concen: 5.367 ug/l
RT: 8.235 min Scan# 1075
Delta R.T. -0.142 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13




Instrument :
MSVOA_N
ClientSampleId :
PB150465TB


Tgt Ion: 75 Resp: 34572
Ion Ratio Lower Upper
75 100
110 8.9 18.8 56.3#
77 0.0 25.0 37.4#

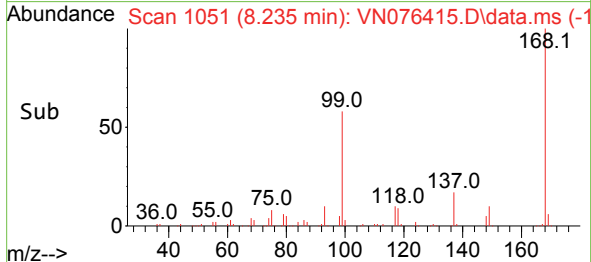

#37
Ethyl Acetate
Concen: 7.464 ug/l
RT: 7.571 min Scan# 938
Delta R.T. 0.006 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13

Tgt Ion: 43 Resp: 38405
Ion Ratio Lower Upper
43 100
61 15.6 11.1 16.7
70 12.3 10.0 15.0




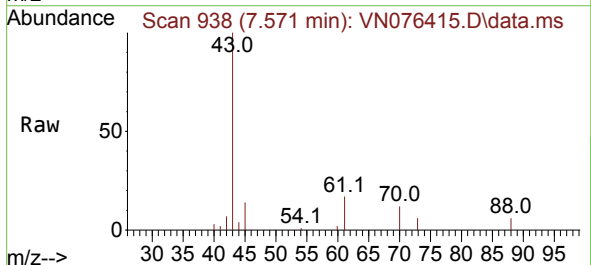




#38
Carbon Tetrachloride
Concen: 6.268 ug/l
RT: 8.230 min Scan# 1107
Delta R.T. -0.135 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13




Instrument :
MSVOA_N
ClientSampleId :
PB150465TB


Tgt Ion:117 Resp: 45030
Ion Ratio Lower Upper
117 100
119 5.9 75.4 113.0#
121 0.0 24.2 36.2#

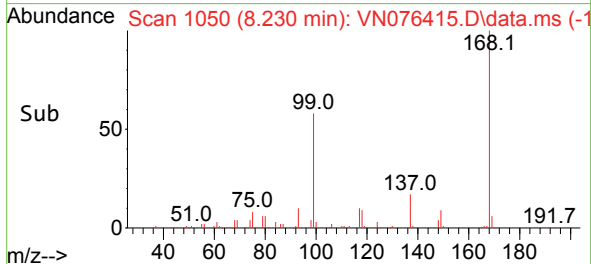

#42
1,2-Dichloroethane
Concen: 0.254 ug/l
RT: 8.694 min Scan# 1129
Delta R.T. 0.017 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13

Tgt Ion: 62 Resp: 1675
Ion Ratio Lower Upper
62 100
98 0.0 0.0 20.4


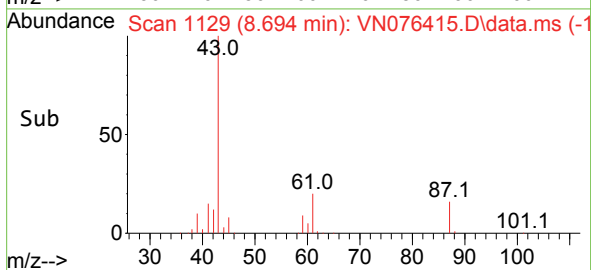






#43
Isopropyl Acetate
Concen: 26.224 ug/l
RT: 8.694 min Scan# 1129
Delta R.T. 0.000 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13




Instrument :
MSVOA_N
ClientSampleId :
PB150465TB


Tgt Ion: 43 Resp: 220439
Ion Ratio Lower Upper
43 100
61 17.4 23.5 35.3#
87 13.4 13.8 20.6#

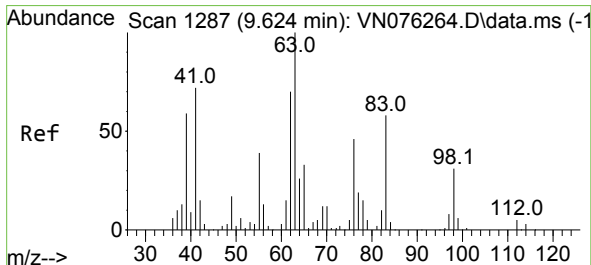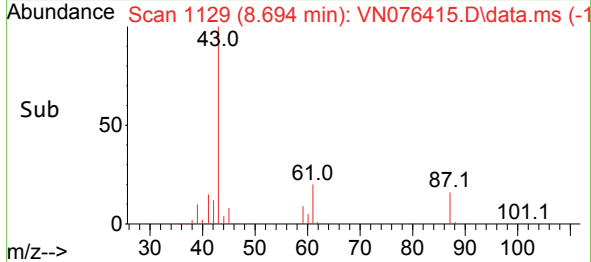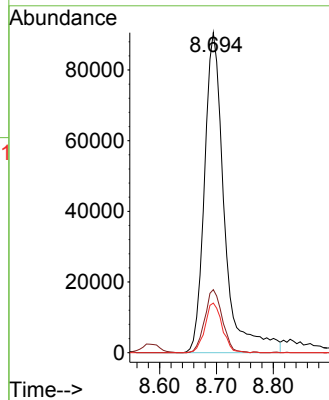

#45
1,2-Dichloropropane
Concen: 0.615 ug/l
RT: 9.741 min Scan# 1307
Delta R.T. 0.117 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13

Tgt Ion: 63 Resp: 2837
Ion Ratio Lower Upper
63 100
65 0.0 26.4 39.6#



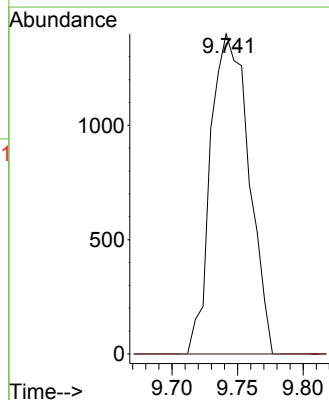
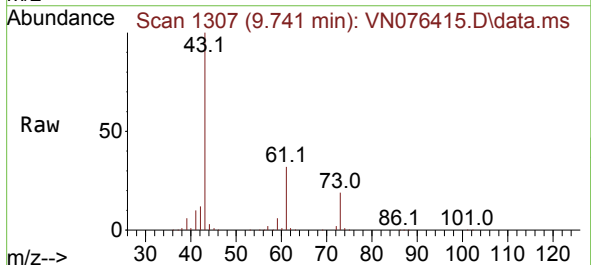




#48
Methyl methacrylate
Concen: 1.300 ug/l
RT: 9.665 min Scan# 1294
Delta R.T. -0.017 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13




Instrument :
MSVOA_N
ClientSampleId :
PB150465TB


Tgt Ion: 41 Resp: 5172
Ion Ratio Lower Upper
41 100
69 5.8 80.8 121.2#
39 0.0 54.4 81.6#

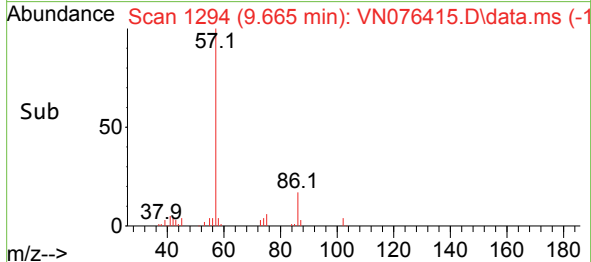

#49
1,4-Dioxane
Concen: 0.655 ug/l
RT: 9.688 min Scan# 1298
Delta R.T. -0.012 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13

Tgt Ion: 88 Resp: 55
Ion Ratio Lower Upper
88 100
43 0.0 18.1 27.1#
58 6634.5 46.5 69.7#




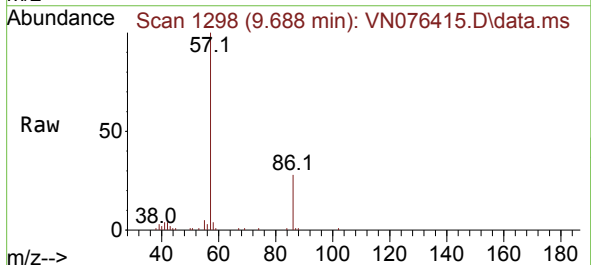


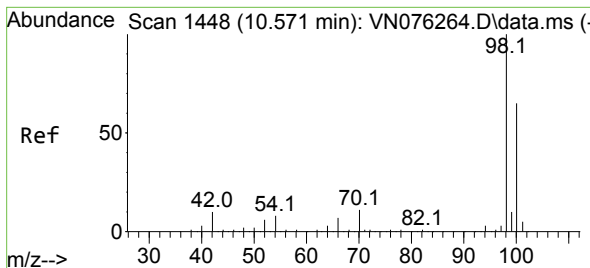

#50
Toluene-d8
Concen: 50.469 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13




Instrument :
MSVOA_N
ClientSampleId :
PB150465TB


Tgt Ion: 98 Resp: 845012
Ion Ratio Lower Upper
98 100
100 65.1 52.2 78.4

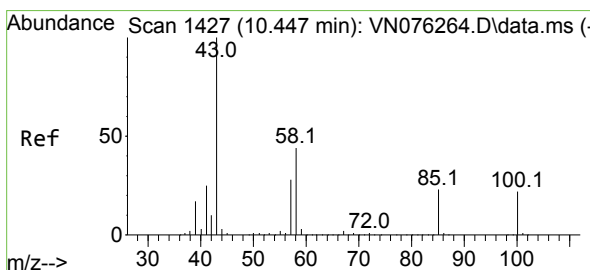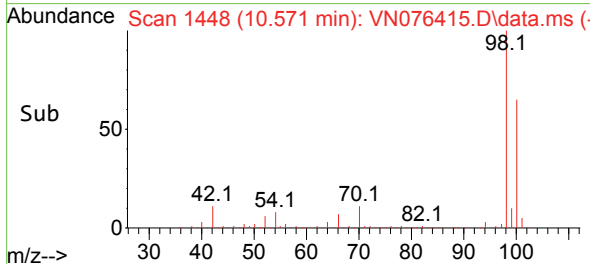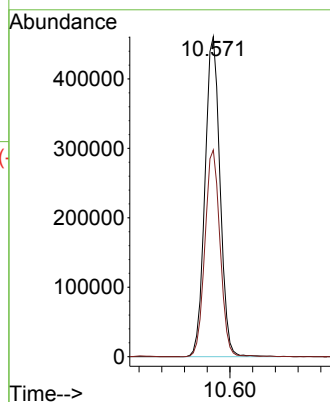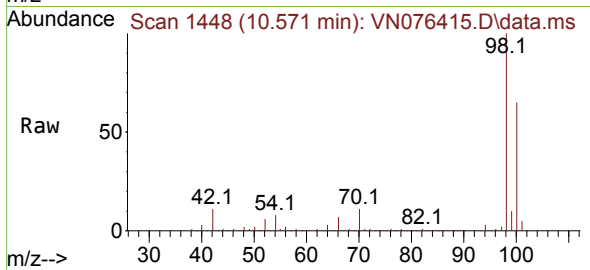

#51
4-Methyl-2-Pentanone
Concen: 3.577 ug/l
RT: 10.453 min Scan# 1428
Delta R.T. 0.006 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13

Tgt Ion: 43 Resp: 17652
Ion Ratio Lower Upper
43 100
58 26.5 35.1 52.7#


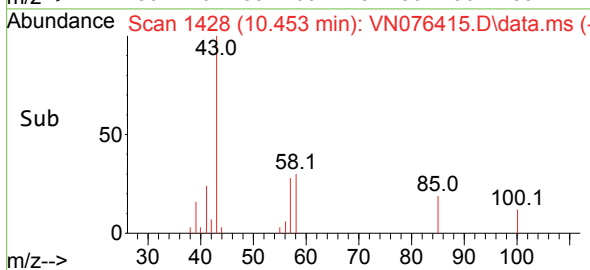
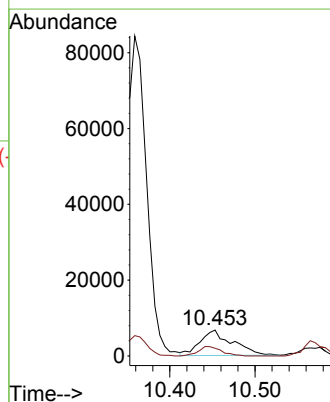
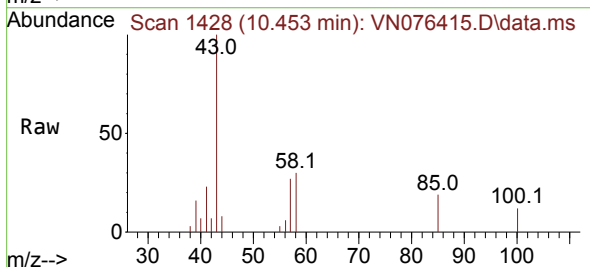


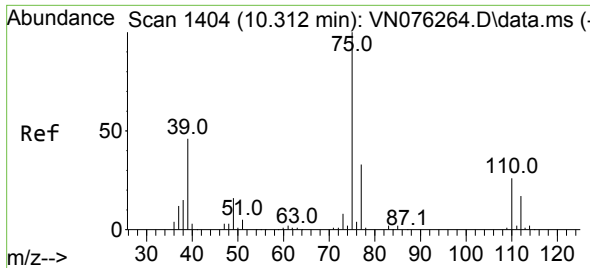

#54
 cis-1,3-Dichloropropene
 Concen: 10.508 ug/l
 RT: 10.359 min Scan# 1412
 Delta R.T. 0.047 min
 Lab File: VN076415.D
 Acq: 26 Jan 2023 13:13




Instrument :
 MSVOA_N
 ClientSampleId :
 PB150465TB


Tgt Ion: 75 Resp: 77833
 Ion Ratio Lower Upper
 75 100
 77 0.6 26.5 39.7#
 39 33.0 37.1 55.7#

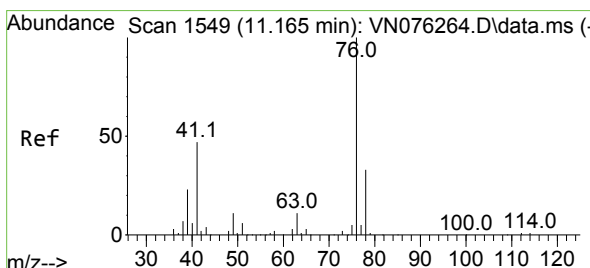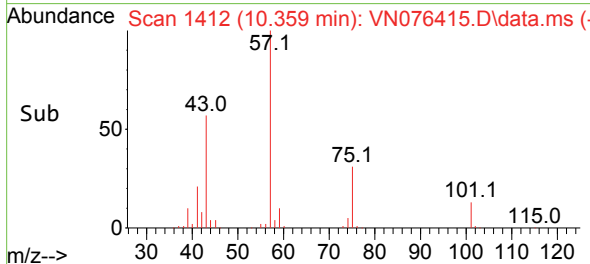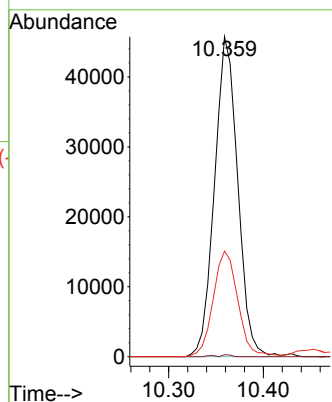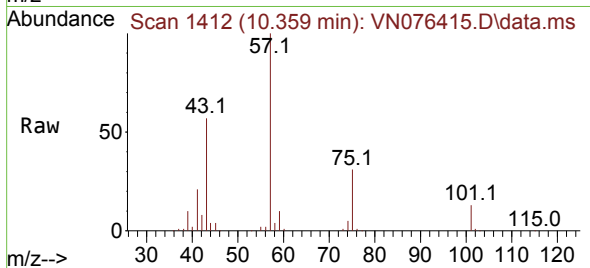

#57
 1,3-Dichloropropane
 Concen: 1.358 ug/l
 RT: 11.206 min Scan# 1556
 Delta R.T. 0.041 min
 Lab File: VN076415.D
 Acq: 26 Jan 2023 13:13

Tgt Ion: 76 Resp: 10863
 Ion Ratio Lower Upper
 76 100
 78 0.0 26.4 39.6#


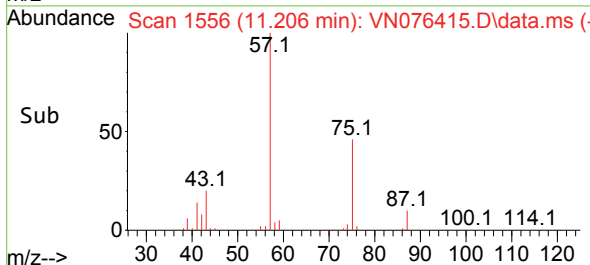

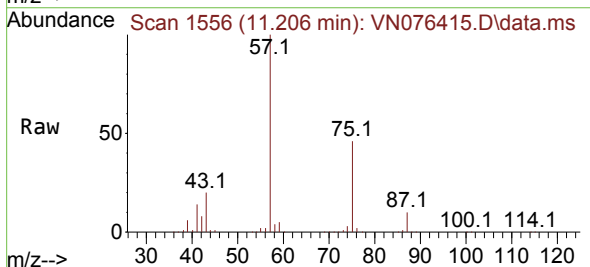




#59
2-Hexanone
Concen: 45.836 ug/l
RT: 11.171 min Scan# 111
Delta R.T. -0.023 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13




Instrument :
MSVOA_N
ClientSampleId :
PB150465TB


Tgt Ion: 43 Resp: 163908
Ion Ratio Lower Upper
43 100
58 0.0 30.1 90.3#

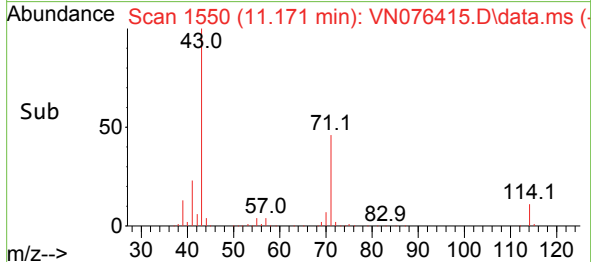

#62
4-Bromofluorobenzene
Concen: 48.415 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.006 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13

Tgt Ion: 95 Resp: 264632
Ion Ratio Lower Upper
95 100
174 83.5 0.0 174.6
176 79.3 0.0 167.8




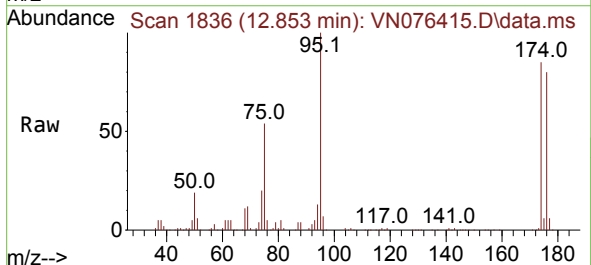


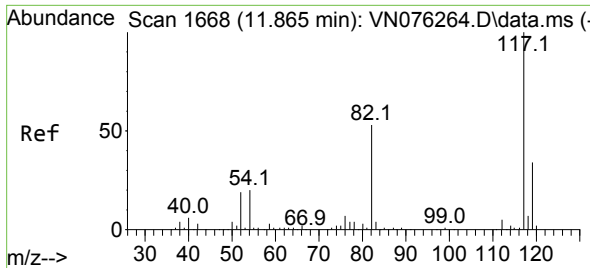

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 117
Delta R.T. 0.006 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13




Instrument :
MSVOA_N
ClientSampleId :
PB150465TB


Tgt Ion:117 Resp: 637506
Ion Ratio Lower Upper
117 100
82 54.5 42.2 63.2
119 32.6 26.9 40.3

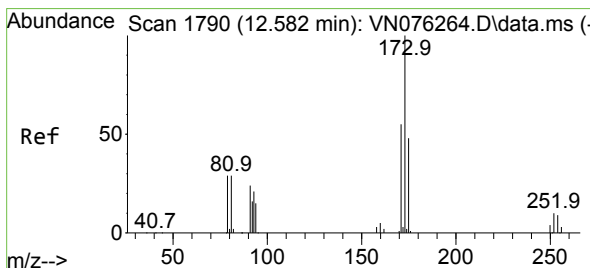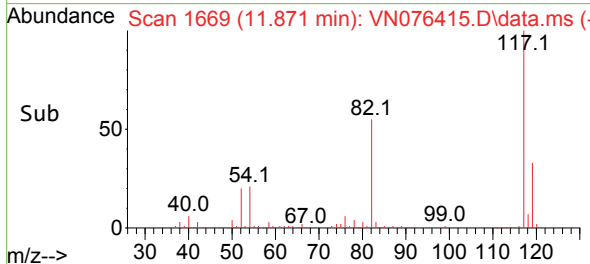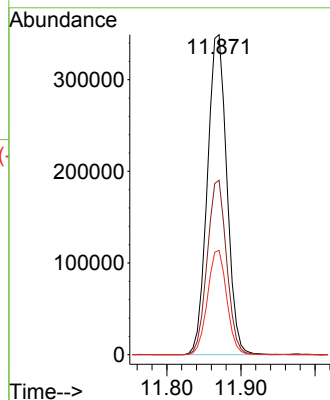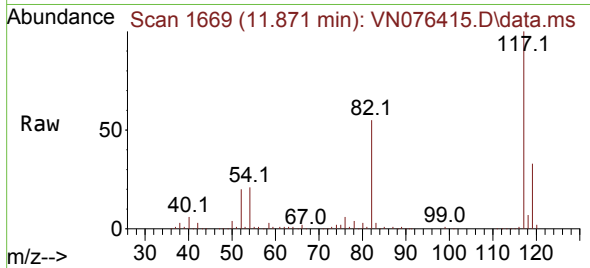

#71
Bromoform
Concen: 0.503 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.271 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13

Tgt Ion:173 Resp: 1821
Ion Ratio Lower Upper
173 100
175 714.8 24.1 72.4#
254 0.0 0.0 0.0


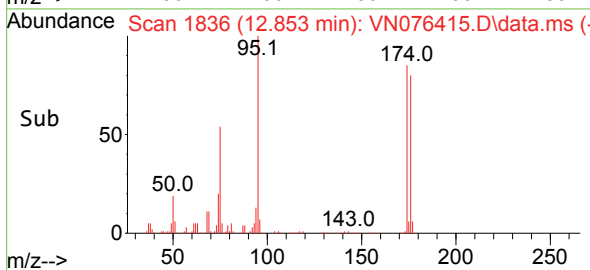
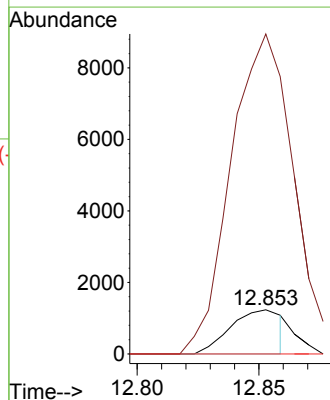
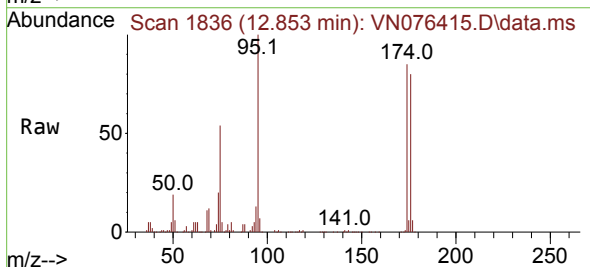


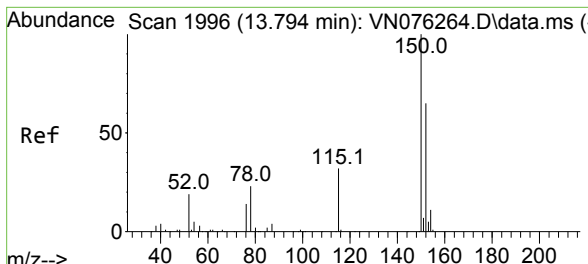

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13




Instrument :
MSVOA_N
ClientSampleId :
PB150465TB


Tgt Ion:152 Resp: 237119
Ion Ratio Lower Upper
152 100
115 60.8 29.6 88.9
150 160.1 0.0 351.4

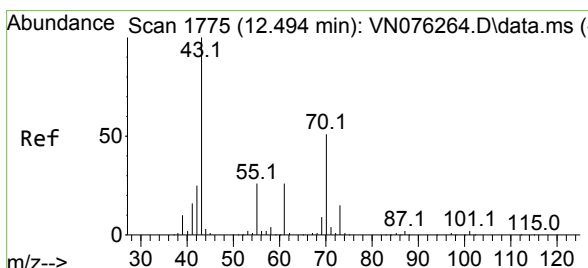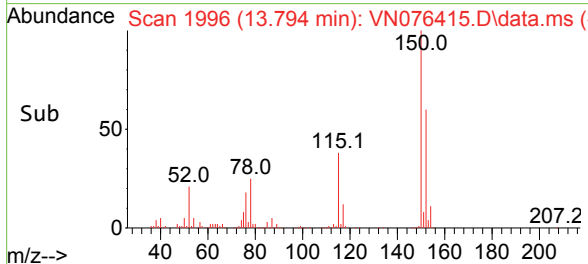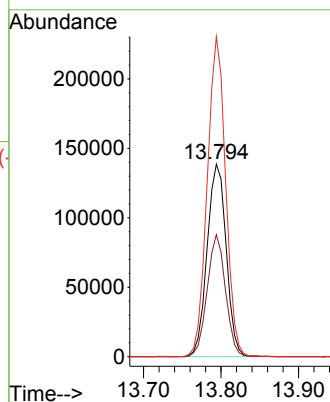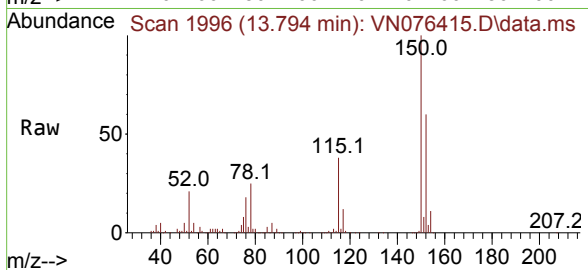

#74
N-ethyl acetate
Concen: 0.803 ug/l
RT: 12.494 min Scan# 1775
Delta R.T. 0.000 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13

Tgt Ion: 43 Resp: 4235
Ion Ratio Lower Upper
43 100
70 18.9 41.2 61.8#
55 15.4 21.0 31.6#
61 9.1 21.6 32.4#


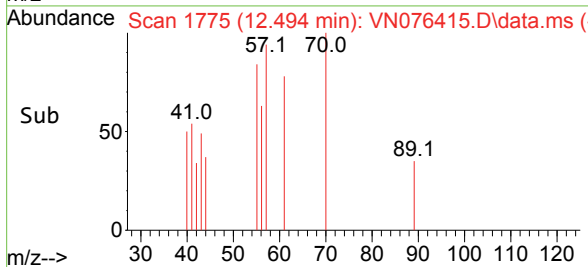
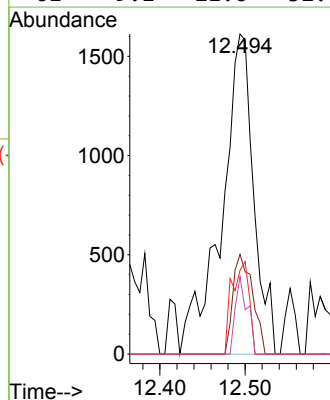
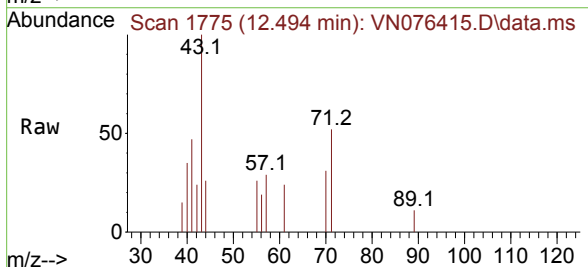




#76
1,2,3-Trichloropropane
Concen: 32.682 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.141 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13




Instrument :
MSVOA_N
ClientSampleId :
PB150465TB


Tgt Ion: 75 Resp: 142593
Ion Ratio Lower Upper
75 100
77 1.0 75.2 225.6#

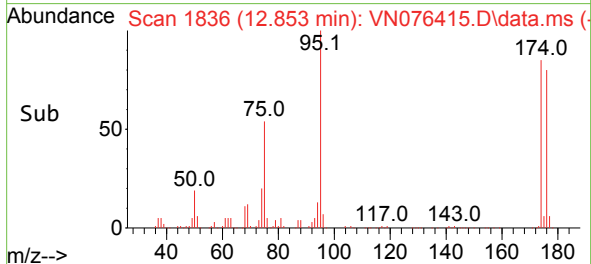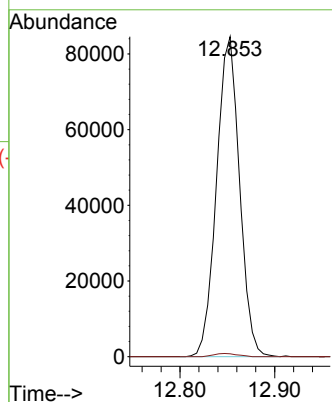

#77
Bromobenzene
Concen: Below Cal
RT: 12.982 min Scan# 1858
Delta R.T. 0.000 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13

Tgt Ion:156 Resp: 743
Ion Ratio Lower Upper
156 100
77 241.3 93.4 280.2
158 131.6 48.4 145.2



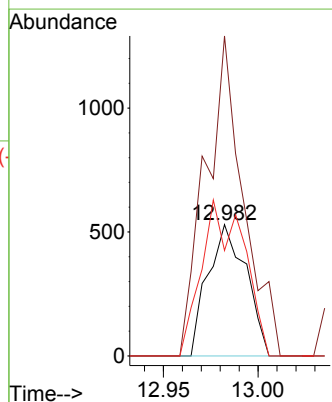





#81
trans-1,4-Dichloro-2-butene
Concen: 100.055 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.118 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13




Instrument :
MSVOA_N
ClientSampleId :
PB150465TB


Tgt Ion: 75 Resp: 142593
Ion Ratio Lower Upper
75 100
53 0.0 75.8 113.8#
89 0.0 37.0 55.6#

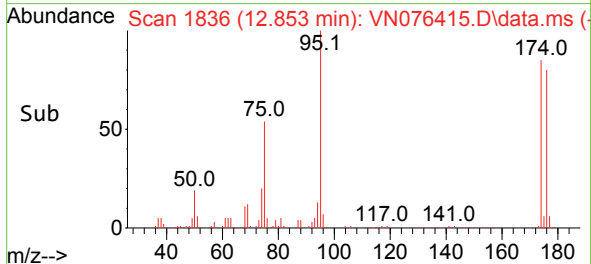

#87
1,3-Dichlorobenzene
Concen: 0.311 ug/l
RT: 13.741 min Scan# 1987
Delta R.T. 0.006 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13

Tgt Ion:146 Resp: 2685
Ion Ratio Lower Upper
146 100
111 42.2 19.9 59.7
148 65.4 31.6 94.8


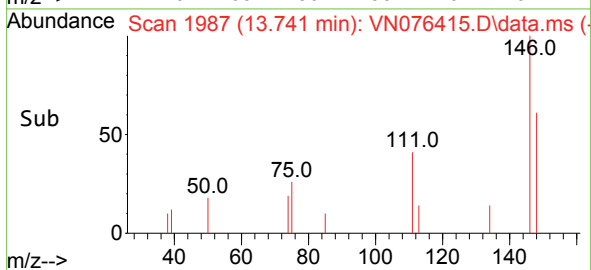

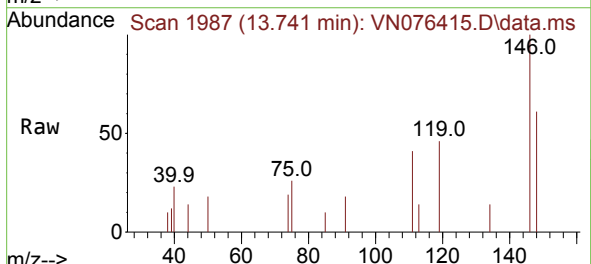




#88
1,4-Dichlorobenzene
Concen: 0.427 ug/l
RT: 13.741 min Scan# 1999
Delta R.T. -0.071 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13




Instrument :
MSVOA_N
ClientSampleId :
PB150465TB


Tgt Ion:146 Resp: 2685
Ion Ratio Lower Upper
146 100
111 42.2 19.1 57.5
148 65.4 31.9 95.9

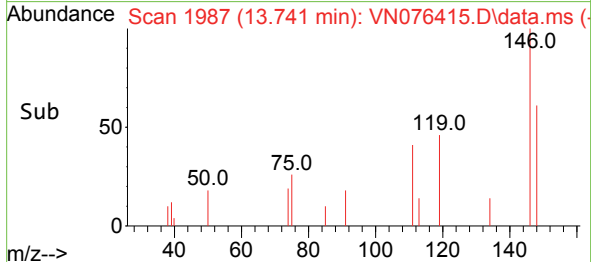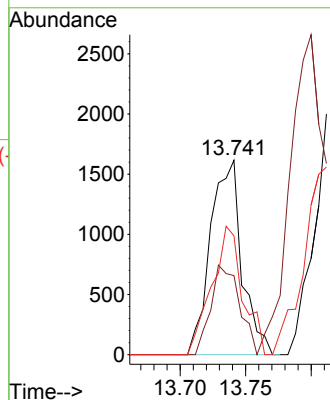

#89
n-Butylbenzene
Concen: 0.315 ug/l
RT: 14.059 min Scan# 2041
Delta R.T. -0.000 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13


Tgt Ion: 91 Resp: 3899
Ion Ratio Lower Upper
91 100
92 46.7 26.3 78.9
134 24.9 13.2 39.5

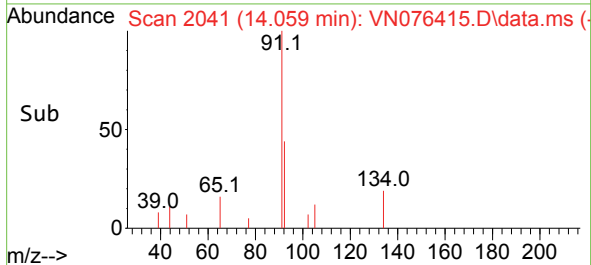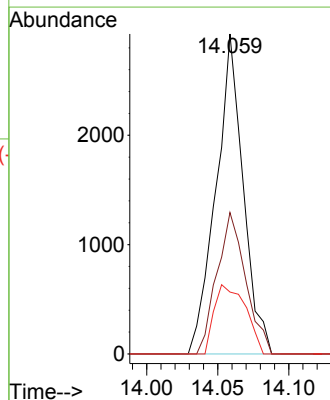






#91
1,2-Dichlorobenzene
Concen: 0.300 ug/l
RT: 14.106 min Scan# 2049
Delta R.T. -0.000 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13

Instrument :
MSVOA_N
ClientSampleId :
PB150465TB







Tgt Ion:146 Resp: 2580
Ion Ratio Lower Upper
146 100
111 40.2 20.3 60.8
148 70.5 31.8 95.4

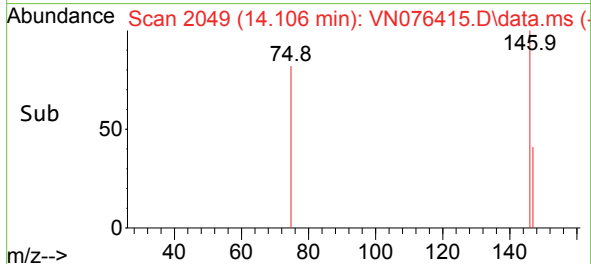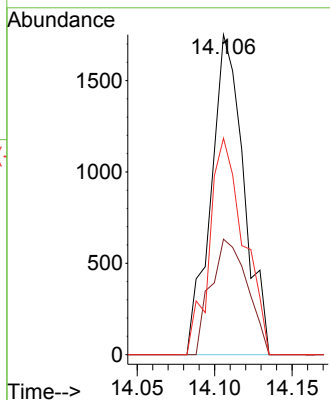

#93
1,2,4-Trichlorobenzene
Concen: 2.048 ug/l
RT: 15.394 min Scan# 2268
Delta R.T. -0.000 min
Lab File: VN076415.D
Acq: 26 Jan 2023 13:13

Tgt Ion:180 Resp: 3175
Ion Ratio Lower Upper
180 100
182 99.2 47.0 141.2
145 21.6 15.2 45.5

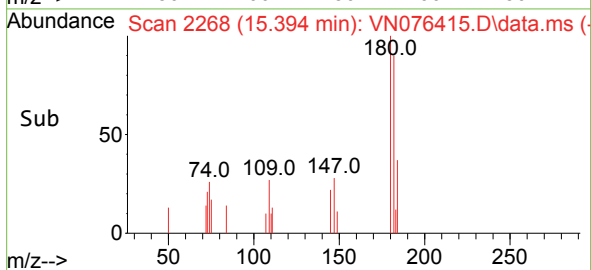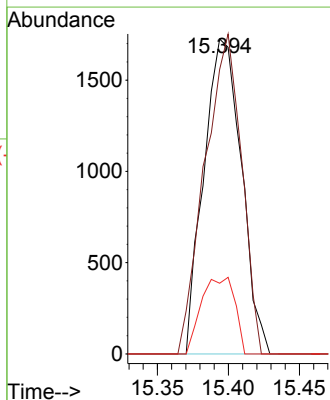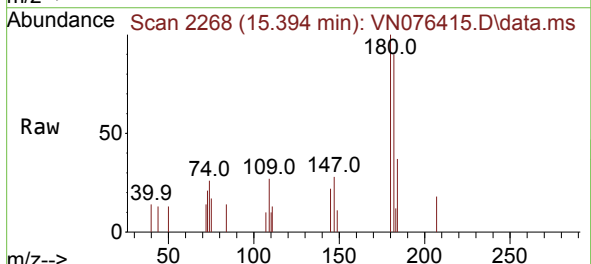



#95

Naphthalene

Concen: 2.878 ug/l

RT: 15.641 min Scan# 21

Delta R.T. -0.000 min

Lab File: VN076415.D

Acq: 26 Jan 2023 13:13

Instrument :

MSVOA_N

ClientSampleId :

PB150465TB





Tgt Ion:128 Resp: 13285

Ion Ratio Lower Upper

128 100

127 15.4 10.3 15.5

129 10.8 8.6 13.0

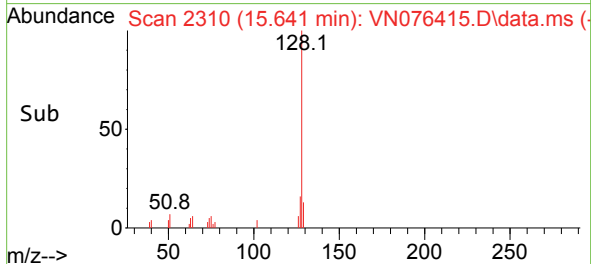

#96

1,2,3-Trichlorobenzene

Concen: 1.970 ug/l

RT: 15.847 min Scan# 2345

Delta R.T. 0.006 min

Lab File: VN076415.D

Acq: 26 Jan 2023 13:13

Tgt Ion:180 Resp: 3315

Ion Ratio Lower Upper

180 100

182 96.5 47.5 142.5

145 31.6 15.9 47.6

