

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012623\
 Data File : VN076418.D
 Acq On : 26 Jan 2023 14:25
 Operator : JC\MD
 Sample : PB150465ZHE#03
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB150465ZHE#03

Quant Time: Jan 27 00:35:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 17 03:59:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.236	168	397125	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	665102	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	592259	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	228550	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	233126	52.429	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 104.860%	
35) Dibromofluoromethane	8.171	113	201926	48.534	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 97.060%	
50) Toluene-d8	10.571	98	778782	50.685	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 101.360%	
62) 4-Bromofluorobenzene	12.853	95	247348	49.312	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 98.620%	
Target Compounds						
					Qvalue	
5) Bromomethane	2.983	94	1208	0.286	ug/l	89
11) Tert butyl alcohol	5.524	59	1008	1.695	ug/l #	72
16) Acetone	4.442	43	38104	26.666	ug/l	91
18) Methyl Acetate	5.047	43	3337	0.691	ug/l #	81
20) Methylene Chloride	5.283	84	29870	6.558	ug/l	96
25) 2-Butanone	7.506	43	3221	1.480	ug/l	100
31) Cyclohexane	8.230	56	8533	1.249	ug/l #	18
36) 1,1-Dichloropropene	8.230	75	30826	5.214	ug/l #	48
37) Ethyl Acetate	7.571	43	35723	7.565	ug/l #	95
38) Carbon Tetrachloride	8.230	117	41536	6.300	ug/l #	16
42) 1,2-Dichloroethane	8.694	62	1527	0.252	ug/l #	73
43) Isopropyl Acetate	8.694	43	416515	53.993	ug/l #	69
45) 1,2-Dichloropropane	9.747	63	2363	0.558	ug/l #	42
48) Methyl methacrylate	9.747	41	167026	45.735	ug/l #	35
49) 1,4-Dioxane	9.735	88	183	2.375	ug/l #	1
51) 4-Methyl-2-Pentanone	10.447	43	15808	3.491	ug/l #	71
53) t-1,3-Dichloropropene	10.729	75	1610	0.273	ug/l	100
54) cis-1,3-Dichloropropene	10.359	75	78127	11.494	ug/l #	66
56) Ethyl methacrylate	10.988	69	2047	0.351	ug/l #	1
57) 1,3-Dichloropropane	11.206	76	10636	1.448	ug/l #	42
59) 2-Hexanone	11.206	43	105761	32.228	ug/l #	53
71) Bromoform	12.853	173	1395	0.415	ug/l #	1
74) N-amyl acetate	12.488	43	2737	0.538	ug/l #	40
76) 1,2,3-Trichloropropane	12.853	75	134707	32.013	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	134707	98.066	ug/l #	11
88) 1,4-Dichlorobenzene	13.812	146	795	0.201	ug/l #	1
93) 1,2,4-Trichlorobenzene	15.394	180	317	1.382	ug/l #	46
95) Naphthalene	15.641	128	2452	2.038	ug/l #	85
96) 1,2,3-Trichlorobenzene	15.841	180	509	1.284	ug/l #	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012623\
Data File : VN076418.D
Acq On : 26 Jan 2023 14:25
Operator : JC\MD
Sample : PB150465ZHE#03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB150465ZHE#03


Quant Time: Jan 27 00:35:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 17 03:59:22 2023
Response via : Initial Calibration

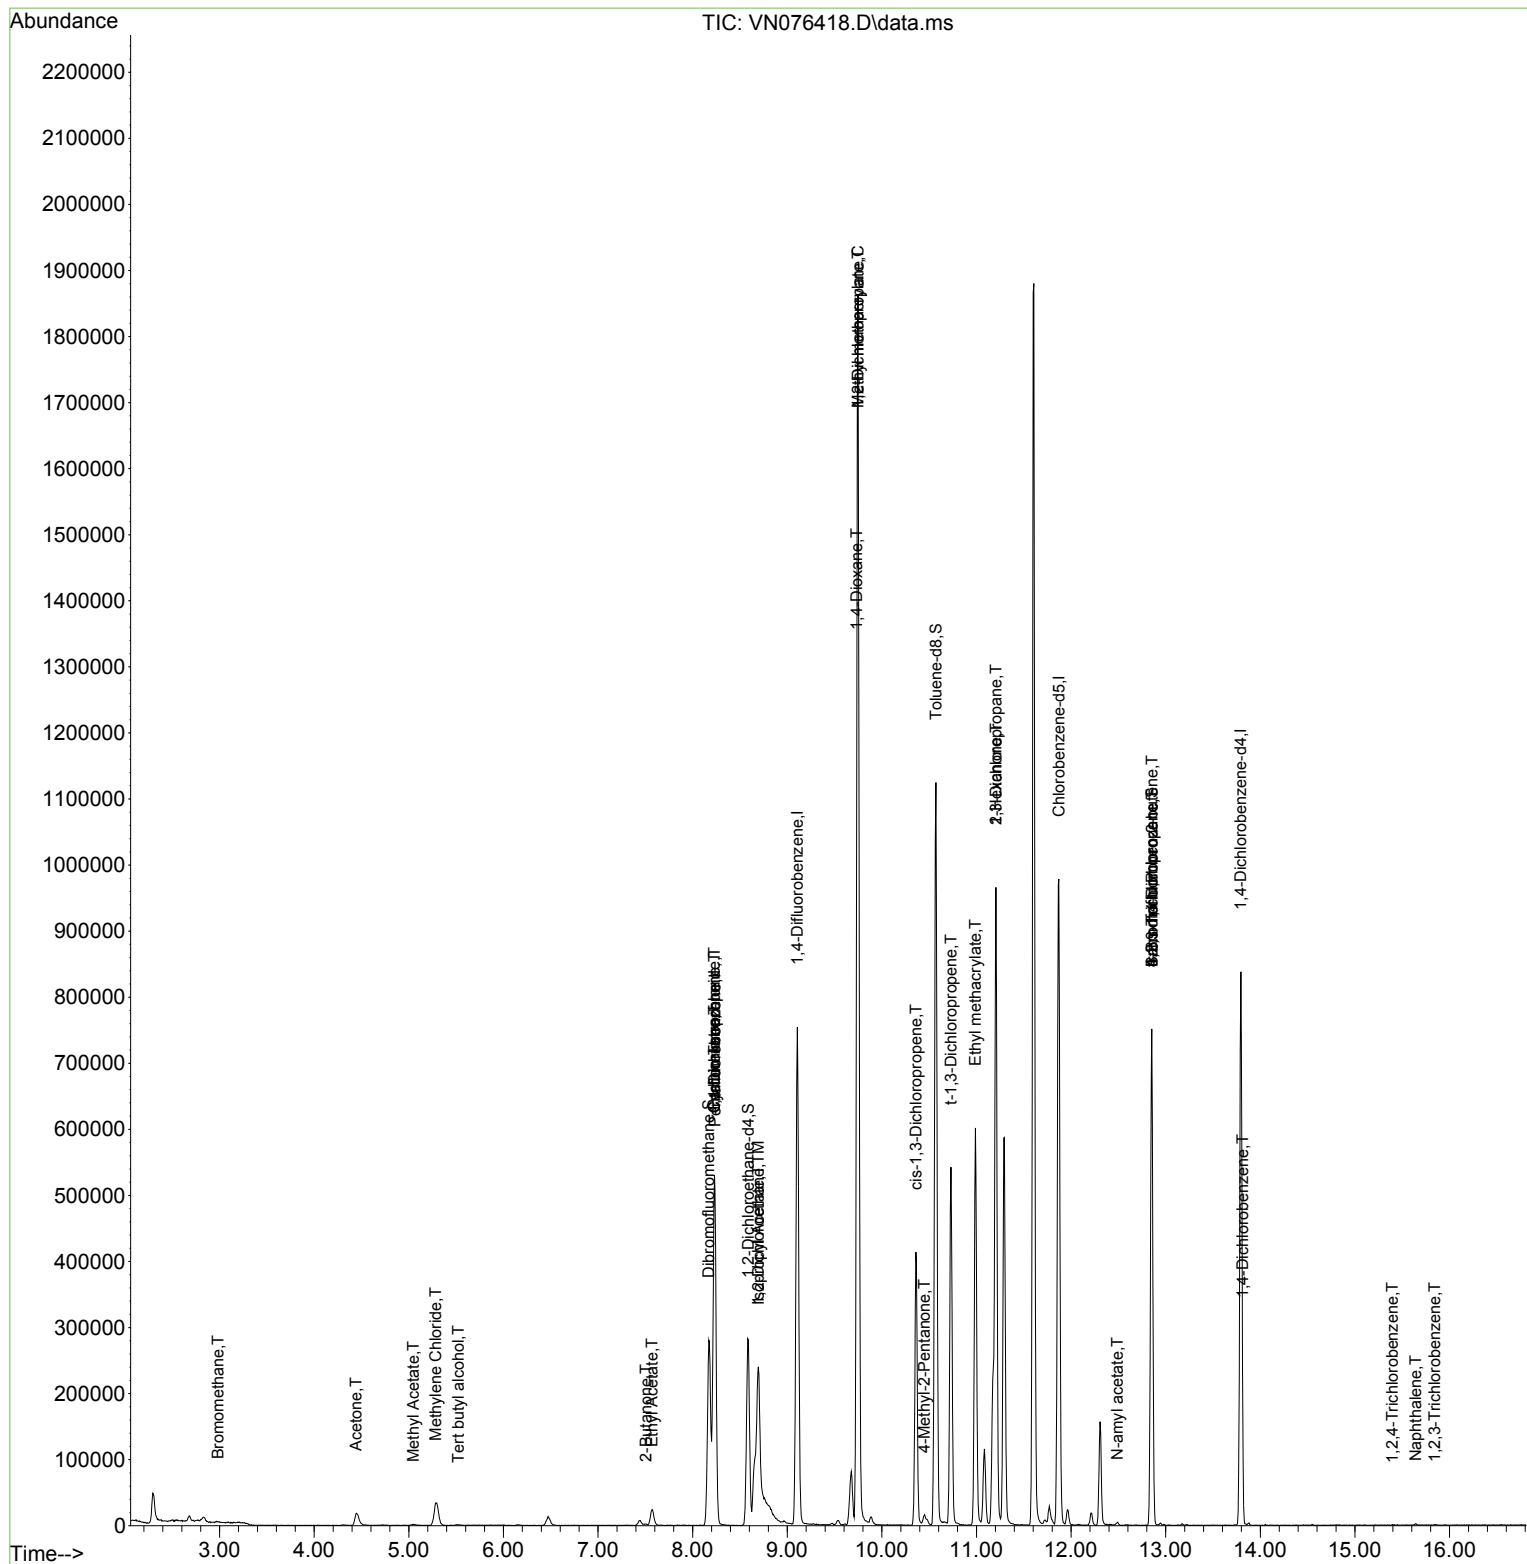






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.236 min Scan# 1051
Delta R.T. 0.006 min
Lab File: VN076418.D
Acq: 26 Jan 2023 14:25

Instrument :
MSVOA_N
ClientSampleId :
PB150465ZHE#03







Tgt Ion:168 Resp: 397125
Ion Ratio Lower Upper
168 100
99 56.9 41.6 62.4

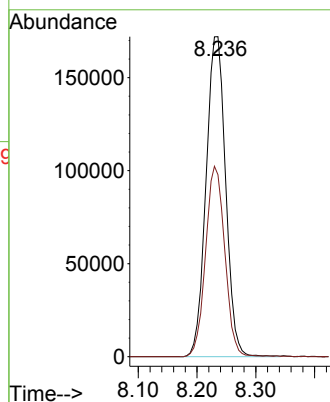

#5
Bromomethane
Concen: 0.286 ug/l
RT: 2.983 min Scan# 158
Delta R.T. 0.030 min
Lab File: VN076418.D
Acq: 26 Jan 2023 14:25

Tgt Ion: 94 Resp: 1208
Ion Ratio Lower Upper
94 100
96 82.9 75.1 112.7


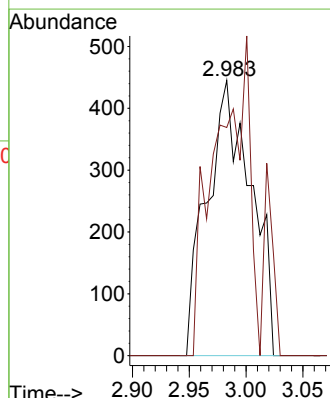






#11
Tert butyl alcohol
Concen: 1.695 ug/l
RT: 5.524 min Scan# 591
Delta R.T. -0.006 min
Lab File: VN076418.D
Acq: 26 Jan 2023 14:25




Instrument :
MSVOA_N
ClientSampleId :
PB150465ZHE#03


Tgt Ion: 59 Resp: 1008
Ion Ratio Lower Upper
59 100
57 0.0 8.5 12.7#



#16
Acetone
Concen: 26.666 ug/l
RT: 4.442 min Scan# 406
Delta R.T. -0.000 min
Lab File: VN076418.D
Acq: 26 Jan 2023 14:25

Tgt Ion: 43 Resp: 38104
Ion Ratio Lower Upper
43 100
58 28.4 26.7 40.1


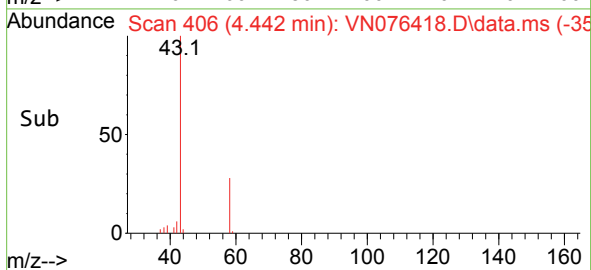

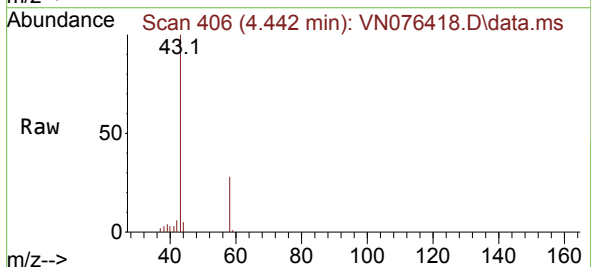




#18
Methyl Acetate
Concen: 0.691 ug/l
RT: 5.047 min Scan# 509
Delta R.T. 0.011 min
Lab File: VN076418.D
Acq: 26 Jan 2023 14:25




Instrument :
MSVOA_N
ClientSampleId :
PB150465ZHE#03


Tgt Ion: 43 Resp: 3337
Ion Ratio Lower Upper
43 100
74 19.0 23.3 34.9#

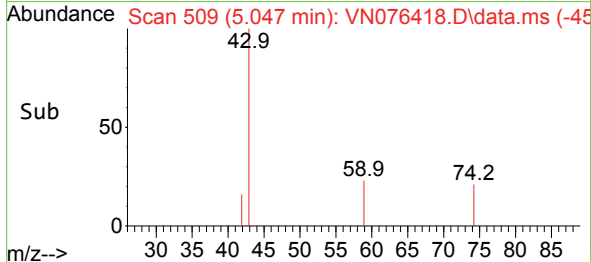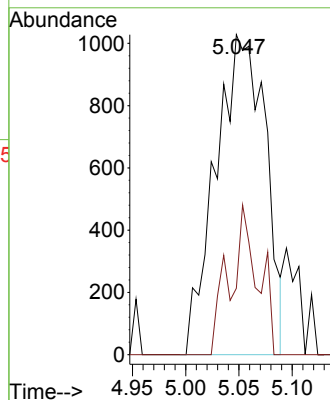

#20
Methylene Chloride
Concen: 6.558 ug/l
RT: 5.283 min Scan# 549
Delta R.T. -0.006 min
Lab File: VN076418.D
Acq: 26 Jan 2023 14:25

Tgt Ion: 84 Resp: 29870
Ion Ratio Lower Upper
84 100
49 107.1 84.5 126.7
51 37.4 26.0 39.0
86 59.5 52.0 78.0


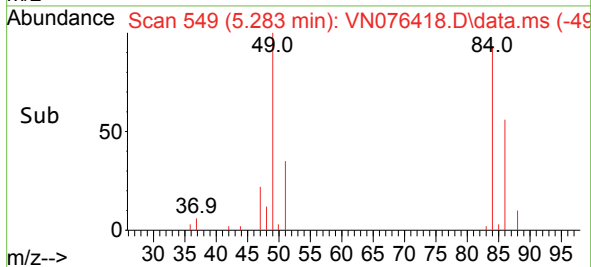
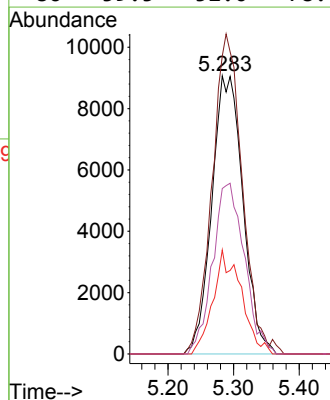
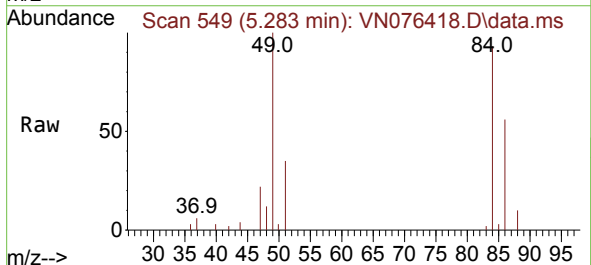




#25
2-Butanone
Concen: 1.480 ug/l
RT: 7.506 min Scan# 91
Delta R.T. 0.018 min
Lab File: VN076418.D
Acq: 26 Jan 2023 14:25




Instrument :
MSVOA_N
ClientSampleId :
PB150465ZHE#03


Tgt Ion: 43 Resp: 3221
Ion Ratio Lower Upper
43 100
72 34.6 27.4 41.2

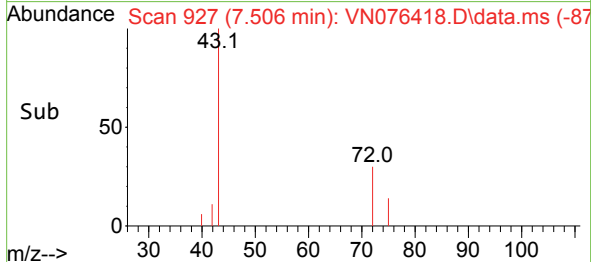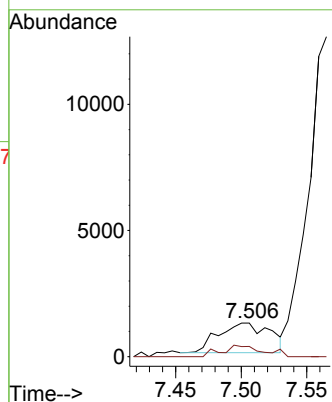

#31
Cyclohexane
Concen: 1.249 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.029 min
Lab File: VN076418.D
Acq: 26 Jan 2023 14:25

Tgt Ion: 56 Resp: 8533
Ion Ratio Lower Upper
56 100
69 157.1 25.8 38.8#
84 134.3 79.0 118.4#

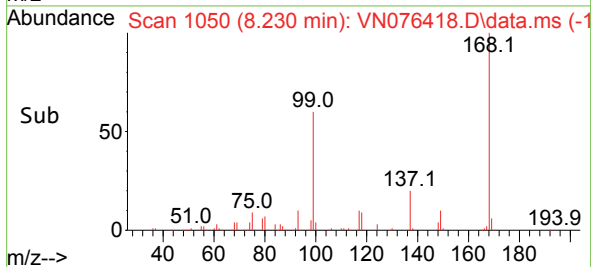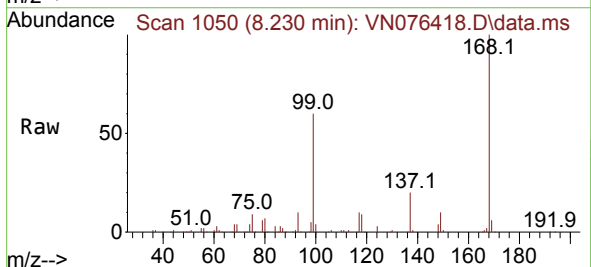



#33

1,2-Dichloroethane-d4

Concen: 52.429 ug/l

RT: 8.588 min Scan# 1111

Delta R.T. 0.006 min

Lab File: VN076418.D

Acq: 26 Jan 2023 14:25

Instrument :

MSVOA_N

ClientSampleId :





PB150465ZHE#03

Tgt Ion: 65 Resp: 233126

Ion Ratio Lower Upper

65 100

67 52.0 0.0 104.6

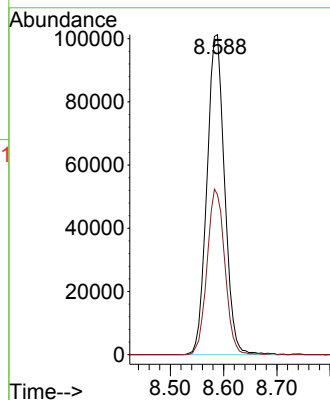

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. 0.000 min

Lab File: VN076418.D

Acq: 26 Jan 2023 14:25




Tgt Ion: 114 Resp: 665102


Ion Ratio Lower Upper

114 100

63 19.4 0.0 35.8

88 14.2 0.0 28.0

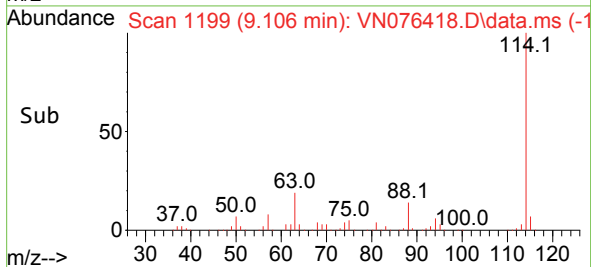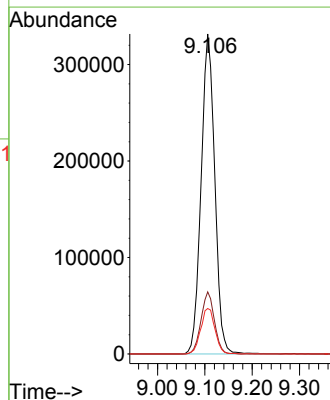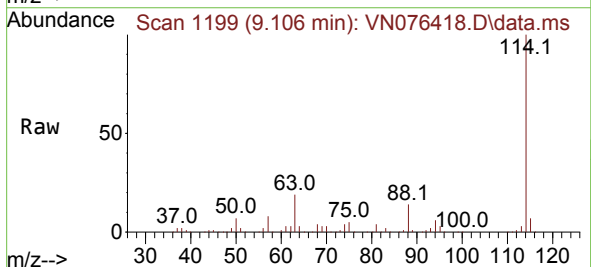



#35

Dibromofluoromethane

Concen: 48.534 ug/l

RT: 8.171 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN076418.D


Acq: 26 Jan 2023 14:25

Instrument :

MSVOA_N

ClientSampleId :

PB150465ZHE#03

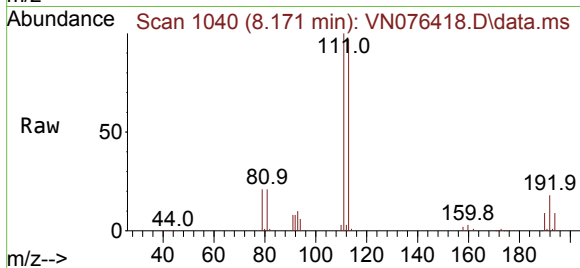




Tgt Ion:113 Resp: 201926

Ion Ratio Lower Upper

113 100

111 103.7 82.7 124.1

192 18.8 15.6 23.4

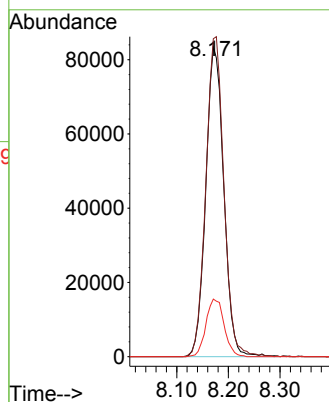

#36

1,1-Dichloropropene

Concen: 5.214 ug/l

RT: 8.230 min Scan# 1050

Delta R.T. -0.147 min

Lab File: VN076418.D

Acq: 26 Jan 2023 14:25




Tgt Ion: 75 Resp: 30826


Ion Ratio Lower Upper

75 100

110 8.5 18.8 56.3#

77 0.0 25.0 37.4#


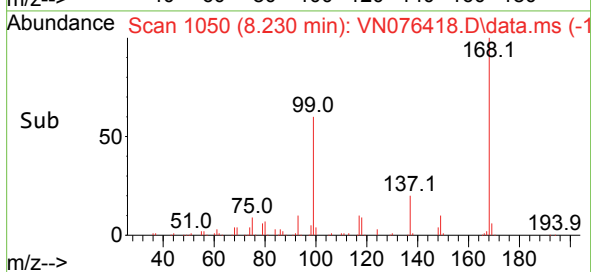
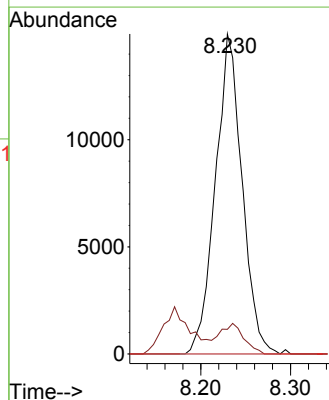
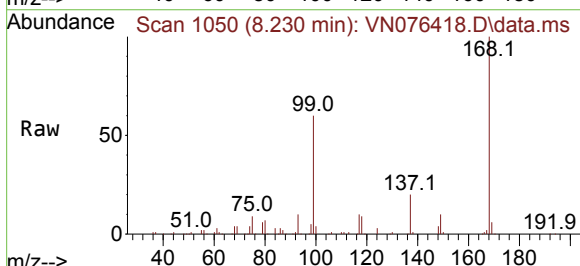




#37
Ethyl Acetate
Concen: 7.565 ug/l
RT: 7.571 min Scan# 91
Delta R.T. 0.006 min
Lab File: VN076418.D
Acq: 26 Jan 2023 14:25




Instrument :
MSVOA_N
ClientSampleId :
PB150465ZHE#03


Tgt Ion: 43 Resp: 35723
Ion Ratio Lower Upper
43 100
61 17.0 11.1 16.7#
70 13.1 10.0 15.0



#38
Carbon Tetrachloride
Concen: 6.300 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.135 min
Lab File: VN076418.D
Acq: 26 Jan 2023 14:25

Tgt Ion: 117 Resp: 41536
Ion Ratio Lower Upper
117 100
119 4.8 75.4 113.0#
121 0.0 24.2 36.2#

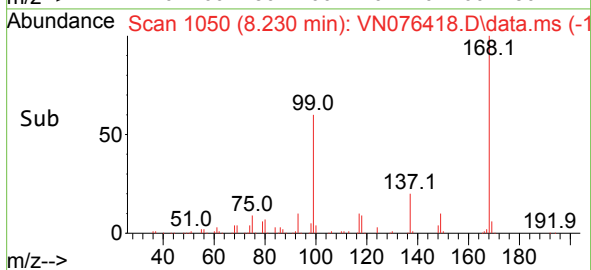



#42

1,2-Dichloroethane

Concen: 0.252 ug/l

RT: 8.694 min Scan# 1129

Delta R.T. 0.017 min

Lab File: VN076418.D

Acq: 26 Jan 2023 14:25

Instrument :

MSVOA_N

ClientSampleId :





PB150465ZHE#03

Tgt Ion: 62 Resp: 1527

Ion Ratio Lower Upper

62 100

98 0.0 0.0 20.4

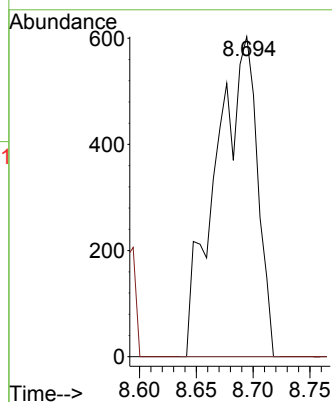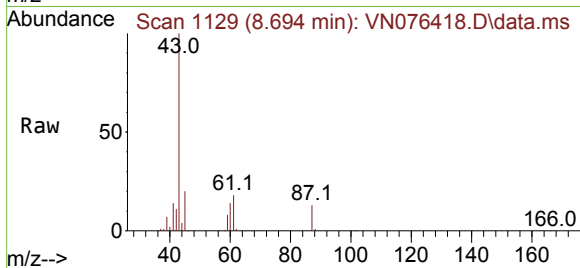

#43

Isopropyl Acetate

Concen: 53.993 ug/l

RT: 8.694 min Scan# 1129

Delta R.T. 0.000 min

Lab File: VN076418.D

Acq: 26 Jan 2023 14:25




Tgt Ion: 43 Resp: 416515


Ion Ratio Lower Upper

43 100

61 10.4 23.5 35.3#

87 7.4 13.8 20.6#




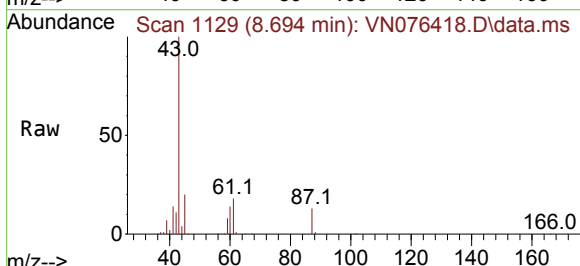


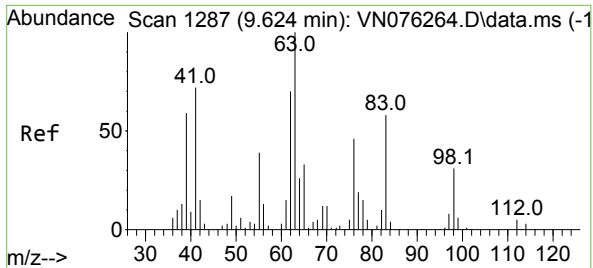

#45
1,2-Dichloropropane
Concen: 0.558 ug/l
RT: 9.747 min Scan# 1308
Delta R.T. 0.123 min
Lab File: VN076418.D
Acq: 26 Jan 2023 14:25




Instrument :
MSVOA_N
ClientSampleId :
PB150465ZHE#03


Tgt Ion: 63 Resp: 2363
Ion Ratio Lower Upper
63 100
65 0.0 26.4 39.6#

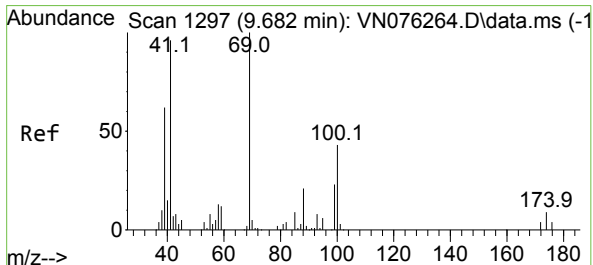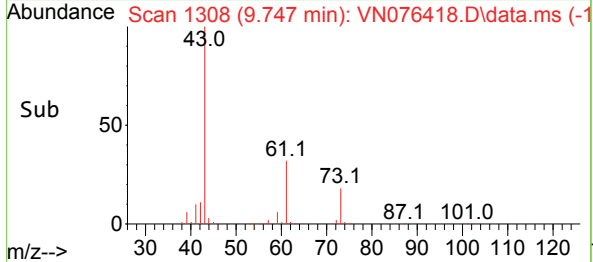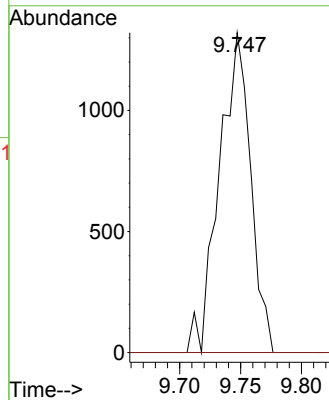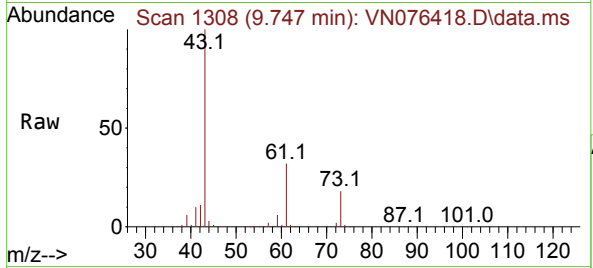

#48
Methyl methacrylate
Concen: 45.735 ug/l
RT: 9.747 min Scan# 1308
Delta R.T. 0.065 min
Lab File: VN076418.D
Acq: 26 Jan 2023 14:25

Tgt Ion: 41 Resp: 167026
Ion Ratio Lower Upper
41 100
69 0.0 80.8 121.2#
39 57.8 54.4 81.6

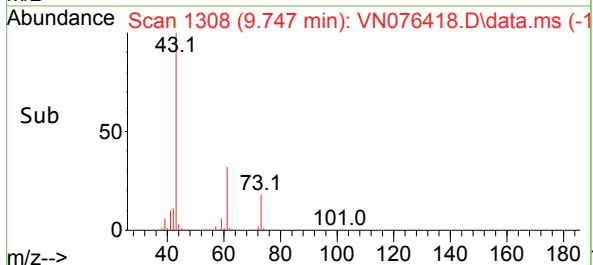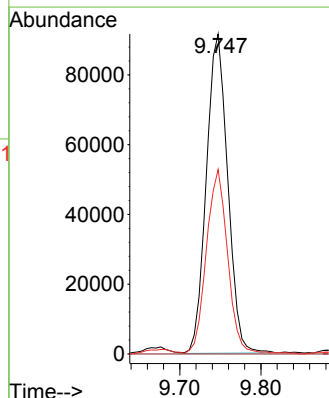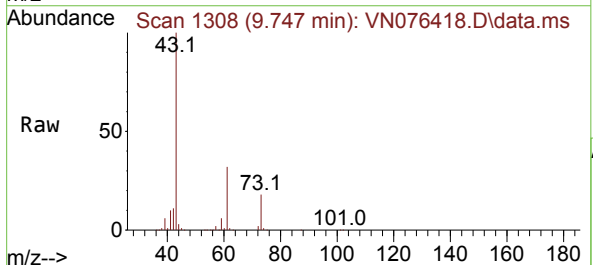



#49

1,4-Dioxane

Concen: 2.375 ug/l

RT: 9.735 min Scan# 1306

Delta R.T. 0.035 min

Lab File: VN076418.D

Acq: 26 Jan 2023 14:25

Instrument :

MSVOA_N

ClientSampleId :

PB150465ZHE#03





Tgt Ion: 88 Resp: 183

Ion Ratio Lower Upper

88 100

43 936190.7 18.1 27.1#

58 4502.2 46.5 69.7#

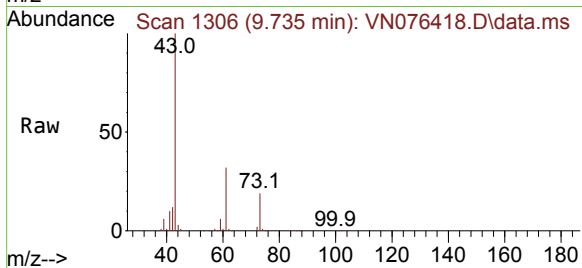

#50

Toluene-d8

Concen: 50.685 ug/l

RT: 10.571 min Scan# 1448

Delta R.T. -0.000 min

Lab File: VN076418.D




Acq: 26 Jan 2023 14:25


Tgt Ion: 98 Resp: 778782

Ion Ratio Lower Upper

98 100

100 65.2 52.2 78.4


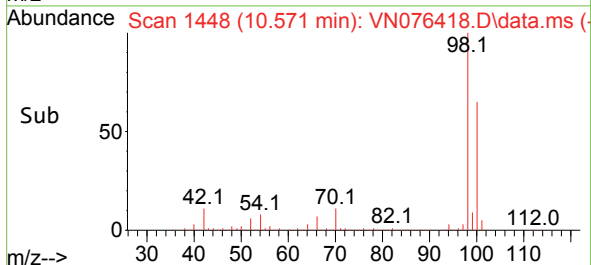
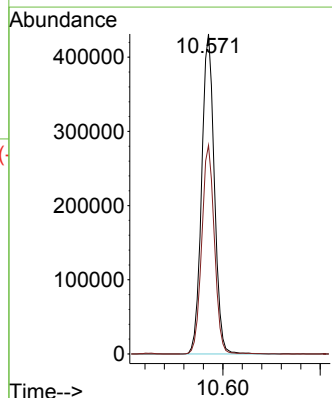
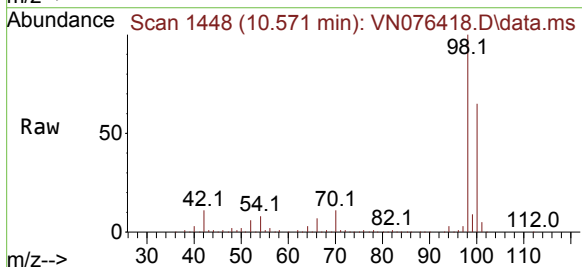




#51
4-Methyl-2-Pentanone
Concen: 3.491 ug/l
RT: 10.447 min Scan# 1427
Delta R.T. 0.000 min
Lab File: VN076418.D
Acq: 26 Jan 2023 14:25




Instrument :
MSVOA_N
ClientSampleId :
PB150465ZHE#03


Tgt Ion: 43 Resp: 15808
Ion Ratio Lower Upper
43 100
58 25.2 35.1 52.7#

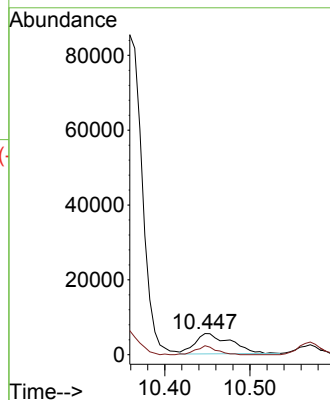

#53
t-1,3-Dichloropropene
Concen: 0.273 ug/l
RT: 10.729 min Scan# 1475
Delta R.T. -0.106 min
Lab File: VN076418.D
Acq: 26 Jan 2023 14:25

Tgt Ion: 75 Resp: 1610
Ion Ratio Lower Upper
75 100
77 32.3 25.8 38.6


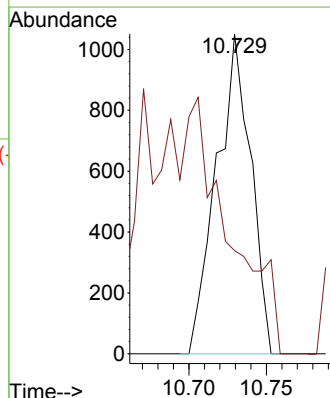
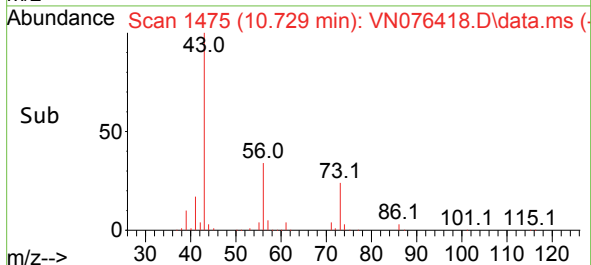
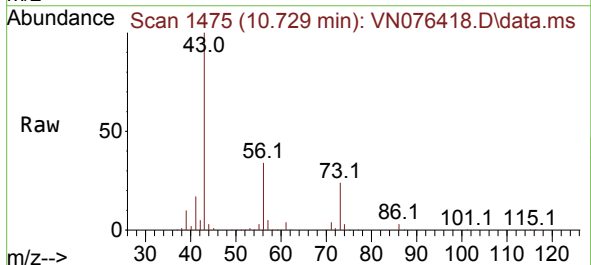


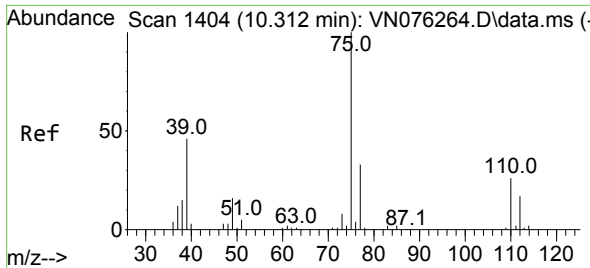

#54
 cis-1,3-Dichloropropene
 Concen: 11.494 ug/l
 RT: 10.359 min Scan# 1412
 Delta R.T. 0.047 min
 Lab File: VN076418.D
 Acq: 26 Jan 2023 14:25




Instrument :
 MSVOA_N
 ClientSampleId :
 PB150465ZHE#03


Tgt Ion: 75 Resp: 78127
 Ion Ratio Lower Upper
 75 100
 77 0.4 26.5 39.7#
 39 34.6 37.1 55.7#

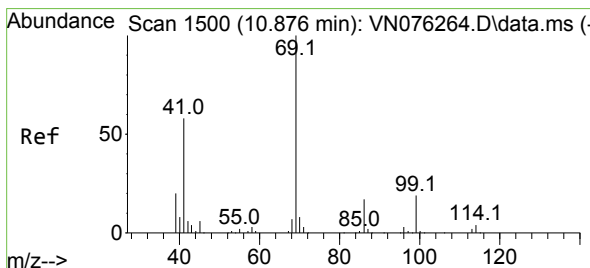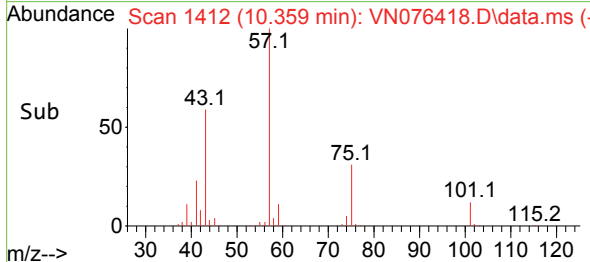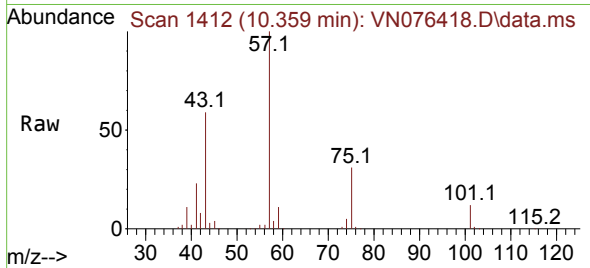

#56
 Ethyl methacrylate
 Concen: 0.351 ug/l
 RT: 10.988 min Scan# 1519
 Delta R.T. 0.112 min
 Lab File: VN076418.D
 Acq: 26 Jan 2023 14:25

Tgt Ion: 69 Resp: 2047
 Ion Ratio Lower Upper
 69 100
 41 5455.3 45.3 67.9#
 39 2504.3 29.3 43.9#


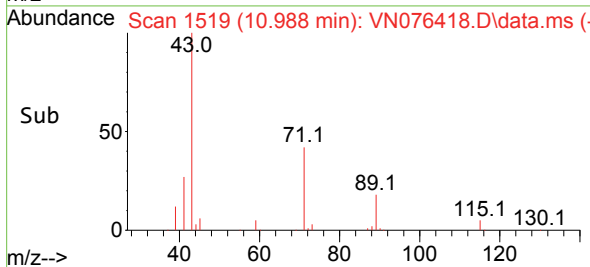

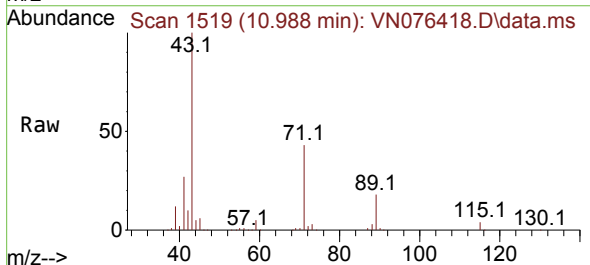




#57
1,3-Dichloropropane
Concen: 1.448 ug/l
RT: 11.206 min Scan# 1556
Delta R.T. 0.041 min
Lab File: VN076418.D
Acq: 26 Jan 2023 14:25




Instrument :
MSVOA_N
ClientSampleId :
PB150465ZHE#03


Tgt Ion: 76 Resp: 10636
Ion Ratio Lower Upper
76 100
78 0.0 26.4 39.6#

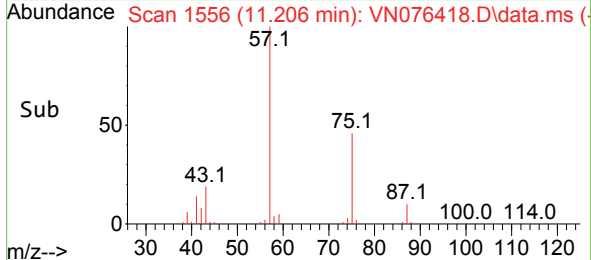

#59
2-Hexanone
Concen: 32.228 ug/l
RT: 11.206 min Scan# 1556
Delta R.T. 0.012 min
Lab File: VN076418.D
Acq: 26 Jan 2023 14:25

Tgt Ion: 43 Resp: 105761
Ion Ratio Lower Upper
43 100
58 24.8 30.1 90.3#

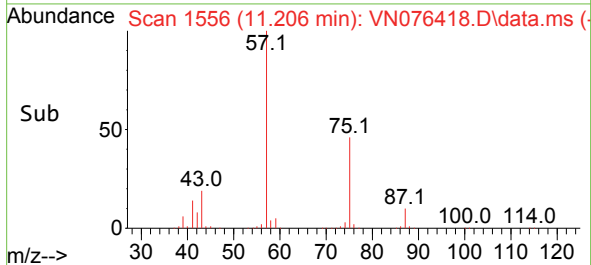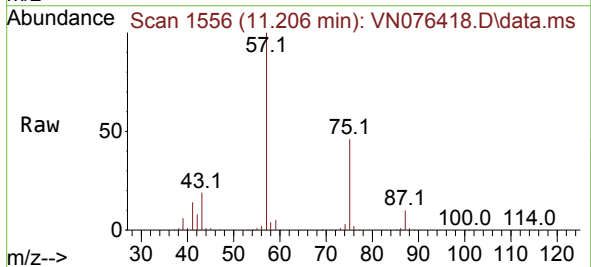



#62

4-Bromofluorobenzene

Concen: 49.312 ug/l

RT: 12.853 min Scan# 1836

Delta R.T. 0.006 min

Lab File: VN076418.D

Acq: 26 Jan 2023 14:25

Instrument :

MSVOA_N

ClientSampleId :

PB150465ZHE#03





Tgt Ion: 95 Resp: 247348

Ion Ratio Lower Upper

95 100

174 81.8 0.0 174.6

176 77.8 0.0 167.8

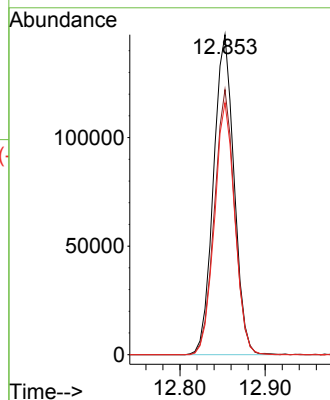

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.871 min Scan# 1669

Delta R.T. 0.006 min

Lab File: VN076418.D

Acq: 26 Jan 2023 14:25




Tgt Ion: 117 Resp: 592259


Ion Ratio Lower Upper

117 100

82 53.2 42.2 63.2

119 31.9 26.9 40.3

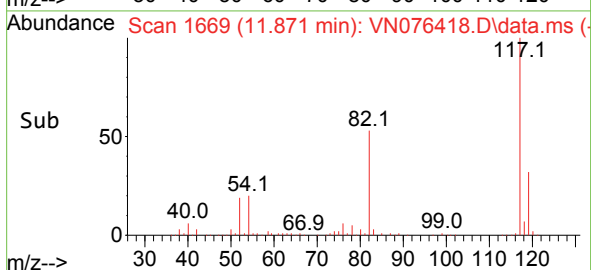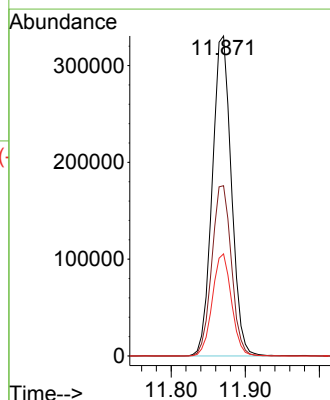



#71

Bromoform

Concen: 0.415 ug/l

RT: 12.853 min Scan# 1836

Delta R.T. 0.271 min

Lab File: VN076418.D

Acq: 26 Jan 2023 14:25

Instrument :

MSVOA_N

ClientSampleId :

PB150465ZHE#03





Tgt Ion:173 Resp: 1395

Ion Ratio Lower Upper

173 100

175 899.4 24.1 72.4#

254 0.0 0.0 0.0

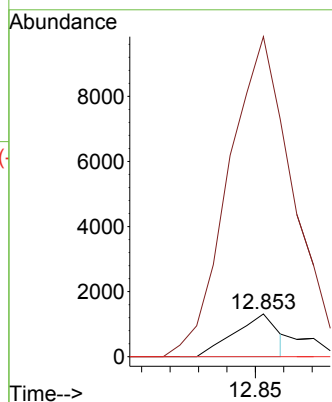

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 1996

Delta R.T. -0.000 min

Lab File: VN076418.D

Acq: 26 Jan 2023 14:25




Tgt Ion:152 Resp: 228550


Ion Ratio Lower Upper

152 100

115 59.5 29.6 88.9

150 158.9 0.0 351.4


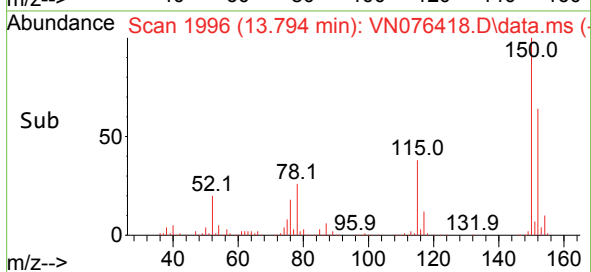
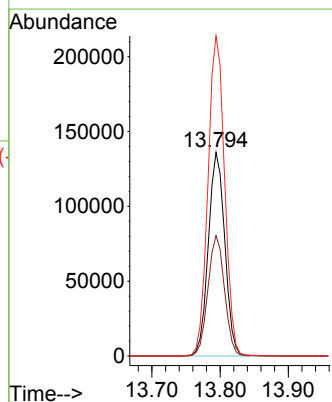





#74
N-amy1 acetate
Concen: 0.538 ug/l
RT: 12.488 min Scan# 1774
Delta R.T. -0.006 min
Lab File: VN076418.D
Acq: 26 Jan 2023 14:25




Instrument :
MSVOA_N
ClientSampleId :
PB150465ZHE#03


Tgt Ion:	43	Resp:	2737
Ion	Ratio	Lower	Upper
43	100		
70	0.0	41.2	61.8#
55	5.0	21.0	31.6#
61	0.0	21.6	32.4#

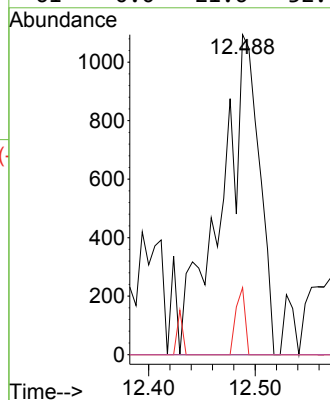

#76
1,2,3-Trichloropropane
Concen: 32.013 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. -0.141 min
Lab File: VN076418.D
Acq: 26 Jan 2023 14:25

Tgt Ion:	75	Resp:	134707
Ion	Ratio	Lower	Upper
75	100		
77	1.2	75.2	225.6#



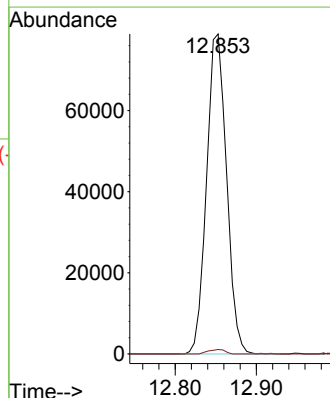
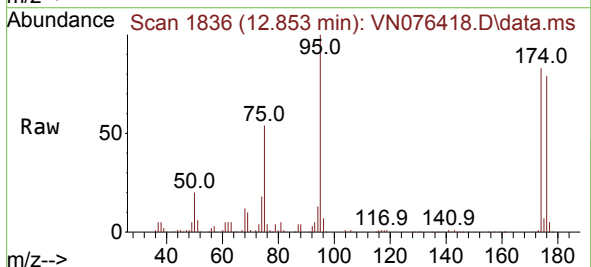




#81
 trans-1,4-Dichloro-2-butene
 Concen: 98.066 ug/l
 RT: 12.853 min Scan# 1836
 Delta R.T. 0.118 min
 Lab File: VN076418.D
 Acq: 26 Jan 2023 14:25




Instrument :
 MSVOA_N
 ClientSampleId :
 PB150465ZHE#03


Tgt Ion: 75 Resp: 134707
 Ion Ratio Lower Upper
 75 100
 53 0.0 75.8 113.8#
 89 0.1 37.0 55.6#



#88
 1,4-Dichlorobenzene
 Concen: 0.201 ug/l
 RT: 13.812 min Scan# 1999
 Delta R.T. -0.000 min
 Lab File: VN076418.D
 Acq: 26 Jan 2023 14:25

Tgt Ion:146 Resp: 795
 Ion Ratio Lower Upper
 146 100
 111 449.8 19.1 57.5#
 148 88.4 31.9 95.9

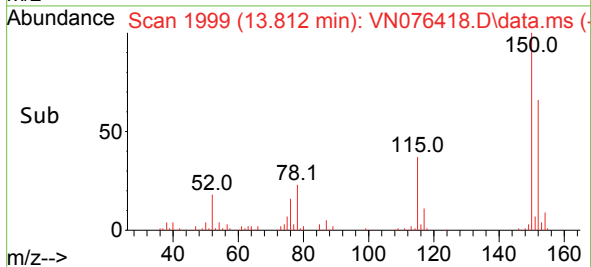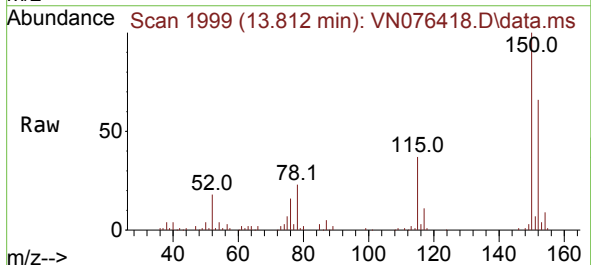

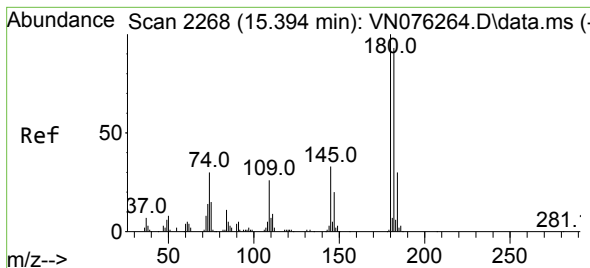

#93

1,2,4-Trichlorobenzene

Concen: 1.382 ug/l

RT: 15.394 min Scan# 21

Delta R.T. -0.000 min

Lab File: VN076418.D


Acq: 26 Jan 2023 14:25

Instrument :



MSVOA_N

ClientSampleId :

PB150465ZHE#03

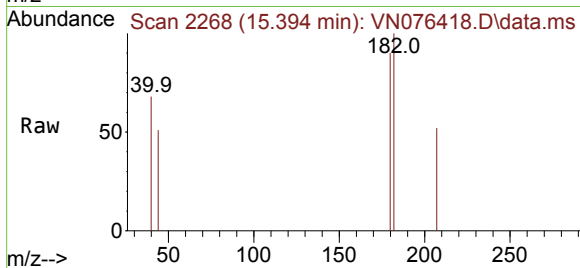

Tgt Ion:180	Resp:	317
Ion	Ratio	Lower Upper
180	100	
182	146.1	47.0 141.2#
145	0.0	15.2 45.5#

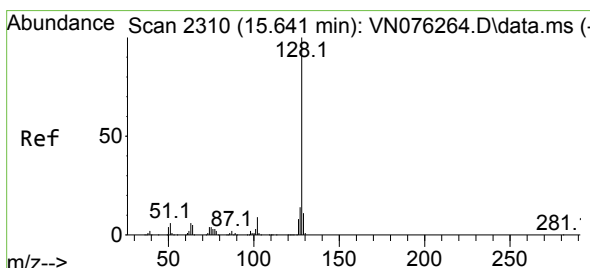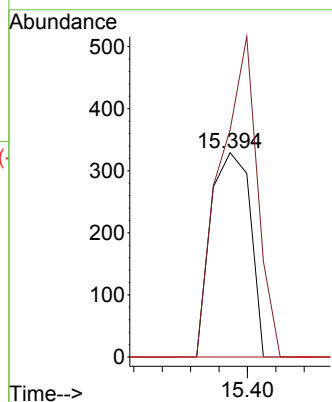

#95

Naphthalene

Concen: 2.038 ug/l




RT: 15.641 min Scan# 2310


Delta R.T. -0.000 min

Lab File: VN076418.D

Acq: 26 Jan 2023 14:25

Tgt Ion:128	Resp:	2452
Ion	Ratio	Lower Upper
128	100	
127	9.5	10.3 15.5#
129	2.2	8.6 13.0#

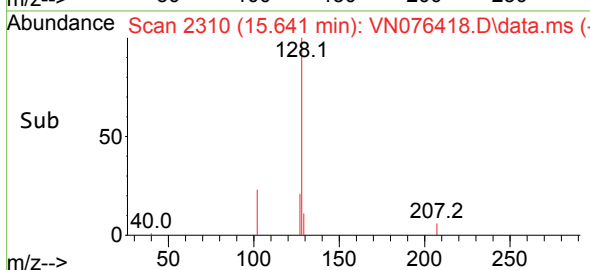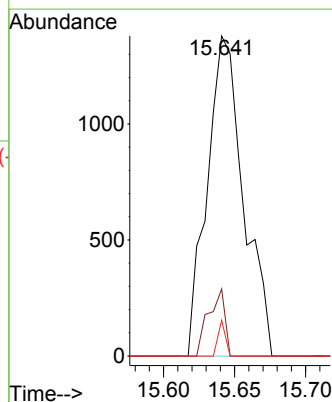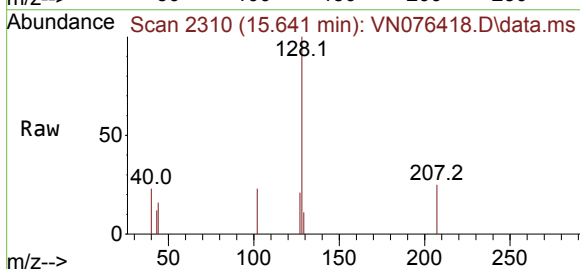



#96

1,2,3-Trichlorobenzene

Concen: 1.284 ug/l

RT: 15.841 min Scan# 21

Delta R.T. -0.000 min

Lab File: VN076418.D


Acq: 26 Jan 2023 14:25

Instrument :

MSVOA_N

ClientSampleId :

PB150465ZHE#03

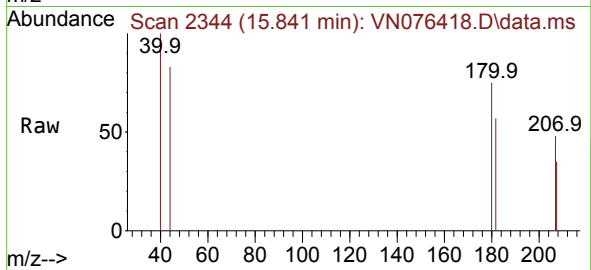

Tgt Ion:180 Resp: 509

Ion Ratio Lower Upper

180 100

182 113.0 47.5 142.5

145 0.0 15.9 47.6#

