

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012623\
 Data File : VN076421.D
 Acq On : 26 Jan 2023 15:37
 Operator : JC\MD
 Sample : 01270-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 JC-1-012323


Quant Time: Jan 27 00:37:16 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 17 03:59:22 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	383737	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	639645	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	579824	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	230947	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	232946	54.216	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 108.440%	
35) Dibromofluoromethane	8.171	113	198184	49.531	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 99.060%	
50) Toluene-d8	10.571	98	762904	51.628	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 103.260%	
62) 4-Bromofluorobenzene	12.853	95	243948	50.569	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 101.140%	
Target Compounds						
					Qvalue	
5) Bromomethane	2.977	94	866	0.212	ug/l #	52
11) Tert butyl alcohol	5.536	59	1876	3.264	ug/l #	72
16) Acetone	4.448	43	37141	26.900	ug/l	92
18) Methyl Acetate	5.047	43	4472	0.958	ug/l #	69
20) Methylene Chloride	5.300	84	15790	3.312	ug/l #	90
25) 2-Butanone	7.500	43	9561	4.545	ug/l	88
29) Tetrahydrofuran	7.859	42	676	0.521	ug/l #	31
31) Cyclohexane	8.230	56	8636	1.308	ug/l #	37
36) 1,1-Dichloropropene	8.230	75	30571	5.377	ug/l #	49
37) Ethyl Acetate	7.565	43	37915	8.344	ug/l	96
38) Carbon Tetrachloride	8.230	117	40855	6.444	ug/l #	17
42) 1,2-Dichloroethane	8.683	62	1863	0.320	ug/l #	73
43) Isopropyl Acetate	8.694	43	264687	35.677	ug/l #	78
45) 1,2-Dichloropropane	9.741	63	2387	0.586	ug/l #	42
48) Methyl methacrylate	9.665	41	5453	1.553	ug/l #	37
49) 1,4-Dioxane	9.753	88	85	1.147	ug/l #	1
51) 4-Methyl-2-Pentanone	10.447	43	15796	3.627	ug/l #	74
52) Toluene	10.629	92	3528	0.310	ug/l	95
53) t-1,3-Dichloropropene	10.724	75	1328	0.234	ug/l #	45
54) cis-1,3-Dichloropropene	10.359	75	74771	11.438	ug/l #	68
56) Ethyl methacrylate	10.988	69	2384	0.425	ug/l #	1
57) 1,3-Dichloropropane	11.206	76	9620	1.362	ug/l #	42
59) 2-Hexanone	11.177	43	160154	50.746	ug/l #	21
71) Bromoform	12.853	173	1715	0.521	ug/l #	1
74) N-amyl acetate	12.471	43	3575	0.696	ug/l #	37
76) 1,2,3-Trichloropropane	12.853	75	131544	30.904	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	131544	94.769	ug/l #	11
93) 1,2,4-Trichlorobenzene	15.394	180	144	1.340	ug/l #	75
95) Naphthalene	15.635	128	2333	2.026	ug/l #	76
96) 1,2,3-Trichlorobenzene	15.841	180	78	1.174	ug/l #	73

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jan 27 00:37:16 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 17 03:59:22 2023
Response via : Initial Calibration







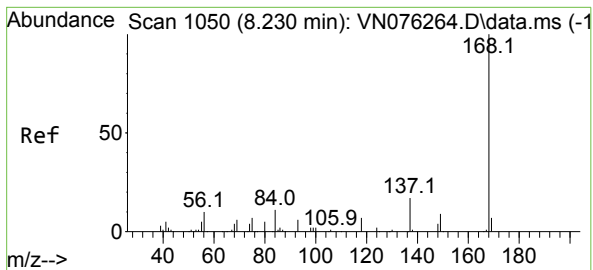

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.000 min
Lab File: VN076421.D
Acq: 26 Jan 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
JC-1-012323


Tgt Ion:168 Resp: 383737
Ion Ratio Lower Upper
168 100
99 58.4 41.6 62.4

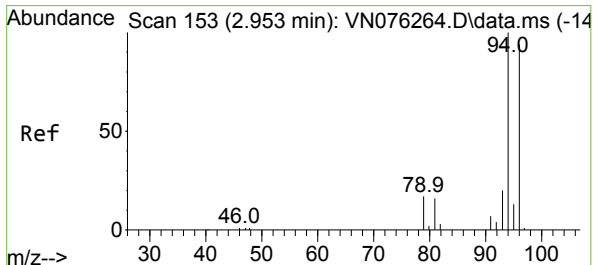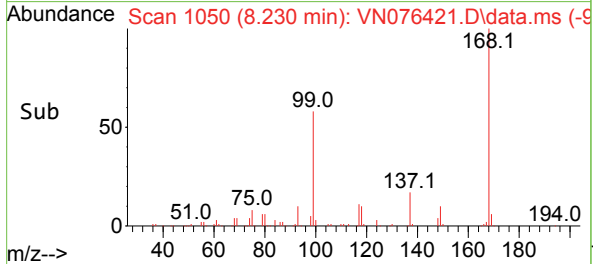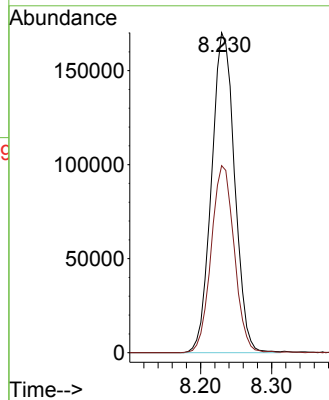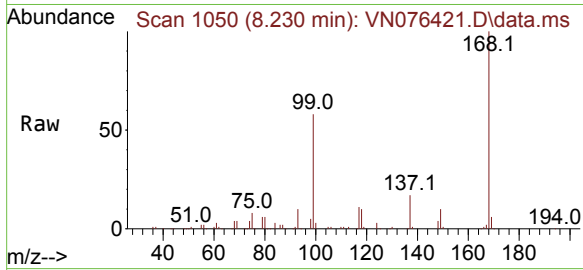

#5
Bromomethane
Concen: 0.212 ug/l
RT: 2.977 min Scan# 157
Delta R.T. 0.024 min
Lab File: VN076421.D
Acq: 26 Jan 2023 15:37

Tgt Ion: 94 Resp: 866
Ion Ratio Lower Upper
94 100
96 47.4 75.1 112.7#


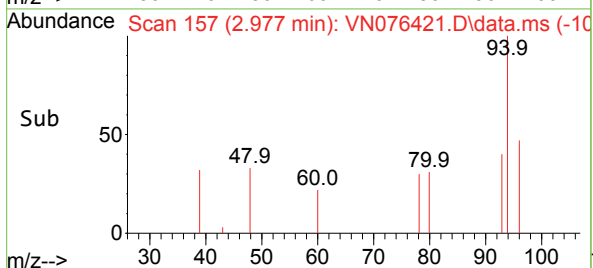
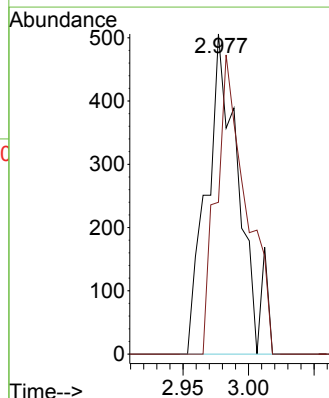
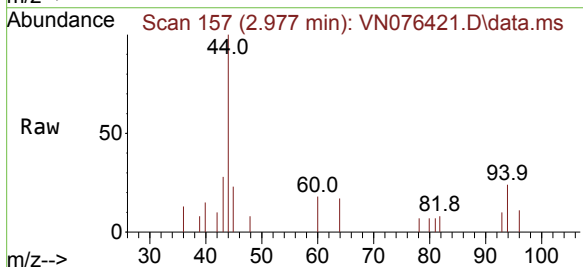




#11
Tert butyl alcohol
Concen: 3.264 ug/l
RT: 5.536 min Scan# 591
Delta R.T. 0.006 min
Lab File: VN076421.D
Acq: 26 Jan 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
JC-1-012323


Tgt Ion: 59 Resp: 1876
Ion Ratio Lower Upper
59 100
57 0.0 8.5 12.7#



#16
Acetone
Concen: 26.900 ug/l
RT: 4.448 min Scan# 407
Delta R.T. 0.006 min
Lab File: VN076421.D
Acq: 26 Jan 2023 15:37

Tgt Ion: 43 Resp: 37141
Ion Ratio Lower Upper
43 100
58 28.8 26.7 40.1









#18
Methyl Acetate
Concen: 0.958 ug/l
RT: 5.047 min Scan# 509
Delta R.T. 0.011 min
Lab File: VN076421.D
Acq: 26 Jan 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
JC-1-012323


Tgt Ion: 43 Resp: 4472
Ion Ratio Lower Upper
43 100
74 12.7 23.3 34.9#

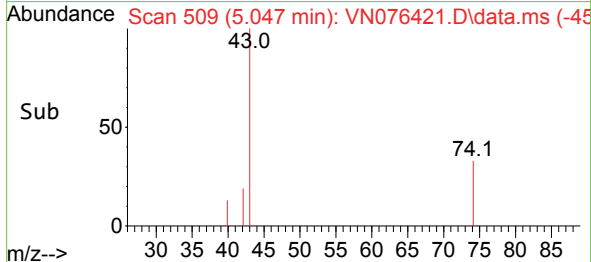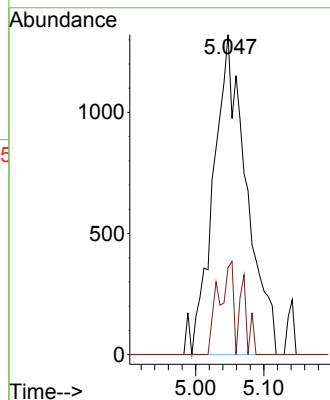

#20
Methylene Chloride
Concen: 3.312 ug/l
RT: 5.300 min Scan# 552
Delta R.T. 0.011 min
Lab File: VN076421.D
Acq: 26 Jan 2023 15:37

Tgt Ion: 84 Resp: 15790
Ion Ratio Lower Upper
84 100
49 101.2 84.5 126.7
51 24.1 26.0 39.0#
86 51.6 52.0 78.0#

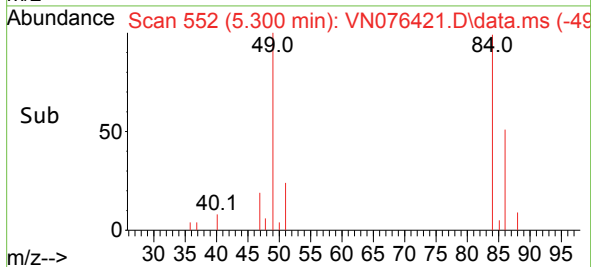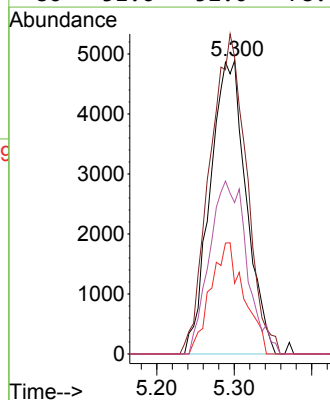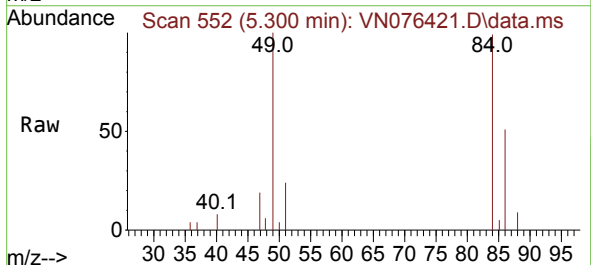

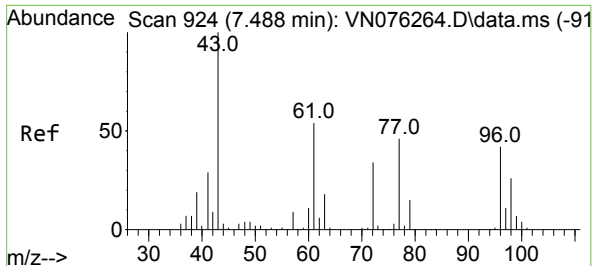

#25

2-Butanone

Concen: 4.545 ug/l

RT: 7.500 min Scan# 91

Delta R.T. 0.012 min

Lab File: VN076421.D

Acq: 26 Jan 2023 15:37

Instrument :

MSVOA_N

ClientSampleId :





JC-1-012323

Tgt Ion: 43 Resp: 9561

Ion Ratio Lower Upper

43 100

72 27.5 27.4 41.2

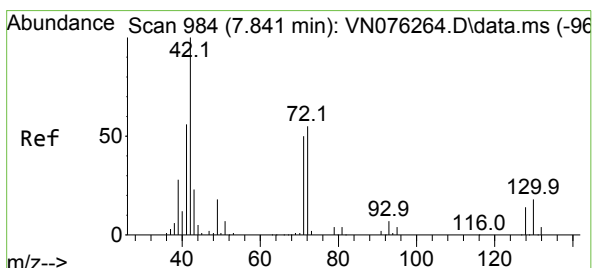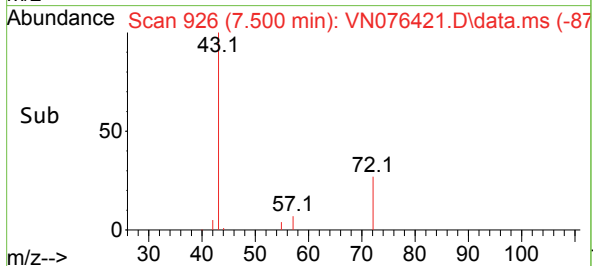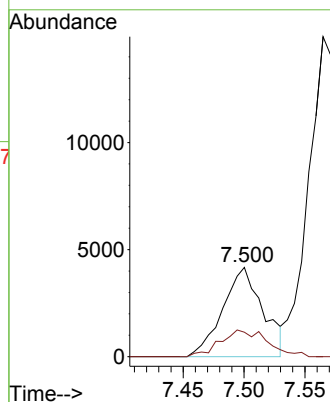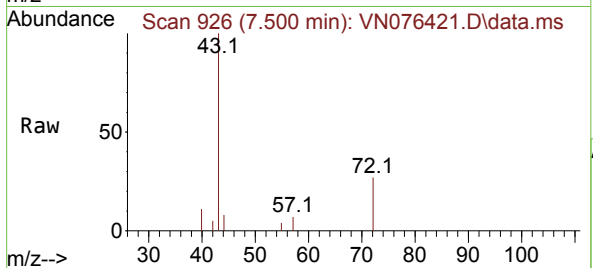

#29

Tetrahydrofuran

Concen: 0.521 ug/l

RT: 7.859 min Scan# 987

Delta R.T. 0.018 min

Lab File: VN076421.D

Acq: 26 Jan 2023 15:37




Tgt Ion: 42 Resp: 676


Ion Ratio Lower Upper

42 100

72 8.1 44.0 66.0#

71 0.0 41.1 61.7#


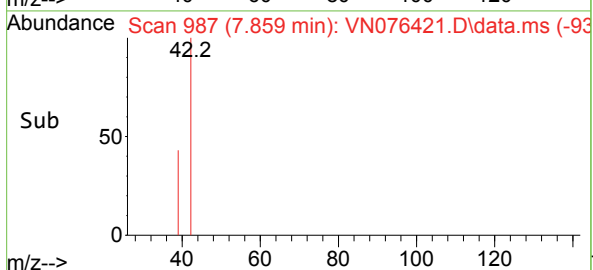
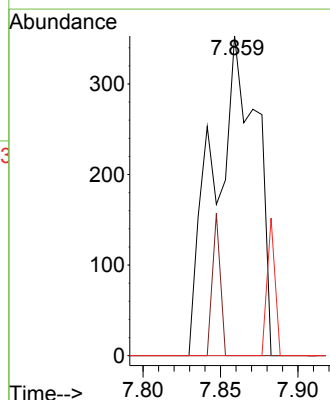
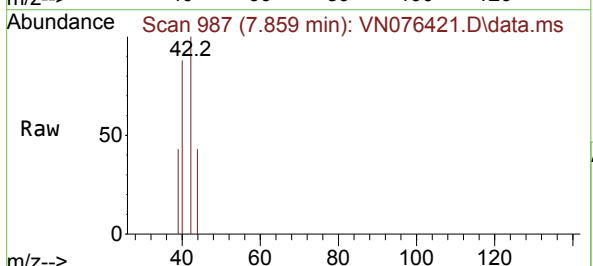




#31
Cyclohexane
Concen: 1.308 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.029 min
Lab File: VN076421.D
Acq: 26 Jan 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
JC-1-012323


Tgt Ion: 56 Resp: 8636
Ion Ratio Lower Upper
56 100
69 146.6 25.8 38.8#
84 115.7 79.0 118.4

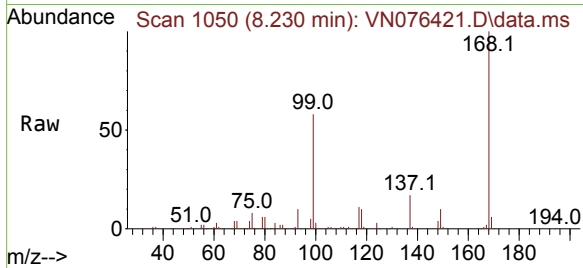

#33
1,2-Dichloroethane-d4
Concen: 54.216 ug/l
RT: 8.583 min Scan# 1110
Delta R.T. 0.001 min
Lab File: VN076421.D
Acq: 26 Jan 2023 15:37

Tgt Ion: 65 Resp: 232946
Ion Ratio Lower Upper
65 100
67 50.9 0.0 104.6




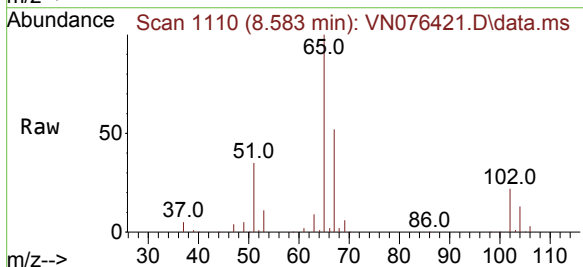




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 1199
Delta R.T. 0.000 min
Lab File: VN076421.D
Acq: 26 Jan 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
JC-1-012323


Tgt Ion:114 Resp: 639645
Ion Ratio Lower Upper
114 100
63 19.5 0.0 35.8
88 16.3 0.0 28.0

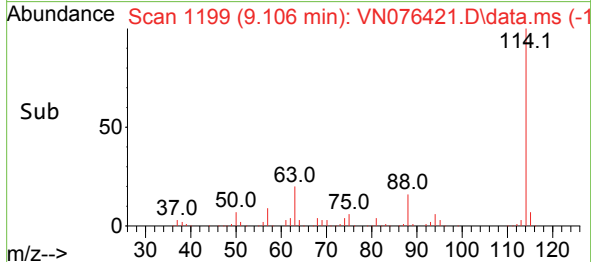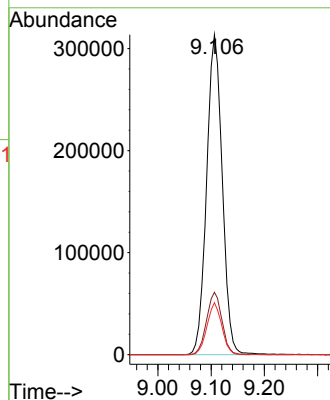

#35
Dibromofluoromethane
Concen: 49.531 ug/l
RT: 8.171 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VN076421.D
Acq: 26 Jan 2023 15:37

Tgt Ion:113 Resp: 198184
Ion Ratio Lower Upper
113 100
111 102.5 82.7 124.1
192 18.4 15.6 23.4

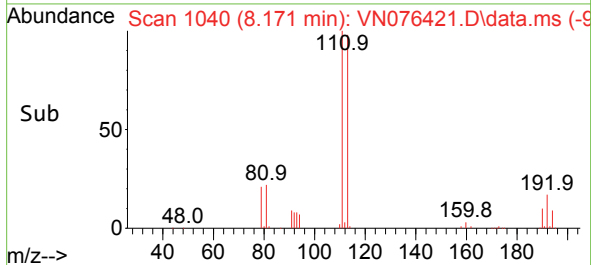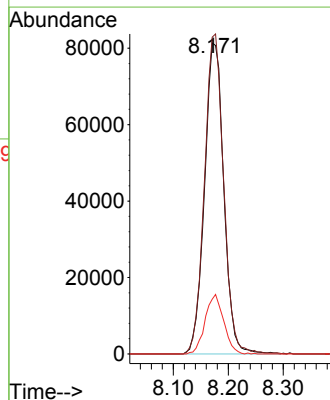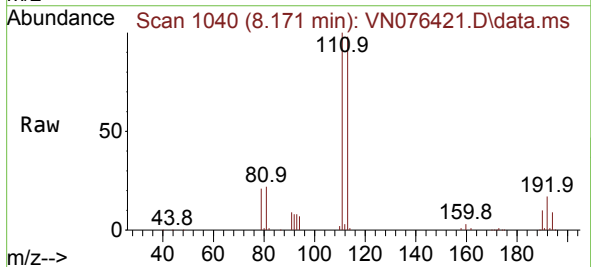



#36

1,1-Dichloropropene

Concen: 5.377 ug/l

RT: 8.230 min Scan# 1050

Delta R.T. -0.147 min

Lab File: VN076421.D

Acq: 26 Jan 2023 15:37

Instrument :

MSVOA_N

ClientSampleId :

JC-1-012323





Tgt Ion: 75 Resp: 30571

Ion Ratio Lower Upper

75 100

110 9.9 18.8 56.3#

77 0.0 25.0 37.4#

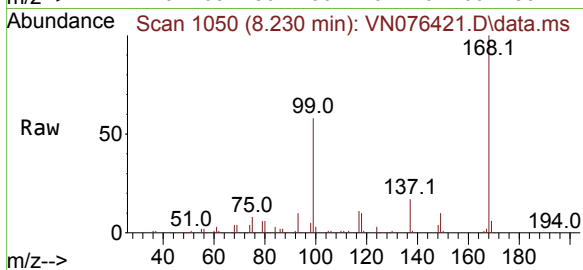

#37

Ethyl Acetate

Concen: 8.344 ug/l

RT: 7.565 min Scan# 937

Delta R.T. -0.000 min

Lab File: VN076421.D

Acq: 26 Jan 2023 15:37




Tgt Ion: 43 Resp: 37915


Ion Ratio Lower Upper

43 100

61 15.7 11.1 16.7

70 11.4 10.0 15.0

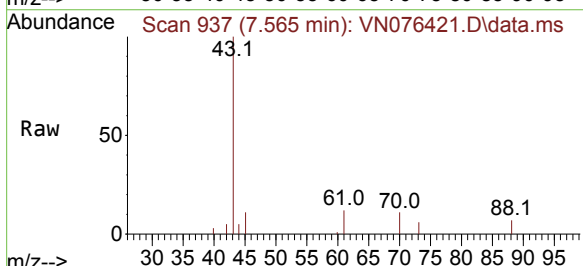



#38

Carbon Tetrachloride

Concen: 6.444 ug/l

RT: 8.230 min Scan# 110

Delta R.T. -0.135 min

Lab File: VN076421.D

Acq: 26 Jan 2023 15:37

Instrument :

MSVOA_N

ClientSampleId :

JC-1-012323





Tgt Ion:117 Resp: 40855

Ion Ratio Lower Upper

117 100

119 4.9 75.4 113.0#

121 0.0 24.2 36.2#

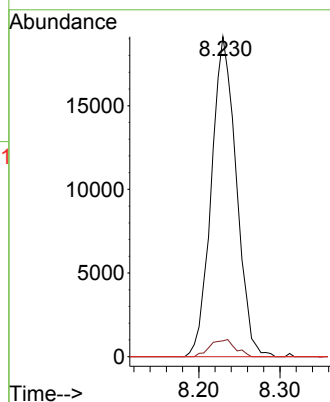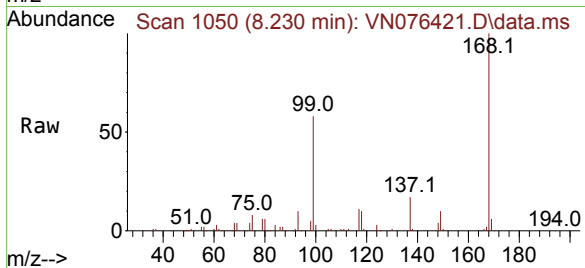

#42

1,2-Dichloroethane

Concen: 0.320 ug/l

RT: 8.683 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VN076421.D




Acq: 26 Jan 2023 15:37


Tgt Ion: 62 Resp: 1863

Ion Ratio Lower Upper

62 100

98 0.0 0.0 20.4

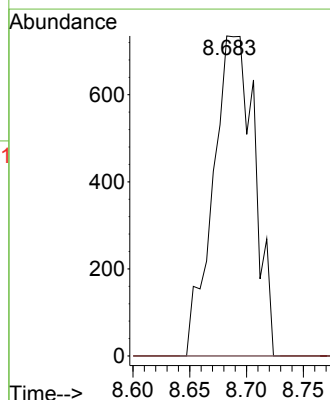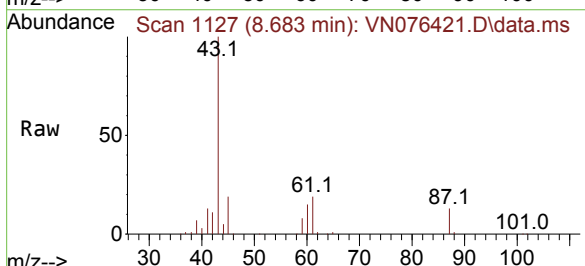

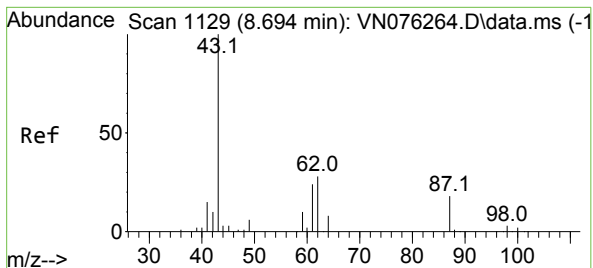

#43

Isopropyl Acetate

Concen: 35.677 ug/l

RT: 8.694 min Scan# 1129

Delta R.T. 0.000 min

Lab File: VN076421.D

Acq: 26 Jan 2023 15:37

Instrument :

MSVOA_N

ClientSampleId :

JC-1-012323





Tgt Ion: 43 Resp: 264687

Ion Ratio Lower Upper

43 100

61 15.2 23.5 35.3#

87 10.9 13.8 20.6#

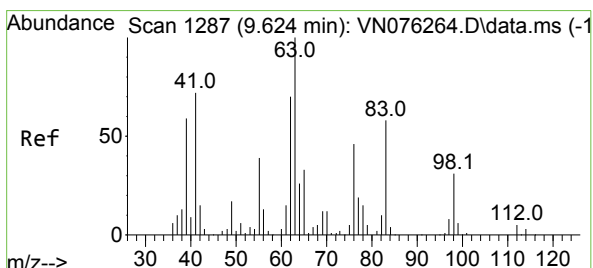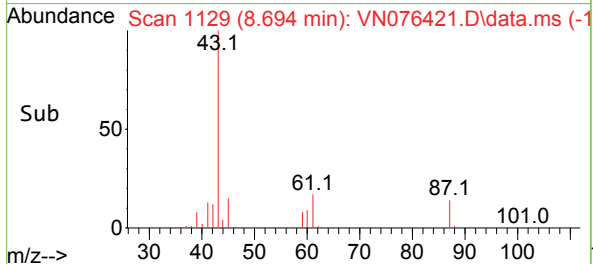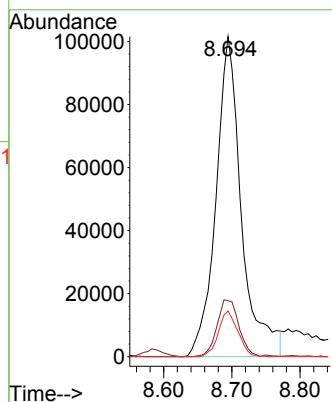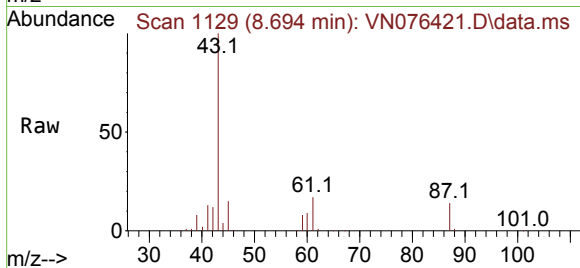

#45

1,2-Dichloropropane

Concen: 0.586 ug/l

RT: 9.741 min Scan# 1307

Delta R.T. 0.117 min

Lab File: VN076421.D




Acq: 26 Jan 2023 15:37


Tgt Ion: 63 Resp: 2387

Ion Ratio Lower Upper

63 100

65 0.0 26.4 39.6#


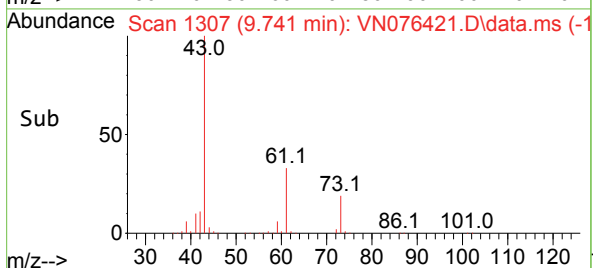

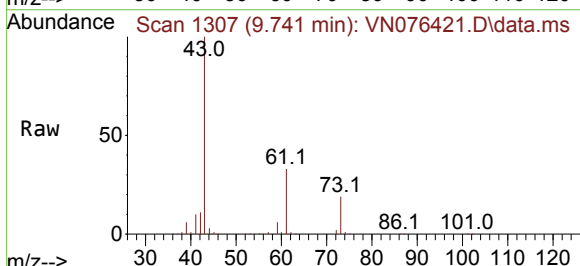




#48
Methyl methacrylate
Concen: 1.553 ug/l
RT: 9.665 min Scan# 11
Delta R.T. -0.017 min
Lab File: VN076421.D
Acq: 26 Jan 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
JC-1-012323


Tgt Ion: 41 Resp: 5453
Ion Ratio Lower Upper
41 100
69 0.0 80.8 121.2#
39 74.3 54.4 81.6

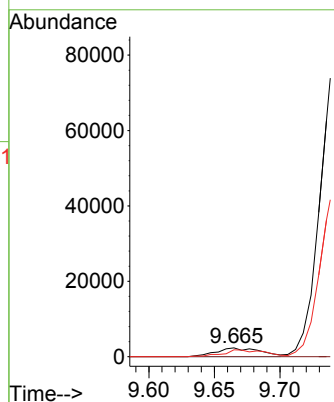

#49
1,4-Dioxane
Concen: 1.147 ug/l
RT: 9.753 min Scan# 1309
Delta R.T. 0.053 min
Lab File: VN076421.D
Acq: 26 Jan 2023 15:37

Tgt Ion: 88 Resp: 85
Ion Ratio Lower Upper
88 100
43 1883436.5 18.1 27.1#
58 9177.6 46.5 69.7#

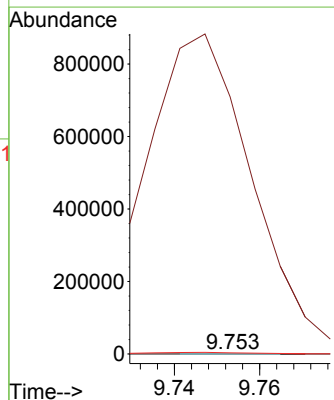



#50

Toluene-d8

Concen: 51.628 ug/l

RT: 10.571 min Scan# 1448

Delta R.T. -0.000 min

Lab File: VN076421.D

Acq: 26 Jan 2023 15:37

Instrument :

MSVOA_N

ClientSampleId :





JC-1-012323

Tgt Ion: 98 Resp: 762904

Ion Ratio Lower Upper

98 100

100 65.2 52.2 78.4

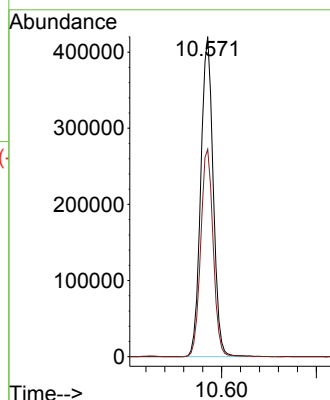

#51

4-Methyl-2-Pentanone

Concen: 3.627 ug/l

RT: 10.447 min Scan# 1427

Delta R.T. 0.000 min

Lab File: VN076421.D




Acq: 26 Jan 2023 15:37


Tgt Ion: 43 Resp: 15796

Ion Ratio Lower Upper

43 100

58 27.1 35.1 52.7#



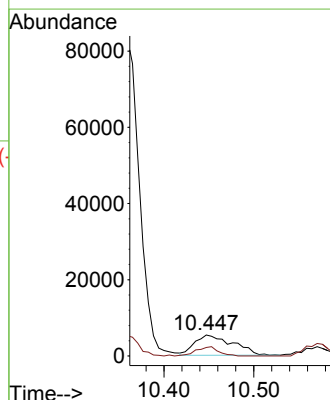





#52
Toluene
Concen: 0.310 ug/l
RT: 10.629 min Scan# 1458
Delta R.T. 0.000 min
Lab File: VN076421.D
Acq: 26 Jan 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
JC-1-012323


Tgt Ion: 92 Resp: 3528
Ion Ratio Lower Upper
92 100
91 163.6 136.6 205.0



#53
t-1,3-Dichloropropene
Concen: 0.234 ug/l
RT: 10.724 min Scan# 1474
Delta R.T. -0.111 min
Lab File: VN076421.D
Acq: 26 Jan 2023 15:37

Tgt Ion: 75 Resp: 1328
Ion Ratio Lower Upper
75 100
77 1.2 25.8 38.6#




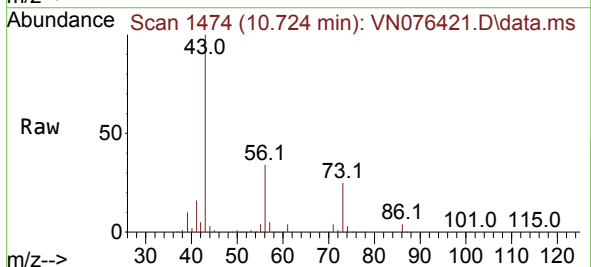




#54
 cis-1,3-Dichloropropene
 Concen: 11.438 ug/l
 RT: 10.359 min Scan# 14
 Delta R.T. 0.047 min
 Lab File: VN076421.D
 Acq: 26 Jan 2023 15:37




Instrument :
 MSVOA_N
 ClientSampleId :
 JC-1-012323


Tgt Ion: 75 Resp: 74771
 Ion Ratio Lower Upper
 75 100
 77 0.5 26.5 39.7#
 39 37.1 37.1 55.7

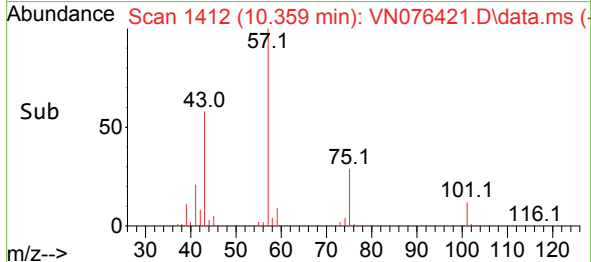

#56
 Ethyl methacrylate
 Concen: 0.425 ug/l
 RT: 10.988 min Scan# 1519
 Delta R.T. 0.112 min
 Lab File: VN076421.D
 Acq: 26 Jan 2023 15:37

Tgt Ion: 69 Resp: 2384
 Ion Ratio Lower Upper
 69 100
 41 4679.1 45.3 67.9#
 39 2203.9 29.3 43.9#

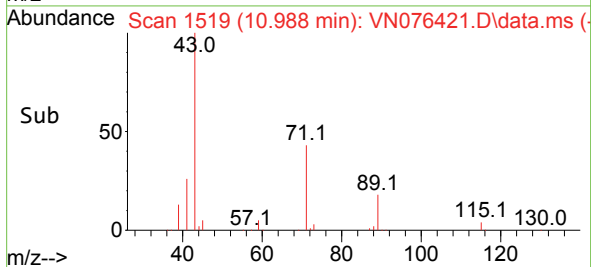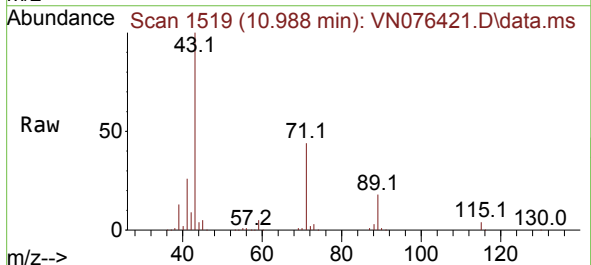

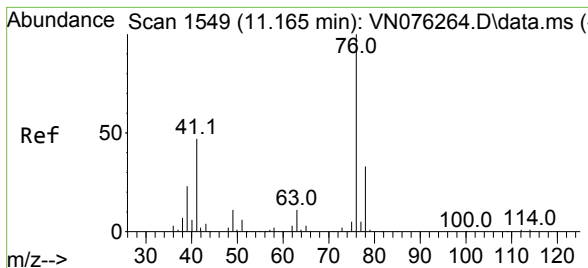

#57

1,3-Dichloropropane

Concen: 1.362 ug/l

RT: 11.206 min Scan# 1556

Delta R.T. 0.041 min

Lab File: VN076421.D

Acq: 26 Jan 2023 15:37

Instrument :

MSVOA_N

ClientSampleId :





JC-1-012323

Tgt Ion: 76 Resp: 9620

Ion Ratio Lower Upper

76 100

78 0.0 26.4 39.6#

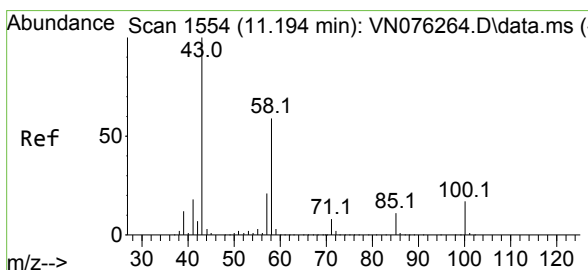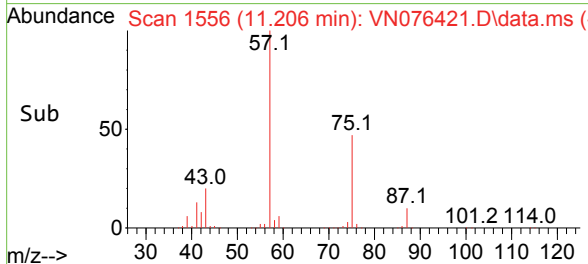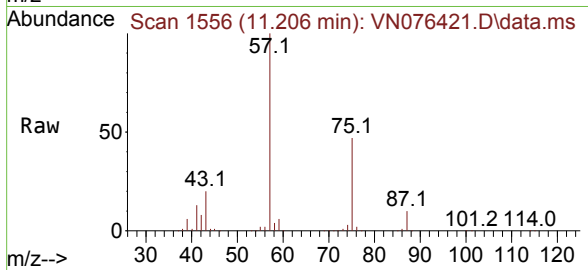

#59

2-Hexanone

Concen: 50.746 ug/l

RT: 11.177 min Scan# 1551

Delta R.T. -0.018 min

Lab File: VN076421.D




Acq: 26 Jan 2023 15:37


Tgt Ion: 43 Resp: 160154

Ion Ratio Lower Upper

43 100

58 0.0 30.1 90.3#


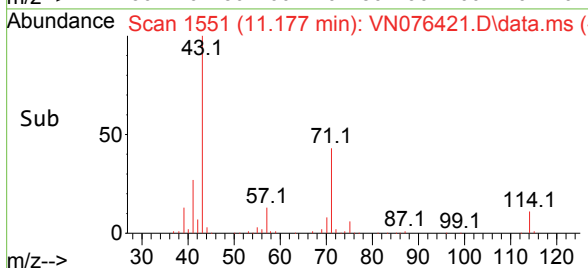

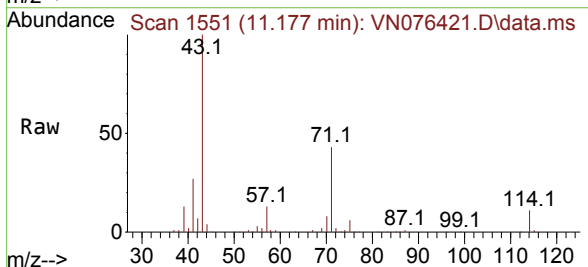




#62
4-Bromofluorobenzene
Concen: 50.569 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.006 min
Lab File: VN076421.D
Acq: 26 Jan 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
JC-1-012323


Tgt Ion: 95 Resp: 243948
Ion Ratio Lower Upper
95 100
174 80.3 0.0 174.6
176 78.1 0.0 167.8



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1669
Delta R.T. 0.006 min
Lab File: VN076421.D
Acq: 26 Jan 2023 15:37

Tgt Ion: 117 Resp: 579824
Ion Ratio Lower Upper
117 100
82 53.0 42.2 63.2
119 31.3 26.9 40.3





#71

Bromoform

Concen: 0.521 ug/l

RT: 12.853 min Scan# 1836

Delta R.T. 0.271 min

Lab File: VN076421.D

Acq: 26 Jan 2023 15:37

Instrument :

MSVOA_N

ClientSampleId :

JC-1-012323





Tgt Ion:173 Resp: 1715

Ion Ratio Lower Upper

173 100

175 733.8 24.1 72.4#

254 0.0 0.0 0.0



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 1996

Delta R.T. -0.000 min

Lab File: VN076421.D

Acq: 26 Jan 2023 15:37




Tgt Ion:152 Resp: 230947


Ion Ratio Lower Upper

152 100

115 59.9 29.6 88.9

150 157.8 0.0 351.4

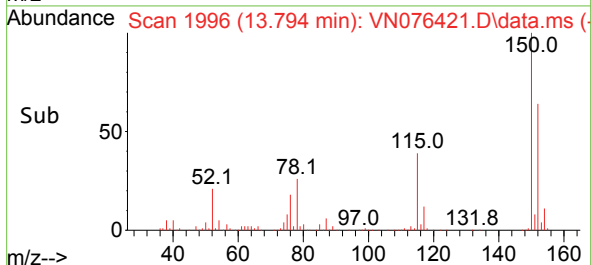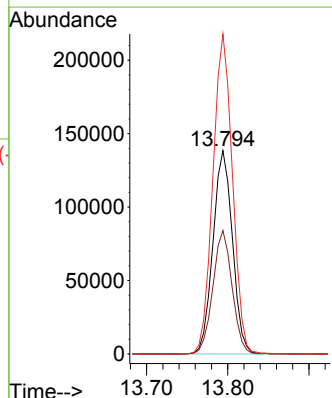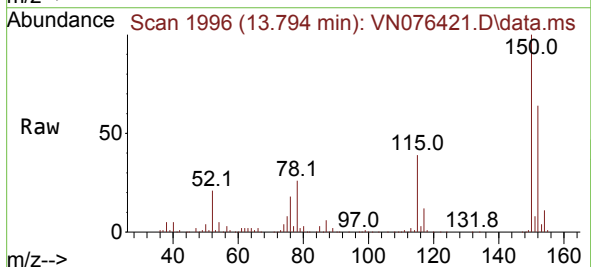



#74

N-amy1 acetate

Concen: 0.696 ug/l

RT: 12.471 min Scan# 1

Delta R.T. -0.023 min

Lab File: VN076421.D

Acq: 26 Jan 2023 15:37

Instrument :

MSVOA_N

ClientSampleId :

JC-1-012323

Tgt Ion: 43 Resp: 3575





Ion Ratio Lower Upper

43 100

70 0.0 41.2 61.8#

55 0.0 21.0 31.6#

61 0.0 21.6 32.4#



#76

1,2,3-Trichloropropane

Concen: 30.904 ug/l

RT: 12.853 min Scan# 1836

Delta R.T. -0.141 min

Lab File: VN076421.D




Acq: 26 Jan 2023 15:37


Tgt Ion: 75 Resp: 131544

Ion Ratio Lower Upper

75 100

77 1.0 75.2 225.6#




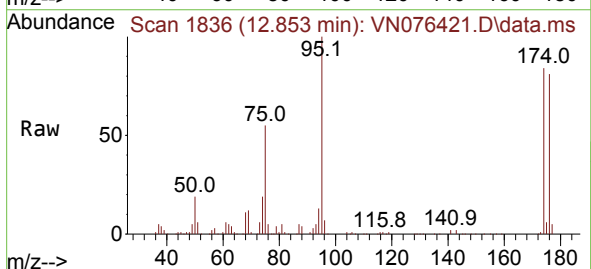




#81
trans-1,4-Dichloro-2-butene
Concen: 94.769 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.118 min
Lab File: VN076421.D
Acq: 26 Jan 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
JC-1-012323


Tgt Ion: 75 Resp: 131544
Ion Ratio Lower Upper
75 100
53 0.0 75.8 113.8#
89 0.0 37.0 55.6#

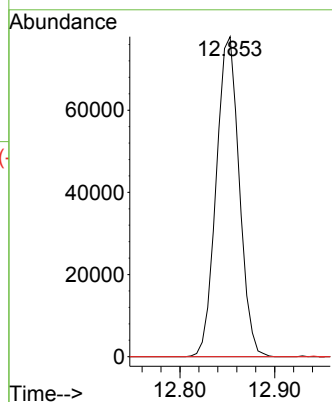

#93
1,2,4-Trichlorobenzene
Concen: 1.340 ug/l
RT: 15.394 min Scan# 2268
Delta R.T. -0.000 min
Lab File: VN076421.D
Acq: 26 Jan 2023 15:37

Tgt Ion: 180 Resp: 144
Ion Ratio Lower Upper
180 100
182 108.3 47.0 141.2
145 0.0 15.2 45.5#

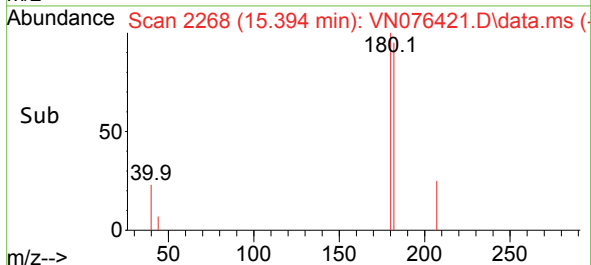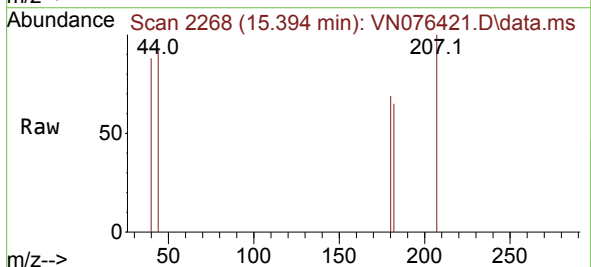

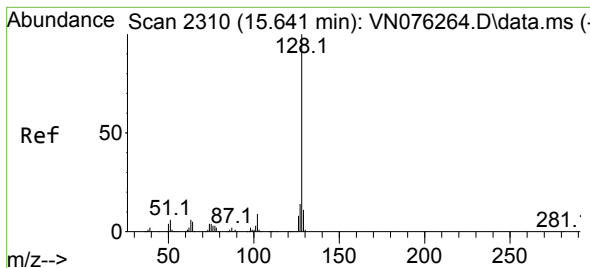

#95

Naphthalene

Concen: 2.026 ug/l

RT: 15.635 min Scan# 2309

Delta R.T. -0.006 min

Lab File: VN076421.D

Acq: 26 Jan 2023 15:37

Instrument :

MSVOA_N

ClientSampleId :

JC-1-012323





Tgt Ion:128 Resp: 2333

Ion Ratio Lower Upper

128 100

127 5.0 10.3 15.5#

129 0.0 8.6 13.0#

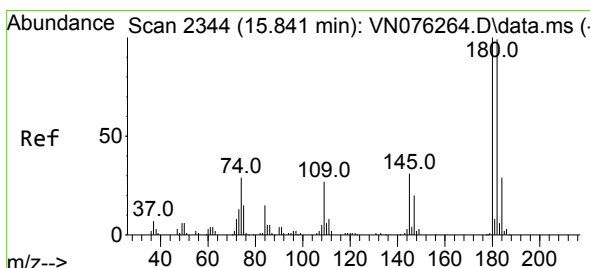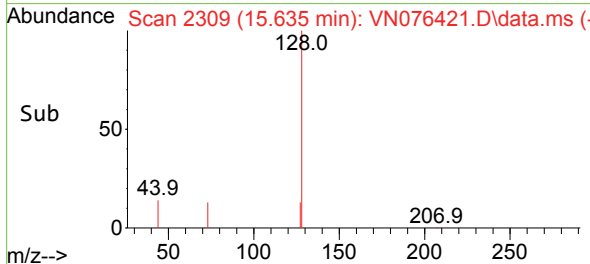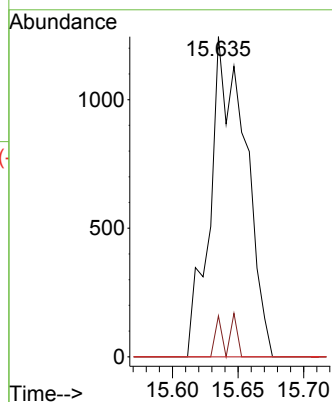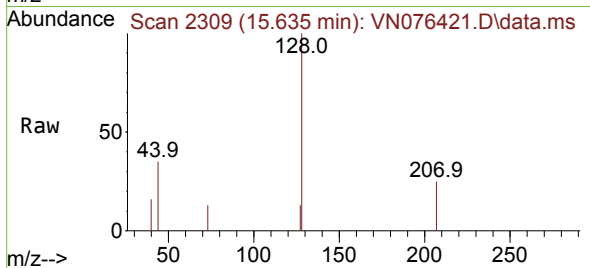

#96

1,2,3-Trichlorobenzene

Concen: 1.174 ug/l

RT: 15.841 min Scan# 2344

Delta R.T. -0.000 min

Lab File: VN076421.D

Acq: 26 Jan 2023 15:37

Tgt Ion:180 Resp: 78

Ion Ratio Lower Upper

180 100

182 111.5 47.5 142.5

145 0.0 15.9 47.6#

