

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012623\
 Data File : VN076423.D
 Acq On : 26 Jan 2023 16:25
 Operator : JC\MD
 Sample : 01283-05
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MH-10

Quant Time: Jan 27 00:38:20 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 17 03:59:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	386263	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	650755	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	596919	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	236260	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	234471	54.214	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 108.420%			
35) Dibromofluoromethane	8.171	113	197591	48.539	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 97.080%			
50) Toluene-d8	10.571	98	778961	51.814	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 103.620%			
62) 4-Bromofluorobenzene	12.853	95	254536	51.863	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 103.720%			
Target Compounds						Qvalue
11) Tert butyl alcohol	5.542	59	1389	2.401	ug/l #	72
13) Acrolein	4.200	56	213	0.308	ug/l #	15
16) Acetone	4.448	43	37944	27.302	ug/l	97
18) Methyl Acetate	5.048	43	4272	0.909	ug/l #	88
20) Methylene Chloride	5.289	84	16106	3.364	ug/l	97
25) 2-Butanone	7.506	43	9791	4.624	ug/l	88
29) Tetrahydrofuran	7.859	42	740	0.566	ug/l #	31
31) Cyclohexane	8.230	56	8928	1.344	ug/l #	29
36) 1,1-Dichloropropene	8.230	75	29667	5.129	ug/l #	48
37) Ethyl Acetate	7.571	43	37019	8.010	ug/l	98
38) Carbon Tetrachloride	8.236	117	41204	6.388	ug/l #	17
42) 1,2-Dichloroethane	8.688	62	1632	0.276	ug/l #	73
43) Isopropyl Acetate	8.694	43	330841	43.833	ug/l #	73
45) 1,2-Dichloropropane	9.747	63	2445	0.590	ug/l #	42
48) Methyl methacrylate	9.665	41	5702	1.596	ug/l #	39
49) 1,4-Dioxane	9.753	88	258	3.422	ug/l #	1
51) 4-Methyl-2-Pentanone	10.447	43	17128	3.866	ug/l #	71
52) Toluene	10.630	92	2396	0.207	ug/l	77
53) t-1,3-Dichloropropene	10.735	75	1495	0.259	ug/l #	45
54) cis-1,3-Dichloropropene	10.365	75	80019	12.032	ug/l #	62
56) Ethyl methacrylate	10.994	69	2411	0.422	ug/l #	1
57) 1,3-Dichloropropane	11.206	76	10259	1.428	ug/l #	42
59) 2-Hexanone	11.171	43	188662	58.758	ug/l #	21
71) Bromoform	12.847	173	2068	0.610	ug/l #	1
74) N-amyl acetate	12.494	43	2187	0.416	ug/l #	39
76) 1,2,3-Trichloropropane	12.853	75	135562	31.139	ug/l #	1
77) Bromobenzene	12.971	156	67	Below Cal	#	61
81) trans-1,4-Dichloro-2-b...	12.853	75	135562	95.468	ug/l #	11
93) 1,2,4-Trichlorobenzene	15.400	180	64	1.320	ug/l #	1
95) Naphthalene	15.635	128	1100	1.925	ug/l #	81
96) 1,2,3-Trichlorobenzene	15.841	180	54	1.167	ug/l #	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012623\
Data File : VN076423.D
Acq On : 26 Jan 2023 16:25
Operator : JC\MD
Sample : 01283-05
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MH-10

Quant Time: Jan 27 00:38:20 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 17 03:59:22 2023
Response via : Initial Calibration




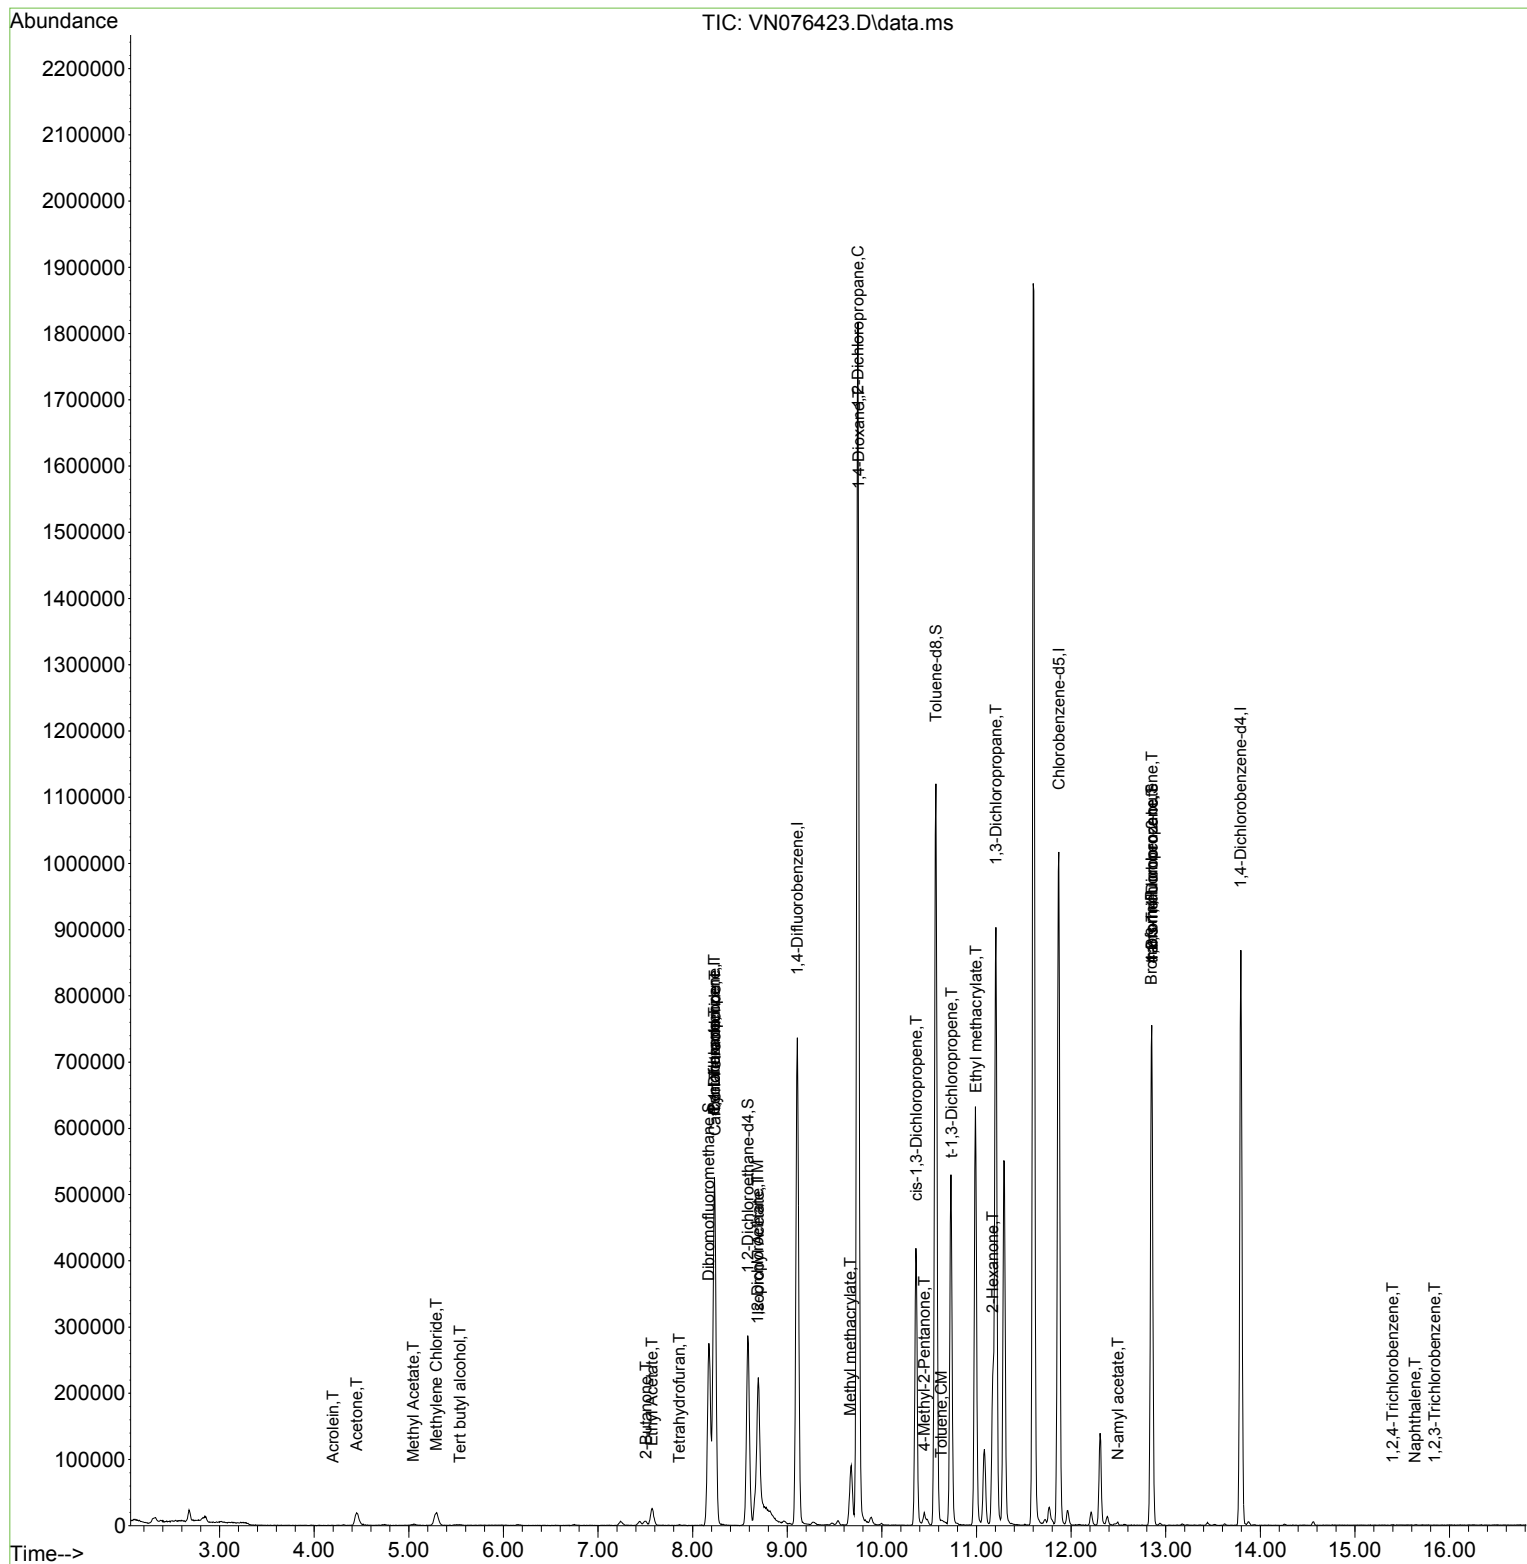




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.000 min
Lab File: VN076423.D
Acq: 26 Jan 2023 16:25




Instrument :
MSVOA_N
ClientSampleId :
MH-10


Tgt Ion:168 Resp: 386263
Ion Ratio Lower Upper
168 100
99 57.9 41.6 62.4

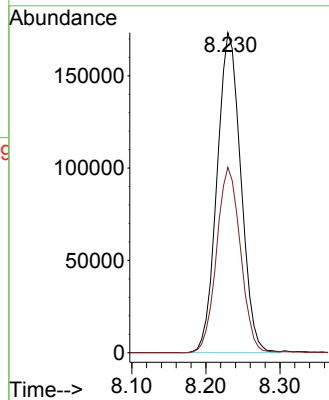

#11
Tert butyl alcohol
Concen: 2.401 ug/l
RT: 5.542 min Scan# 593
Delta R.T. 0.012 min
Lab File: VN076423.D
Acq: 26 Jan 2023 16:25

Tgt Ion: 59 Resp: 1389
Ion Ratio Lower Upper
59 100
57 0.0 8.5 12.7#

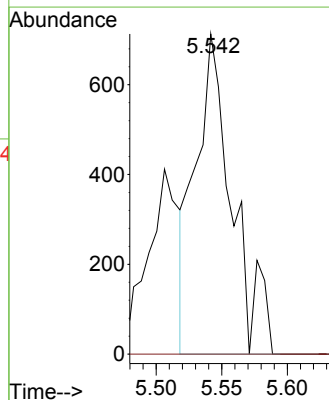



#13

Acrolein

Concen: 0.308 ug/l

RT: 4.200 min Scan# 30

Delta R.T. 0.011 min

Lab File: VN076423.D

Acq: 26 Jan 2023 16:25

Instrument :

MSVOA_N

ClientSampleId :





MH-10

Tgt Ion: 56 Resp: 213

Ion Ratio Lower Upper

56 100

55 0.0 55.8 83.6#



#16

Acetone

Concen: 27.302 ug/l

RT: 4.448 min Scan# 407

Delta R.T. 0.006 min

Lab File: VN076423.D




Acq: 26 Jan 2023 16:25


Tgt Ion: 43 Resp: 37944

Ion Ratio Lower Upper

43 100

58 34.8 26.7 40.1




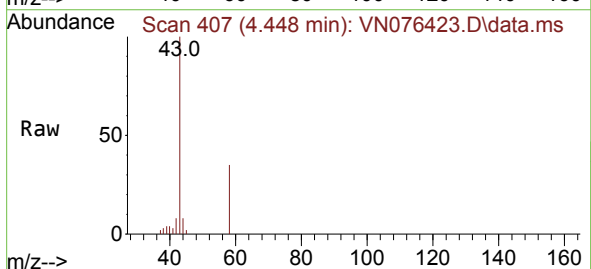




#18
Methyl Acetate
Concen: 0.909 ug/l
RT: 5.048 min Scan# 507
Delta R.T. 0.012 min
Lab File: VN076423.D
Acq: 26 Jan 2023 16:25




Instrument :
MSVOA_N
ClientSampleId :
MH-10


Tgt Ion: 43 Resp: 4272
Ion Ratio Lower Upper
43 100
74 22.5 23.3 34.9#

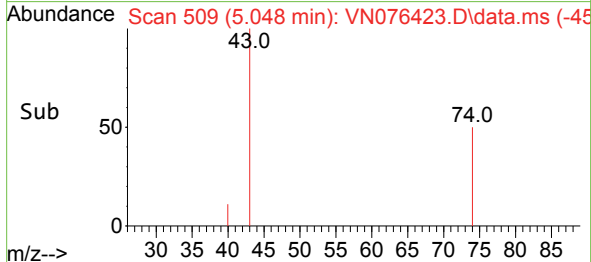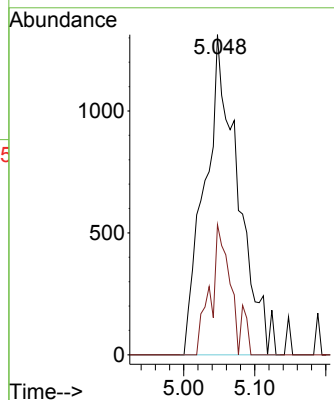

#20
Methylene Chloride
Concen: 3.364 ug/l
RT: 5.289 min Scan# 550
Delta R.T. -0.000 min
Lab File: VN076423.D
Acq: 26 Jan 2023 16:25

Tgt Ion: 84 Resp: 16106
Ion Ratio Lower Upper
84 100
49 101.4 84.5 126.7
51 35.7 26.0 39.0
86 64.8 52.0 78.0

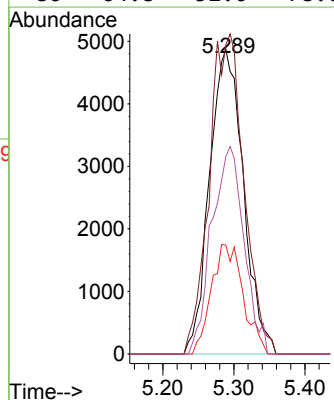

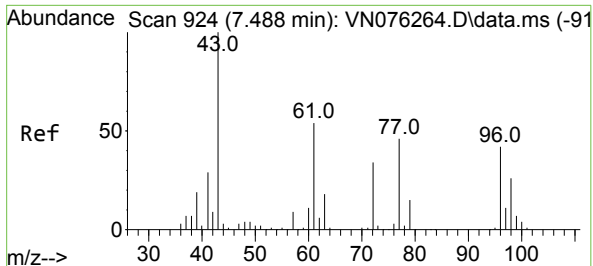

#25

2-Butanone

Concen: 4.624 ug/l

RT: 7.506 min Scan# 91

Delta R.T. 0.018 min

Lab File: VN076423.D

Acq: 26 Jan 2023 16:25

Instrument :

MSVOA_N

ClientSampleId :





MH-10

Tgt Ion: 43 Resp: 9791

Ion Ratio Lower Upper

43 100

72 27.5 27.4 41.2

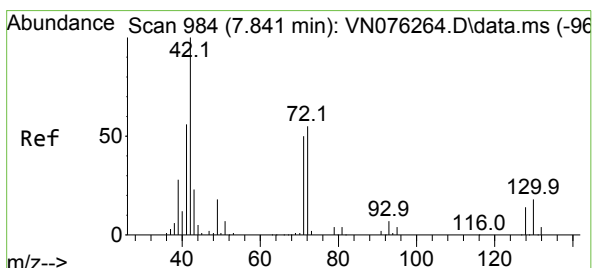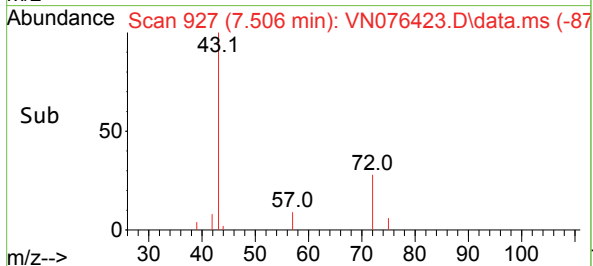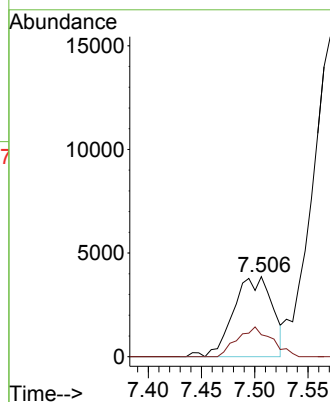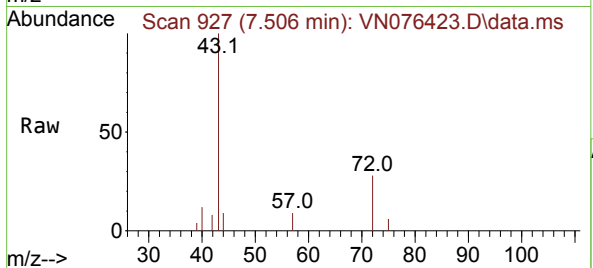

#29

Tetrahydrofuran

Concen: 0.566 ug/l

RT: 7.859 min Scan# 987

Delta R.T. 0.018 min

Lab File: VN076423.D

Acq: 26 Jan 2023 16:25




Tgt Ion: 42 Resp: 740


Ion Ratio Lower Upper

42 100

72 8.4 44.0 66.0#

71 0.0 41.1 61.7#


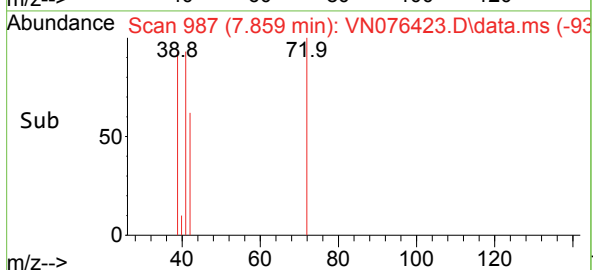
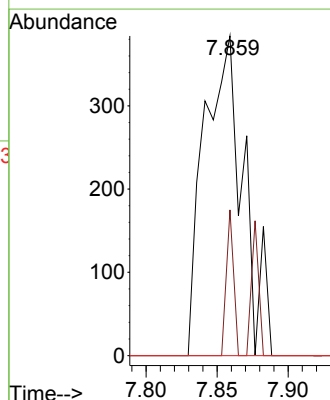
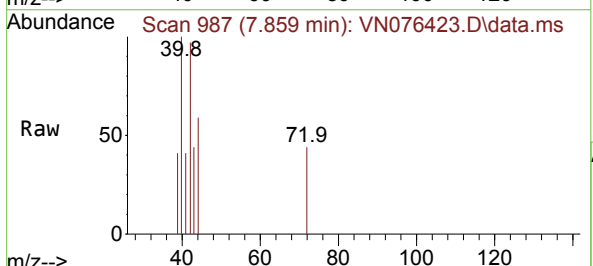




#31
Cyclohexane
Concen: 1.344 ug/l
RT: 8.230 min Scan# 1050
Delta R.T. -0.029 min
Lab File: VN076423.D
Acq: 26 Jan 2023 16:25




Instrument :
MSVOA_N
ClientSampleId :
MH-10


Tgt Ion: 56 Resp: 8928
Ion Ratio Lower Upper
56 100
69 149.7 25.8 38.8#
84 123.7 79.0 118.4#

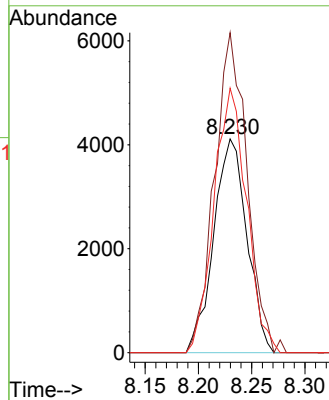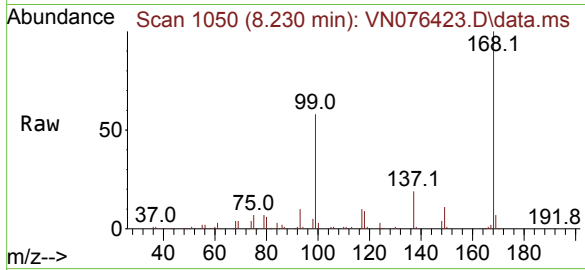

#33
1,2-Dichloroethane-d4
Concen: 54.214 ug/l
RT: 8.583 min Scan# 1110
Delta R.T. 0.001 min
Lab File: VN076423.D
Acq: 26 Jan 2023 16:25

Tgt Ion: 65 Resp: 234471
Ion Ratio Lower Upper
65 100
67 51.3 0.0 104.6

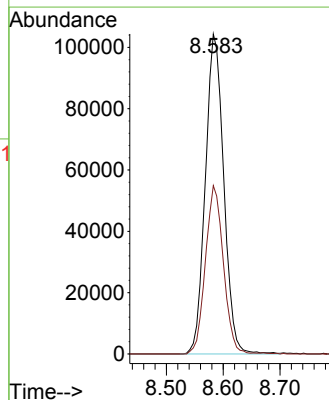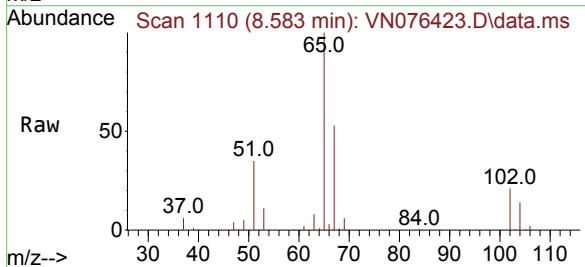



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. 0.000 min

Lab File: VN076423.D

Acq: 26 Jan 2023 16:25

Instrument :

MSVOA_N

ClientSampleId :

MH-10





Tgt Ion:114 Resp: 650755

Ion Ratio Lower Upper

114 100

63 18.8 0.0 35.8

88 15.1 0.0 28.0



#35

Dibromofluoromethane

Concen: 48.539 ug/l

RT: 8.171 min Scan# 1040

Delta R.T. -0.000 min

Lab File: VN076423.D

Acq: 26 Jan 2023 16:25




Tgt Ion:113 Resp: 197591


Ion Ratio Lower Upper

113 100

111 102.5 82.7 124.1

192 19.4 15.6 23.4


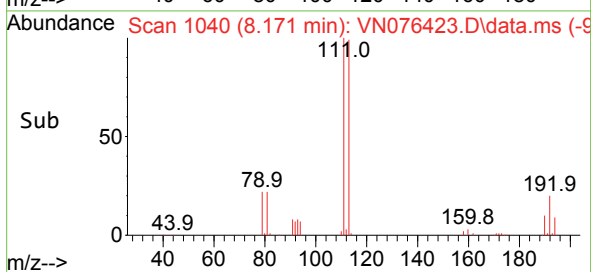






#36
1,1-Dichloropropene
Concen: 5.129 ug/l
RT: 8.230 min Scan# 1075
Delta R.T. -0.147 min
Lab File: VN076423.D
Acq: 26 Jan 2023 16:25




Instrument :
MSVOA_N
ClientSampleId :
MH-10


Tgt Ion: 75 Resp: 29667
Ion Ratio Lower Upper
75 100
110 8.6 18.8 56.3#
77 0.0 25.0 37.4#



#37
Ethyl Acetate
Concen: 8.010 ug/l
RT: 7.571 min Scan# 938
Delta R.T. 0.006 min
Lab File: VN076423.D
Acq: 26 Jan 2023 16:25

Tgt Ion: 43 Resp: 37019
Ion Ratio Lower Upper
43 100
61 15.4 11.1 16.7
70 12.8 10.0 15.0

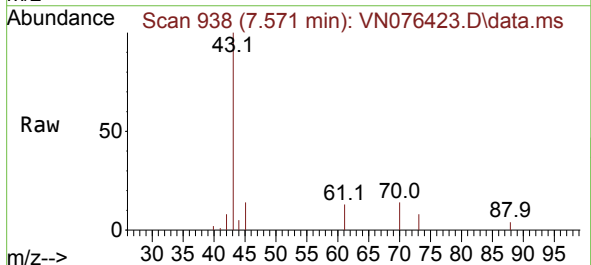

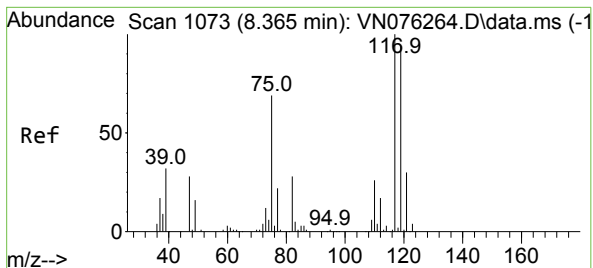

#38

Carbon Tetrachloride

Concen: 6.388 ug/l

RT: 8.236 min Scan# 110

Delta R.T. -0.129 min

Lab File: VN076423.D


Acq: 26 Jan 2023 16:25

Instrument :

MSVOA_N

ClientSampleId :

MH-10

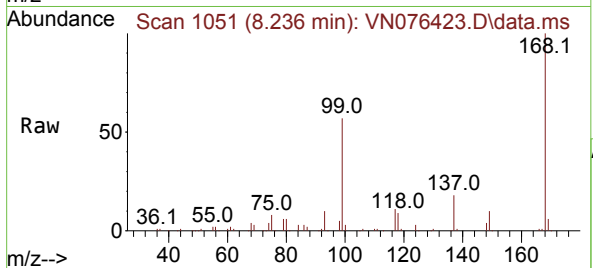




Tgt Ion:117 Resp: 41204

Ion Ratio Lower Upper

117 100

119 5.1 75.4 113.0#

121 0.0 24.2 36.2#

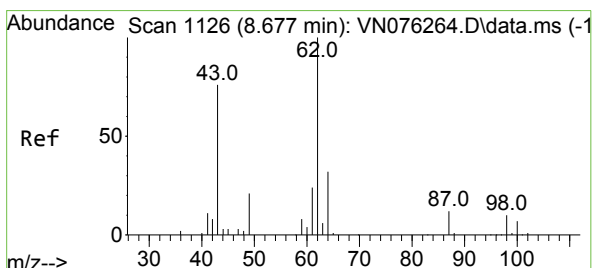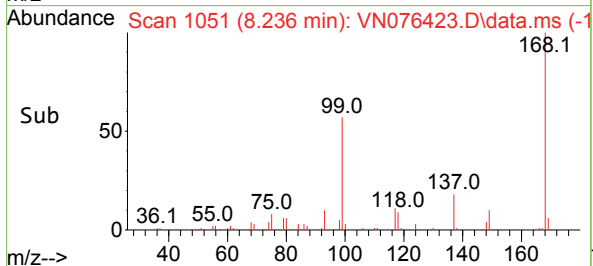

#42

1,2-Dichloroethane

Concen: 0.276 ug/l

RT: 8.688 min Scan# 1128

Delta R.T. 0.011 min

Lab File: VN076423.D




Acq: 26 Jan 2023 16:25


Tgt Ion: 62 Resp: 1632

Ion Ratio Lower Upper

62 100

98 0.0 0.0 20.4


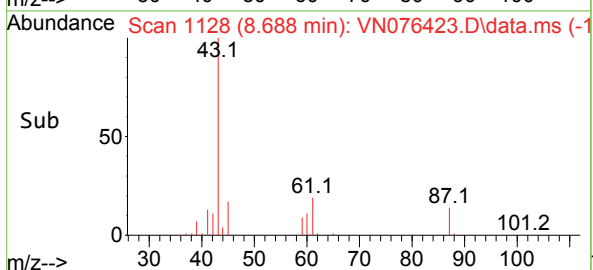

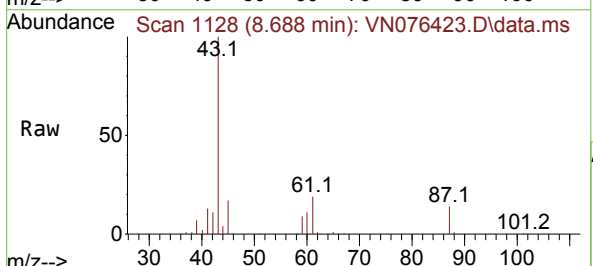




#43
Isopropyl Acetate
Concen: 43.833 ug/l
RT: 8.694 min Scan# 1129
Delta R.T. 0.000 min
Lab File: VN076423.D
Acq: 26 Jan 2023 16:25




Instrument :
MSVOA_N
ClientSampleId :
MH-10


Tgt Ion: 43 Resp: 330841
Ion Ratio Lower Upper
43 100
61 12.5 23.5 35.3#
87 9.2 13.8 20.6#

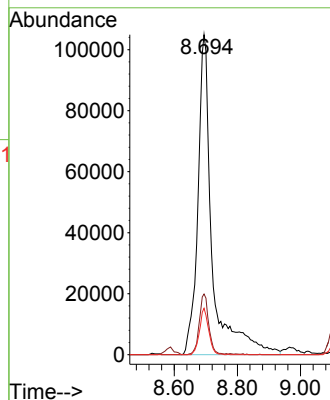

#45
1,2-Dichloropropane
Concen: 0.590 ug/l
RT: 9.747 min Scan# 1308
Delta R.T. 0.123 min
Lab File: VN076423.D
Acq: 26 Jan 2023 16:25

Tgt Ion: 63 Resp: 2445
Ion Ratio Lower Upper
63 100
65 0.0 26.4 39.6#



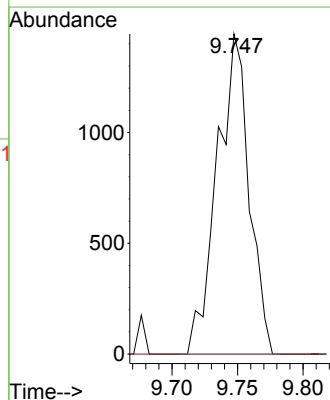





#48
Methyl methacrylate
Concen: 1.596 ug/l
RT: 9.665 min Scan# 11
Delta R.T. -0.017 min
Lab File: VN076423.D
Acq: 26 Jan 2023 16:25




Instrument :
MSVOA_N
ClientSampleId :
MH-10


Tgt Ion: 41 Resp: 5702
Ion Ratio Lower Upper
41 100
69 0.0 80.8 121.2#
39 66.6 54.4 81.6

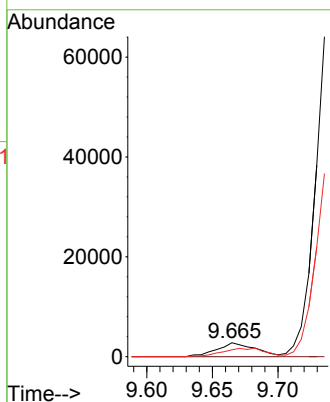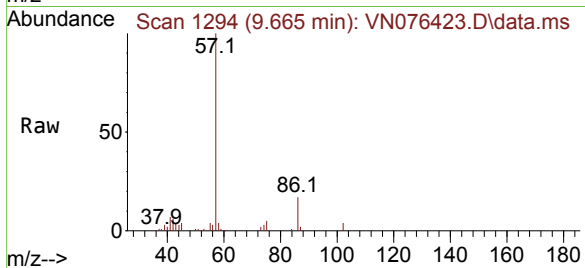

#49
1,4-Dioxane
Concen: 3.422 ug/l
RT: 9.753 min Scan# 1309
Delta R.T. 0.053 min
Lab File: VN076423.D
Acq: 26 Jan 2023 16:25

Tgt Ion: 88 Resp: 258
Ion Ratio Lower Upper
88 100
43 641419.4 18.1 27.1#
58 3106.2 46.5 69.7#



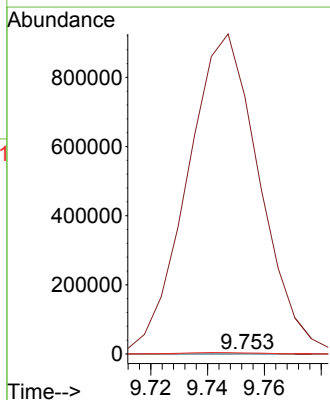
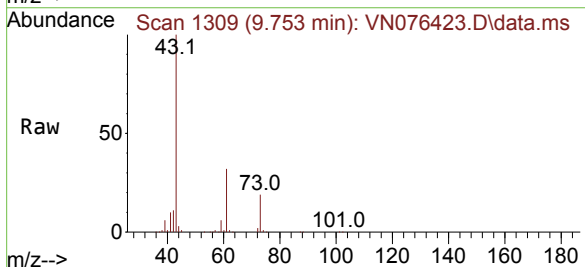




#50
Toluene-d8
Concen: 51.814 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN076423.D
Acq: 26 Jan 2023 16:25




Instrument :
MSVOA_N
ClientSampleId :
MH-10


Tgt Ion: 98 Resp: 778961
Ion Ratio Lower Upper
98 100
100 65.7 52.2 78.4

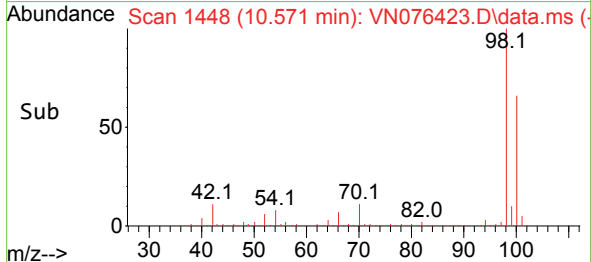

#51
4-Methyl-2-Pentanone
Concen: 3.866 ug/l
RT: 10.447 min Scan# 1427
Delta R.T. 0.000 min
Lab File: VN076423.D
Acq: 26 Jan 2023 16:25

Tgt Ion: 43 Resp: 17128
Ion Ratio Lower Upper
43 100
58 25.2 35.1 52.7#


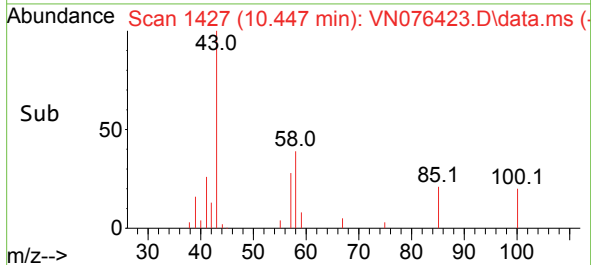






#52
Toluene
Concen: 0.207 ug/l
RT: 10.630 min Scan# 1458
Delta R.T. 0.001 min
Lab File: VN076423.D
Acq: 26 Jan 2023 16:25




Instrument :
MSVOA_N
ClientSampleId :
MH-10


Tgt Ion: 92 Resp: 2396
Ion Ratio Lower Upper
92 100
91 139.5 136.6 205.0



#53
t-1,3-Dichloropropene
Concen: 0.259 ug/l
RT: 10.735 min Scan# 1476
Delta R.T. -0.100 min
Lab File: VN076423.D
Acq: 26 Jan 2023 16:25

Tgt Ion: 75 Resp: 1495
Ion Ratio Lower Upper
75 100
77 1.6 25.8 38.6#









#54
 cis-1,3-Dichloropropene
 Concen: 12.032 ug/l
 RT: 10.365 min Scan# 14
 Delta R.T. 0.053 min
 Lab File: VN076423.D
 Acq: 26 Jan 2023 16:25




Instrument :
 MSVOA_N
 ClientSampleId :
 MH-10


Tgt Ion: 75 Resp: 80019
 Ion Ratio Lower Upper
 75 100
 77 0.7 26.5 39.7#
 39 29.8 37.1 55.7#



#56
 Ethyl methacrylate
 Concen: 0.422 ug/l
 RT: 10.994 min Scan# 1520
 Delta R.T. 0.118 min
 Lab File: VN076423.D
 Acq: 26 Jan 2023 16:25

Tgt Ion: 69 Resp: 2411
 Ion Ratio Lower Upper
 69 100
 41 4965.5 45.3 67.9#
 39 2263.9 29.3 43.9#





#57

1,3-Dichloropropane

Concen: 1.428 ug/l

RT: 11.206 min Scan# 1556

Delta R.T. 0.041 min

Lab File: VN076423.D

Acq: 26 Jan 2023 16:25

Instrument :

MSVOA_N

ClientSampleId :





MH-10

Tgt Ion: 76 Resp: 10259

Ion Ratio Lower Upper

76 100

78 0.0 26.4 39.6#

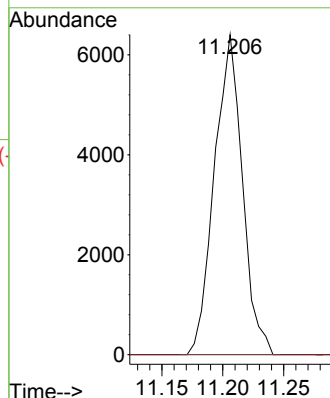

#59

2-Hexanone

Concen: 58.758 ug/l

RT: 11.171 min Scan# 1550

Delta R.T. -0.023 min

Lab File: VN076423.D




Acq: 26 Jan 2023 16:25


Tgt Ion: 43 Resp: 188662

Ion Ratio Lower Upper

43 100

58 0.0 30.1 90.3#


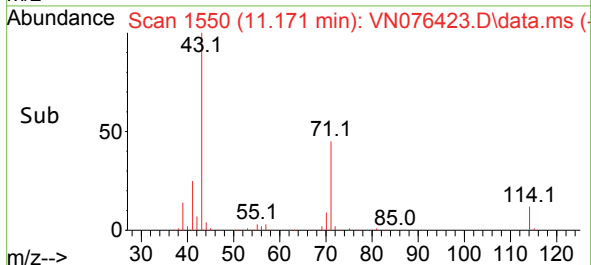
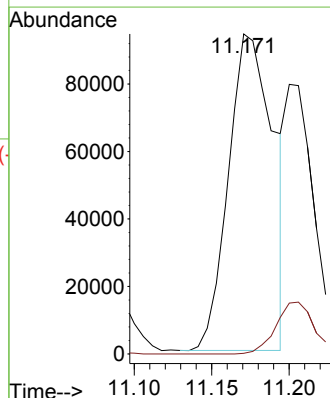





#62
4-Bromofluorobenzene
Concen: 51.863 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.006 min
Lab File: VN076423.D
Acq: 26 Jan 2023 16:25




Instrument :
MSVOA_N
ClientSampleId :
MH-10


Tgt Ion: 95 Resp: 254536
Ion Ratio Lower Upper
95 100
174 80.7 0.0 174.6
176 78.6 0.0 167.8

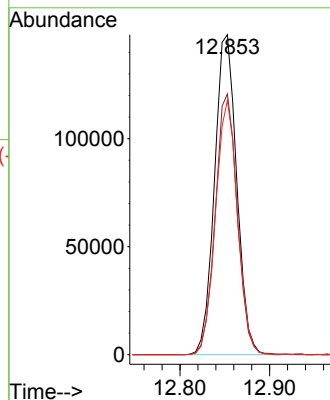

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1669
Delta R.T. 0.006 min
Lab File: VN076423.D
Acq: 26 Jan 2023 16:25

Tgt Ion: 117 Resp: 596919
Ion Ratio Lower Upper
117 100
82 54.1 42.2 63.2
119 31.9 26.9 40.3

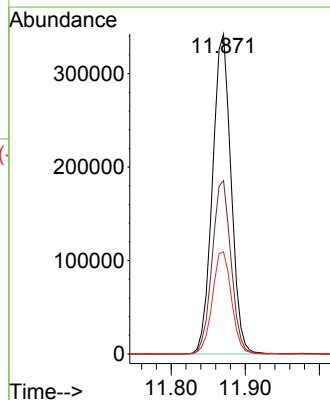



#71

Bromoform

Concen: 0.610 ug/l

RT: 12.847 min Scan# 1835

Delta R.T. 0.265 min

Lab File: VN076423.D

Acq: 26 Jan 2023 16:25

Instrument :

MSVOA_N

ClientSampleId :

MH-10





Tgt Ion:173 Resp: 2068

Ion Ratio Lower Upper

173 100

175 589.1 24.1 72.4#

254 0.0 0.0 0.0



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 1996

Delta R.T. 0.000 min

Lab File: VN076423.D

Acq: 26 Jan 2023 16:25




Tgt Ion:152 Resp: 236260


Ion Ratio Lower Upper

152 100

115 59.5 29.6 88.9

150 157.6 0.0 351.4

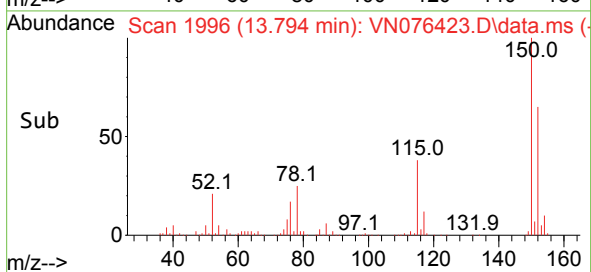



#74

N-amy1 acetate

Concen: 0.416 ug/l

RT: 12.494 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN076423.D

Acq: 26 Jan 2023 16:25

Instrument :

MSVOA_N

ClientSampleId :

MH-10

Tgt Ion: 43 Resp: 2187





Ion Ratio Lower Upper

43 100

70 0.0 41.2 61.8#

55 3.7 21.0 31.6#

61 0.0 21.6 32.4#



#76

1,2,3-Trichloropropane

Concen: 31.139 ug/l

RT: 12.853 min Scan# 1836

Delta R.T. -0.141 min

Lab File: VN076423.D




Acq: 26 Jan 2023 16:25


Tgt Ion: 75 Resp: 135562

Ion Ratio Lower Upper

75 100

77 1.1 75.2 225.6#









#77
Bromobenzene
Concen: Below Cal
RT: 12.971 min Scan# 1856
Delta R.T. -0.011 min
Lab File: VN076423.D
Acq: 26 Jan 2023 16:25




Instrument :
MSVOA_N
ClientSampleId :
MH-10


Tgt Ion:156 Resp: 67
Ion Ratio Lower Upper
156 100
77 198.5 93.4 280.2
158 0.0 48.4 145.2#

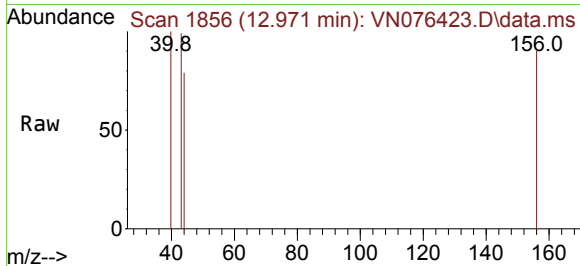

#81
trans-1,4-Dichloro-2-butene
Concen: 95.468 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.118 min
Lab File: VN076423.D
Acq: 26 Jan 2023 16:25

Tgt Ion: 75 Resp: 135562
Ion Ratio Lower Upper
75 100
53 0.0 75.8 113.8#
89 0.0 37.0 55.6#

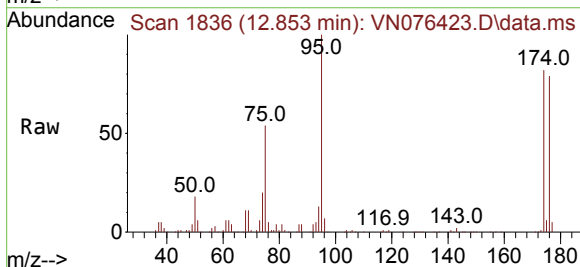



#93

1,2,4-Trichlorobenzene

Concen: 1.320 ug/l

RT: 15.400 min Scan# 21

Delta R.T. 0.006 min

Lab File: VN076423.D

Acq: 26 Jan 2023 16:25

Instrument :

MSVOA_N

ClientSampleId :

MH-10





Tgt Ion:180 Resp: 64

Ion Ratio Lower Upper

180 100

182 417.2 47.0 141.2#

145 0.0 15.2 45.5#



#95

Naphthalene

Concen: 1.925 ug/l

RT: 15.635 min Scan# 2309

Delta R.T. -0.006 min

Lab File: VN076423.D

Acq: 26 Jan 2023 16:25




Tgt Ion:128 Resp: 1100


Ion Ratio Lower Upper

128 100

127 8.4 10.3 15.5#

129 0.0 8.6 13.0#





#96

1,2,3-Trichlorobenzene

Concen: 1.167 ug/l

RT: 15.841 min Scan# 21

Delta R.T. -0.000 min

Lab File: VN076423.D


Acq: 26 Jan 2023 16:25

Instrument :

MSVOA_N

ClientSampleId :

MH-10



Tgt Ion:180 Resp: 54

Ion Ratio Lower Upper

180 100

182 103.7 47.5 142.5

145 0.0 15.9 47.6#

