


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012623\
Data File : VN076409.D
Acq On : 26 Jan 2023 08:43
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Title : SW846 8260
Last Update : Tue Jan 17 03:59:22 2023

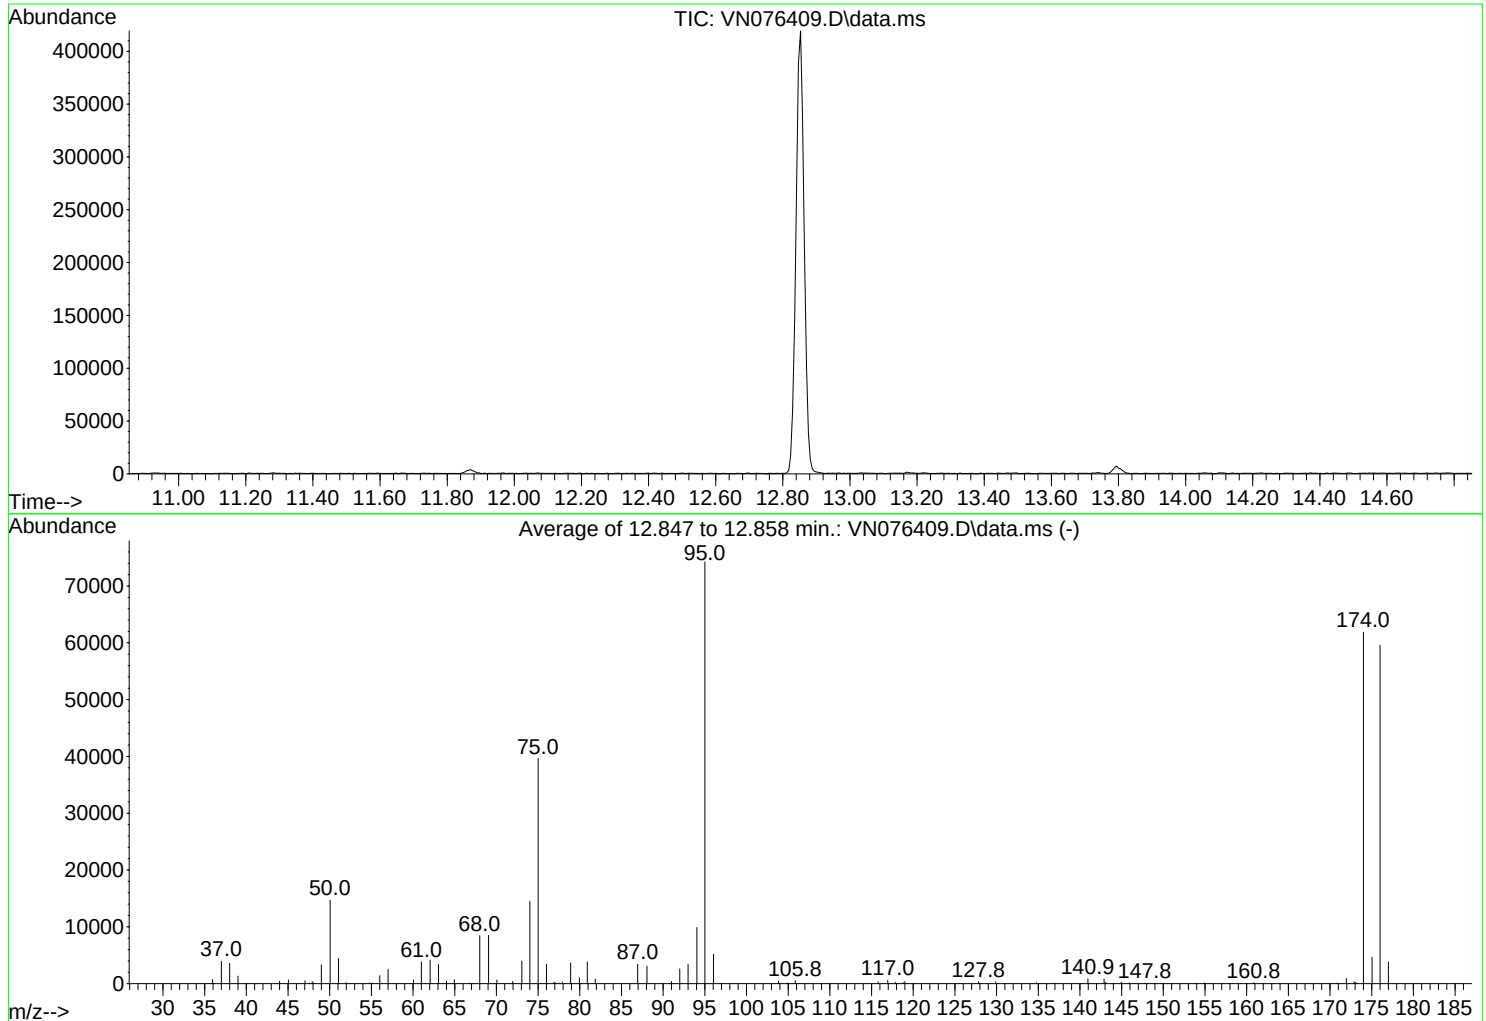

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.8	14697	PASS
75	95	30	60	53.4	39637	PASS
95	95	100	100	100.0	74261	PASS
96	95	5	9	7.0	5175	PASS
173	174	0.00	2	0.6	353	PASS
174	95	50	100	83.3	61835	PASS
175	174	5	9	7.6	4679	PASS
176	174	95	101	96.4	59592	PASS
177	176	5	9	6.4	3794	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	723	49.00	3287	63.05	3366	75.00	3963
37.00	3941	50.05	14697	64.00	481	76.00	341
38.00	3572	51.05	4412	64.95	707	76.90	26
39.00	1333	52.00	200	66.80	117	77.10	14
39.95	64	54.80	152	67.10	50	77.50	116
44.00	432	55.10	75	68.00	8454	77.90	284
45.05	666	56.00	1410	69.05	8514	78.90	3666
47.05	519	57.00	2496	70.05	647	79.95	1016
47.60	96	60.05	661	71.95	397	80.90	3800
47.90	365	61.00	3861	73.05	3980	81.85	784
48.10	147	62.05	4158	74.00	14487	86.95	3408

Average of 12.847 to 12.858 min.: VN076409.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
88.05	3097	115.80	317	142.90	821	170.80	72
91.00	405	116.95	569	143.10	247	171.95	938
92.00	2603	117.85	271	144.95	247	172.90	353
93.00	3368	118.80	167	145.90	144	173.10	229
94.05	9889	119.00	376	147.80	87	174.00	61835
95.00	74261	127.85	365	148.10	67	175.05	4679
96.05	5175	129.90	307	149.70	61	176.00	59592
97.00	61	130.90	53	153.90	59	177.00	3794
103.85	449	134.80	177	154.95	137		
104.90	149	136.90	82	157.10	53		
105.85	542	140.95	854	160.85	173		

Instrument :

MSVOA_N

ClientSampleId :

BFB