

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012624\
 Data File : VN080775.D
 Acq On : 26 Jan 2024 17:24
 Operator : JC\MD
 Sample : P1243-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MR-308-0-2

Quant Time: Jan 29 02:34:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011024W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 11 06:34:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	104669	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	240789	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	254314	50.000	ug/l	# 0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	97438	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	83972	45.684	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	91.360%		
35) Dibromofluoromethane	8.171	113	64875	47.420	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	94.840%		
50) Toluene-d8	10.571	98	272729	52.280	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	104.560%		
62) 4-Bromofluorobenzene	12.853	95	106628	53.301	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	106.600%		
Target Compounds						
					Qvalue	
3) Chloromethane	2.365	50	2111	0.451	ug/l #	80
5) Bromomethane	2.953	94	122	0.208	ug/l #	4
6) Chloroethane	3.136	64	99	Below Cal	#	43
11) Tert butyl alcohol	5.518	59	65	0.209	ug/l #	72
13) Acrolein	4.171	56	59	0.227	ug/l #	16
16) Acetone	4.424	43	23307	38.622	ug/l #	87
18) Methyl Acetate	5.030	43	1972	1.097	ug/l #	42
20) Methylene Chloride	5.271	84	5555	3.153	ug/l #	77
25) 2-Butanone	7.494	43	4220	3.869	ug/l #	87
29) Tetrahydrofuran	7.841	42	548	0.745	ug/l #	66
31) Cyclohexane	8.218	56	3783	1.332	ug/l #	44
36) 1,1-Dichloropropene	8.230	75	10312	3.680	ug/l #	46
37) Ethyl Acetate	7.559	43	3524	1.297	ug/l #	76
38) Carbon Tetrachloride	8.230	117	12498	4.967	ug/l #	15
41) Methacrylonitrile	7.847	41	392	0.249	ug/l #	7
42) 1,2-Dichloroethane	8.694	62	1171	0.388	ug/l #	73
43) Isopropyl Acetate	8.694	43	130314	26.088	ug/l #	79
48) Methyl methacrylate	9.671	41	3436	1.453	ug/l #	31
49) 1,4-Dioxane	9.735	88	55	1.866	ug/l #	1
51) 4-Methyl-2-Pentanone	10.453	43	11287	4.188	ug/l #	70
54) cis-1,3-Dichloropropene	10.365	75	40278	11.667	ug/l #	63
56) Ethyl methacrylate	10.988	69	1087	0.349	ug/l #	1
57) 1,3-Dichloropropane	11.200	76	3481	1.097	ug/l #	42
59) 2-Hexanone	11.171	43	164782	82.831	ug/l #	19
74) N-amyl acetate	12.470	43	1225	0.220	ug/l #	36
76) 1,2,3-Trichloropropane	12.853	75	61593	20.500	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	61593	48.326	ug/l #	15
92) 1,2-Dibromo-3-Chloropr...	14.700	75	77	Below Cal	#	4
95) Naphthalene	15.653	128	2276	0.335	ug/l #	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012624\
Data File : VN080775.D
Acq On : 26 Jan 2024 17:24
Operator : JC\MD
Sample : P1243-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MR-308-0-2

Quant Time: Jan 29 02:34:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011024W.M
Quant Title : SW846 8260
QLast Update : Thu Jan 11 06:34:36 2024
Response via : Initial Calibration




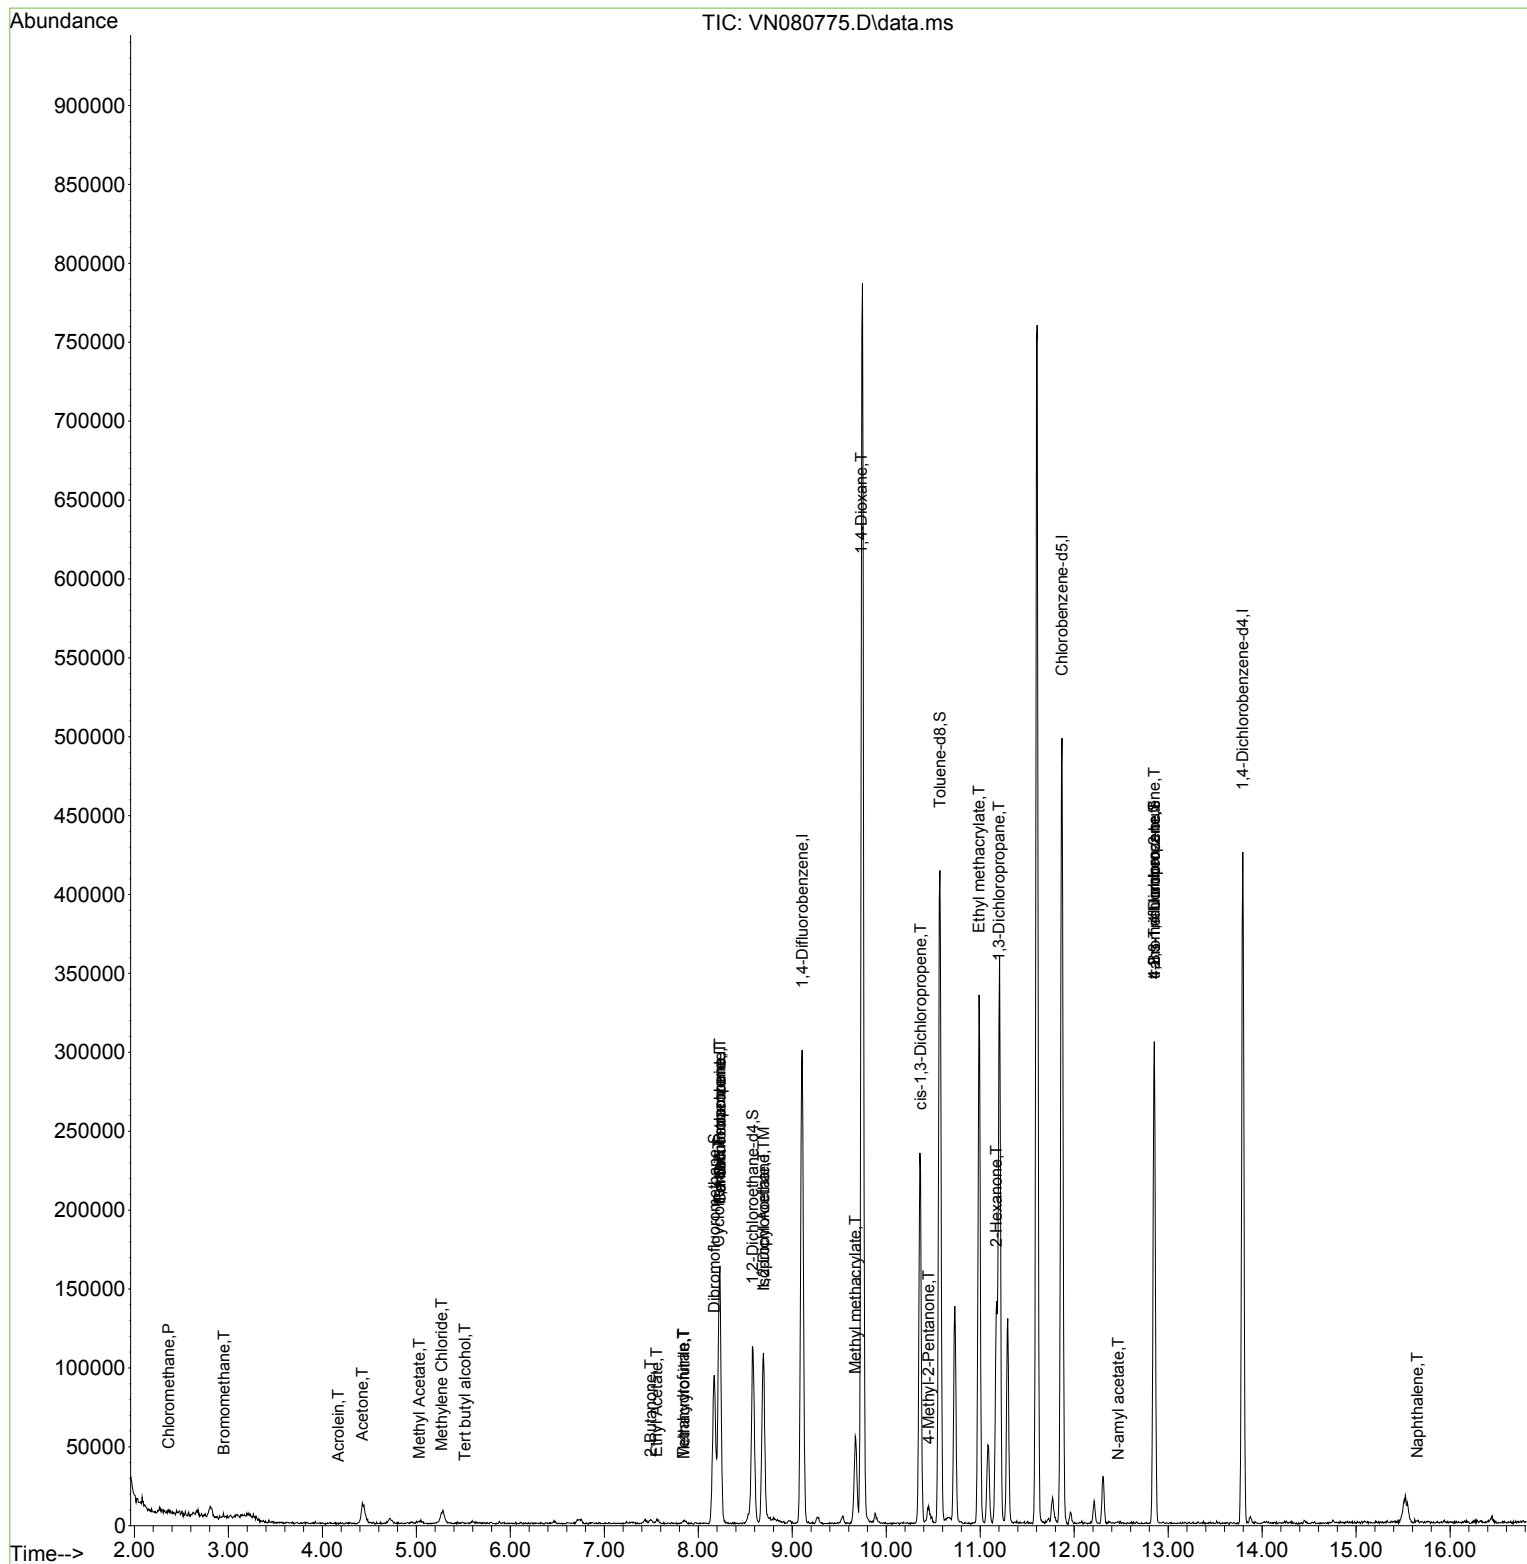




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 10
Delta R.T. 0.006 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24




Instrument :
MSVOA_N
ClientSampleId :
MR-308-0-2


Tgt Ion:168 Resp: 104669
Ion Ratio Lower Upper
168 100
99 69.6 53.0 79.6

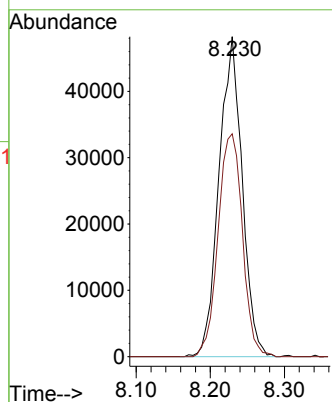

#3
Chloromethane
Concen: 0.451 ug/l
RT: 2.365 min Scan# 70
Delta R.T. 0.006 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24

Tgt Ion: 50 Resp: 2111
Ion Ratio Lower Upper
50 100
52 44.2 26.5 39.7#









#5
Bromomethane
Concen: 0.208 ug/l
RT: 2.953 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24




Instrument :
MSVOA_N
ClientSampleId :
MR-308-0-2


Tgt Ion: 94 Resp: 122
Ion Ratio Lower Upper
94 100
96 0.0 73.1 109.7#

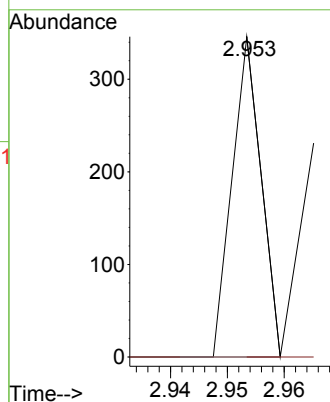

#6
Chloroethane
Concen: Below Cal
RT: 3.136 min Scan# 201
Delta R.T. 0.018 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24

Tgt Ion: 64 Resp: 99
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.2#

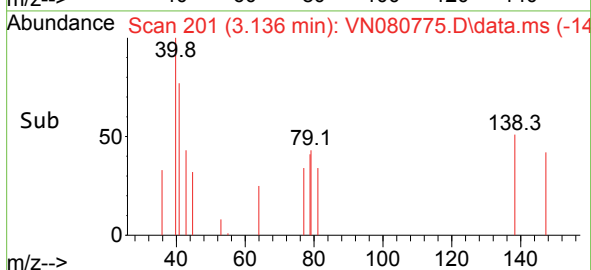



#11

Tert butyl alcohol

Concen: 0.209 ug/l

RT: 5.518 min Scan# 605

Delta R.T. 0.006 min

Lab File: VN080775.D

Acq: 26 Jan 2024 17:24

Instrument :

MSVOA_N

ClientSampleId :





MR-308-0-2

Tgt Ion: 59 Resp: 65

Ion Ratio Lower Upper

59 100

57 0.0 8.2 12.4#

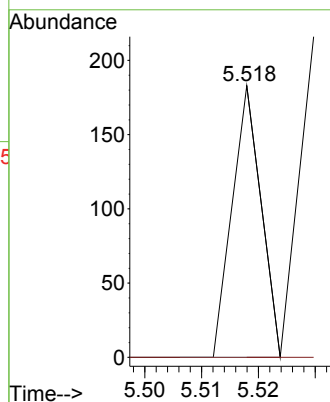

#13

Acrolein

Concen: 0.227 ug/l

RT: 4.171 min Scan# 377

Delta R.T. -0.000 min

Lab File: VN080775.D




Acq: 26 Jan 2024 17:24


Tgt Ion: 56 Resp: 59

Ion Ratio Lower Upper

56 100

55 0.0 54.5 81.7#


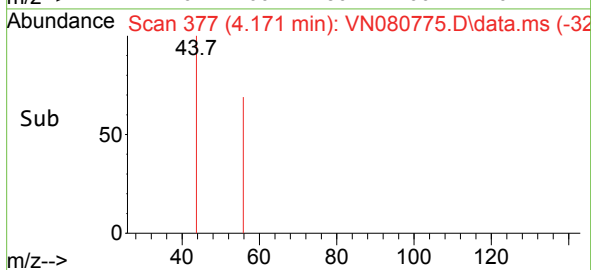






#16
Acetone
Concen: 38.622 ug/l
RT: 4.424 min Scan# 431
Delta R.T. 0.000 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24




Instrument :
MSVOA_N
ClientSampleId :
MR-308-0-2


Tgt Ion: 43 Resp: 23307
Ion Ratio Lower Upper
43 100
58 27.7 28.0 42.0#

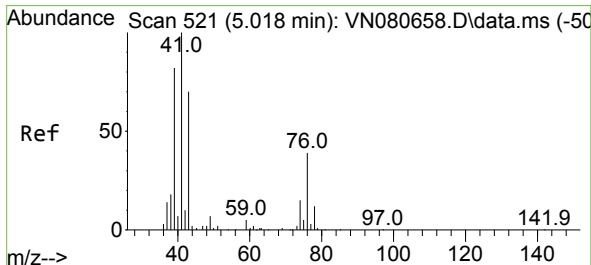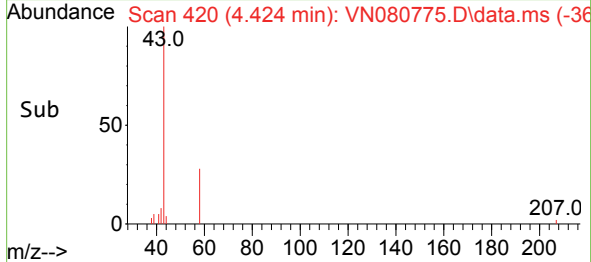

#18
Methyl Acetate
Concen: 1.097 ug/l
RT: 5.030 min Scan# 523
Delta R.T. 0.012 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24

Tgt Ion: 43 Resp: 1972
Ion Ratio Lower Upper
43 100
74 0.0 26.2 39.4#




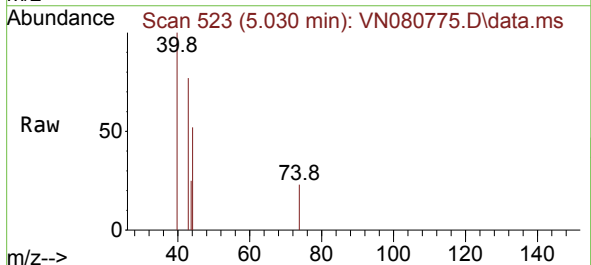




#20
Methylene Chloride
Concen: 3.153 ug/l
RT: 5.271 min Scan# 51
Delta R.T. -0.000 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24




Instrument :
MSVOA_N
ClientSampleId :
MR-308-0-2


Tgt Ion: 84	Resp:	5555
Ion	Ratio	Lower Upper
84	100	
49	91.4	79.7 119.5
51	63.7	25.2 37.8#
86	42.6	53.3 79.9#

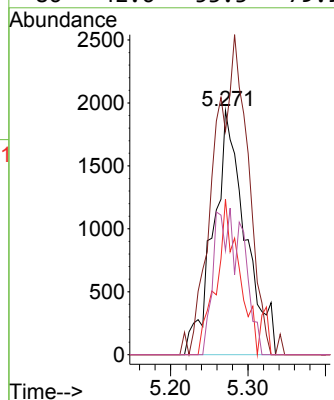

#25
2-Butanone
Concen: 3.869 ug/l
RT: 7.494 min Scan# 942
Delta R.T. 0.018 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24

Tgt Ion: 43	Resp:	4220
Ion	Ratio	Lower Upper
43	100	
72	29.9	30.2 45.2#

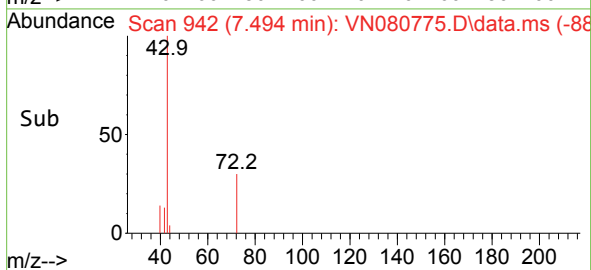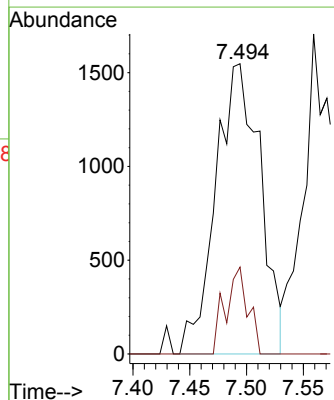



#29

Tetrahydrofuran

Concen: 0.745 ug/l

RT: 7.841 min Scan# 10

Delta R.T. 0.006 min

Lab File: VN080775.D

Acq: 26 Jan 2024 17:24





Instrument :

MSVOA_N

ClientSampleId :

MR-308-0-2

Tgt Ion: 42	Resp: 548
Ion Ratio	Lower Upper
42	100
72	28.8 49.8 74.6#
71	41.8 47.4 71.2#



#31

Cyclohexane

Concen: 1.332 ug/l




RT: 8.218 min Scan# 1065


Delta R.T. -0.041 min

Lab File: VN080775.D

Acq: 26 Jan 2024 17:24

Tgt Ion: 56	Resp: 3783
Ion Ratio	Lower Upper
56	100
69	109.3 26.8 40.2#
84	70.8 81.8 122.6#

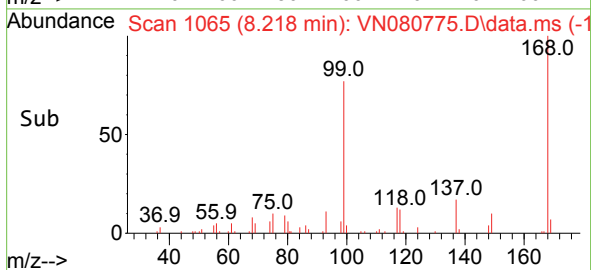



#33

1,2-Dichloroethane-d4

Concen: 45.684 ug/l

RT: 8.577 min Scan# 1126

Delta R.T. -0.000 min

Lab File: VN080775.D

Acq: 26 Jan 2024 17:24

Instrument :

MSVOA_N

ClientSampleId :





MR-308-0-2

Tgt Ion: 65 Resp: 83972

Ion Ratio Lower Upper

65 100

67 53.3 0.0 106.6

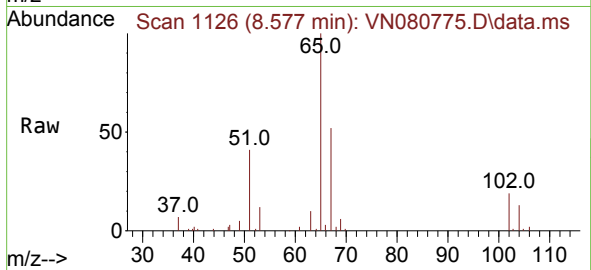

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. 0.006 min

Lab File: VN080775.D

Acq: 26 Jan 2024 17:24




Tgt Ion: 114 Resp: 240789


Ion Ratio Lower Upper

114 100

63 23.0 0.0 36.4

88 19.8 0.0 30.6


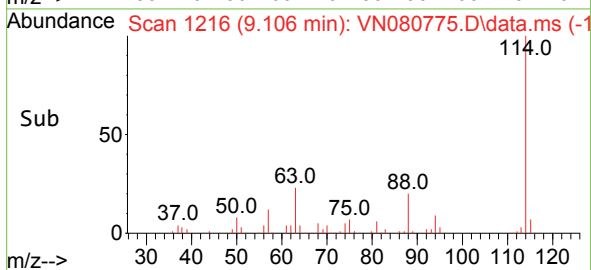






#35
Dibromofluoromethane
Concen: 47.420 ug/l
RT: 8.171 min Scan# 1056
Delta R.T. 0.006 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24




Instrument :
MSVOA_N
ClientSampleId :
MR-308-0-2


Tgt Ion:113 Resp: 64875
Ion Ratio Lower Upper
113 100
111 103.7 82.6 123.8
192 15.8 12.7 19.1

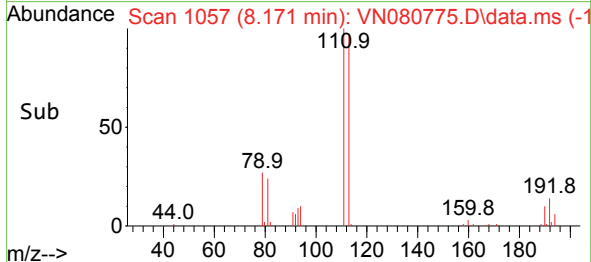

#36
1,1-Dichloropropene
Concen: 3.680 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.147 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24

Tgt Ion: 75 Resp: 10312
Ion Ratio Lower Upper
75 100
110 6.6 19.1 57.3#
77 0.0 25.0 37.4#

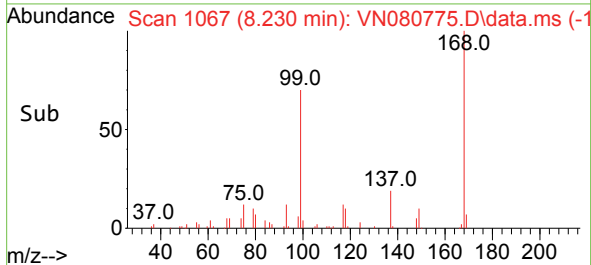



#37

Ethyl Acetate

Concen: 1.297 ug/l

RT: 7.559 min Scan# 91

Delta R.T. 0.006 min

Lab File: VN080775.D

Acq: 26 Jan 2024 17:24





Instrument :

MSVOA_N

ClientSampleId :

MR-308-0-2

Tgt Ion: 43	Resp: 3524
Ion Ratio	Lower Upper
43 100	
61 7.6	13.2 19.8#
70 2.6	11.3 16.9#



#38

Carbon Tetrachloride

Concen: 4.967 ug/l




RT: 8.230 min Scan# 1067


Delta R.T. -0.135 min

Lab File: VN080775.D

Acq: 26 Jan 2024 17:24

Tgt Ion: 117	Resp: 12498
Ion Ratio	Lower Upper
117 100	
119 4.7	77.3 115.9#
121 0.0	23.3 34.9#




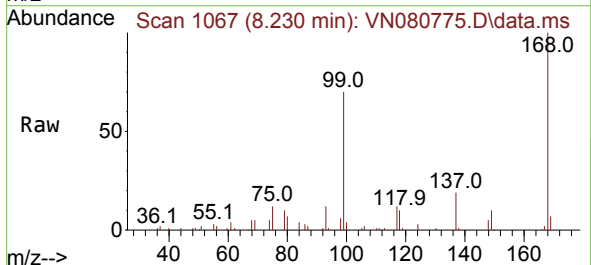




#41
Methacrylonitrile
Concen: 0.249 ug/l
RT: 7.847 min Scan# 1002
Delta R.T. 0.071 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24




Instrument :
MSVOA_N
ClientSampleId :
MR-308-0-2


Tgt Ion: 41	Resp: 392
Ion Ratio	Lower Upper
41 100	
39 128.6	42.6 64.0#
67 0.0	77.5 116.3#
52 0.0	28.9 43.3#

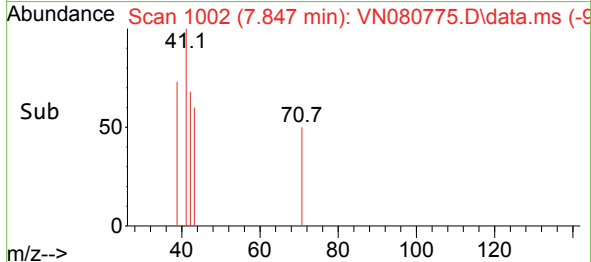

#42
1,2-Dichloroethane
Concen: 0.388 ug/l
RT: 8.694 min Scan# 1146
Delta R.T. 0.024 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24

Tgt Ion: 62	Resp: 1171
Ion Ratio	Lower Upper
62 100	
98 0.0	0.0 19.8




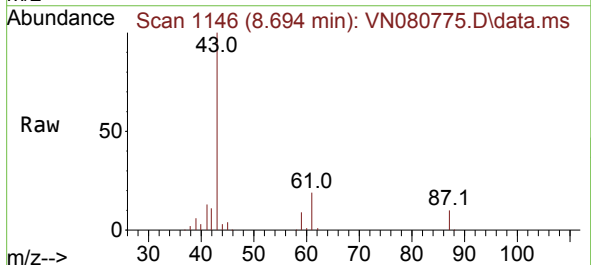




#43
Isopropyl Acetate
Concen: 26.088 ug/l
RT: 8.694 min Scan# 1146
Delta R.T. 0.006 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24




Instrument :
MSVOA_N
ClientSampleId :
MR-308-0-2


Tgt Ion: 43 Resp: 130314
Ion Ratio Lower Upper
43 100
61 18.0 24.7 37.1#
87 11.0 14.6 21.8#

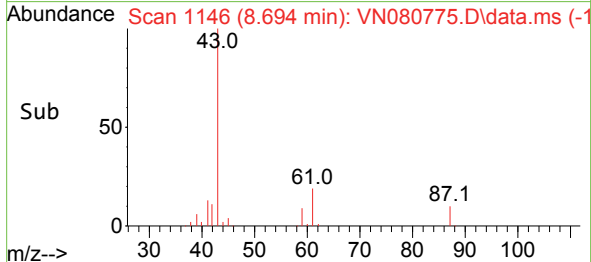

#48
Methyl methacrylate
Concen: 1.453 ug/l
RT: 9.671 min Scan# 1312
Delta R.T. -0.012 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24

Tgt Ion: 41 Resp: 3436
Ion Ratio Lower Upper
41 100
69 0.0 90.4 135.6#
39 60.2 54.6 81.8





#49

1,4-Dioxane

Concen: 1.866 ug/l

RT: 9.735 min Scan# 11

Delta R.T. 0.041 min

Lab File: VN080775.D

Acq: 26 Jan 2024 17:24

Instrument :

MSVOA_N

ClientSampleId :

MR-308-0-2





Tgt Ion: 88 Resp: 55

Ion Ratio Lower Upper

88 100

43 1446889.1 17.0 25.6#

58 6089.1 47.0 70.4#

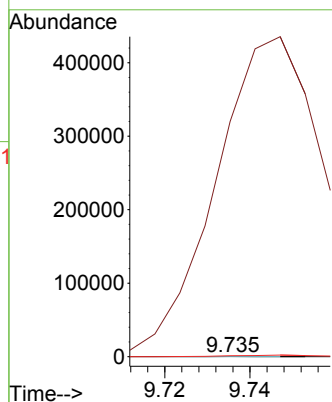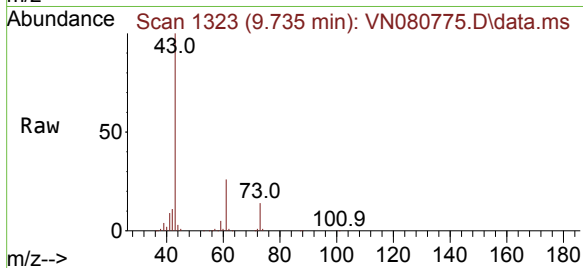

#50

Toluene-d8

Concen: 52.280 ug/l

RT: 10.571 min Scan# 1465

Delta R.T. 0.000 min

Lab File: VN080775.D




Acq: 26 Jan 2024 17:24


Tgt Ion: 98 Resp: 272729

Ion Ratio Lower Upper

98 100

100 65.5 52.0 78.0




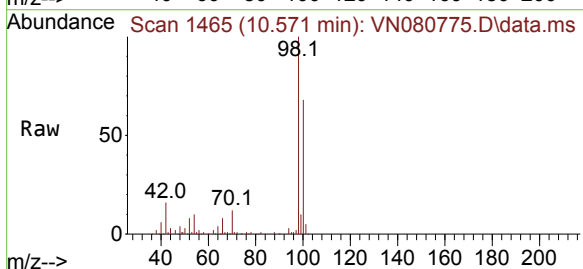


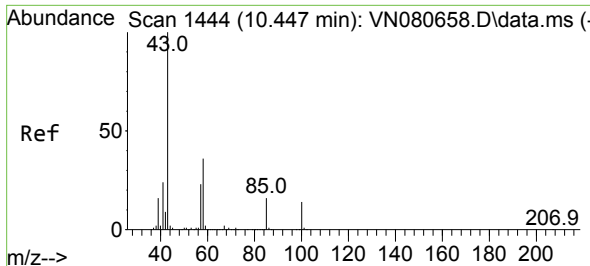

#51
4-Methyl-2-Pentanone
Concen: 4.188 ug/l
RT: 10.453 min Scan# 1445
Delta R.T. 0.006 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24




Instrument : MSVOA_N
ClientSampleId : MR-308-0-2


Tgt Ion: 43 Resp: 11287
Ion Ratio Lower Upper
43 100
58 25.7 36.6 54.8#

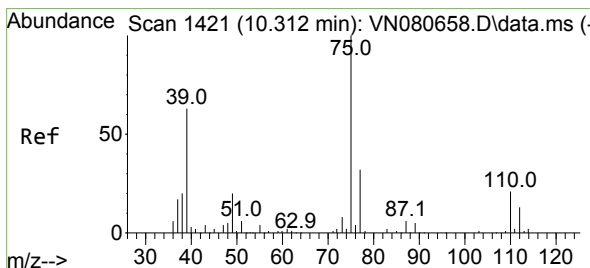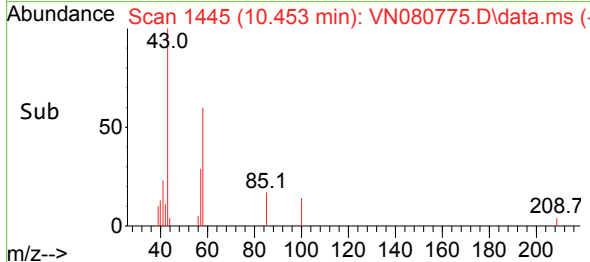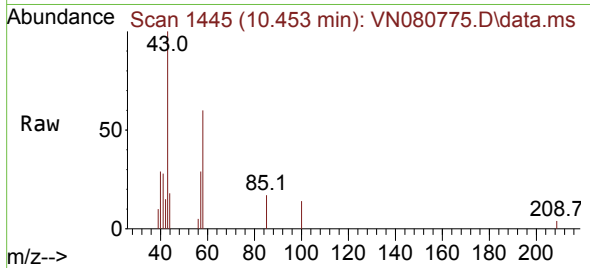

#54
cis-1,3-Dichloropropene
Concen: 11.667 ug/l
RT: 10.365 min Scan# 1430
Delta R.T. 0.053 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24

Tgt Ion: 75 Resp: 40278
Ion Ratio Lower Upper
75 100
77 1.0 26.1 39.1#
39 26.2 31.6 47.4#


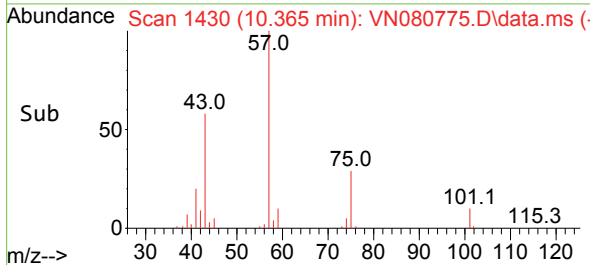

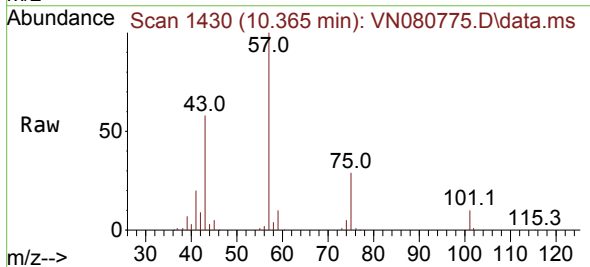


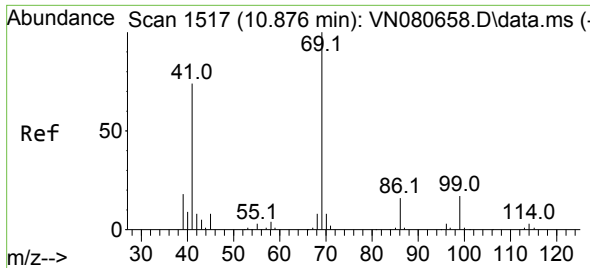

#56
Ethyl methacrylate
Concen: 0.349 ug/l
RT: 10.988 min Scan# 1536
Delta R.T. 0.112 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24




Instrument :
MSVOA_N
ClientSampleId :
MR-308-0-2


Tgt Ion: 69 Resp: 1087
Ion Ratio Lower Upper
69 100
41 5683.7 39.6 59.4#
39 2588.0 28.6 43.0#

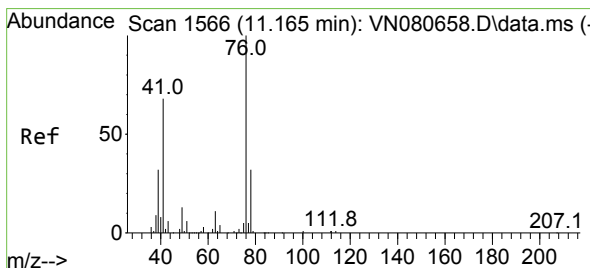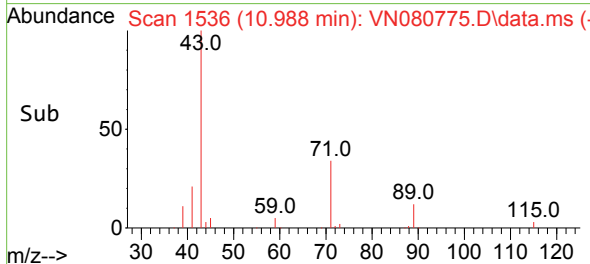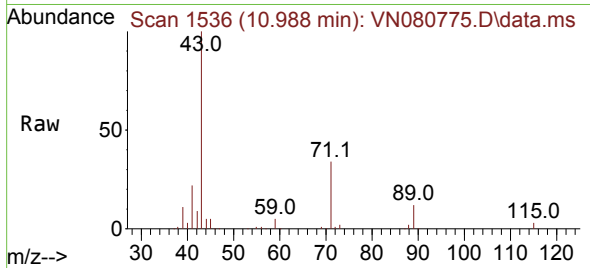

#57
1,3-Dichloropropane
Concen: 1.097 ug/l
RT: 11.200 min Scan# 1572
Delta R.T. 0.035 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24

Tgt Ion: 76 Resp: 3481
Ion Ratio Lower Upper
76 100
78 0.0 26.1 39.1#


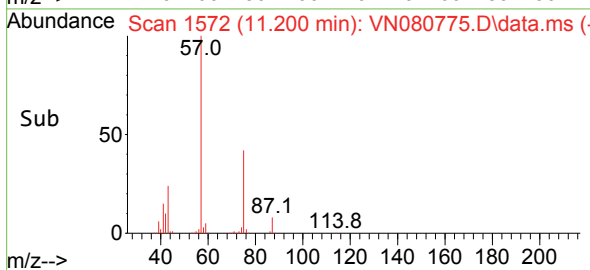

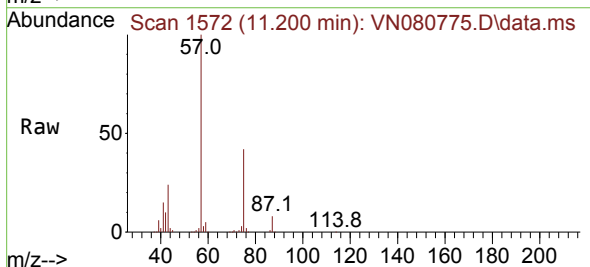




#59
2-Hexanone
Concen: 82.831 ug/l
RT: 11.171 min Scan# 1567
Delta R.T. -0.024 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24




Instrument :
MSVOA_N
ClientSampleId :
MR-308-0-2


Tgt Ion: 43 Resp: 164782
Ion Ratio Lower Upper
43 100
58 0.0 31.7 95.1#

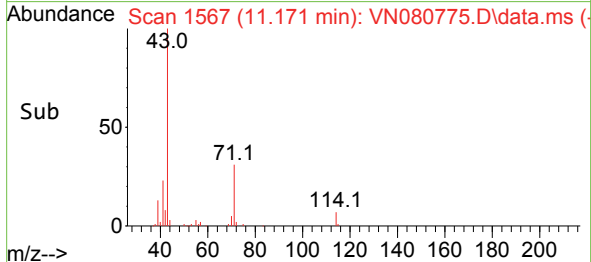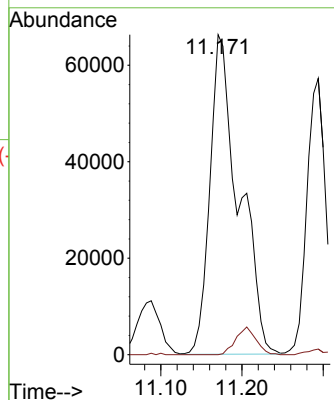

#62
4-Bromofluorobenzene
Concen: 53.301 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24

Tgt Ion: 95 Resp: 106628
Ion Ratio Lower Upper
95 100
174 59.9 0.0 143.8
176 59.7 0.0 135.8



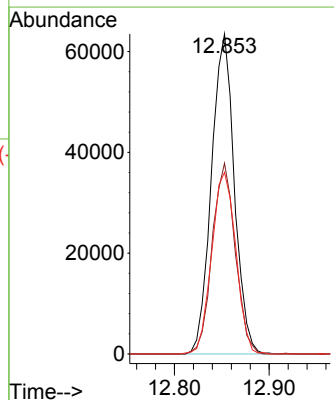
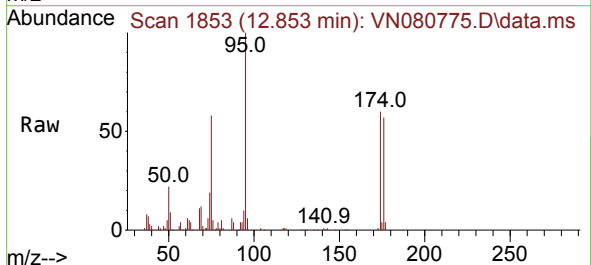




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24




Instrument :
MSVOA_N
ClientSampleId :
MR-308-0-2


Tgt Ion:117 Resp: 254314
Ion Ratio Lower Upper
117 100
82 69.7 44.0 66.0#
119 33.2 25.6 38.4



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.000 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24

Tgt Ion:152 Resp: 97438
Ion Ratio Lower Upper
152 100
115 68.8 32.3 96.8
150 160.4 0.0 355.8


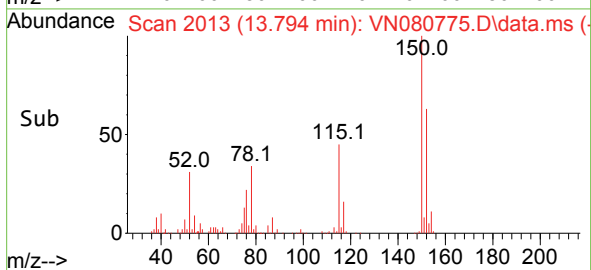






#74
N-amy1 acetate
Concen: 0.220 ug/l
RT: 12.470 min Scan# 1788
Delta R.T. -0.023 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24




Instrument :
MSVOA_N
ClientSampleId :
MR-308-0-2


Tgt Ion: 43	Resp: 1225
Ion Ratio	Lower Upper
43 100	
70 0.0	43.4 65.2#
55 0.0	21.4 32.0#
61 0.0	22.8 34.2#

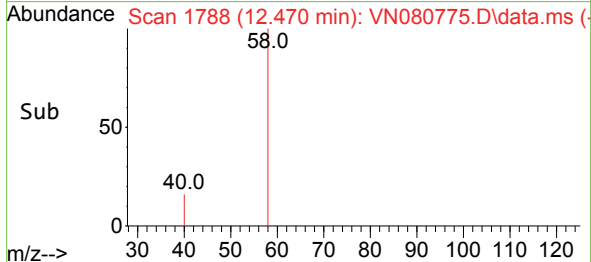

#76
1,2,3-Trichloropropane
Concen: 20.500 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.141 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24

Tgt Ion: 75	Resp: 61593
Ion Ratio	Lower Upper
75 100	
77 1.3	84.5 253.5#







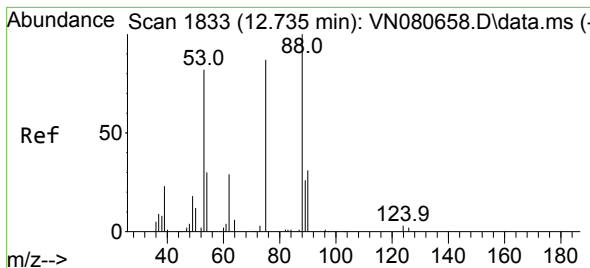

#81
trans-1,4-Dichloro-2-butene
Concen: 48.326 ug/l
RT: 12.853 min Scan# 11
Delta R.T. 0.118 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24




Instrument :
MSVOA_N
ClientSampleId :
MR-308-0-2


Tgt Ion: 75 Resp: 61593
Ion Ratio Lower Upper
75 100
53 0.0 67.4 101.2#
89 0.0 38.8 58.2#

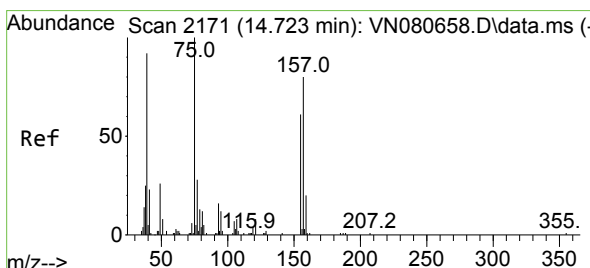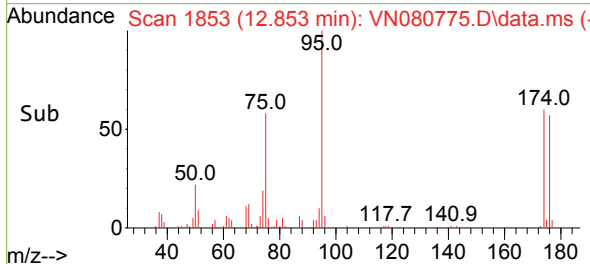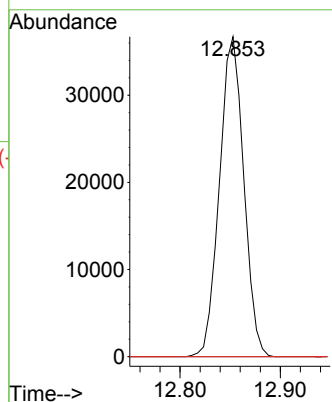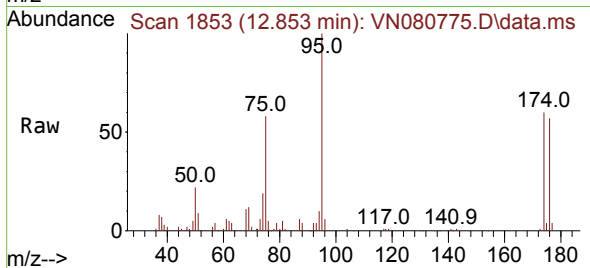

#92
1,2-Dibromo-3-Chloropropane
Concen: Below Cal
RT: 14.700 min Scan# 2167
Delta R.T. -0.023 min
Lab File: VN080775.D
Acq: 26 Jan 2024 17:24


Tgt Ion: 75 Resp: 77
Ion Ratio Lower Upper
75 100
155 0.0 39.1 117.2#
157 0.0 50.3 150.9#

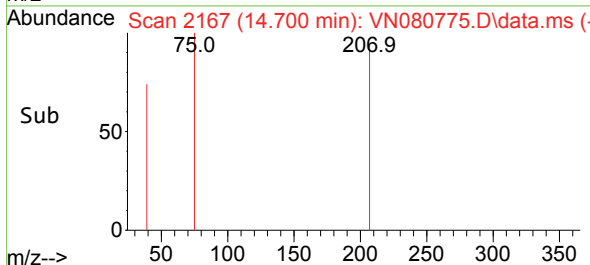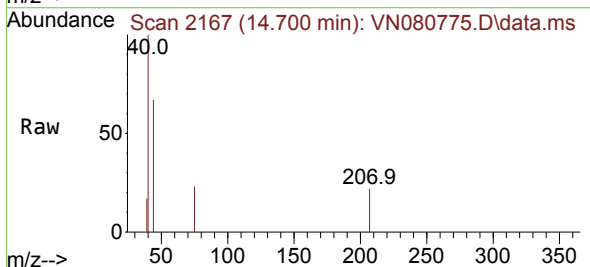

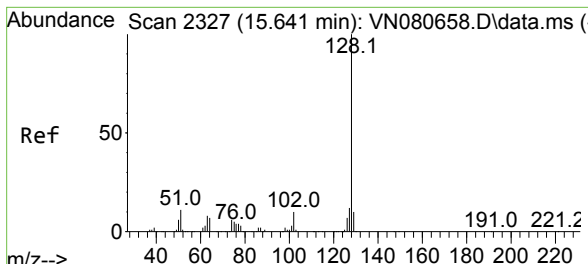

#95
 Naphthalene
 Concen: 0.335 ug/l
 RT: 15.653 min Scan# 21
 Delta R.T. 0.012 min
 Lab File: VN080775.D
 Acq: 26 Jan 2024 17:24

Instrument :
 MSVOA_N
 ClientSampleId :
 MR-308-0-2

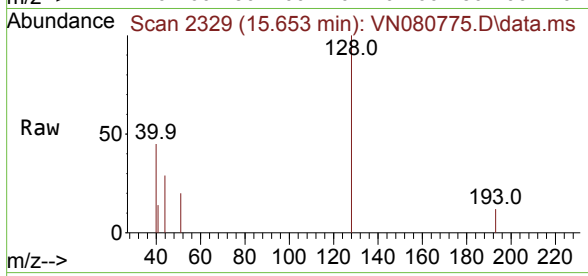

Tgt Ion:128 Resp: 2276

Ion	Ratio	Lower	Upper
128	100		
127	2.7	10.0	15.0#
129	0.0	8.7	13.1#

