
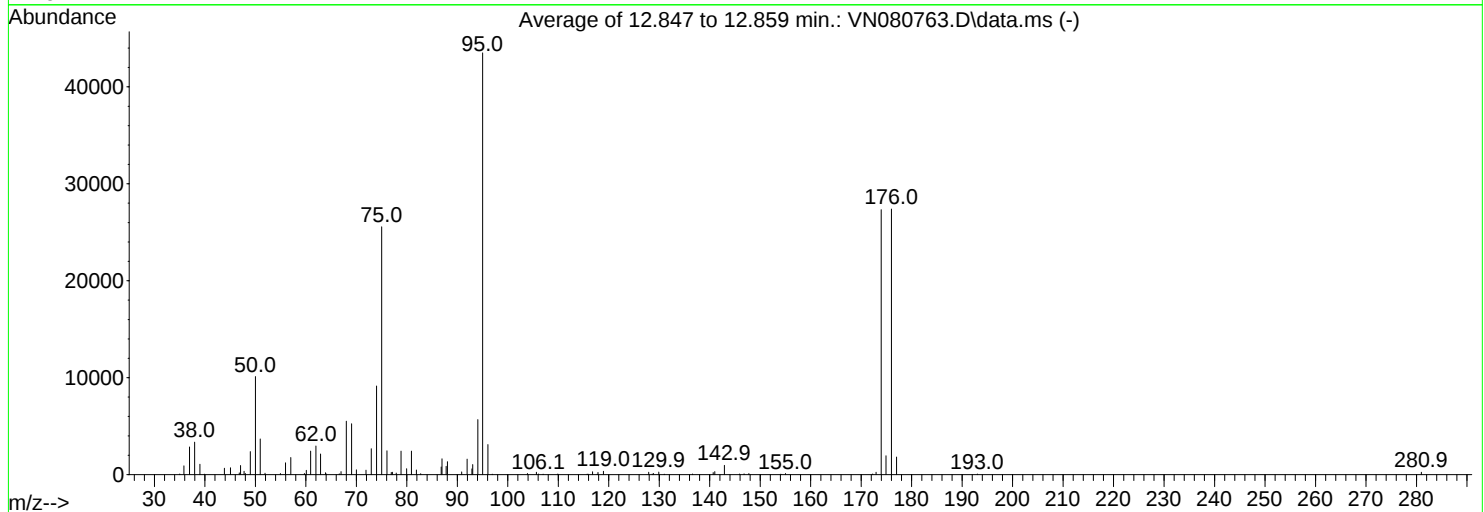


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012624\
Data File : VN080763.D
Acq On : 26 Jan 2024 09:41
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011024W.M
Title : SW846 8260
Last Update : Thu Jan 11 06:34:36 2024

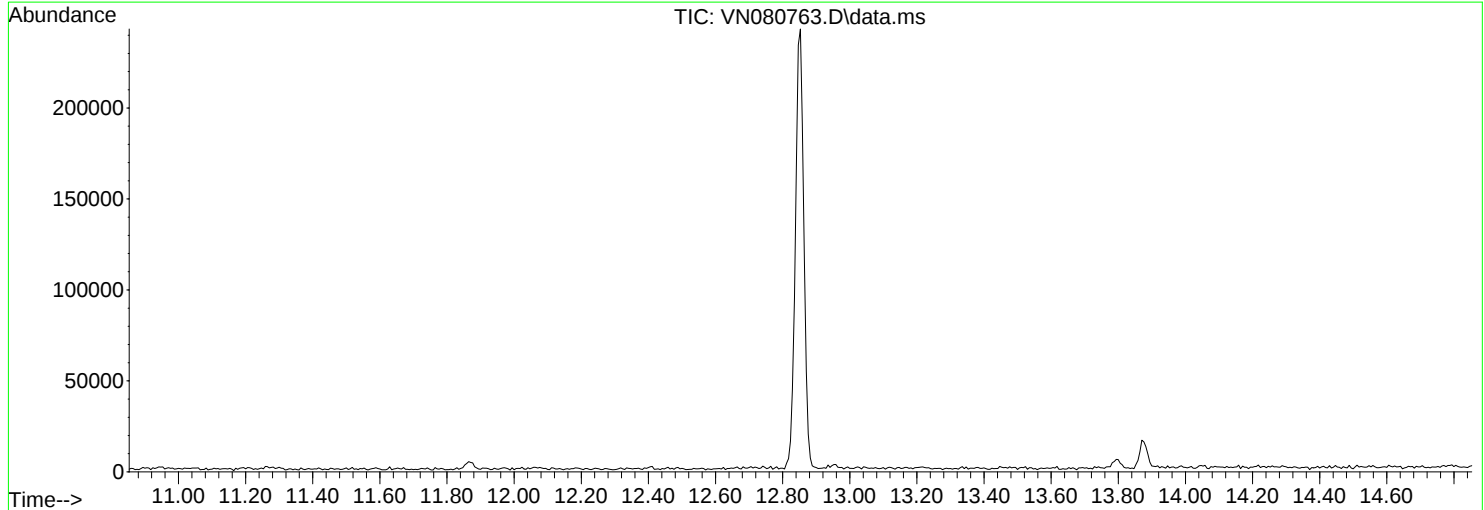

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	10111	PASS
75	95	30	60	58.8	25565	PASS
95	95	100	100	100.0	43507	PASS
96	95	5	9	7.1	3103	PASS
173	174	0.00	2	0.9	250	PASS
174	95	50	100	62.8	27325	PASS
175	174	5	9	7.2	1955	PASS
176	174	95	101	100.3	27395	PASS
177	176	5	9	6.6	1812	PASS

Average of 12.847 to 12.859 min.: VN080763.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.00	61	48.00	121	62.00	2952	74.00	913
35.85	908	49.00	2373	62.90	2129	75.00	2556
36.95	2863	50.00	10111	63.90	200	76.05	246
37.95	3350	50.95	3677	64.10	65	76.90	23
39.00	1074	51.90	146	66.60	90	77.15	252
39.90	45	54.95	125	66.95	308	77.90	168
43.85	669	55.95	1228	68.00	5510	78.85	2421
45.05	712	57.00	1761	69.05	5254	79.95	618
46.80	185	59.70	112	70.00	499	80.90	2429
47.05	947	60.10	439	71.90	469	81.90	474
47.75	352	60.95	2430	72.95	2680	82.75	107

Average of 12.847 to 12.859 min.: VN080763.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.80	794	96.90	50	118.95	340	146.80	91
86.95	1635	103.90	115	127.90	257	147.75	125
87.80	854	105.65	242	128.60	73	154.10	55
88.05	1339	106.10	73	128.85	122	155.00	122
90.85	284	107.00	51	129.90	266	172.30	67
91.95	1604	109.90	67	131.00	50	172.95	250
92.90	600	115.70	50	136.60	60	173.95	27325
93.05	1035	115.90	58	140.70	212	174.90	1955
94.05	5670	116.80	293	141.00	308	176.00	27395
95.00	43507	117.70	59	142.90	958	177.00	1812
96.05	3103	117.85	229	145.90	61	193.00	60

Average of 12.847 to 12.859 min.: VN080763.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
280.95	241						

Instrument :
MSVOA_N
ClientSampleId :
BFB