

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN012720\
 Data File : VN059872.D
 Acq On : 27 Jan 2020 15:06
 Operator : JC/MD
 Sample : PB126348TB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB126348TB

Quant Time: Jan 27 15:27:44 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011320W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jan 18 03:09:32 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.64	168	217458	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.56	114	323101	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.40	117	280183	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	115340	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.00	65	112144	46.44	ug/l	0.00
Spiked Amount			Recovery	=	92.88%	
35) Dibromofluoromethane	7.57	113	95007	49.31	ug/l	0.00
Spiked Amount			Recovery	=	98.62%	
50) Toluene-d8	10.08	98	375707	50.33	ug/l	0.00
Spiked Amount			Recovery	=	100.66%	
62) 4-Bromofluorobenzene	12.40	95	122894	45.66	ug/l	0.00
Spiked Amount			Recovery	=	91.32%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	4.72	59	193	0.47	ug/l	# 72
16) Acetone	3.79	43	3781	Below Cal		# 91
17) Carbon Disulfide	4.02	76	1225	0.22	ug/l	# 75
18) Methyl Acetate	4.31	43	2182	0.77	ug/l	# 57
25) 2-Butanone	6.82	43	422	0.31	ug/l	# 50
31) Cyclohexane	7.64	56	3892	1.09	ug/l	# 1
36) 1,1-Dichloropropene	7.64	75	14252	5.07	ug/l	# 50
38) Carbon Tetrachloride	7.64	117	19760	6.46	ug/l	# 15
43) Isopropyl Acetate	8.14	43	48882	10.77	ug/l	# 91
45) 1,2-Dichloropropane	9.25	63	1024	0.49	ug/l	# 44
48) Methyl methacrylate	9.25	41	77350	38.10	ug/l	# 46
51) 4-Methyl-2-Pentanone	9.97	43	3596	1.37	ug/l	# 88
54) cis-1,3-Dichloropropene	9.89	75	23899	6.89	ug/l	# 54
57) 1,3-Dichloropropane	10.75	76	3954	1.19	ug/l	# 42
59) 2-Hexanone	10.75	43	50859	26.31	ug/l	# 56
74) N-amyl acetate	12.03	43	1296	0.39	ug/l	# 45
76) 1,2,3-Trichloropropane	12.40	75	62145	32.02	ug/l	# 100
77) Bromobenzene	12.53	156	2182	1.02	ug/l	# 1
80) 1,3,5-Trimethylbenzene	12.73	105	6952	0.98	ug/l	# 98
81) trans-1,4-Dichloro-2-buten	12.40	75	62145	68.75	ug/l	# 11
92) 1,2-Dibromo-3-Chloropropan	14.25	75	240	Below Cal		# 6
93) 1,2,4-Trichlorobenzene	14.91	180	1046	0.47	ug/l	# 87
94) Hexachlorobutadiene	15.01	225	296	0.24	ug/l	# 80
95) Naphthalene	15.13	128	16327	2.60	ug/l	# 98
96) 1,2,3-Trichlorobenzene	15.32	180	1683	0.78	ug/l	# 90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN012720\
Data File : VN059872.D
Acq On : 27 Jan 2020 15:06
Operator : JC/MD
Sample : PB126348TB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB126348TB

Quant Time: Jan 27 15:27:44 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N011320W.M
Quant Title : SW846 8260
QLast Update : Sat Jan 18 03:09:32 2020
Response via : Initial Calibration

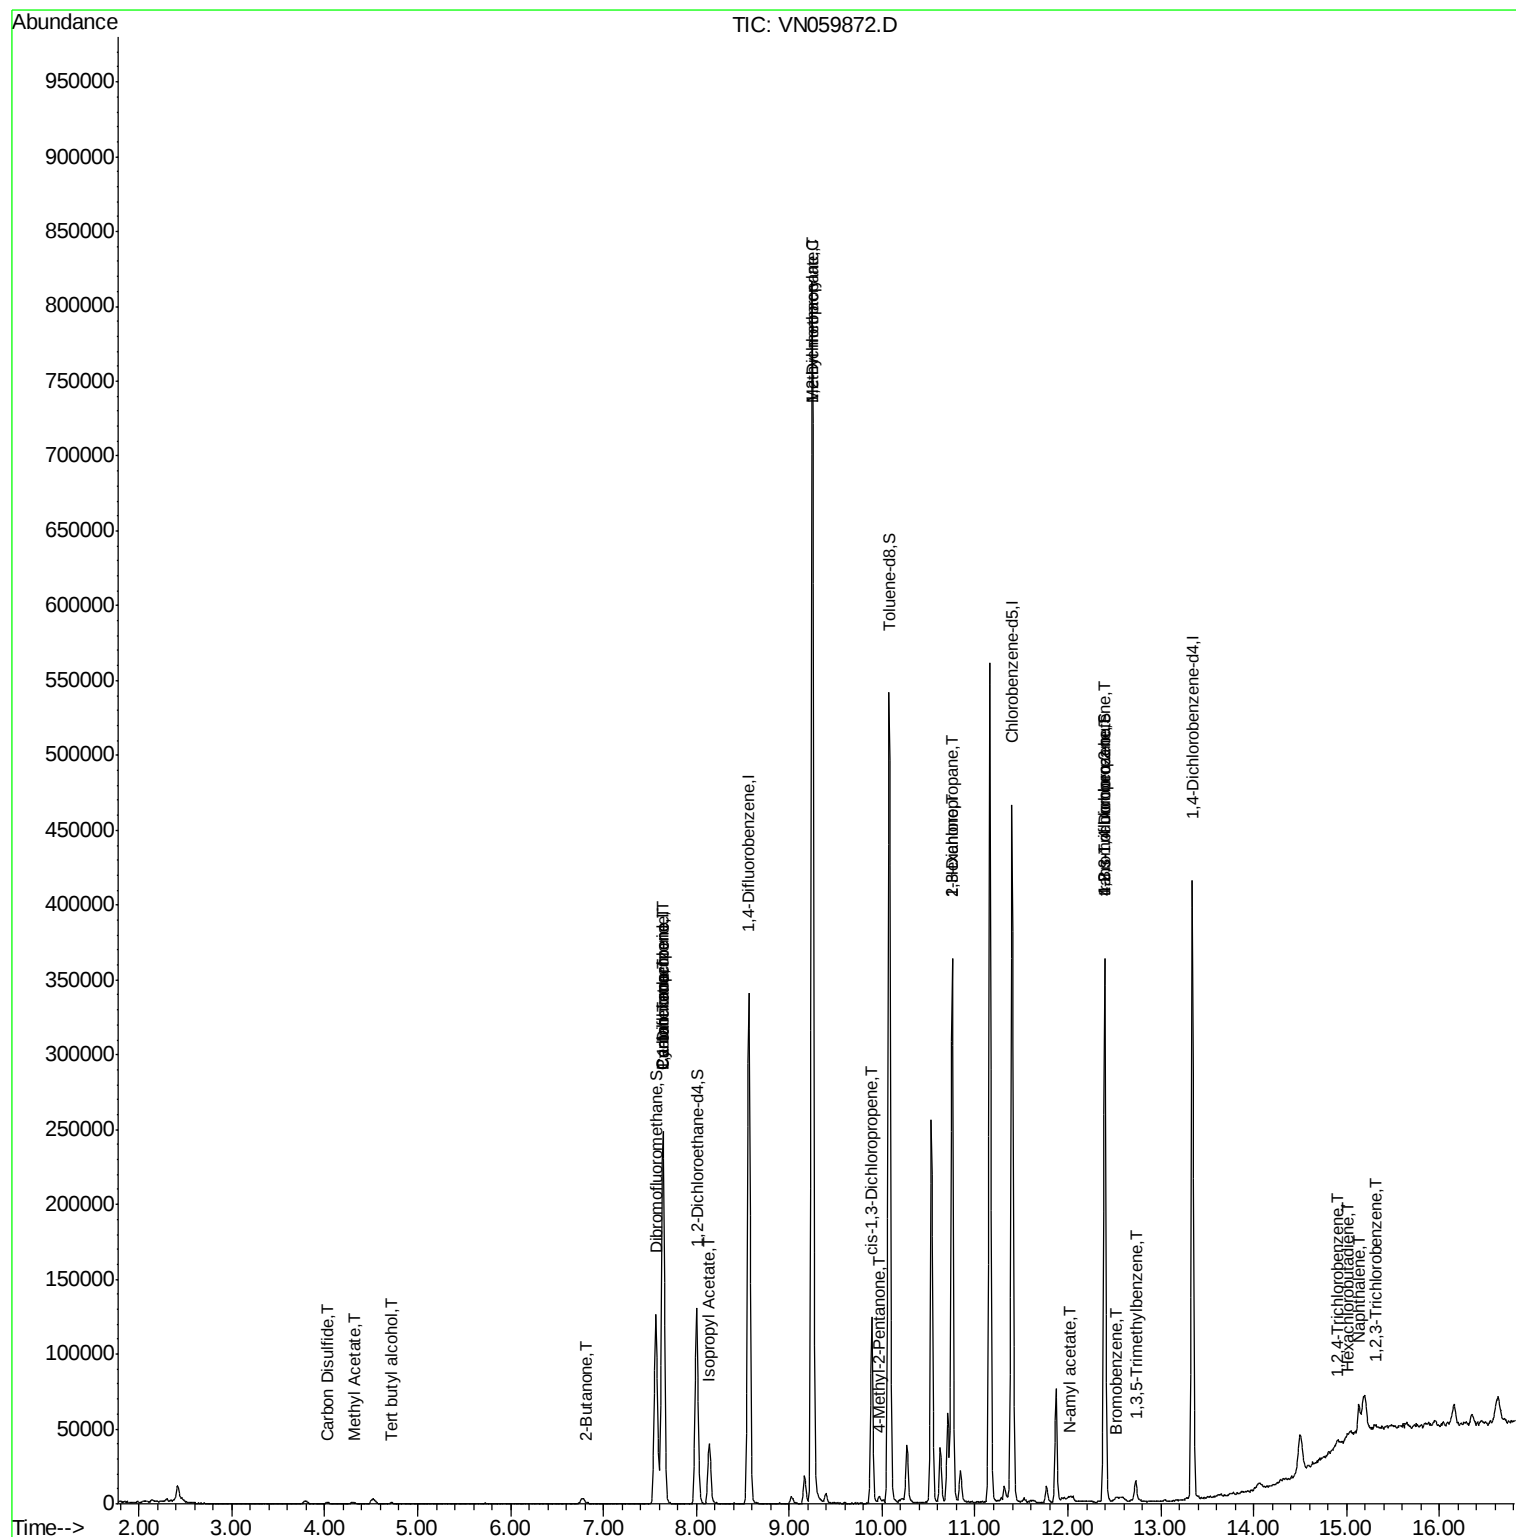



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.64 min Scan# 1825

Delta R.T. 0.00 min

Lab File: VN059872.D

Acq: 27 Jan 2020 15:06

Instrument :

MSVOA_N

ClientSampled :


PB126348TB

Tgt Ion:168 Resp: 217458

Ion Ratio Lower Upper




168 100

99 50.8 48.2 72.4



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

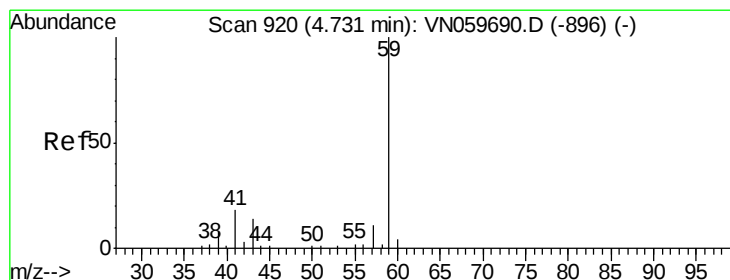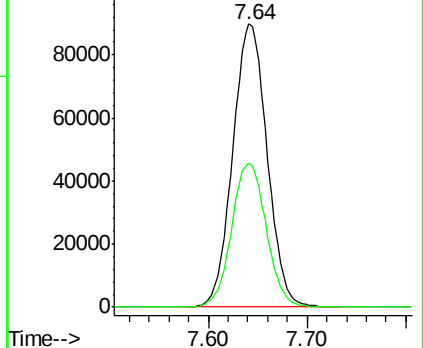

#11

Tert butyl alcohol

Concen: 0.47 ug/l

RT: 4.72 min Scan# 917

Delta R.T. -0.01 min

Lab File: VN059872.D


Acq: 27 Jan 2020 15:06

Tgt Ion: 59 Resp: 193

Ion Ratio Lower Upper



59 100


57 0.0 8.6 12.8#

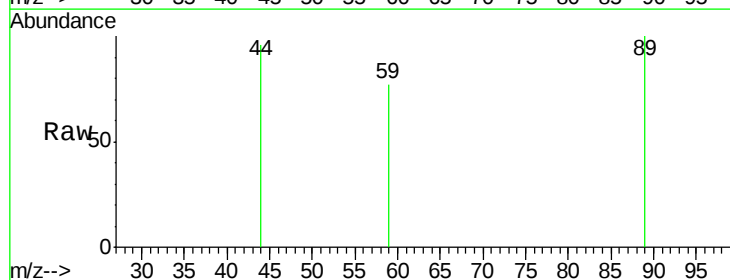

Abundance Ion 59.00 (58.70 to 59.70): VNO

Ion 57.00 (56.70 to 57.70): VNO

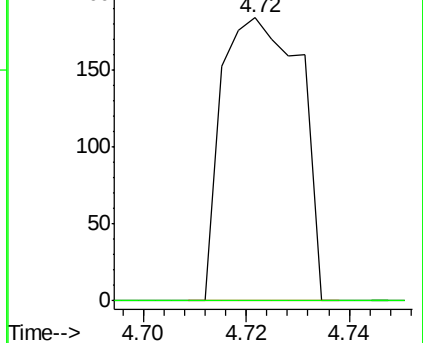

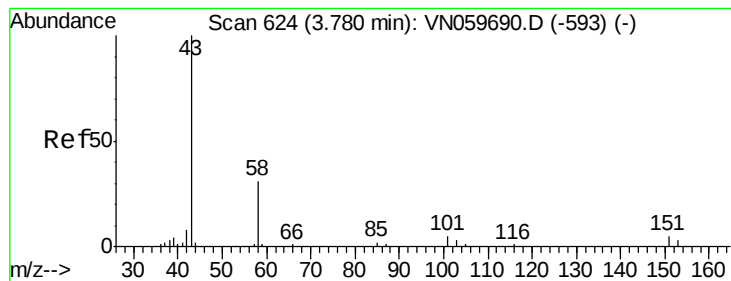

#16

Acetone

Concen: Below Cal

RT: 3.79 min Scan# 627

Delta R.T. 0.01 min

Lab File: VN059872.D

Acq: 27 Jan 2020 15:06

Instrument :

MSVOA_N

ClientSampled :


PB126348TB

Tgt Ion: 43 Resp: 3781

Ion Ratio Lower Upper




43 100

58 24.6 23.6 35.4



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

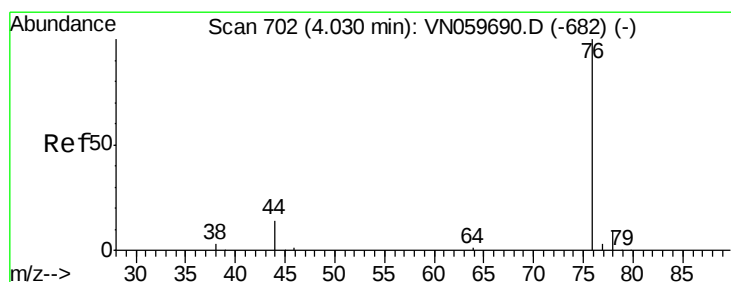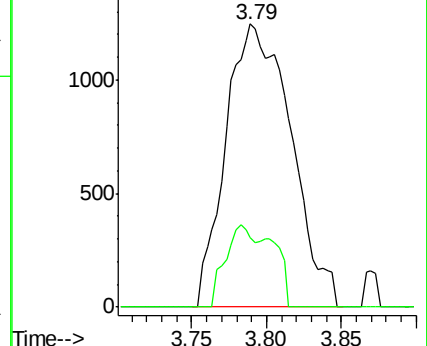

#17

Carbon Disulfide

Concen: 0.22 ug/l

RT: 4.02 min Scan# 700

Delta R.T. -0.01 min

Lab File: VN059872.D


Acq: 27 Jan 2020 15:06

Tgt Ion: 76 Resp: 1225

Ion Ratio Lower Upper



76 100


78 0.0 7.4 11.0#



Abundance Ion 75.90 (75.60 to 76.60): VN0

Ion 77.90 (77.60 to 78.60): VN0




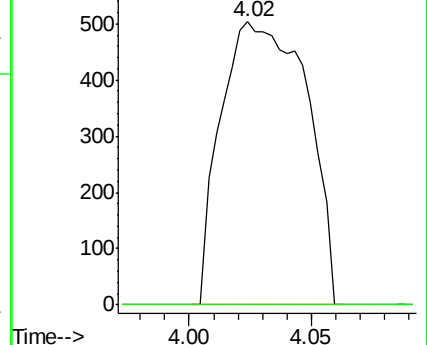


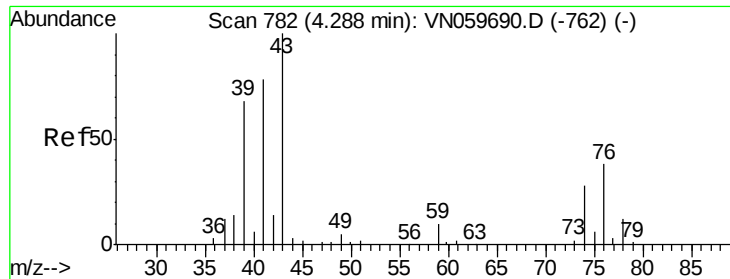

#18
Methyl Acetate
Concen: 0.77 ug/l
RT: 4.31 min Scan# 790
Delta R.T. 0.03 min
Lab File: VN059872.D
Acq: 27 Jan 2020 15:06




Instrument :
MSVOA_N
ClientSampleId :
PB126348TB


Tgt Ion: 43 Resp: 2182
Ion Ratio Lower Upper
43 100
74 1.3 17.5 26.3#

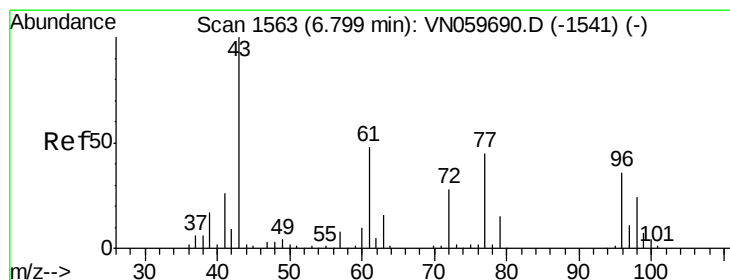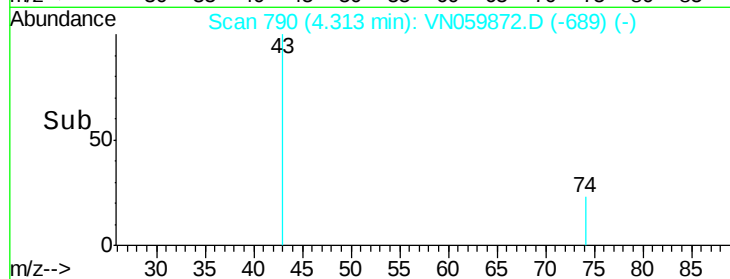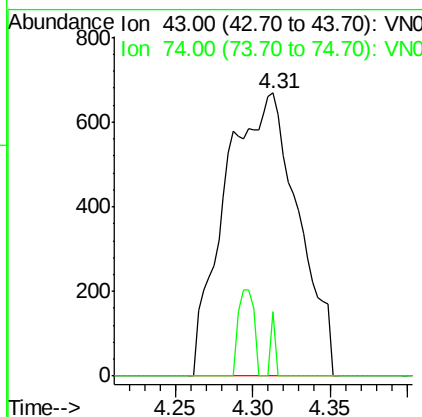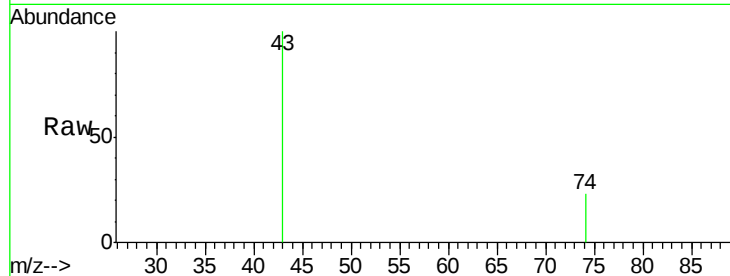

#25
2-Butanone
Concen: 0.31 ug/l
RT: 6.82 min Scan# 1571
Delta R.T. 0.03 min
Lab File: VN059872.D
Acq: 27 Jan 2020 15:06

Tgt Ion: 43 Resp: 422
Ion Ratio Lower Upper
43 100
72 0.0 19.9 29.9#

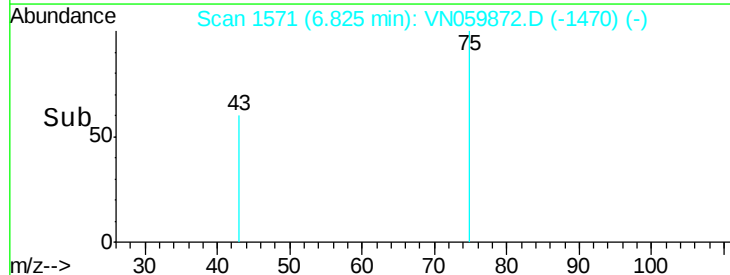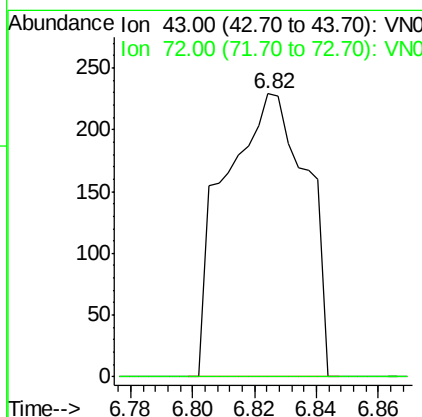

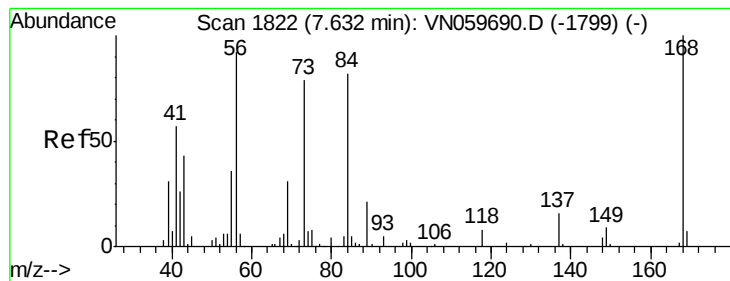

#31

Cyclohexane

Concen: 1.09 ug/l

RT: 7.64 min Scan# 1824

Delta R.T. 0.01 min

Lab File: VN059872.D

Acq: 27 Jan 2020 15:06

Instrument :

MSVOA_N

ClientSampleId :

PB126348TB


Tgt Ion: 56 Resp: 3892

Ion Ratio Lower Upper

56 100

69 176.8 26.5 39.7#




84 138.2 65.3 97.9#

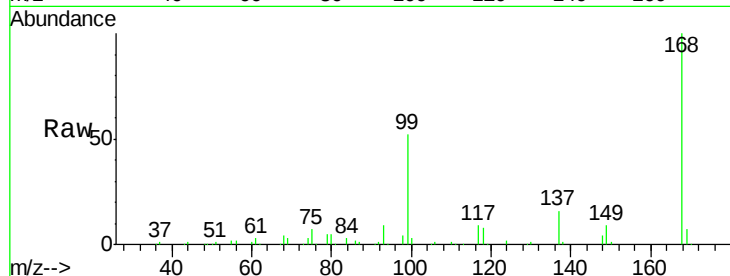

Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 69.00 (68.70 to 69.70): VN0

Ion 84.00 (83.70 to 84.70): VN0

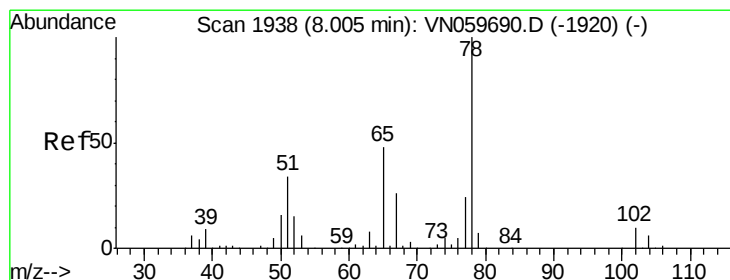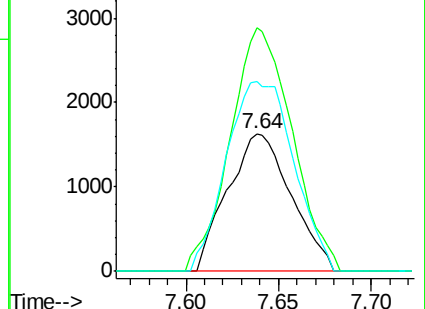

#33

1,2-Dichloroethane-d4

Concen: 46.44 ug/l

RT: 8.00 min Scan# 1938

Delta R.T. 0.00 min

Lab File: VN059872.D


Acq: 27 Jan 2020 15:06

Tgt Ion: 65 Resp: 112144

Ion Ratio Lower Upper



65 100


67 53.0 0.0 103.0



Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0

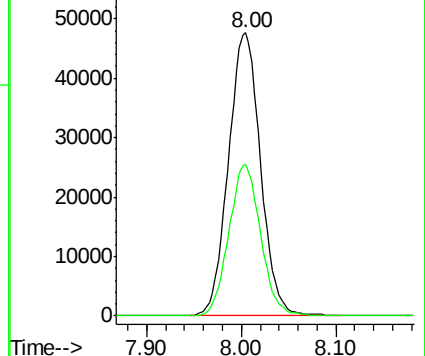


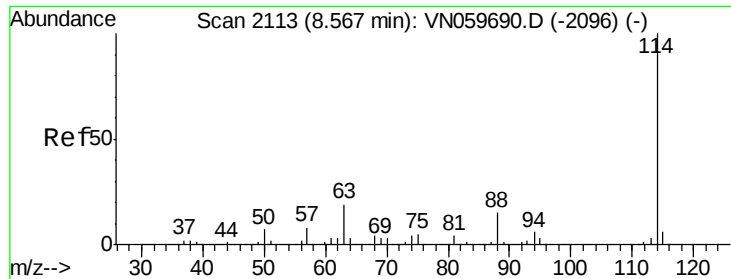




#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.56 min Scan# 2112
Delta R.T. -0.00 min
Lab File: VN059872.D
Acq: 27 Jan 2020 15:06

Instrument :
MSVOA_N
ClientSampleId :
PB126348TB

Tgt Ion:114 Resp: 323101
Ion Ratio Lower Upper
114 100
63 18.5 0.0 43.6
88 15.2 0.0 31.4

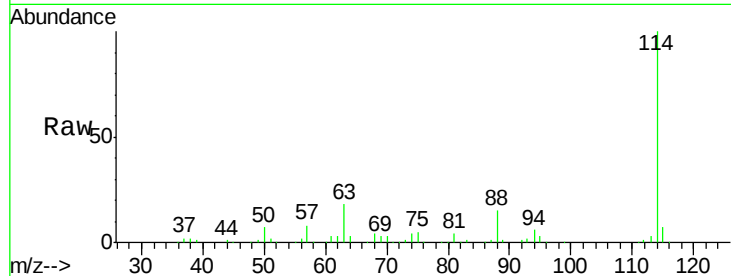


Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VN
Ion 87.90 (87.60 to 88.60): VN

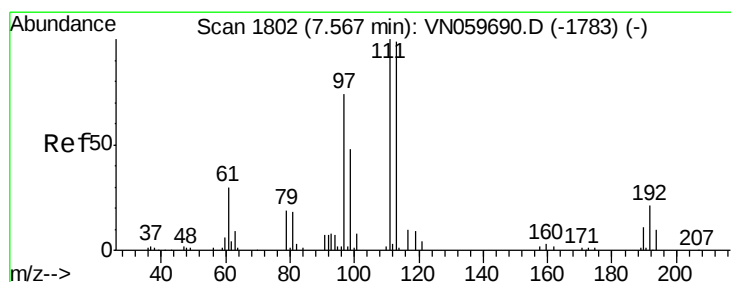
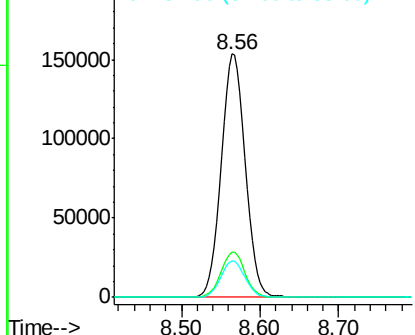



#35
Dibromofluoromethane
Concen: 49.31 ug/l
RT: 7.57 min Scan# 1802
Delta R.T. 0.00 min
Lab File: VN059872.D
Acq: 27 Jan 2020 15:06

Tgt Ion:113 Resp: 95007
Ion Ratio Lower Upper
113 100
111 104.2 83.5 125.3
192 21.9 15.4 23.2



Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V




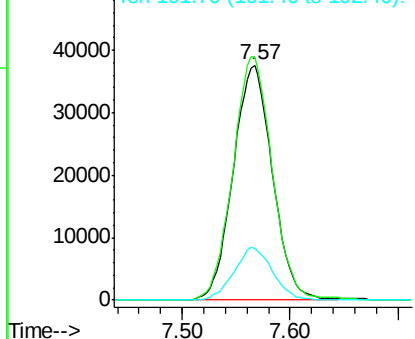


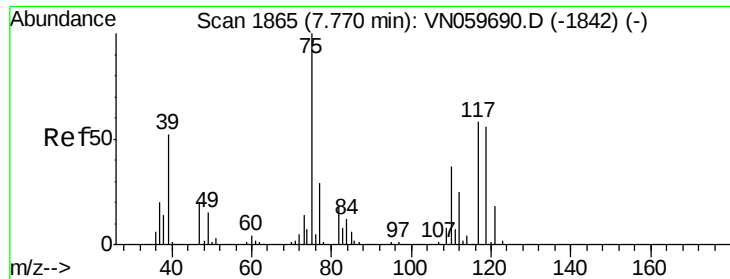

#36
 1,1-Dichloropropene
 Concen: 5.07 ug/l
 RT: 7.64 min Scan# 1824
 Delta R.T. -0.13 min
 Lab File: VN059872.D
 Acq: 27 Jan 2020 15:06




Instrument :
 MSVOA_N
 ClientSampleId :
 PB126348TB


Tgt Ion: 75 Resp: 14252
 Ion Ratio Lower Upper
 75 100
 110 8.6 16.6 49.7#
 77 0.0 25.1 37.7#

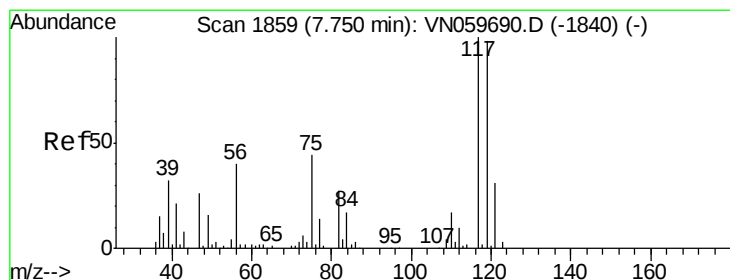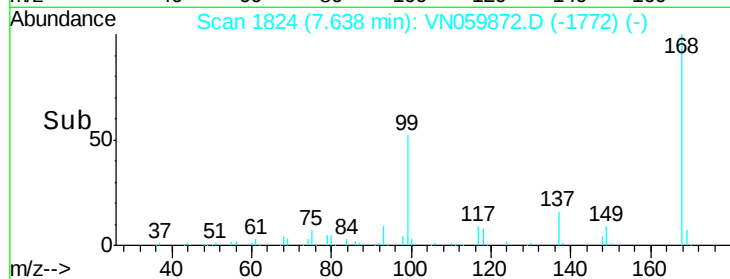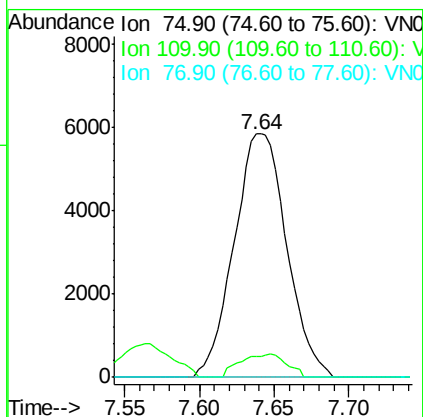

#38
 Carbon Tetrachloride
 Concen: 6.46 ug/l
 RT: 7.64 min Scan# 1825
 Delta R.T. -0.11 min
 Lab File: VN059872.D
 Acq: 27 Jan 2020 15:06

Tgt Ion: 117 Resp: 19760
 Ion Ratio Lower Upper
 117 100
 119 4.4 76.5 114.7#
 121 0.0 25.1 37.7#


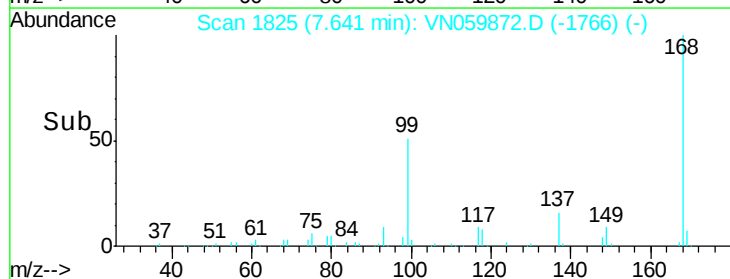
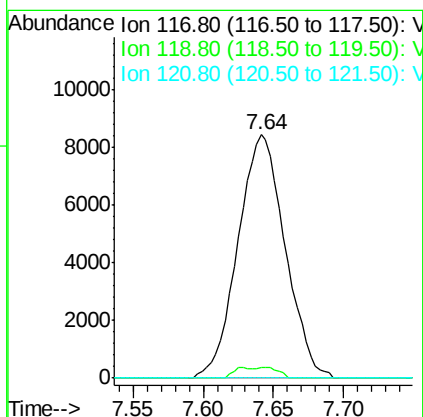
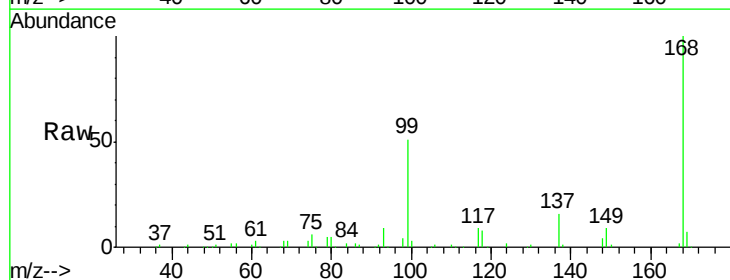


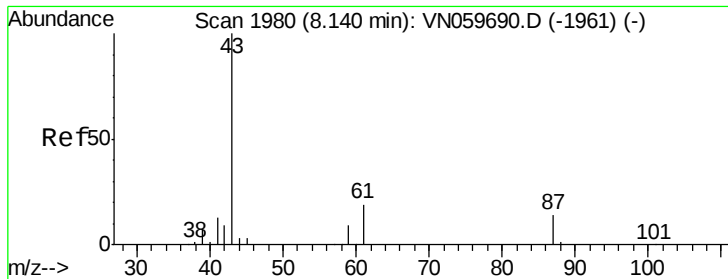

#43
Isopropyl Acetate
Concen: 10.77 ug/l
RT: 8.14 min Scan# 1980
Delta R.T. 0.00 min
Lab File: VN059872.D
Acq: 27 Jan 2020 15:06




Instrument :
MSVOA_N
ClientSampled :
PB126348TB


Tgt Ion: 43 Resp: 48882
Ion Ratio Lower Upper
43 100
61 20.4 20.2 30.2
87 15.1 9.5 14.3#

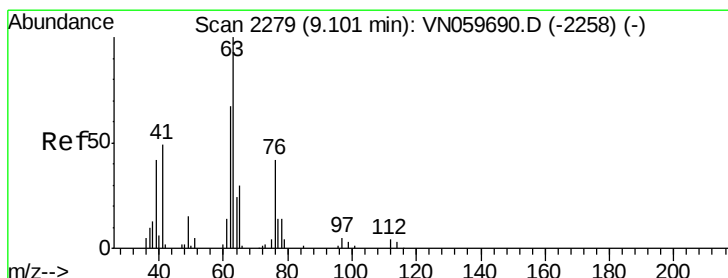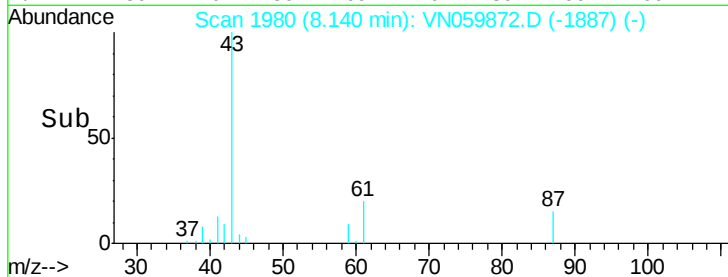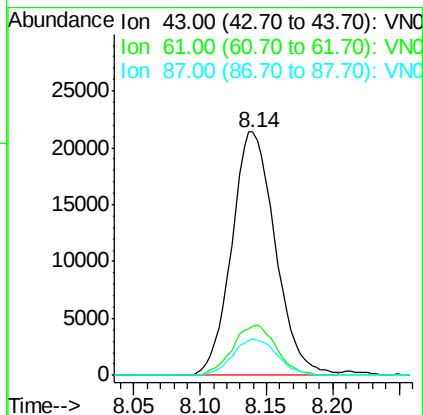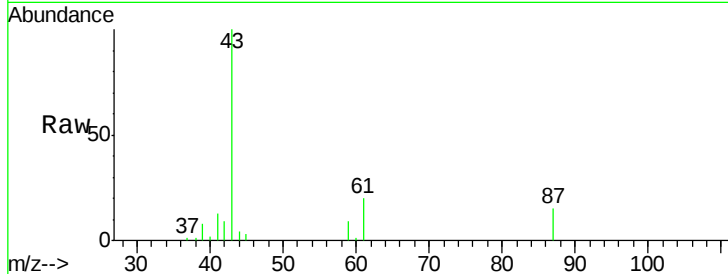

#45
1,2-Dichloropropane
Concen: 0.49 ug/l
RT: 9.25 min Scan# 2324
Delta R.T. 0.14 min
Lab File: VN059872.D
Acq: 27 Jan 2020 15:06

Tgt Ion: 63 Resp: 1024
Ion Ratio Lower Upper
63 100
65 0.0 24.9 37.3#


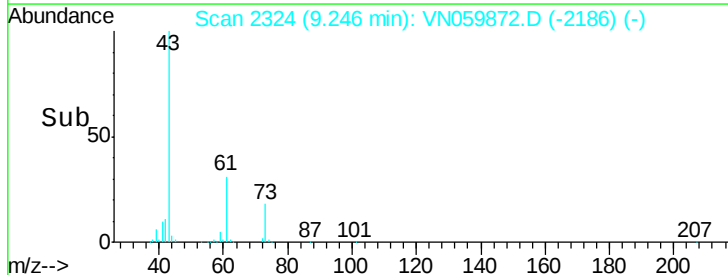
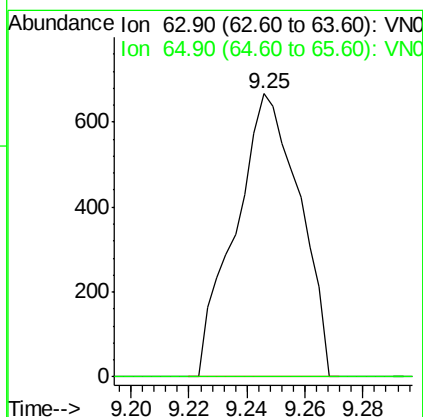
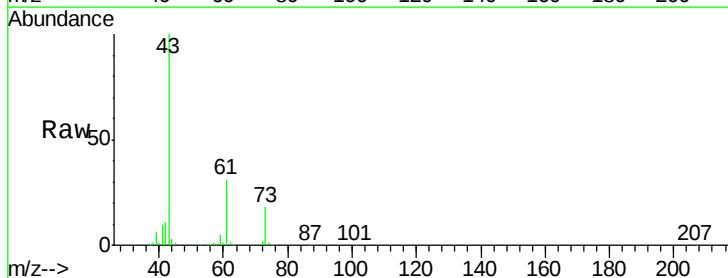


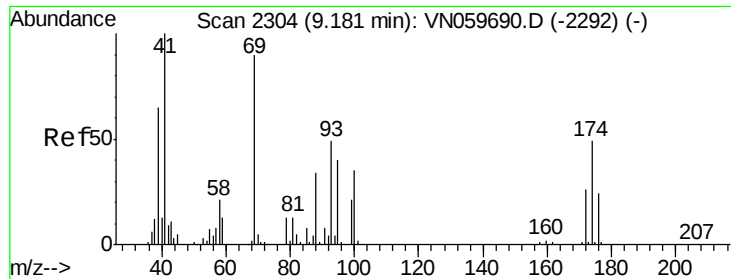

#48
Methyl methacrylate
Concen: 38.10 ug/l
RT: 9.25 min Scan# 2325
Delta R.T. 0.07 min
Lab File: VN059872.D
Acq: 27 Jan 2020 15:06




Instrument :
MSVOA_N
ClientSampleId :
PB126348TB


Tgt Ion: 41 Resp: 77350
Ion Ratio Lower Upper
41 100
69 0.0 64.4 96.6#
39 57.3 51.3 76.9

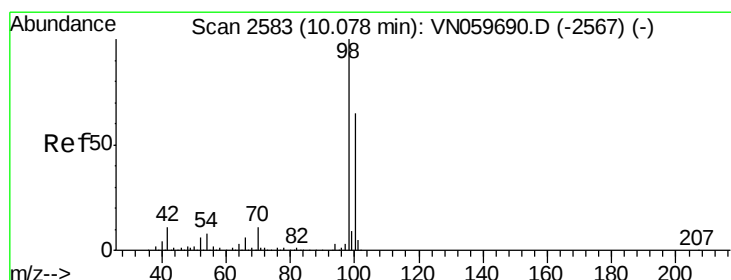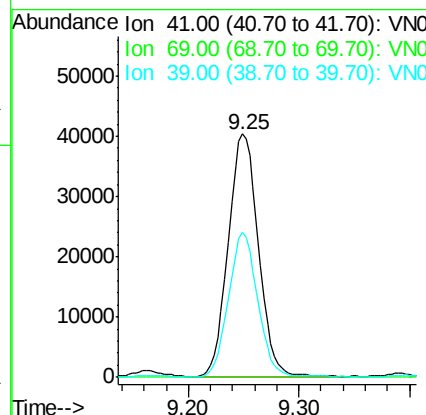

#50
Toluene-d8
Concen: 50.33 ug/l
RT: 10.08 min Scan# 2582
Delta R.T. -0.00 min
Lab File: VN059872.D
Acq: 27 Jan 2020 15:06

Tgt Ion: 98 Resp: 375707
Ion Ratio Lower Upper
98 100
100 64.7 51.2 76.8

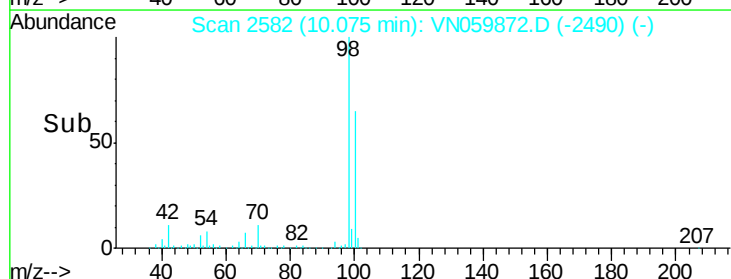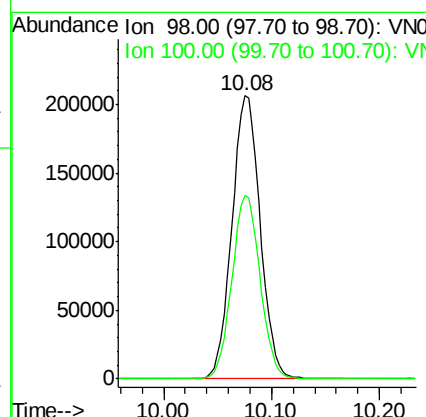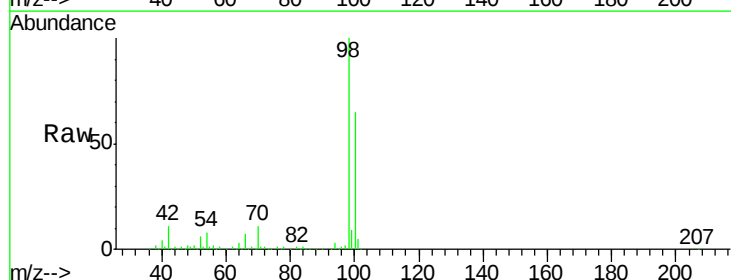



#51

4-Methyl-2-Pentanone

Concen: 1.37 ug/l

RT: 9.97 min Scan# 2548

Delta R.T. -0.00 min

Lab File: VN059872.D

Acq: 27 Jan 2020 15:06

Instrument :

MSVOA_N

ClientSampled :





PB126348TB

Tgt Ion: 43 Resp: 3596

Ion Ratio Lower Upper

43 100

58 30.0 29.8 44.8

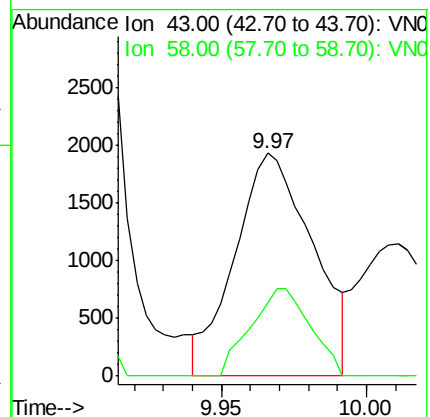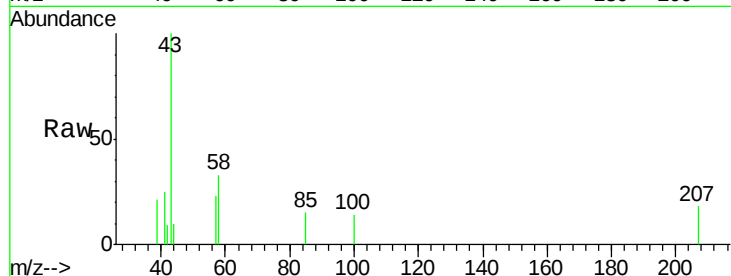

#54

cis-1,3-Dichloropropene

Concen: 6.89 ug/l

RT: 9.89 min Scan# 2524

Delta R.T. 0.06 min

Lab File: VN059872.D

Acq: 27 Jan 2020 15:06




Tgt Ion: 75 Resp: 23899


Ion Ratio Lower Upper

75 100

77 0.0 25.1 37.7#

39 28.2 46.1 69.1#



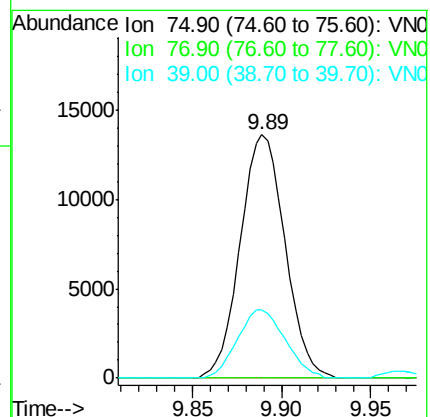





#57
 1,3-Dichloropropane
 Concen: 1.19 ug/l
 RT: 10.75 min Scan# 2792
 Delta R.T. 0.05 min
 Lab File: VN059872.D
 Acq: 27 Jan 2020 15:06




Instrument :
 MSVOA_N
 ClientSampleID :
 PB126348TB


Tgt Ion: 76 Resp: 3954
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.8 38.8#

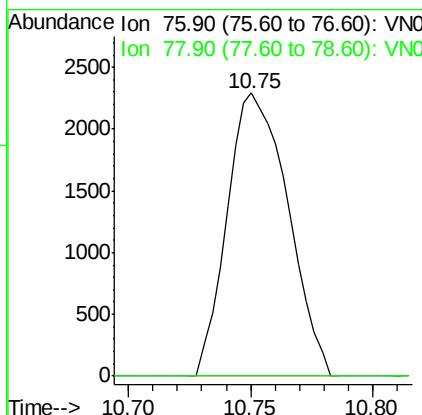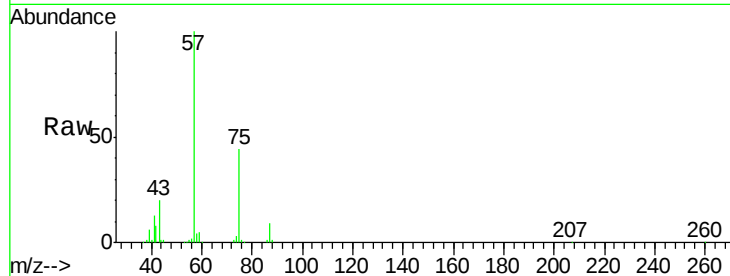

#59
 2-Hexanone
 Concen: 26.31 ug/l
 RT: 10.75 min Scan# 2793
 Delta R.T. 0.01 min
 Lab File: VN059872.D
 Acq: 27 Jan 2020 15:06

Tgt Ion: 43 Resp: 50859
 Ion Ratio Lower Upper
 43 100
 58 20.8 25.8 77.3#

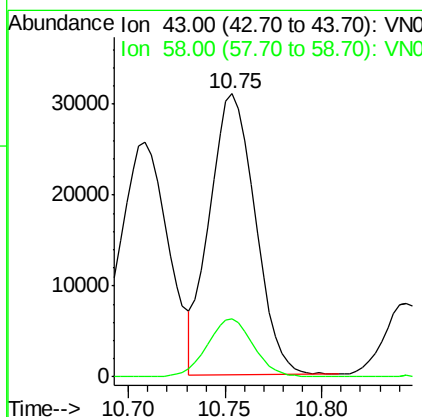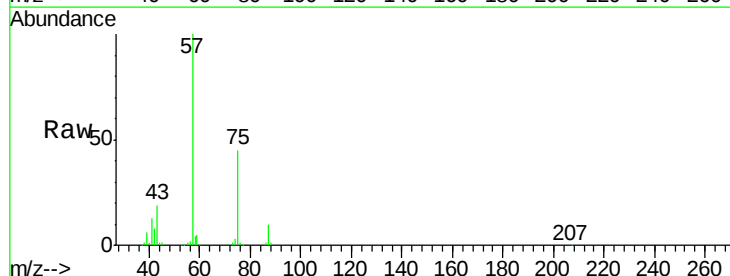


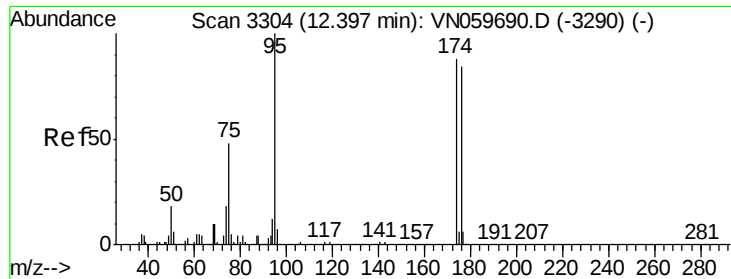

#62
4-Bromofluorobenzene
Concen: 45.66 ug/l
RT: 12.40 min Scan# 3304
Delta R.T. 0.00 min
Lab File: VN059872.D
Acq: 27 Jan 2020 15:06

Instrument :
MSVOA_N
ClientSampleId :
PB126348TB




Tgt Ion	Ratio	Lower	Upper
95	100		
174	89.0	0.0	151.4
176	85.9	0.0	146.0

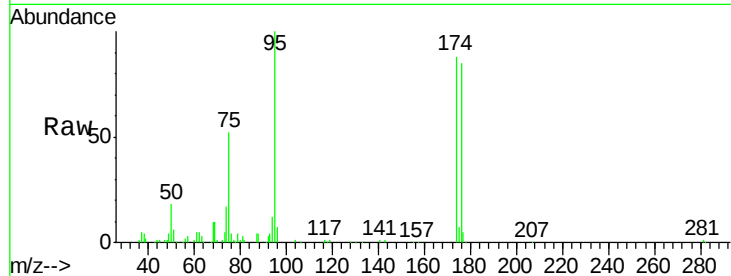

Abundance Ion 94.90 (94.60 to 95.60): VN059872.D (-3211) (-)


Ion 173.80 (173.50 to 174.50): VN059872.D (-3211) (-)

Ion 175.80 (175.50 to 176.50): VN059872.D (-3211) (-)

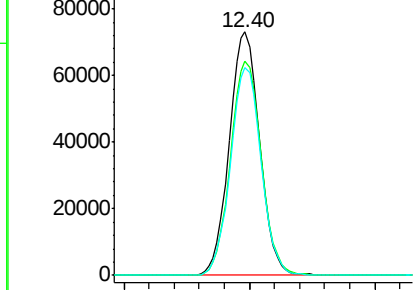

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.40 min Scan# 2994
Delta R.T. 0.00 min
Lab File: VN059872.D
Acq: 27 Jan 2020 15:06



Tgt Ion	Ratio	Lower	Upper
117	100		
82	52.0	45.9	68.9
119	31.8	25.5	38.3




Abundance Ion 116.90 (116.60 to 117.60): VN059872.D (-2901) (-)

Ion 82.00 (81.70 to 82.70): VN059872.D (-2901) (-)

Ion 118.90 (118.60 to 119.60): VN059872.D (-2901) (-)

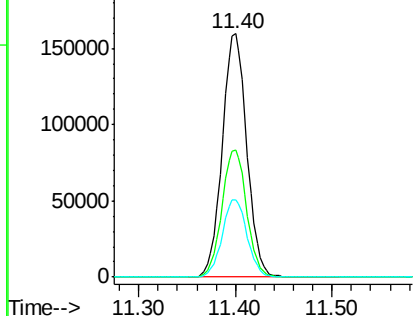



#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 13.34 min Scan# 3597

Delta R.T. 0.00 min

Lab File: VN059872.D

Acq: 27 Jan 2020 15:06

Instrument :

MSVOA_N

ClientSampled :

PB126348TB


Tgt Ion:152 Resp: 115340

Ion Ratio Lower Upper

152 100

115 57.0 30.3 90.9




150 154.0 0.0 345.2



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

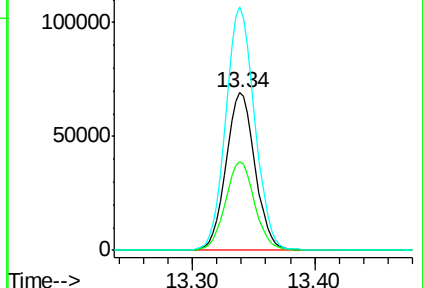

#74

N-ethyl acetate

Concen: 0.39 ug/l

RT: 12.03 min Scan# 3189

Delta R.T. -0.04 min

Lab File: VN059872.D

Acq: 27 Jan 2020 15:06

Tgt Ion: 43 Resp: 1296


Ion Ratio Lower Upper

43 100

70 0.0 31.3 46.9#

55 0.0 19.8 29.6#

61 0.0 18.3 27.5#






Abundance Ion 43.00 (42.70 to 43.70): VNO

Ion 70.00 (69.70 to 70.70): VNO

Ion 55.00 (54.70 to 55.70): VNO

Ion 61.00 (60.70 to 61.70): VNO

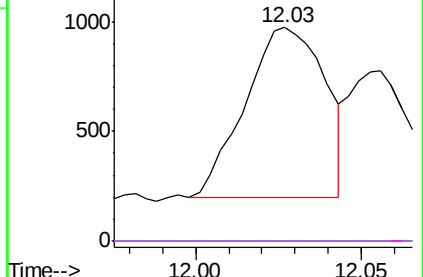

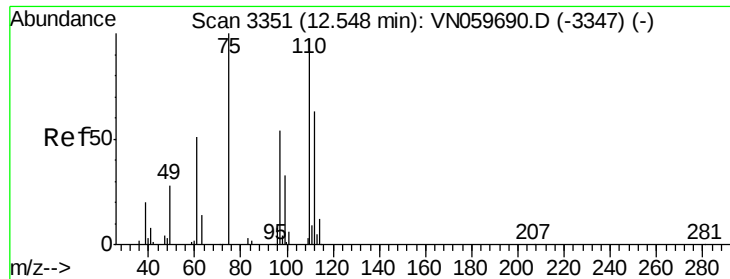

#76

1,2,3-Trichloropropane

Concen: 32.02 ug/l

RT: 12.40 min Scan# 3304

Delta R.T. -0.15 min

Lab File: VN059872.D

Acq: 27 Jan 2020 15:06

Instrument :

MSVOA_N

ClientSampleId :


PB126348TB

Tgt Ion: 75 Resp: 62145

Ion Ratio Lower Upper

75 100

77 1.1 0.0 0.0#

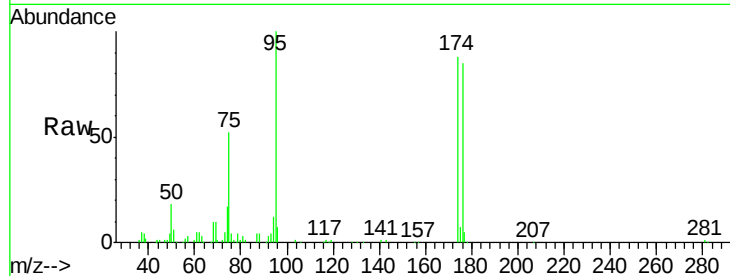

Abundance Ion 74.90 (74.60 to 75.60): VN059872.D (-3258) (-)

Ion 77.00 (76.70 to 77.70): VN059872.D (-3258) (-)

12.40

40000

30000



20000

10000

0

12.35 12.40 12.45

Time-->



#77

Bromobenzene

Concen: 1.02 ug/l

RT: 12.53 min Scan# 3345

Delta R.T. 0.01 min

Lab File: VN059872.D

Acq: 27 Jan 2020 15:06


Tgt Ion: 156 Resp: 2182

Ion Ratio Lower Upper

156 100

77 24.2 115.8 347.4#

158 0.0 49.2 147.6#



Abundance Ion 155.80 (155.50 to 156.50): VN059872.D (-3250) (-)

Ion 77.00 (76.70 to 77.70): VN059872.D (-3250) (-)

Ion 157.80 (157.50 to 158.50): VN059872.D (-3250) (-)

12.53


1000


500

0

12.45 12.50 12.55

Time-->









#80
 1,3,5-Trimethylbenzene
 Concen: 0.98 ug/l
 RT: 12.73 min Scan# 3408
 Delta R.T. 0.00 min
 Lab File: VN059872.D
 Acq: 27 Jan 2020 15:06




Instrument :
 MSVOA_N
 ClientSampled :
 PB126348TB


Tgt Ion: 105 Resp: 6952
 Ion Ratio Lower Upper
 105 100
 120 49.7 24.1 72.4

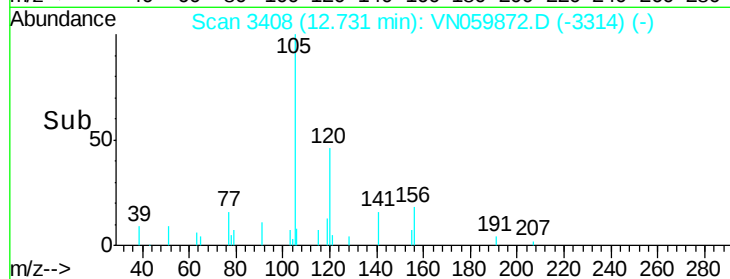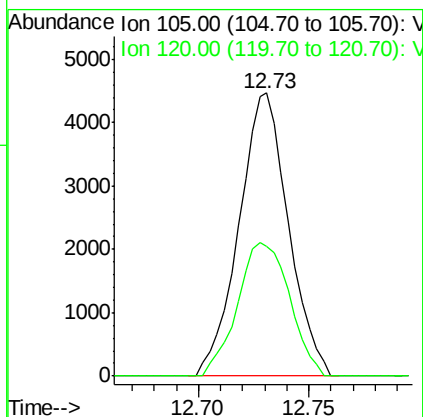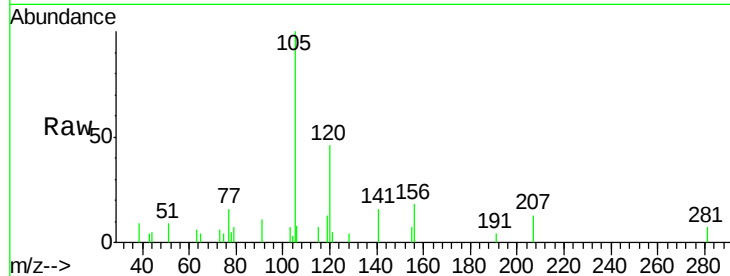

#81
 trans-1,4-Dichloro-2-butene
 Concen: 68.75 ug/l
 RT: 12.40 min Scan# 3304
 Delta R.T. 0.10 min
 Lab File: VN059872.D
 Acq: 27 Jan 2020 15:06

Tgt Ion: 75 Resp: 62145
 Ion Ratio Lower Upper
 75 100
 53 0.0 78.1 117.1#
 89 0.0 35.4 53.2#

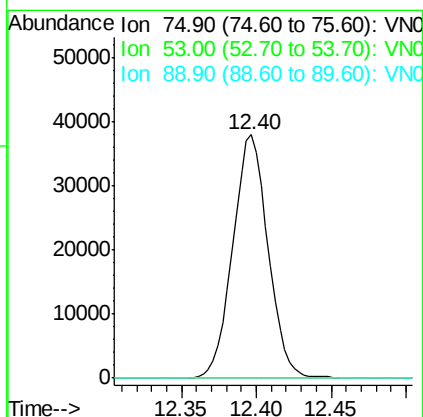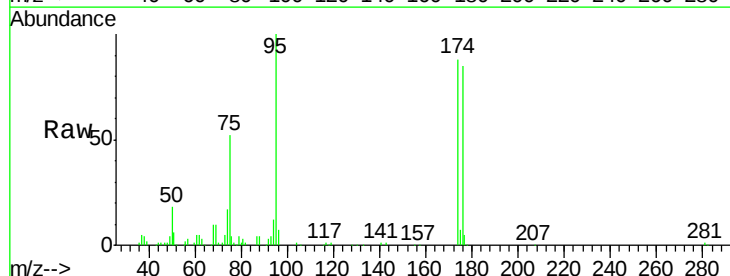

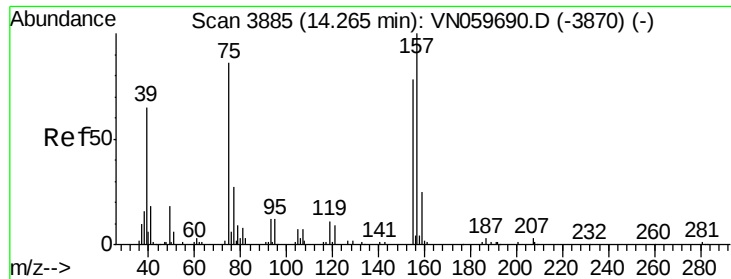

#92

1,2-Dibromo-3-Chloropropane

Concen: Below Cal

RT: 14.25 min Scan# 3880

Delta R.T. -0.02 min

Lab File: VN059872.D

Acq: 27 Jan 2020 15:06

Instrument :

MSVOA_N

ClientSampled :

PB126348TB


Tgt Ion: 75 Resp: 240

Ion Ratio Lower Upper

75 100

155 0.0 37.0 110.9#

157 0.0 48.4 145.2#



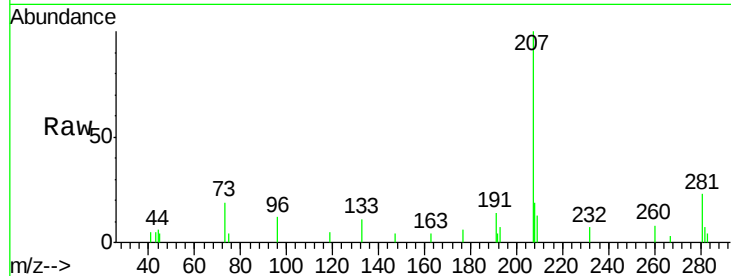


Abundance Ion 74.90 (74.60 to 75.60): VN059690.D (-3870) (-)

Ion 154.80 (154.50 to 155.50): VN059690.D (-3870) (-)

Ion 156.80 (156.50 to 157.50): VN059690.D (-3870) (-)

Time-->

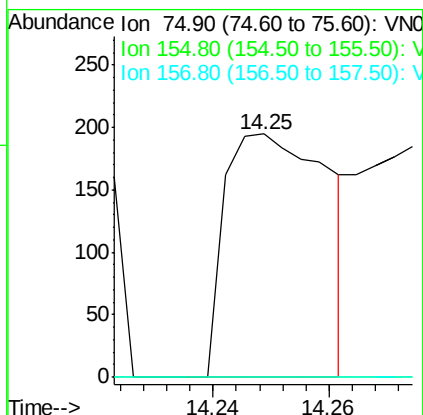

#93

1,2,4-Trichlorobenzene

Concen: 0.47 ug/l

RT: 14.91 min Scan# 4085

Delta R.T. 0.00 min

Lab File: VN059872.D

Acq: 27 Jan 2020 15:06


Tgt Ion: 180 Resp: 1046

Ion Ratio Lower Upper

180 100

182 97.4 46.9 140.7

145 53.5 15.0 45.1#






Abundance Ion 179.80 (179.50 to 180.50): VN059690.D (-4071) (-)

Ion 181.80 (181.50 to 182.50): VN059690.D (-4071) (-)

Ion 144.80 (144.50 to 145.50): VN059690.D (-4071) (-)

Time-->

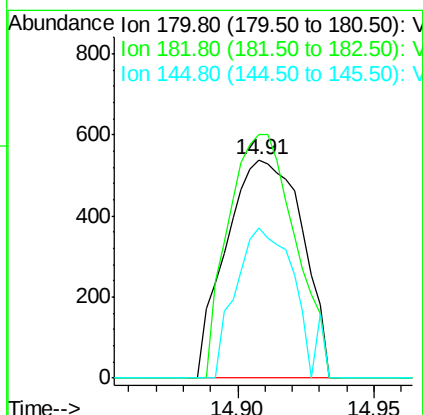

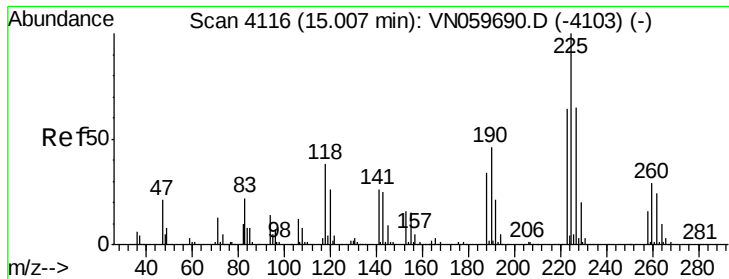

#94

Hexachlorobutadiene

Concen: 0.24 ug/l

RT: 15.01 min Scan# 4117

Delta R.T. 0.00 min

Lab File: VN059872.D

Acq: 27 Jan 2020 15:06

Instrument :

MSVOA_N

ClientSampled :

PB126348TB


Tgt Ion:225 Resp: 296

Ion Ratio Lower Upper

225 100

223 63.2 31.8 95.3


227 32.8 32.1 96.5

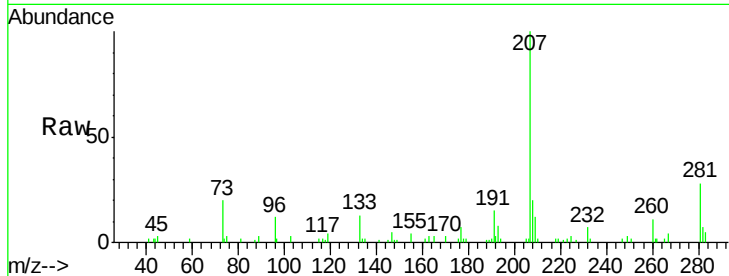



Abundance Ion 224.70 (224.40 to 225.40): V

Ion 222.70 (222.40 to 223.40): V

Ion 226.70 (226.40 to 227.40): V

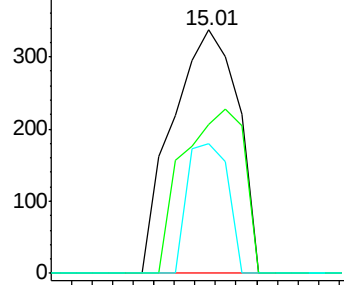

Time-->

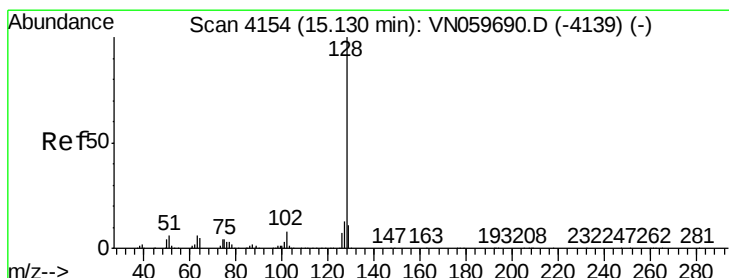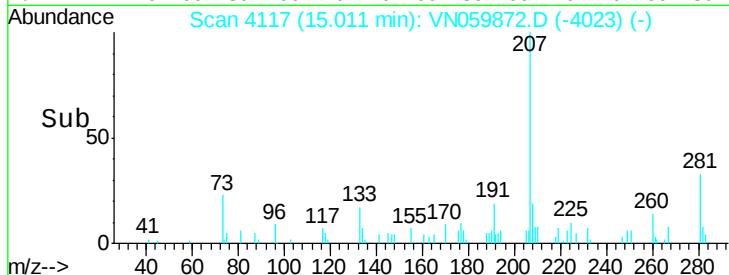

#95

Naphthalene

Concen: 2.60 ug/l

RT: 15.13 min Scan# 4154

Delta R.T. 0.00 min

Lab File: VN059872.D

Acq: 27 Jan 2020 15:06


Tgt Ion:128 Resp: 16327

Ion Ratio Lower Upper

128 100

127 13.5 10.4 15.6


129 11.7 8.6 12.8

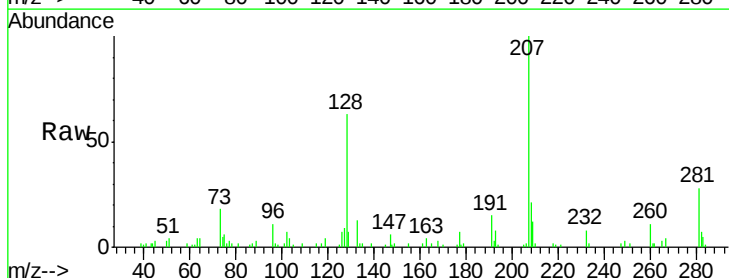


Abundance Ion 128.00 (127.70 to 128.70): V


Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

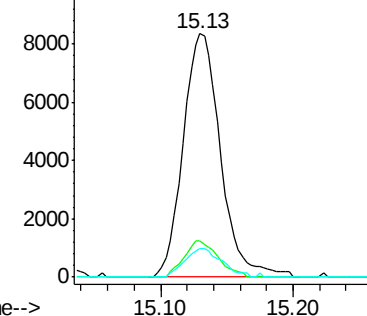

Time-->

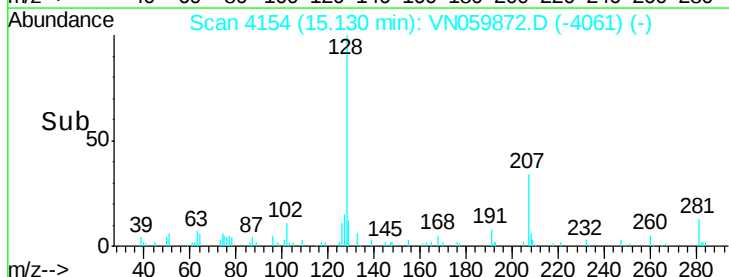



#96
 1,2,3-Trichlorobenzene
 Concen: 0.78 ug/l
 RT: 15.32 min Scan# 4212
 Delta R.T. 0.01 min
 Lab File: VN059872.D
 Acq: 27 Jan 2020 15:06

Instrument :
 MSVOA_N
 ClientSampleId :
 PB126348TB

Tgt Ion	Ratio	Lower	Upper
180	100		
182	83.8	47.4	142.3
145	37.0	16.3	48.9

