

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012721\
 Data File : VN065624.D
 Acq On : 27 Jan 2021 12:57
 Operator : JC/MD
 Sample : M1190-03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jan 28 02:11:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012521W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jan 25 13:47:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.624	168	204004	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.547	114	355478	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.376	117	304949	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.315	152	112864	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.987	65	128904	48.03	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	96.06%		
35) Dibromofluoromethane	7.550	113	103571	49.17	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	98.34%		
50) Toluene-d8	10.058	98	443381	53.55	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	107.10%		
62) 4-Bromofluorobenzene	12.373	95	145261	48.72	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	97.44%		
Target Compounds						
					Qvalue	
13) Acrolein	3.569	56	359	18.85	ug/l #	15
16) Acetone	3.782	43	12027	11.51	ug/l	97
18) Methyl Acetate	4.303	43	1026	0.35	ug/l #	51
19) Methyl tert-butyl Ether	5.003	73	6187	0.75	ug/l #	90
20) Methylene Chloride	4.505	84	2719	0.94	ug/l #	82
22) Diisopropyl ether	5.901	45	3287	0.35	ug/l #	80
25) 2-Butanone	6.804	43	1233	0.75	ug/l	98
29) Tetrahydrofuran	7.187	42	268	0.23	ug/l #	32
31) Cyclohexane	7.621	56	5267	1.04	ug/l #	1
36) 1,1-Dichloropropene	7.624	75	17024	4.76	ug/l #	47
38) Carbon Tetrachloride	7.624	117	19790	6.72	ug/l #	17
40) Benzene	8.000	78	2351	0.22	ug/l	96
51) 4-Methyl-2-Pentanone	9.955	43	2185	0.65	ug/l #	65
52) Toluene	10.122	92	26464	4.09	ug/l	98
68) m/p-Xylenes	11.595	106	2330	0.54	ug/l	88
69) o-Xylene	11.916	106	36074	8.58	ug/l	96
70) Styrene	11.926	104	3297	0.48	ug/l #	1
71) Bromoform	12.376	173	670	0.43	ug/l #	1
76) 1,2,3-Trichloropropane	12.373	75	67554	22.89	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.704	105	35439	4.21	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.373	75	67554	58.63	ug/l #	12
84) 1,2,4-Trimethylbenzene	13.010	105	4451	0.53	ug/l	95
85) sec-Butylbenzene	13.145	105	3470	0.37	ug/l	97
86) p-Isopropyltoluene	13.260	119	3318	0.40	ug/l	94
89) n-Butylbenzene	13.553	91	5231	0.70	ug/l #	1
90) Hexachloroethane	13.858	117	3770	2.58	ug/l #	12
92) 1,2-Dibromo-3-Chloropr...	14.222	75	393	0.68	ug/l #	1
93) 1,2,4-Trichlorobenzene	14.878	180	909	3.74	ug/l #	1
94) Hexachlorobutadiene	14.974	225	288	0.52	ug/l	63
95) Naphthalene	15.100	128	6413	4.27	ug/l #	86
96) 1,2,3-Trichlorobenzene	15.273	180	1205	3.35	ug/l #	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012721\
Data File : VN065624.D
Acq On : 27 Jan 2021 12:57
Operator : JC/MD
Sample : M1190-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :


Quant Time: Jan 28 02:11:40 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012521W.M
Quant Title : SW846 8260
QLast Update : Mon Jan 25 13:47:28 2021
Response via : Initial Calibration

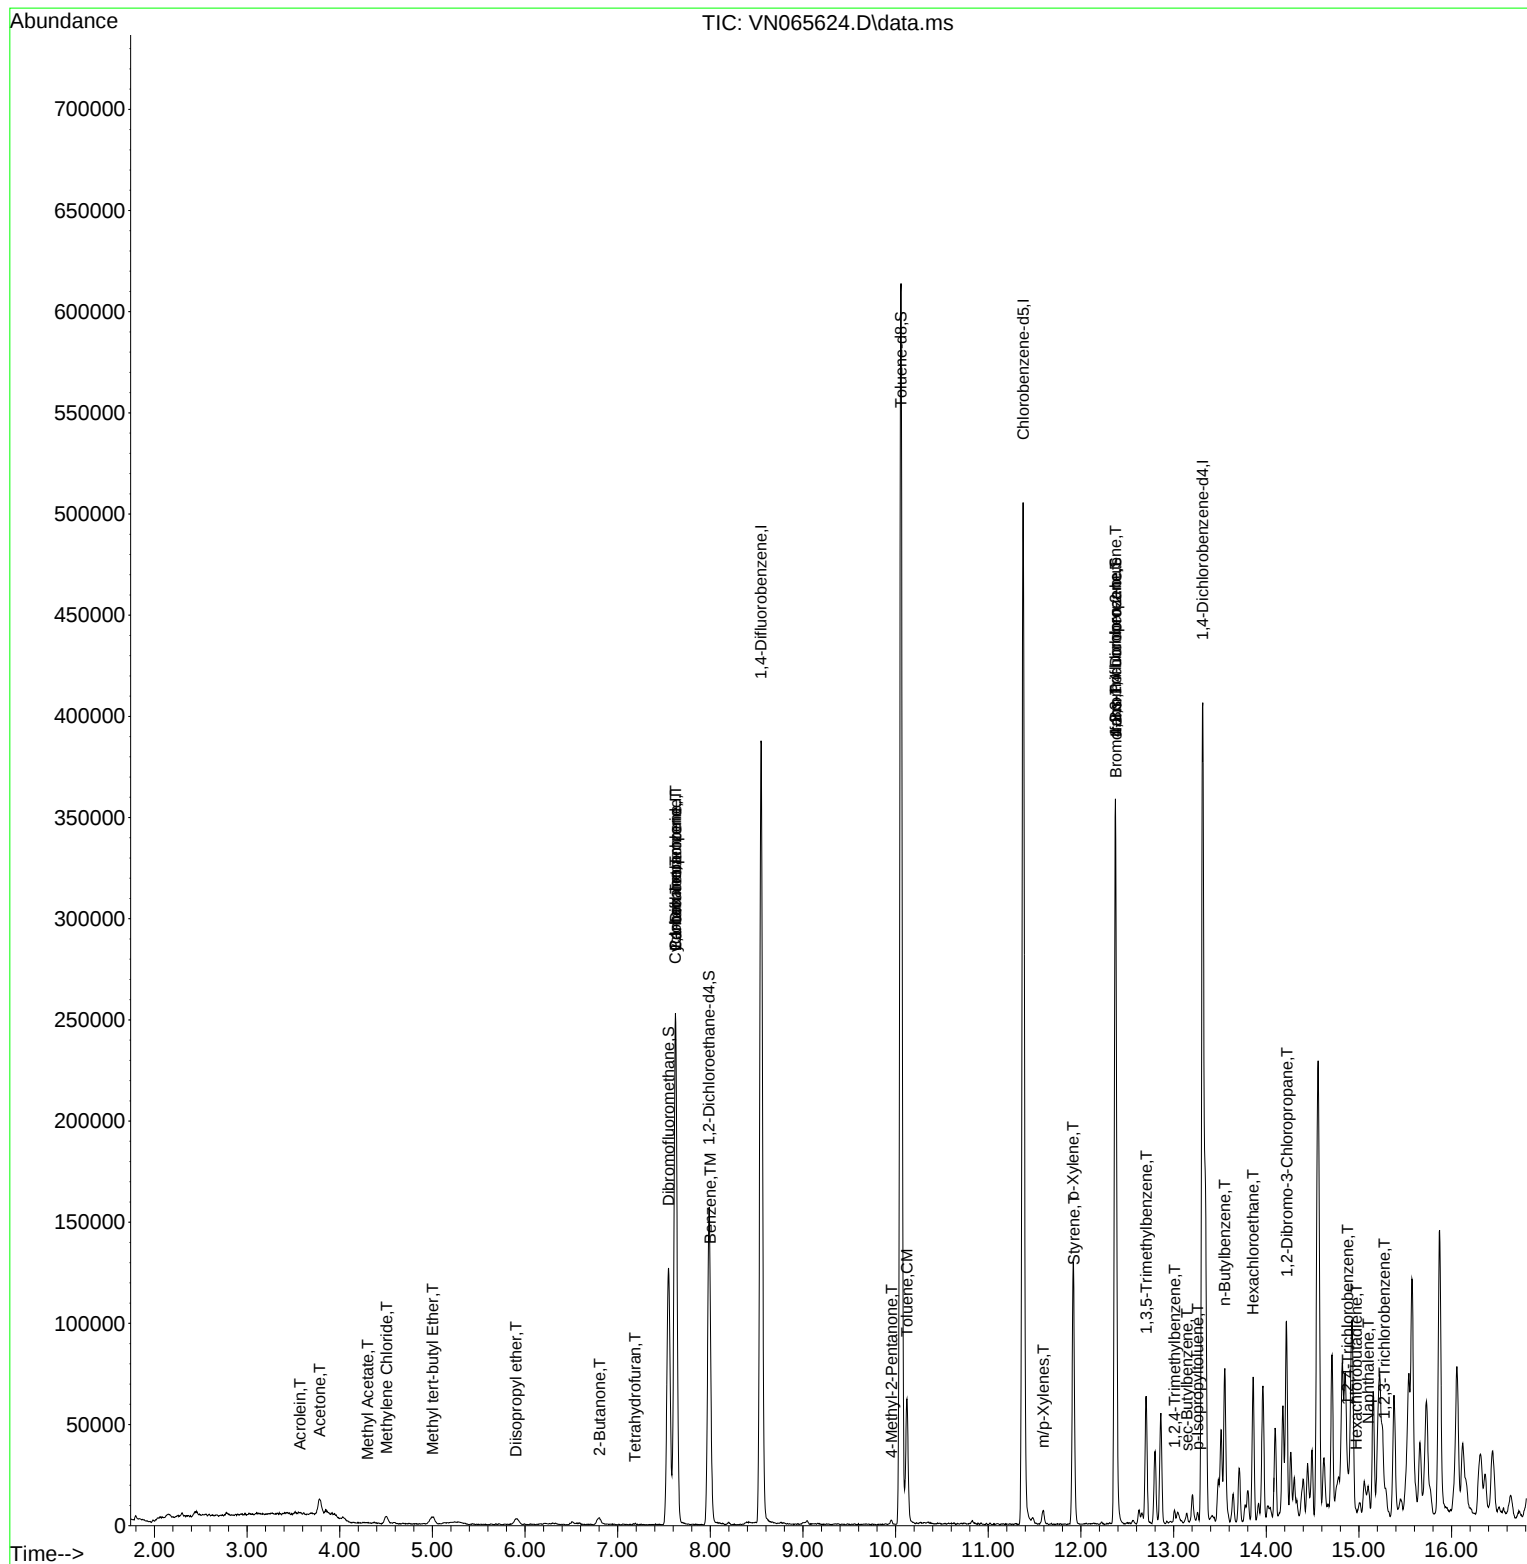






#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.624 min Scan# 1830
Delta R.T. -0.000 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57

Instrument :
MSVOA_N
ClientSampleId :






Tgt Ion:168 Resp: 204004
Ion Ratio Lower Upper
168 100
99 59.9 42.6 63.8

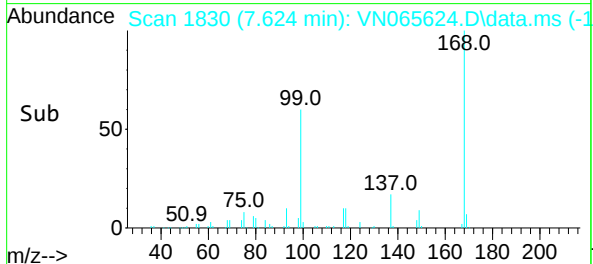

#13
Acrolein
Concen: 18.85 ug/l
RT: 3.569 min Scan# 569
Delta R.T. 0.000 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57


Tgt Ion: 56 Resp: 359
Ion Ratio Lower Upper
56 100
55 0.0 56.0 84.0#








#16
Acetone
Concen: 11.51 ug/l
RT: 3.782 min Scan# 635
Delta R.T. -0.000 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57

Instrument :
MSVOA_N
ClientSampled :



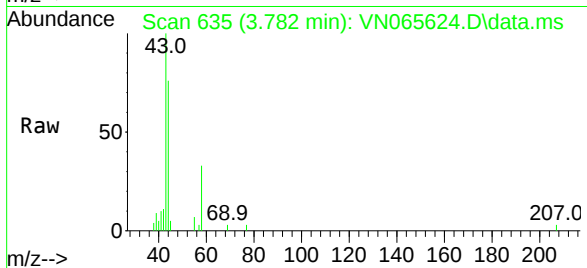



Tgt Ion: 43 Resp: 12027
Ion Ratio Lower Upper
43 100
58 35.6 27.0 40.6

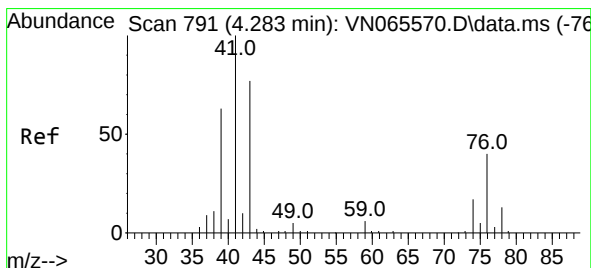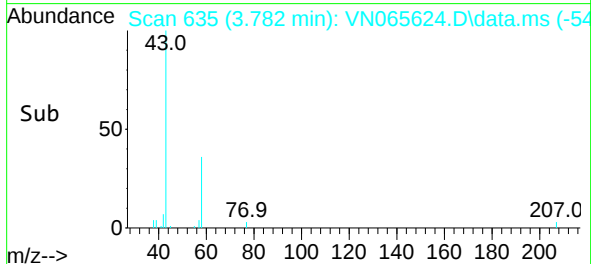

#18
Methyl Acetate
Concen: 0.35 ug/l
RT: 4.303 min Scan# 797
Delta R.T. 0.020 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57

Tgt Ion: 43 Resp: 1026
Ion Ratio Lower Upper
43 100
74 0.0 19.5 29.3#

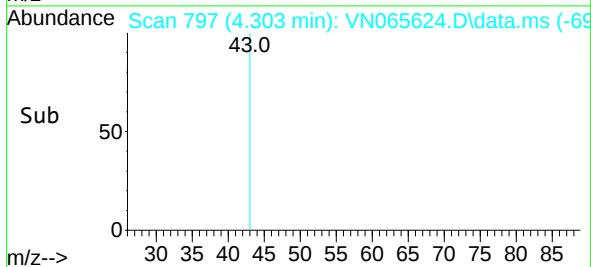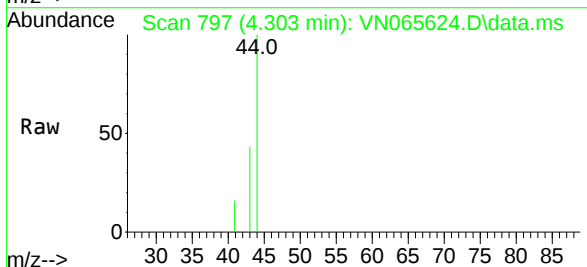







#19

Methyl tert-butyl Ether
 Concen: 0.75 ug/l
 RT: 5.003 min Scan# 1015
 Delta R.T. 0.006 min
 Lab File: VN065624.D
 Acq: 27 Jan 2021 12:57

Instrument :
 MSVOA_N
 ClientSampled :




Tgt Ion: 73 Resp: 6187
 Ion Ratio Lower Upper
 73 100
 57 26.3 17.3 25.9#

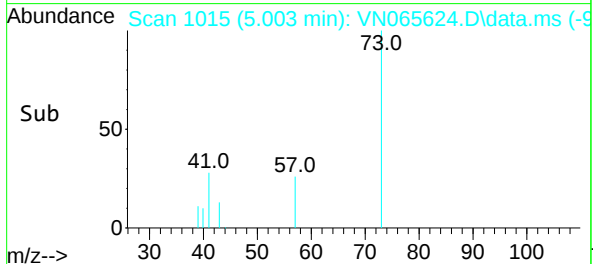


#20

Methylene Chloride
 Concen: 0.94 ug/l
 RT: 4.505 min Scan# 860
 Delta R.T. 0.003 min
 Lab File: VN065624.D
 Acq: 27 Jan 2021 12:57

Tgt Ion: 84 Resp: 2719
 Ion Ratio Lower Upper
 84 100
 49 146.4 94.6 141.8#
 51 46.2 29.9 44.9#
 86 69.9 51.4 77.2





#22

Diisopropyl ether

Concen: 0.35 ug/l

RT: 5.901 min Scan# 1294

Delta R.T. -0.006 min

Lab File: VN065624.D

Acq: 27 Jan 2021 12:57

Tgt Ion: 45 Resp: 3287





Ion Ratio Lower Upper

45 100

43 39.4 48.9 73.3#

87 24.0 23.7 35.5

59 12.0 9.9 14.9



#25

2-Butanone

Concen: 0.75 ug/l

RT: 6.804 min Scan# 1575

Delta R.T. 0.013 min

Lab File: VN065624.D




Acq: 27 Jan 2021 12:57


Tgt Ion: 43 Resp: 1233

Ion Ratio Lower Upper

43 100

72 27.6 23.1 34.7









#29
Tetrahydrofuran
Concen: 0.23 ug/l
RT: 7.187 min Scan# 1694
Delta R.T. 0.016 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 42 Resp: 268
Ion Ratio Lower Upper
42 100
72 0.0 36.6 55.0#
71 0.0 34.3 51.5#

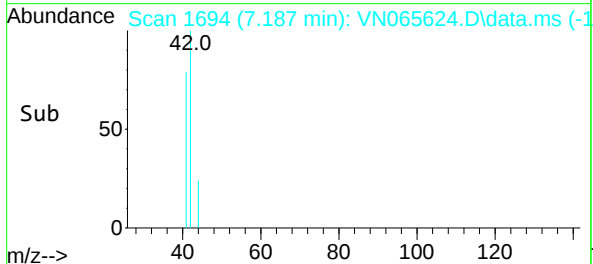

#31
Cyclohexane
Concen: 1.04 ug/l
RT: 7.621 min Scan# 1829
Delta R.T. 0.010 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57

Tgt Ion: 56 Resp: 5267
Ion Ratio Lower Upper
56 100
69 167.3 26.6 39.8#
84 154.9 70.4 105.6#





#33

1,2-Dichloroethane-d4

Concen: 48.03 ug/l

RT: 7.987 min Scan# 1943

Delta R.T. 0.000 min





Lab File: VN065624.D

Acq: 27 Jan 2021 12:57

Tgt Ion: 65 Resp: 128904

Ion Ratio Lower Upper

Ion	Ratio	Lower	Upper
65	100		
67	55.8	0.0	107.2

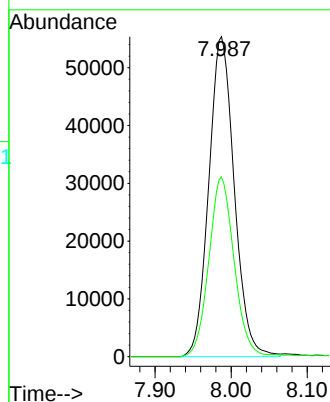

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 8.547 min Scan# 2117

Delta R.T. -0.003 min




Lab File: VN065624.D


Acq: 27 Jan 2021 12:57

Tgt Ion: 114 Resp: 355478

Ion Ratio Lower Upper

Ion	Ratio	Lower	Upper
114	100		
63	22.2	0.0	38.6
88	16.5	0.0	30.6

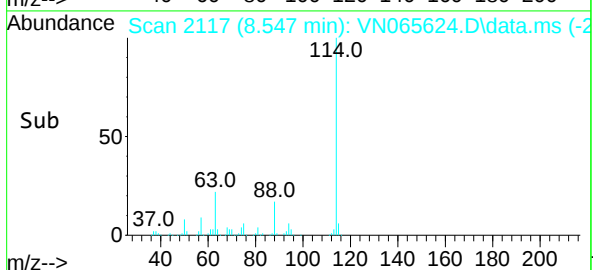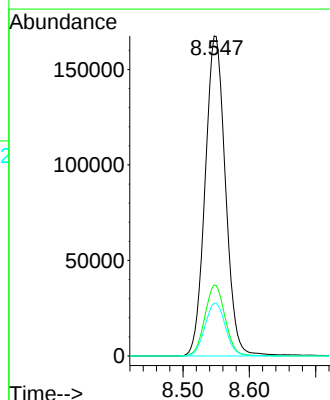



#35

Dibromofluoromethane

Concen: 49.17 ug/l

RT: 7.550 min Scan# 1807

Delta R.T. 0.003 min

Lab File: VN065624.D

Acq: 27 Jan 2021 12:57





Tgt Ion:113 Resp: 103571

Ion Ratio Lower Upper

113 100

111 102.6 82.2 123.2

192 17.9 15.4 23.0

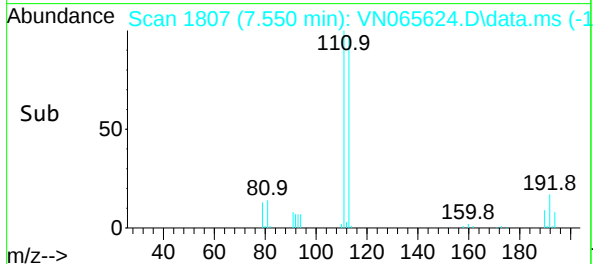

#36

1,1-Dichloropropene

Concen: 4.76 ug/l

RT: 7.624 min Scan# 1830

Delta R.T. -0.125 min

Lab File: VN065624.D

Acq: 27 Jan 2021 12:57




Tgt Ion: 75 Resp: 17024


Ion Ratio Lower Upper

75 100

110 6.3 18.2 54.6#


77 0.0 24.9 37.3#

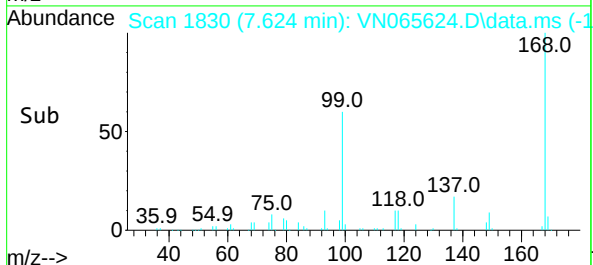






#38
Carbon Tetrachloride
Concen: 6.72 ug/l
RT: 7.624 min Scan# 1830
Delta R.T. -0.106 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57

Instrument :
MSVOA_N
ClientSampled :



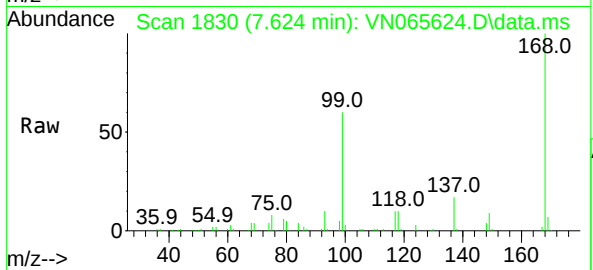



Tgt Ion:117 Resp: 19790
Ion Ratio Lower Upper
117 100
119 5.4 76.0 114.0#
121 0.0 24.5 36.7#

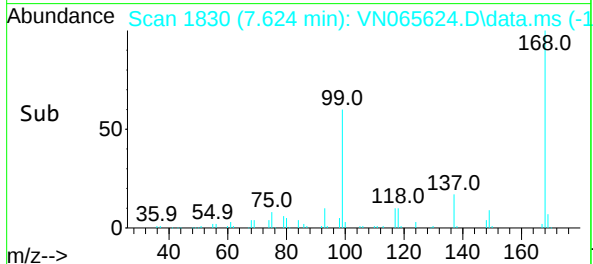

#40
Benzene
Concen: 0.22 ug/l
RT: 8.000 min Scan# 1947
Delta R.T. 0.000 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57

Tgt Ion: 78 Resp: 2351
Ion Ratio Lower Upper
78 100
77 21.8 19.0 28.4







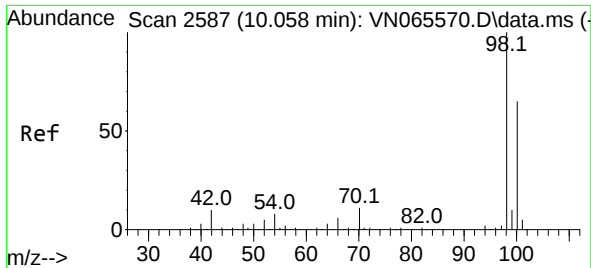

#50
Toluene-d8
Concen: 53.55 ug/l
RT: 10.058 min Scan# 2587
Delta R.T. -0.000 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 98 Resp: 443381
Ion Ratio Lower Upper
98 100
100 64.4 50.5 75.7

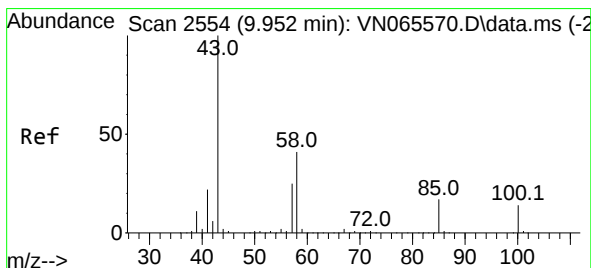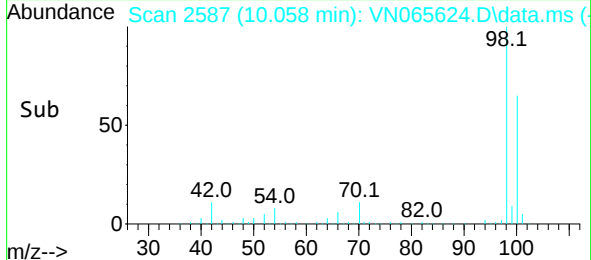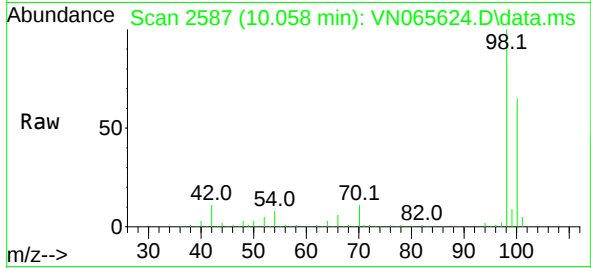

#51
4-Methyl-2-Pentanone
Concen: 0.65 ug/l
RT: 9.955 min Scan# 2555
Delta R.T. 0.003 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57

Tgt Ion: 43 Resp: 2185
Ion Ratio Lower Upper
43 100
58 19.1 32.5 48.7#


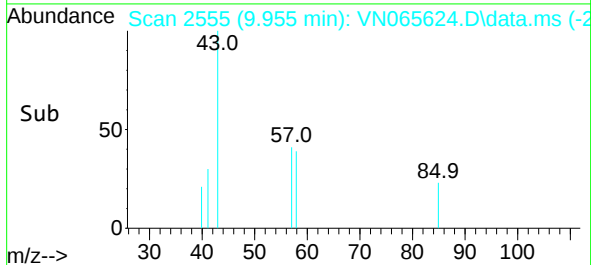

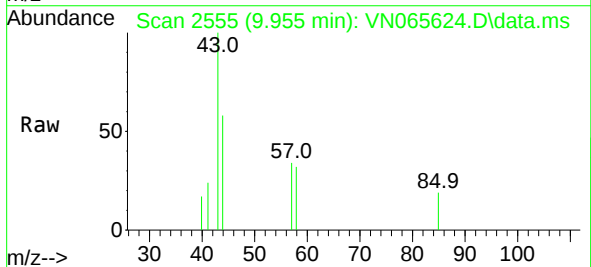


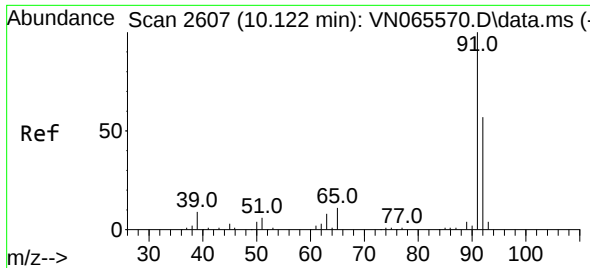

#52
Toluene
Concen: 4.09 ug/l
RT: 10.122 min Scan# 2607
Delta R.T. 0.000 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 92 Resp: 26464
Ion Ratio Lower Upper
92 100
91 173.8 140.7 211.1

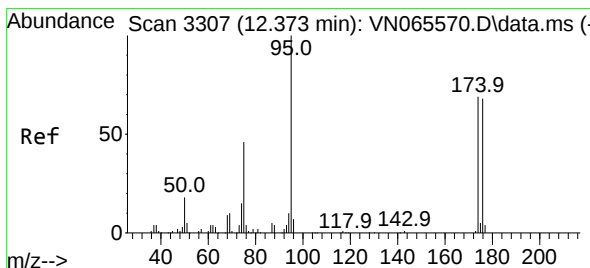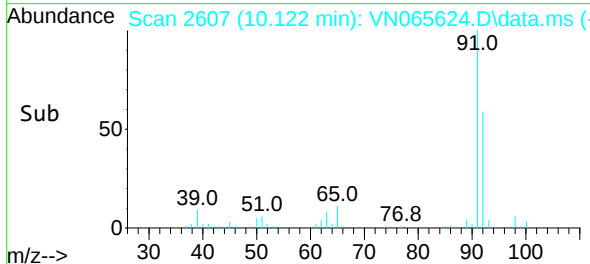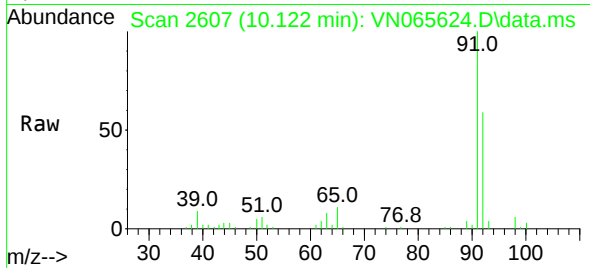

#62
4-Bromofluorobenzene
Concen: 48.72 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. -0.000 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57

Tgt Ion: 95 Resp: 145261
Ion Ratio Lower Upper
95 100
174 68.0 0.0 169.0
176 65.8 0.0 162.4


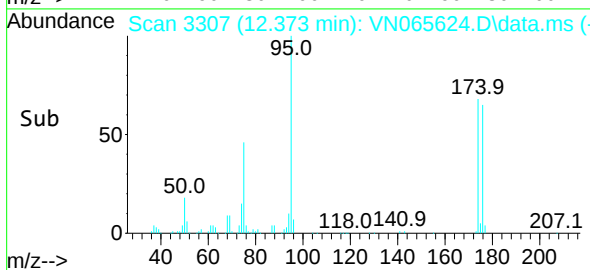

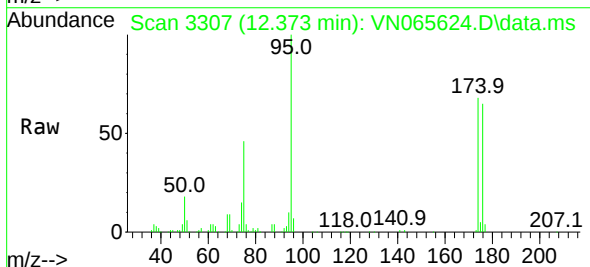


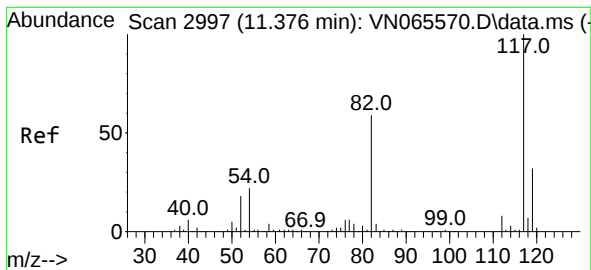

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.376 min Scan# 2997
Delta R.T. 0.000 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 304949
Ion Ratio Lower Upper
117 100
82 58.1 43.7 65.5
119 31.6 26.1 39.1

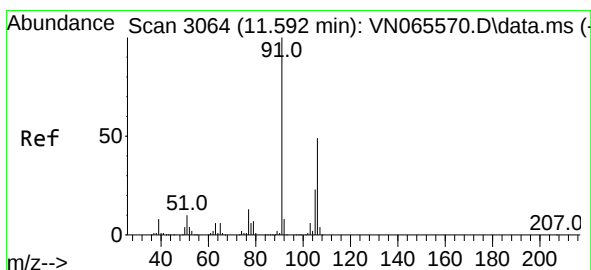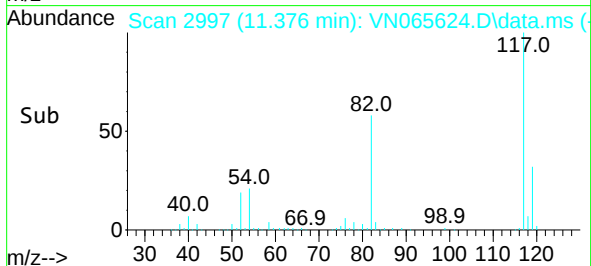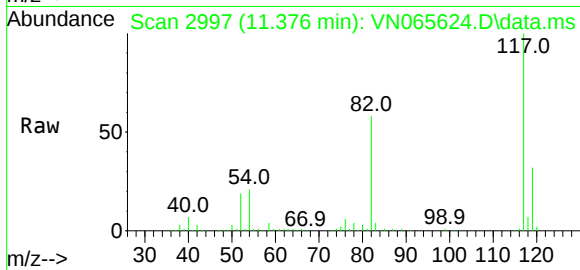

#68
m/p-Xylenes
Concen: 0.54 ug/l
RT: 11.595 min Scan# 3065
Delta R.T. 0.003 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57

Tgt Ion:106 Resp: 2330
Ion Ratio Lower Upper
106 100
91 220.7 161.4 242.0

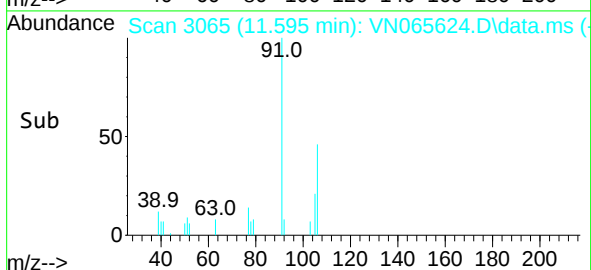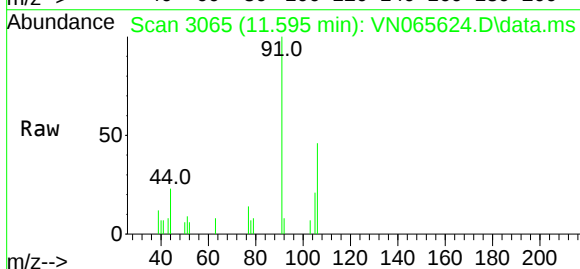

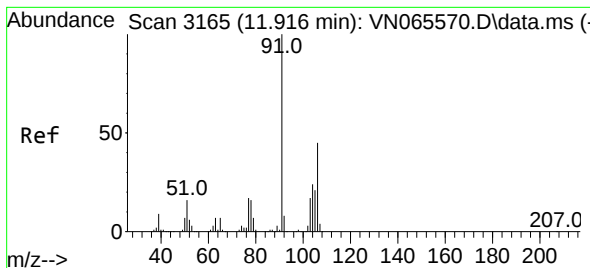

#69

o-Xylene

Concen: 8.58 ug/l

RT: 11.916 min Scan# 3165

Delta R.T. 0.000 min

Lab File: VN065624.D





Acq: 27 Jan 2021 12:57

Tgt Ion:106 Resp: 36074

Ion Ratio Lower Upper

106 100

91 219.2 106.8 320.4

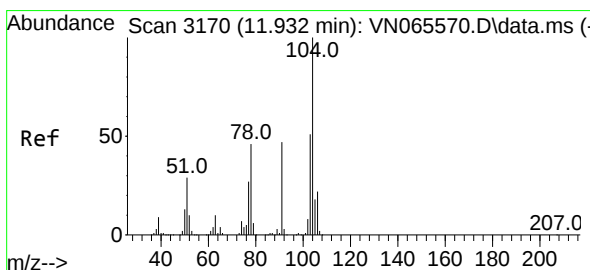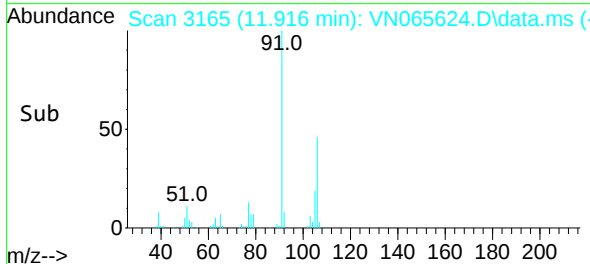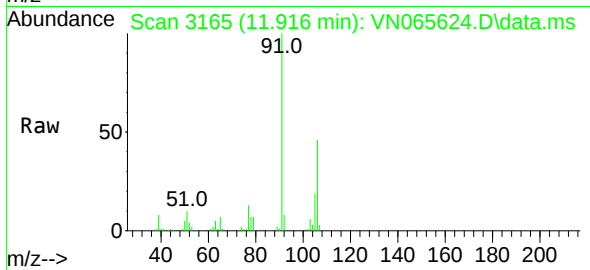

#70

Styrene

Concen: 0.48 ug/l

RT: 11.926 min Scan# 3168

Delta R.T. -0.006 min

Lab File: VN065624.D

Acq: 27 Jan 2021 12:57




Tgt Ion:104 Resp: 3297


Ion Ratio Lower Upper

104 100

78 175.1 39.0 58.4#

103 170.6 44.5 66.7#

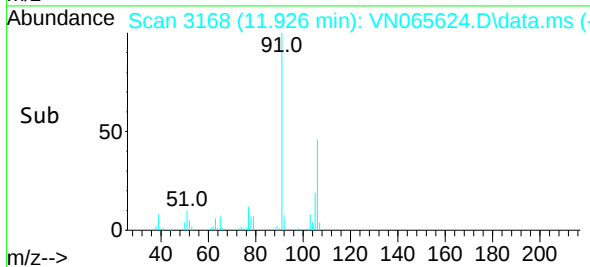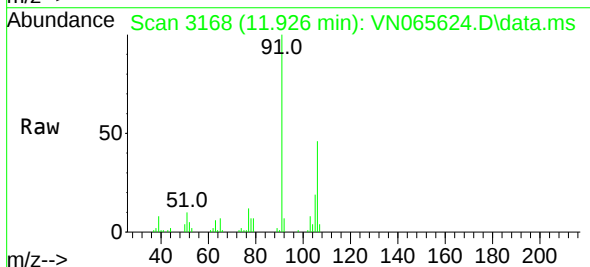

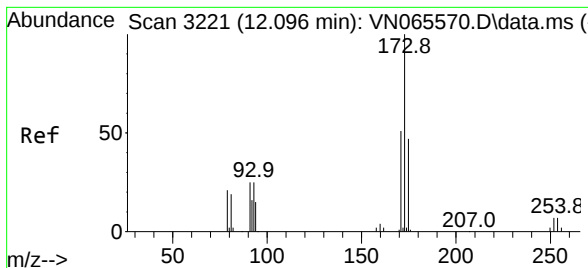

#71

Bromoform

Concen: 0.43 ug/l

RT: 12.376 min Scan# 3308

Delta R.T. 0.280 min





Lab File: VN065624.D

Acq: 27 Jan 2021 12:57

Tgt Ion:173 Resp: 670

Ion	Ratio	Lower	Upper
173	100		
175	862.1	23.8	71.2#
254	0.0	0.0	0.0

Instrument :
MSVOA_N
ClientSampleId :

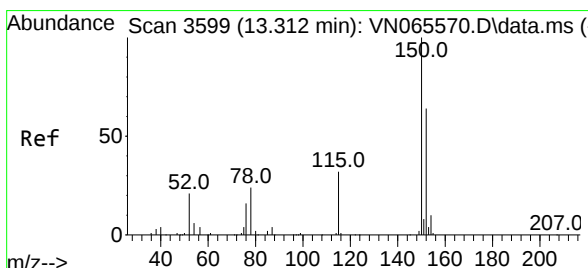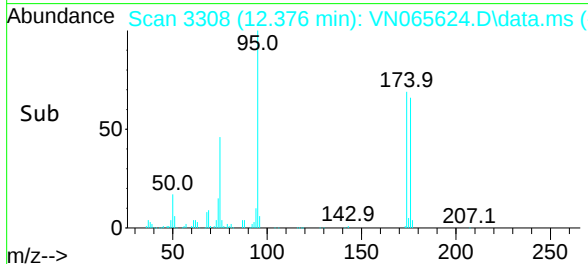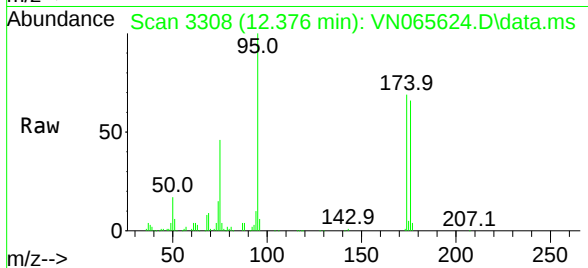

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 13.315 min Scan# 3600




Delta R.T. 0.003 min


Lab File: VN065624.D

Acq: 27 Jan 2021 12:57

Tgt Ion:152 Resp: 112864

Ion	Ratio	Lower	Upper
152	100		
115	66.4	28.5	85.6
150	159.1	0.0	347.6


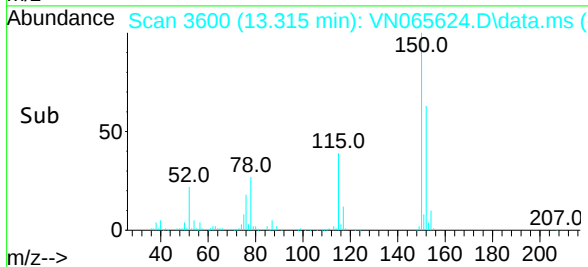

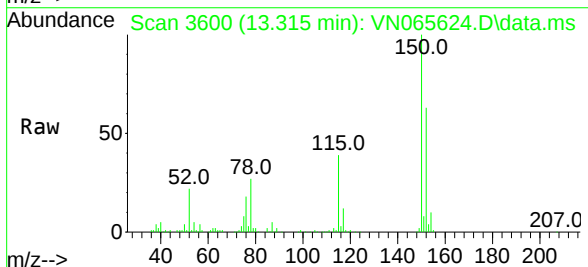


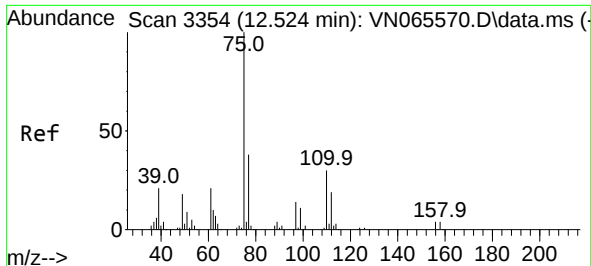

#76
1,2,3-Trichloropropane
Concen: 22.89 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. -0.151 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 67554
Ion Ratio Lower Upper
75 100
77 1.4 0.0 0.0#

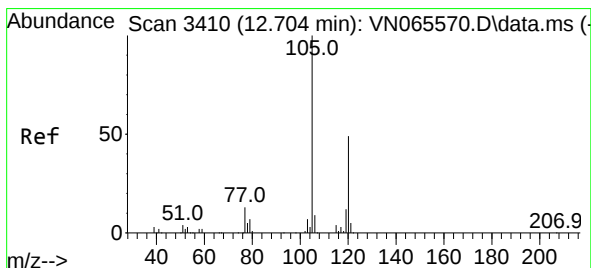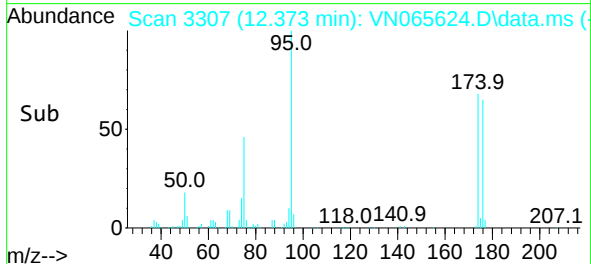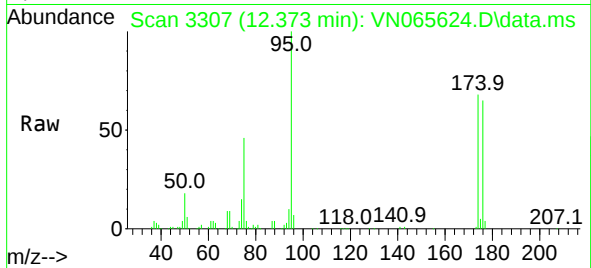

#80
1,3,5-Trimethylbenzene
Concen: 4.21 ug/l
RT: 12.704 min Scan# 3410
Delta R.T. 0.000 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57

Tgt Ion: 105 Resp: 35439
Ion Ratio Lower Upper
105 100
120 47.7 24.3 72.8


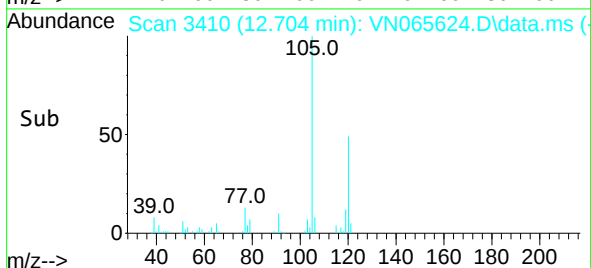

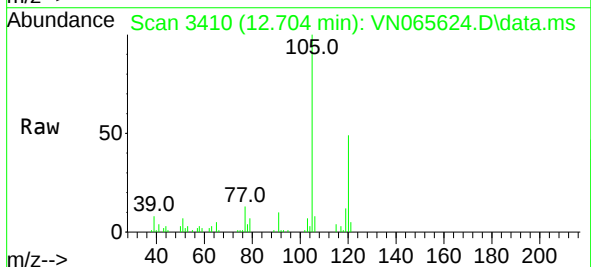


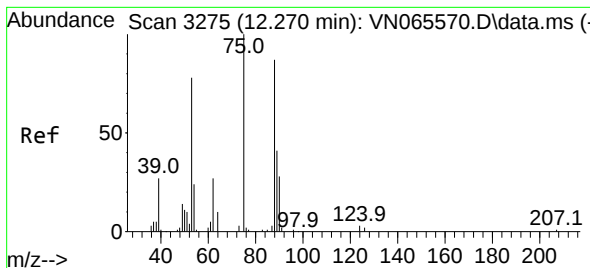

#81
trans-1,4-Dichloro-2-butene
Concen: 58.63 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. 0.103 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 67554
Ion Ratio Lower Upper
75 100
53 0.0 74.6 111.8#
89 0.0 35.8 53.8#

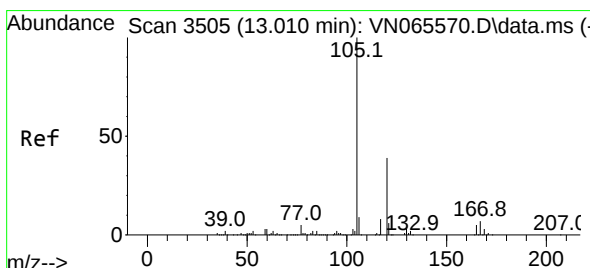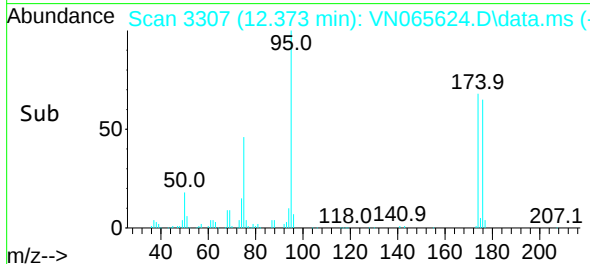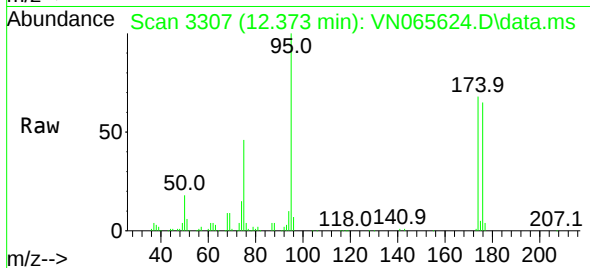

#84
1,2,4-Trimethylbenzene
Concen: 0.53 ug/l
RT: 13.010 min Scan# 3505
Delta R.T. -0.000 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57

Tgt Ion: 105 Resp: 4451
Ion Ratio Lower Upper
105 100
120 41.2 22.4 67.0


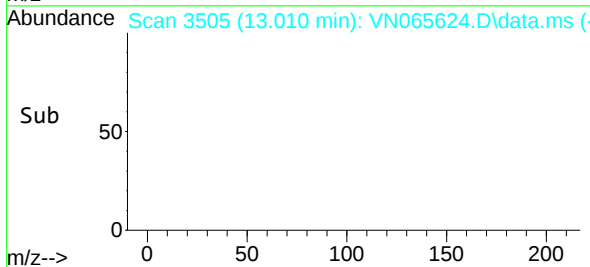

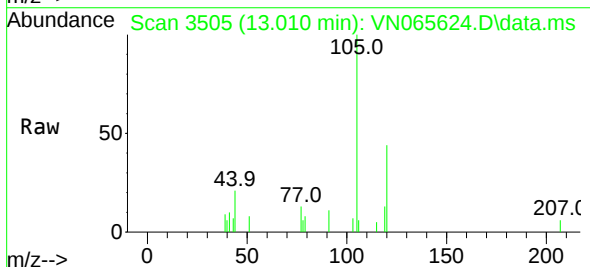


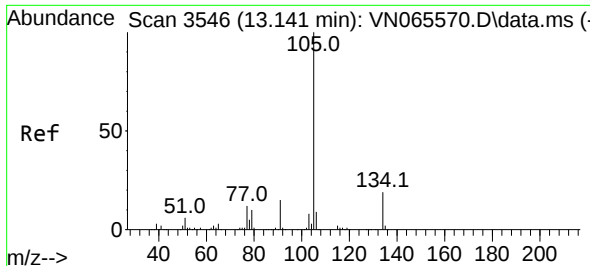

#85
 sec-Butylbenzene
 Concen: 0.37 ug/l
 RT: 13.145 min Scan# 3547
 Delta R.T. 0.004 min
 Lab File: VN065624.D
 Acq: 27 Jan 2021 12:57




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion:105 Resp: 3470
 Ion Ratio Lower Upper
 105 100
 134 18.4 10.0 30.0

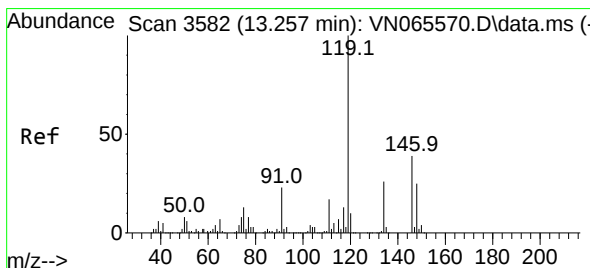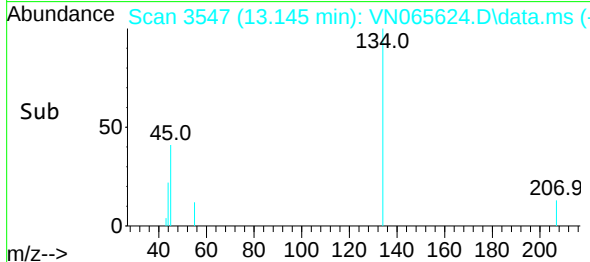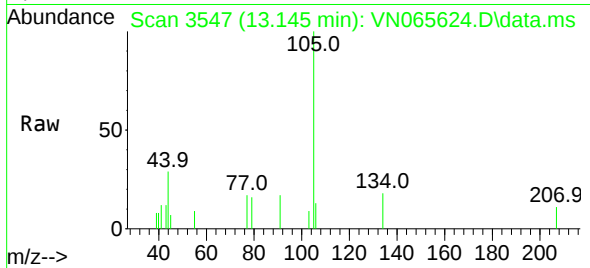

#86
 p-Isopropyltoluene
 Concen: 0.40 ug/l
 RT: 13.260 min Scan# 3583
 Delta R.T. 0.003 min
 Lab File: VN065624.D
 Acq: 27 Jan 2021 12:57

Tgt Ion:119 Resp: 3318
 Ion Ratio Lower Upper
 119 100
 134 20.9 13.3 39.8
 91 23.6 11.8 35.3


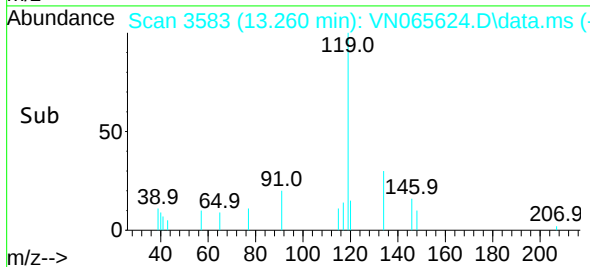

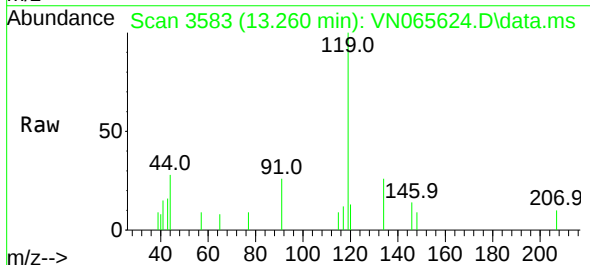


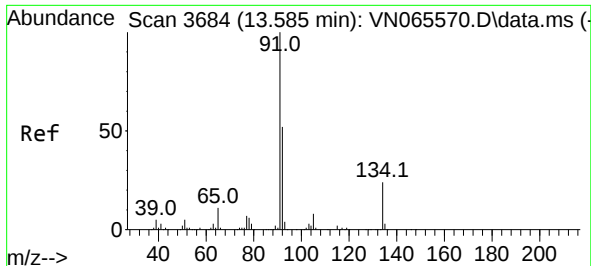

#89
n-Butylbenzene
Concen: 0.70 ug/l
RT: 13.553 min Scan# 3674
Delta R.T. -0.032 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 5231
Ion Ratio Lower Upper
91 100
92 15.6 26.1 78.3#
134 281.0 13.0 38.9#

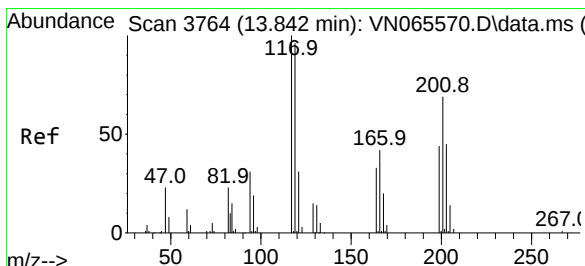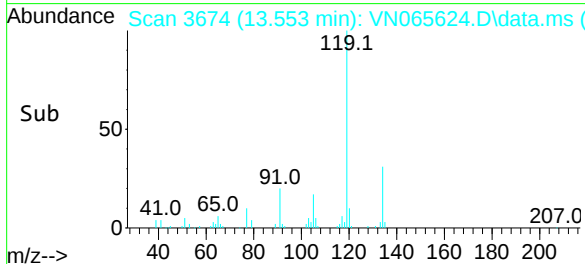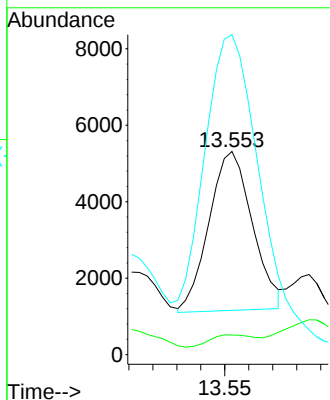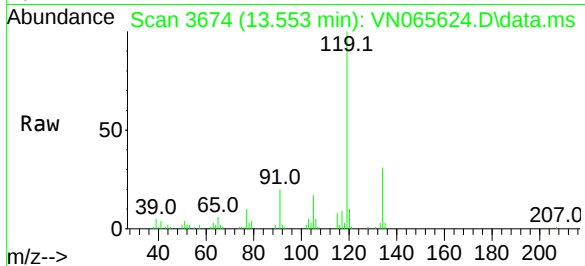

#90
Hexachloroethane
Concen: 2.58 ug/l
RT: 13.858 min Scan# 3769
Delta R.T. 0.016 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57


Tgt Ion: 117 Resp: 3770
Ion Ratio Lower Upper
117 100
201 0.0 37.8 113.3#

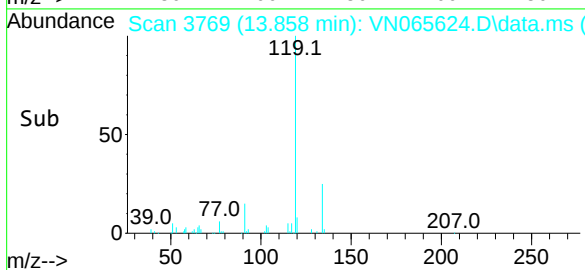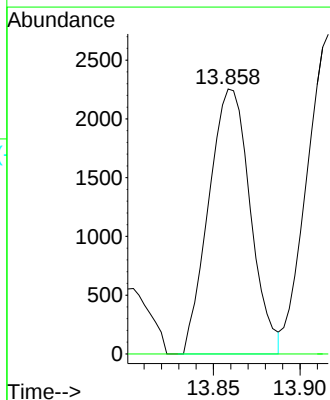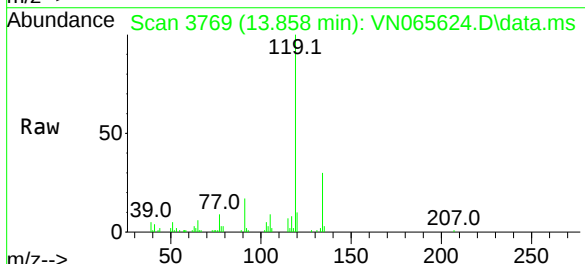



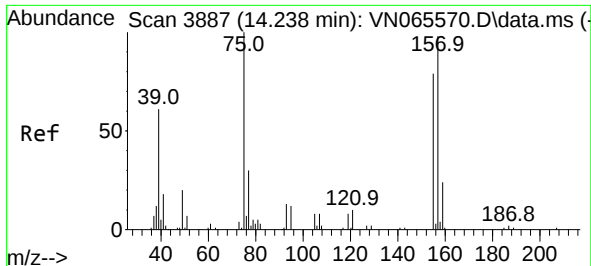


#92
1,2-Dibromo-3-Chloropropane
Concen: 0.68 ug/l
RT: 14.222 min Scan# 3882
Delta R.T. -0.016 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57

Instrument :
MSVOA_N
ClientSampleId :



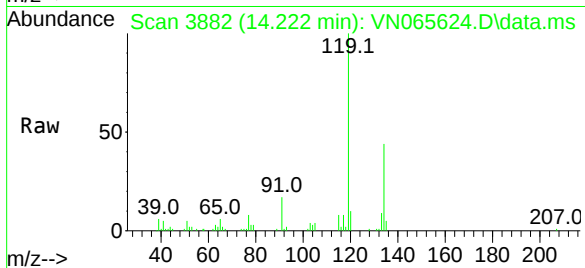



Tgt Ion: 75 Resp: 393
Ion Ratio Lower Upper
75 100
155 0.0 44.1 132.4#
157 0.0 56.0 168.2#

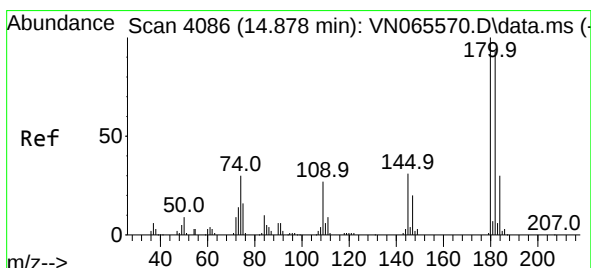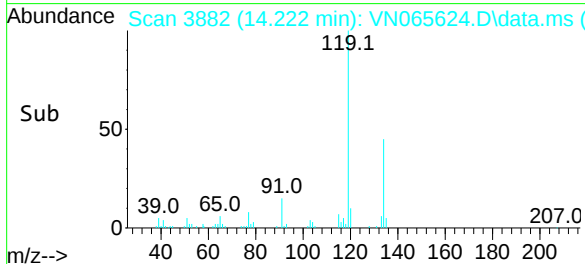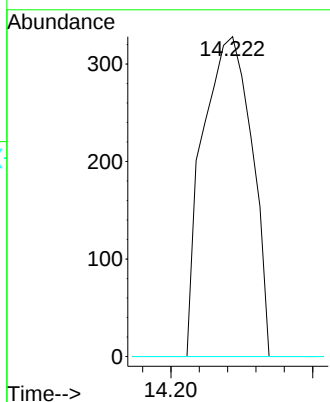

#93
1,2,4-Trichlorobenzene
Concen: 3.74 ug/l
RT: 14.878 min Scan# 4086
Delta R.T. -0.000 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57


Tgt Ion: 180 Resp: 909
Ion Ratio Lower Upper
180 100
182 83.9 47.3 142.0
145 534.8 15.6 46.8#

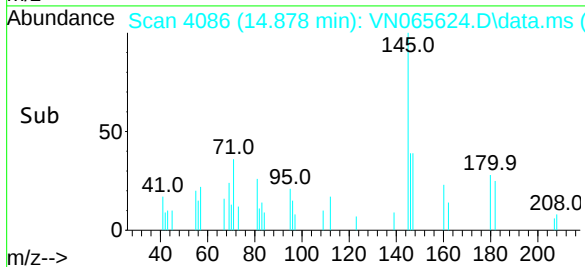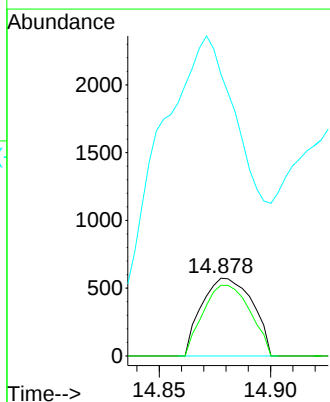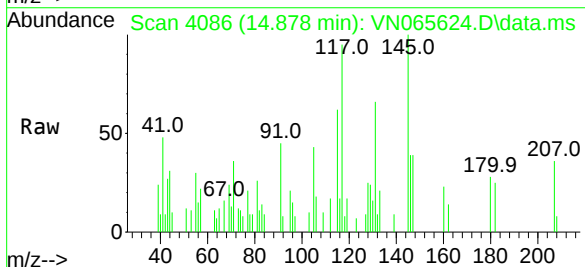



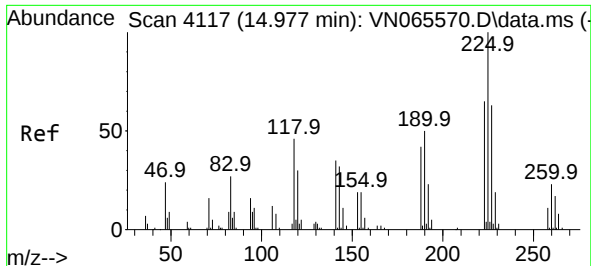


#94
Hexachlorobutadiene
Concen: 0.52 ug/l
RT: 14.974 min Scan# 4116
Delta R.T. -0.003 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57

Instrument :
MSVOA_N
ClientSampleId :



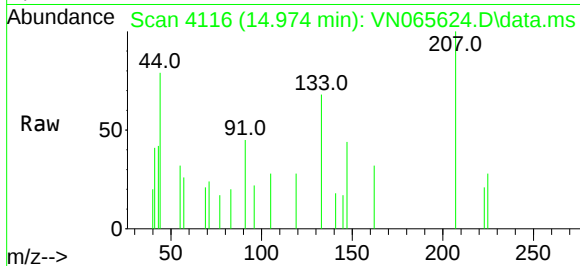



Tgt Ion:225 Resp: 288
Ion Ratio Lower Upper
225 100
223 35.4 31.9 95.9
227 33.7 31.6 95.0

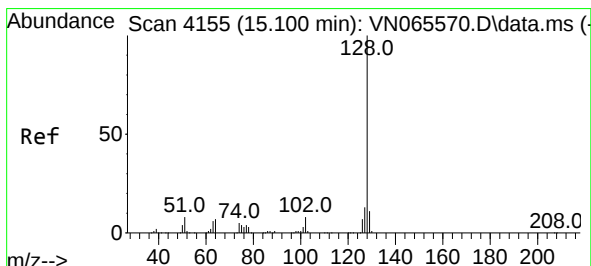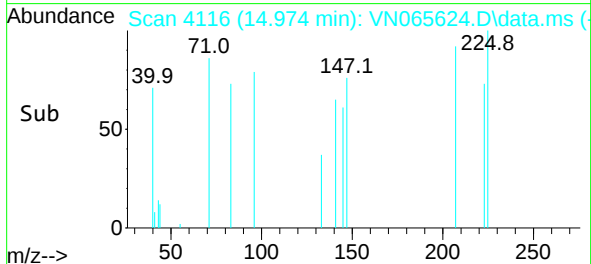

#95
Naphthalene
Concen: 4.27 ug/l
RT: 15.100 min Scan# 4155
Delta R.T. -0.000 min
Lab File: VN065624.D
Acq: 27 Jan 2021 12:57


Tgt Ion:128 Resp: 6413
Ion Ratio Lower Upper
128 100
127 12.0 10.2 15.2
129 0.0 8.6 13.0#

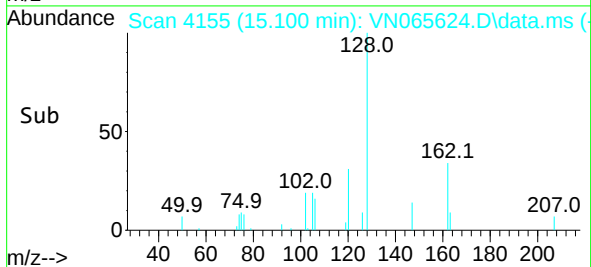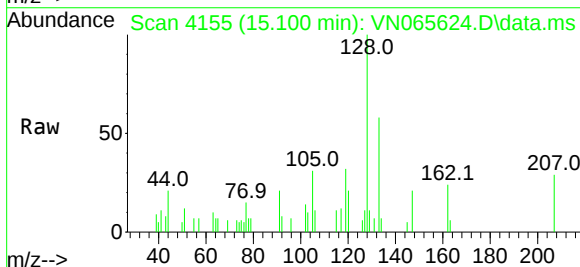

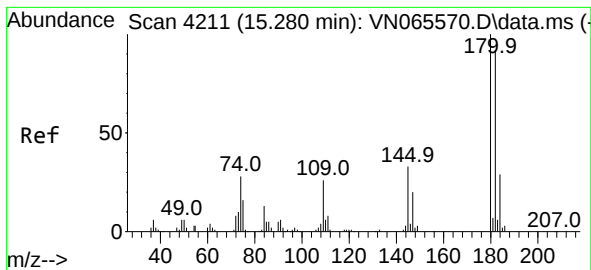

#96
 1,2,3-Trichlorobenzene
 Concen: 3.35 ug/l
 RT: 15.273 min Scan# 4209
 Delta R.T. -0.007 min
 Lab File: VN065624.D
 Acq: 27 Jan 2021 12:57

Instrument :
 MSVOA_N
 ClientSampleId :

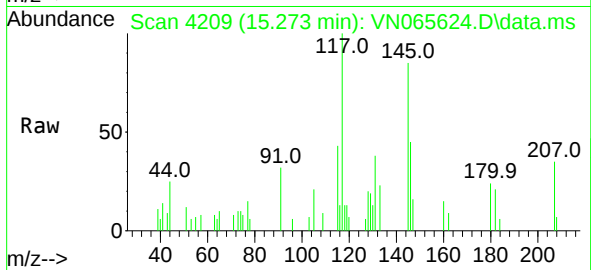

Tgt Ion:180 Resp: 1205
 Ion Ratio Lower Upper
 180 100
 182 88.2 47.4 142.3
 145 0.0 16.5 49.5#

