

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012722\
 Data File : VN070814.D
 Acq On : 27 Jan 2022 18:37
 Operator : JC/MD
 Sample : PB142314TB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB142314TB

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
 Title : SW846 8260

Signal : TIC: VN070814.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	8.021	2225	2249	2260	rBV	512761	1228604	10.54%	2.285%
2	8.086	2261	2273	2299	rVB	1055049	2404047	20.62%	4.471%
3	8.437	2382	2404	2434	rBV	622531	1475241	12.66%	2.744%
4	8.560	2436	2450	2471	rVV2	62487	138806	1.19%	0.258%
5	8.968	2582	2602	2637	rBV	1520244	3200593	27.46%	5.953%
6	9.547	2798	2818	2830	rBV3	71032	175451	1.51%	0.326%
7	9.623	2830	2846	2890	rVV	4255665	8279951	71.04%	15.399%
8	10.242	3058	3077	3100	rBV	685236	1227129	10.53%	2.282%
9	10.441	3133	3151	3182	rBV	2369920	4447255	38.15%	8.271%
10	10.615	3204	3216	3233	rVB	77052	145683	1.25%	0.271%
11	10.875	3296	3313	3329	rBV	189542	334004	2.87%	0.621%
12	10.964	3331	3346	3368	rVV	436062	790978	6.79%	1.471%
13	11.090	3370	3393	3414	rVV	6639262	11656033	100.00%	21.678%
14	11.178	3416	3426	3466	rVB	707576	1370957	11.76%	2.550%
15	11.492	3525	3543	3579	rBV	4036852	7176506	61.57%	13.347%
16	11.744	3620	3637	3670	rBV	2115052	3834959	32.90%	7.132%
17	12.197	3791	3806	3824	rBV	112326	207666	1.78%	0.386%
18	12.731	3986	4005	4032	rBV	1514625	2705945	23.21%	5.033%
19	13.675	4339	4357	4382	rBV	1680849	2968824	25.47%	5.521%


Sum of corrected areas: 53768632

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012722\
Data File : VN070814.D
Acq On : 27 Jan 2022 18:37
Operator : JC/MD
Sample : PB142314TB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB142314TB

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

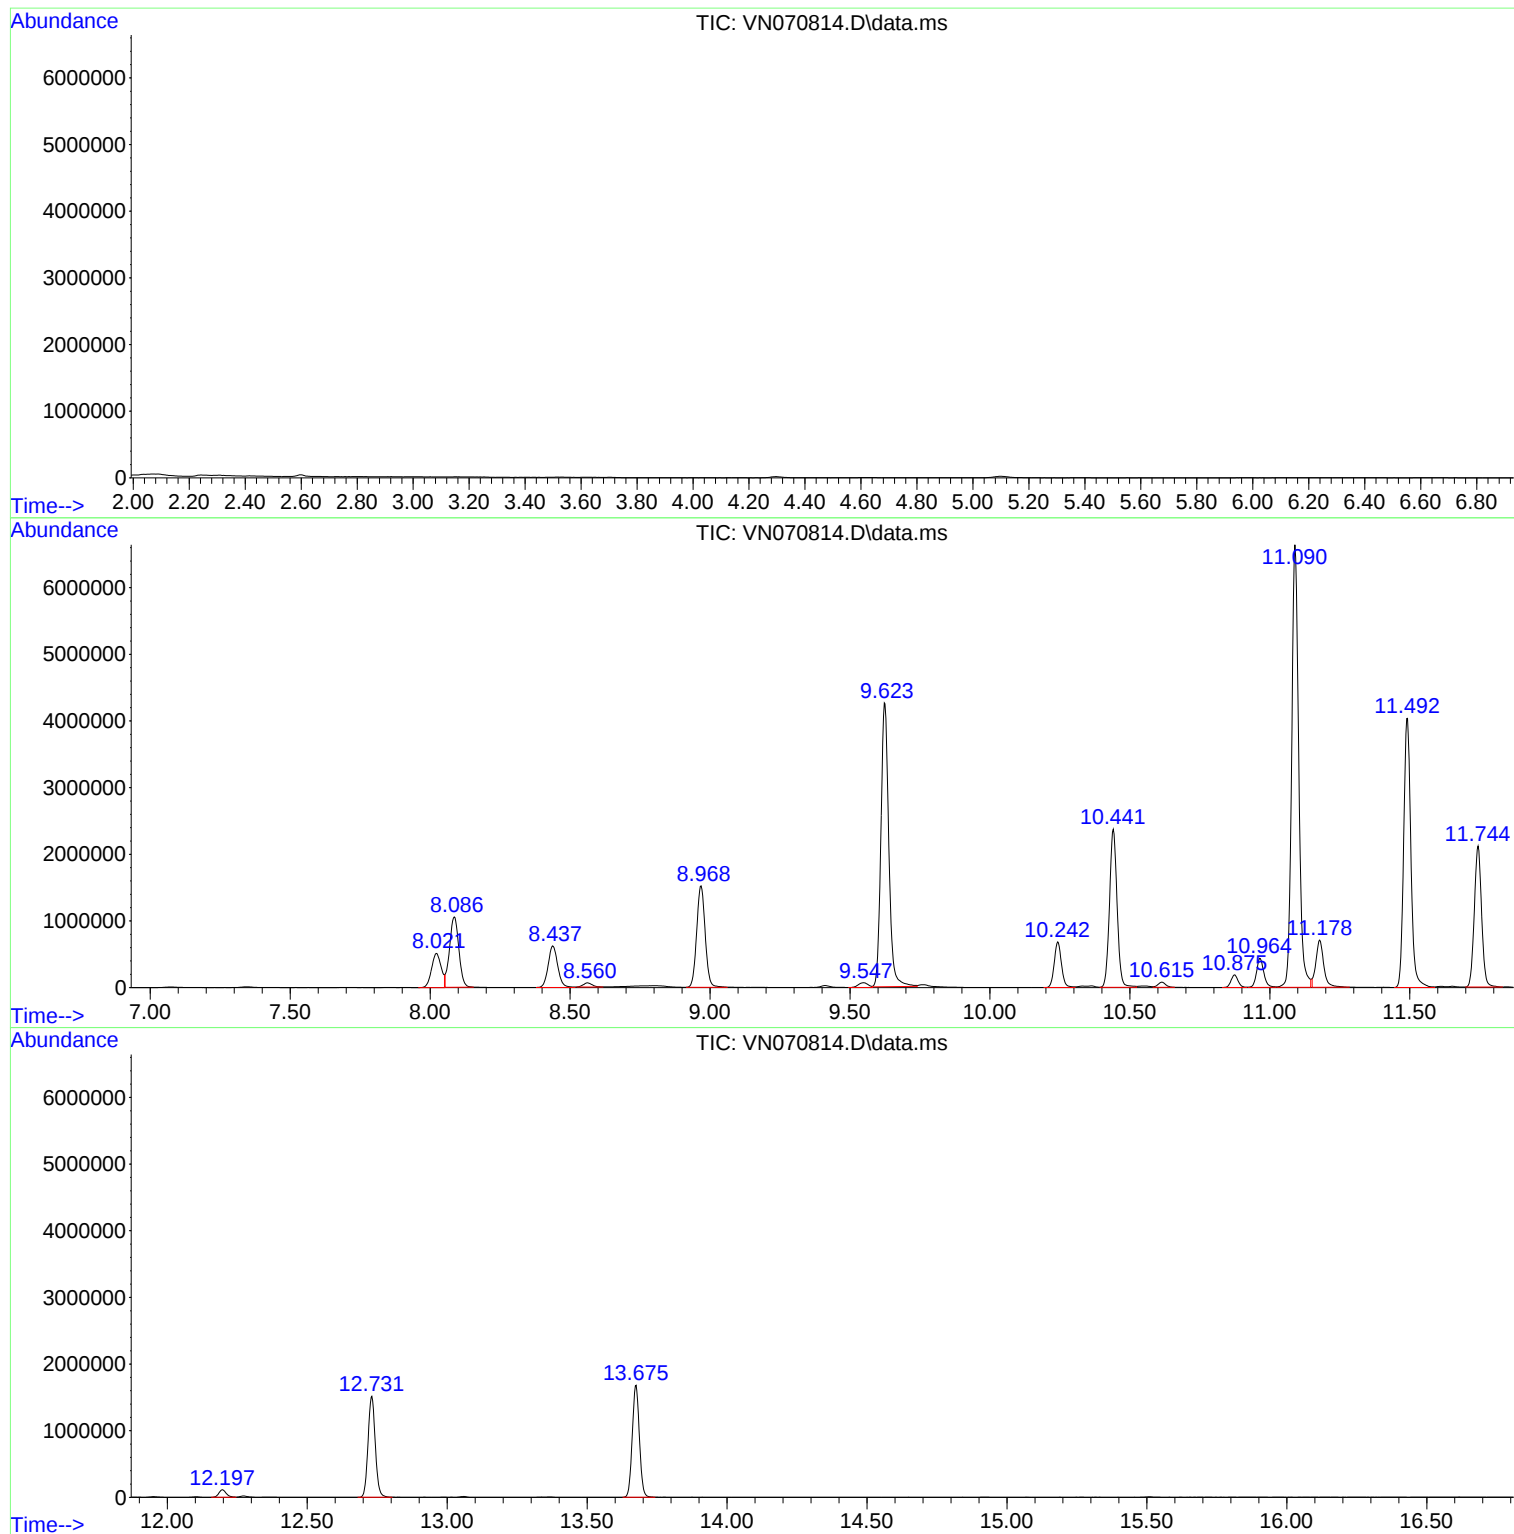

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012722\
Data File : VN070814.D
Acq On : 27 Jan 2022 18:37
Operator : JC/MD
Sample : PB142314TB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB142314TB

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012722\
Data File : VN070814.D
Acq On : 27 Jan 2022 18:37
Operator : JC/MD
Sample : PB142314TB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB142314TB

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------