
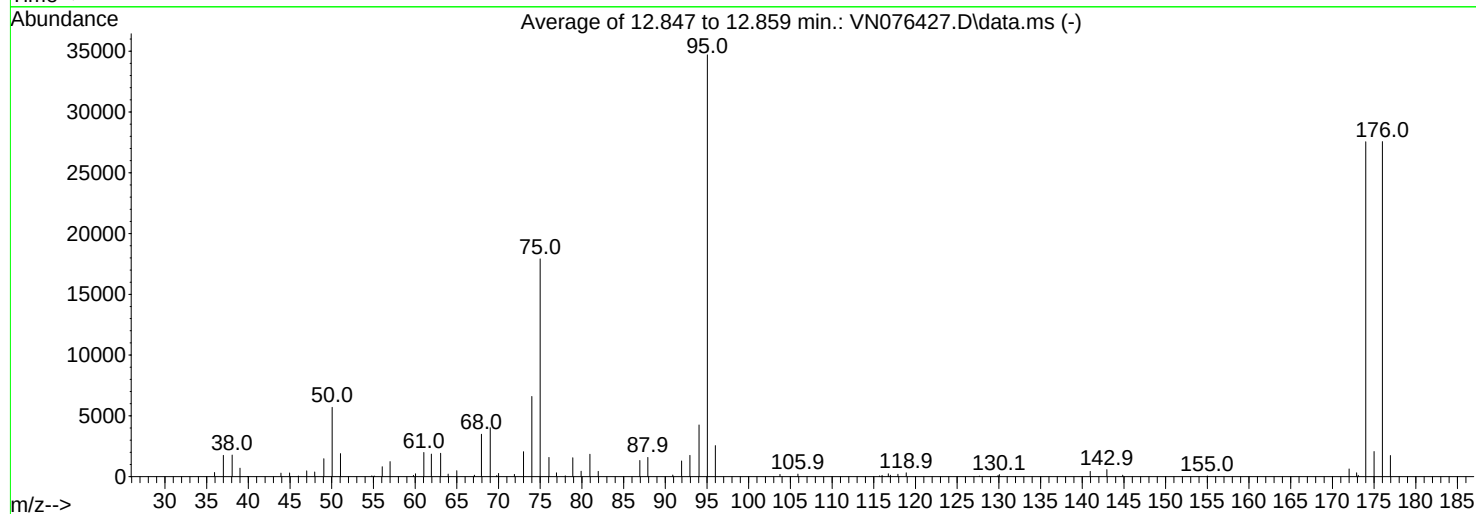


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012723\
Data File : VN076427.D
Acq On : 27 Jan 2023 09:07
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Title : SW846 8260
Last Update : Tue Jan 17 03:59:22 2023

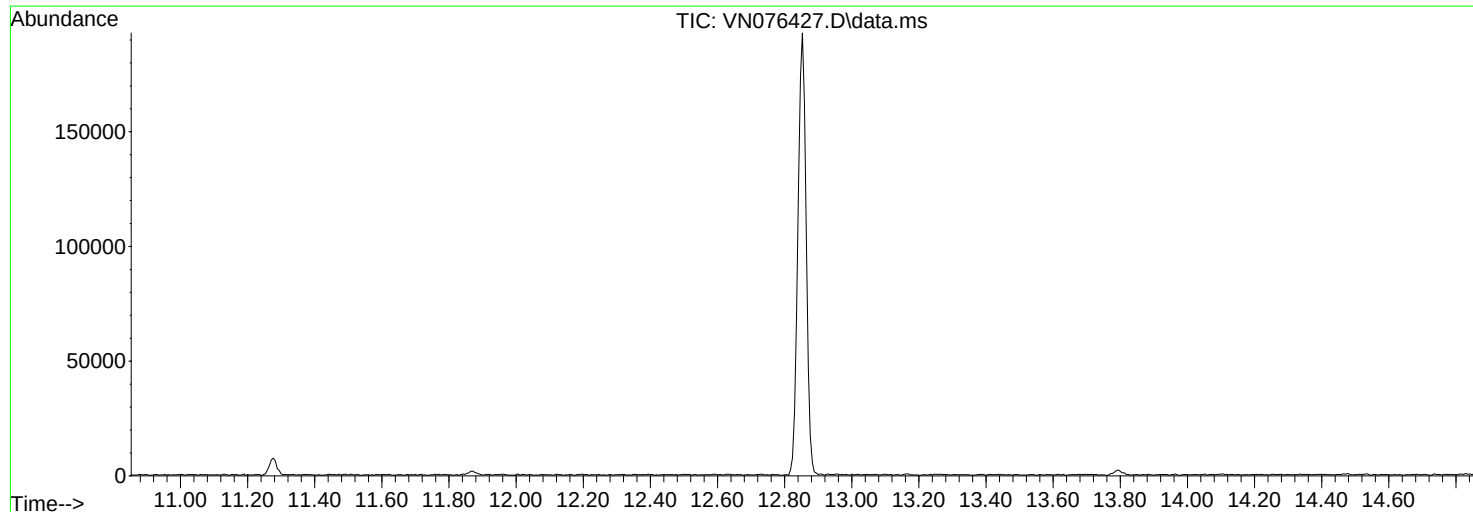

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	5704	PASS
75	95	30	60	51.6	17923	PASS
95	95	100	100	100.0	34704	PASS
96	95	5	9	7.4	2556	PASS
173	174	0.00	2	1.2	317	PASS
174	95	50	100	79.4	27557	PASS
175	174	5	9	7.5	2062	PASS
176	174	95	101	100.1	27571	PASS
177	176	5	9	6.3	1744	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	348	50.05	5704	63.95	210	76.05	1581
37.00	1749	51.05	1899	65.00	493	76.95	311
38.05	1784	54.80	67	67.10	118	78.00	6
39.00	695	55.10	52	67.95	3484	78.90	155
39.90	18	56.05	819	69.00	4033	79.90	444
43.90	284	57.00	1234	69.80	95	80.95	1840
44.95	308	59.80	111	70.00	269	81.95	435
46.00	53	60.05	234	71.90	187	86.95	1334
47.00	471	61.05	1995	73.00	2055	87.90	1584
47.95	381	61.95	1861	74.00	6594	90.90	133
49.05	1478	63.05	1925	75.00	17923	91.95	1286

Average of 12.847 to 12.859 min.: VN076427.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.95	1751	118.90	320	174.00	27557		
94.05	4255	127.70	55	175.00	2062		
95.05	34704	129.90	106	176.00	27571		
96.00	2556	130.05	177	176.95	1744		
103.75	190	140.95	436				
105.90	213	142.95	581				
115.70	62	144.85	120				
116.00	104	155.00	55				
116.75	234	172.00	638				
117.00	125	172.90	317				
117.90	203	173.10	103				

Instrument :

MSVOA_N

ClientSampleId :

BFB