
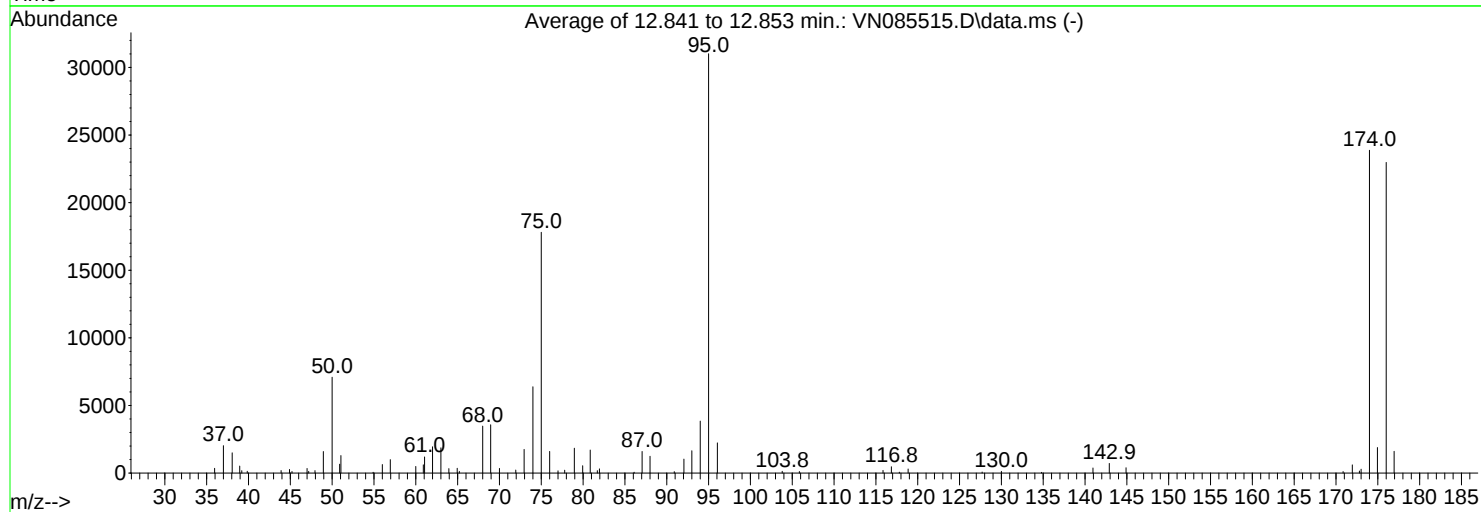


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012725\
Data File : VN085515.D
Acq On : 27 Jan 2025 13:08
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
Title : SW846 8260
Last Update : Wed Jan 15 02:16:08 2025

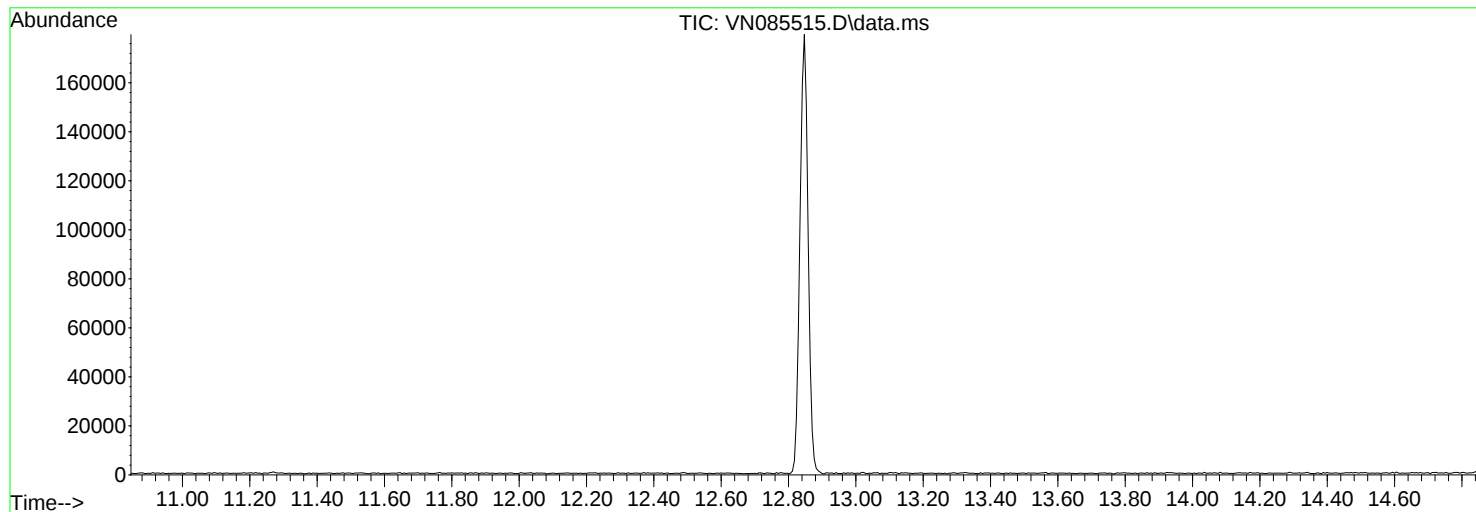

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	7090	PASS
75	95	30	60	57.4	17807	PASS
95	95	100	100	100.0	31013	PASS
96	95	5	9	7.2	2233	PASS
173	174	0.00	2	1.2	289	PASS
174	95	50	100	77.0	23872	PASS
175	174	5	9	7.9	1888	PASS
176	174	95	101	96.2	22976	PASS
177	176	5	9	7.0	1608	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	350	47.95	185	62.00	1945	75.00	17807
37.00	2027	48.95	1595	63.00	1868	76.00	1600
38.05	1498	50.00	7090	63.95	331	77.00	168
38.95	518	50.90	657	64.95	355	77.80	213
39.20	176	51.05	1297	65.20	124	78.95	1839
39.85	135	54.90	59	68.00	3473	79.95	544
43.90	187	56.00	633	68.95	3572	80.85	1705
44.90	267	56.95	993	70.00	343	81.70	181
45.20	117	60.00	491	71.95	222	81.95	312
47.00	341	60.90	609	72.95	1751	86.10	63
47.20	124	61.05	1194	74.00	6383	87.05	1596

Average of 12.841 to 12.853 min.: VN085515.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
88.00	1243	117.80	67	173.00	289		
90.90	106	118.85	301	174.00	23872		
92.05	1033	127.70	79	174.95	1888		
93.00	1652	130.00	127	176.00	22976		
94.00	3846	134.80	54	176.95	1608		
95.00	31013	140.95	377				
96.05	2233	142.90	713				
103.80	130	144.90	394				
105.85	116	170.85	113				
115.85	198	171.95	608				
116.85	468	172.80	153				

Instrument :

MSVOA_N

ClientSampleId :

BFB