


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012821\
Data File : VN065638.D
Acq On : 28 Jan 2021 9:56
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012521W.M
Title : SW846 8260
Last Update : Mon Jan 25 13:47:28 2021

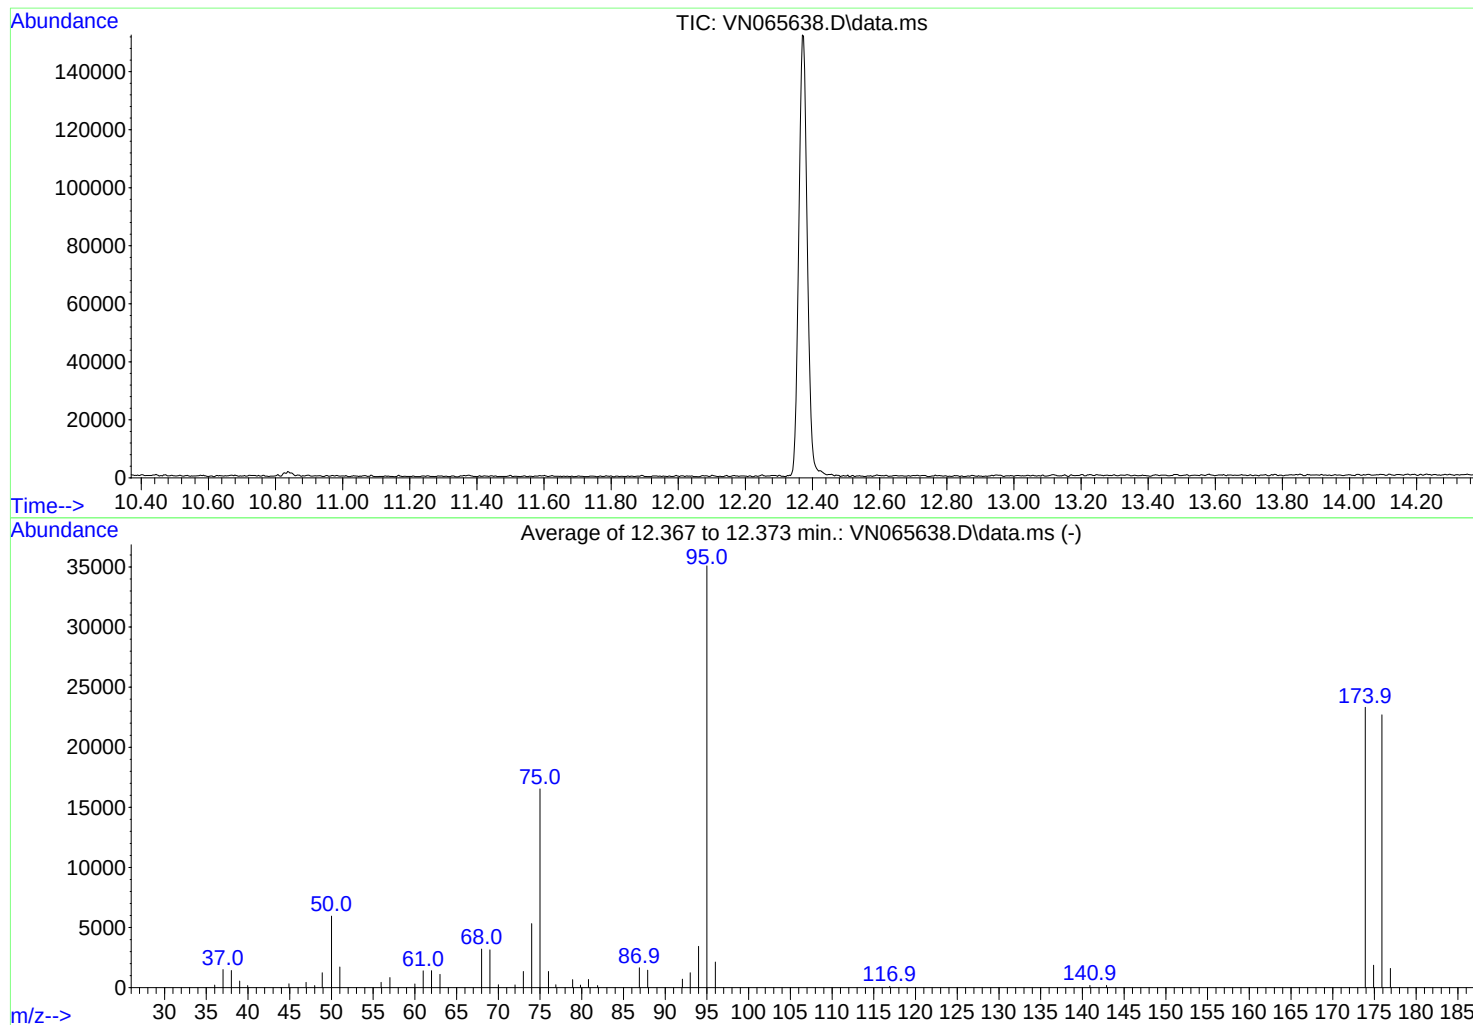

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3293

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.9	5948	PASS
75	95	30	60	47.1	16534	PASS
95	95	100	100	100.0	35093	PASS
96	95	5	9	6.1	2132	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	66.5	23320	PASS
175	174	5	9	8.0	1858	PASS
176	174	95	101	97.3	22693	PASS
177	176	5	9	7.0	1593	PASS