

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012822\
 Data File : VN070826.D
 Acq On : 28 Jan 2022 14:03
 Operator : JC/MD
 Sample : N1224-10
 Misc : 6.67g/5mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 AREA-1-B-2@4-B6S

Quant Time: Jan 28 23:16:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 18 13:32:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.080	168	728364	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1191092	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	1161021	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	564312	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.432	65	525865	50.377	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 100.760%			
35) Dibromofluoromethane	8.018	113	338892	45.868	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 91.740%			
50) Toluene-d8	10.440	98	1579553	50.748	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 101.500%			
62) 4-Bromofluorobenzene	12.731	95	602975	54.365	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 108.720%			
Target Compounds						
					Qvalue	
5) Bromomethane	2.815	94	2392	0.392	ug/l #	75
10) Methyl Iodide	4.390	142	2096	0.201	ug/l #	59
13) Acrolein	4.028	56	623	0.231	ug/l #	64
16) Acetone	4.304	43	12874	1.777	ug/l	100
18) Methyl Acetate	4.859	43	36447	2.558	ug/l #	71
20) Methylene Chloride	5.066	84	5336	0.559	ug/l #	91
30) Chloroform	7.809	83	1038	Below Cal	#	79
31) Cyclohexane	8.080	56	17584	0.957	ug/l #	10
36) 1,1-Dichloropropene	8.078	75	61747	4.964	ug/l #	49
38) Carbon Tetrachloride	8.080	117	74326	6.717	ug/l #	16
39) Methylcyclohexane	9.453	83	11555	0.753	ug/l #	63
43) Isopropyl Acetate	8.563	43	64065	2.540	ug/l #	57
47) Bromodichloromethane	9.740	83	7782	0.624	ug/l #	25
49) 1,4-Dioxane	9.587	88	59	0.327	ug/l #	1
53) t-1,3-Dichloropropene	10.714	75	513	2.436	ug/l	91
55) 1,1,2-Trichloroethane	10.872	97	84217	9.299	ug/l #	22
56) Ethyl methacrylate	10.778	69	32393	4.096	ug/l #	1
58) 2-Chloroethyl Vinyl ether	10.049	63	155	21.269	ug/l #	45
59) 2-Hexanone	11.049	43	186931	15.988	ug/l #	29
68) m/p-Xylenes	11.953	106	4577	0.270	ug/l #	58
73) Isopropylbenzene	12.578	105	36081	0.676	ug/l	93
74) N-amyl acetate	12.366	43	410209	18.793	ug/l #	68
75) 1,1,2,2-Tetrachloroethane	12.809	83	42724	2.370	ug/l #	1
76) 1,2,3-Trichloropropane	12.731	75	320654	21.424	ug/l #	1
78) n-propylbenzene	12.916	91	27060	0.453	ug/l	93
81) trans-1,4-Dichloro-2-b...	12.731	75	320654	63.826	ug/l #	5
85) sec-Butylbenzene	13.500	105	22827	0.447	ug/l #	67
89) n-Butylbenzene	13.943	91	31202	0.942	ug/l #	78
90) Hexachloroethane	14.214	117	20689	2.949	ug/l #	6
92) 1,2-Dibromo-3-Chloropr...	14.611	75	1286	0.420	ug/l #	1
93) 1,2,4-Trichlorobenzene	15.260	180	4625	3.838	ug/l #	1
95) Naphthalene	15.504	128	12354	5.329	ug/l #	76
96) 1,2,3-Trichlorobenzene	15.646	180	961	3.306	ug/l #	12

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

MSVOA_N


ClientSampleId :


AREA-1-B-2@4-B6S

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012822\
Data File : VN070826.D
Acq On : 28 Jan 2022 14:03
Operator : JC/MD
Sample : N1224-10
Misc : 6.67g/5mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-B6S

Quant Time: Jan 28 23:16:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 18 13:32:07 2022
Response via : Initial Calibration




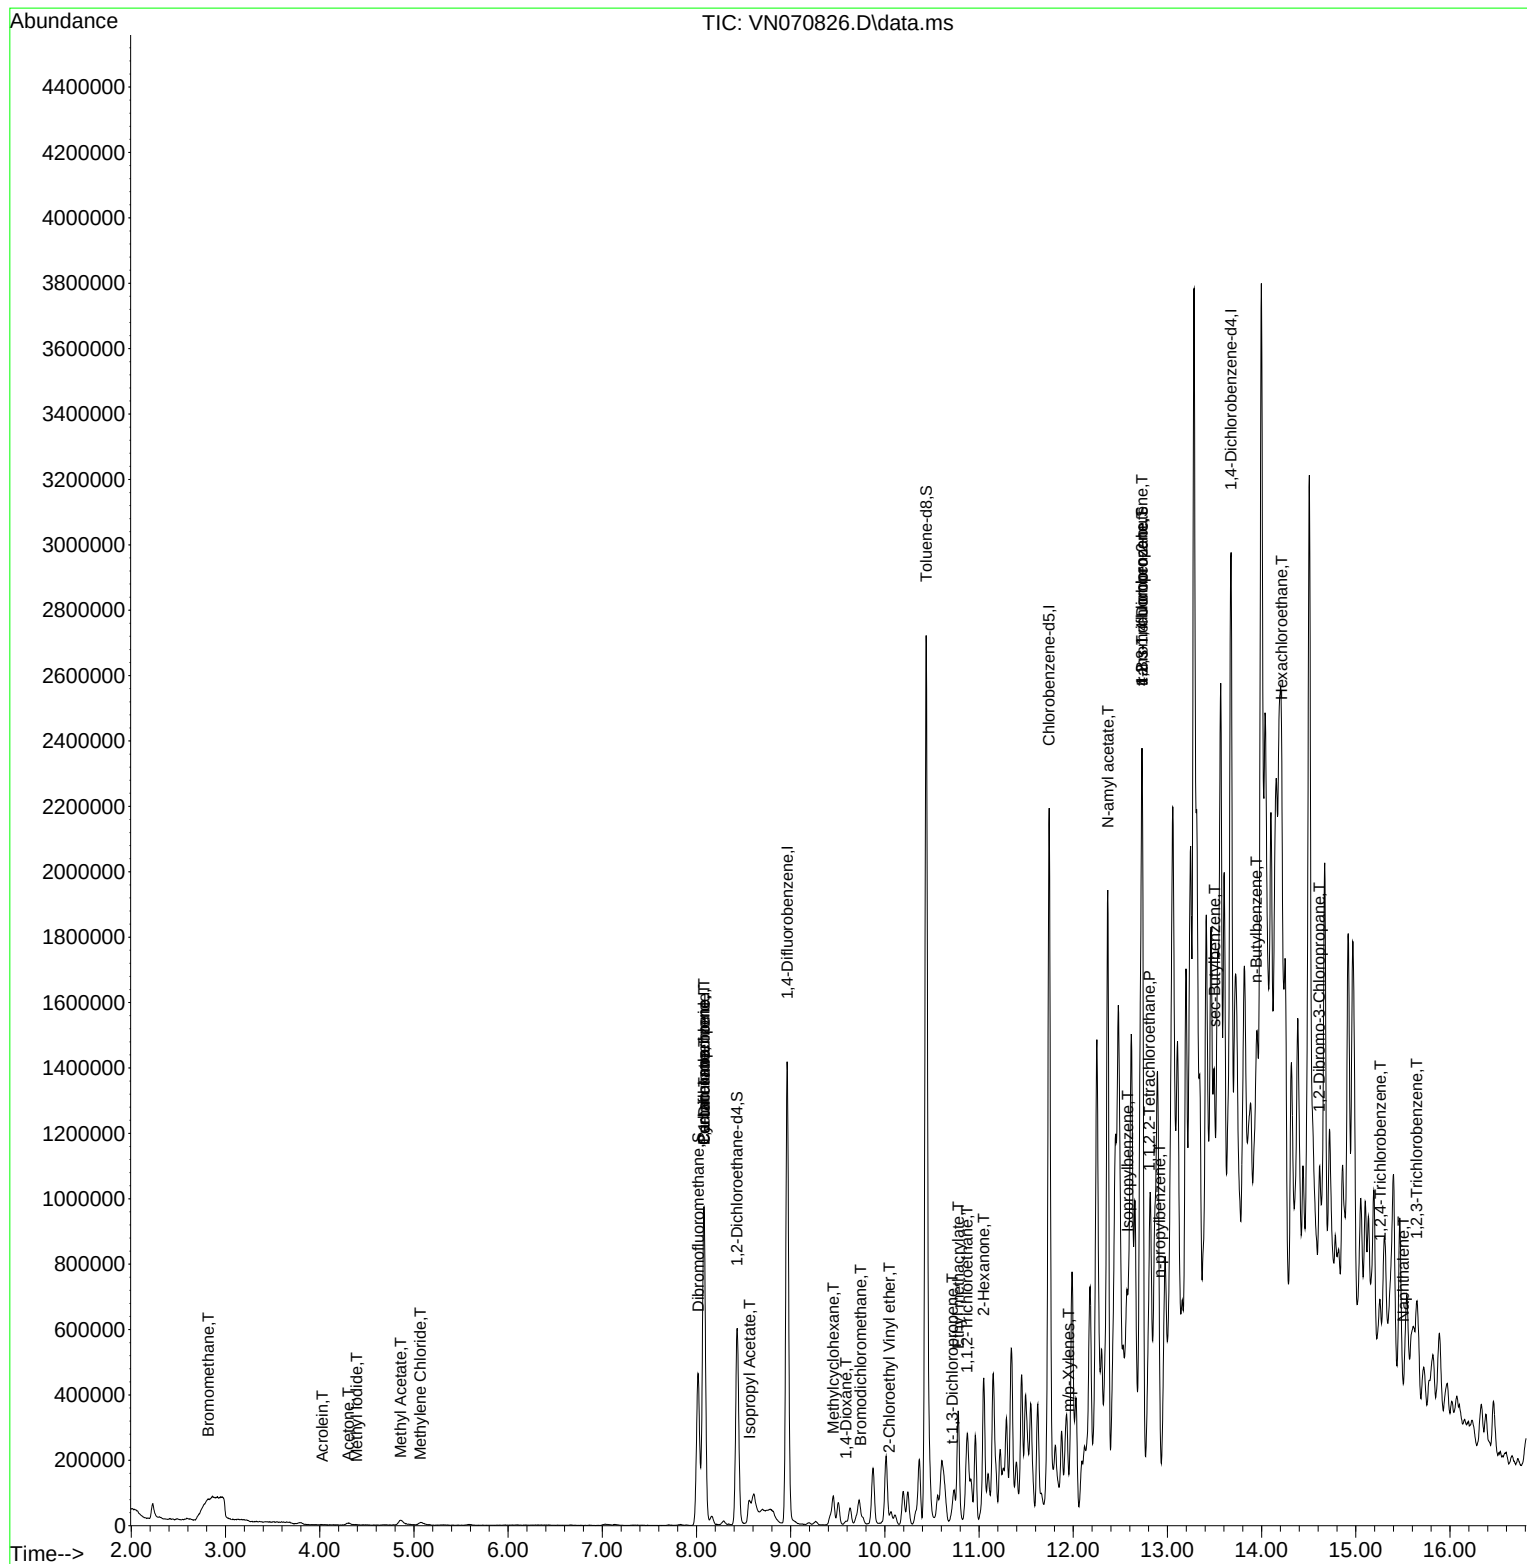




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.080 min Scan# 21
Delta R.T. -0.003 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-B6S


Tgt Ion:168 Resp: 728364
Ion Ratio Lower Upper
168 100
99 61.9 41.3 61.9

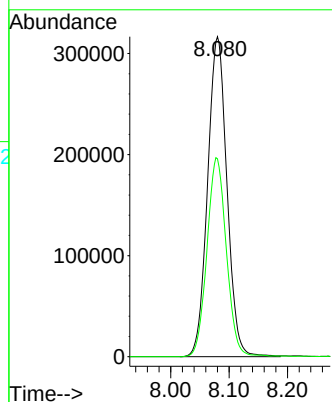

#5
Bromomethane
Concen: 0.392 ug/l
RT: 2.815 min Scan# 308
Delta R.T. -0.033 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03

Tgt Ion: 94 Resp: 2392
Ion Ratio Lower Upper
94 100
96 68.6 73.8 110.8#


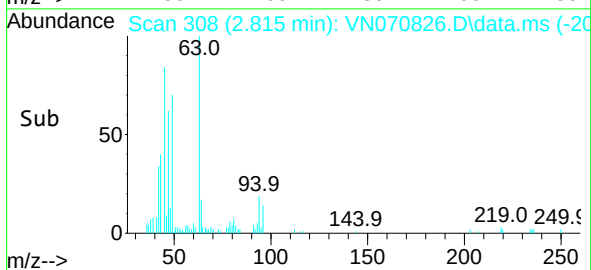
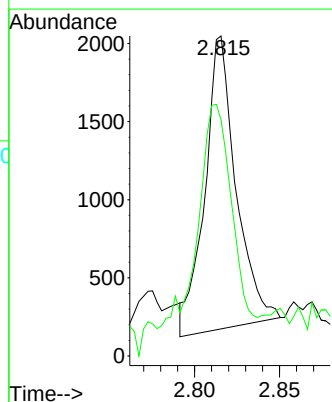





#10
Methyl Iodide
Concen: 0.201 ug/l
RT: 4.390 min Scan# 895
Delta R.T. -0.029 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-B6S


Tgt Ion:142 Resp: 2096
Ion Ratio Lower Upper
142 100
127 14.8 35.4 53.0#
141 2.8 11.6 17.4#

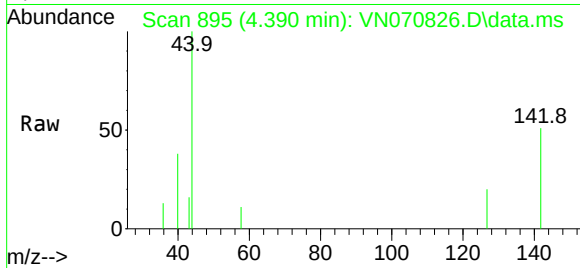

#13
Acrolein
Concen: 0.231 ug/l
RT: 4.028 min Scan# 760
Delta R.T. -0.011 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03

Tgt Ion: 56 Resp: 623
Ion Ratio Lower Upper
56 100
55 100.6 56.6 85.0#


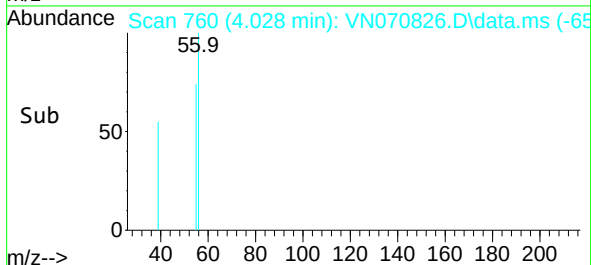
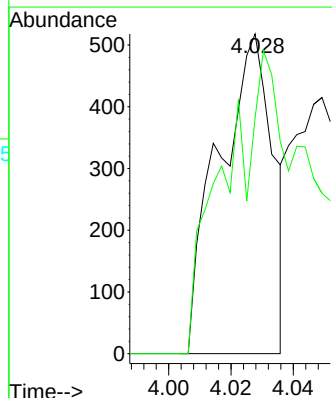
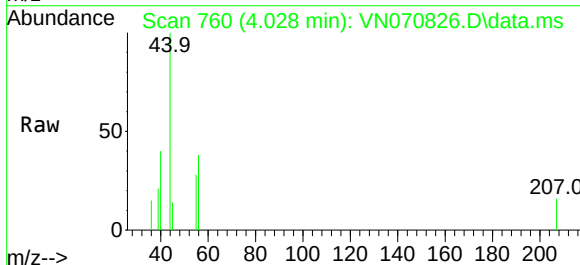




#16
Acetone
Concen: 1.777 ug/l
RT: 4.304 min Scan# 80
Delta R.T. 0.019 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-B6S


Tgt Ion: 43 Resp: 12874
Ion Ratio Lower Upper
43 100
58 28.7 23.1 34.7

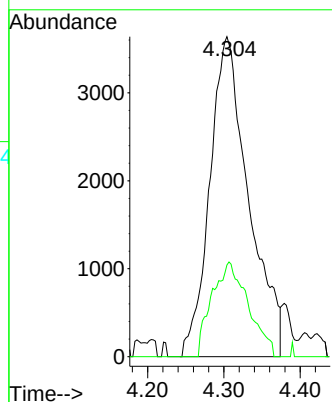

#18
Methyl Acetate
Concen: 2.558 ug/l
RT: 4.859 min Scan# 1070
Delta R.T. 0.005 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03


Tgt Ion: 43 Resp: 36447
Ion Ratio Lower Upper
43 100
74 9.9 19.4 29.2#

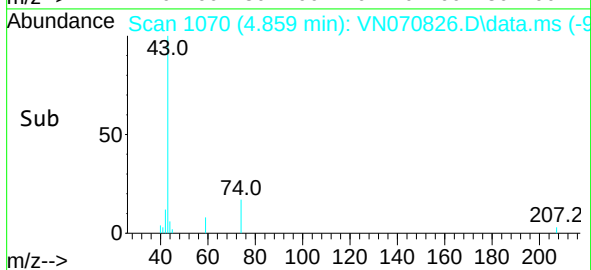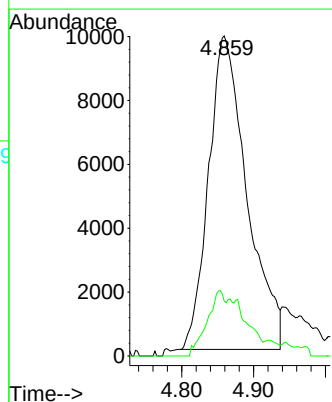



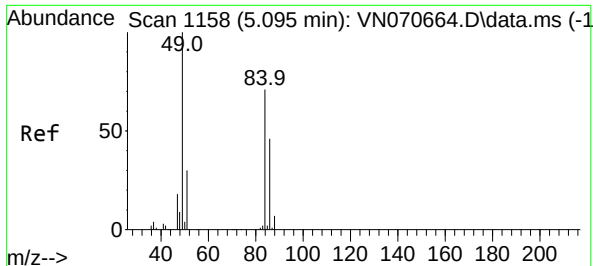


#20
Methylene Chloride
Concen: 0.559 ug/l
RT: 5.066 min Scan# 1158
Delta R.T. -0.029 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03

Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-B6S



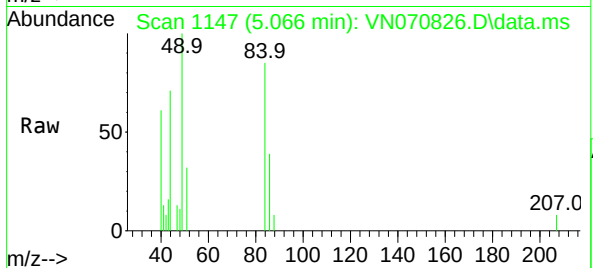



Tgt Ion:	84	Resp:	5336
Ion	Ratio	Lower	Upper
84	100		
49	118.0	93.5	140.3
51	38.1	29.4	44.2
86	45.8	53.0	79.4

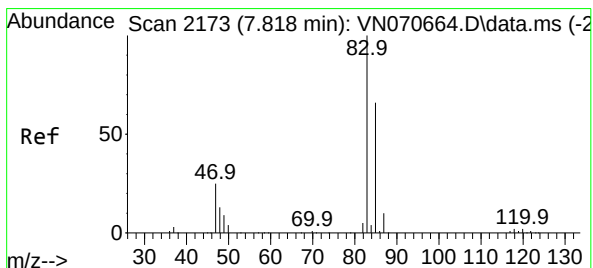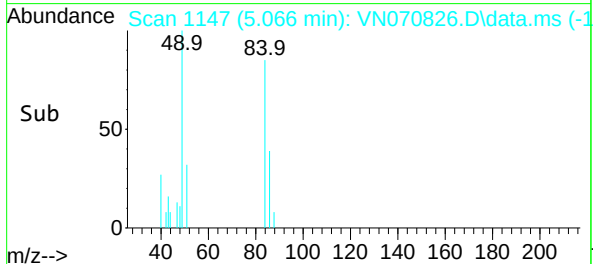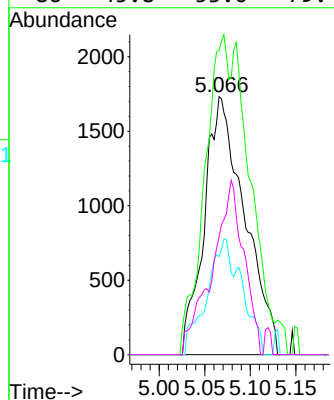

#30
Chloroform
Concen: Below Cal
RT: 7.809 min Scan# 2170
Delta R.T. -0.009 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03

Tgt Ion:	83	Resp:	1038
Ion	Ratio	Lower	Upper
83	100		
85	81.8	51.9	77.9

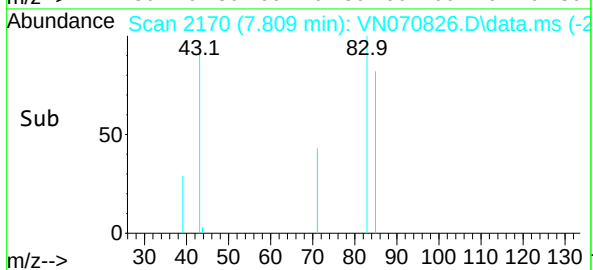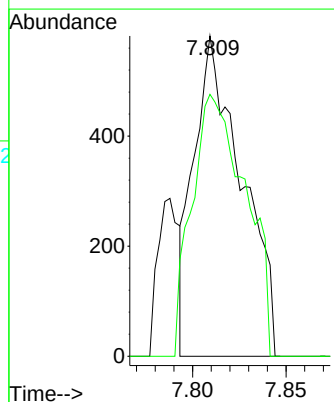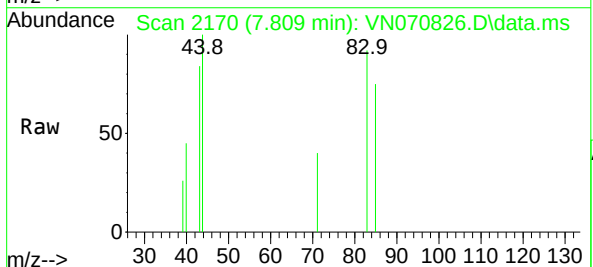



#31

Cyclohexane

Concen: 0.957 ug/l

RT: 8.080 min Scan# 21

Delta R.T. -0.014 min

Lab File: VN070826.D

Acq: 28 Jan 2022 14:03

Instrument :

MSVOA_N

ClientSampleId :

AREA-1-B-2@4-B6S





Tgt Ion: 56 Resp: 17584

Ion Ratio Lower Upper

56 100

69 169.4 27.1 40.7#

84 125.5 73.4 110.0#

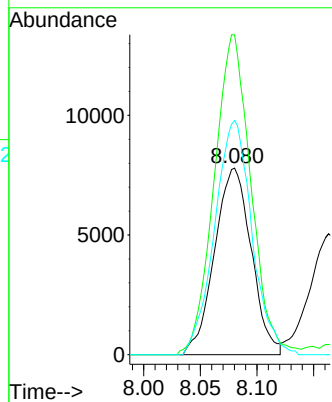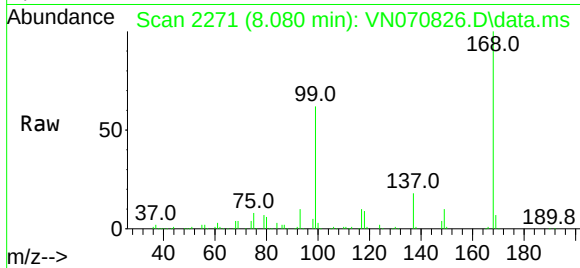

#33

1,2-Dichloroethane-d4

Concen: 50.377 ug/l

RT: 8.432 min Scan# 2402

Delta R.T. -0.002 min

Lab File: VN070826.D




Acq: 28 Jan 2022 14:03


Tgt Ion: 65 Resp: 525865

Ion Ratio Lower Upper

65 100

67 51.4 0.0 103.0


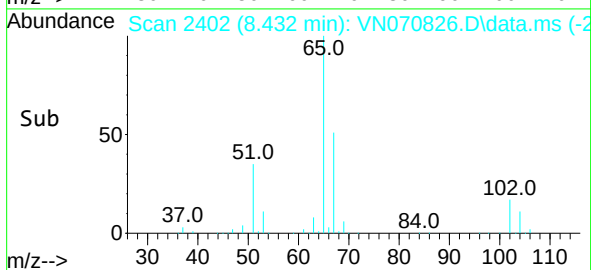

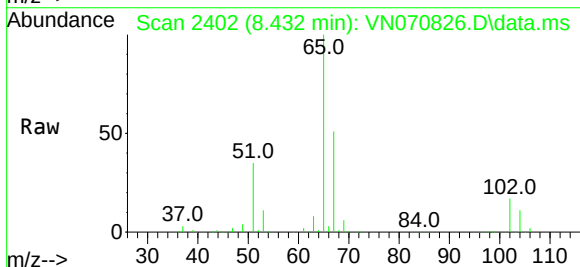




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.963 min Scan# 2600
Delta R.T. -0.002 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-B6S


Tgt Ion:114 Resp: 1191092
Ion Ratio Lower Upper
114 100
63 23.9 0.0 37.8
88 17.0 0.0 27.4

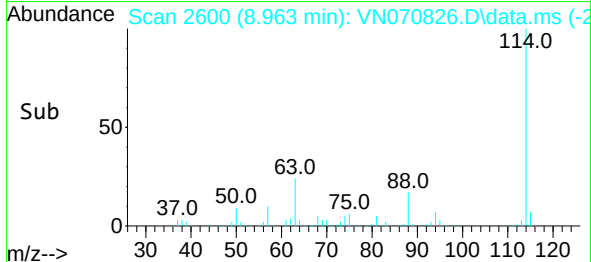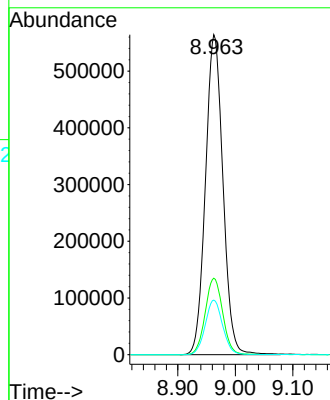

#35
Dibromofluoromethane
Concen: 45.868 ug/l
RT: 8.018 min Scan# 2248
Delta R.T. -0.001 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03

Tgt Ion:113 Resp: 338892
Ion Ratio Lower Upper
113 100
111 102.8 82.2 123.2
192 19.7 16.9 25.3



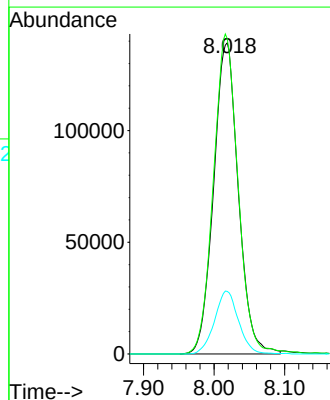
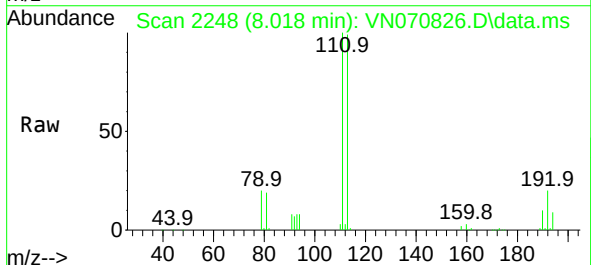




#36
1,1-Dichloropropene
Concen: 4.964 ug/l
RT: 8.078 min Scan# 21
Delta R.T. -0.143 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-B6S


Tgt Ion: 75 Resp: 61747
Ion Ratio Lower Upper
75 100
110 8.7 18.4 55.2#
77 0.0 24.4 36.6#

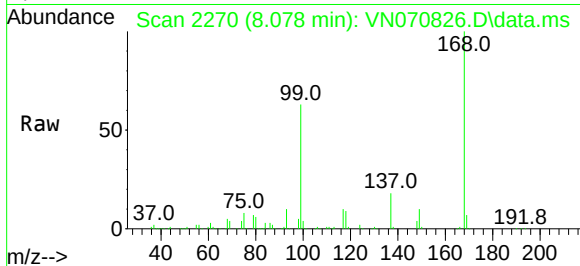

#38
Carbon Tetrachloride
Concen: 6.717 ug/l
RT: 8.080 min Scan# 2271
Delta R.T. -0.126 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03

Tgt Ion: 117 Resp: 74326
Ion Ratio Lower Upper
117 100
119 4.9 76.1 114.1#
121 0.0 24.2 36.2#




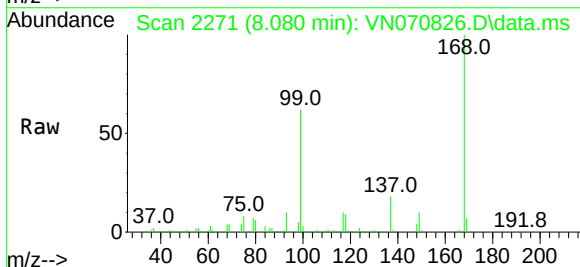




#39
Methylcyclohexane
Concen: 0.753 ug/l
RT: 9.453 min Scan# 21
Delta R.T. -0.006 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-B6S


Tgt Ion: 83 Resp: 11555
Ion Ratio Lower Upper
83 100
55 121.0 58.1 87.1#
98 43.6 38.4 57.6



#43
Isopropyl Acetate
Concen: 2.540 ug/l
RT: 8.563 min Scan# 2451
Delta R.T. 0.003 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03

Tgt Ion: 43 Resp: 64065
Ion Ratio Lower Upper
43 100
61 1.5 20.4 30.6#
87 0.0 11.2 16.8#









#47
Bromodichloromethane
Concen: 0.624 ug/l
RT: 9.740 min Scan# 21
Delta R.T. -0.019 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-B6S


Tgt Ion: 83 Resp: 7782
Ion Ratio Lower Upper
83 100
85 0.0 50.9 76.3#
127 0.0 7.1 10.7#

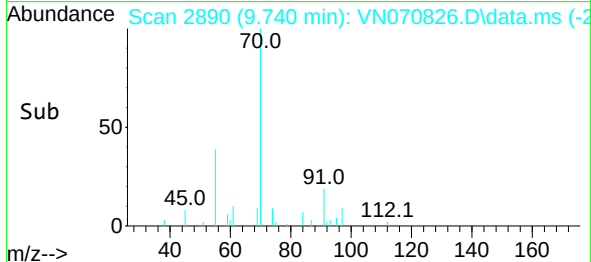

#49
1,4-Dioxane
Concen: 0.327 ug/l
RT: 9.587 min Scan# 2833
Delta R.T. 0.018 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03

Tgt Ion: 88 Resp: 59
Ion Ratio Lower Upper
88 100
43 0.0 23.4 35.2#
58 998.3 50.6 75.8#


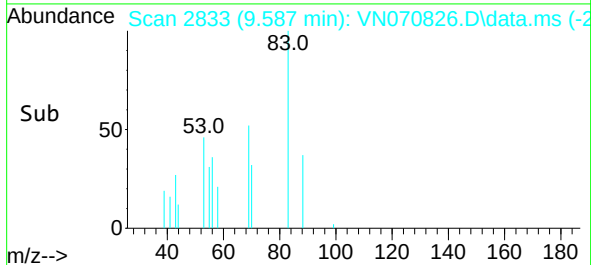






#50
Toluene-d8
Concen: 50.748 ug/l
RT: 10.440 min Scan# 3150
Delta R.T. 0.002 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-B6S


Tgt Ion: 98 Resp: 1579553
Ion Ratio Lower Upper
98 100
100 63.5 50.4 75.6

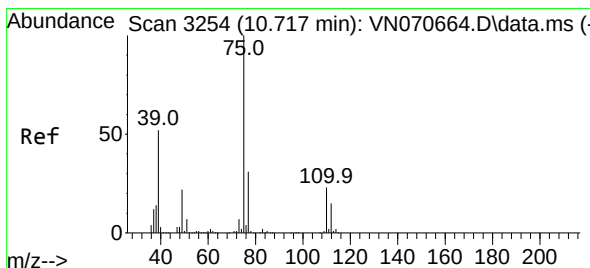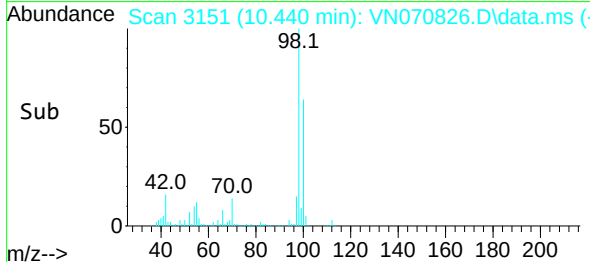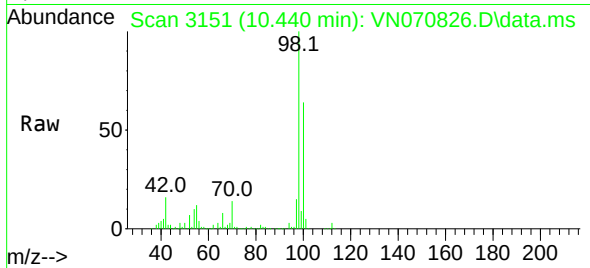

#53
t-1,3-Dichloropropene
Concen: 2.436 ug/l
RT: 10.714 min Scan# 3253
Delta R.T. -0.003 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03

Tgt Ion: 75 Resp: 513
Ion Ratio Lower Upper
75 100
77 37.1 25.6 38.4


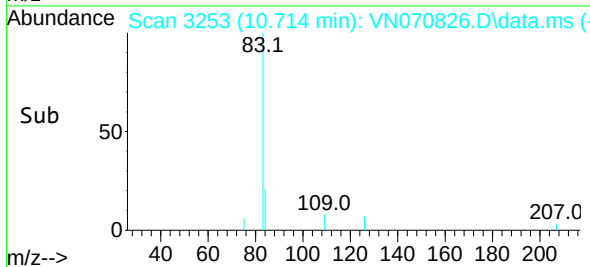

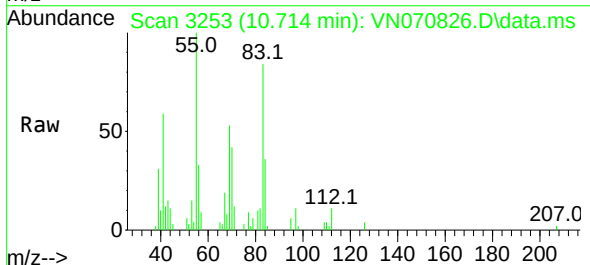




#55
1,1,2-Trichloroethane
Concen: 9.299 ug/l
RT: 10.872 min Scan# 311
Delta R.T. -0.024 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-B6S


Tgt Ion:	97	Resp:	84217
Ion	Ratio	Lower	Upper
97	100		
83	7.5	67.8	101.6#
85	8.2	45.4	68.2#
99	0.0	49.4	74.0#

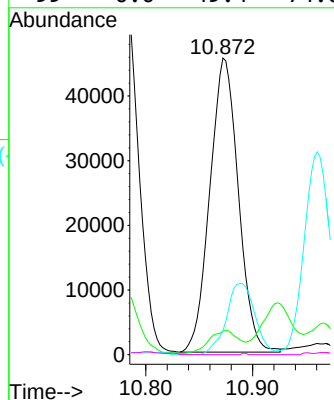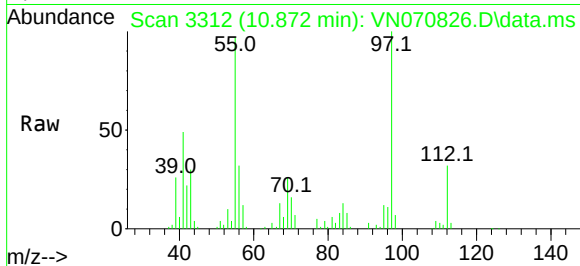

#56
Ethyl methacrylate
Concen: 4.096 ug/l
RT: 10.778 min Scan# 3277
Delta R.T. 0.018 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03

Tgt Ion:	69	Resp:	32393
Ion	Ratio	Lower	Upper
69	100		
41	170.8	51.4	77.0#
39	87.2	34.6	52.0#



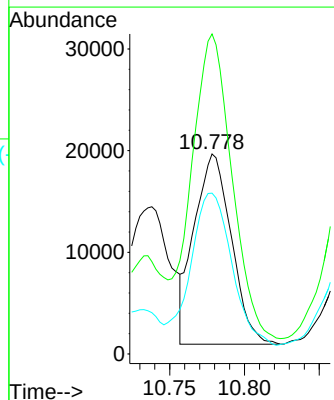
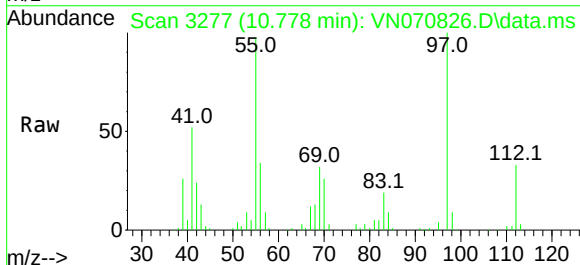




#58
2-Chloroethyl Vinyl ether
Concen: 21.269 ug/l
RT: 10.049 min Scan# 3001
Delta R.T. 0.011 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-B6S


Tgt Ion: 63 Resp: 155
Ion Ratio Lower Upper
63 100
106 0.0 23.9 35.9#

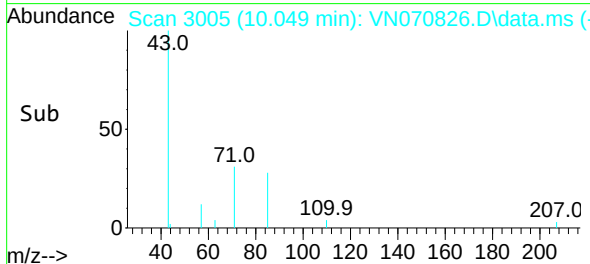

#59
2-Hexanone
Concen: 15.988 ug/l
RT: 11.049 min Scan# 3378
Delta R.T. -0.035 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03

Tgt Ion: 43 Resp: 186931
Ion Ratio Lower Upper
43 100
58 2.9 26.9 80.7#


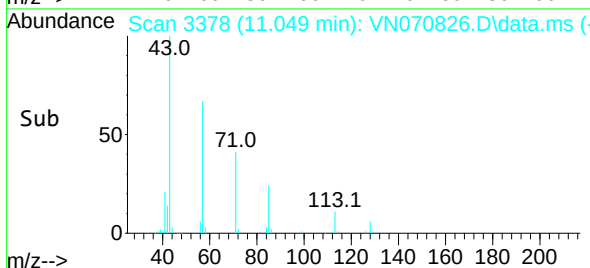
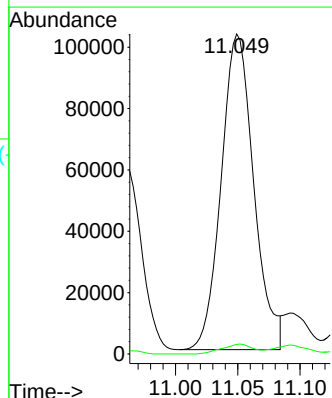
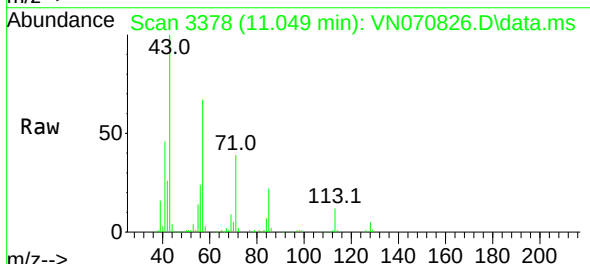




#62
4-Bromofluorobenzene
Concen: 54.365 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.003 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-B6S


Tgt Ion: 95 Resp: 602975
Ion Ratio Lower Upper
95 100
174 72.2 0.0 187.2
176 69.5 0.0 181.4

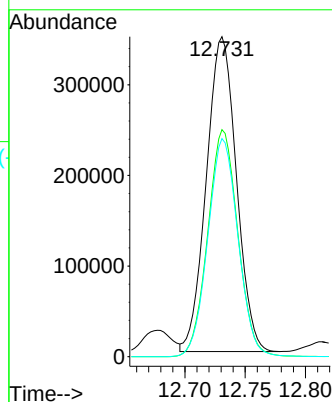

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3637
Delta R.T. 0.003 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03

Tgt Ion: 117 Resp: 1161021
Ion Ratio Lower Upper
117 100
82 60.5 42.4 63.6
119 32.6 25.4 38.2


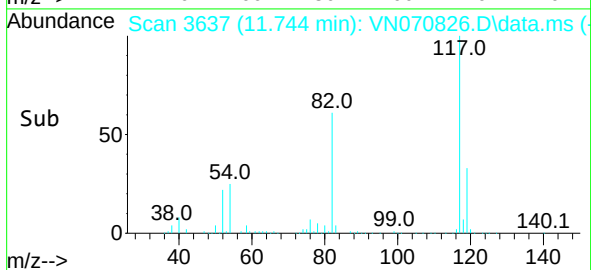






#68
m/p-Xylenes
Concen: 0.270 ug/l
RT: 11.953 min Scan# 31
Delta R.T. 0.003 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-B6S


Tgt Ion:106 Resp: 4577
Ion Ratio Lower Upper
106 100
91 264.1 160.6 240.8#



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 4357
Delta R.T. 0.003 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03

Tgt Ion:152 Resp: 564312
Ion Ratio Lower Upper
152 100
115 61.5 27.5 82.5
150 153.6 0.0 344.4


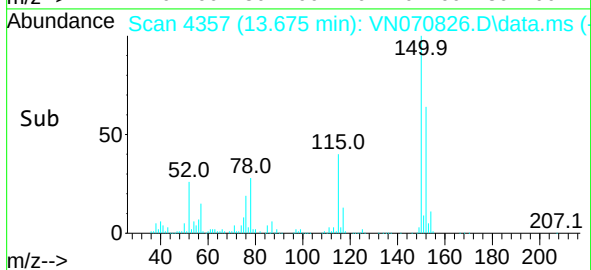






#73
Isopropylbenzene
Concen: 0.676 ug/l
RT: 12.578 min Scan# 3947
Delta R.T. 0.003 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-B6S


Tgt Ion:105 Resp: 36081
Ion Ratio Lower Upper
105 100
120 23.0 13.4 40.1



#74
N-ethyl acetate
Concen: 18.793 ug/l
RT: 12.366 min Scan# 3869
Delta R.T. -0.019 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03

Tgt Ion: 43 Resp: 410209
Ion Ratio Lower Upper
43 100
70 17.5 33.4 50.0#
55 27.3 19.3 28.9
61 0.1 18.5 27.7#


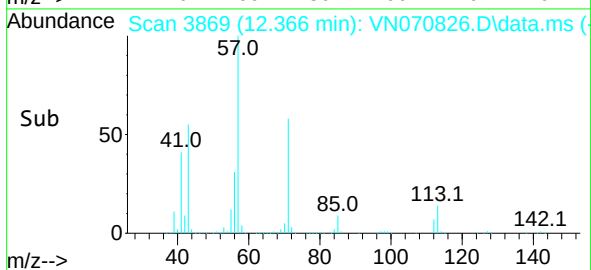






#75
 1,1,2,2-Tetrachloroethane
 Concen: 2.370 ug/l
 RT: 12.809 min Scan# 4034
 Delta R.T. -0.016 min
 Lab File: VN070826.D
 Acq: 28 Jan 2022 14:03




Instrument :
 MSVOA_N
 ClientSampleId :
 AREA-1-B-2@4-B6S


Tgt Ion: 83 Resp: 42724
 Ion Ratio Lower Upper
 83 100
 131 0.0 5.5 16.5#
 85 205.7 32.4 97.2#

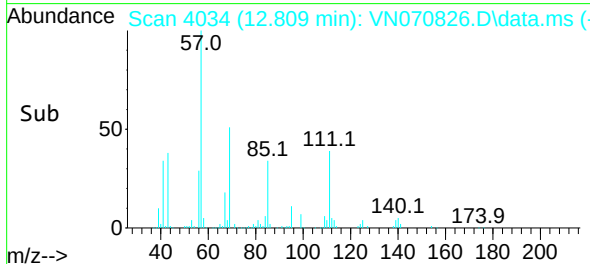

#76
 1,2,3-Trichloropropane
 Concen: 21.424 ug/l
 RT: 12.731 min Scan# 4005
 Delta R.T. -0.147 min
 Lab File: VN070826.D
 Acq: 28 Jan 2022 14:03

Tgt Ion: 75 Resp: 320654
 Ion Ratio Lower Upper
 75 100
 77 2.6 82.6 247.8#


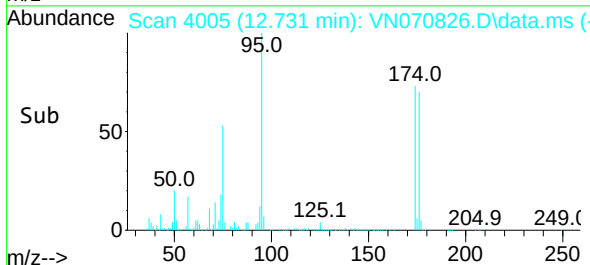
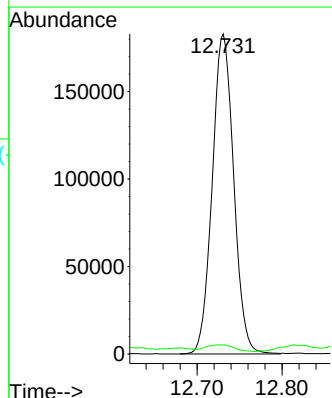
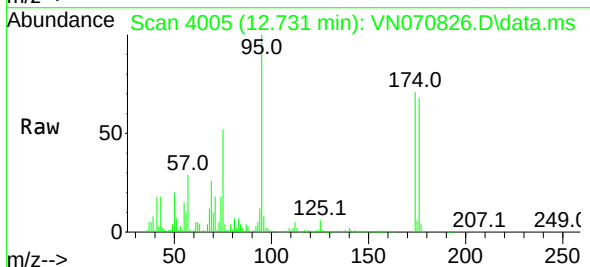




#78
n-propylbenzene
Concen: 0.453 ug/l
RT: 12.916 min Scan# 4075
Delta R.T. -0.003 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-B6S


Tgt Ion: 91 Resp: 27060
Ion Ratio Lower Upper
91 100
120 20.5 11.9 35.9

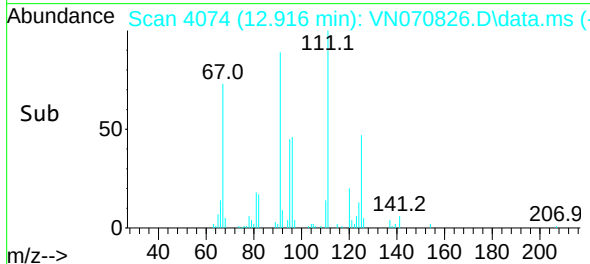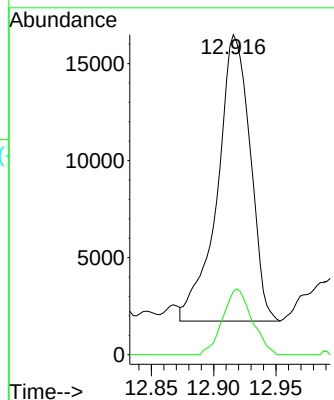

#81
trans-1,4-Dichloro-2-butene
Concen: 63.826 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.107 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03

Tgt Ion: 75 Resp: 320654
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 38.2 57.4#


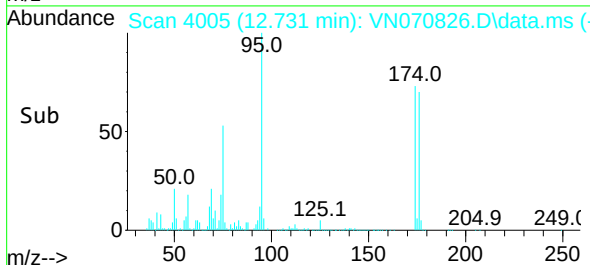
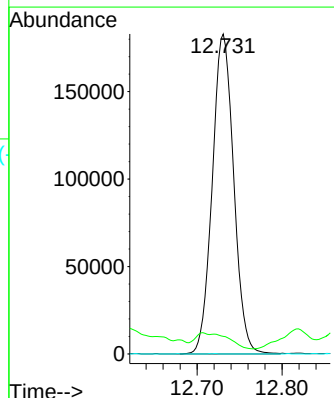
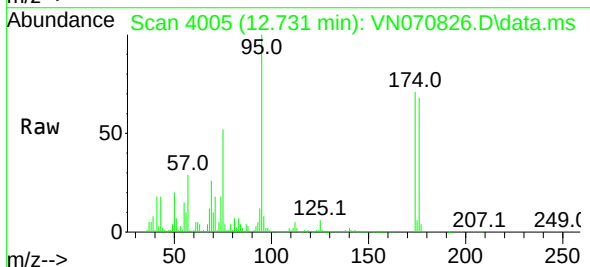




#85
 sec-Butylbenzene
 Concen: 0.447 ug/l
 RT: 13.500 min Scan# 41
 Delta R.T. 0.002 min
 Lab File: VN070826.D
 Acq: 28 Jan 2022 14:03




Instrument :
 MSVOA_N
 ClientSampleId :
 AREA-1-B-2@4-B6S


Tgt Ion:105 Resp: 22827
 Ion Ratio Lower Upper
 105 100
 134 36.1 10.4 31.1#

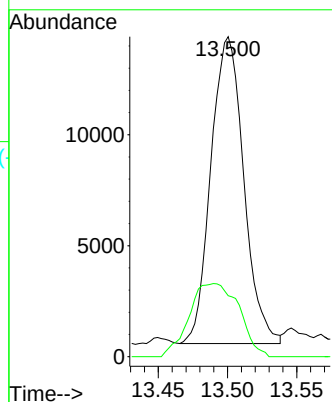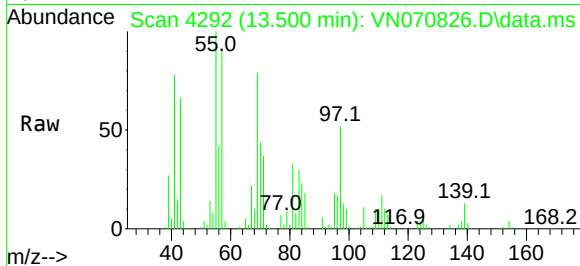

#89
 n-Butylbenzene
 Concen: 0.942 ug/l
 RT: 13.943 min Scan# 4457
 Delta R.T. 0.003 min
 Lab File: VN070826.D
 Acq: 28 Jan 2022 14:03

Tgt Ion: 91 Resp: 31202
 Ion Ratio Lower Upper
 91 100
 92 46.3 25.4 76.0
 134 0.0 13.6 40.8#









#90
Hexachloroethane
Concen: 2.949 ug/l
RT: 14.214 min Scan# 41
Delta R.T. 0.005 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03




Instrument :
MSVOA_N
ClientSampleId :
AREA-1-B-2@4-B6S


Tgt Ion:117 Resp: 20689
Ion Ratio Lower Upper
117 100
201 0.0 43.9 131.6#

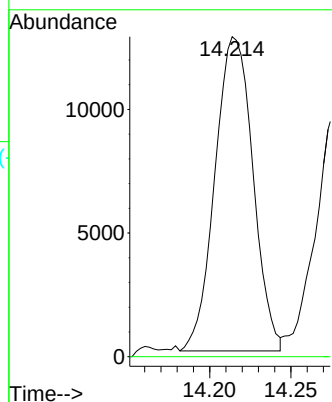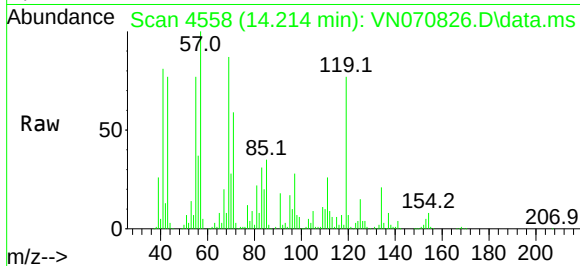

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.420 ug/l
RT: 14.611 min Scan# 4706
Delta R.T. 0.011 min
Lab File: VN070826.D
Acq: 28 Jan 2022 14:03

Tgt Ion: 75 Resp: 1286
Ion Ratio Lower Upper
75 100
155 0.0 46.9 140.7#
157 0.0 60.6 181.7#









#93
 1,2,4-Trichlorobenzene
 Concen: 3.838 ug/l
 RT: 15.260 min Scan# 4949
 Delta R.T. -0.003 min
 Lab File: VN070826.D
 Acq: 28 Jan 2022 14:03




Instrument :
 MSVOA_N
 ClientSampleId :
 AREA-1-B-2@4-B6S


Tgt Ion:180 Resp: 4625
 Ion Ratio Lower Upper
 180 100
 182 75.3 48.3 144.9
 145 987.5 14.5 43.5#

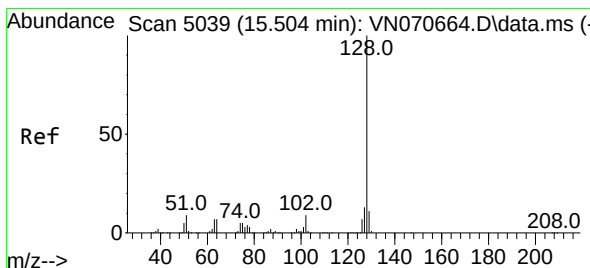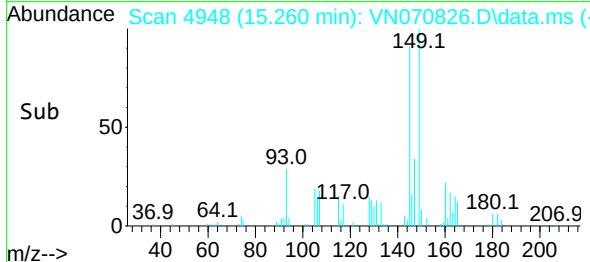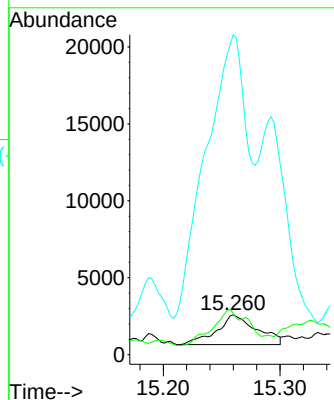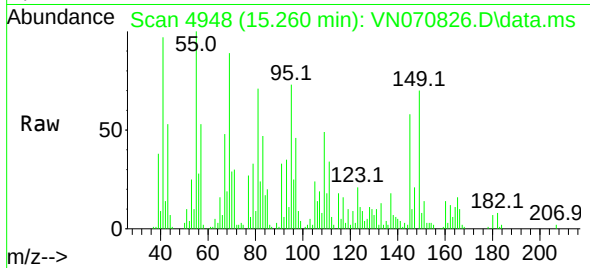

#95
 Naphthalene
 Concen: 5.329 ug/l
 RT: 15.504 min Scan# 5039
 Delta R.T. -0.000 min
 Lab File: VN070826.D
 Acq: 28 Jan 2022 14:03


Tgt Ion:128 Resp: 12354
 Ion Ratio Lower Upper
 128 100
 127 0.0 10.5 15.7#
 129 5.5 8.7 13.1#

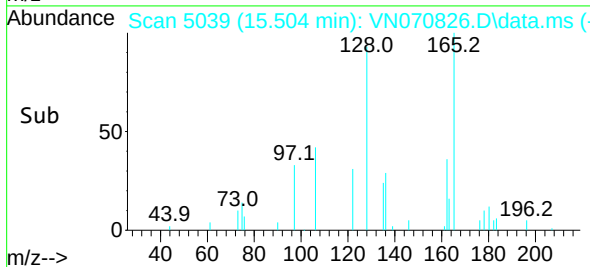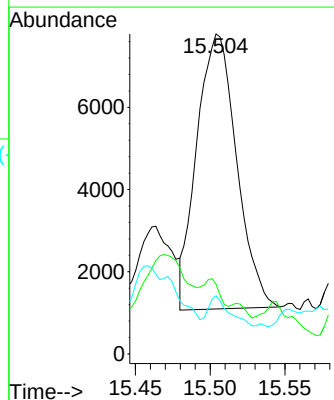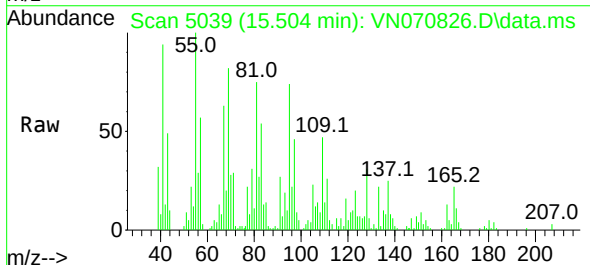



#96
 1,2,3-Trichlorobenzene
 Concen: 3.306 ug/l
 RT: 15.646 min Scan# 50
 Delta R.T. -0.051 min
 Lab File: VN070826.D
 Acq: 28 Jan 2022 14:03

Instrument :
 MSVOA_N
 ClientSampleId :
 AREA-1-B-2@4-B6S



Tgt Ion:180 Resp: 961
 Ion Ratio Lower Upper
 180 100
 182 0.0 47.4 142.2#
 145 0.0 15.0 45.1#

