

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012822\
 Data File : VN070829.D
 Acq On : 28 Jan 2022 15:19
 Operator : JC/MD
 Sample : PB142316ZHE#06
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB142316ZHE#06

Quant Time: Jan 28 23:17:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 18 13:32:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.086	168	987085	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	1652698	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	1530943	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	656692	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	670453	47.394	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	94.780%		
35) Dibromofluoromethane	8.024	113	462199	45.085	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	90.180%		
50) Toluene-d8	10.440	98	2056348	47.614	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	95.220%		
62) 4-Bromofluorobenzene	12.731	95	748095	48.610	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	97.220%		
Target Compounds						Qvalue
11) Tert butyl alcohol	5.385	59	3566	1.397	ug/l #	73
16) Acetone	4.296	43	56805	5.785	ug/l	98
20) Methylene Chloride	5.098	84	27212	2.104	ug/l	89
25) 2-Butanone	7.343	43	31643	2.561	ug/l	97
29) Tetrahydrofuran	7.699	42	3358	0.444	ug/l #	57
30) Chloroform	8.069	83	59	Below Cal	#	18
31) Cyclohexane	8.086	56	22596	0.907	ug/l #	11
36) 1,1-Dichloropropene	8.086	75	80629	4.672	ug/l #	48
37) Ethyl Acetate	7.343	43	31643	1.381	ug/l #	68
38) Carbon Tetrachloride	8.088	117	99708	6.494	ug/l #	16
43) Isopropyl Acetate	8.563	43	127616	3.646	ug/l #	83
48) Methyl methacrylate	9.545	41	29514	1.770	ug/l #	8
49) 1,4-Dioxane	9.609	88	219	0.874	ug/l #	27
51) 4-Methyl-2-Pentanone	10.333	43	15008	0.672	ug/l #	82
52) Toluene	10.507	92	17049	0.533	ug/l	98
53) t-1,3-Dichloropropene	10.719	75	287	2.417	ug/l #	43
54) cis-1,3-Dichloropropene	10.245	75	161947	7.809	ug/l #	60
56) Ethyl methacrylate	10.875	69	1910	2.378	ug/l #	1
57) 1,3-Dichloropropane	11.089	76	94432	4.245	ug/l #	43
59) 2-Hexanone	11.089	43	1552379	95.691	ug/l #	49
67) Ethyl Benzene	11.843	91	36830	0.599	ug/l	92
68) m/p-Xylenes	11.948	106	62982	2.815	ug/l	90
69) o-Xylene	12.277	106	9001	0.405	ug/l	82
74) N-amyl acetate	12.363	43	12205	0.480	ug/l #	52
76) 1,2,3-Trichloropropane	12.731	75	392281	22.523	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.058	105	11033	0.220	ug/l	94
81) trans-1,4-Dichloro-2-b...	12.731	75	392281	67.099	ug/l #	5
84) 1,2,4-Trimethylbenzene	13.369	105	15896	0.329	ug/l	97
93) 1,2,4-Trichlorobenzene	15.262	180	1227	3.519	ug/l	76
95) Naphthalene	15.507	128	32777	5.816	ug/l	98
96) 1,2,3-Trichlorobenzene	15.700	180	1404	3.329	ug/l #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012822\
Data File : VN070829.D
Acq On : 28 Jan 2022 15:19
Operator : JC/MD
Sample : PB142316ZHE#06
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#06

Quant Time: Jan 28 23:17:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 18 13:32:07 2022
Response via : Initial Calibration




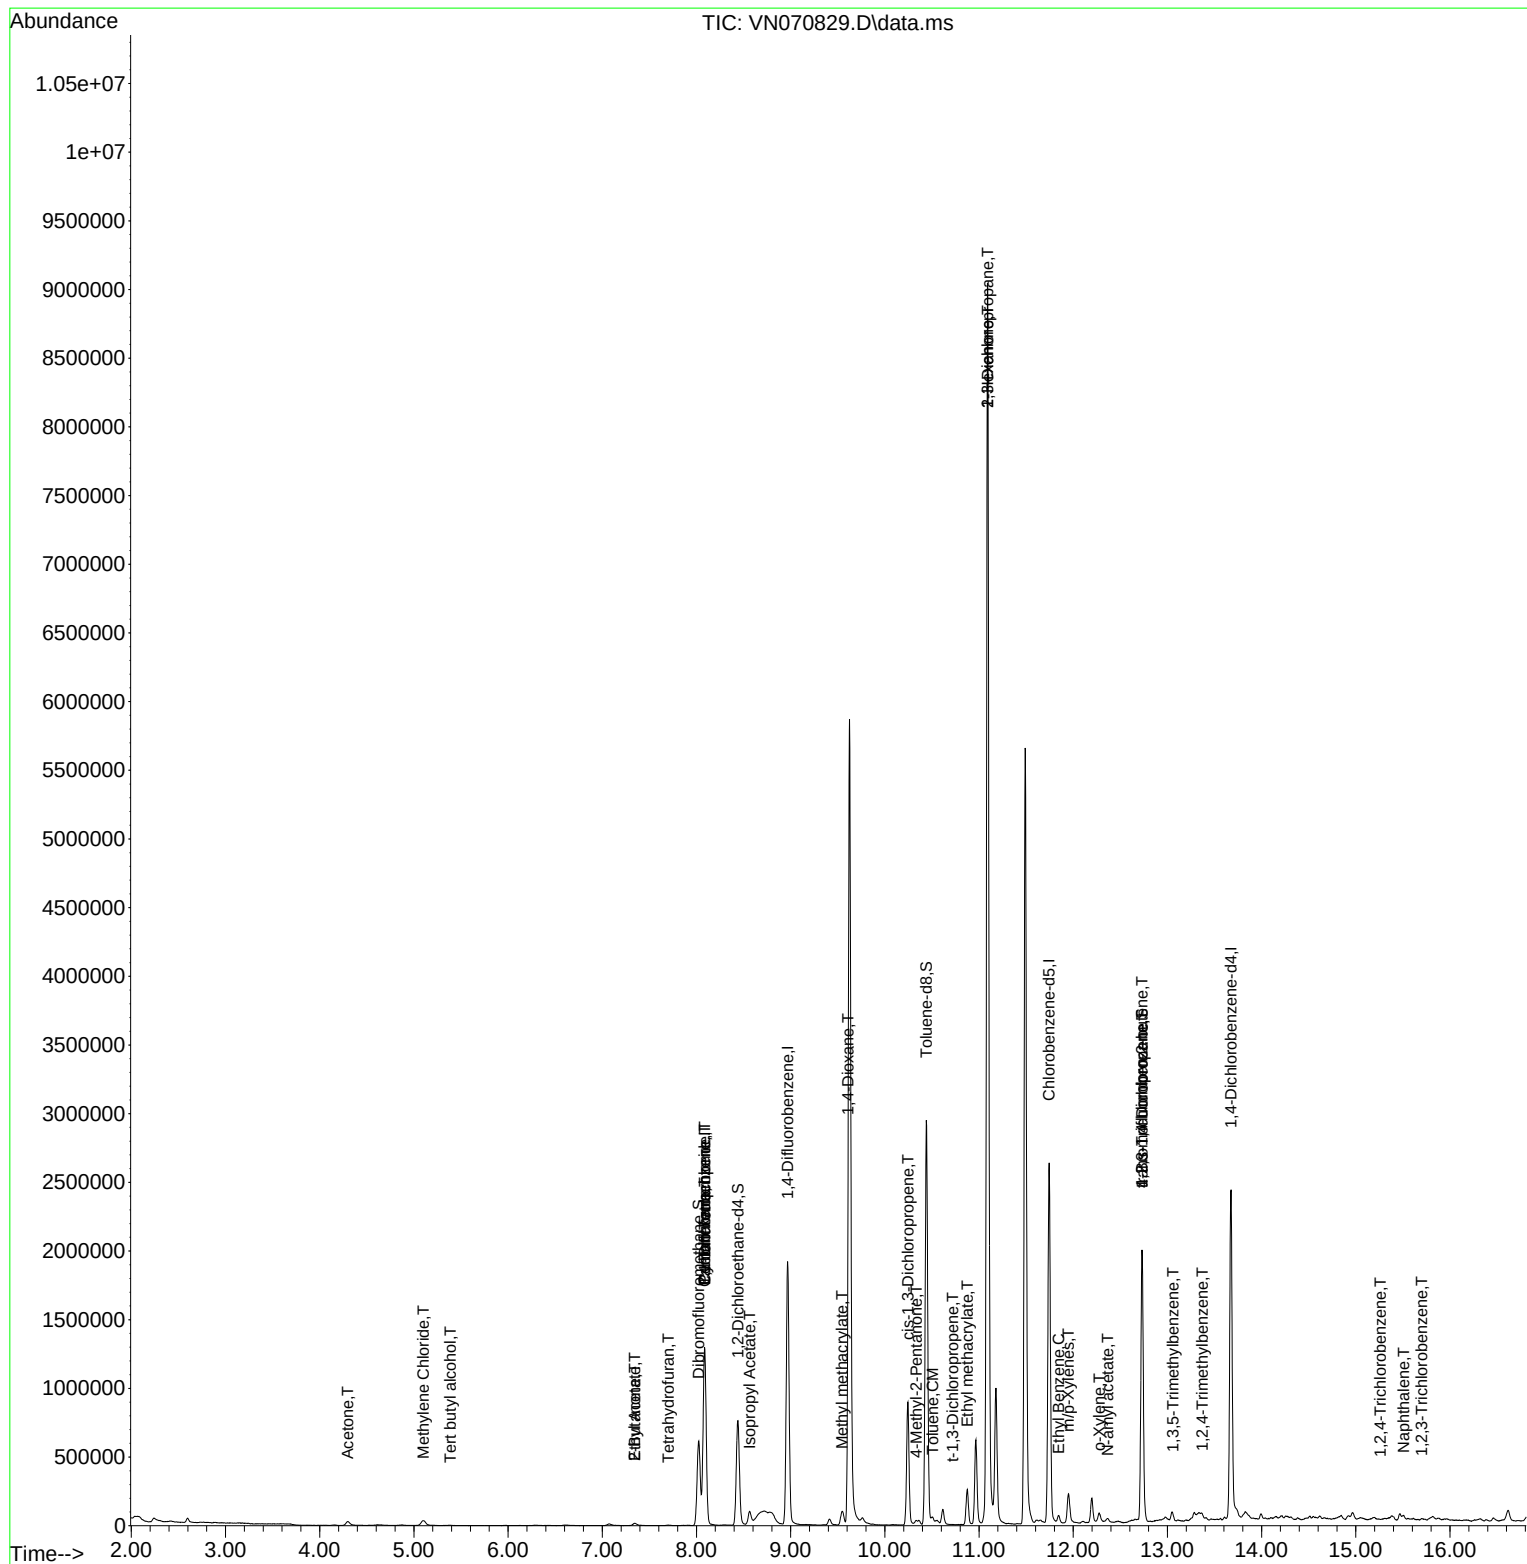




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 21
Delta R.T. 0.003 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#06


Tgt Ion:168 Resp: 987085
Ion Ratio Lower Upper
168 100
99 61.3 41.3 61.9

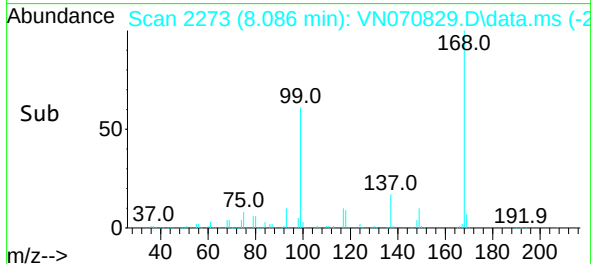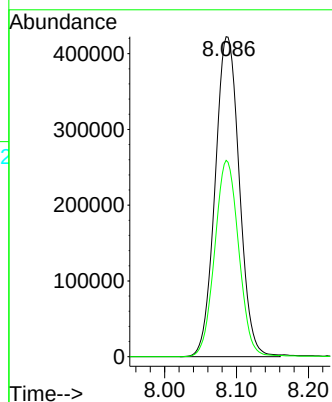

#11
Tert butyl alcohol
Concen: 1.397 ug/l
RT: 5.385 min Scan# 1266
Delta R.T. 0.008 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19

Tgt Ion: 59 Resp: 3566
Ion Ratio Lower Upper
59 100
57 0.7 8.7 13.1#


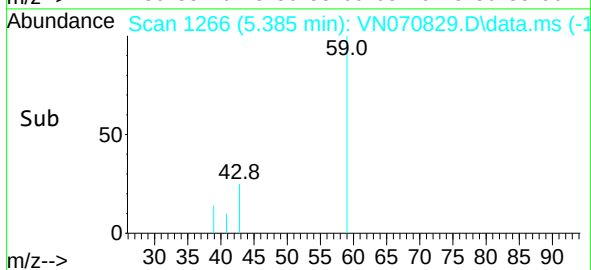
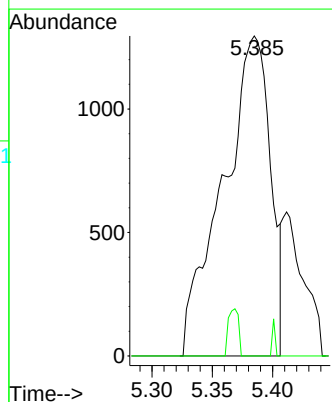
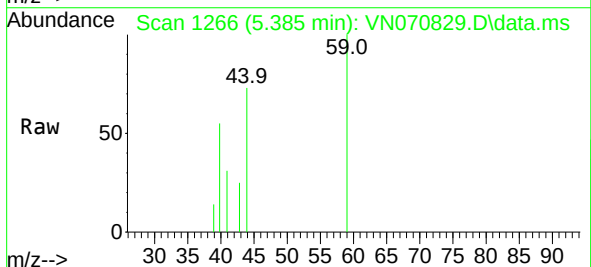




#16
Acetone
Concen: 5.785 ug/l
RT: 4.296 min Scan# 80
Delta R.T. 0.011 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#06


Tgt Ion: 43 Resp: 56805
Ion Ratio Lower Upper
43 100
58 28.0 23.1 34.7

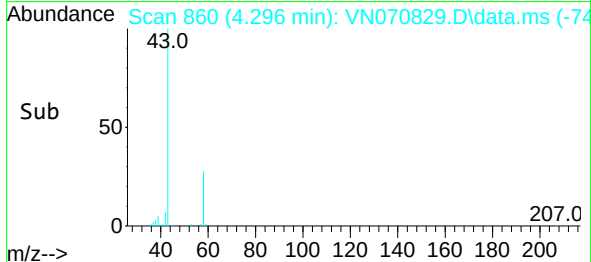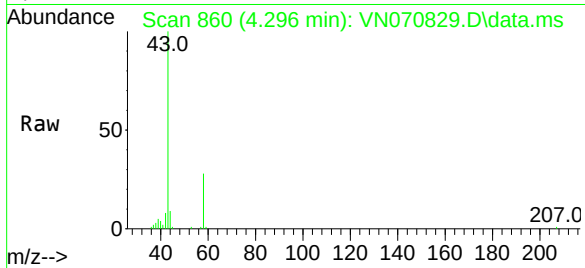

#20
Methylene Chloride
Concen: 2.104 ug/l
RT: 5.098 min Scan# 1159
Delta R.T. 0.003 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19

Tgt Ion: 84 Resp: 27212
Ion Ratio Lower Upper
84 100
49 133.8 93.5 140.3
51 39.0 29.4 44.2
86 59.5 53.0 79.4

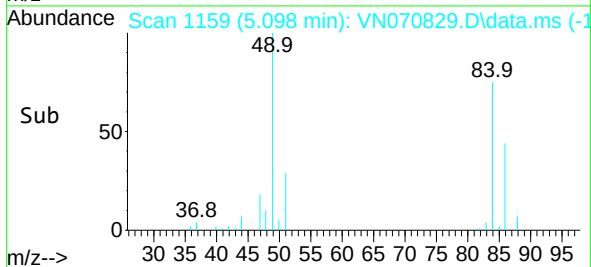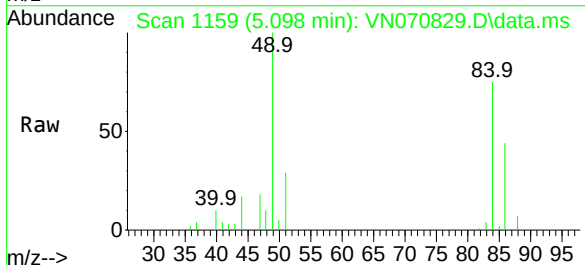

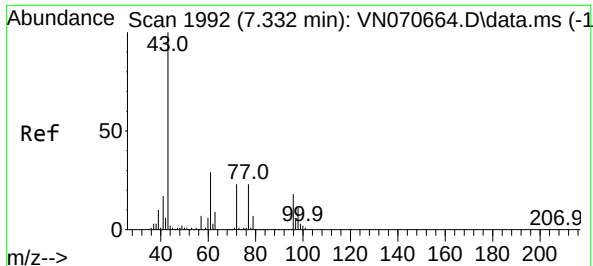

#25

2-Butanone

Concen: 2.561 ug/l

RT: 7.343 min Scan# 1992

Delta R.T. 0.011 min

Lab File: VN070829.D

Acq: 28 Jan 2022 15:19

Instrument :

MSVOA_N

ClientSampleId :





PB142316ZHE#06

Tgt Ion: 43 Resp: 31643

Ion Ratio Lower Upper

43 100

72 25.7 21.7 32.5

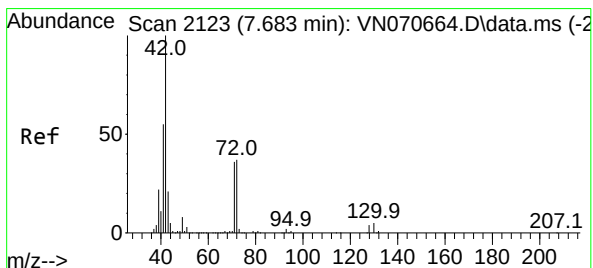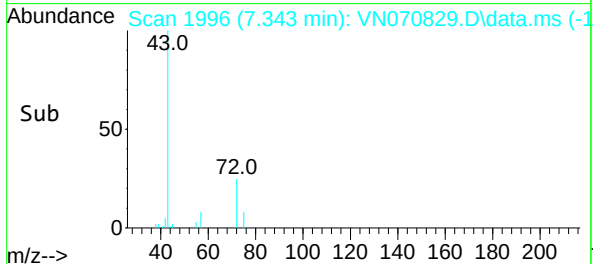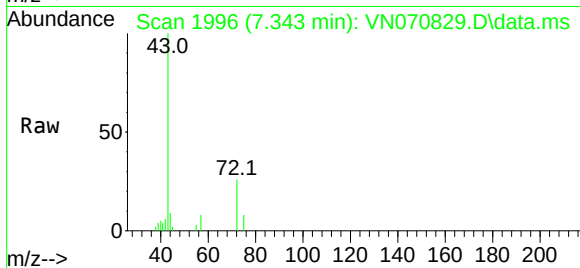

#29

Tetrahydrofuran

Concen: 0.444 ug/l

RT: 7.699 min Scan# 2129

Delta R.T. 0.016 min

Lab File: VN070829.D

Acq: 28 Jan 2022 15:19




Tgt Ion: 42 Resp: 3358


Ion Ratio Lower Upper

42 100

72 11.1 36.3 54.5#

71 22.0 34.7 52.1#


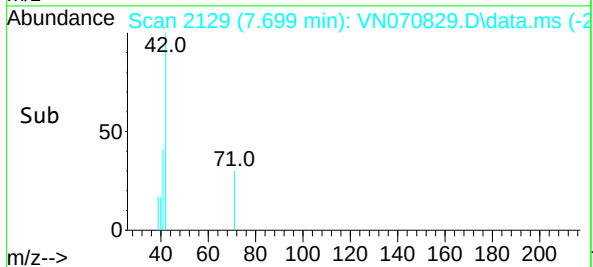

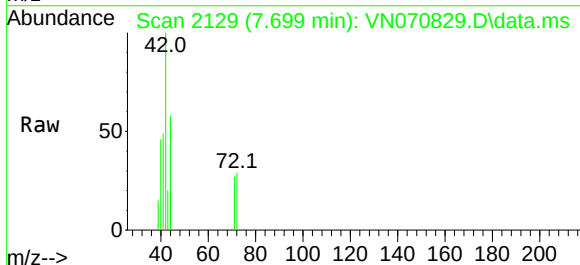




#30
Chloroform
Concen: Below Cal
RT: 8.069 min Scan# 2173
Delta R.T. 0.251 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#06


Tgt Ion: 83 Resp: 59
Ion Ratio Lower Upper
83 100
85 0.0 51.9 77.9#

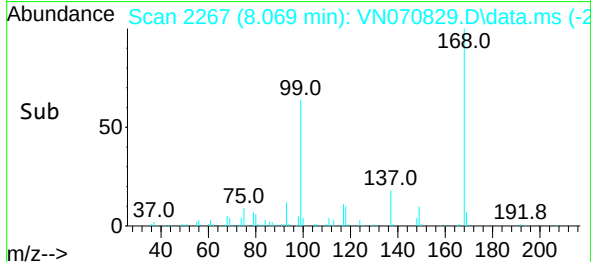

#31
Cyclohexane
Concen: 0.907 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.008 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19

Tgt Ion: 56 Resp: 22596
Ion Ratio Lower Upper
56 100
69 159.3 27.1 40.7#
84 130.1 73.4 110.0#

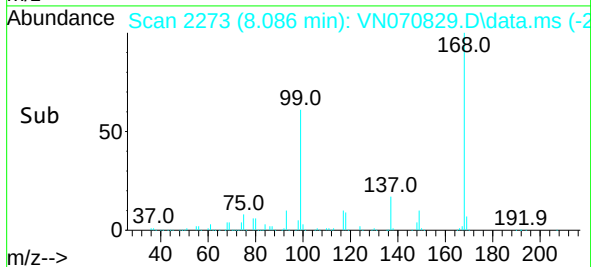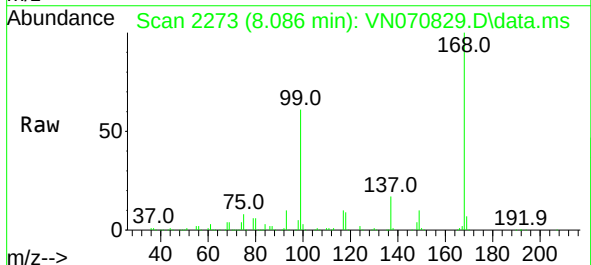



#33

1,2-Dichloroethane-d4

Concen: 47.394 ug/l

RT: 8.440 min Scan# 2403

Delta R.T. 0.006 min

Lab File: VN070829.D

Acq: 28 Jan 2022 15:19

Instrument :

MSVOA_N

ClientSampleId :





PB142316ZHE#06

Tgt Ion: 65 Resp: 670453

Ion Ratio Lower Upper

65 100

67 53.1 0.0 103.0

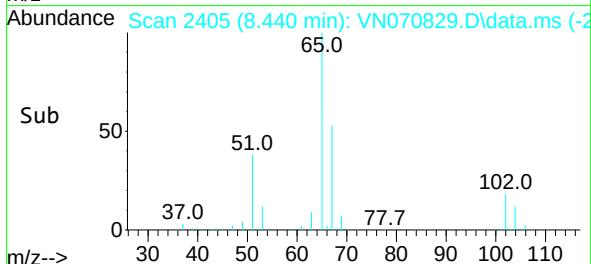

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.968 min Scan# 2602

Delta R.T. 0.003 min

Lab File: VN070829.D

Acq: 28 Jan 2022 15:19




Tgt Ion: 114 Resp: 1652698


Ion Ratio Lower Upper

114 100

63 23.0 0.0 37.8

88 17.2 0.0 27.4


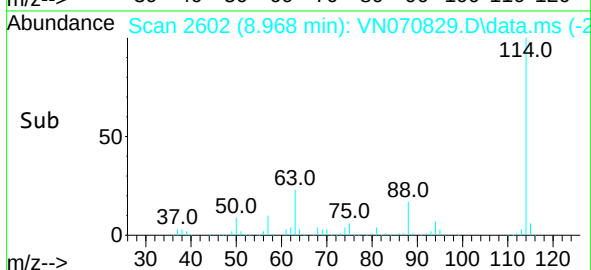






#35
Dibromofluoromethane
Concen: 45.085 ug/l
RT: 8.024 min Scan# 21
Delta R.T. 0.005 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#06


Tgt Ion:113 Resp: 462199
Ion Ratio Lower Upper
113 100
111 103.6 82.2 123.2
192 19.4 16.9 25.3

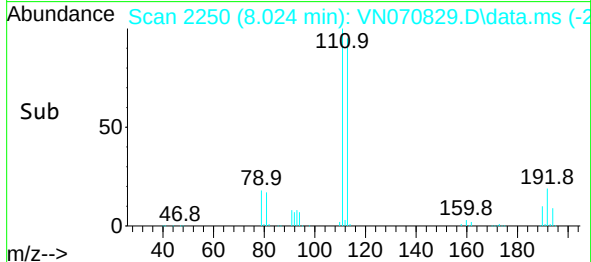

#36
1,1-Dichloropropene
Concen: 4.672 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.134 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19

Tgt Ion: 75 Resp: 80629
Ion Ratio Lower Upper
75 100
110 8.2 18.4 55.2#
77 0.0 24.4 36.6#

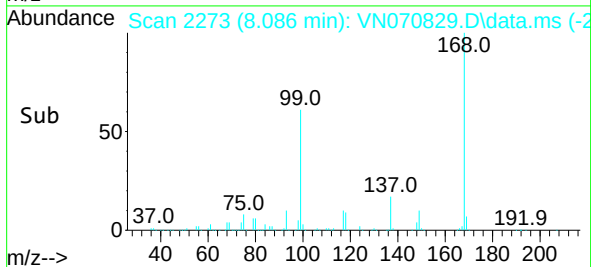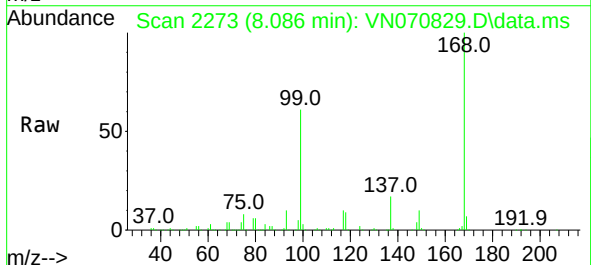



#37

Ethyl Acetate

Concen: 1.381 ug/l

RT: 7.343 min Scan# 1996

Delta R.T. -0.067 min

Lab File: VN070829.D


Acq: 28 Jan 2022 15:19

Instrument :

MSVOA_N

ClientSampleId :

PB142316ZHE#06

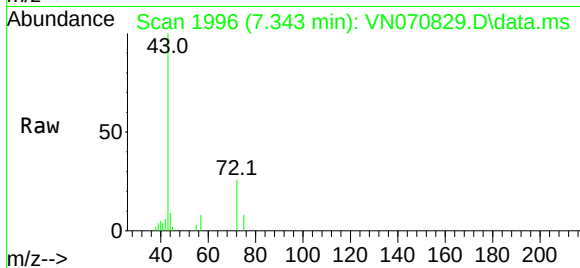




Tgt Ion: 43 Resp: 31643

Ion Ratio Lower Upper

43 100

61 0.0 11.5 17.3#

70 0.0 7.9 11.9#

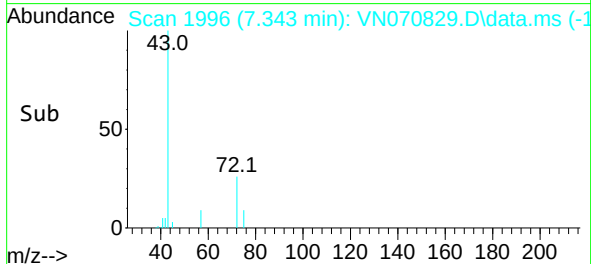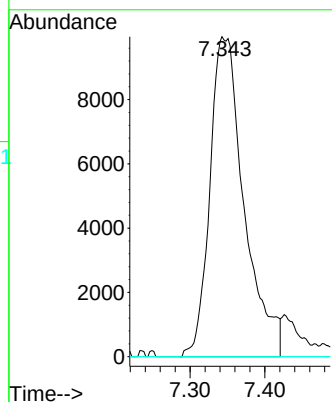

#38

Carbon Tetrachloride

Concen: 6.494 ug/l

RT: 8.088 min Scan# 2274

Delta R.T. -0.118 min

Lab File: VN070829.D

Acq: 28 Jan 2022 15:19




Tgt Ion: 117 Resp: 99708


Ion Ratio Lower Upper

117 100

119 4.9 76.1 114.1#

121 0.0 24.2 36.2#


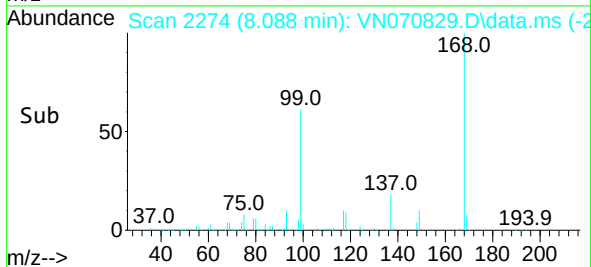
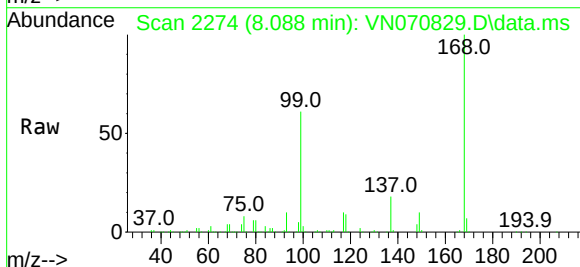
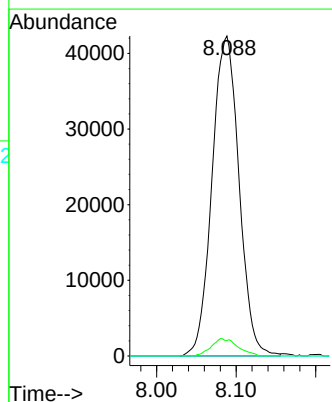




#43
Isopropyl Acetate
Concen: 3.646 ug/l
RT: 8.563 min Scan# 24
Delta R.T. 0.003 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#06


Tgt Ion: 43 Resp: 127616
Ion Ratio Lower Upper
43 100
61 14.8 20.4 30.6#
87 9.8 11.2 16.8#

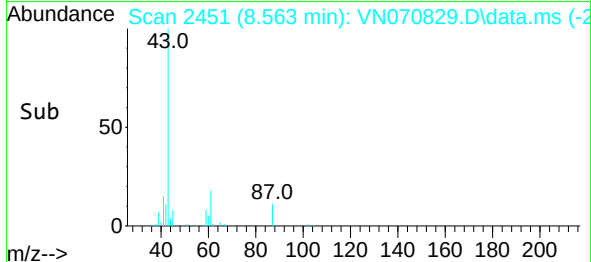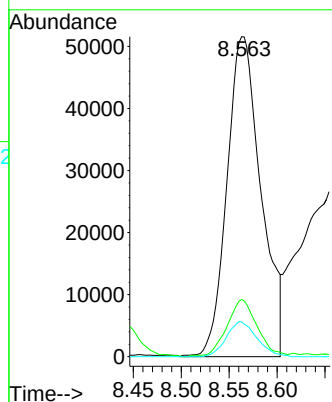

#48
Methyl methacrylate
Concen: 1.770 ug/l
RT: 9.545 min Scan# 2817
Delta R.T. -0.013 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19

Tgt Ion: 41 Resp: 29514
Ion Ratio Lower Upper
41 100
69 0.5 72.4 108.6#
39 0.0 58.4 87.6#

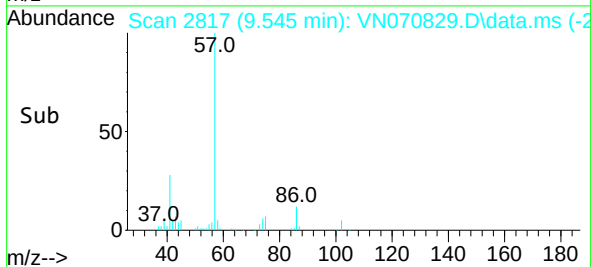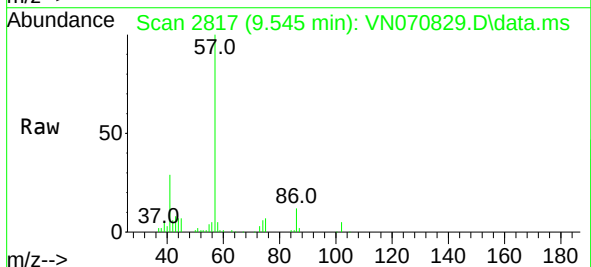



#49

1,4-Dioxane

Concen: 0.874 ug/l

RT: 9.609 min Scan# 219

Delta R.T. 0.040 min

Lab File: VN070829.D

Acq: 28 Jan 2022 15:19

Instrument :

MSVOA_N

ClientSampleId :

PB142316ZHE#06





Tgt Ion: 88 Resp: 219

Ion Ratio Lower Upper

88 100

43 0.0 23.4 35.2#

58 0.0 50.6 75.8#

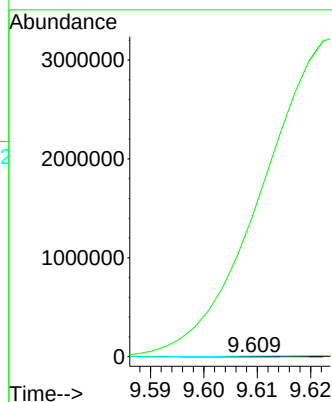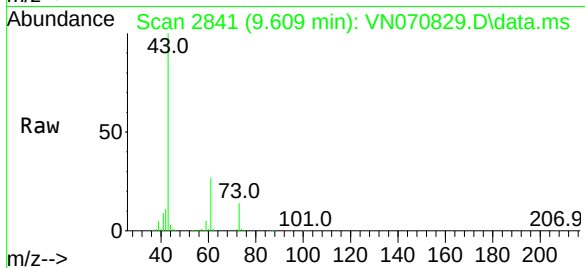

#50

Toluene-d8

Concen: 47.614 ug/l

RT: 10.440 min Scan# 3151

Delta R.T. 0.002 min

Lab File: VN070829.D




Acq: 28 Jan 2022 15:19


Tgt Ion: 98 Resp: 2056348

Ion Ratio Lower Upper

98 100

100 64.7 50.4 75.6


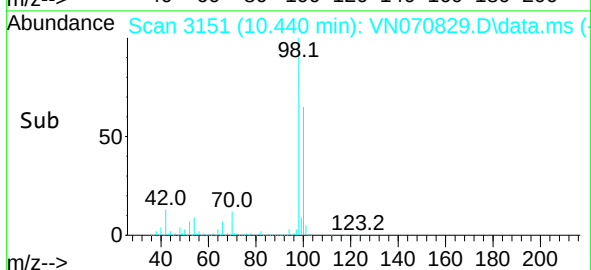

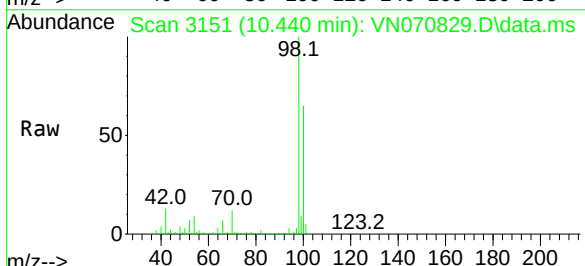




#51
4-Methyl-2-Pentanone
Concen: 0.672 ug/l
RT: 10.333 min Scan# 3111
Delta R.T. 0.005 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#06


Tgt Ion: 43 Resp: 15008
Ion Ratio Lower Upper
43 100
58 48.7 30.4 45.6#

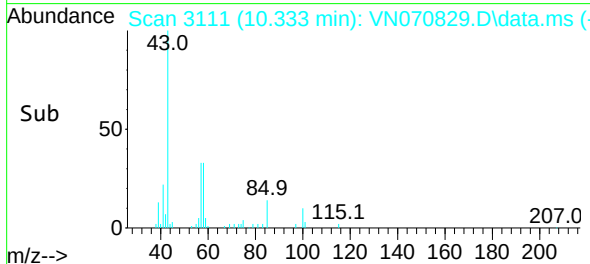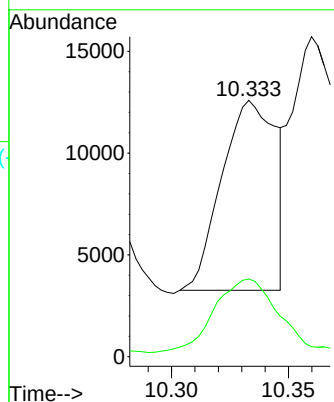

#52
Toluene
Concen: 0.533 ug/l
RT: 10.507 min Scan# 3176
Delta R.T. 0.005 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19

Tgt Ion: 92 Resp: 17049
Ion Ratio Lower Upper
92 100
91 174.1 142.0 213.0


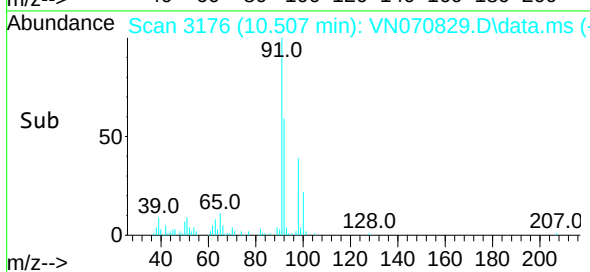
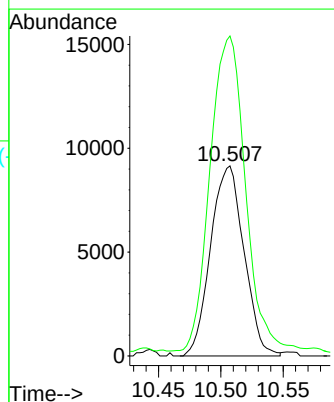





#53
 t-1,3-Dichloropropene
 Concen: 2.417 ug/l
 RT: 10.719 min Scan# 31
 Delta R.T. 0.002 min
 Lab File: VN070829.D
 Acq: 28 Jan 2022 15:19




Instrument :
 MSVOA_N
 ClientSampleId :
 PB142316ZHE#06


Tgt Ion: 75 Resp: 287
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.6 38.4#

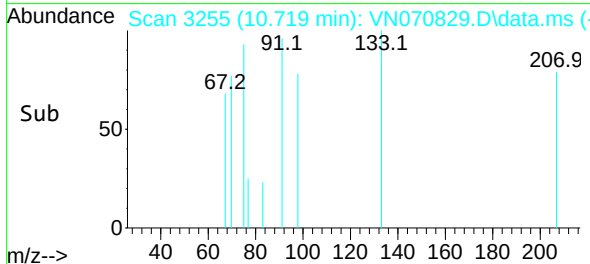

#54
 cis-1,3-Dichloropropene
 Concen: 7.809 ug/l
 RT: 10.245 min Scan# 3078
 Delta R.T. 0.057 min
 Lab File: VN070829.D
 Acq: 28 Jan 2022 15:19

Tgt Ion: 75 Resp: 161947
 Ion Ratio Lower Upper
 75 100
 77 0.6 26.4 39.6#
 39 32.7 42.5 63.7#


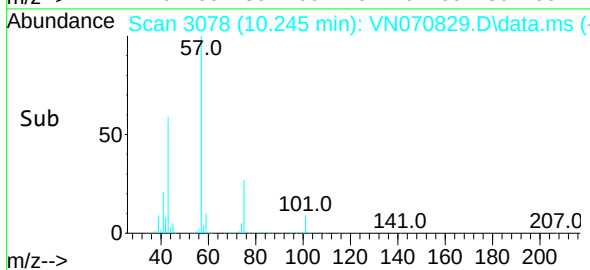

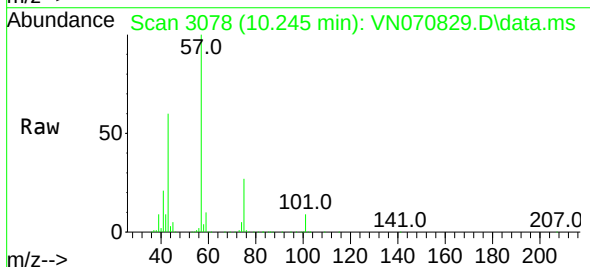




#56
Ethyl methacrylate
Concen: 2.378 ug/l
RT: 10.875 min Scan# 311
Delta R.T. 0.115 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#06


Tgt Ion: 69 Resp: 1910
Ion Ratio Lower Upper
69 100
41 2696.0 51.4 77.0#
39 1097.6 34.6 52.0#

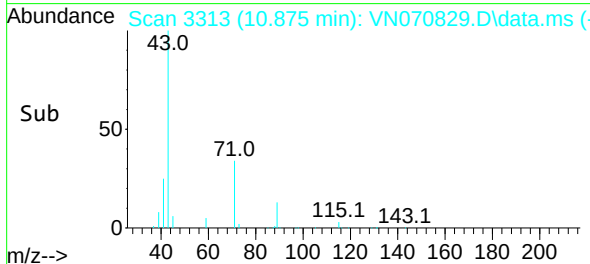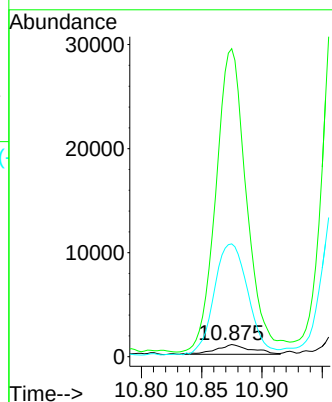

#57
1,3-Dichloropropane
Concen: 4.245 ug/l
RT: 11.089 min Scan# 3393
Delta R.T. 0.045 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19

Tgt Ion: 76 Resp: 94432
Ion Ratio Lower Upper
76 100
78 0.4 25.7 38.5#


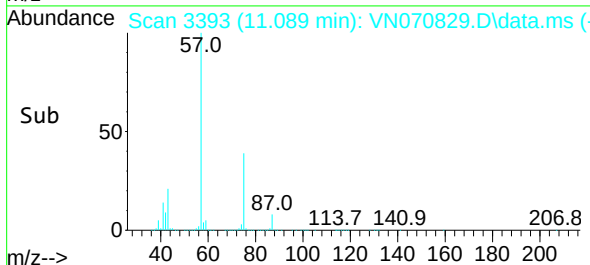

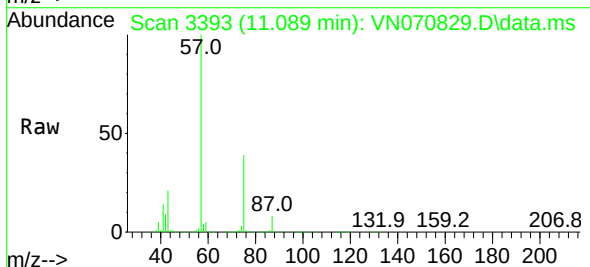




#59
2-Hexanone
Concen: 95.691 ug/l
RT: 11.089 min Scan# 31
Delta R.T. 0.005 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#06


Tgt Ion: 43 Resp: 1552379
Ion Ratio Lower Upper
43 100
58 17.6 26.9 80.7#

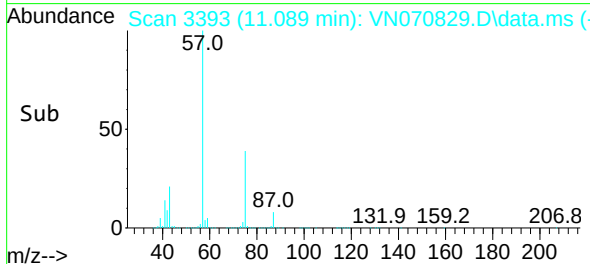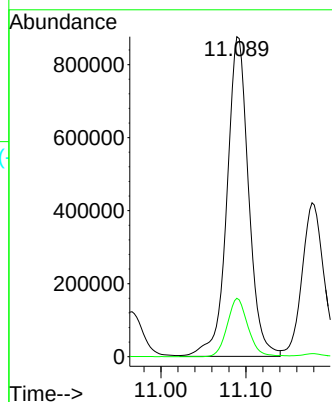

#62
4-Bromofluorobenzene
Concen: 48.610 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.003 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19

Tgt Ion: 95 Resp: 748095
Ion Ratio Lower Upper
95 100
174 74.2 0.0 187.2
176 71.3 0.0 181.4


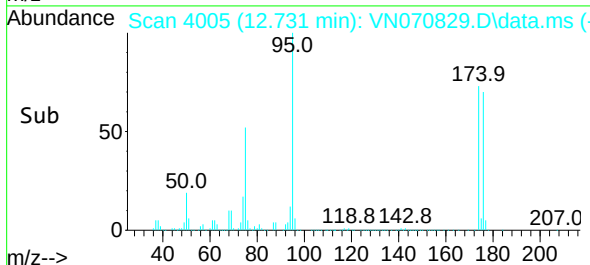

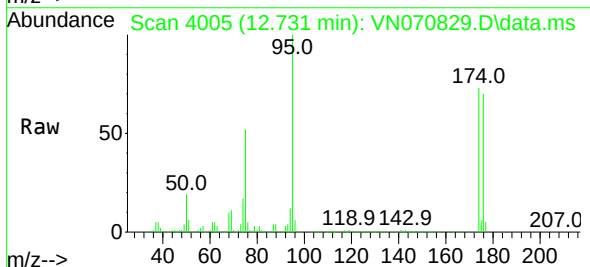




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3636
Delta R.T. 0.003 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#06


Tgt Ion:117 Resp: 1530943
Ion Ratio Lower Upper
117 100
82 60.3 42.4 63.6
119 32.1 25.4 38.2

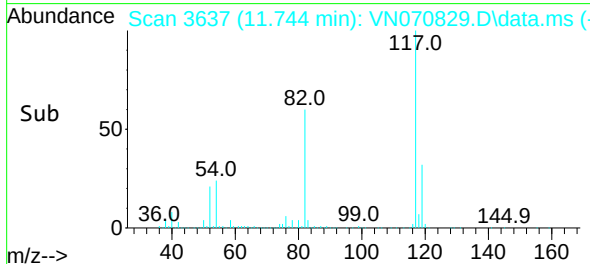

#67
Ethyl Benzene
Concen: 0.599 ug/l
RT: 11.843 min Scan# 3674
Delta R.T. 0.000 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19

Tgt Ion: 91 Resp: 36830
Ion Ratio Lower Upper
91 100
106 27.8 25.7 38.5


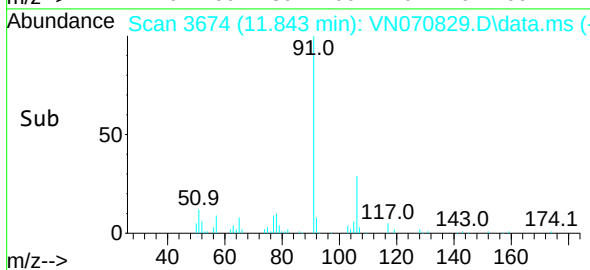

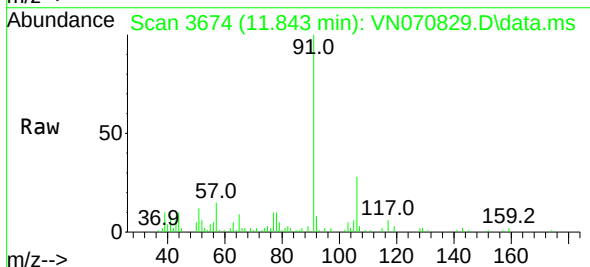




#68
m/p-Xylenes
Concen: 2.815 ug/l
RT: 11.948 min Scan# 31
Delta R.T. -0.002 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#06


Tgt Ion:106 Resp: 62982
Ion Ratio Lower Upper
106 100
91 216.4 160.6 240.8

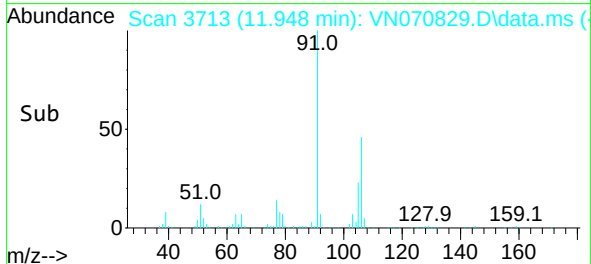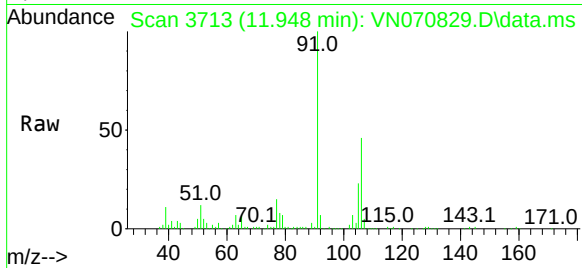

#69
o-Xylene
Concen: 0.405 ug/l
RT: 12.277 min Scan# 3836
Delta R.T. -0.001 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19

Tgt Ion:106 Resp: 9001
Ion Ratio Lower Upper
106 100
91 240.3 105.8 317.3



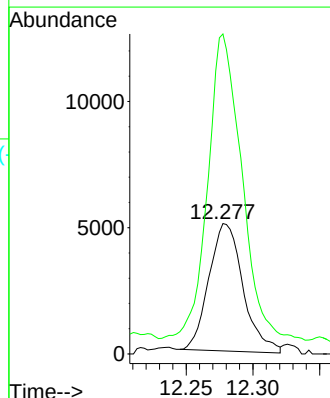
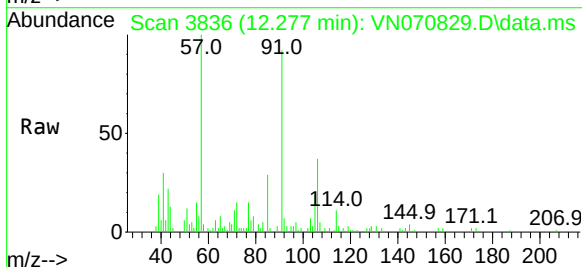




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 41
Delta R.T. 0.003 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#06


Tgt Ion:152 Resp: 656692
Ion Ratio Lower Upper
152 100
115 63.6 27.5 82.5
150 156.0 0.0 344.4

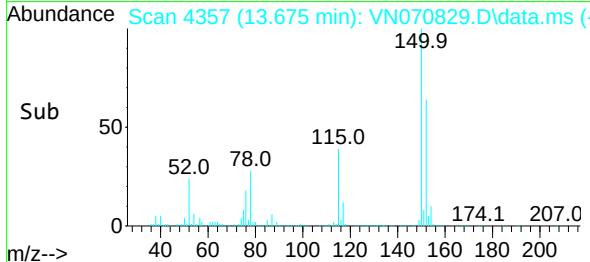

#74
N-ethyl acetate
Concen: 0.480 ug/l
RT: 12.363 min Scan# 3868
Delta R.T. -0.022 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19

Tgt Ion: 43 Resp: 12205
Ion Ratio Lower Upper
43 100
70 4.0 33.4 50.0#
55 11.2 19.3 28.9#
61 0.0 18.5 27.7#


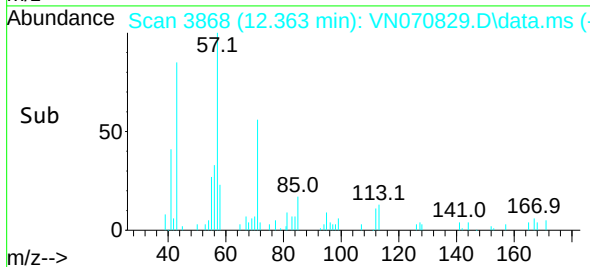

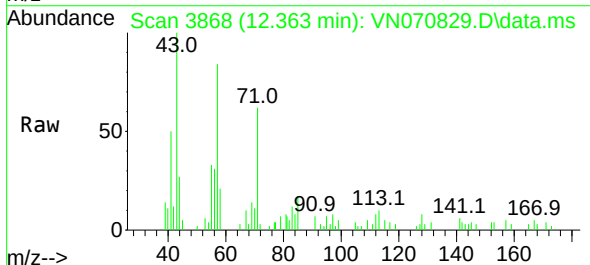




#76
1,2,3-Trichloropropane
Concen: 22.523 ug/l
RT: 12.731 min Scan# 4060
Delta R.T. -0.147 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#06


Tgt Ion: 75 Resp: 392281
Ion Ratio Lower Upper
75 100
77 1.3 82.6 247.8#

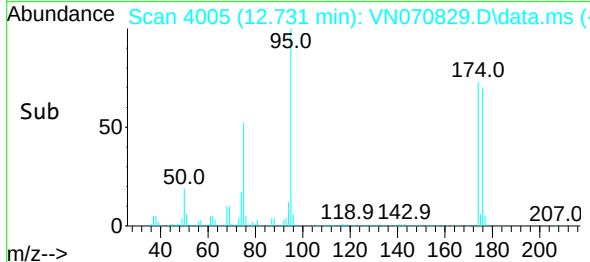

#80
1,3,5-Trimethylbenzene
Concen: 0.220 ug/l
RT: 13.058 min Scan# 4127
Delta R.T. -0.000 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19

Tgt Ion: 105 Resp: 11033
Ion Ratio Lower Upper
105 100
120 53.0 24.6 73.6


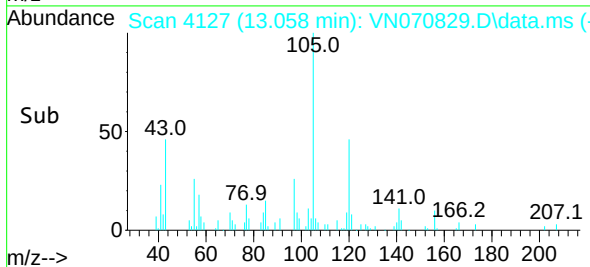

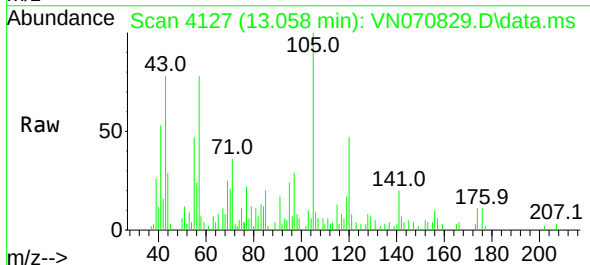




#81
trans-1,4-Dichloro-2-butene
Concen: 67.099 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.107 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#06


Tgt Ion: 75 Resp: 392281
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 38.2 57.4#

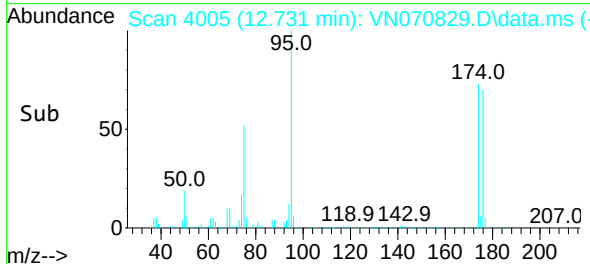

#84
1,2,4-Trimethylbenzene
Concen: 0.329 ug/l
RT: 13.369 min Scan# 4243
Delta R.T. 0.002 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19

Tgt Ion: 105 Resp: 15896
Ion Ratio Lower Upper
105 100
120 43.8 22.8 68.4


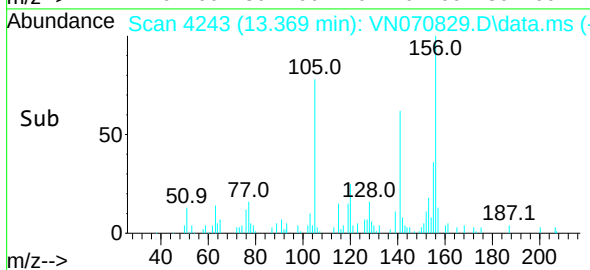

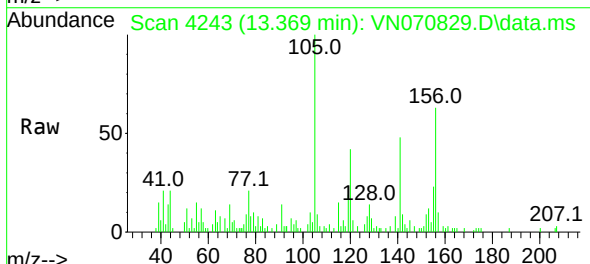




#93
1,2,4-Trichlorobenzene
Concen: 3.519 ug/l
RT: 15.262 min Scan# 4949
Delta R.T. -0.001 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#06


Tgt Ion:180 Resp: 1227
Ion Ratio Lower Upper
180 100
182 120.0 48.3 144.9
145 41.6 14.5 43.5

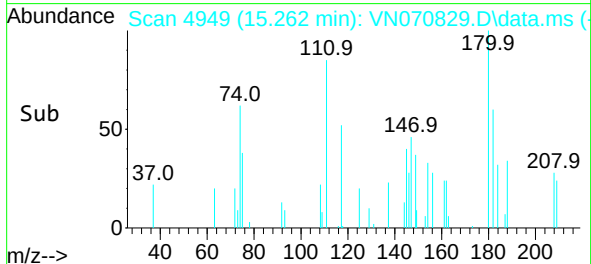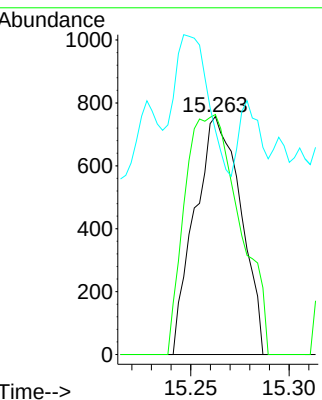

#95
Naphthalene
Concen: 5.816 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. 0.003 min
Lab File: VN070829.D
Acq: 28 Jan 2022 15:19


Tgt Ion:128 Resp: 32777
Ion Ratio Lower Upper
128 100
127 13.8 10.5 15.7
129 11.6 8.7 13.1

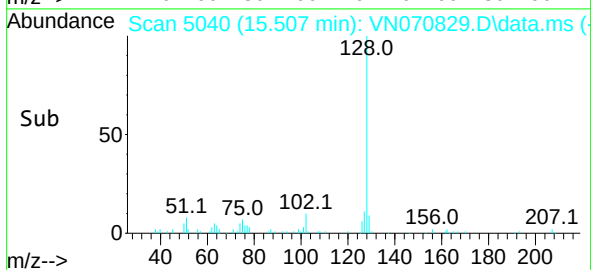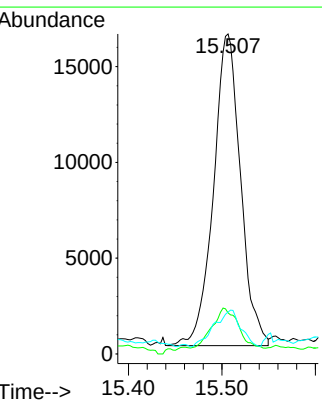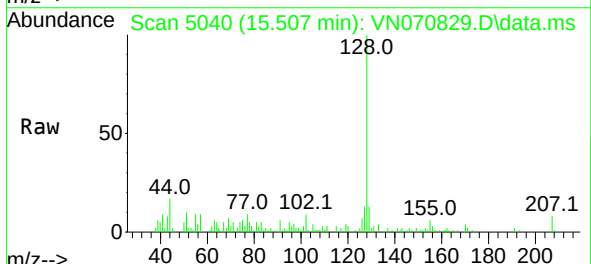



#96
 1,2,3-Trichlorobenzene
 Concen: 3.329 ug/l
 RT: 15.700 min Scan# 51
 Delta R.T. 0.003 min
 Lab File: VN070829.D
 Acq: 28 Jan 2022 15:19

Instrument :
 MSVOA_N
 ClientSampleId :
 PB142316ZHE#06

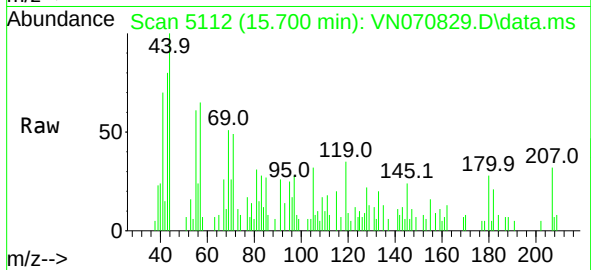

Tgt Ion:180	Resp:	1404
Ion	Ratio	Lower Upper
180	100	
182	65.7	47.4 142.2
145	0.0	15.0 45.1#

