

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012822\
 Data File : VN070835.D
 Acq On : 28 Jan 2022 17:52
 Operator : JC/MD
 Sample : PB142316ZHE#03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB142316ZHE#03

Quant Time: Jan 28 23:18:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 18 13:32:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.086	168	949223	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	1604634	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	1461735	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	588142	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	657497	48.332	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	96.660%		
35) Dibromofluoromethane	8.021	113	454701	45.682	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	91.360%		
50) Toluene-d8	10.441	98	1983407	47.301	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	94.600%		
62) 4-Bromofluorobenzene	12.731	95	688671	46.089	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	92.180%		
Target Compounds						
					Qvalue	
13) Acrolein	4.052	56	798	0.227	ug/l #	21
16) Acetone	4.299	43	99751	10.565	ug/l	98
18) Methyl Acetate	4.870	43	4974	0.268	ug/l #	73
20) Methylene Chloride	5.090	84	5578	0.448	ug/l	90
25) 2-Butanone	7.348	43	20919	1.761	ug/l	92
29) Tetrahydrofuran	7.705	42	1599	0.220	ug/l #	56
30) Chloroform	7.823	83	25	Below Cal	#	18
31) Cyclohexane	8.088	56	20961	0.875	ug/l #	1
36) 1,1-Dichloropropene	8.086	75	77357	4.616	ug/l #	49
37) Ethyl Acetate	7.348	43	20919	0.940	ug/l #	68
38) Carbon Tetrachloride	8.088	117	97659	6.551	ug/l #	16
43) Isopropyl Acetate	8.566	43	148856	4.381	ug/l #	82
45) 1,2-Dichloropropane	9.620	63	7271	0.515	ug/l #	44
48) Methyl methacrylate	9.545	41	27518	1.700	ug/l #	8
49) 1,4-Dioxane	9.617	88	362	1.489	ug/l #	1
51) 4-Methyl-2-Pentanone	10.331	43	17880	0.825	ug/l #	81
53) t-1,3-Dichloropropene	10.714	75	67	2.407	ug/l #	43
54) cis-1,3-Dichloropropene	10.245	75	163074	8.098	ug/l #	60
56) Ethyl methacrylate	10.706	69	560	2.325	ug/l #	24
57) 1,3-Dichloropropane	11.090	76	95393	4.417	ug/l #	43
59) 2-Hexanone	11.090	43	1583868	100.557	ug/l #	49
68) m/p-Xylenes	11.948	106	8936	0.418	ug/l	82
74) N-amyl acetate	12.195	43	64070	2.816	ug/l #	53
76) 1,2,3-Trichloropropane	12.731	75	362089	23.212	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.058	105	21542	0.479	ug/l	96
81) trans-1,4-Dichloro-2-b...	12.731	75	362089	69.153	ug/l #	5
93) 1,2,4-Trichlorobenzene	15.271	180	400	3.459	ug/l	89
95) Naphthalene	15.507	128	3628	5.056	ug/l #	84
96) 1,2,3-Trichlorobenzene	15.695	180	213	3.235	ug/l #	48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012822\
Data File : VN070835.D
Acq On : 28 Jan 2022 17:52
Operator : JC/MD
Sample : PB142316ZHE#03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#03

Quant Time: Jan 28 23:18:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 18 13:32:07 2022
Response via : Initial Calibration




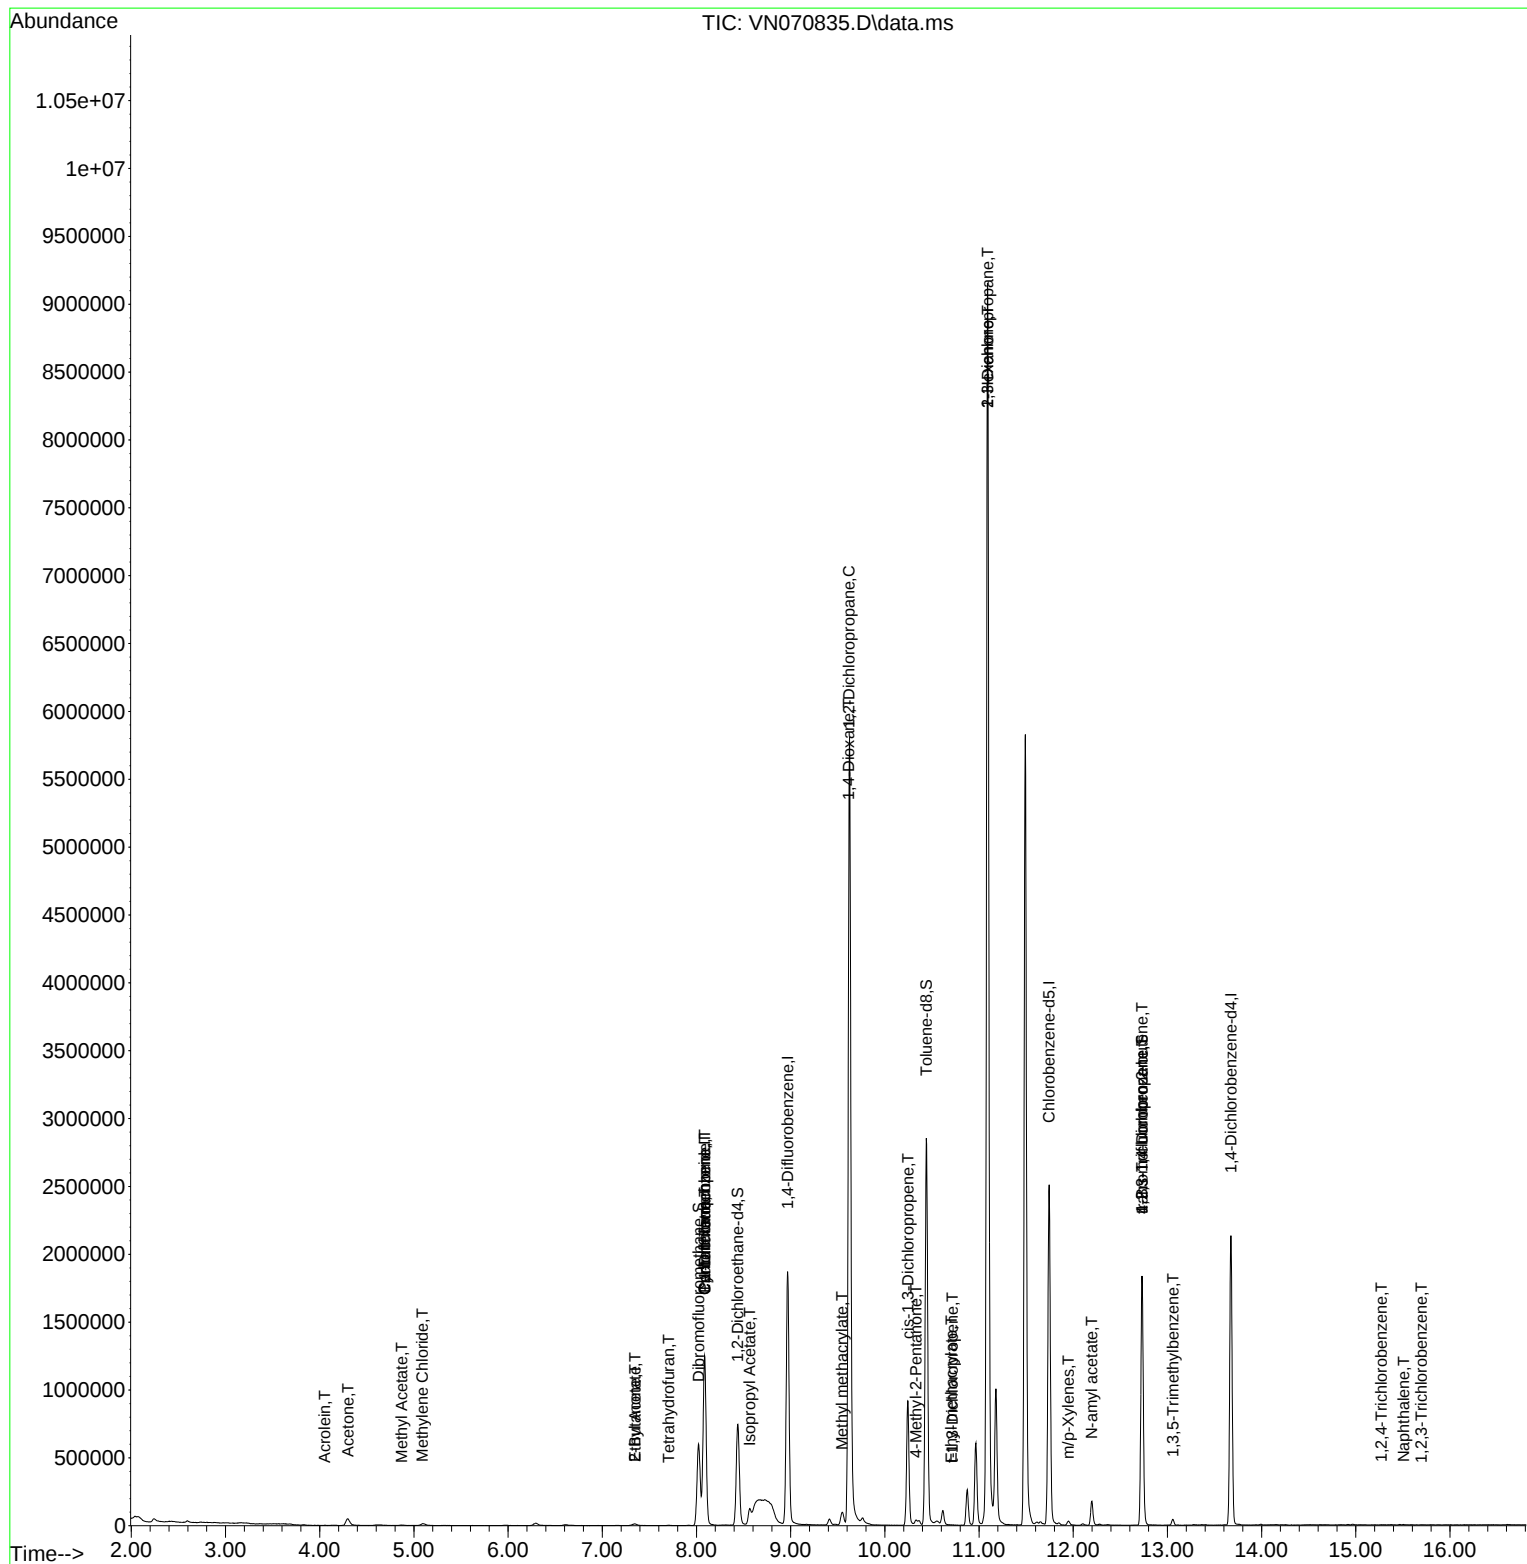




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 21
Delta R.T. 0.003 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#03


Tgt Ion:168 Resp: 949223
Ion Ratio Lower Upper
168 100
99 59.8 41.3 61.9

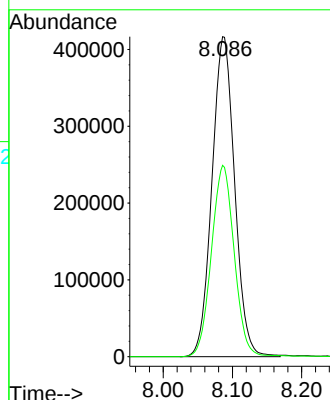

#13
Acrolein
Concen: 0.227 ug/l
RT: 4.052 min Scan# 769
Delta R.T. 0.013 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52

Tgt Ion: 56 Resp: 798
Ion Ratio Lower Upper
56 100
55 5.9 56.6 85.0#


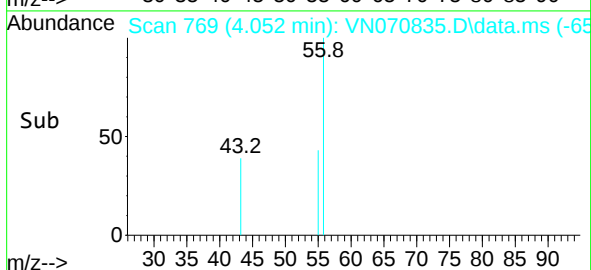
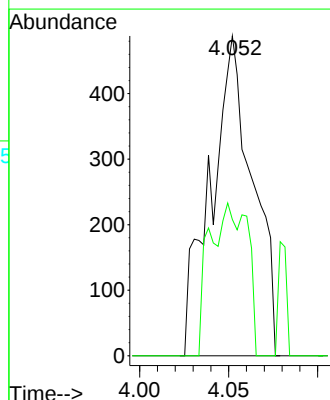





#16
Acetone
Concen: 10.565 ug/l
RT: 4.299 min Scan# 80
Delta R.T. 0.014 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#03


Tgt Ion: 43 Resp: 99751
Ion Ratio Lower Upper
43 100
58 30.0 23.1 34.7

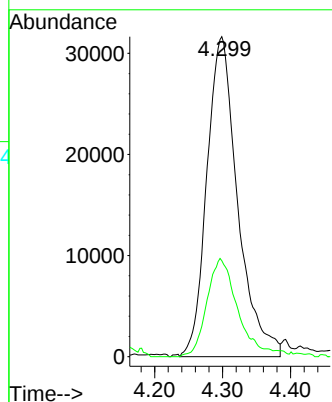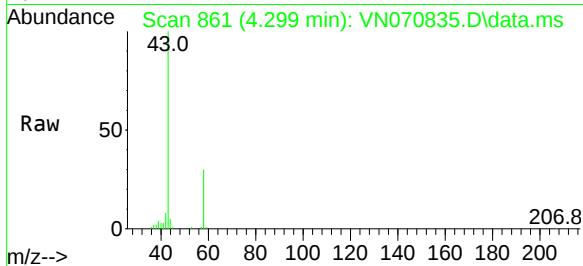

#18
Methyl Acetate
Concen: 0.268 ug/l
RT: 4.870 min Scan# 1074
Delta R.T. 0.016 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52

Tgt Ion: 43 Resp: 4974
Ion Ratio Lower Upper
43 100
74 11.1 19.4 29.2#

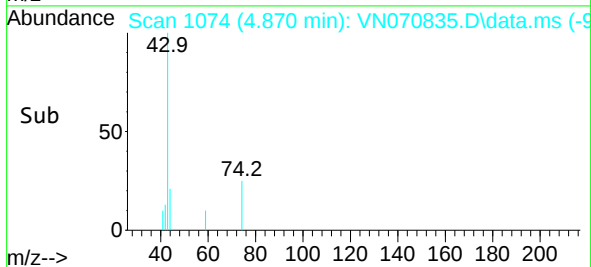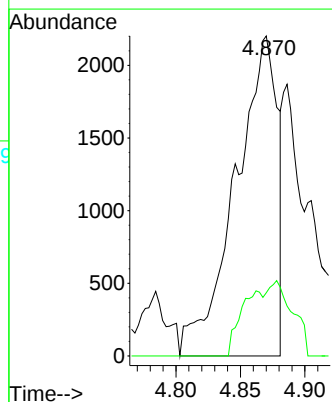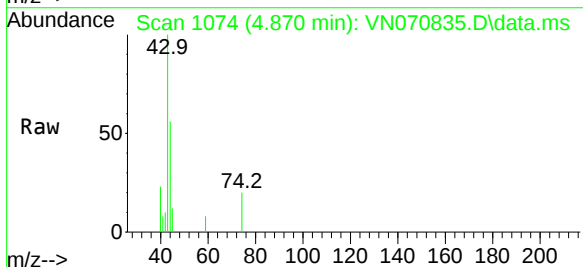

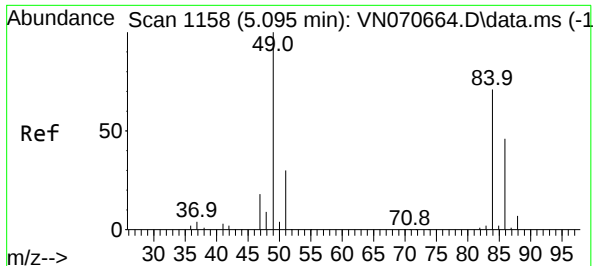

#20

Methylene Chloride

Concen: 0.448 ug/l

RT: 5.090 min Scan# 1158

Delta R.T. -0.005 min

Lab File: VN070835.D


Acq: 28 Jan 2022 17:52

Instrument :

MSVOA_N

ClientSampleId :

PB142316ZHE#03

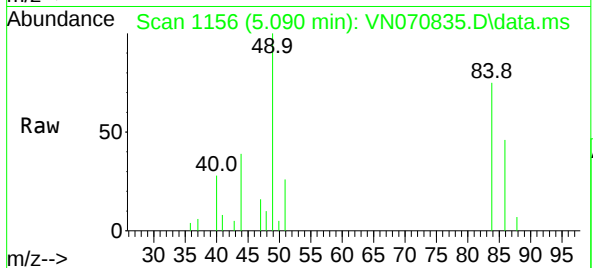

Tgt Ion: 84 Resp: 5578




Ion Ratio Lower Upper

84 100

49 133.4 93.5 140.3

51 34.6 29.4 44.2

86 61.5 53.0 79.4

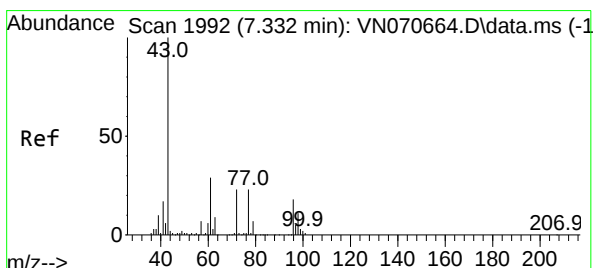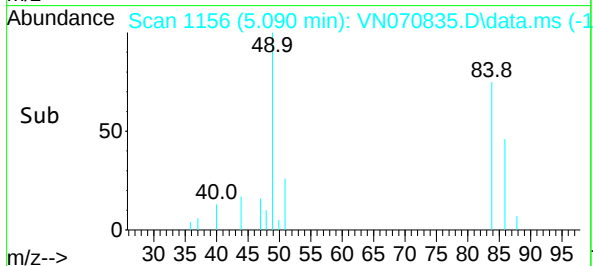

#25

2-Butanone

Concen: 1.761 ug/l

RT: 7.348 min Scan# 1998

Delta R.T. 0.016 min

Lab File: VN070835.D




Acq: 28 Jan 2022 17:52


Tgt Ion: 43 Resp: 20919

Ion Ratio Lower Upper

43 100

72 22.8 21.7 32.5

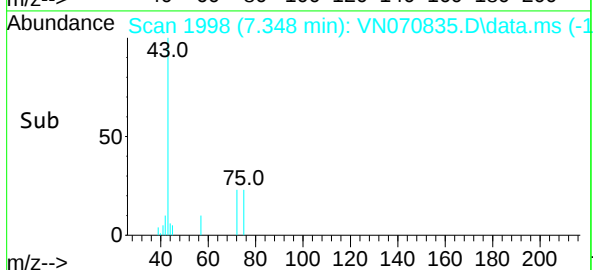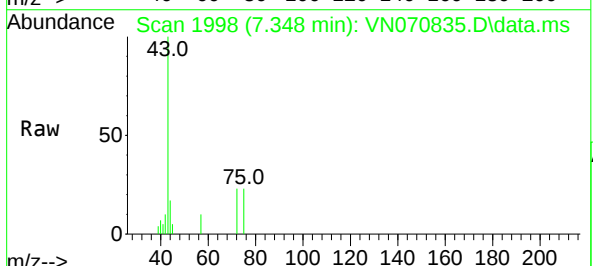



#29

Tetrahydrofuran

Concen: 0.220 ug/l

RT: 7.705 min Scan# 21

Delta R.T. 0.022 min

Lab File: VN070835.D


Acq: 28 Jan 2022 17:52

Instrument :

MSVOA_N

ClientSampleId :

PB142316ZHE#03





Tgt Ion: 42 Resp: 1599

Ion Ratio Lower Upper

42 100

72 10.4 36.3 54.5#

71 21.3 34.7 52.1#

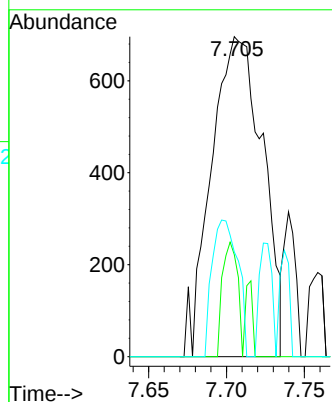

#30

Chloroform

Concen: Below Cal

RT: 7.823 min Scan# 2175

Delta R.T. 0.005 min

Lab File: VN070835.D




Acq: 28 Jan 2022 17:52


Tgt Ion: 83 Resp: 25

Ion Ratio Lower Upper

83 100

85 0.0 51.9 77.9#


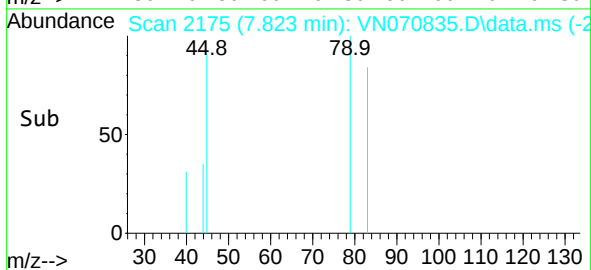
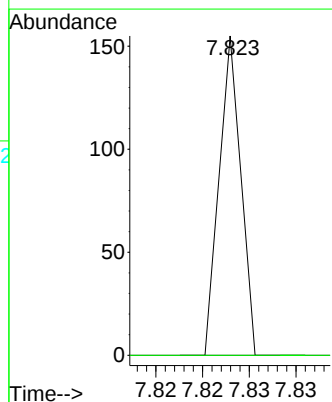
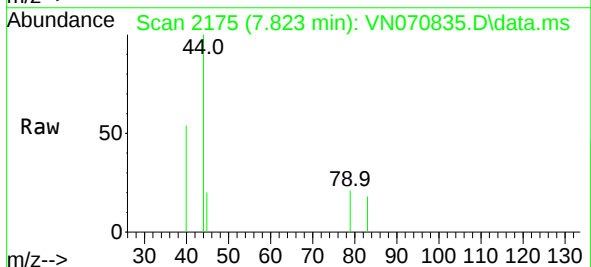




#31
Cyclohexane
Concen: 0.875 ug/l
RT: 8.088 min Scan# 21
Delta R.T. -0.006 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#03


Tgt Ion: 56 Resp: 20961
Ion Ratio Lower Upper
56 100
69 180.9 27.1 40.7#
84 142.1 73.4 110.0#



#33
1,2-Dichloroethane-d4
Concen: 48.332 ug/l
RT: 8.437 min Scan# 2404
Delta R.T. 0.003 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52

Tgt Ion: 65 Resp: 657497
Ion Ratio Lower Upper
65 100
67 52.8 0.0 103.0


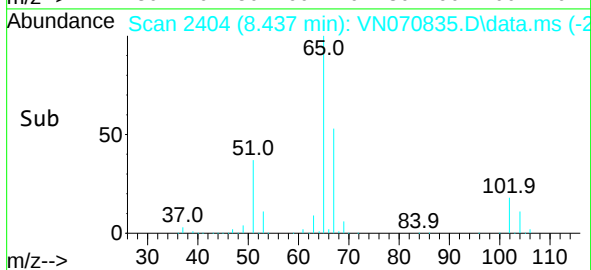






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.968 min Scan# 2601
Delta R.T. 0.003 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#03


Tgt Ion:114 Resp: 1604634
Ion Ratio Lower Upper
114 100
63 23.4 0.0 37.8
88 16.7 0.0 27.4

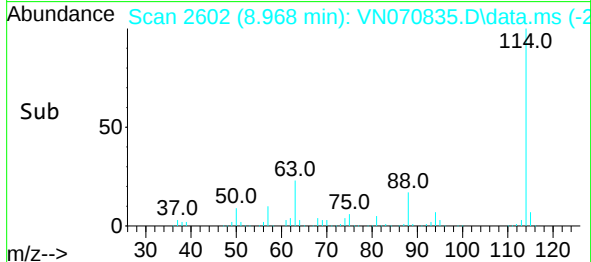

#35
Dibromofluoromethane
Concen: 45.682 ug/l
RT: 8.021 min Scan# 2249
Delta R.T. 0.002 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52

Tgt Ion:113 Resp: 454701
Ion Ratio Lower Upper
113 100
111 102.7 82.2 123.2
192 19.4 16.9 25.3


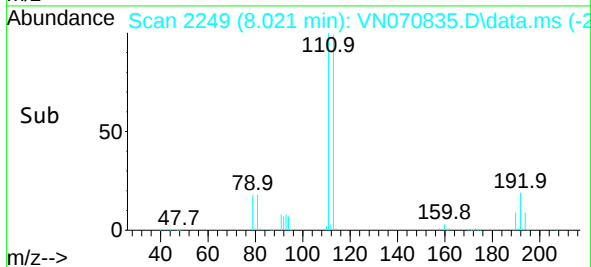

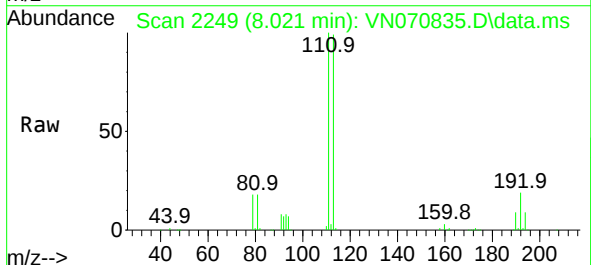




#36
1,1-Dichloropropene
Concen: 4.616 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.134 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#03


Tgt Ion: 75 Resp: 77357
Ion Ratio Lower Upper
75 100
110 9.0 18.4 55.2#
77 0.0 24.4 36.6#



#37
Ethyl Acetate
Concen: 0.940 ug/l
RT: 7.348 min Scan# 1998
Delta R.T. -0.062 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52

Tgt Ion: 43 Resp: 20919
Ion Ratio Lower Upper
43 100
61 0.0 11.5 17.3#
70 0.0 7.9 11.9#


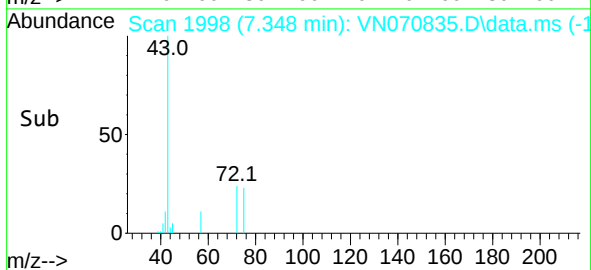






#38
Carbon Tetrachloride
Concen: 6.551 ug/l
RT: 8.088 min Scan# 211
Delta R.T. -0.118 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#03


Tgt Ion:117 Resp: 97659
Ion Ratio Lower Upper
117 100
119 5.2 76.1 114.1#
121 0.0 24.2 36.2#

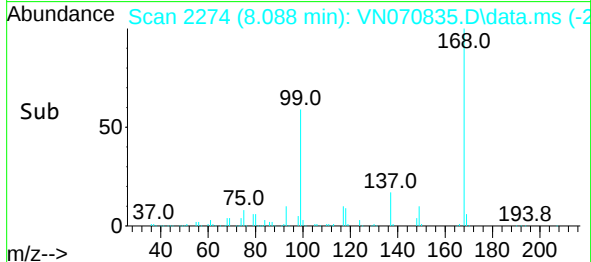

#43
Isopropyl Acetate
Concen: 4.381 ug/l
RT: 8.566 min Scan# 2452
Delta R.T. 0.006 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52

Tgt Ion: 43 Resp: 148856
Ion Ratio Lower Upper
43 100
61 15.2 20.4 30.6#
87 8.0 11.2 16.8#

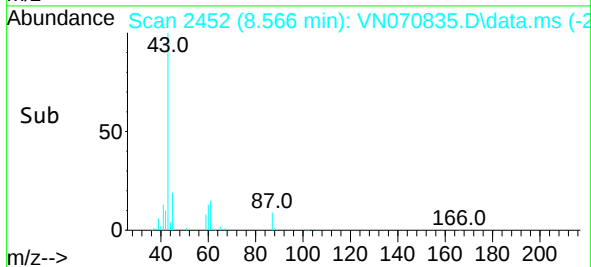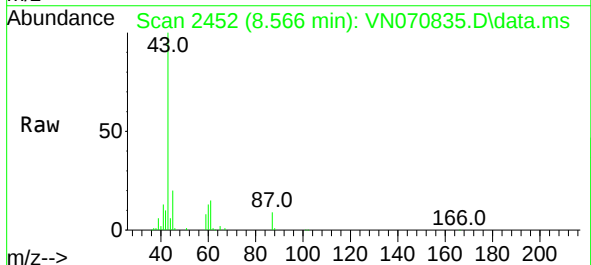



#45

1,2-Dichloropropane

Concen: 0.515 ug/l

RT: 9.620 min Scan# 21

Delta R.T. 0.132 min

Lab File: VN070835.D

Acq: 28 Jan 2022 17:52

Instrument :

MSVOA_N

ClientSampleId :





PB142316ZHE#03

Tgt Ion: 63 Resp: 7271

Ion Ratio Lower Upper

63 100

65 0.0 24.7 37.1#

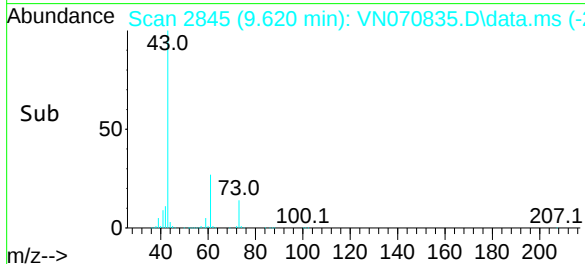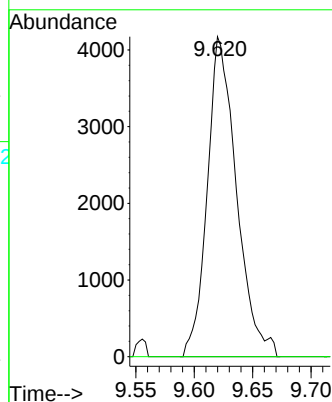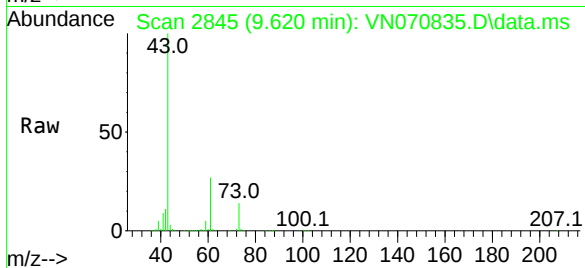

#48

Methyl methacrylate

Concen: 1.700 ug/l

RT: 9.545 min Scan# 2817

Delta R.T. -0.013 min

Lab File: VN070835.D

Acq: 28 Jan 2022 17:52




Tgt Ion: 41 Resp: 27518


Ion Ratio Lower Upper

41 100

69 0.0 72.4 108.6#

39 0.0 58.4 87.6#

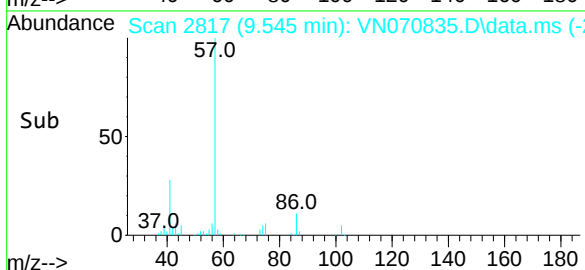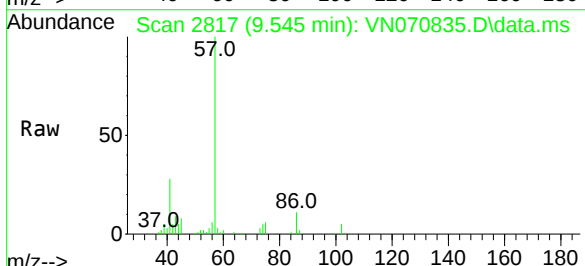



#49

1,4-Dioxane

Concen: 1.489 ug/l

RT: 9.617 min Scan# 21

Delta R.T. 0.048 min

Lab File: VN070835.D


Acq: 28 Jan 2022 17:52

Instrument :

MSVOA_N

ClientSampleId :

PB142316ZHE#03

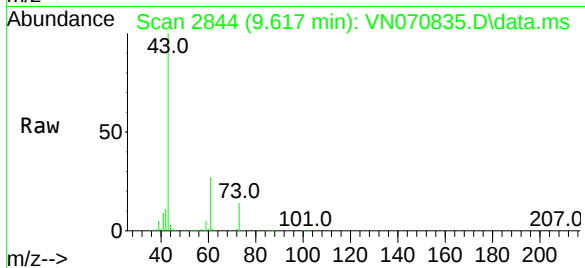




Tgt Ion: 88 Resp: 362

Ion Ratio Lower Upper

88 100

43 1722526.2 23.4 35.2#

58 6302.2 50.6 75.8#

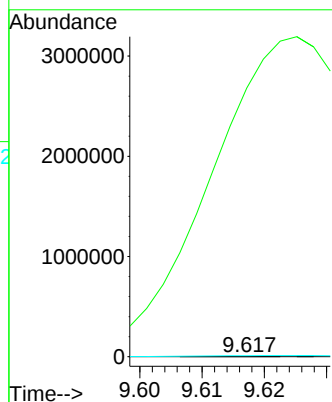

#50

Toluene-d8

Concen: 47.301 ug/l

RT: 10.441 min Scan# 3151

Delta R.T. 0.003 min

Lab File: VN070835.D




Acq: 28 Jan 2022 17:52


Tgt Ion: 98 Resp: 1983407

Ion Ratio Lower Upper

98 100

100 64.2 50.4 75.6


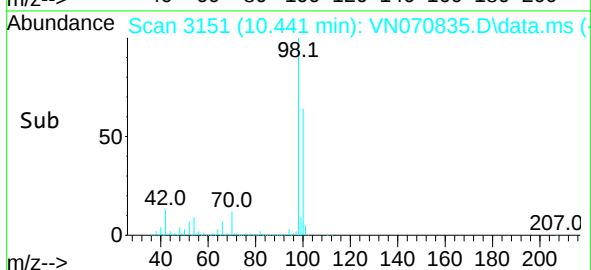

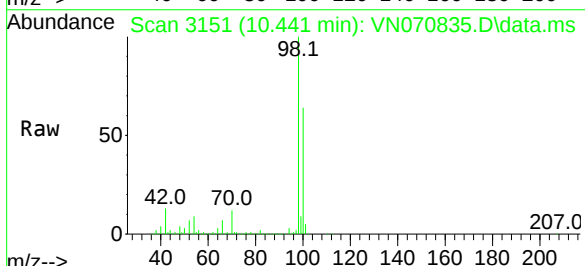


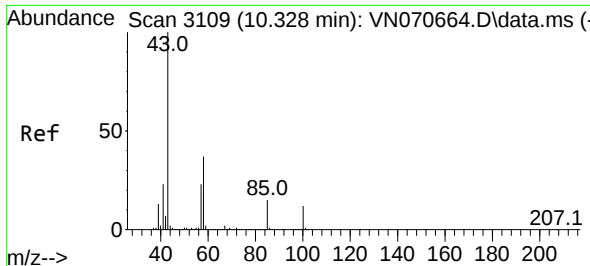

#51
4-Methyl-2-Pentanone
Concen: 0.825 ug/l
RT: 10.331 min Scan# 3109
Delta R.T. 0.003 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#03


Tgt Ion: 43 Resp: 17880
Ion Ratio Lower Upper
43 100
58 49.4 30.4 45.6#

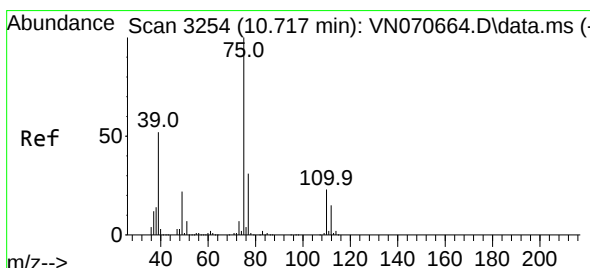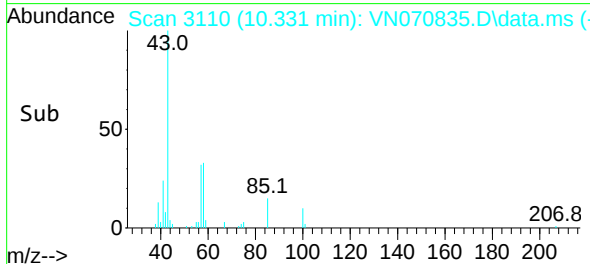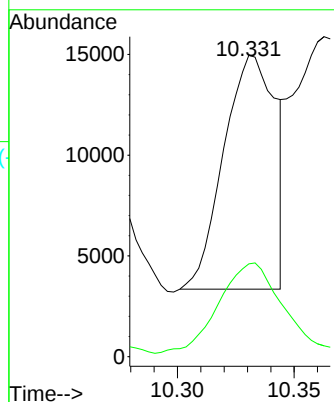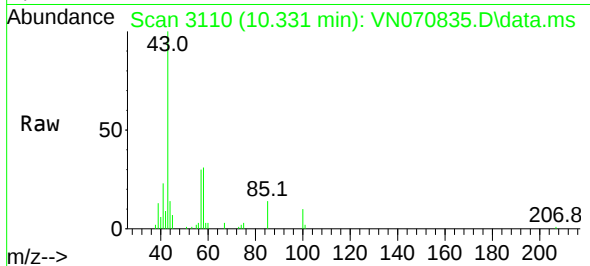

#53
t-1,3-Dichloropropene
Concen: 2.407 ug/l
RT: 10.714 min Scan# 3253
Delta R.T. -0.003 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52

Tgt Ion: 75 Resp: 67
Ion Ratio Lower Upper
75 100
77 0.0 25.6 38.4#


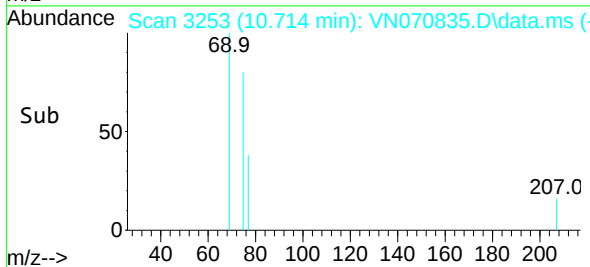
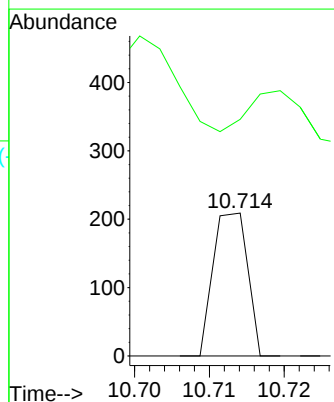
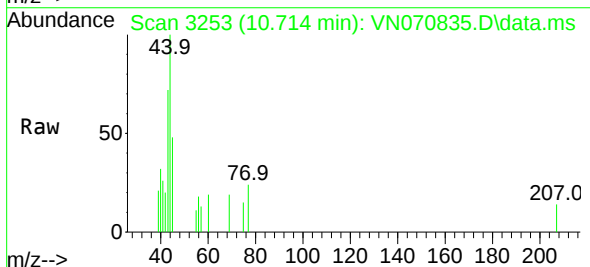


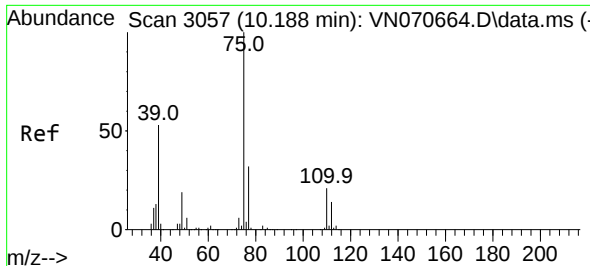

#54
cis-1,3-Dichloropropene
Concen: 8.098 ug/l
RT: 10.245 min Scan# 3057
Delta R.T. 0.057 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#03


Tgt Ion: 75 Resp: 163074
Ion Ratio Lower Upper
75 100
77 0.4 26.4 39.6#
39 32.0 42.5 63.7#

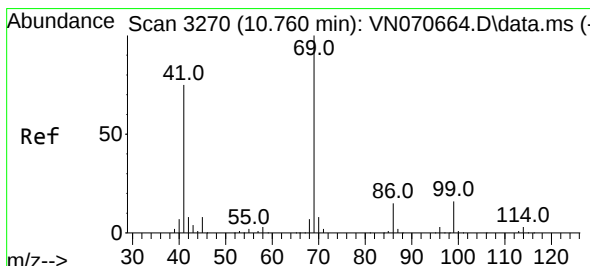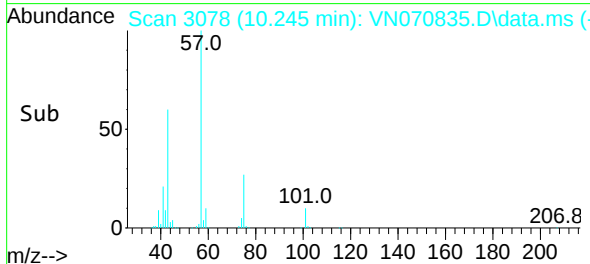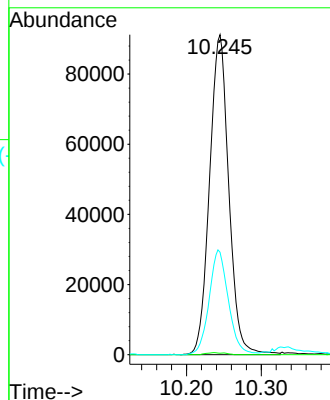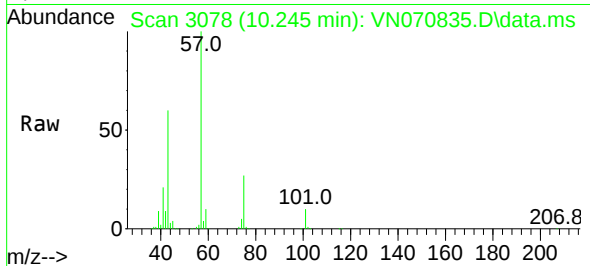

#56
Ethyl methacrylate
Concen: 2.325 ug/l
RT: 10.706 min Scan# 3250
Delta R.T. -0.054 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52

Tgt Ion: 69 Resp: 560
Ion Ratio Lower Upper
69 100
41 0.0 51.4 77.0#
39 0.0 34.6 52.0#

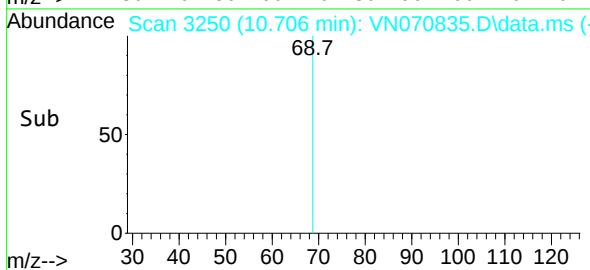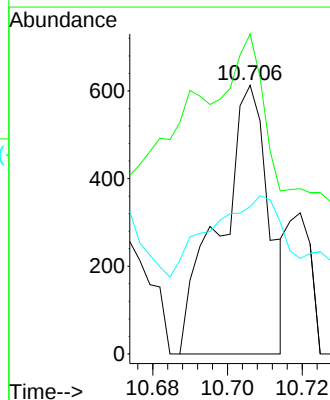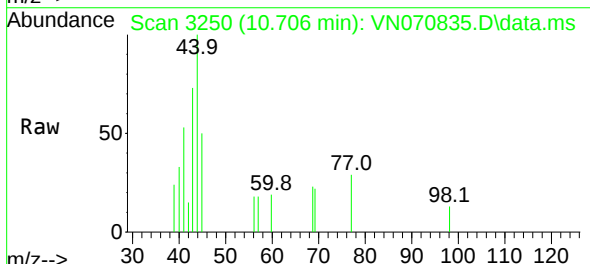

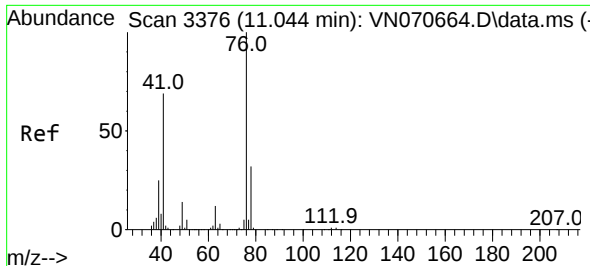

#57

1,3-Dichloropropane

Concen: 4.417 ug/l

RT: 11.090 min Scan# 31

Delta R.T. 0.046 min

Lab File: VN070835.D

Acq: 28 Jan 2022 17:52

Instrument :

MSVOA_N

ClientSampleId :





PB142316ZHE#03

Tgt Ion: 76 Resp: 95393

Ion Ratio Lower Upper

76 100

78 0.3 25.7 38.5#

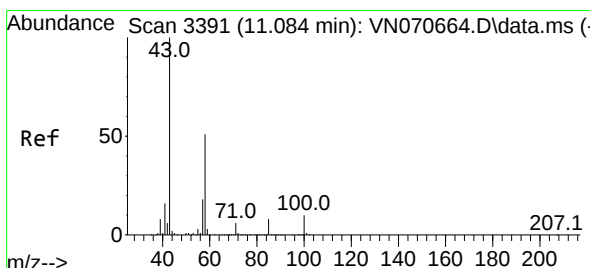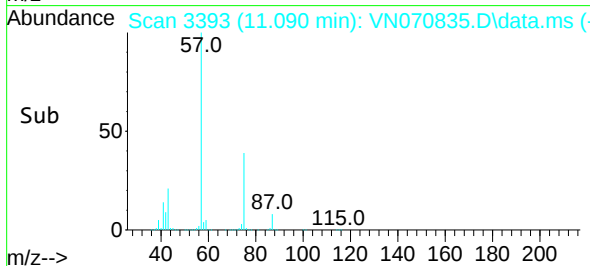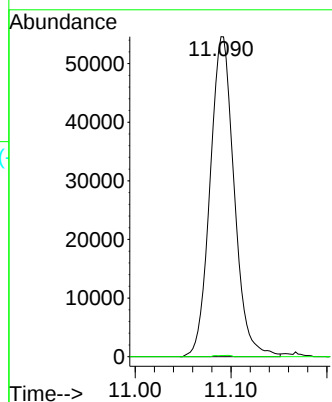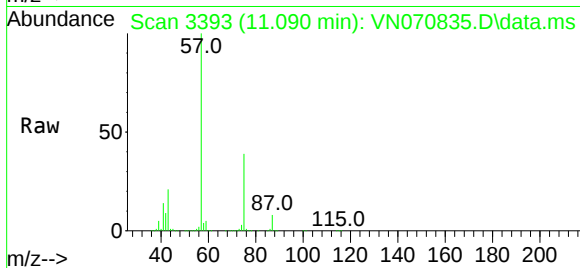

#59

2-Hexanone

Concen: 100.557 ug/l

RT: 11.090 min Scan# 3393

Delta R.T. 0.006 min

Lab File: VN070835.D




Acq: 28 Jan 2022 17:52


Tgt Ion: 43 Resp: 1583868

Ion Ratio Lower Upper

43 100

58 17.1 26.9 80.7#


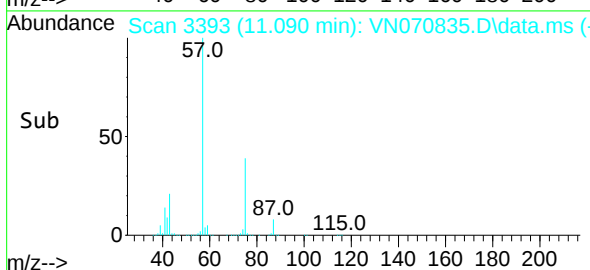

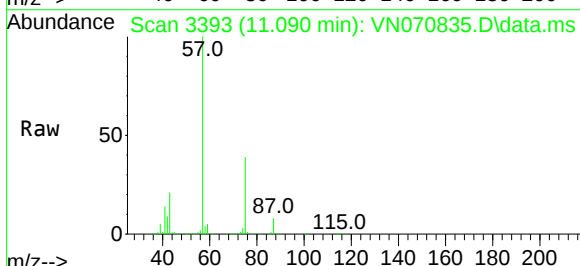




#62
4-Bromofluorobenzene
Concen: 46.089 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.003 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#03


Tgt Ion: 95 Resp: 688671
Ion Ratio Lower Upper
95 100
174 74.2 0.0 187.2
176 71.6 0.0 181.4



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3637
Delta R.T. 0.003 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52

Tgt Ion: 117 Resp: 1461735
Ion Ratio Lower Upper
117 100
82 61.4 42.4 63.6
119 32.5 25.4 38.2


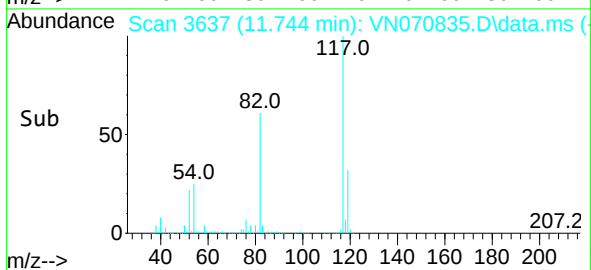

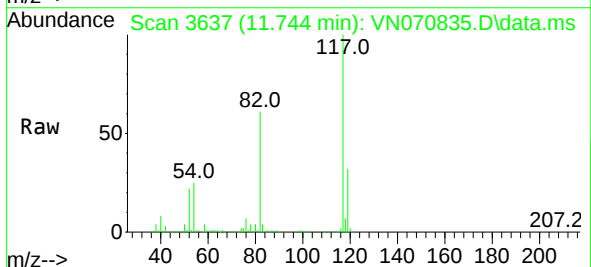


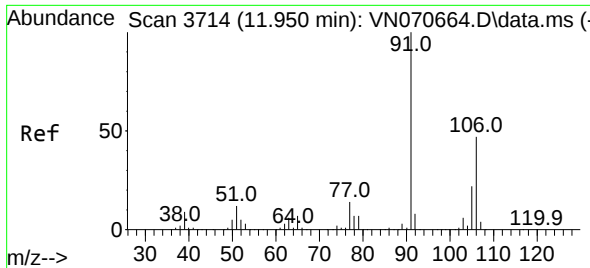

#68
m/p-Xylenes
Concen: 0.418 ug/l
RT: 11.948 min Scan# 31
Delta R.T. -0.002 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#03


Tgt Ion:106 Resp: 8936
Ion Ratio Lower Upper
106 100
91 228.2 160.6 240.8

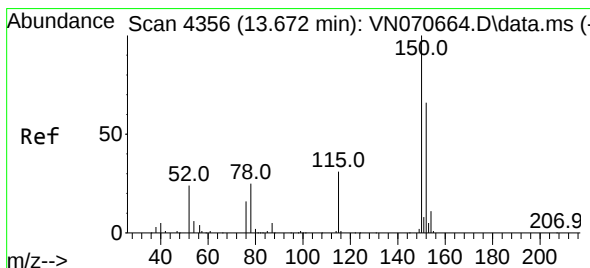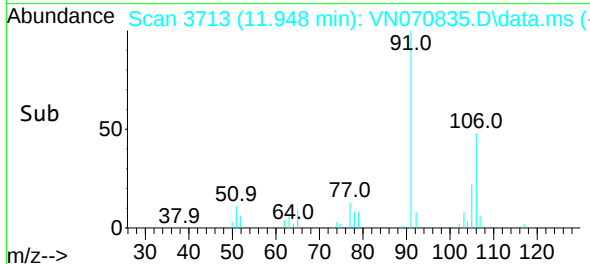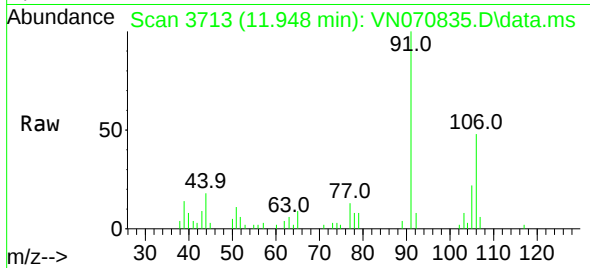

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 4357
Delta R.T. 0.003 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52

Tgt Ion:152 Resp: 588142
Ion Ratio Lower Upper
152 100
115 62.5 27.5 82.5
150 158.5 0.0 344.4


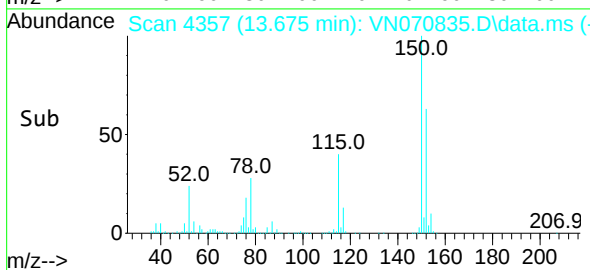

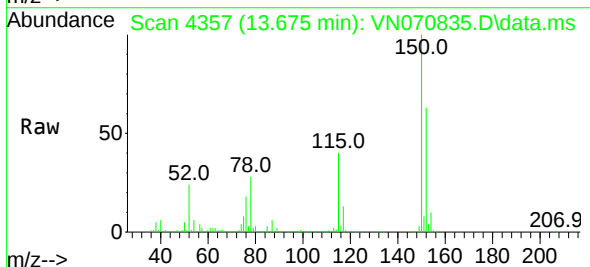




#74
N-ethyl acetate
Concen: 2.816 ug/l
RT: 12.195 min Scan# 3876
Delta R.T. -0.190 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#03


Tgt Ion: 43	Resp: 64070
Ion Ratio	Lower Upper
43 100	
70 1.9	33.4 50.0#
55 5.1	19.3 28.9#
61 10.5	18.5 27.7#

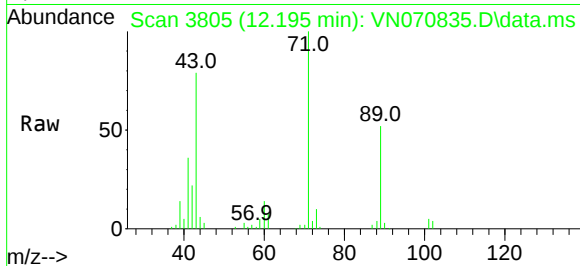

#76
1,2,3-Trichloropropane
Concen: 23.212 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.147 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52

Tgt Ion: 75	Resp: 362089
Ion Ratio	Lower Upper
75 100	
77 1.1	82.6 247.8#


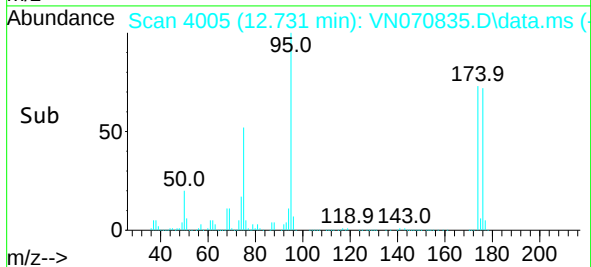

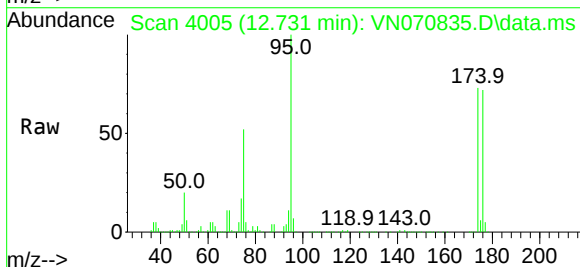


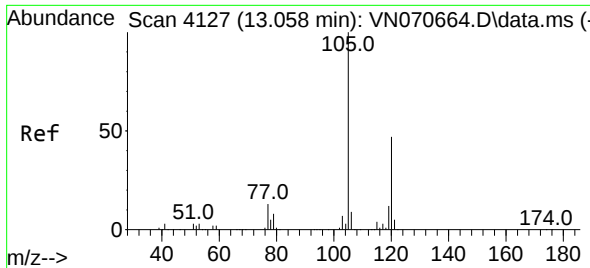

#80
 1,3,5-Trimethylbenzene
 Concen: 0.479 ug/l
 RT: 13.058 min Scan# 4127
 Delta R.T. 0.000 min
 Lab File: VN070835.D
 Acq: 28 Jan 2022 17:52




Instrument :
 MSVOA_N
 ClientSampleId :
 PB142316ZHE#03


Tgt Ion:105 Resp: 21542
 Ion Ratio Lower Upper
 105 100
 120 46.4 24.6 73.6

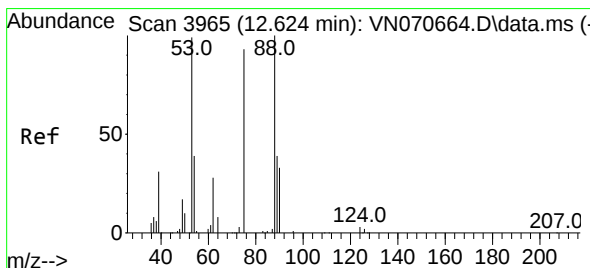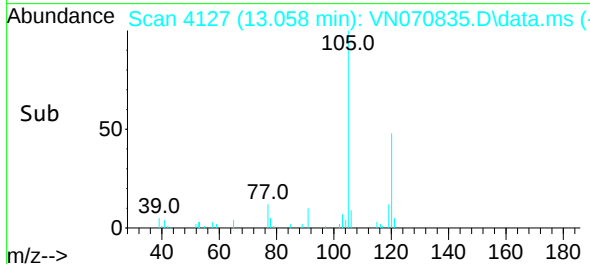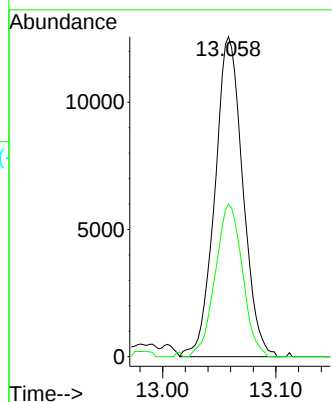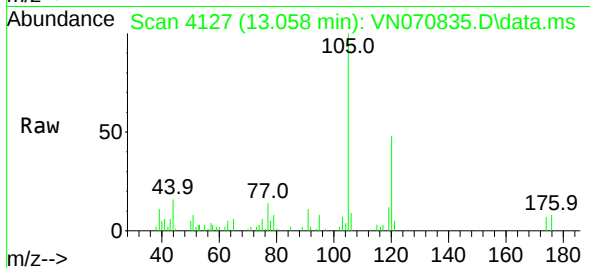

#81
 trans-1,4-Dichloro-2-butene
 Concen: 69.153 ug/l
 RT: 12.731 min Scan# 4005
 Delta R.T. 0.107 min
 Lab File: VN070835.D
 Acq: 28 Jan 2022 17:52

Tgt Ion: 75 Resp: 362089
 Ion Ratio Lower Upper
 75 100
 53 0.0 90.5 135.7#
 89 0.0 38.2 57.4#


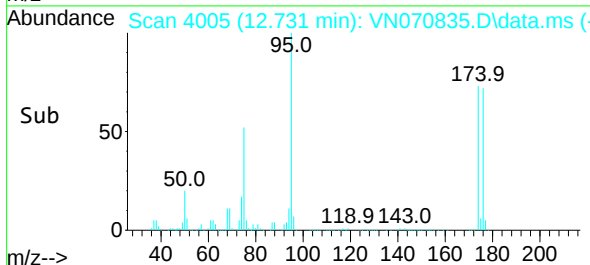

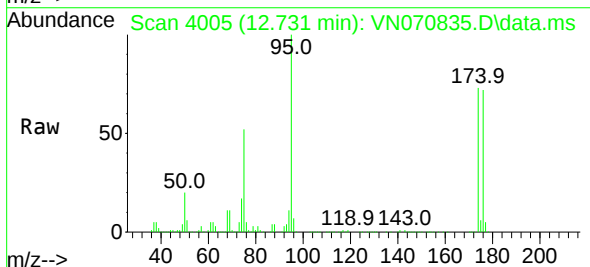




#93
1,2,4-Trichlorobenzene
Concen: 3.459 ug/l
RT: 15.271 min Scan# 4949
Delta R.T. 0.008 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52




Instrument :
MSVOA_N
ClientSampleId :
PB142316ZHE#03


Tgt Ion:180 Resp: 400
Ion Ratio Lower Upper
180 100
182 85.3 48.3 144.9
145 25.3 14.5 43.5

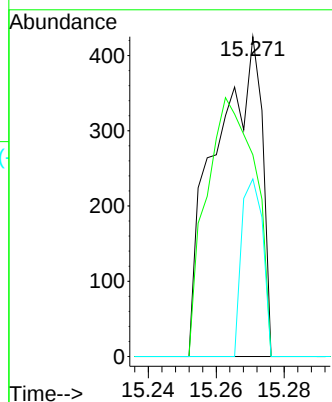

#95
Naphthalene
Concen: 5.056 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. 0.003 min
Lab File: VN070835.D
Acq: 28 Jan 2022 17:52


Tgt Ion:128 Resp: 3628
Ion Ratio Lower Upper
128 100
127 7.9 10.5 15.7#
129 3.5 8.7 13.1#

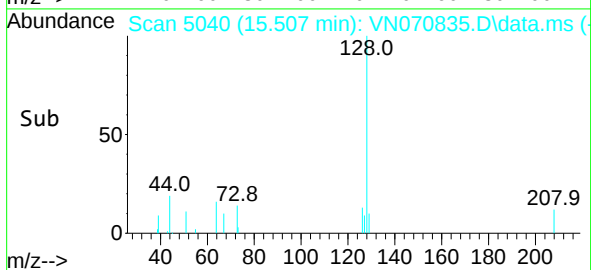



#96
 1,2,3-Trichlorobenzene
 Concen: 3.235 ug/l
 RT: 15.695 min Scan# 51
 Delta R.T. -0.002 min
 Lab File: VN070835.D
 Acq: 28 Jan 2022 17:52

Instrument :
 MSVOA_N
 ClientSampleId :
 PB142316ZHE#03

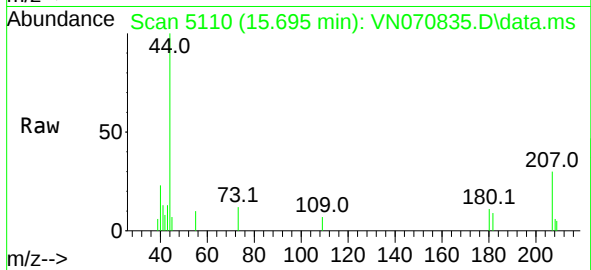

Tgt Ion:180 Resp: 213
 Ion Ratio Lower Upper
 180 100
 182 144.1 47.4 142.2#
 145 0.0 15.0 45.1#

