

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012822\
 Data File : VN070836.D
 Acq On : 28 Jan 2022 18:18
 Operator : JC/MD
 Sample : N1303-04
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 CC-6

Quant Time: Jan 28 23:18:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 18 13:32:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	961110	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	1607077	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	1485194	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	625497	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	659893	47.908	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	95.820%		
35) Dibromofluoromethane	8.024	113	450562	45.198	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	90.400%		
50) Toluene-d8	10.440	98	1972166	46.961	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	93.920%		
62) 4-Bromofluorobenzene	12.731	95	700481	46.808	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	93.620%		
Target Compounds					Qvalue	
16) Acetone	4.299	43	173307	18.128	ug/l	98
20) Methylene Chloride	5.098	84	10151	0.806	ug/l	95
25) 2-Butanone	7.351	43	22421	1.864	ug/l #	88
29) Tetrahydrofuran	7.707	42	1661	0.225	ug/l #	55
30) Chloroform	8.080	83	150	Below Cal	#	18
31) Cyclohexane	8.088	56	20523	0.846	ug/l #	1
36) 1,1-Dichloropropene	8.086	75	78245	4.662	ug/l #	49
37) Ethyl Acetate	7.351	43	22421	1.006	ug/l #	68
38) Carbon Tetrachloride	8.088	117	95715	6.411	ug/l #	17
43) Isopropyl Acetate	8.652	43	159769	4.695	ug/l #	56
48) Methyl methacrylate	9.550	41	25635	1.581	ug/l #	21
51) 4-Methyl-2-Pentanone	10.333	43	31618	1.456	ug/l	92
53) t-1,3-Dichloropropene	10.719	75	110	2.409	ug/l #	43
54) cis-1,3-Dichloropropene	10.245	75	12925	0.641	ug/l #	62
56) Ethyl methacrylate	10.692	69	203	2.310	ug/l #	1
59) 2-Hexanone	11.057	43	51243	3.248	ug/l #	25
67) Ethyl Benzene	11.843	91	92668	1.553	ug/l	95
68) m/p-Xylenes	11.948	106	151541	6.982	ug/l	91
69) o-Xylene	12.280	106	66721	3.098	ug/l	92
73) Isopropylbenzene	12.581	105	14045	0.237	ug/l	96
76) 1,2,3-Trichloropropane	12.731	75	369019	22.244	ug/l #	1
78) n-propylbenzene	12.921	91	25355	0.383	ug/l	95
79) 2-Chlorotoluene	12.983	91	11317	0.270	ug/l #	38
80) 1,3,5-Trimethylbenzene	13.058	105	90158	1.884	ug/l	97
81) trans-1,4-Dichloro-2-b...	12.731	75	369019	66.268	ug/l #	5
82) 4-Chlorotoluene	13.058	91	9127	0.233	ug/l #	38
84) 1,2,4-Trimethylbenzene	13.366	105	295907	6.433	ug/l	97
85) sec-Butylbenzene	13.366	105	295907	5.225	ug/l #	56
86) p-Isopropyltoluene	13.616	119	12471	0.280	ug/l	91
90) Hexachloroethane	14.219	117	3927	0.505	ug/l #	6
93) 1,2,4-Trichlorobenzene	15.255	180	479	3.464	ug/l #	1
95) Naphthalene	15.507	128	107362	7.931	ug/l	100
96) 1,2,3-Trichlorobenzene	15.686	180	87	3.223	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_N
ClientSampleId :
CC-6

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012822\
Data File : VN070836.D
Acq On : 28 Jan 2022 18:18
Operator : JC/MD
Sample : N1303-04
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
CC-6

Quant Time: Jan 28 23:18:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 18 13:32:07 2022
Response via : Initial Calibration




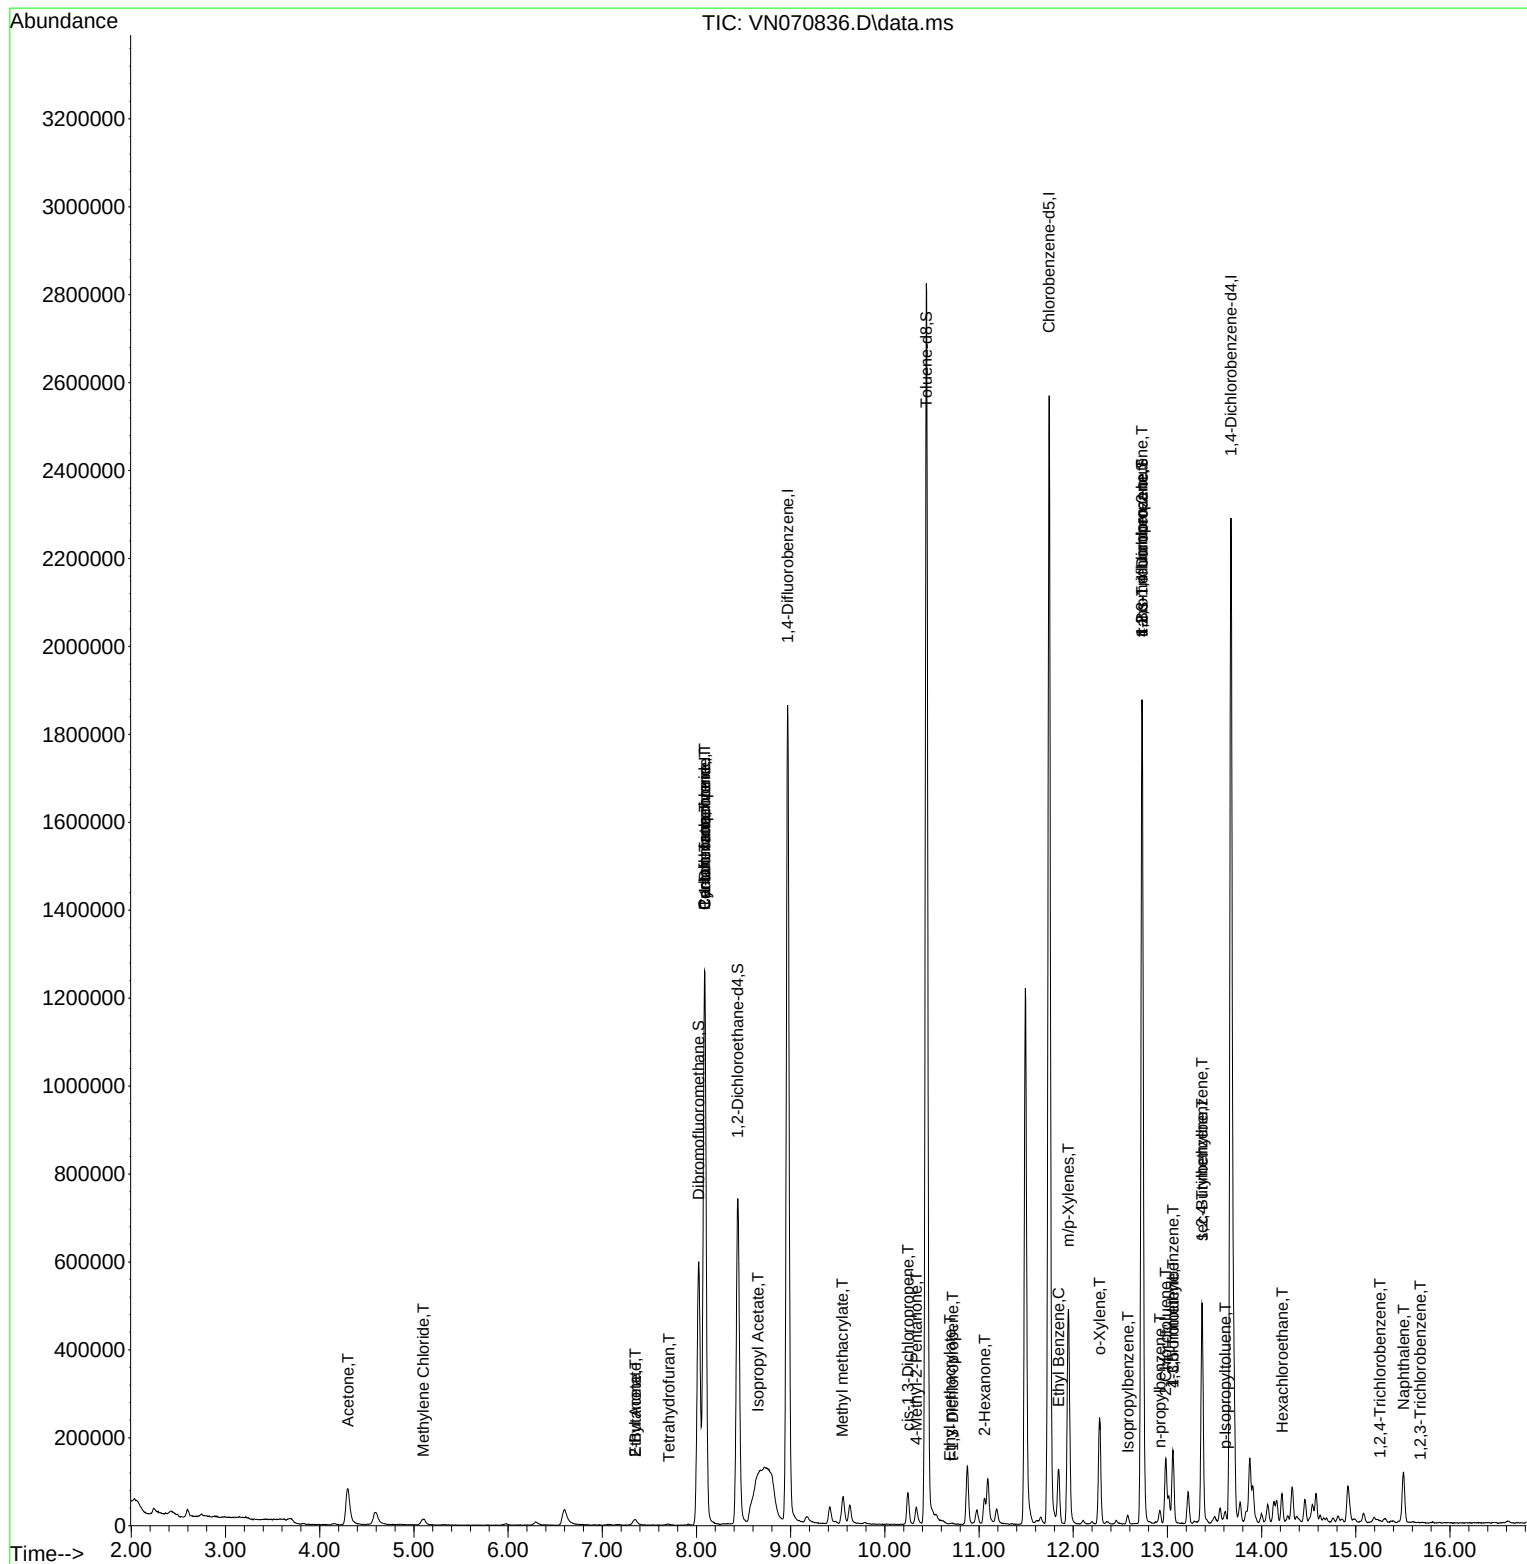




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 21
Delta R.T. 0.005 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18




Instrument :
MSVOA_N
ClientSampleId :
CC-6


Tgt Ion:168 Resp: 961110
Ion Ratio Lower Upper
168 100
99 60.1 41.3 61.9

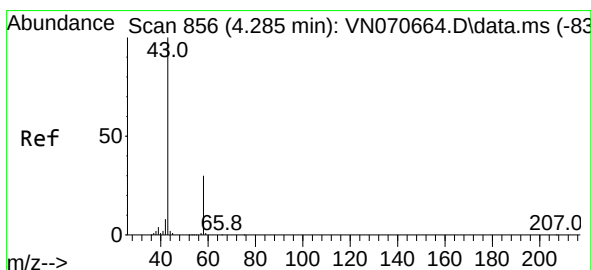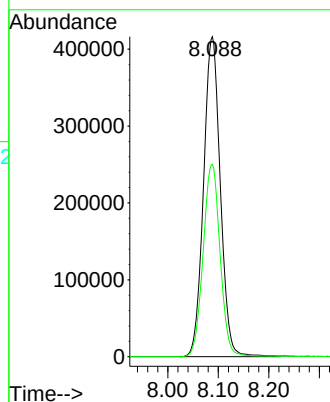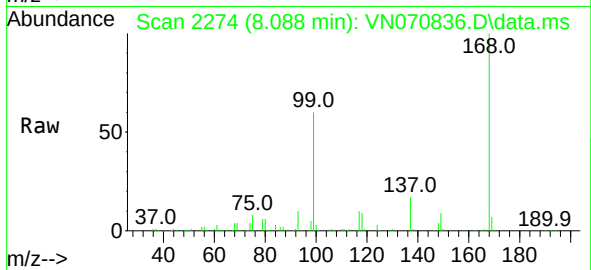

#16
Acetone
Concen: 18.128 ug/l
RT: 4.299 min Scan# 861
Delta R.T. 0.014 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18

Tgt Ion: 43 Resp: 173307
Ion Ratio Lower Upper
43 100
58 30.2 23.1 34.7


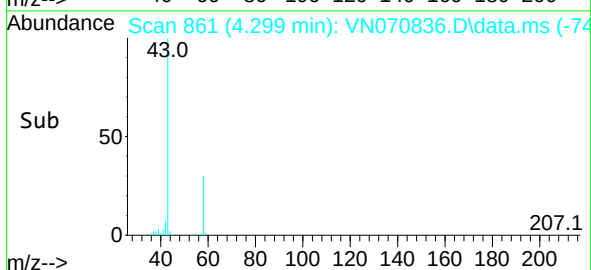
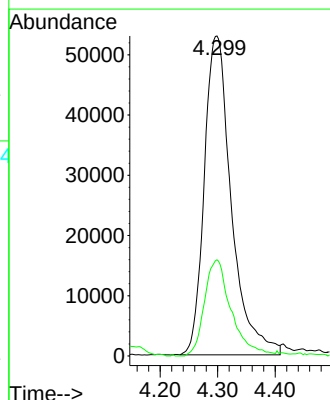
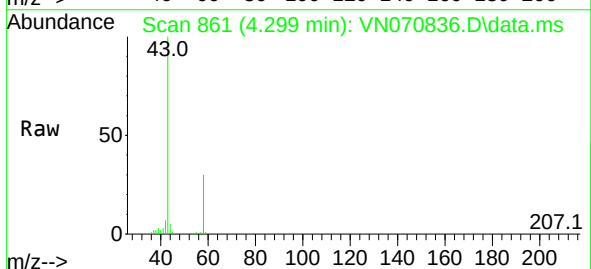


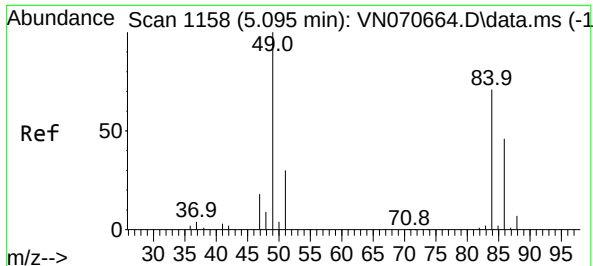

#20
Methylene Chloride
Concen: 0.806 ug/l
RT: 5.098 min Scan# 1158
Delta R.T. 0.003 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18




Instrument :
MSVOA_N
ClientSampleId :
CC-6


Tgt Ion:	84	Resp:	10151
Ion	Ratio	Lower	Upper
84	100		
49	119.0	93.5	140.3
51	34.7	29.4	44.2
86	57.4	53.0	79.4

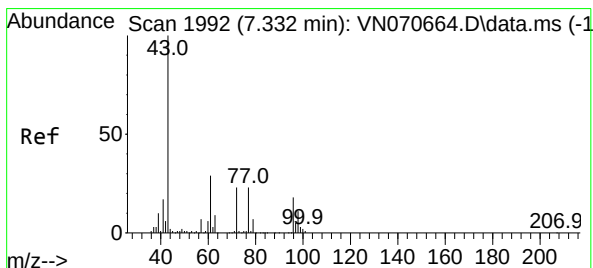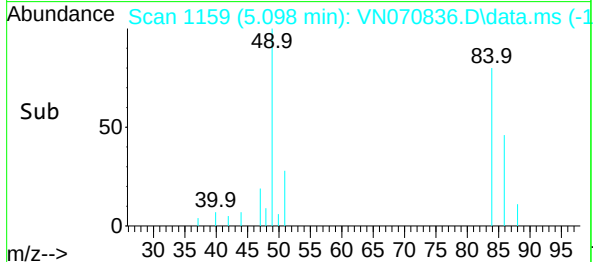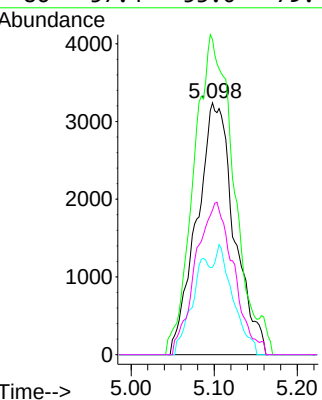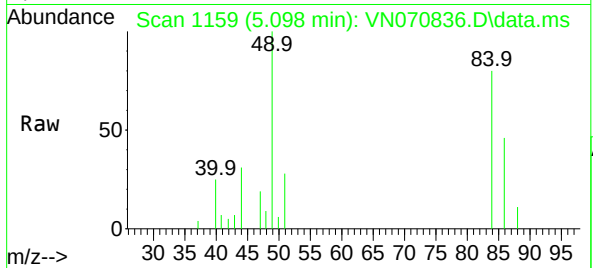

#25
2-Butanone
Concen: 1.864 ug/l
RT: 7.351 min Scan# 1999
Delta R.T. 0.019 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18

Tgt Ion:	43	Resp:	22421
Ion	Ratio	Lower	Upper
43	100		
72	20.8	21.7	32.5#

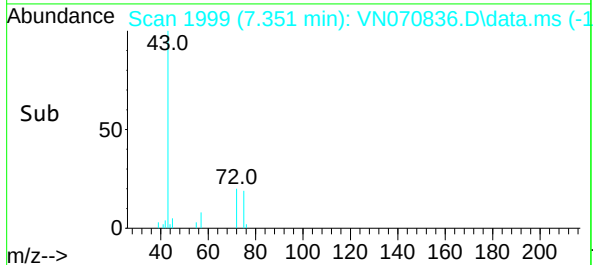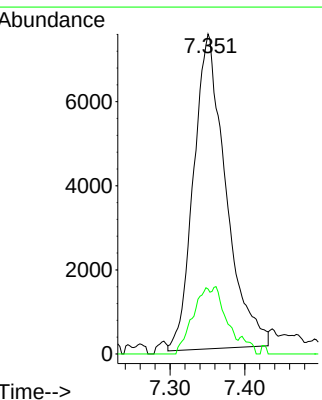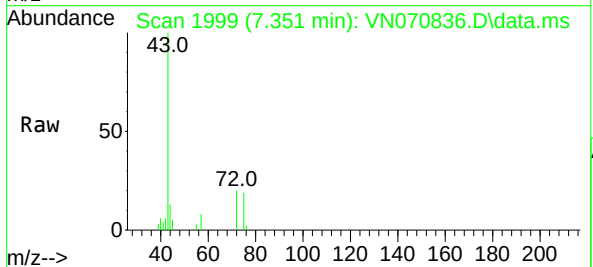

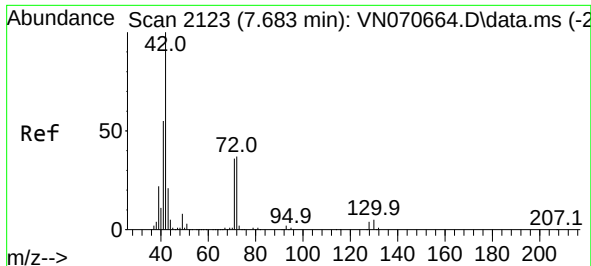

#29

Tetrahydrofuran

Concen: 0.225 ug/l

RT: 7.707 min Scan# 21

Delta R.T. 0.024 min

Lab File: VN070836.D

Acq: 28 Jan 2022 18:18

Instrument :

MSVOA_N

ClientSampleId :

CC-6





Tgt Ion: 42 Resp: 1661

Ion Ratio Lower Upper

42 100

72 17.0 36.3 54.5#

71 13.6 34.7 52.1#

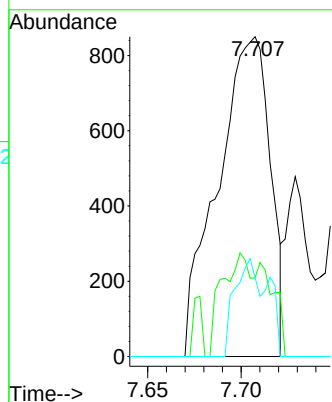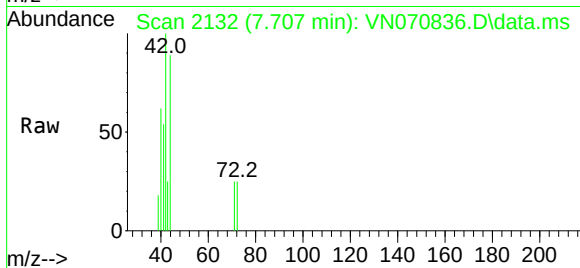

#30

Chloroform

Concen: Below Cal

RT: 8.080 min Scan# 2271

Delta R.T. 0.262 min

Lab File: VN070836.D




Acq: 28 Jan 2022 18:18


Tgt Ion: 83 Resp: 150

Ion Ratio Lower Upper

83 100

85 0.0 51.9 77.9#


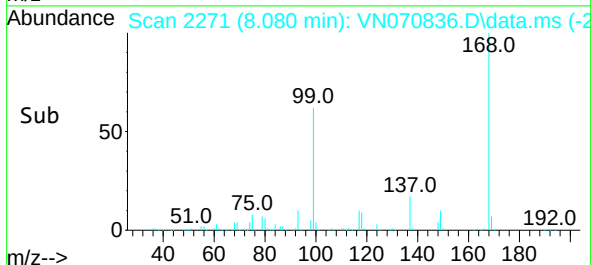

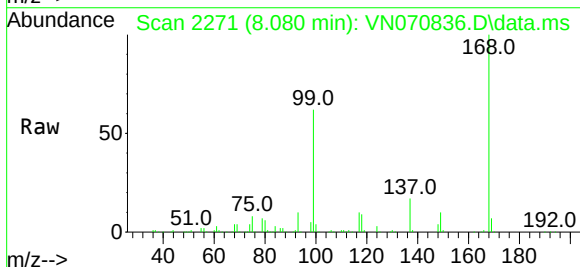




#31
Cyclohexane
Concen: 0.846 ug/l
RT: 8.088 min Scan# 21
Delta R.T. -0.006 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18




Instrument :
MSVOA_N
ClientSampleId :
CC-6


Tgt Ion: 56 Resp: 20523
Ion Ratio Lower Upper
56 100
69 179.3 27.1 40.7#
84 150.7 73.4 110.0#

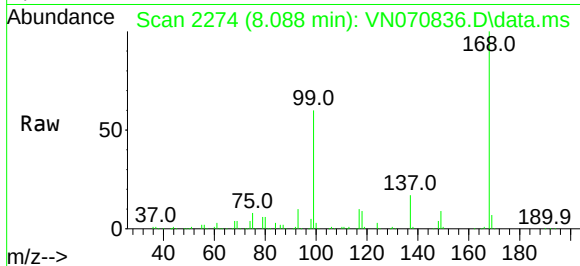

#33
1,2-Dichloroethane-d4
Concen: 47.908 ug/l
RT: 8.437 min Scan# 2404
Delta R.T. 0.003 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18

Tgt Ion: 65 Resp: 659893
Ion Ratio Lower Upper
65 100
67 52.3 0.0 103.0


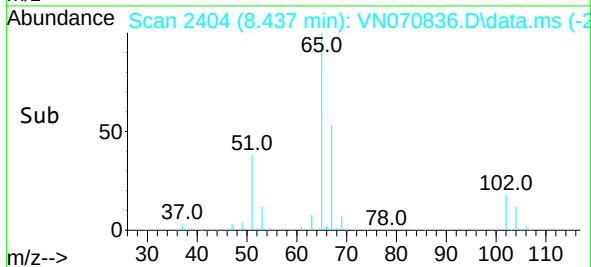

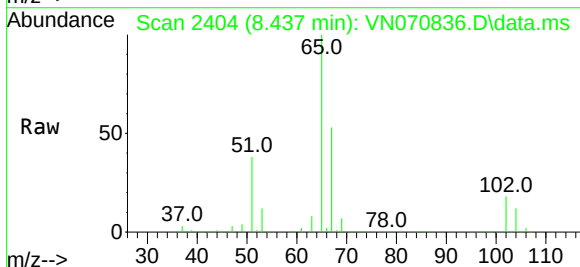


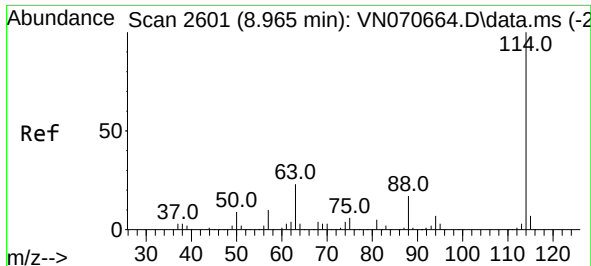

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.968 min Scan# 21
Delta R.T. 0.003 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18




Instrument :
MSVOA_N
ClientSampleId :
CC-6


Tgt Ion:114 Resp: 1607077
Ion Ratio Lower Upper
114 100
63 23.3 0.0 37.8
88 16.8 0.0 27.4

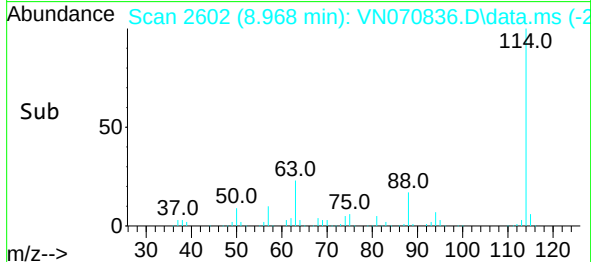

#35
Dibromofluoromethane
Concen: 45.198 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.005 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18

Tgt Ion:113 Resp: 450562
Ion Ratio Lower Upper
113 100
111 103.5 82.2 123.2
192 19.4 16.9 25.3


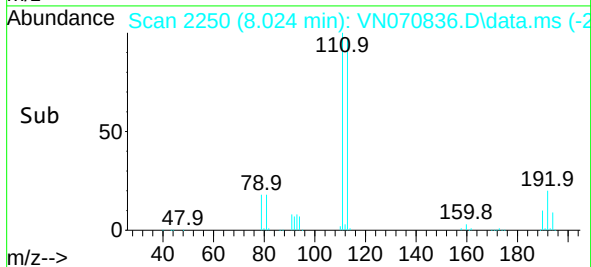

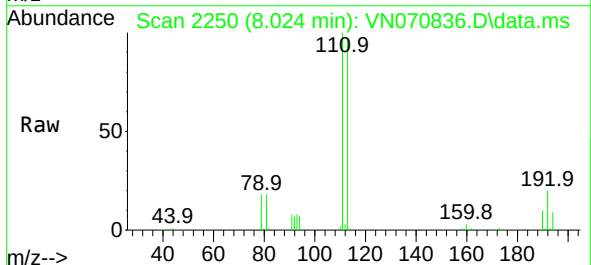


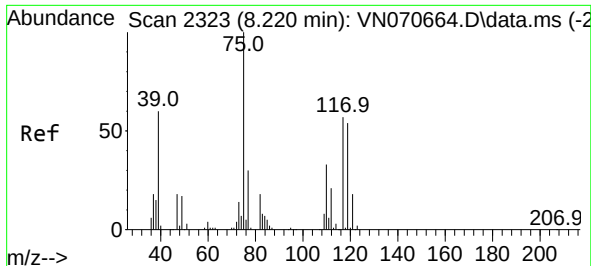

#36
1,1-Dichloropropene
Concen: 4.662 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.134 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18




Instrument :
MSVOA_N
ClientSampleId :
CC-6


Tgt Ion: 75 Resp: 78245
Ion Ratio Lower Upper
75 100
110 8.8 18.4 55.2#
77 0.0 24.4 36.6#

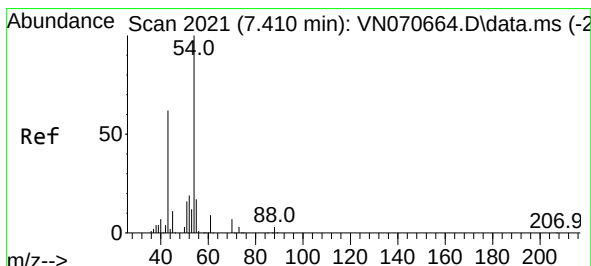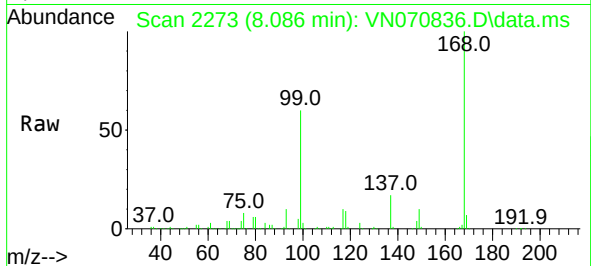

#37
Ethyl Acetate
Concen: 1.006 ug/l
RT: 7.351 min Scan# 1999
Delta R.T. -0.059 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18

Tgt Ion: 43 Resp: 22421
Ion Ratio Lower Upper
43 100
61 0.0 11.5 17.3#
70 0.0 7.9 11.9#



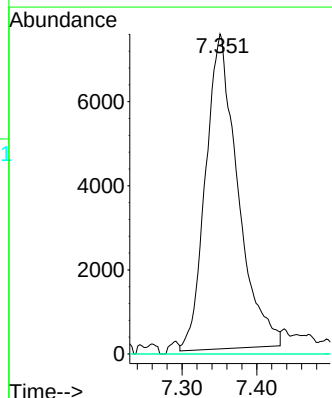



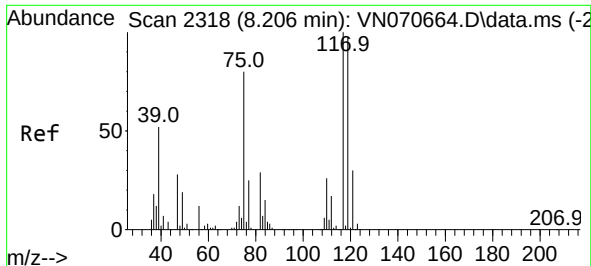

#38
Carbon Tetrachloride
Concen: 6.411 ug/l
RT: 8.088 min Scan# 21
Delta R.T. -0.118 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18




Instrument :
MSVOA_N
ClientSampleId :
CC-6


Tgt Ion:117 Resp: 95715
Ion Ratio Lower Upper
117 100
119 5.4 76.1 114.1#
121 0.0 24.2 36.2#

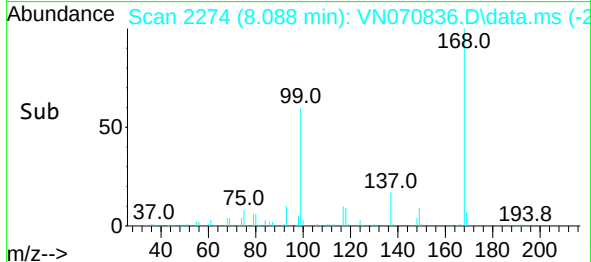

#43
Isopropyl Acetate
Concen: 4.695 ug/l
RT: 8.652 min Scan# 2484
Delta R.T. 0.091 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18

Tgt Ion: 43 Resp: 159769
Ion Ratio Lower Upper
43 100
61 0.2 20.4 30.6#
87 0.0 11.2 16.8#


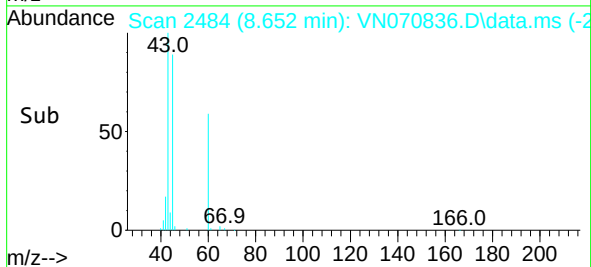

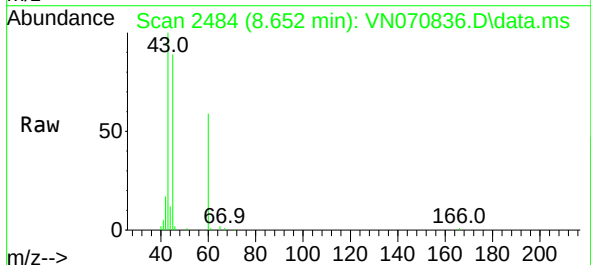




#48
Methyl methacrylate
Concen: 1.581 ug/l
RT: 9.550 min Scan# 2822
Delta R.T. -0.008 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18




Instrument :
MSVOA_N
ClientSampleId :
CC-6


Tgt Ion: 41 Resp: 25635
Ion Ratio Lower Upper
41 100
69 0.0 72.4 108.6#
39 23.6 58.4 87.6#

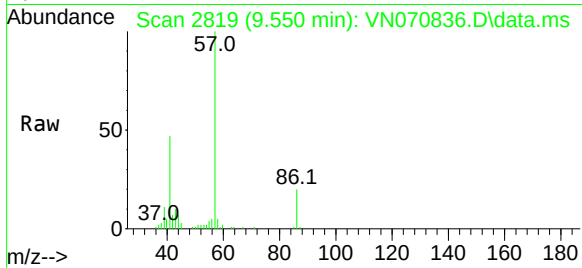

#50
Toluene-d8
Concen: 46.961 ug/l
RT: 10.440 min Scan# 3151
Delta R.T. 0.002 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18

Tgt Ion: 98 Resp: 1972166
Ion Ratio Lower Upper
98 100
100 63.9 50.4 75.6


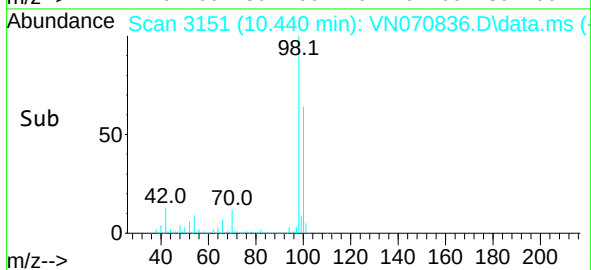

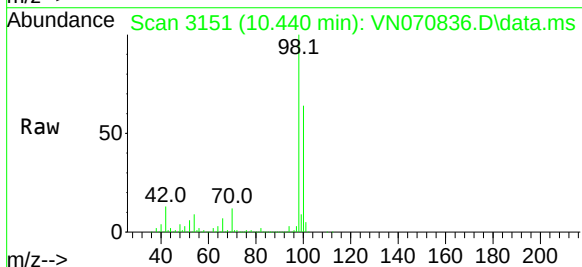


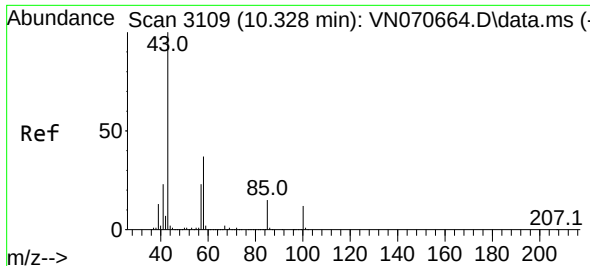

#51
4-Methyl-2-Pentanone
Concen: 1.456 ug/l
RT: 10.333 min Scan# 3109
Delta R.T. 0.005 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18




Instrument :
MSVOA_N
ClientSampleId :
CC-6


Tgt Ion: 43 Resp: 31618
Ion Ratio Lower Upper
43 100
58 33.1 30.4 45.6

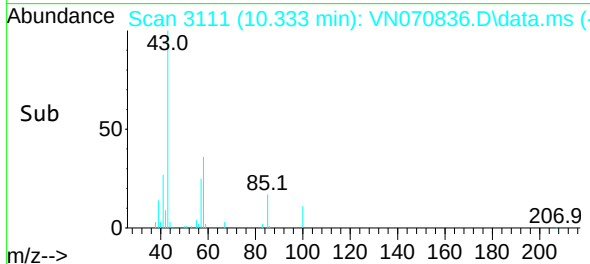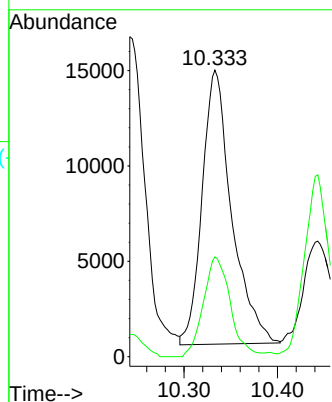

#53
t-1,3-Dichloropropene
Concen: 2.409 ug/l
RT: 10.719 min Scan# 3255
Delta R.T. 0.002 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18

Tgt Ion: 75 Resp: 110
Ion Ratio Lower Upper
75 100
77 0.0 25.6 38.4#




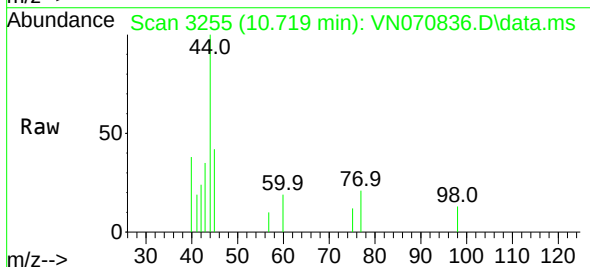




#54
cis-1,3-Dichloropropene
Concen: 0.641 ug/l
RT: 10.245 min Scan# 3057
Delta R.T. 0.057 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18




Instrument :
MSVOA_N
ClientSampleId :
CC-6


Tgt Ion: 75 Resp: 12925
Ion Ratio Lower Upper
75 100
77 0.0 26.4 39.6#
39 34.8 42.5 63.7#



#56
Ethyl methacrylate
Concen: 2.310 ug/l
RT: 10.692 min Scan# 3245
Delta R.T. -0.068 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18

Tgt Ion: 69 Resp: 203
Ion Ratio Lower Upper
69 100
41 0.0 51.4 77.0#
39 217.7 34.6 52.0#


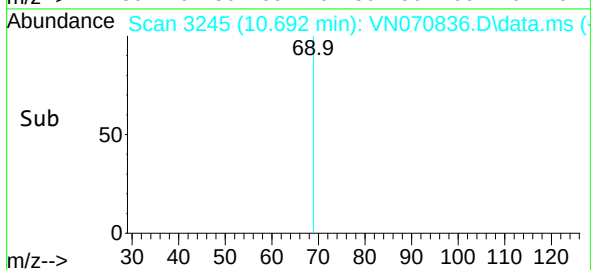

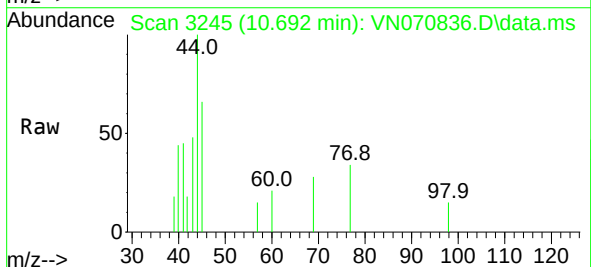


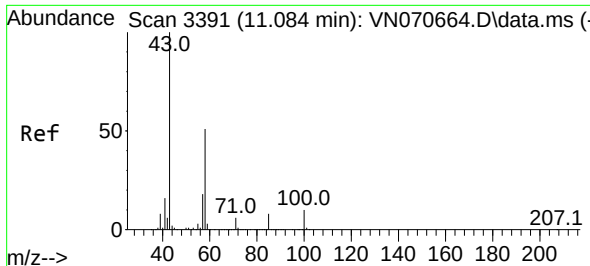

#59
2-Hexanone
Concen: 3.248 ug/l
RT: 11.057 min Scan# 31
Delta R.T. -0.027 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18




Instrument :
MSVOA_N
ClientSampleId :
CC-6


Tgt Ion: 43 Resp: 51243
Ion Ratio Lower Upper
43 100
58 0.0 26.9 80.7#

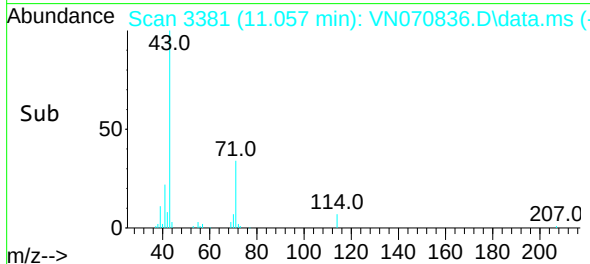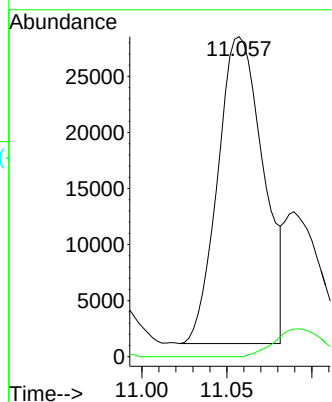

#62
4-Bromofluorobenzene
Concen: 46.808 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.003 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18

Tgt Ion: 95 Resp: 700481
Ion Ratio Lower Upper
95 100
174 74.3 0.0 187.2
176 71.4 0.0 181.4


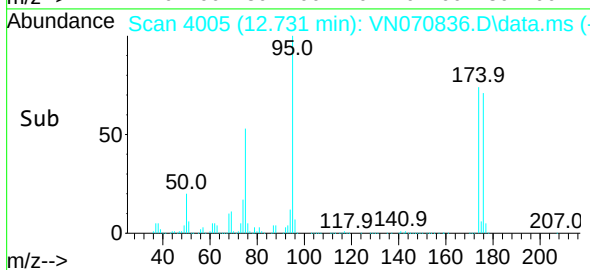

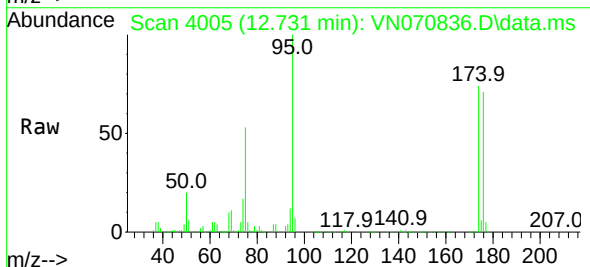


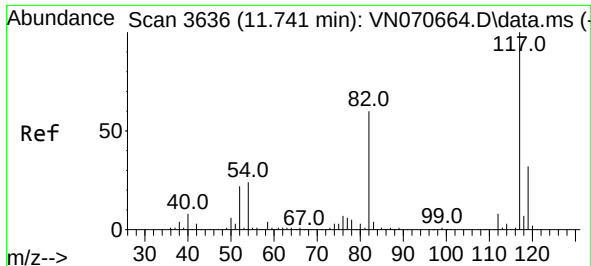

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3636
Delta R.T. 0.003 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18




Instrument :
MSVOA_N
ClientSampleId :
CC-6


Tgt Ion:117 Resp: 1485194
Ion Ratio Lower Upper
117 100
82 61.5 42.4 63.6
119 31.8 25.4 38.2

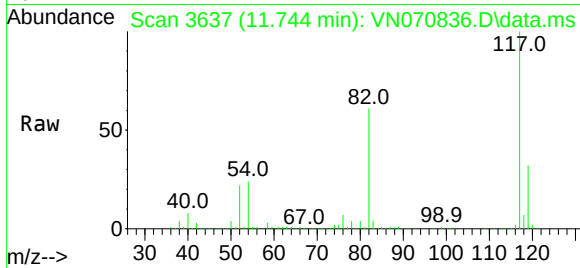

#67
Ethyl Benzene
Concen: 1.553 ug/l
RT: 11.843 min Scan# 3674
Delta R.T. 0.000 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18

Tgt Ion: 91 Resp: 92668
Ion Ratio Lower Upper
91 100
106 29.2 25.7 38.5

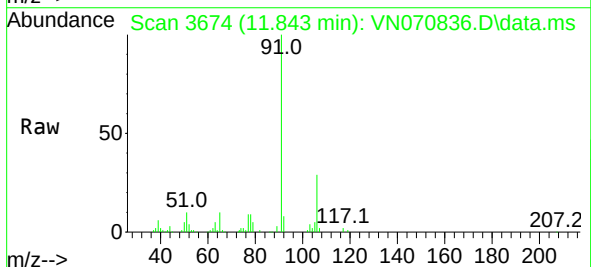



#68

m/p-Xylenes

Concen: 6.982 ug/l

RT: 11.948 min Scan# 31

Delta R.T. -0.002 min

Lab File: VN070836.D

Acq: 28 Jan 2022 18:18

Instrument :

MSVOA_N

ClientSampleId :





CC-6

Tgt Ion:106 Resp: 151541

Ion Ratio Lower Upper

106 100

91 214.7 160.6 240.8

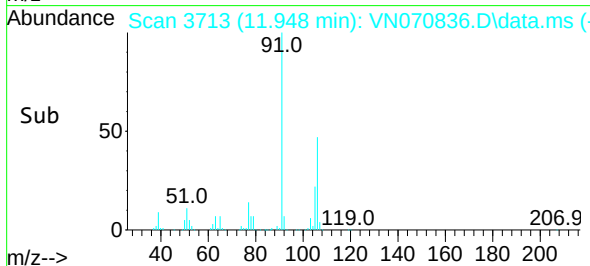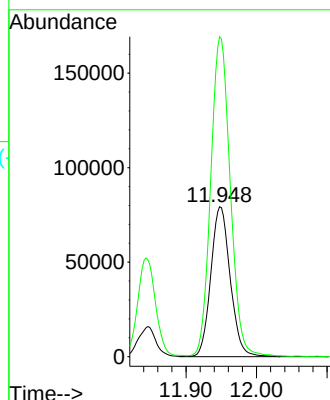

#69

o-Xylene

Concen: 3.098 ug/l

RT: 12.280 min Scan# 3837

Delta R.T. 0.002 min

Lab File: VN070836.D




Acq: 28 Jan 2022 18:18


Tgt Ion:106 Resp: 66721

Ion Ratio Lower Upper

106 100

91 223.9 105.8 317.3


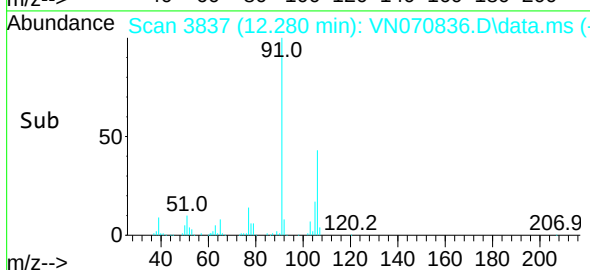
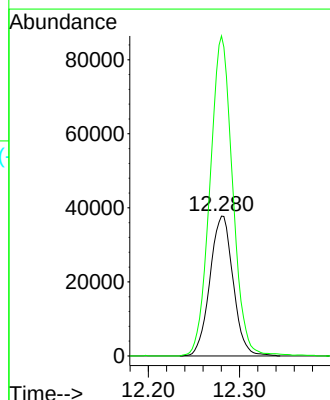
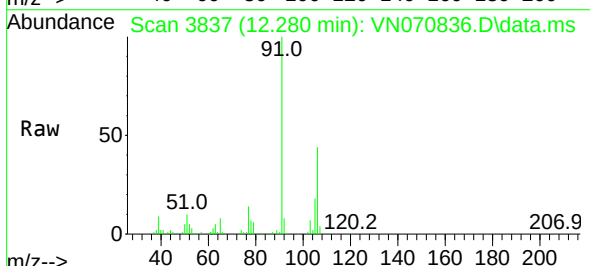


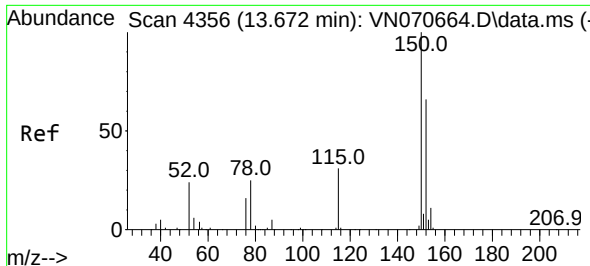

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 41
Delta R.T. 0.003 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18




Instrument :
MSVOA_N
ClientSampleId :
CC-6


Tgt Ion:152 Resp: 625497
Ion Ratio Lower Upper
152 100
115 63.4 27.5 82.5
150 157.4 0.0 344.4

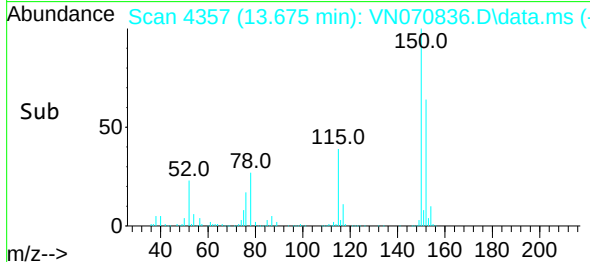

#73
Isopropylbenzene
Concen: 0.237 ug/l
RT: 12.581 min Scan# 3949
Delta R.T. 0.006 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18

Tgt Ion:105 Resp: 14045
Ion Ratio Lower Upper
105 100
120 24.6 13.4 40.1

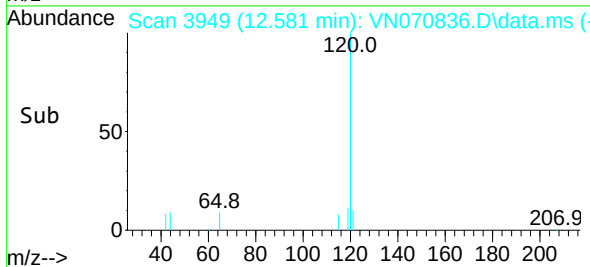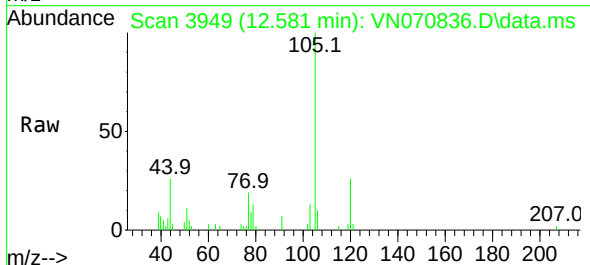



#76

1,2,3-Trichloropropane

Concen: 22.244 ug/l

RT: 12.731 min Scan# 4005

Delta R.T. -0.147 min

Lab File: VN070836.D

Acq: 28 Jan 2022 18:18

Instrument :

MSVOA_N

ClientSampleId :





CC-6

Tgt Ion: 75 Resp: 369019

Ion Ratio Lower Upper

75 100

77 1.2 82.6 247.8#

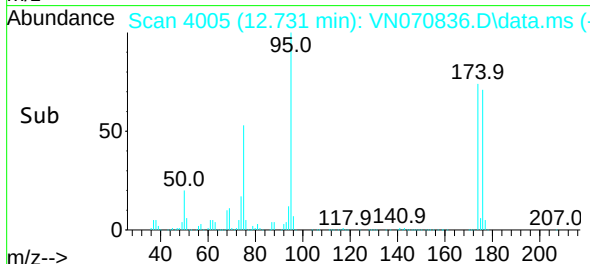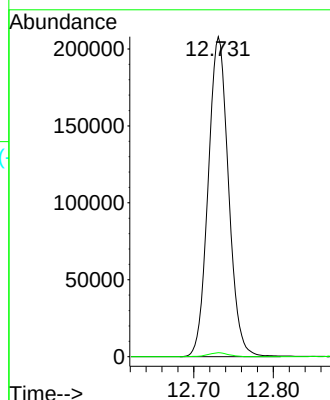

#78

n-propylbenzene

Concen: 0.383 ug/l

RT: 12.921 min Scan# 4076

Delta R.T. 0.002 min

Lab File: VN070836.D




Acq: 28 Jan 2022 18:18


Tgt Ion: 91 Resp: 25355

Ion Ratio Lower Upper

91 100

120 21.5 11.9 35.9


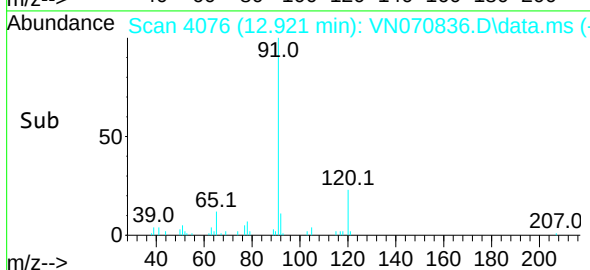
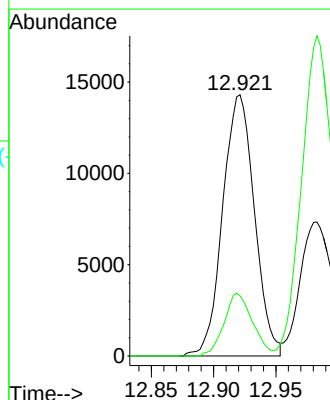
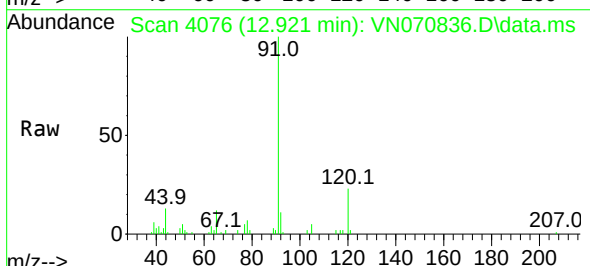




#79
2-Chlorotoluene
Concen: 0.270 ug/l
RT: 12.983 min Scan# 4099
Delta R.T. -0.021 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18




Instrument :
MSVOA_N
ClientSampleId :
CC-6


Tgt Ion: 91 Resp: 11317
Ion Ratio Lower Upper
91 100
126 0.0 18.3 54.8#

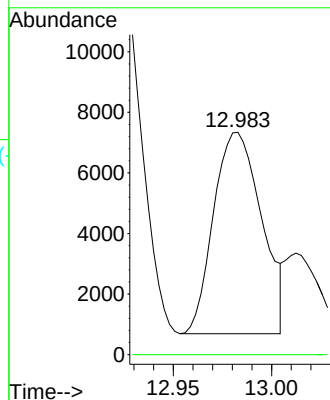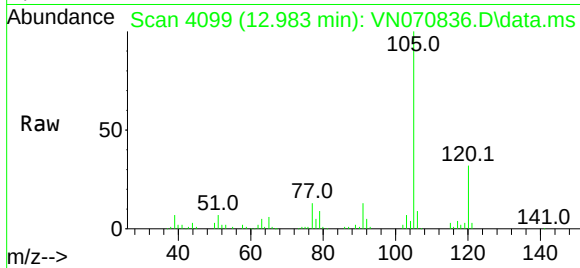

#80
1,3,5-Trimethylbenzene
Concen: 1.884 ug/l
RT: 13.058 min Scan# 4127
Delta R.T. -0.000 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18

Tgt Ion: 105 Resp: 90158
Ion Ratio Lower Upper
105 100
120 47.2 24.6 73.6


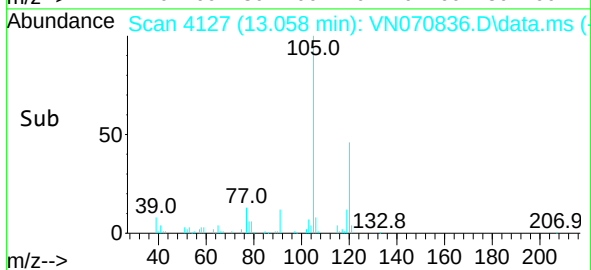
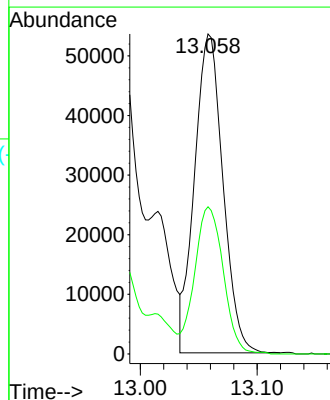
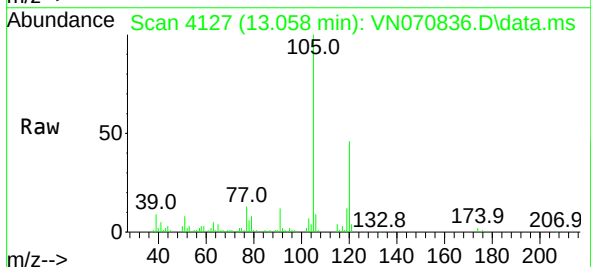


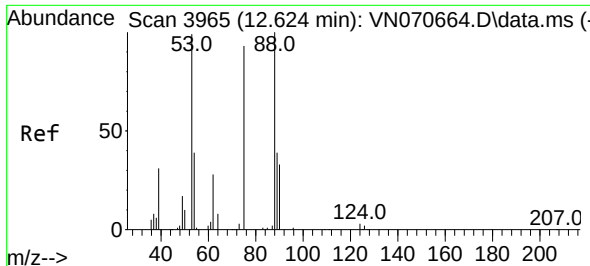

#81
trans-1,4-Dichloro-2-butene
Concen: 66.268 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.107 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18




Instrument :
MSVOA_N
ClientSampleId :
CC-6


Tgt Ion: 75 Resp: 369019
Ion Ratio Lower Upper
75 100
53 0.1 90.5 135.7#
89 0.0 38.2 57.4#

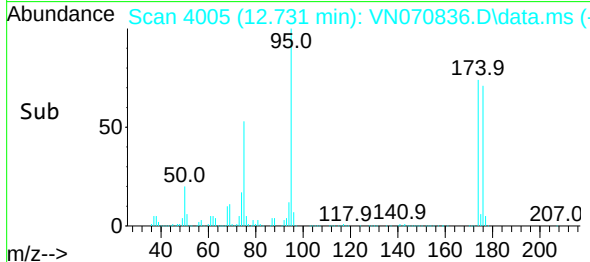

#82
4-Chlorotoluene
Concen: 0.233 ug/l
RT: 13.058 min Scan# 4127
Delta R.T. -0.046 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18

Tgt Ion: 91 Resp: 9127
Ion Ratio Lower Upper
91 100
126 0.0 18.2 54.6#


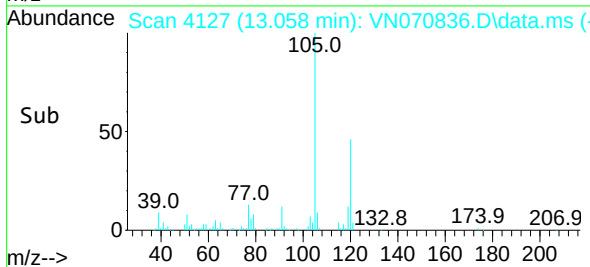

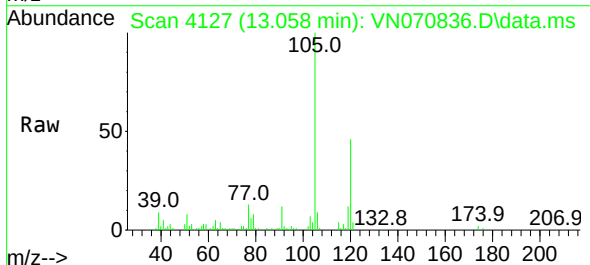


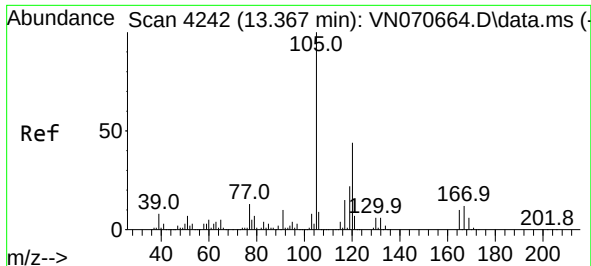

#84
1,2,4-Trimethylbenzene
Concen: 6.433 ug/l
RT: 13.366 min Scan# 41
Delta R.T. -0.001 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18




Instrument :
MSVOA_N
ClientSampleId :
CC-6


Tgt Ion:105 Resp: 295907
Ion Ratio Lower Upper
105 100
120 43.6 22.8 68.4

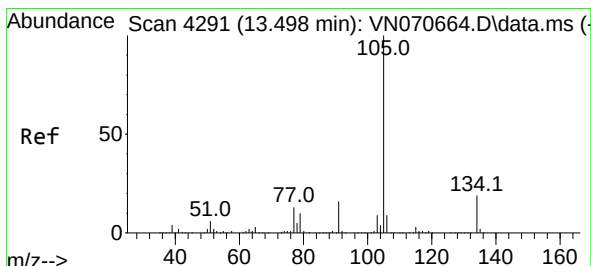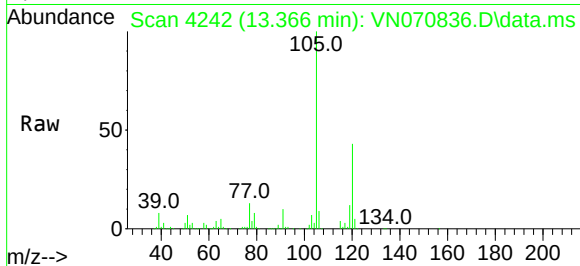

#85
sec-Butylbenzene
Concen: 5.225 ug/l
RT: 13.366 min Scan# 4242
Delta R.T. -0.132 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18

Tgt Ion:105 Resp: 295907
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#


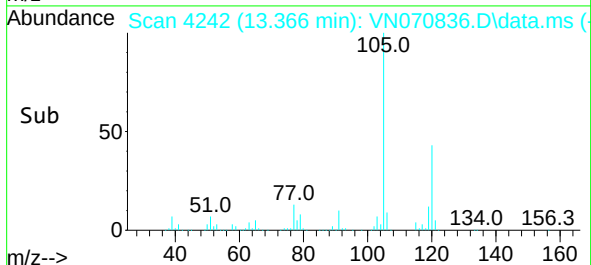

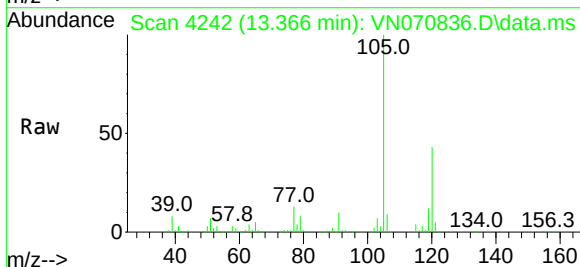




#86
p-Isopropyltoluene
Concen: 0.280 ug/l
RT: 13.616 min Scan# 41
Delta R.T. 0.003 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18




Instrument :
MSVOA_N
ClientSampleId :
CC-6


Tgt Ion:119 Resp: 12471
Ion Ratio Lower Upper
119 100
134 26.1 13.6 40.7
91 30.8 11.4 34.1

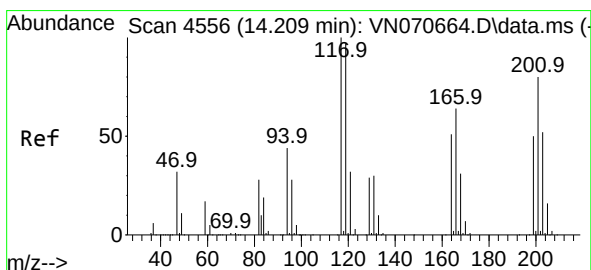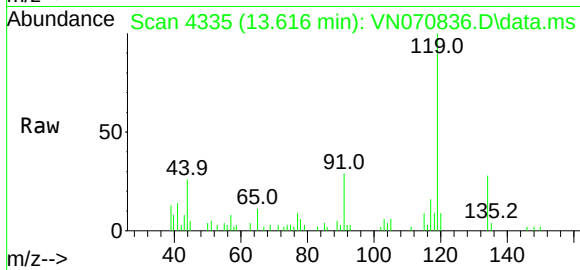

#90
Hexachloroethane
Concen: 0.505 ug/l
RT: 14.219 min Scan# 4560
Delta R.T. 0.010 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18

Tgt Ion:117 Resp: 3927
Ion Ratio Lower Upper
117 100
201 0.0 43.9 131.6#




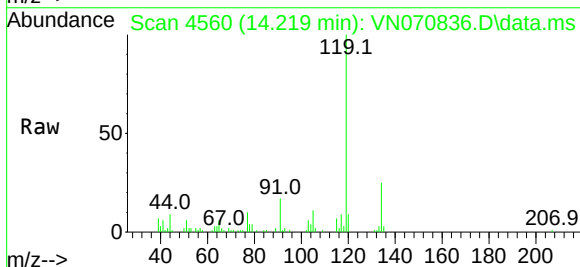




#93
1,2,4-Trichlorobenzene
Concen: 3.464 ug/l
RT: 15.255 min Scan# 4949
Delta R.T. -0.008 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18




Instrument :
MSVOA_N
ClientSampleId :
CC-6


Tgt Ion:180 Resp: 479
Ion Ratio Lower Upper
180 100
182 71.4 48.3 144.9
145 352.2 14.5 43.5#

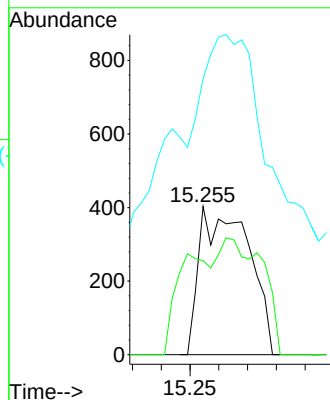

#95
Naphthalene
Concen: 7.931 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. 0.003 min
Lab File: VN070836.D
Acq: 28 Jan 2022 18:18


Tgt Ion:128 Resp: 107362
Ion Ratio Lower Upper
128 100
127 13.0 10.5 15.7
129 11.1 8.7 13.1

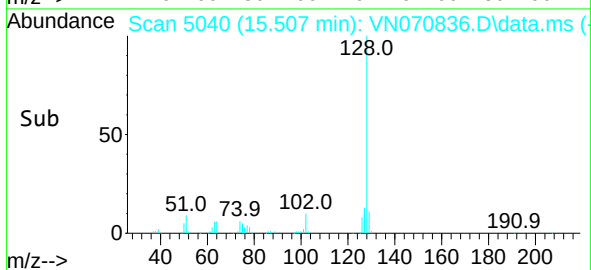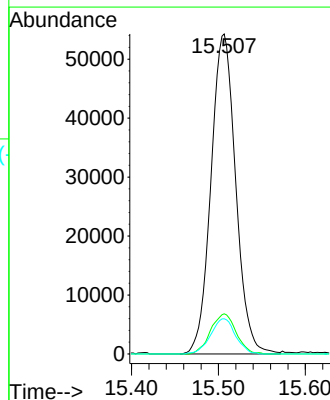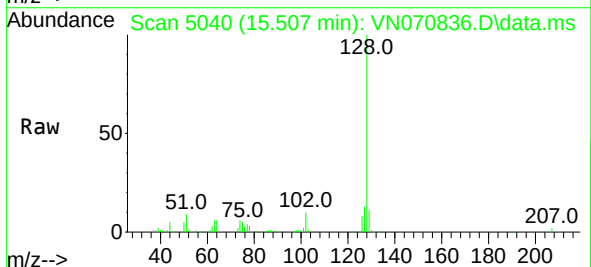



#96
 1,2,3-Trichlorobenzene
 Concen: 3.223 ug/l
 RT: 15.686 min Scan# 51
 Delta R.T. -0.011 min
 Lab File: VN070836.D
 Acq: 28 Jan 2022 18:18

Instrument :
 MSVOA_N
 ClientSampleId :
 CC-6

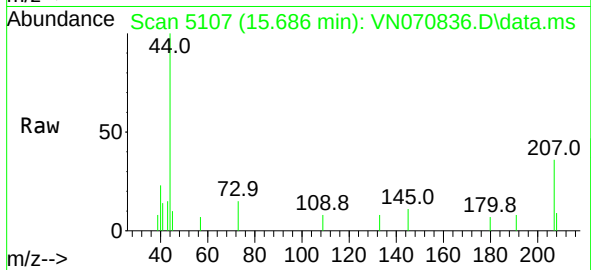

Tgt Ion:180 Resp: 87
 Ion Ratio Lower Upper
 180 100
 182 0.0 47.4 142.2#
 145 394.3 15.0 45.1#

