

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012822\
 Data File : VN070840.D
 Acq On : 28 Jan 2022 20:00
 Operator : JC/MD
 Sample : N1303-02
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 CC-5

Quant Time: Jan 28 23:19:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 18 13:32:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	884140	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.968	114	1465074	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	1371876	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	575327	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	605416	47.779	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	95.560%
35) Dibromofluoromethane	8.021	113	402055	44.241	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	88.480%
50) Toluene-d8	10.440	98	1825619	47.685	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	95.380%
62) 4-Bromofluorobenzene	12.731	95	644158	47.217	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	94.440%


Target Compounds			Qvalue			
11) Tert butyl alcohol	5.390	59	461	0.202	ug/l	# 71
16) Acetone	4.296	43	193858	22.043	ug/l	98
20) Methylene Chloride	5.095	84	9618	0.830	ug/l	94
25) 2-Butanone	7.348	43	22758	2.056	ug/l	# 86
30) Chloroform	8.070	83	69	Below Cal	#	18
31) Cyclohexane	8.083	56	18969	0.850	ug/l	# 1
36) 1,1-Dichloropropene	8.088	75	72734	4.754	ug/l	# 49
37) Ethyl Acetate	7.348	43	22758	1.120	ug/l	# 69
38) Carbon Tetrachloride	8.088	117	90652	6.660	ug/l	# 17
43) Isopropyl Acetate	8.692	43	107227	3.456	ug/l	# 55
48) Methyl methacrylate	9.547	41	26000	1.759	ug/l	# 14
51) 4-Methyl-2-Pentanone	10.333	43	25424	1.284	ug/l	94
53) t-1,3-Dichloropropene	10.443	75	602	2.435	ug/l	# 1
54) cis-1,3-Dichloropropene	10.242	75	4041	0.220	ug/l	# 63
56) Ethyl methacrylate	10.711	69	435	2.321	ug/l	# 24
59) 2-Hexanone	11.060	43	54434	3.785	ug/l	# 25
67) Ethyl Benzene	11.843	91	66470	1.206	ug/l	94
68) m/p-Xylenes	11.948	106	113511	5.662	ug/l	91
69) o-Xylene	12.280	106	51323	2.580	ug/l	92
73) Isopropylbenzene	12.583	105	11496	0.211	ug/l	99
76) 1,2,3-Trichloropropane	12.731	75	342048	22.416	ug/l	# 1
78) n-propylbenzene	12.921	91	21376	0.351	ug/l	94
79) 2-Chlorotoluene	12.986	91	15028	0.390	ug/l	# 38
80) 1,3,5-Trimethylbenzene	13.058	105	82897	1.883	ug/l	94
81) trans-1,4-Dichloro-2-b...	12.731	75	342048	66.781	ug/l	# 5
82) 4-Chlorotoluene	13.055	91	9759	0.271	ug/l	# 38
84) 1,2,4-Trimethylbenzene	13.367	105	263494	6.228	ug/l	97
86) p-Isopropyltoluene	13.616	119	12217	0.299	ug/l	98
90) Hexachloroethane	14.214	117	2945	0.412	ug/l	# 6
93) 1,2,4-Trichlorobenzene	15.257	180	219	3.444	ug/l	# 1
95) Naphthalene	15.507	128	115609	8.440	ug/l	100
96) 1,2,3-Trichlorobenzene	15.697	180	91	3.224	ug/l	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012822\
Data File : VN070840.D
Acq On : 28 Jan 2022 20:00
Operator : JC/MD
Sample : N1303-02
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
CC-5

Quant Time: Jan 28 23:19:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 18 13:32:07 2022
Response via : Initial Calibration




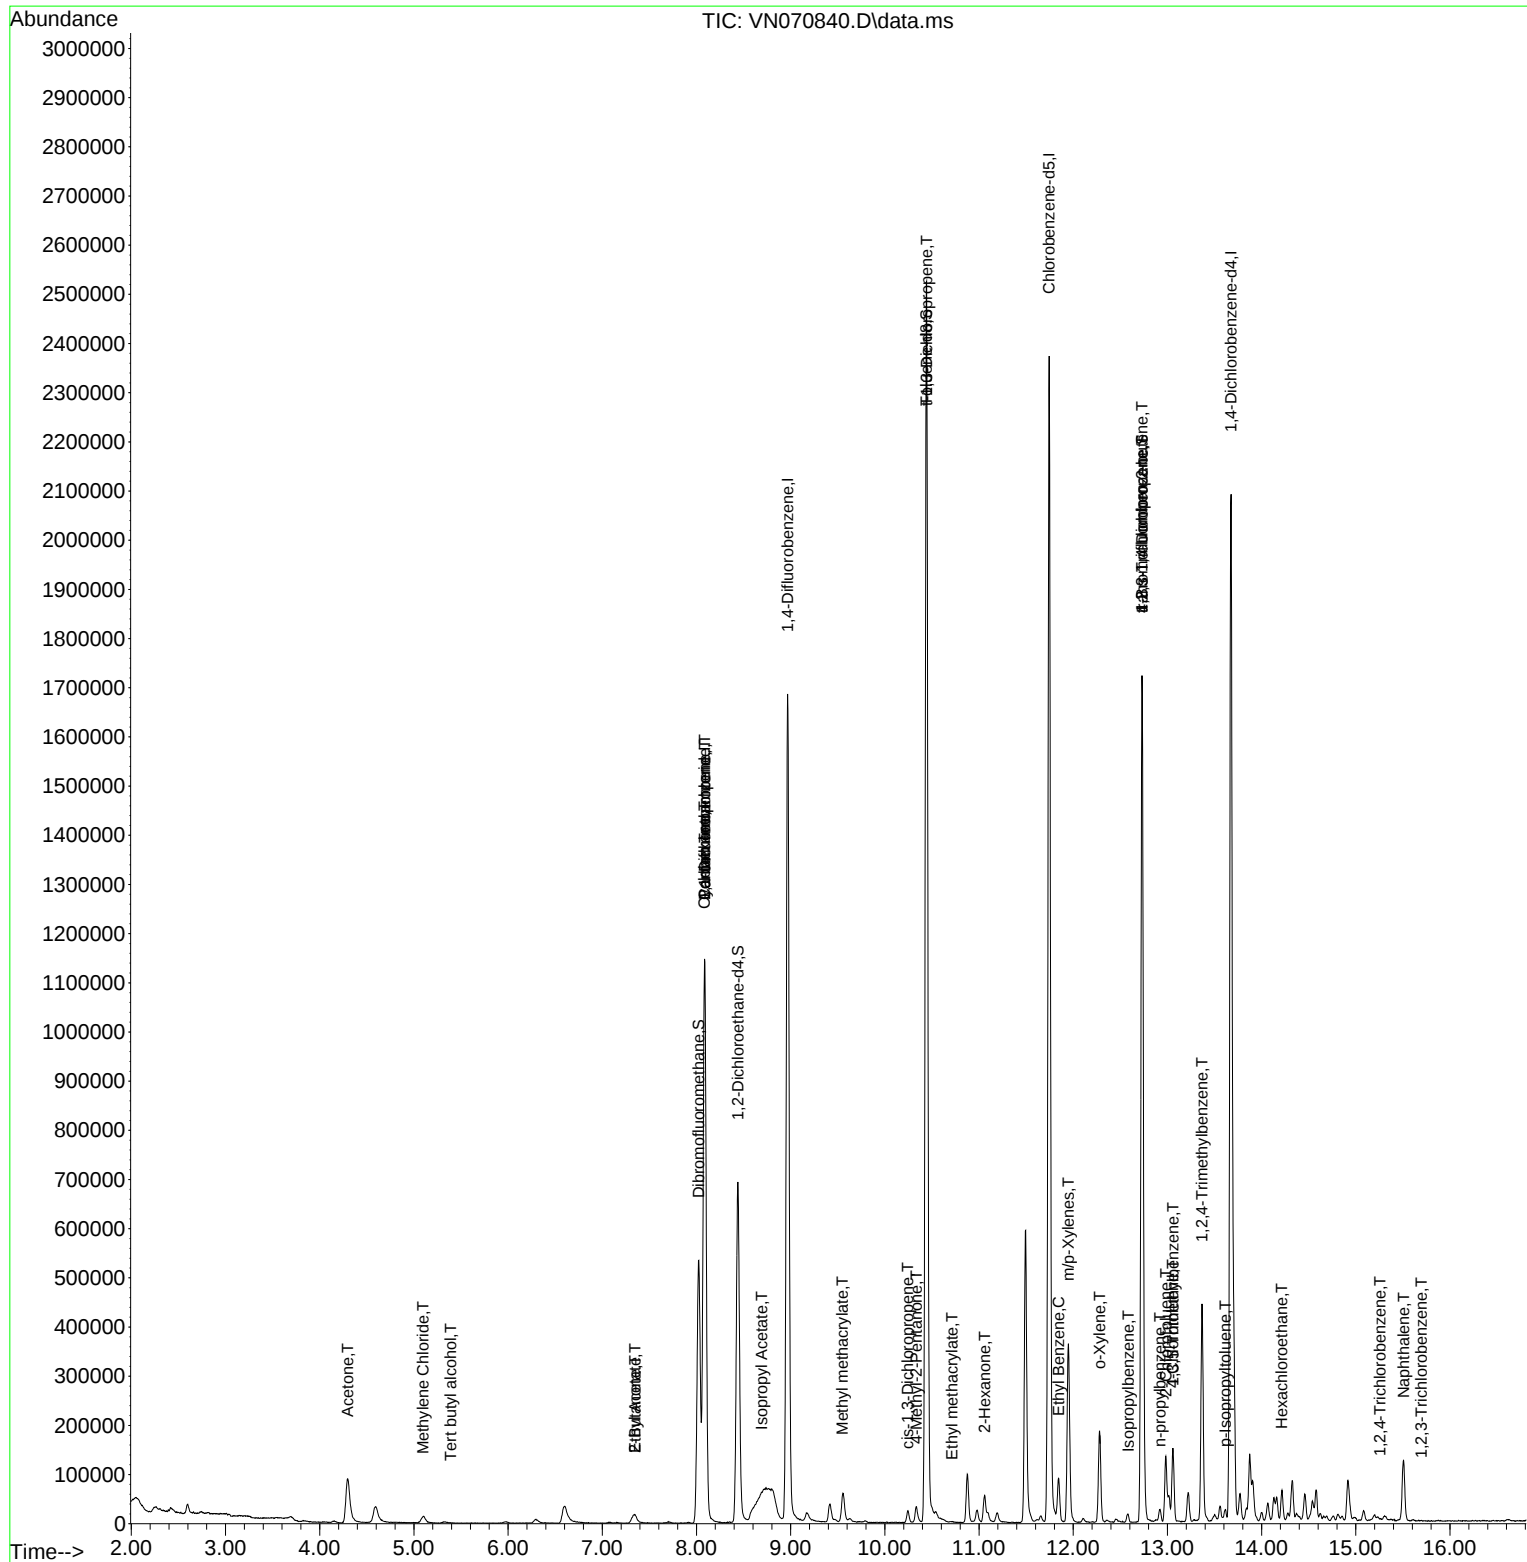




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 21
Delta R.T. 0.005 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00




Instrument :
MSVOA_N
ClientSampleId :
CC-5


Tgt Ion:168 Resp: 884140
Ion Ratio Lower Upper
168 100
99 62.0 41.3 61.9#

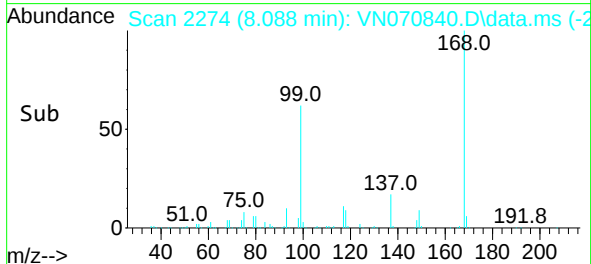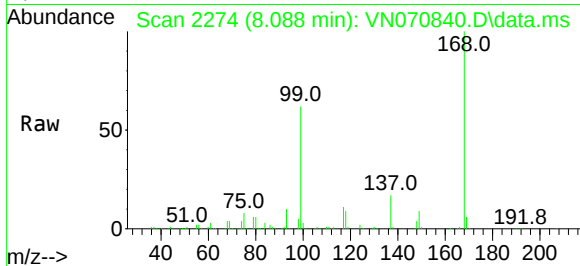

#11
Tert butyl alcohol
Concen: 0.202 ug/l
RT: 5.390 min Scan# 1268
Delta R.T. 0.013 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00

Tgt Ion: 59 Resp: 461
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#


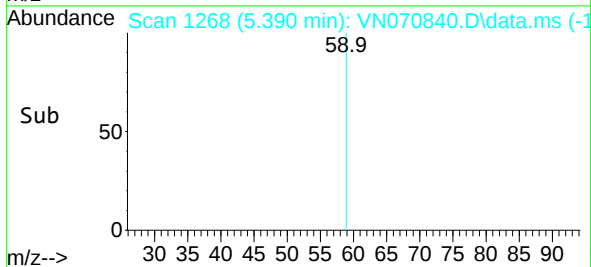

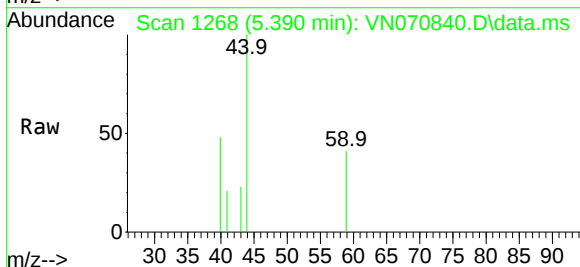




#16
Acetone
Concen: 22.043 ug/l
RT: 4.296 min Scan# 856
Delta R.T. 0.011 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00




Instrument :
MSVOA_N
ClientSampleId :
CC-5


Tgt Ion: 43 Resp: 193858
Ion Ratio Lower Upper
43 100
58 29.7 23.1 34.7

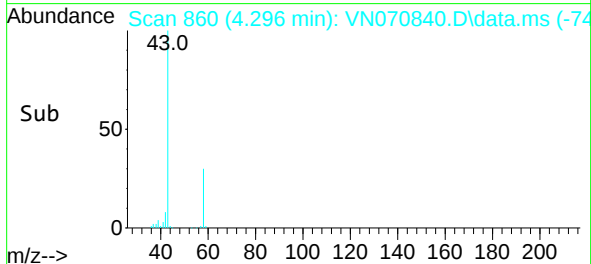

#20
Methylene Chloride
Concen: 0.830 ug/l
RT: 5.095 min Scan# 1158
Delta R.T. 0.000 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00

Tgt Ion: 84 Resp: 9618
Ion Ratio Lower Upper
84 100
49 123.6 93.5 140.3
51 38.7 29.4 44.2
86 61.3 53.0 79.4

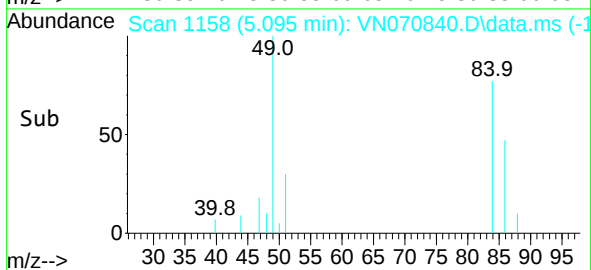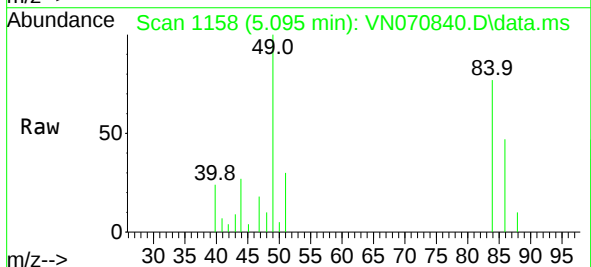

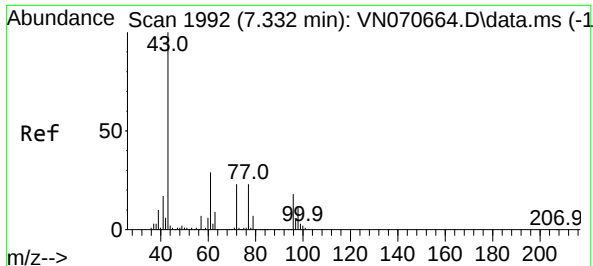

#25

2-Butanone

Concen: 2.056 ug/l

RT: 7.348 min Scan# 1992

Delta R.T. 0.016 min

Lab File: VN070840.D

Acq: 28 Jan 2022 20:00

Instrument :

MSVOA_N

ClientSampleId :





CC-5

Tgt Ion: 43 Resp: 22758

Ion Ratio Lower Upper

43 100

72 19.7 21.7 32.5#

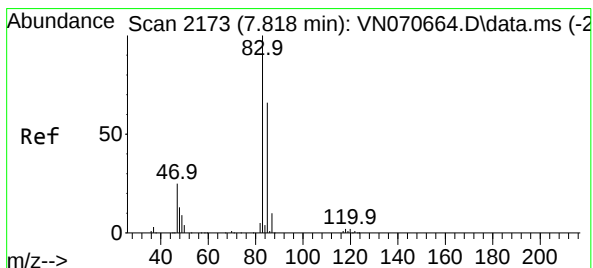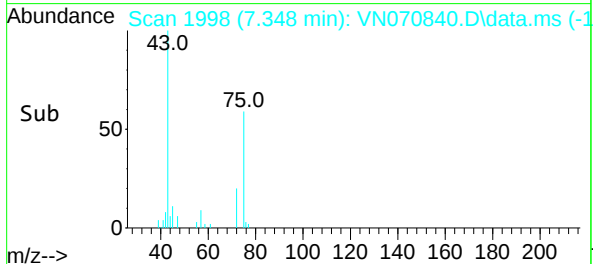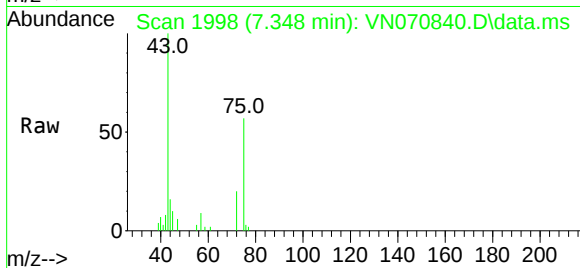

#30

Chloroform

Concen: Below Cal

RT: 8.070 min Scan# 2267

Delta R.T. 0.252 min

Lab File: VN070840.D




Acq: 28 Jan 2022 20:00


Tgt Ion: 83 Resp: 69

Ion Ratio Lower Upper

83 100

85 0.0 51.9 77.9#


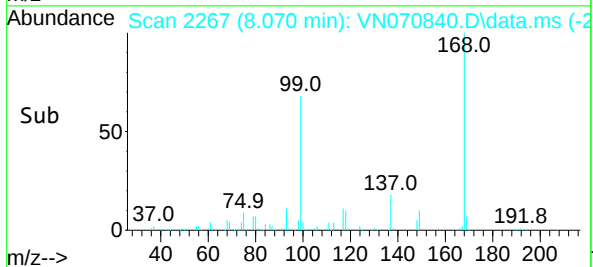

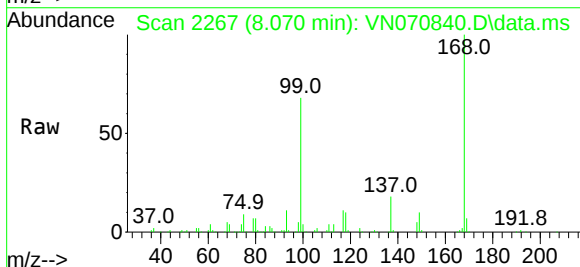




#31
Cyclohexane
Concen: 0.850 ug/l
RT: 8.083 min Scan# 21
Delta R.T. -0.011 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00




Instrument :
MSVOA_N
ClientSampleId :
CC-5


Tgt Ion: 56 Resp: 18969
Ion Ratio Lower Upper
56 100
69 176.5 27.1 40.7#
84 150.0 73.4 110.0#

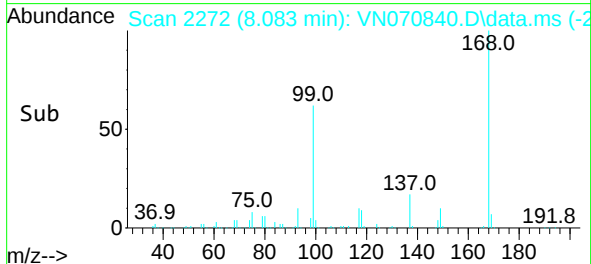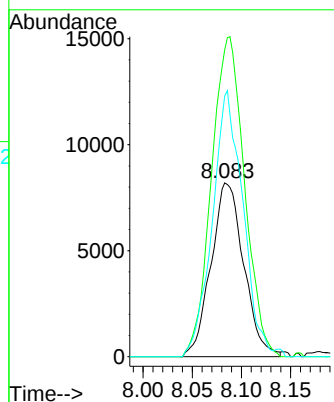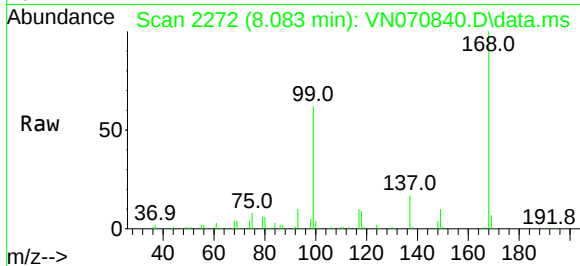

#33
1,2-Dichloroethane-d4
Concen: 47.779 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. 0.006 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00

Tgt Ion: 65 Resp: 605416
Ion Ratio Lower Upper
65 100
67 52.7 0.0 103.0


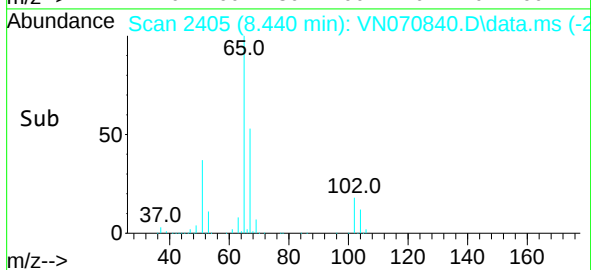
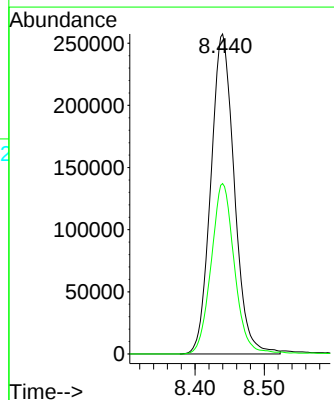
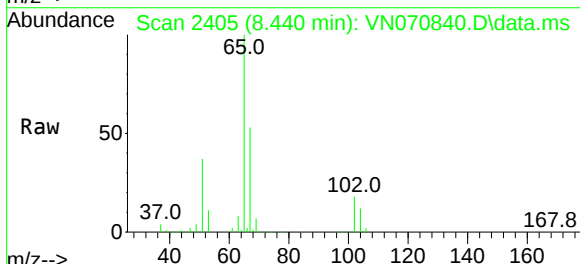




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.968 min Scan# 2602
Delta R.T. 0.003 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00




Instrument :
MSVOA_N
ClientSampleId :
CC-5


Tgt Ion:114 Resp: 1465074
Ion Ratio Lower Upper
114 100
63 23.5 0.0 37.8
88 16.9 0.0 27.4

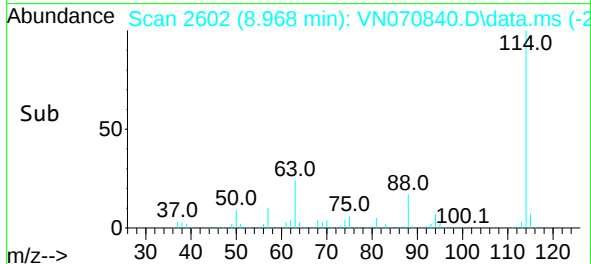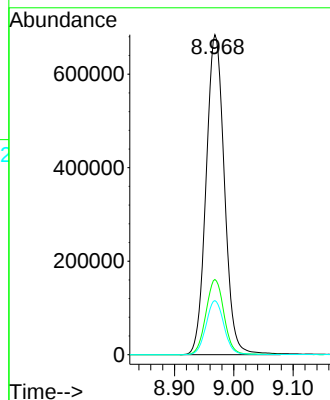

#35
Dibromofluoromethane
Concen: 44.241 ug/l
RT: 8.021 min Scan# 2249
Delta R.T. 0.002 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00

Tgt Ion:113 Resp: 402055
Ion Ratio Lower Upper
113 100
111 103.9 82.2 123.2
192 19.7 16.9 25.3


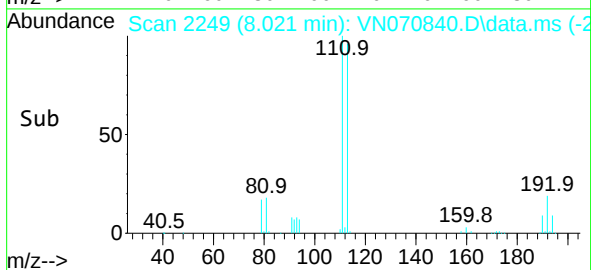
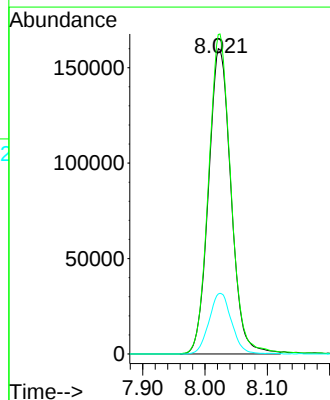
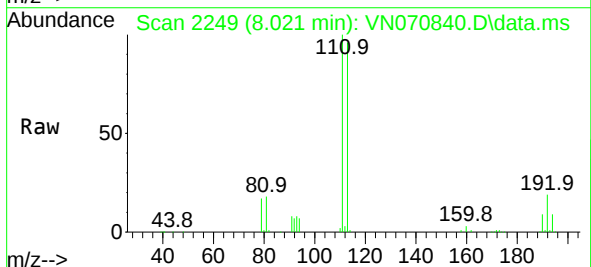




#36
 1,1-Dichloropropene
 Concen: 4.754 ug/l
 RT: 8.088 min Scan# 21
 Delta R.T. -0.132 min
 Lab File: VN070840.D
 Acq: 28 Jan 2022 20:00




Instrument :
 MSVOA_N
 ClientSampleId :
 CC-5


Tgt Ion: 75 Resp: 72734
 Ion Ratio Lower Upper
 75 100
 110 9.0 18.4 55.2#
 77 0.0 24.4 36.6#

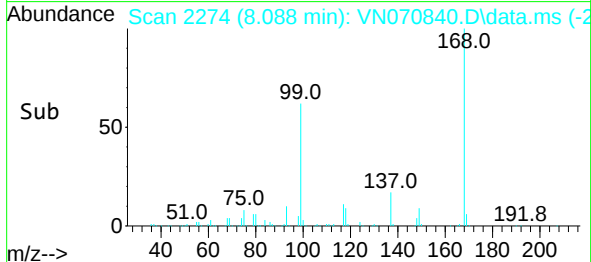

#37
 Ethyl Acetate
 Concen: 1.120 ug/l
 RT: 7.348 min Scan# 1998
 Delta R.T. -0.062 min
 Lab File: VN070840.D
 Acq: 28 Jan 2022 20:00

Tgt Ion: 43 Resp: 22758
 Ion Ratio Lower Upper
 43 100
 61 0.7 11.5 17.3#
 70 0.0 7.9 11.9#


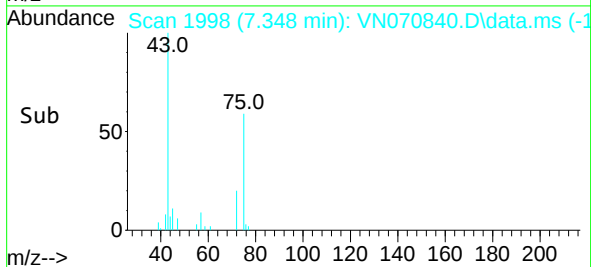

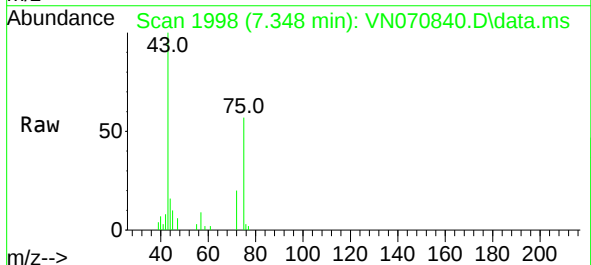




#38
Carbon Tetrachloride
Concen: 6.660 ug/l
RT: 8.088 min Scan# 21
Delta R.T. -0.118 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00




Instrument :
MSVOA_N
ClientSampleId :
CC-5


Tgt Ion:117 Resp: 90652
Ion Ratio Lower Upper
117 100
119 5.4 76.1 114.1#
121 0.0 24.2 36.2#

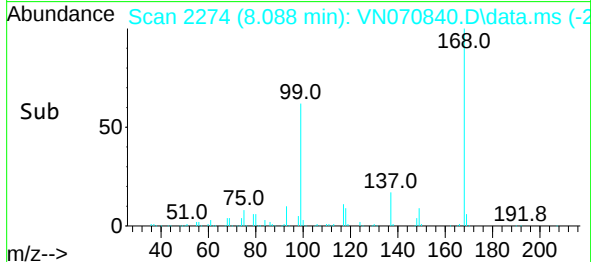

#43
Isopropyl Acetate
Concen: 3.456 ug/l
RT: 8.692 min Scan# 2499
Delta R.T. 0.132 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00

Tgt Ion: 43 Resp: 107227
Ion Ratio Lower Upper
43 100
61 0.0 20.4 30.6#
87 0.0 11.2 16.8#


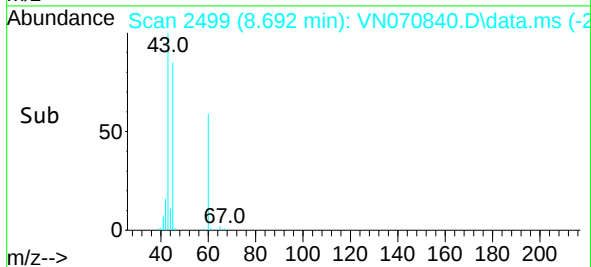

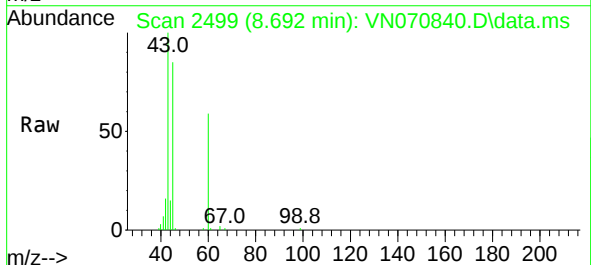




#48
Methyl methacrylate
Concen: 1.759 ug/l
RT: 9.547 min Scan# 2818
Delta R.T. -0.011 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00




Instrument :
MSVOA_N
ClientSampleId :
CC-5


Tgt Ion: 41 Resp: 26000
Ion Ratio Lower Upper
41 100
69 0.0 72.4 108.6#
39 11.2 58.4 87.6#

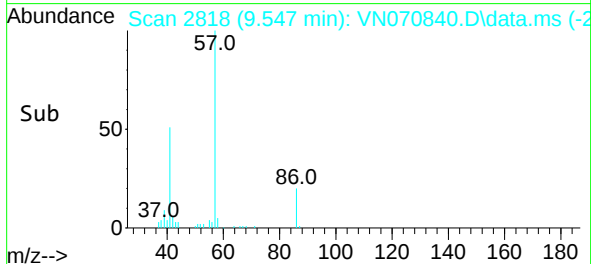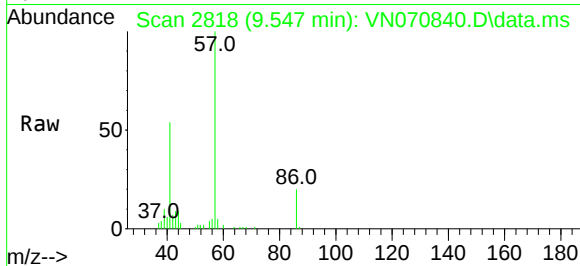

#50
Toluene-d8
Concen: 47.685 ug/l
RT: 10.440 min Scan# 3151
Delta R.T. 0.002 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00

Tgt Ion: 98 Resp: 1825619
Ion Ratio Lower Upper
98 100
100 63.7 50.4 75.6

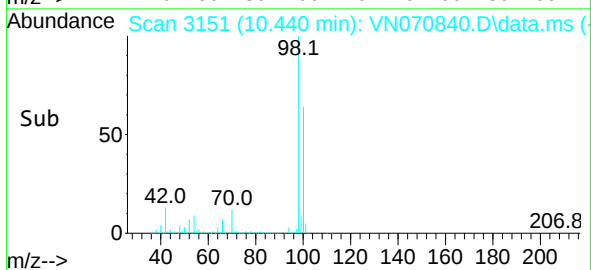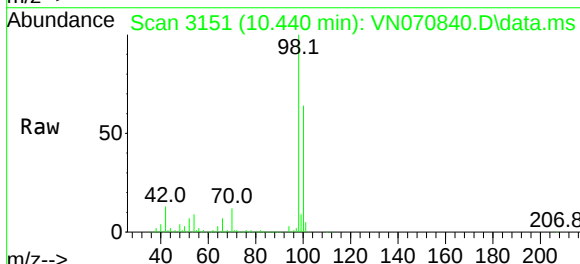

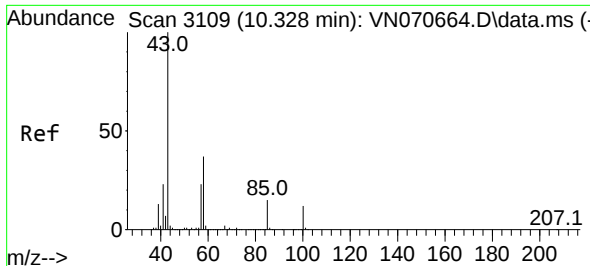

#51

4-Methyl-2-Pentanone

Concen: 1.284 ug/l

RT: 10.333 min Scan# 3111

Delta R.T. 0.005 min

Lab File: VN070840.D

Acq: 28 Jan 2022 20:00

Instrument :

MSVOA_N

ClientSampleId :





CC-5

Tgt Ion: 43 Resp: 25424

Ion Ratio Lower Upper

43 100

58 34.5 30.4 45.6

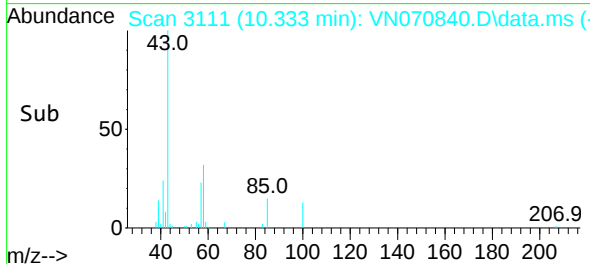

#53

t-1,3-Dichloropropene

Concen: 2.435 ug/l

RT: 10.443 min Scan# 3152

Delta R.T. -0.274 min

Lab File: VN070840.D




Acq: 28 Jan 2022 20:00


Tgt Ion: 75 Resp: 602

Ion Ratio Lower Upper

75 100

77 158.8 25.6 38.4#


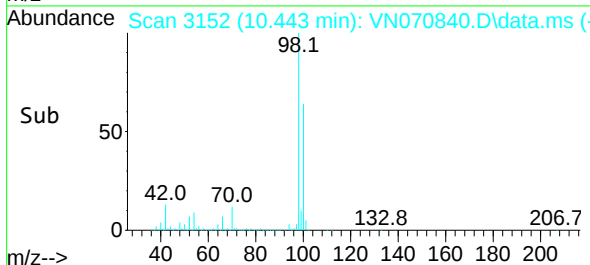

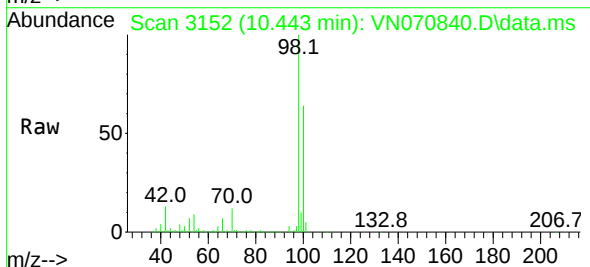




#54
 cis-1,3-Dichloropropene
 Concen: 0.220 ug/l
 RT: 10.242 min Scan# 3057
 Delta R.T. 0.054 min
 Lab File: VN070840.D
 Acq: 28 Jan 2022 20:00




Instrument :
 MSVOA_N
 ClientSampleId :
 CC-5


Tgt Ion: 75 Resp: 4041
 Ion Ratio Lower Upper
 75 100
 77 0.0 26.4 39.6#
 39 35.8 42.5 63.7#

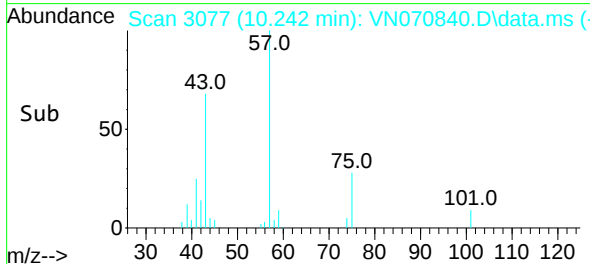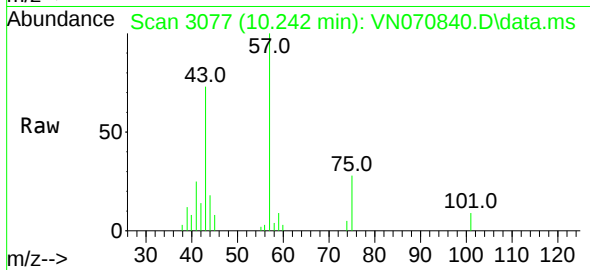

#56
 Ethyl methacrylate
 Concen: 2.321 ug/l
 RT: 10.711 min Scan# 3252
 Delta R.T. -0.049 min
 Lab File: VN070840.D
 Acq: 28 Jan 2022 20:00

Tgt Ion: 69 Resp: 435
 Ion Ratio Lower Upper
 69 100
 41 0.0 51.4 77.0#
 39 0.0 34.6 52.0#



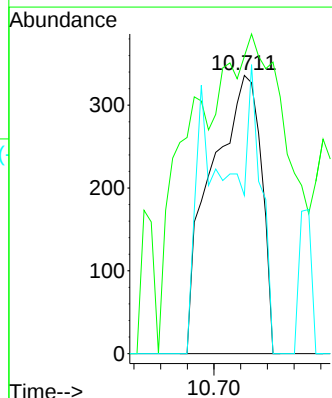
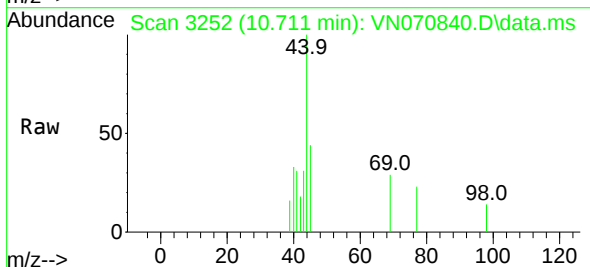


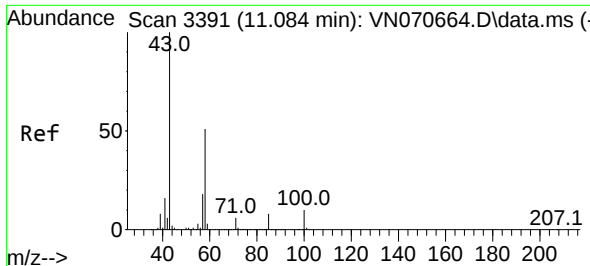

#59
2-Hexanone
Concen: 3.785 ug/l
RT: 11.060 min Scan# 31
Delta R.T. -0.024 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00




Instrument :
MSVOA_N
ClientSampleId :
CC-5


Tgt Ion: 43 Resp: 54434
Ion Ratio Lower Upper
43 100
58 0.0 26.9 80.7#

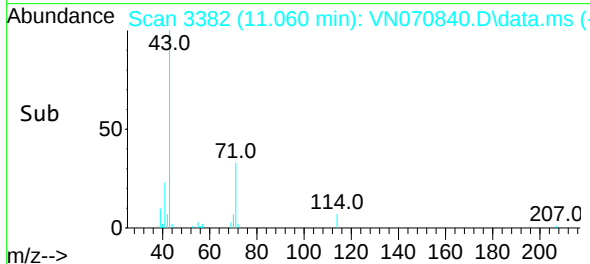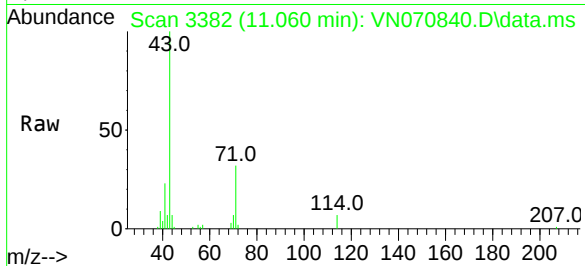

#62
4-Bromofluorobenzene
Concen: 47.217 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.003 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00

Tgt Ion: 95 Resp: 644158
Ion Ratio Lower Upper
95 100
174 74.2 0.0 187.2
176 71.7 0.0 181.4


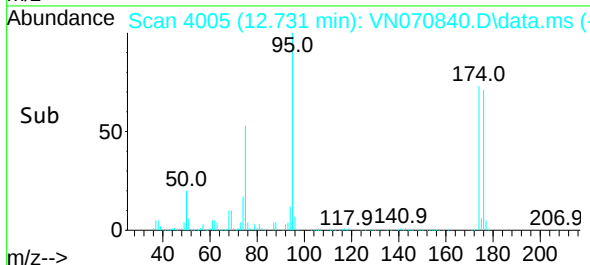

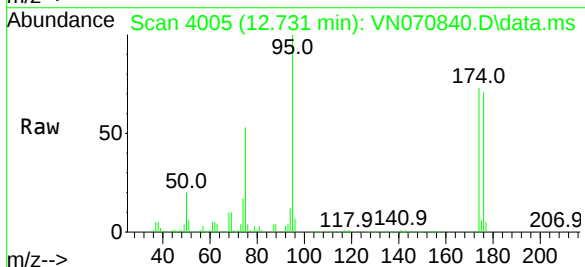




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3637
Delta R.T. 0.003 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00




Instrument :
MSVOA_N
ClientSampleId :
CC-5


Tgt Ion:117 Resp: 1371876
Ion Ratio Lower Upper
117 100
82 60.0 42.4 63.6
119 32.0 25.4 38.2

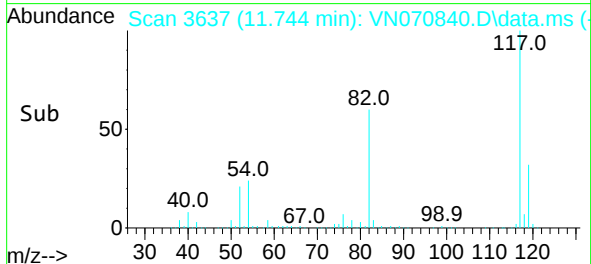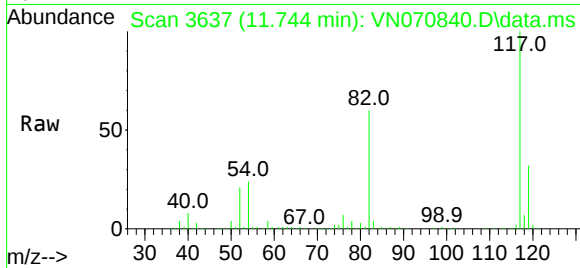

#67
Ethyl Benzene
Concen: 1.206 ug/l
RT: 11.843 min Scan# 3674
Delta R.T. 0.000 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00

Tgt Ion: 91 Resp: 66470
Ion Ratio Lower Upper
91 100
106 28.6 25.7 38.5




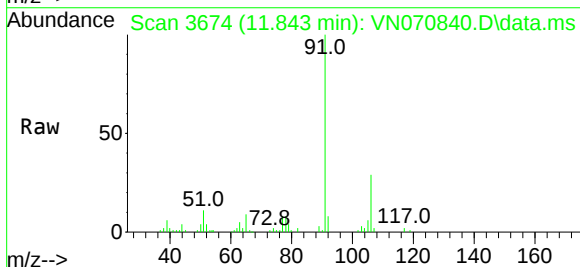


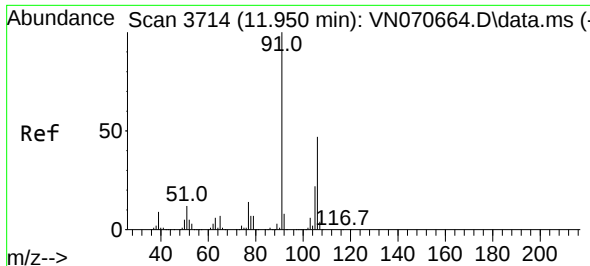

#68
m/p-Xylenes
Concen: 5.662 ug/l
RT: 11.948 min Scan# 31
Delta R.T. -0.002 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00




Instrument :
MSVOA_N
ClientSampleId :
CC-5


Tgt Ion:106 Resp: 113511
Ion Ratio Lower Upper
106 100
91 215.1 160.6 240.8

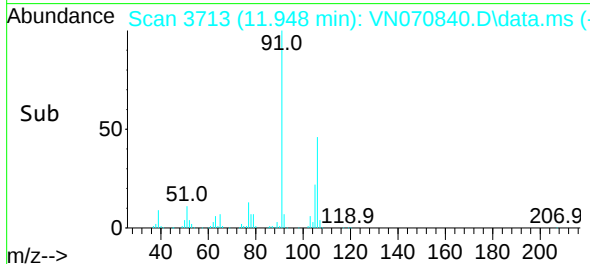

#69
o-Xylene
Concen: 2.580 ug/l
RT: 12.280 min Scan# 3837
Delta R.T. 0.002 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00

Tgt Ion:106 Resp: 51323
Ion Ratio Lower Upper
106 100
91 224.5 105.8 317.3


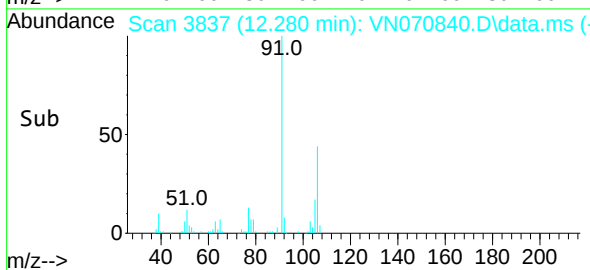

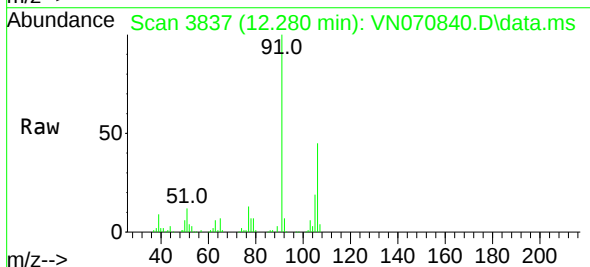


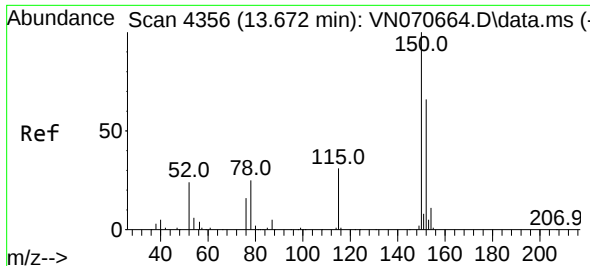

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 41
Delta R.T. 0.003 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00




Instrument :
MSVOA_N
ClientSampleId :
CC-5


Tgt Ion:152 Resp: 575327
Ion Ratio Lower Upper
152 100
115 63.6 27.5 82.5
150 157.6 0.0 344.4

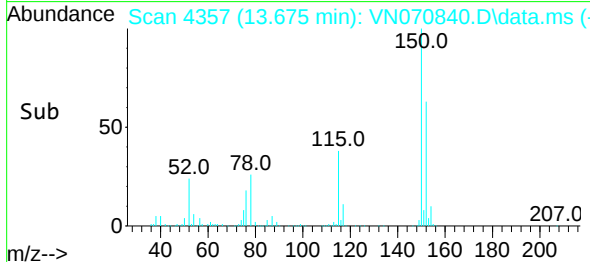

#73
Isopropylbenzene
Concen: 0.211 ug/l
RT: 12.583 min Scan# 3950
Delta R.T. 0.008 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00

Tgt Ion:105 Resp: 11496
Ion Ratio Lower Upper
105 100
120 27.1 13.4 40.1


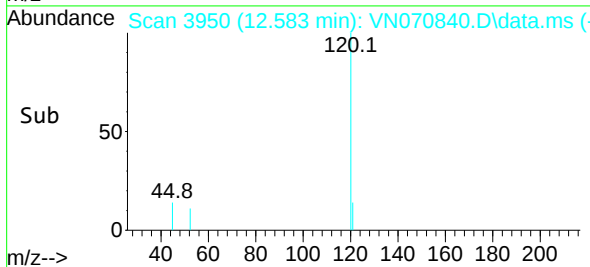

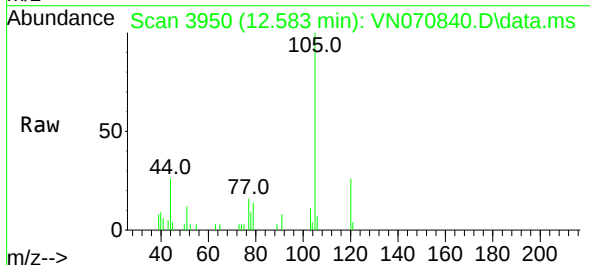


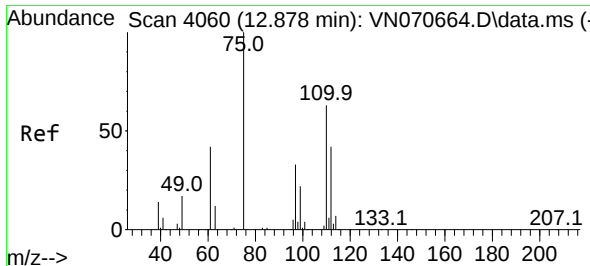

#76
1,2,3-Trichloropropane
Concen: 22.416 ug/l
RT: 12.731 min Scan# 4060
Delta R.T. -0.147 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00




Instrument :
MSVOA_N
ClientSampleId :
CC-5


Tgt Ion: 75 Resp: 342048
Ion Ratio Lower Upper
75 100
77 1.1 82.6 247.8#

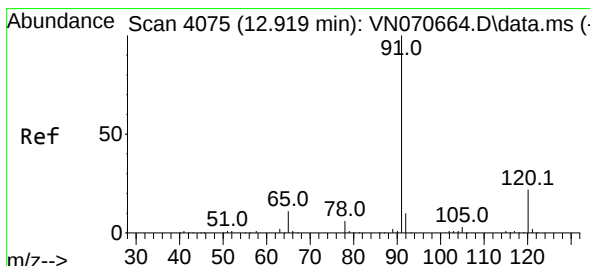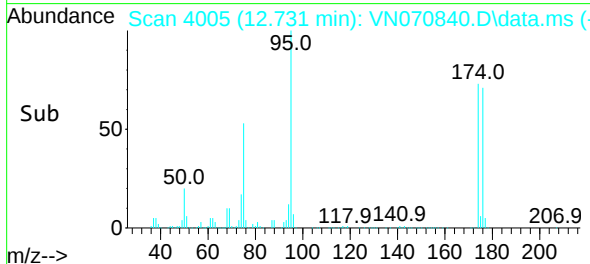

#78
n-propylbenzene
Concen: 0.351 ug/l
RT: 12.921 min Scan# 4076
Delta R.T. 0.002 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00

Tgt Ion: 91 Resp: 21376
Ion Ratio Lower Upper
91 100
120 21.1 11.9 35.9


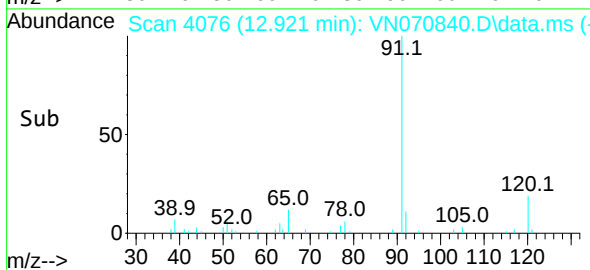

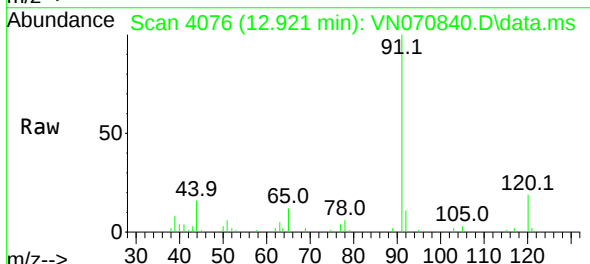




#79
2-Chlorotoluene
Concen: 0.390 ug/l
RT: 12.986 min Scan# 4107
Delta R.T. -0.018 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00




Instrument :
MSVOA_N
ClientSampleId :
CC-5


Tgt Ion: 91 Resp: 15028
Ion Ratio Lower Upper
91 100
126 0.0 18.3 54.8#

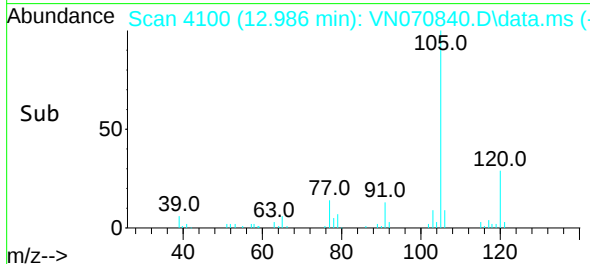

#80
1,3,5-Trimethylbenzene
Concen: 1.883 ug/l
RT: 13.058 min Scan# 4127
Delta R.T. 0.000 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00

Tgt Ion: 105 Resp: 82897
Ion Ratio Lower Upper
105 100
120 45.1 24.6 73.6


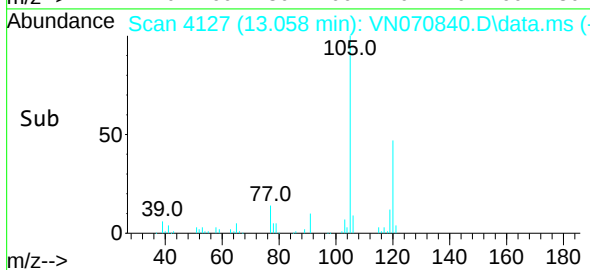

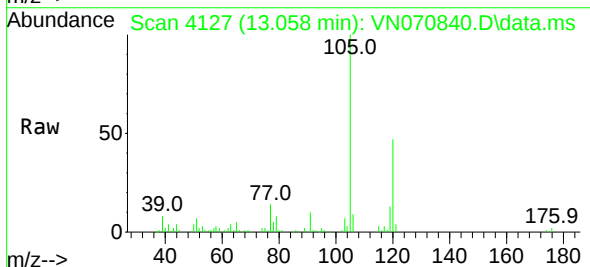


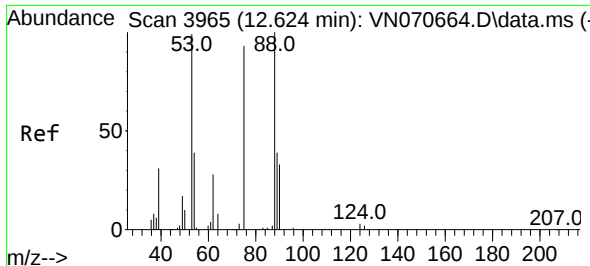

#81
trans-1,4-Dichloro-2-butene
Concen: 66.781 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.107 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00




Instrument :
MSVOA_N
ClientSampleId :
CC-5


Tgt Ion: 75 Resp: 342048
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 38.2 57.4#

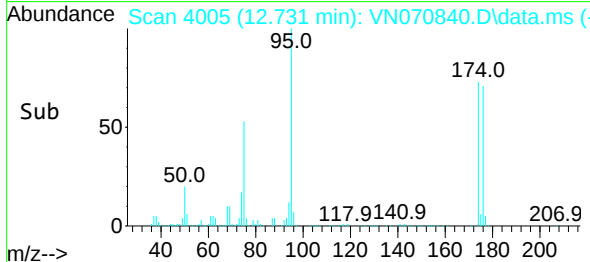

#82
4-Chlorotoluene
Concen: 0.271 ug/l
RT: 13.055 min Scan# 4126
Delta R.T. -0.049 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00

Tgt Ion: 91 Resp: 9759
Ion Ratio Lower Upper
91 100
126 0.0 18.2 54.6#


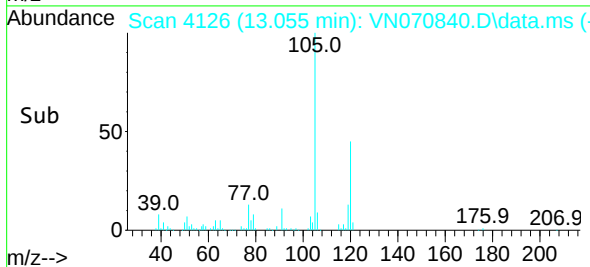

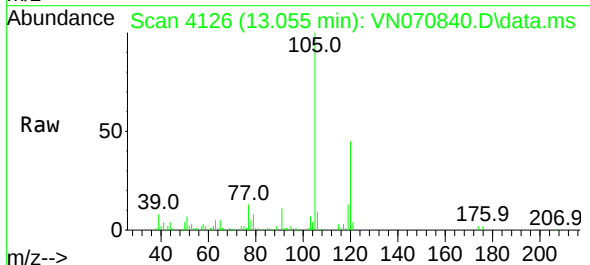




#84
1,2,4-Trimethylbenzene
Concen: 6.228 ug/l
RT: 13.367 min Scan# 41
Delta R.T. -0.001 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00




Instrument :
MSVOA_N
ClientSampleId :
CC-5


Tgt Ion:105 Resp: 263494
Ion Ratio Lower Upper
105 100
120 43.4 22.8 68.4

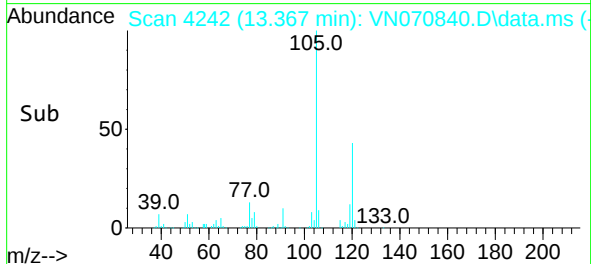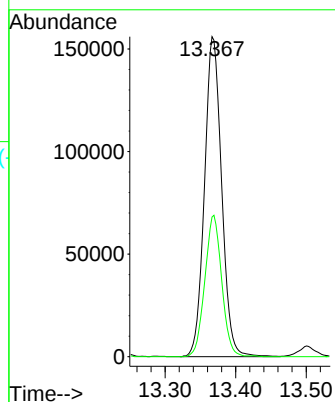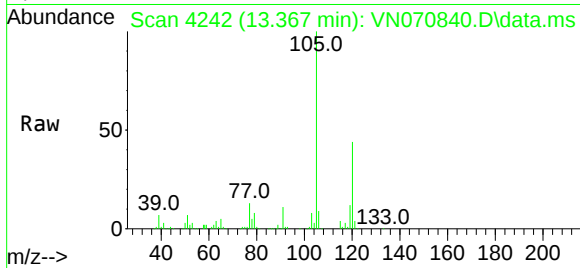

#86
p-Isopropyltoluene
Concen: 0.299 ug/l
RT: 13.616 min Scan# 4335
Delta R.T. 0.003 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00

Tgt Ion:119 Resp: 12217
Ion Ratio Lower Upper
119 100
134 25.3 13.6 40.7
91 22.5 11.4 34.1


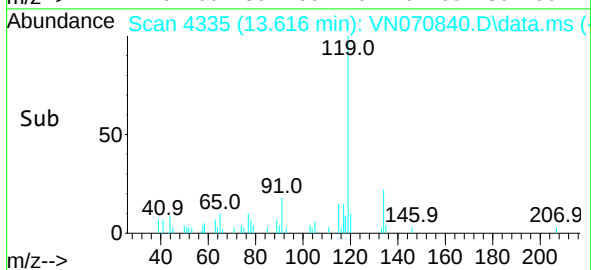
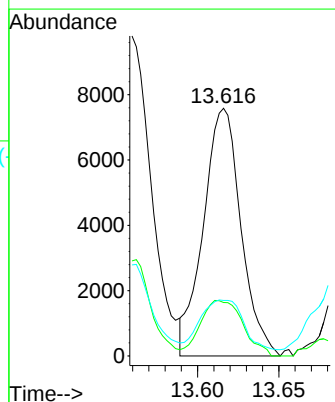
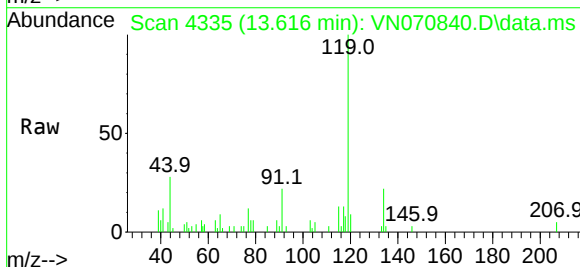




#90
Hexachloroethane
Concen: 0.412 ug/l
RT: 14.214 min Scan# 4558
Delta R.T. 0.005 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00




Instrument :
MSVOA_N
ClientSampleId :
CC-5


Tgt Ion:117 Resp: 2945
Ion Ratio Lower Upper
117 100
201 0.0 43.9 131.6#

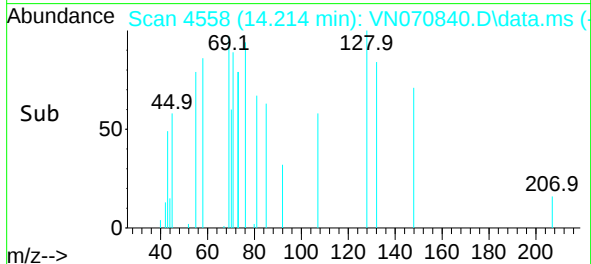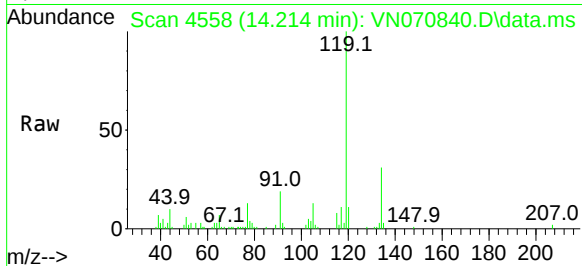

#93
1,2,4-Trichlorobenzene
Concen: 3.444 ug/l
RT: 15.257 min Scan# 4947
Delta R.T. -0.006 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00

Tgt Ion:180 Resp: 219
Ion Ratio Lower Upper
180 100
182 104.6 48.3 144.9
145 870.8 14.5 43.5#


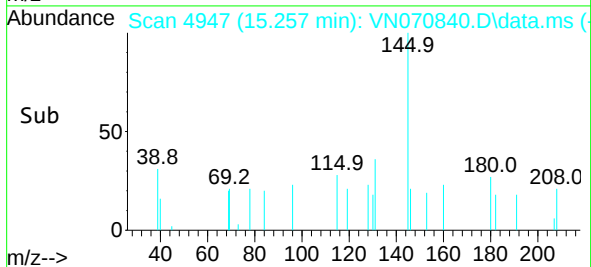

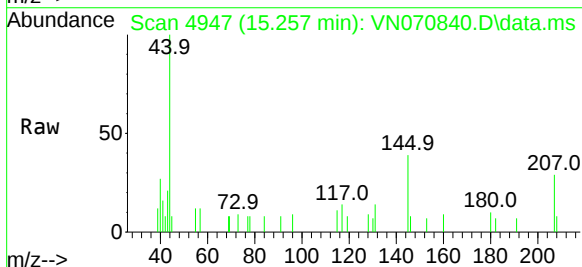


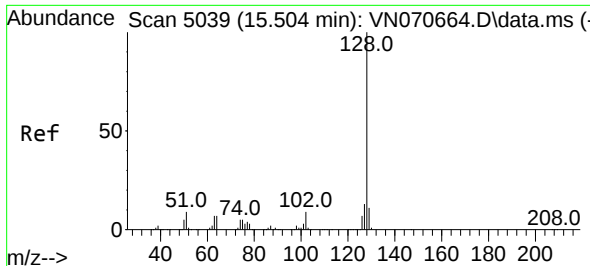

#95
Naphthalene
Concen: 8.440 ug/l
RT: 15.507 min Scan# 5039
Delta R.T. 0.003 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00

Instrument :
MSVOA_N
ClientSampleId :
CC-5

Tgt Ion:128 Resp: 115609
Ion Ratio Lower Upper
128 100
127 13.2 10.5 15.7
129 11.1 8.7 13.1

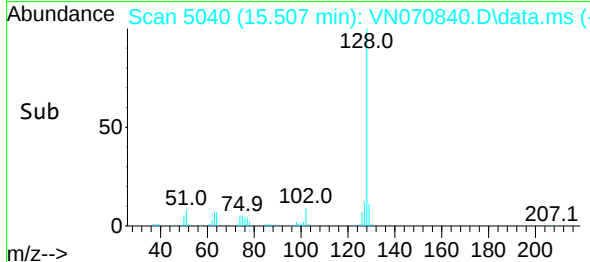

#96
1,2,3-Trichlorobenzene
Concen: 3.224 ug/l
RT: 15.697 min Scan# 5111
Delta R.T. 0.000 min
Lab File: VN070840.D
Acq: 28 Jan 2022 20:00

Tgt Ion:180 Resp: 91
Ion Ratio Lower Upper
180 100
182 203.3 47.4 142.2#
145 389.0 15.0 45.1#

