


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012822\
 Data File : VN070817.D
 Acq On : 28 Jan 2022 9:46
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011822W.M
 Title : SW846 8260
 Last Update : Tue Jan 18 13:32:07 2022

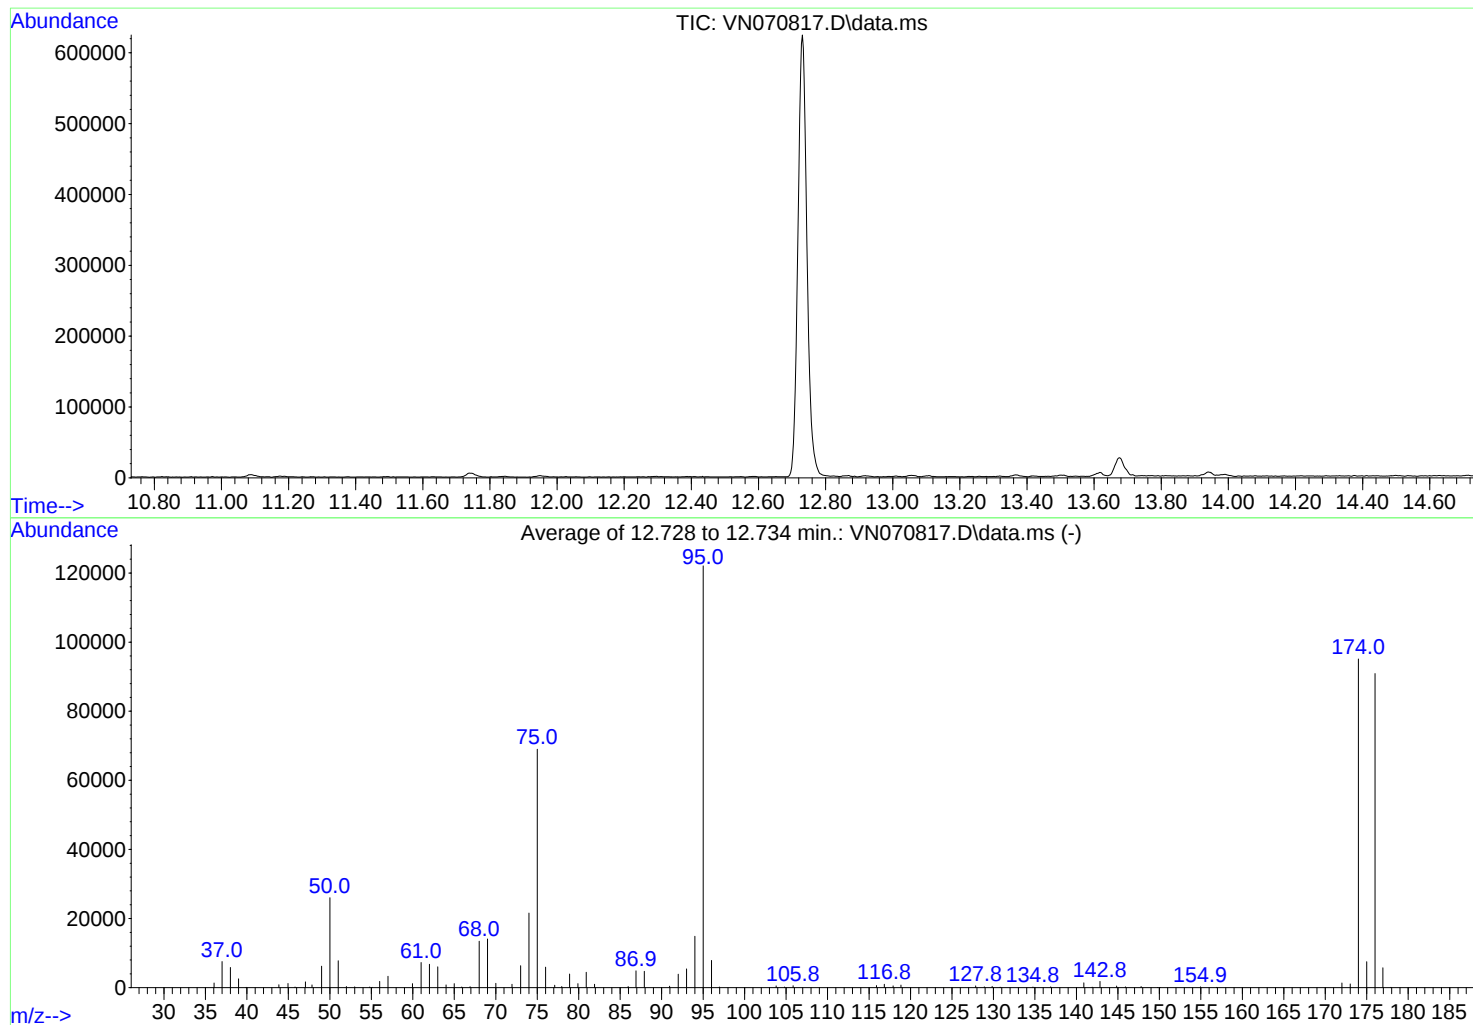

AutoFind: Scans 4004, 4005, 4006; Background Corrected with Scan 3986

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	26043	PASS
75	95	30	60	56.5	68984	PASS
95	95	100	100	100.0	122075	PASS
96	95	5	9	6.5	7890	PASS
173	174	0.00	2	1.1	1050	PASS
174	95	50	100	77.9	95131	PASS
175	174	5	9	7.9	7522	PASS
176	174	95	101	95.6	90912	PASS
177	176	5	9	6.3	5755	PASS