
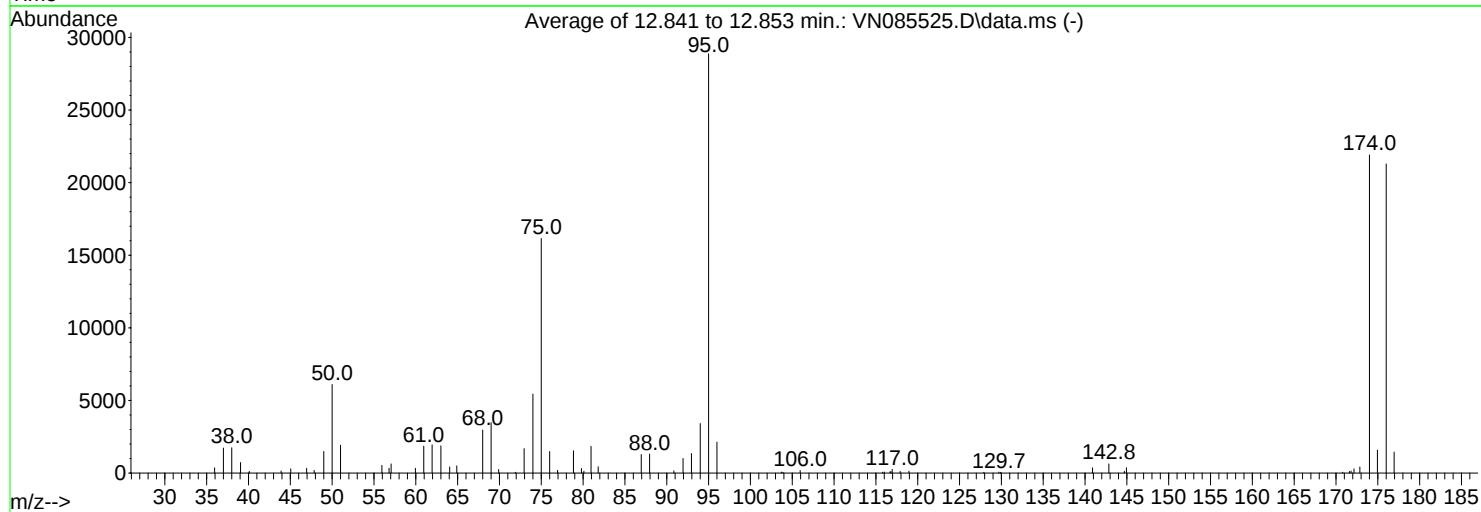


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012825\
Data File : VN085525.D
Acq On : 28 Jan 2025 09:17
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
Title : SW846 8260
Last Update : Wed Jan 15 02:16:08 2025

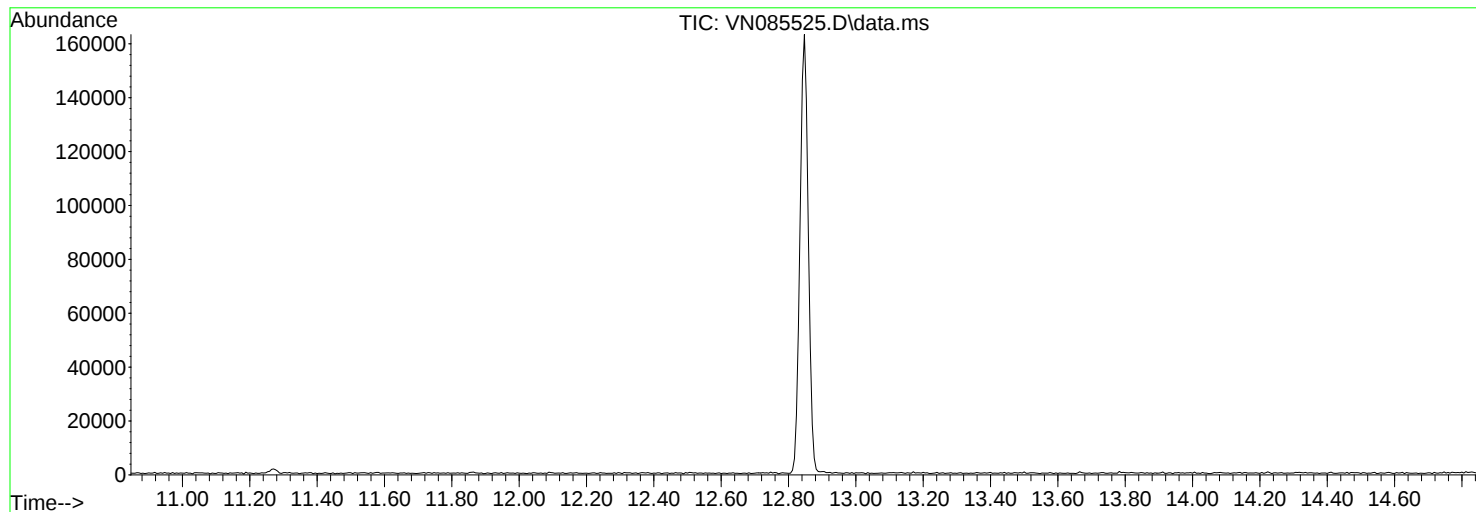

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	6102	PASS
75	95	30	60	55.9	16153	PASS
95	95	100	100	100.0	28877	PASS
96	95	5	9	7.4	2133	PASS
173	174	0.00	2	1.9	424	PASS
174	95	50	100	75.9	21904	PASS
175	174	5	9	7.2	1583	PASS
176	174	95	101	97.2	21288	PASS
177	176	5	9	6.8	1447	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	363	51.00	1921	69.00	3472	80.95	1841
37.00	1726	55.95	530	69.90	245	81.80	440
38.00	1741	56.80	336	71.90	57	86.95	1278
39.05	725	57.05	630	72.95	1686	87.95	1312
40.10	118	59.95	329	74.00	5442	90.85	154
43.90	145	60.95	1853	75.00	16153	91.95	1004
45.05	294	61.95	1942	76.00	1483	92.95	1350
46.95	330	63.00	1876	76.95	185	94.00	3411
47.85	189	64.05	424	78.85	1535	95.00	28877
49.00	1492	64.90	496	79.80	317	96.00	2133
50.00	6102	68.00	2970	80.10	130	103.70	73

Average of 12.841 to 12.853 min.: VN085525.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
103.90	55	129.90	51	174.95	1583		
105.95	177	140.90	363	176.00	21288		
115.80	56	142.85	633	176.95	1447		
116.00	75	144.70	122				
116.70	104	144.95	371				
116.80	97	170.80	59				
116.95	261	171.60	114				
117.90	119	171.80	147				
118.95	137	172.15	294				
127.90	52	172.85	424				
129.70	69	174.00	21904				

Instrument :

MSVOA_N

ClientSampleId :

BFB