
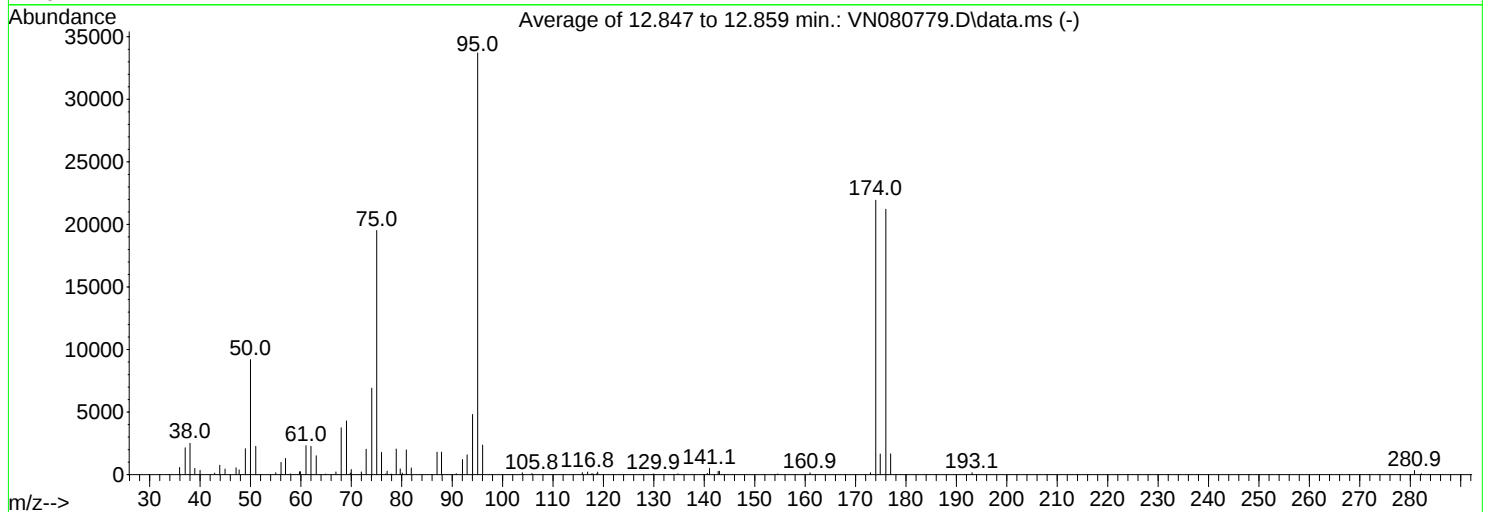


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012924\
Data File : VN080779.D
Acq On : 29 Jan 2024 09:00
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012924W.M
Title : SW846 8260
Last Update : Mon Jan 29 12:54:23 2024

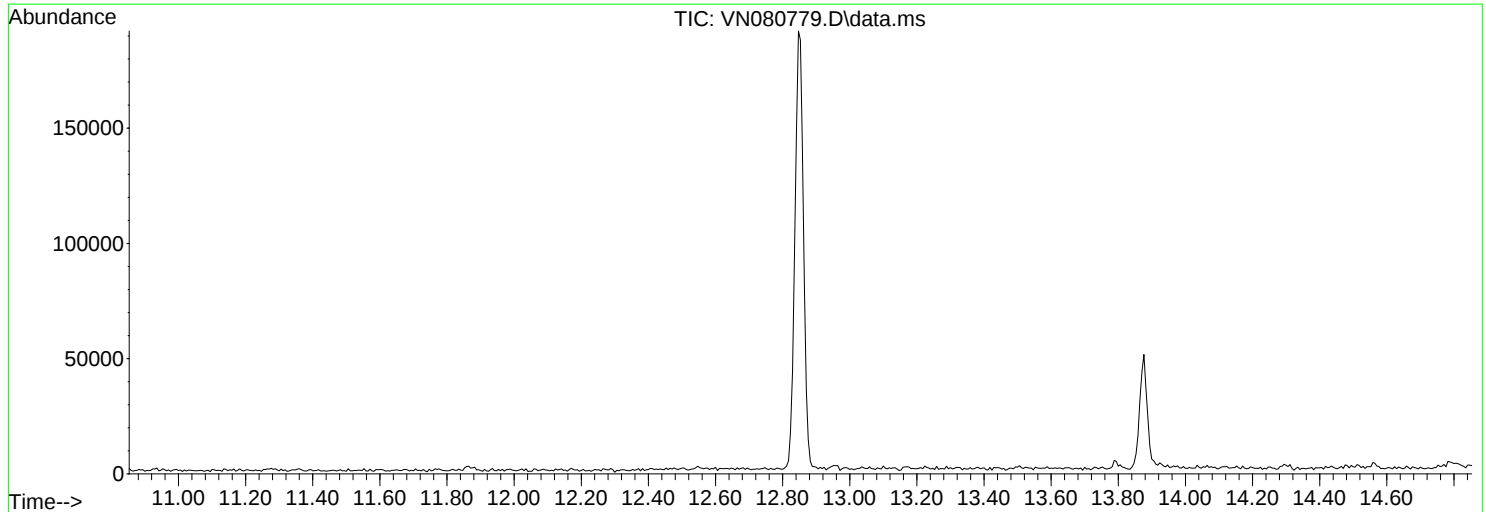

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	27.3	9199	PASS
75	95	30	60	57.9	19512	PASS
95	95	100	100	100.0	33717	PASS
96	95	5	9	7.0	2373	PASS
173	174	0.00	2	0.7	150	PASS
174	95	50	100	65.0	21931	PASS
175	174	5	9	7.5	1645	PASS
176	174	95	101	96.8	21221	PASS
177	176	5	9	7.8	1664	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	573	50.00	9199	64.90	56	76.80	51
37.05	2146	51.05	2270	66.95	221	77.10	281
38.00	2509	55.00	154	68.00	3753	77.90	5
38.95	503	56.05	981	69.05	4294	78.90	205
40.00	347	56.95	1288	69.80	126	79.70	464
42.90	123	57.90	58	70.00	410	80.10	135
43.90	754	59.70	231	72.00	217	80.90	1985
44.95	449	59.90	246	72.95	2029	81.90	538
47.15	551	61.00	2313	74.05	6923	87.00	1807
47.75	379	62.00	2259	75.05	19512	87.90	1810
49.00	2068	63.05	1506	76.00	1782	90.80	82

Average of 12.847 to 12.859 min.: VN080779.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.05	1214	118.60	60	174.00	21931		
92.95	1582	118.85	204	174.90	1645		
94.05	4804	129.90	64	176.00	21221		
95.05	33717	134.80	75	176.95	1664		
96.05	2373	140.60	108	193.10	148		
103.90	149	141.05	496	280.85	331		
105.80	91	142.75	268	282.20	63		
115.80	167	143.00	274				
116.85	209	154.60	59				
117.60	64	160.95	136				
117.90	79	172.95	150				

Instrument :

MSVOA_N

ClientSampleId :

BFB