
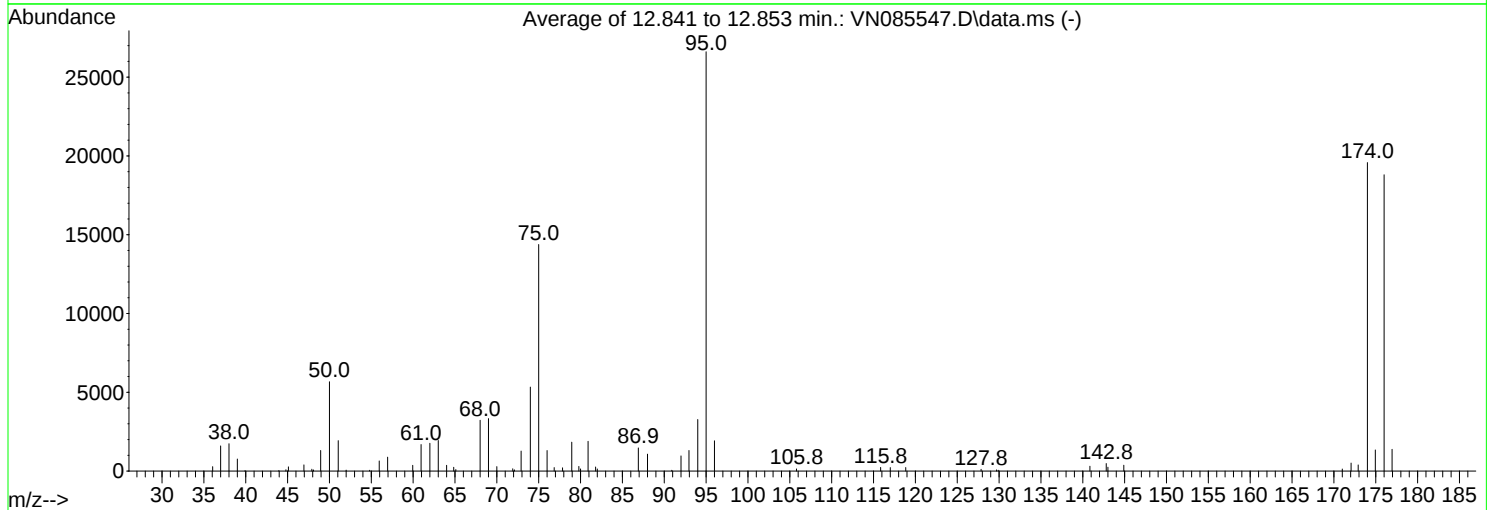


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN012925\
Data File : VN085547.D
Acq On : 29 Jan 2025 10:35
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
Title : SW846 8260
Last Update : Wed Jan 15 02:16:08 2025

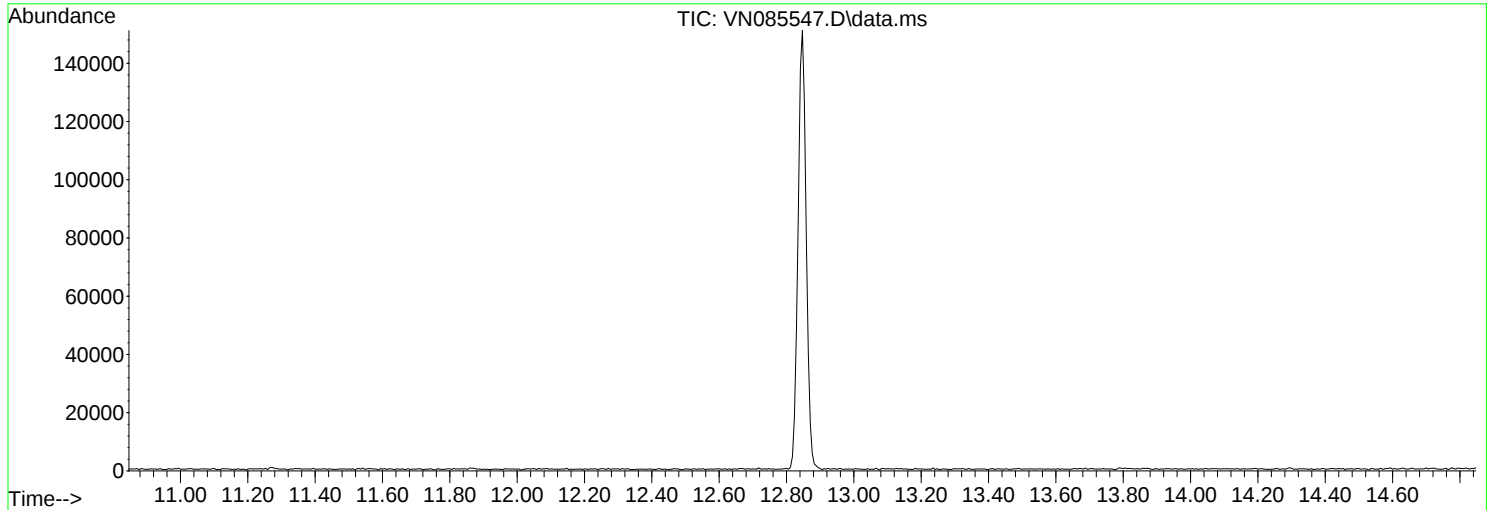

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	5669	PASS
75	95	30	60	54.0	14378	PASS
95	95	100	100	100.0	26613	PASS
96	95	5	9	7.2	1922	PASS
173	174	0.00	2	2.0	389	PASS
174	95	50	100	73.6	19579	PASS
175	174	5	9	6.8	1340	PASS
176	174	95	101	96.0	18805	PASS
177	176	5	9	7.3	1380	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	280	48.95	1307	64.00	366	76.00	1303
37.00	1595	50.00	5669	64.85	240	76.85	221
38.00	1735	51.05	1930	65.10	98	77.85	208
39.00	764	52.00	60	68.00	3225	78.95	1834
39.90	14	54.80	51	69.00	3330	79.80	295
43.95	28	55.95	642	70.00	282	80.00	138
44.80	84	56.95	883	71.90	146	80.90	1889
45.10	267	59.95	366	72.10	75	81.80	259
46.95	394	60.95	1685	72.90	1271	82.00	133
47.90	120	62.00	1765	74.00	5331	86.90	1469
48.10	72	63.00	1941	75.00	14378	88.00	1074

Average of 12.841 to 12.853 min.: VN085547.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.90	53	129.70	76	176.00	18805		
92.00	962	129.90	53	176.95	1380		
92.95	1306	140.85	308				
94.00	3271	142.80	479				
95.00	26613	143.00	247				
96.00	1922	144.90	373				
105.80	137	171.00	132				
115.85	232	172.05	510				
117.00	221	172.90	389				
118.85	226	174.00	19579				
127.85	112	174.95	1340				

Instrument :

MSVOA_N

ClientSampleId :

BFB