



Dichlorodifluoromethane

Response Ratio

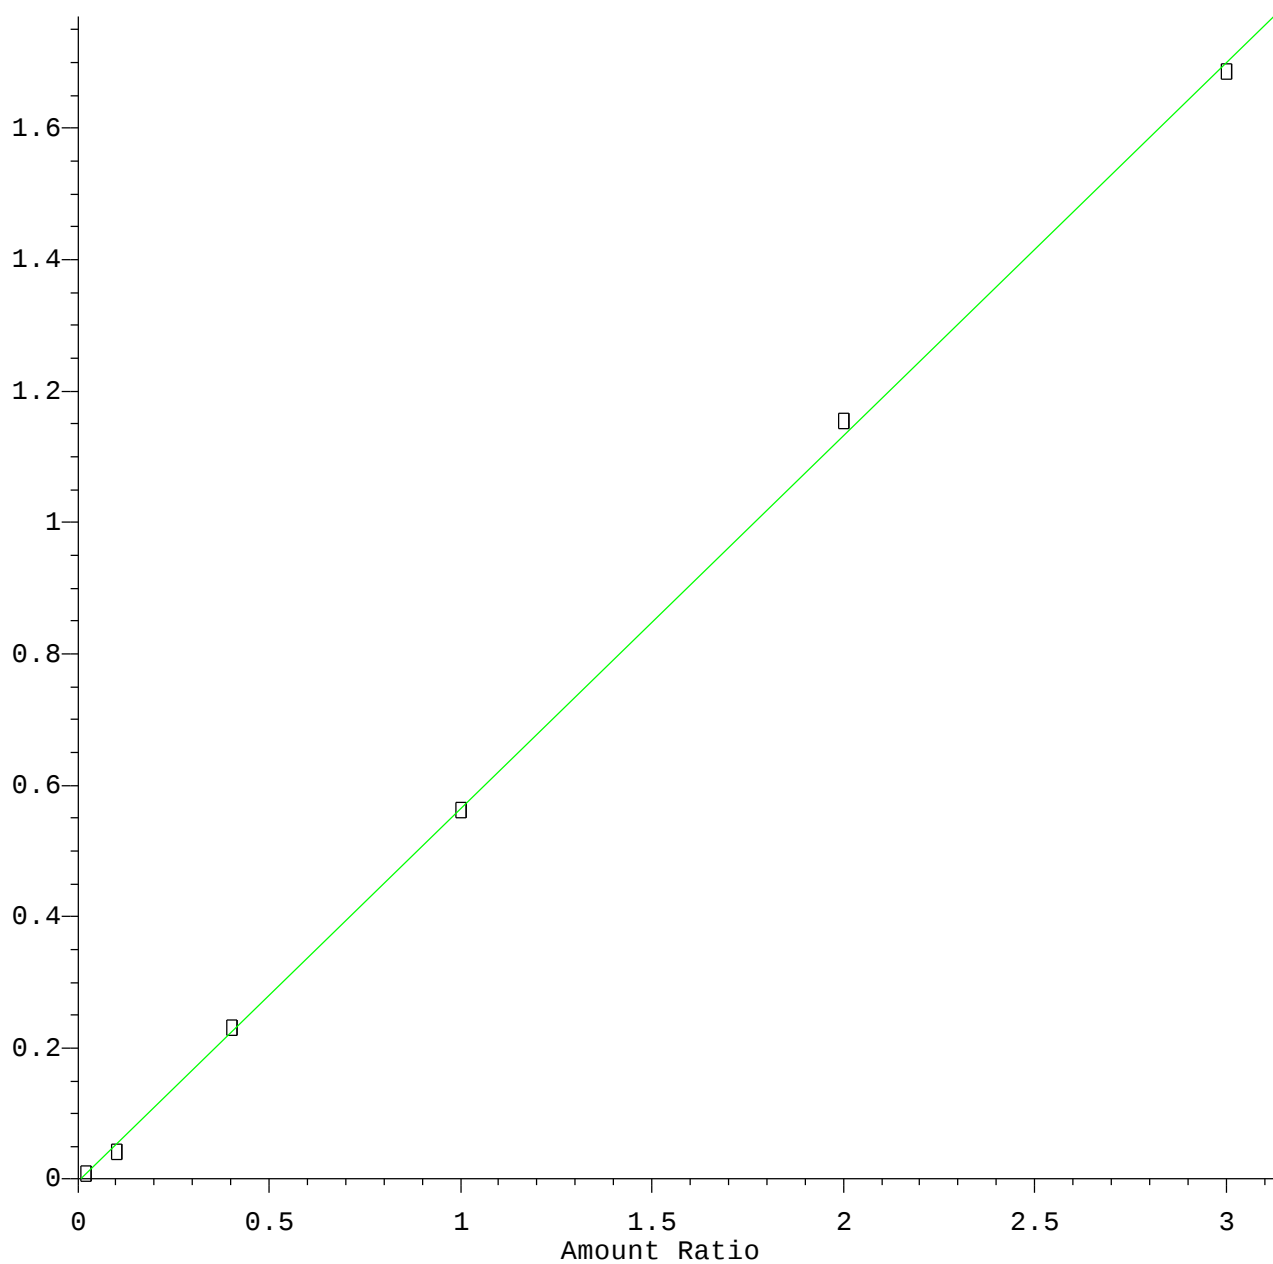


Resp Ratio = $5.68 \times 10^{-1} \times \text{Amt} - 3.83 \times 10^{-3}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N013019W.M
Calibration Table Last Updated: Fri Feb 01 09:11:52 2019

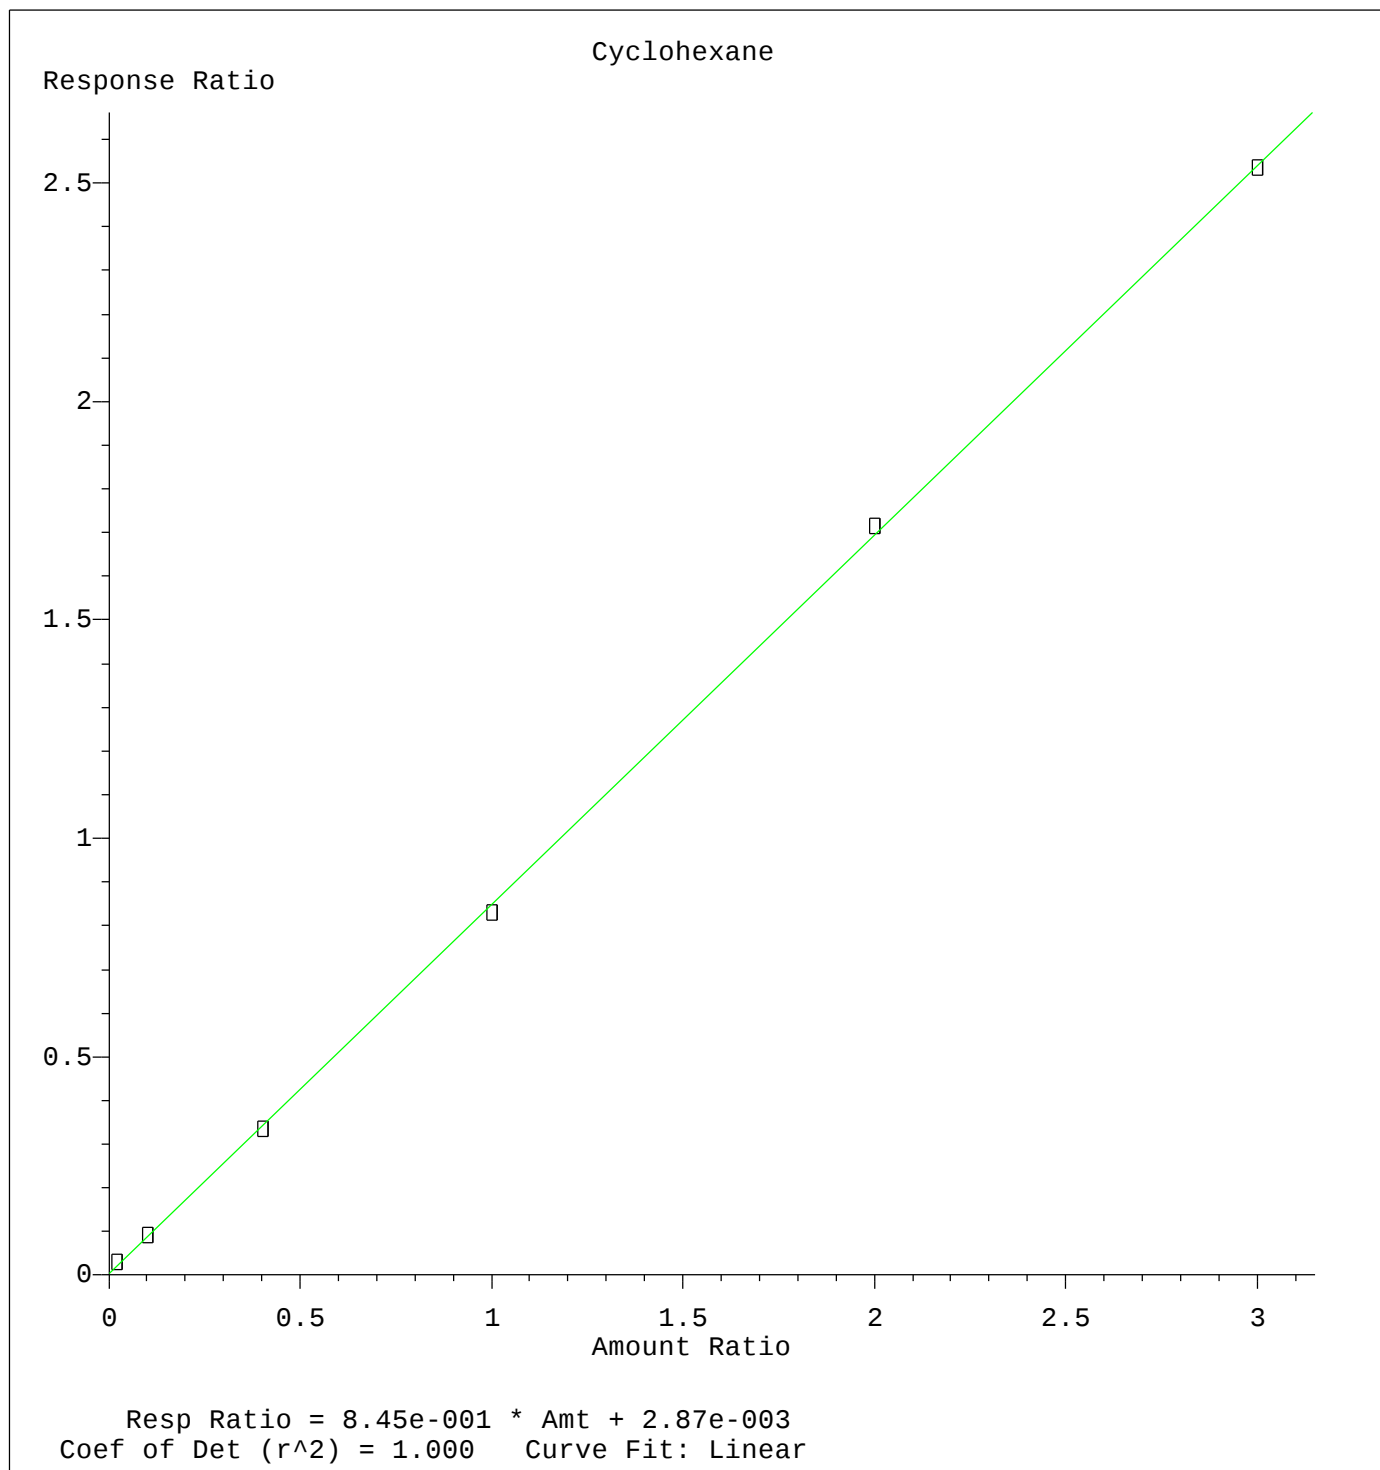


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N013019W.M
Calibration Table Last Updated: Fri Feb 01 09:11:52 2019

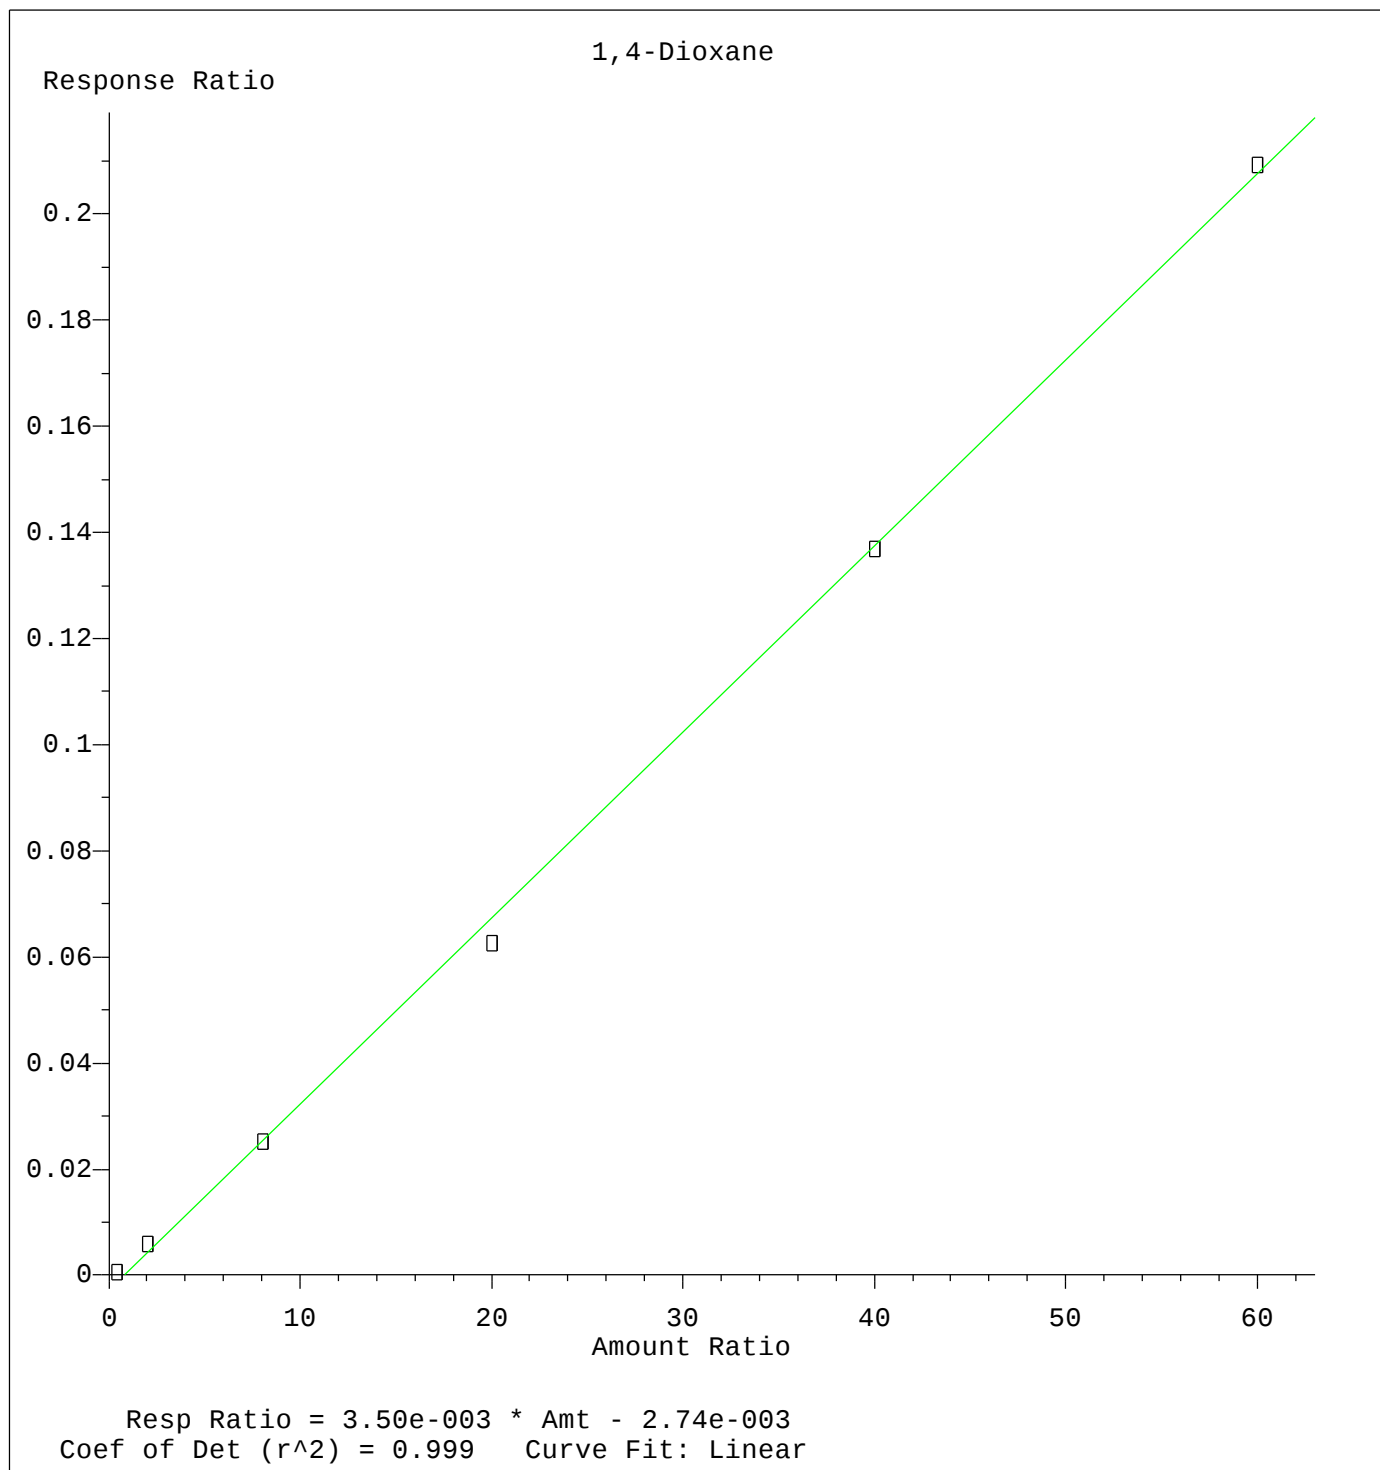

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N013019W.M
Calibration Table Last Updated: Fri Feb 01 09:11:52 2019

2-Chloroethyl Vinyl ether

Response Ratio

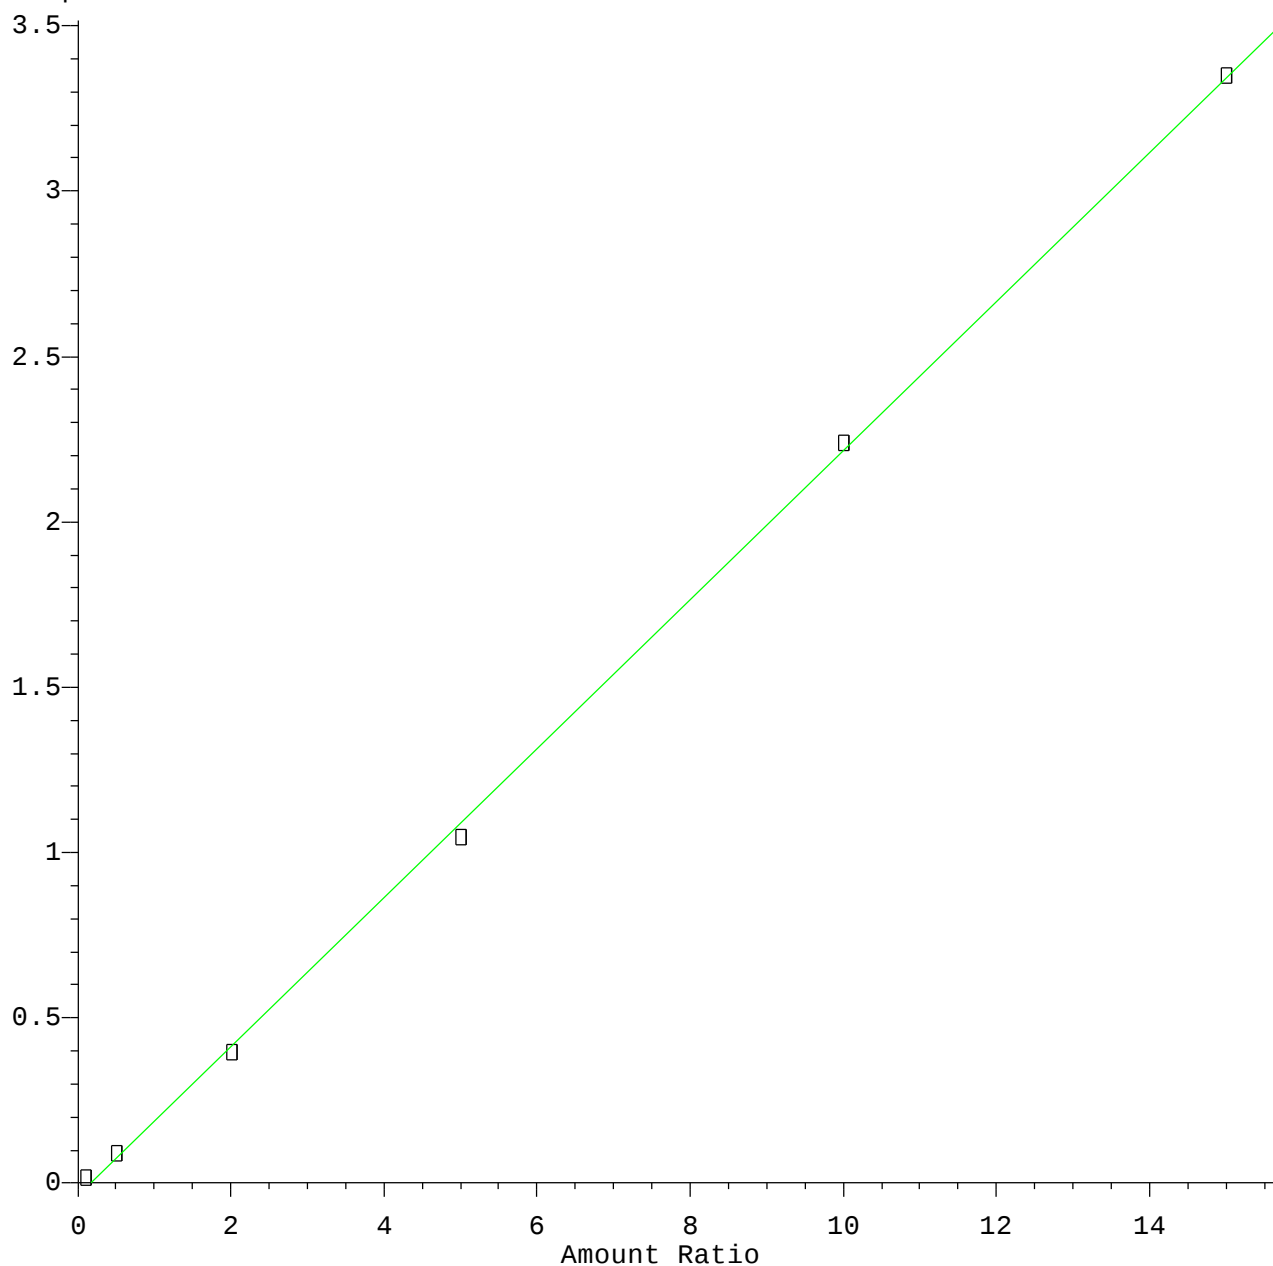


Resp Ratio = $2.25 \times 10^{-1} \times \text{Amt} - 3.61 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N013019W.M
Calibration Table Last Updated: Fri Feb 01 09:11:52 2019

Naphthalene

Response Ratio

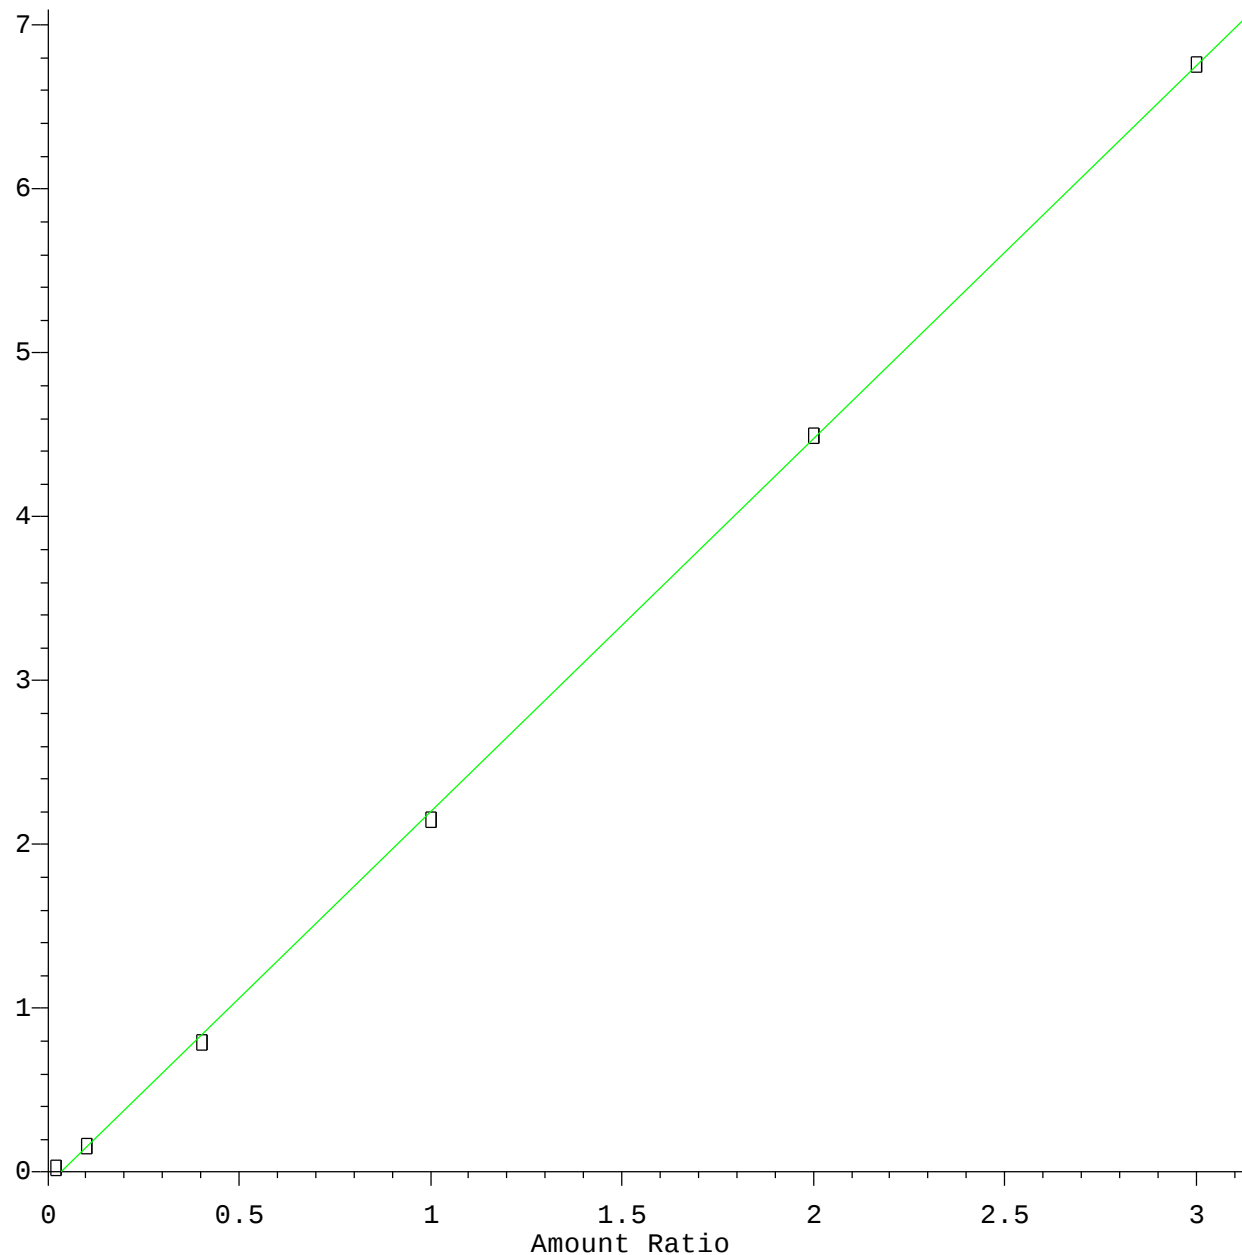

Resp Ratio = 2.28e+000 * Amt - 7.90e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N013019W.M
Calibration Table Last Updated: Fri Feb 01 09:11:52 2019