


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN013019\
 Data File : VN053557.D
 Acq On : 30 Jan 2019 8:21
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N013019W.M
 Title : SW846 8260
 Last Update : Fri Feb 01 09:11:52 2019

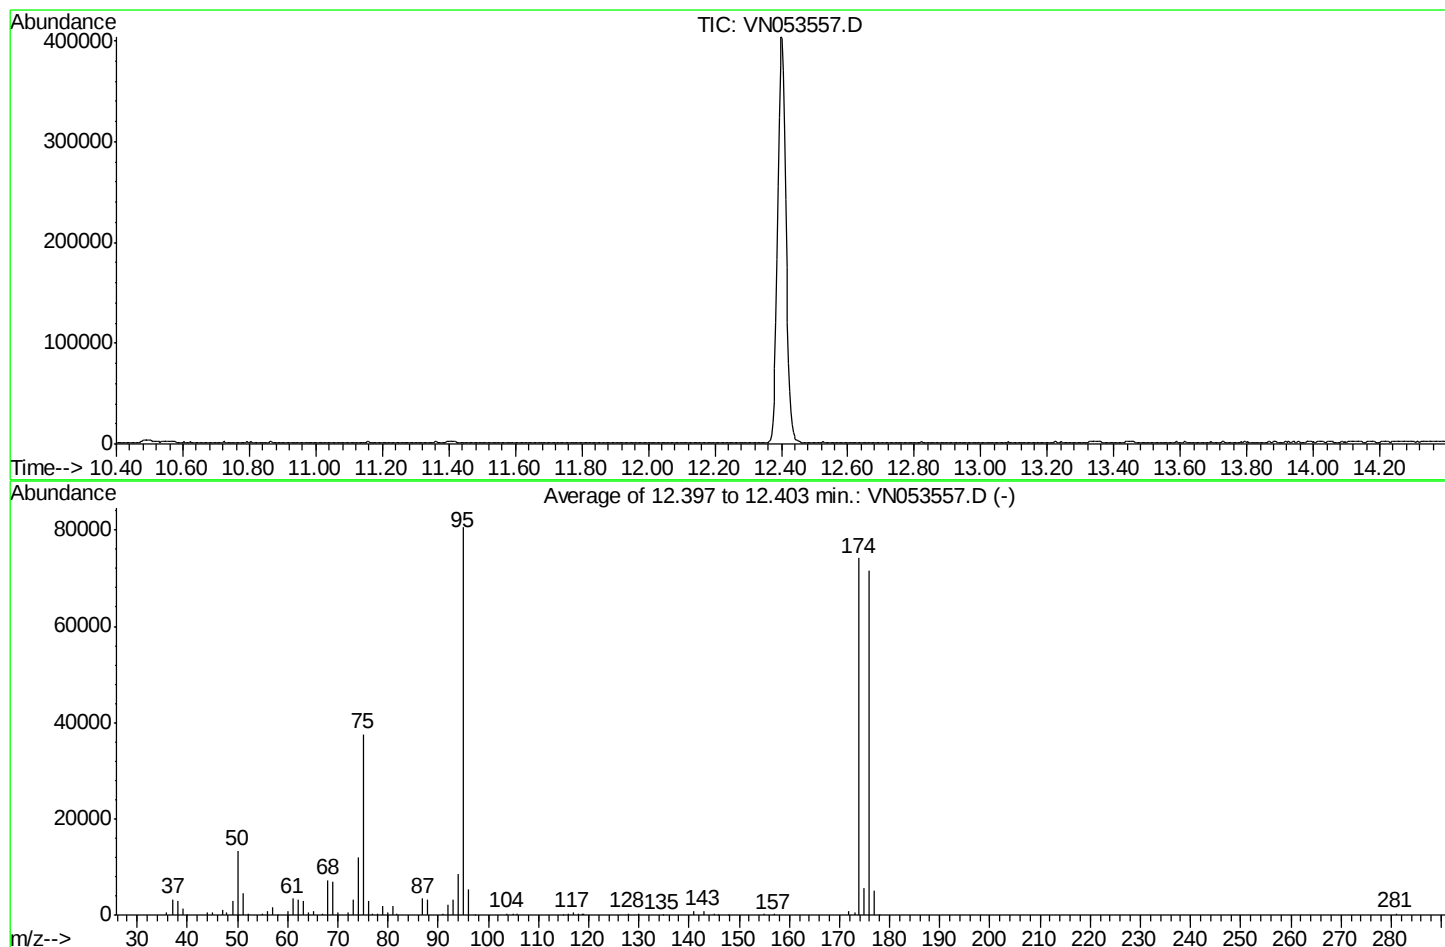

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	13345	PASS
75	95	30	60	46.7	37653	PASS
95	95	100	100	100.0	80578	PASS
96	95	5	9	6.5	5204	PASS
173	174	0.00	2	0.6	430	PASS
174	95	50	100	92.1	74216	PASS
175	174	5	9	7.6	5657	PASS
176	174	95	101	96.3	71498	PASS
177	176	5	9	7.0	5022	PASS