

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN013023\
 Data File : VN076456.D
 Acq On : 30 Jan 2023 14:53
 Operator : JC\MD
 Sample : PB150523ZHE#04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB150523ZHE#04

Quant Time: Jan 31 00:39:56 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 17 03:59:22 2023
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	456079	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	809078	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	692319	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	286625	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	286339	56.072	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	112.140%
35) Dibromofluoromethane	8.177	113	237273	46.882	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	93.760%
50) Toluene-d8	10.571	98	965672	51.664	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	103.320%
62) 4-Bromofluorobenzene	12.853	95	301797	49.460	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	98.920%
Target Compounds						
					Qvalue	
16) Acetone	4.453	43	32021	19.493	ug/l	92
20) Methylene Chloride	5.289	84	17570	3.062	ug/l	97
37) Ethyl Acetate	7.571	43	41993	7.311	ug/l	99
43) Isopropyl Acetate	8.694	43	482961	51.466	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN013023\
Data File : VN076456.D
Acq On : 30 Jan 2023 14:53
Operator : JC\MD
Sample : PB150523ZHE#04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB150523ZHE#04

Quant Time: Jan 31 00:39:56 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 17 03:59:22 2023
Response via : Initial Calibration




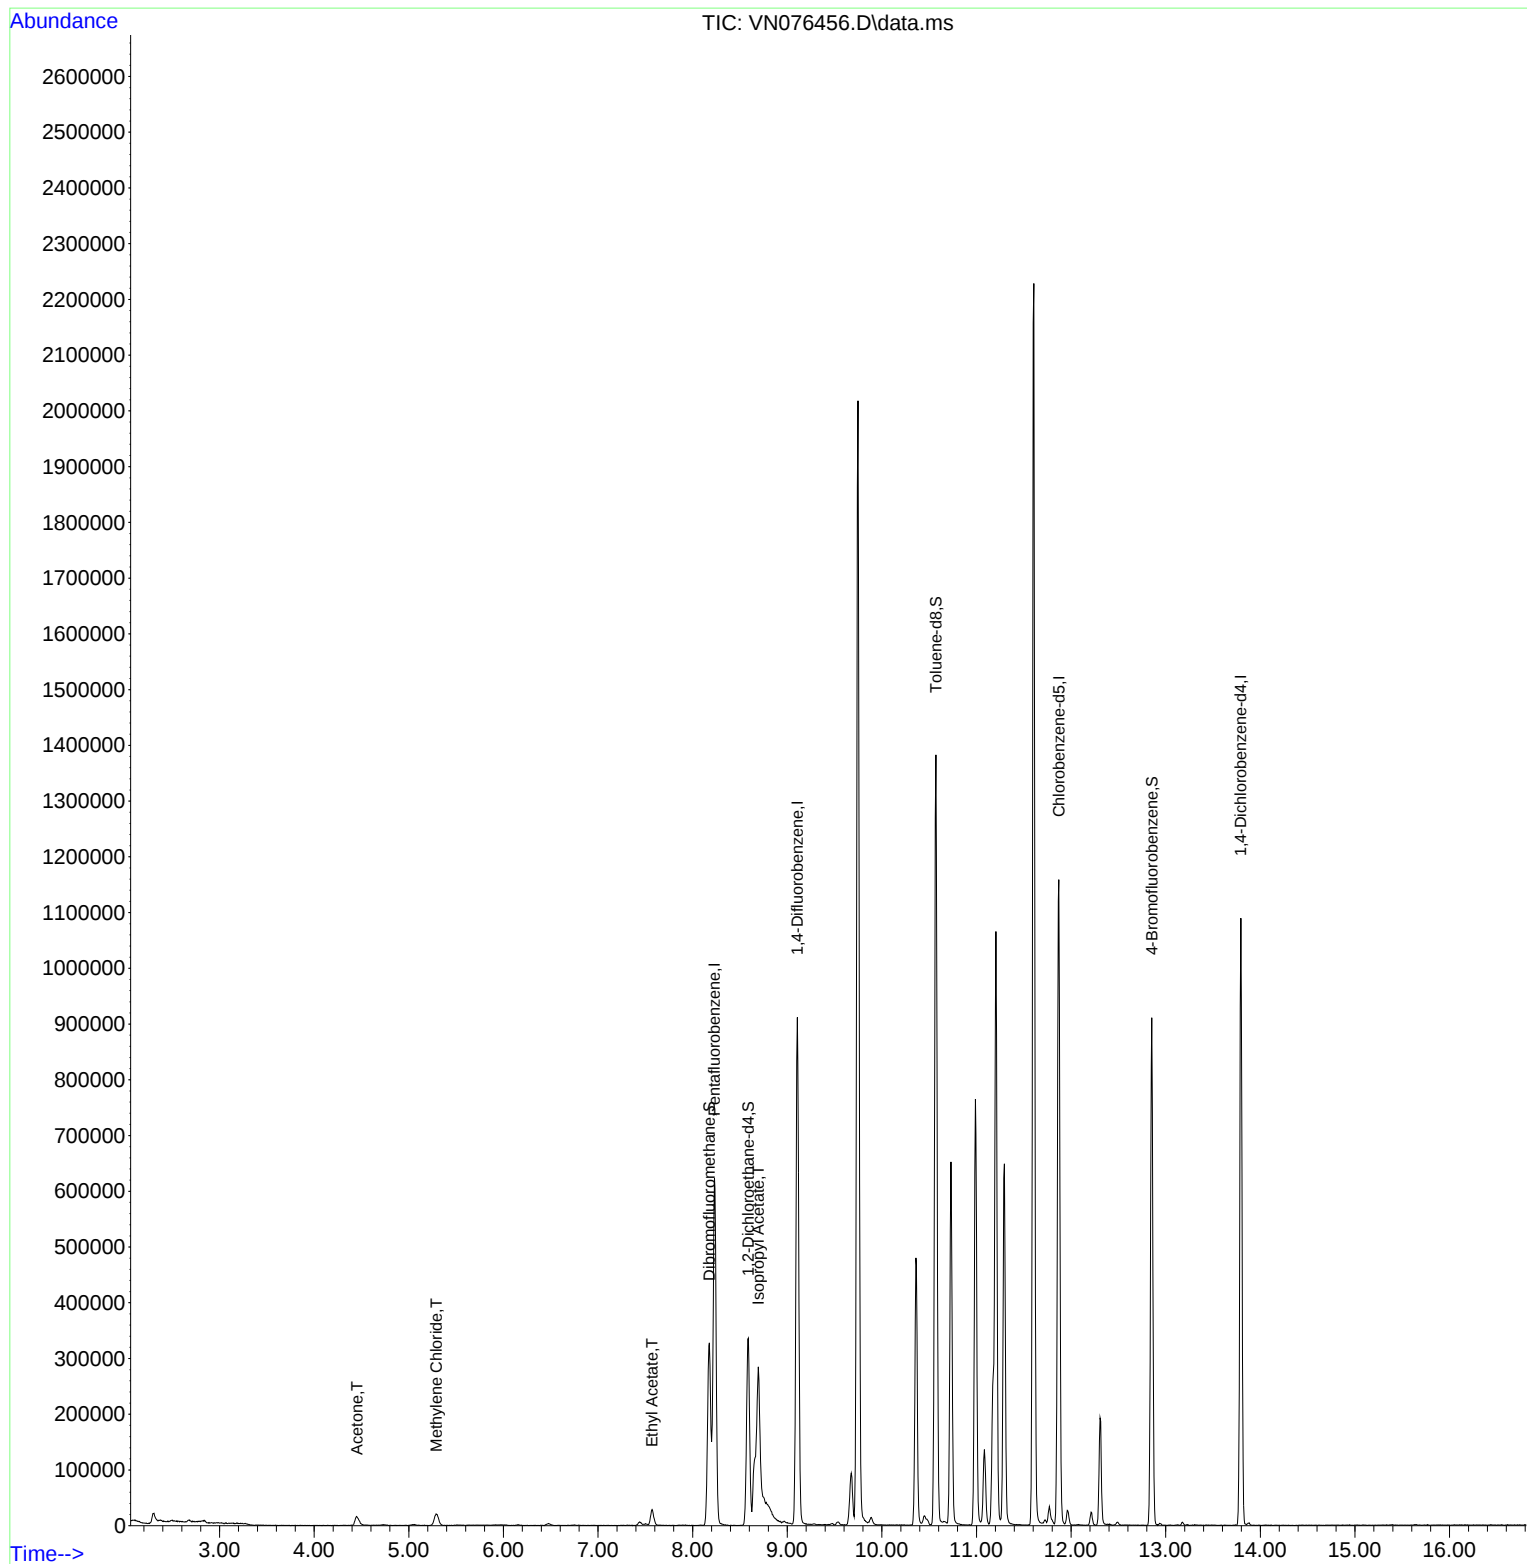


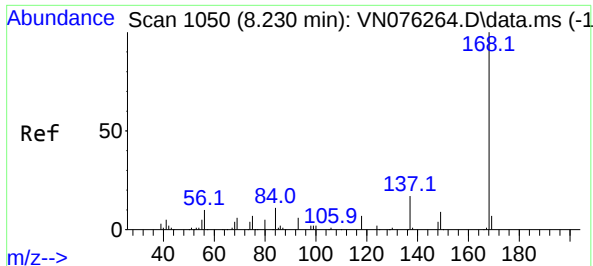

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1
Delta R.T. -0.000 min
Lab File: VN076456.D
Acq: 30 Jan 2023 14:53




Instrument :
MSVOA_N
ClientSampleId :
PB150523ZHE#04


Tgt Ion:168 Resp: 456079
Ion Ratio Lower Upper
168 100
99 58.9 41.6 62.4

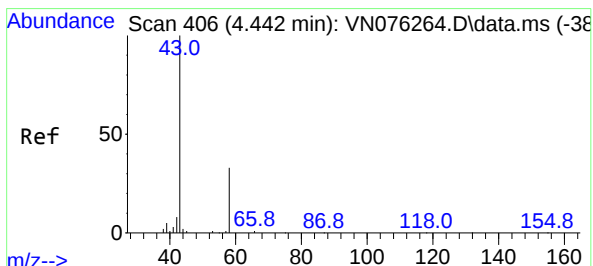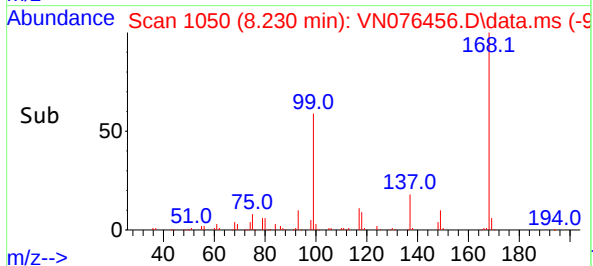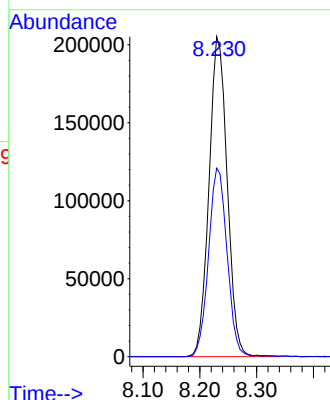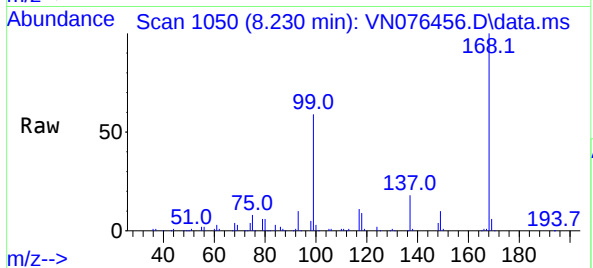

#16
Acetone
Concen: 19.493 ug/l
RT: 4.453 min Scan# 408
Delta R.T. 0.011 min
Lab File: VN076456.D
Acq: 30 Jan 2023 14:53


Tgt Ion: 43 Resp: 32021
Ion Ratio Lower Upper
43 100
58 28.8 26.7 40.1

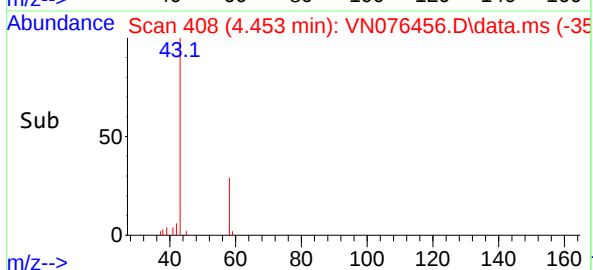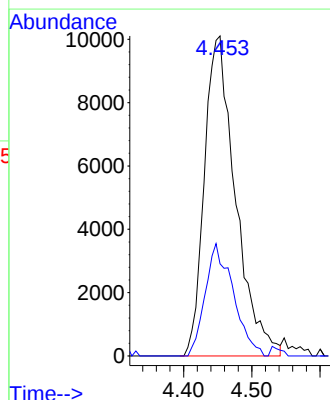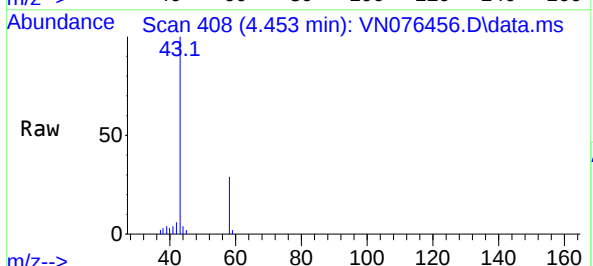

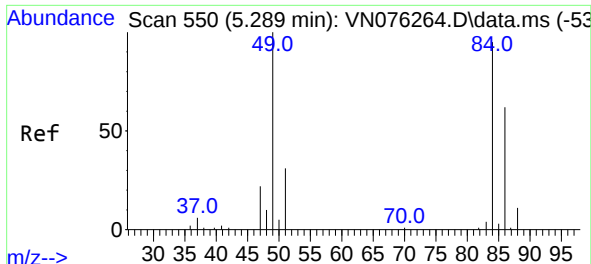




#20
Methylene Chloride
Concen: 3.062 ug/l
RT: 5.289 min Scan# 511
Delta R.T. -0.000 min
Lab File: VN076456.D
Acq: 30 Jan 2023 14:53

Instrument :
MSVOA_N
ClientSampleId :
PB150523ZHE#04

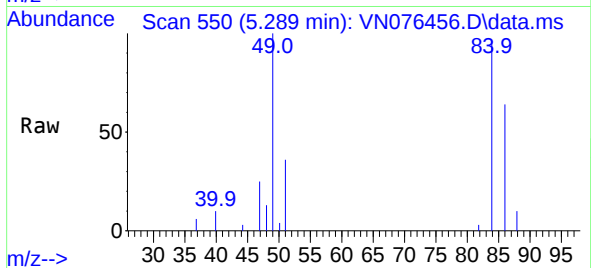

Tgt Ion: 84 Resp: 17570




Ion	Ratio	Lower	Upper
84	100		
49	103.8	84.5	126.7
51	36.9	26.0	39.0
86	66.9	52.0	78.0

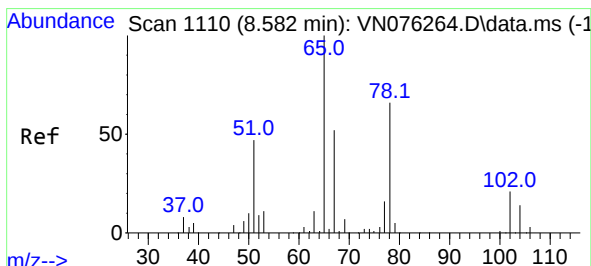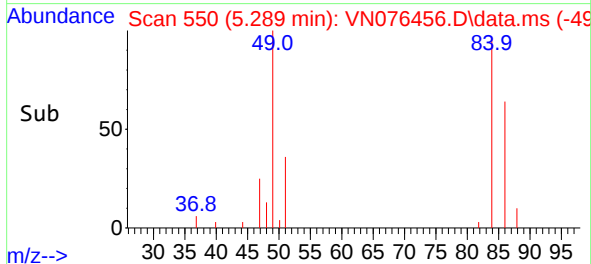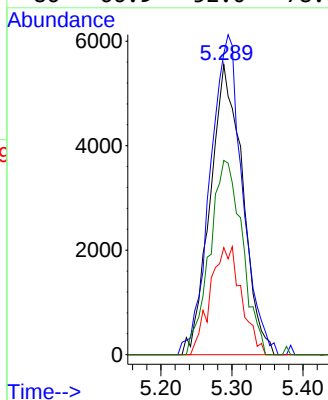


#33
1,2-Dichloroethane-d4
Concen: 56.072 ug/l
RT: 8.588 min Scan# 1111
Delta R.T. 0.006 min
Lab File: VN076456.D
Acq: 30 Jan 2023 14:53

Tgt Ion: 65 Resp: 286339

Ion	Ratio	Lower	Upper
65	100		
67	50.8	0.0	104.6

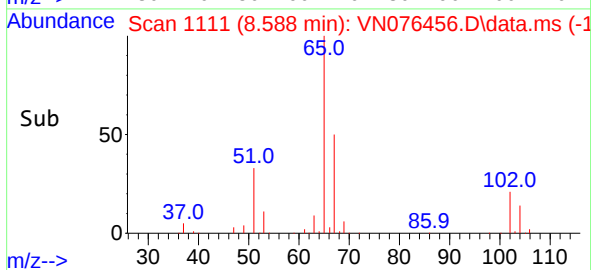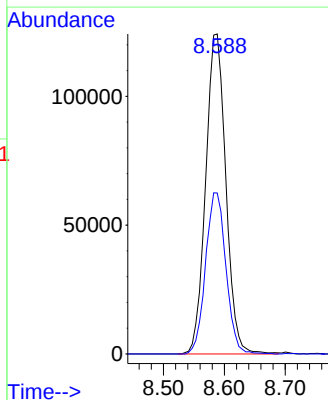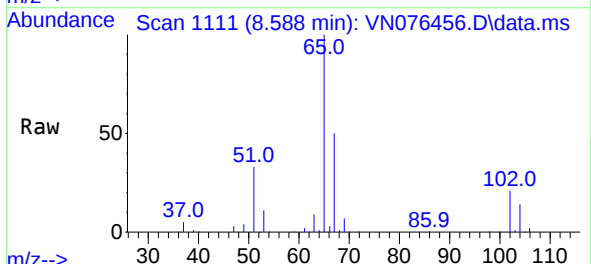

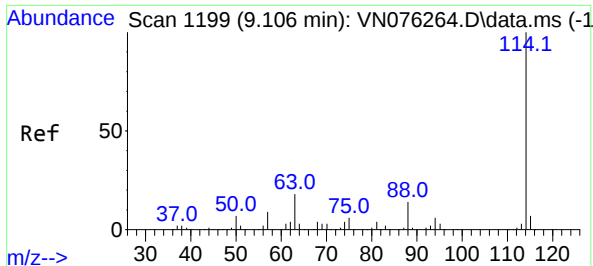

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1199

Delta R.T. -0.000 min

Lab File: VN076456.D

Acq: 30 Jan 2023 14:53

Instrument :

MSVOA_N

ClientSampleId :

PB150523ZHE#04





Tgt Ion:114 Resp: 809078

Ion Ratio Lower Upper

114 100

63 19.3 0.0 35.8

88 15.4 0.0 28.0

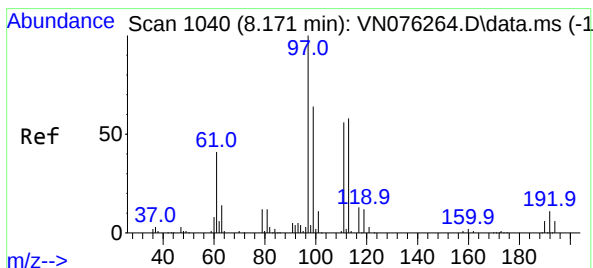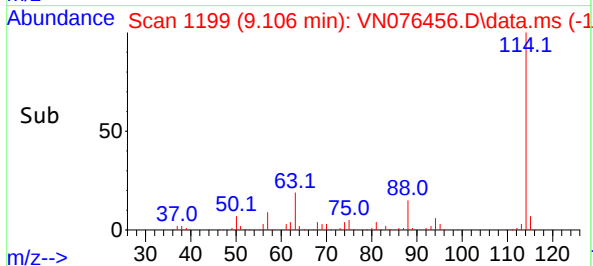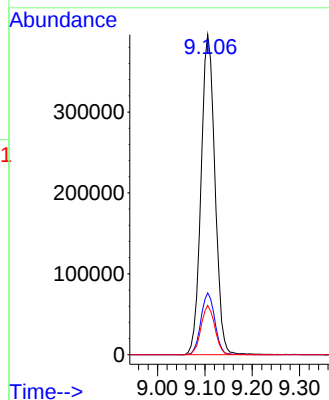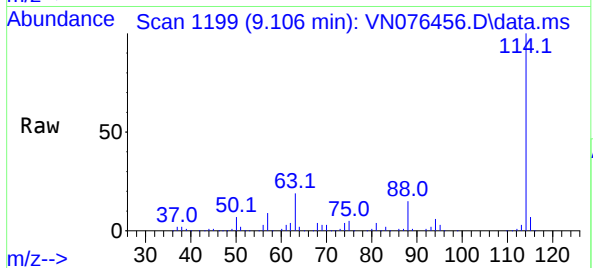

#35

Dibromofluoromethane

Concen: 46.882 ug/l

RT: 8.177 min Scan# 1041

Delta R.T. 0.006 min

Lab File: VN076456.D

Acq: 30 Jan 2023 14:53




Tgt Ion:113 Resp: 237273


Ion Ratio Lower Upper

113 100

111 101.3 82.7 124.1

192 18.5 15.6 23.4


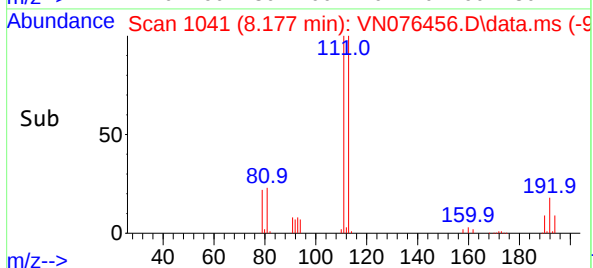
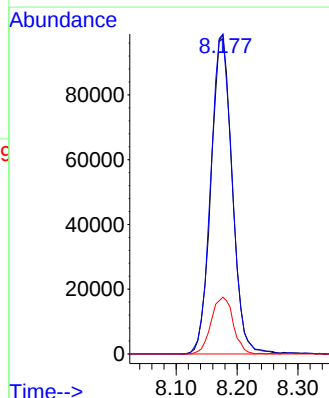
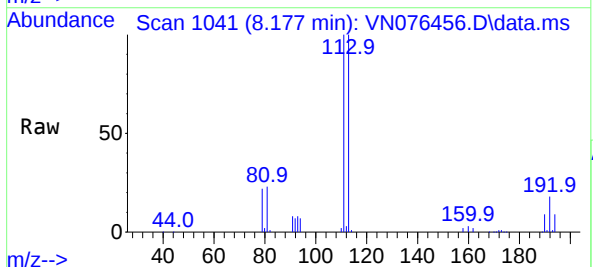


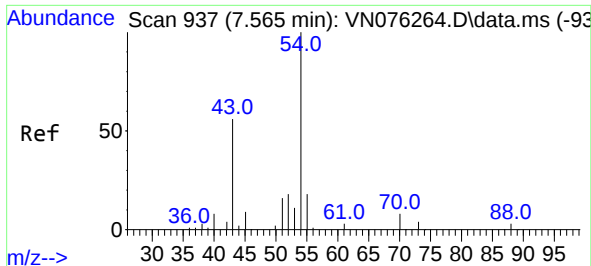

#37
Ethyl Acetate
Concen: 7.311 ug/l
RT: 7.571 min Scan# 91
Delta R.T. 0.006 min
Lab File: VN076456.D
Acq: 30 Jan 2023 14:53




Instrument :
MSVOA_N
ClientSampleId :
PB150523ZHE#04


Tgt Ion:	43	Resp:	41993
Ion	Ratio	Lower	Upper
43	100		
61	13.9	11.1	16.7
70	11.8	10.0	15.0

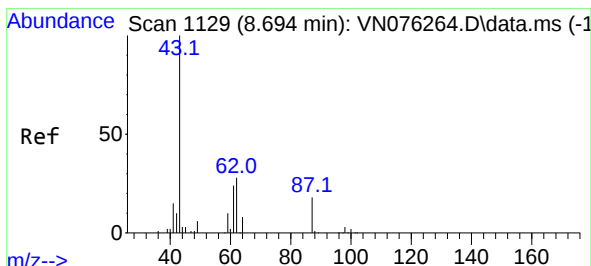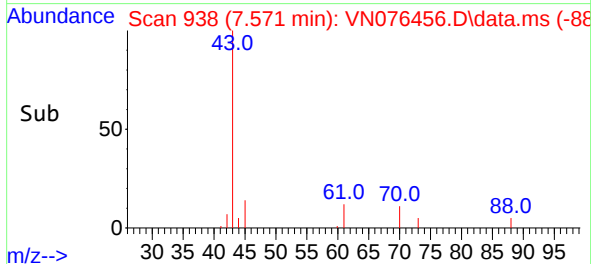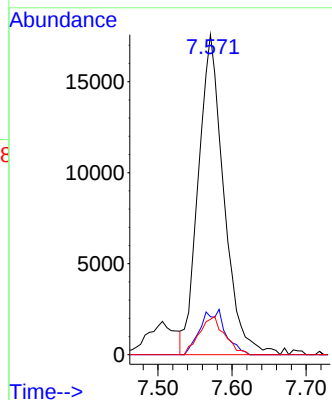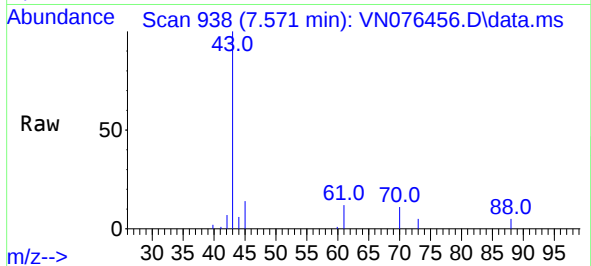

#43
Isopropyl Acetate
Concen: 51.466 ug/l
RT: 8.694 min Scan# 1129
Delta R.T. 0.000 min
Lab File: VN076456.D
Acq: 30 Jan 2023 14:53

Tgt Ion:	43	Resp:	482961
Ion	Ratio	Lower	Upper
43	100		
61	10.2	23.5	35.3#
87	7.4	13.8	20.6#


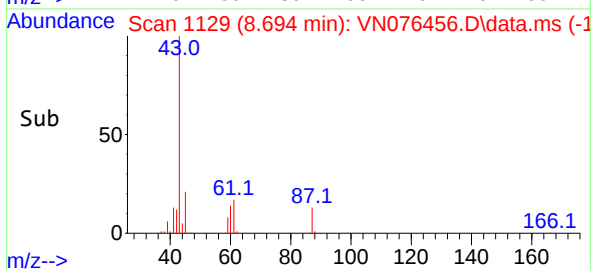
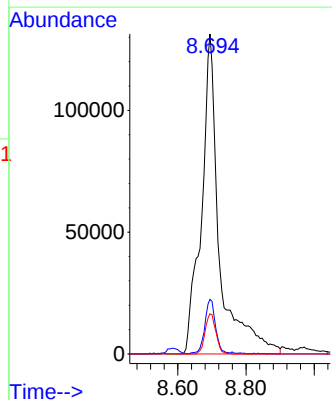
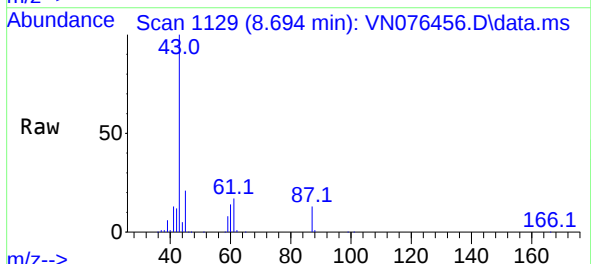


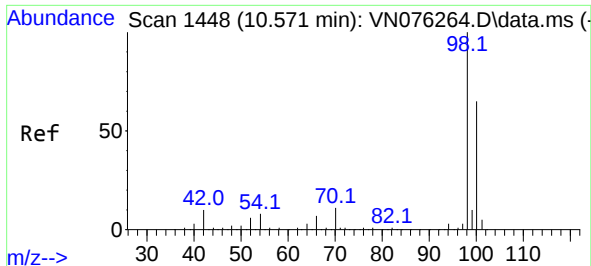

#50
Toluene-d8
Concen: 51.664 ug/l
RT: 10.571 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN076456.D
Acq: 30 Jan 2023 14:53




Instrument :
MSVOA_N
ClientSampleId :
PB150523ZHE#04


Tgt Ion: 98 Resp: 965672
Ion Ratio Lower Upper
98 100
100 65.1 52.2 78.4

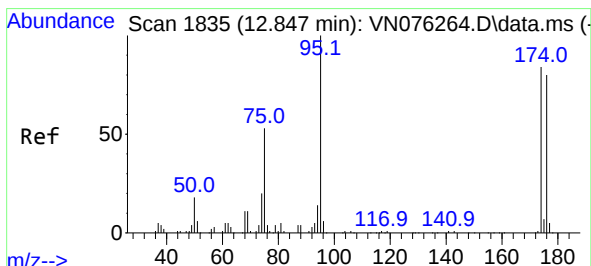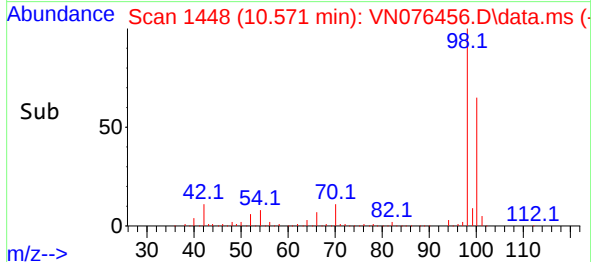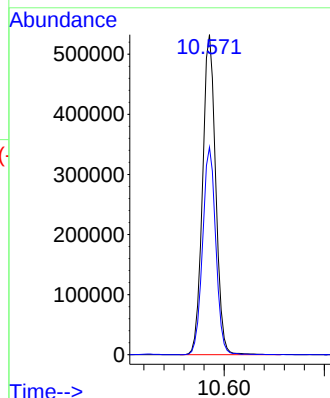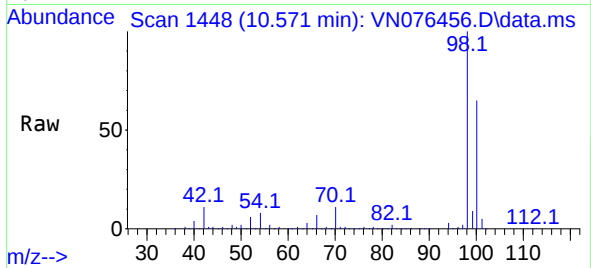

#62
4-Bromofluorobenzene
Concen: 49.460 ug/l
RT: 12.853 min Scan# 1836
Delta R.T. 0.006 min
Lab File: VN076456.D
Acq: 30 Jan 2023 14:53

Tgt Ion: 95 Resp: 301797
Ion Ratio Lower Upper
95 100
174 80.4 0.0 174.6
176 77.1 0.0 167.8


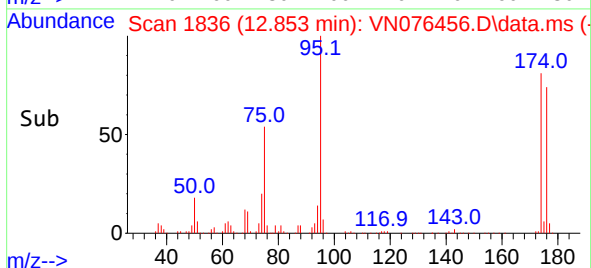
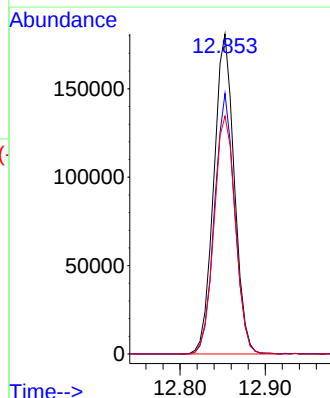
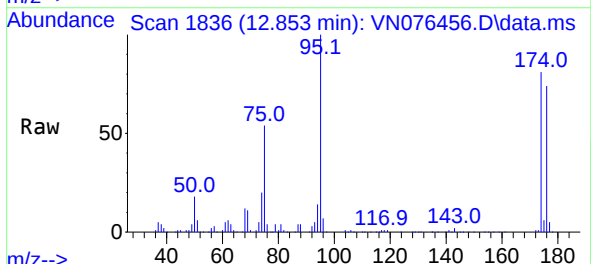


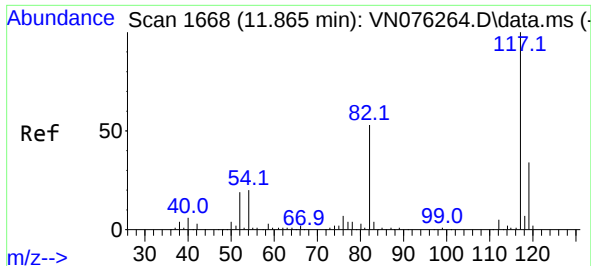

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 11
Delta R.T. 0.005 min
Lab File: VN076456.D
Acq: 30 Jan 2023 14:53

Instrument :
MSVOA_N
ClientSampleId :
PB150523ZHE#04

Tgt Ion:117 Resp: 692319
Ion Ratio Lower Upper
117 100
82 56.1 42.2 63.2
119 33.1 26.9 40.3

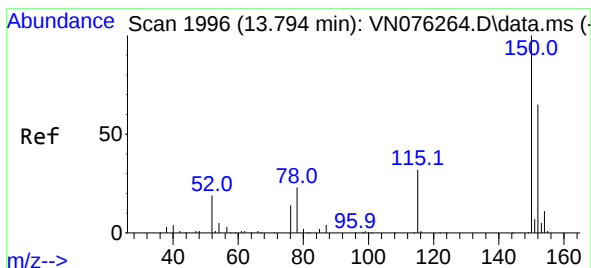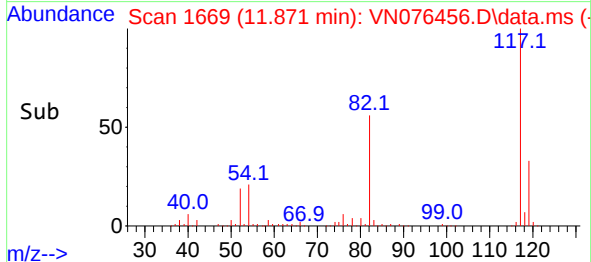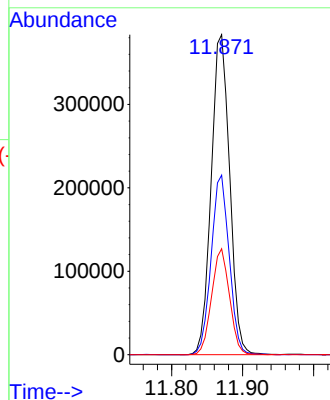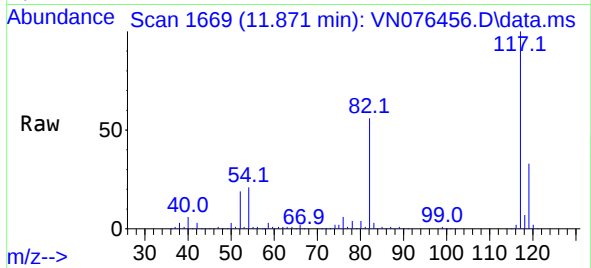

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 1996
Delta R.T. -0.000 min
Lab File: VN076456.D
Acq: 30 Jan 2023 14:53

Tgt Ion:152 Resp: 286625
Ion Ratio Lower Upper
152 100
115 60.4 29.6 88.9
150 157.7 0.0 351.4

