
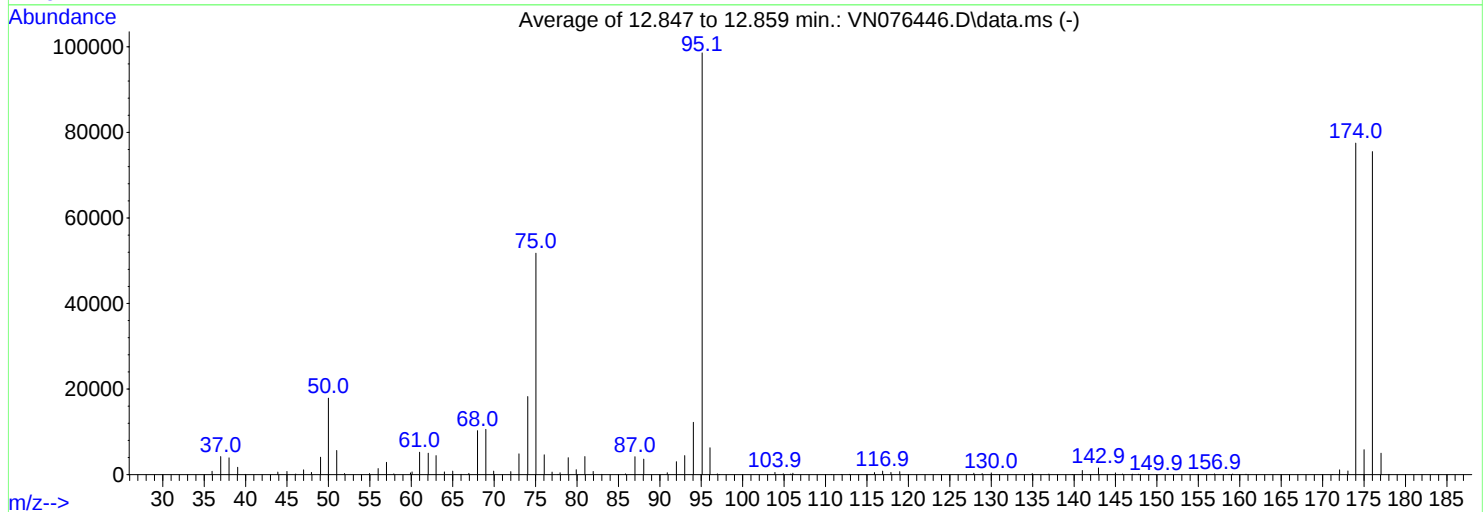


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN013023\
Data File : VN076446.D
Acq On : 30 Jan 2023 09:38
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Title : SW846 8260
Last Update : Tue Jan 17 03:59:22 2023

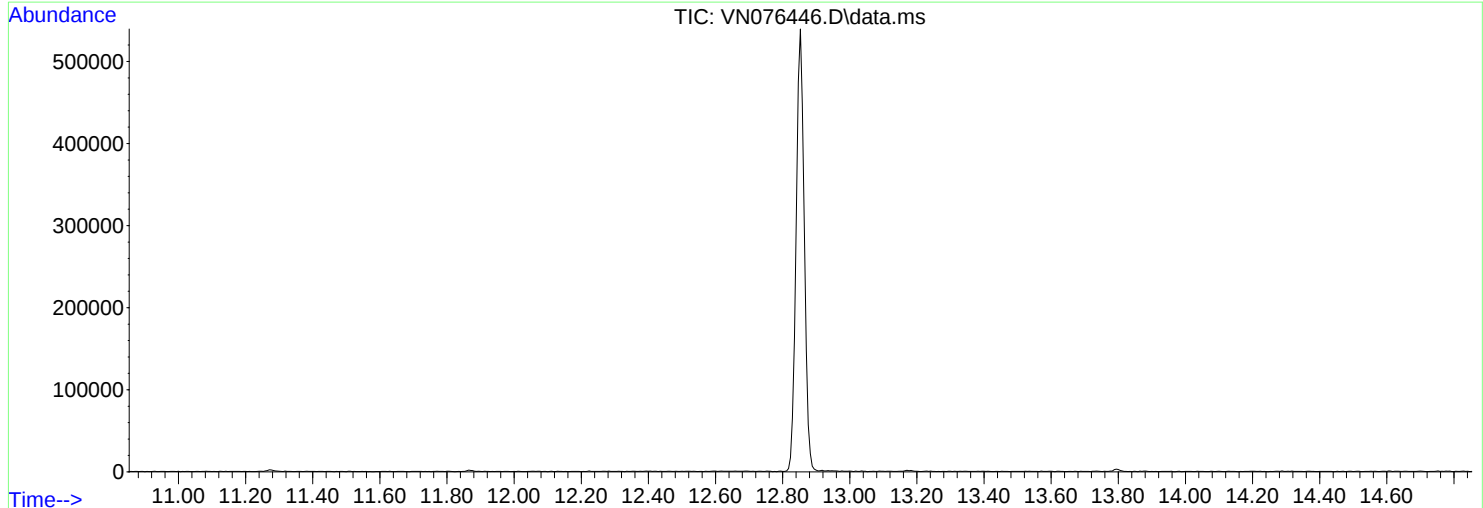

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1826

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.1	17880	PASS
75	95	30	60	52.5	51760	PASS
95	95	100	100	100.0	98592	PASS
96	95	5	9	6.4	6273	PASS
173	174	0.00	2	1.1	878	PASS
174	95	50	100	78.6	77507	PASS
175	174	5	9	7.5	5838	PASS
176	174	95	101	97.4	75493	PASS
177	176	5	9	6.6	5017	PASS

Average of 12.847 to 12.859 min.: VN076446.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	771	50.00	17880	63.00	4453	75.05	5176
37.00	4226	51.00	5664	64.00	653	76.05	4621
38.00	3938	51.95	274	65.00	812	77.00	601
39.05	1723	54.95	264	66.00	64	77.70	71
39.95	82	56.00	1416	66.95	298	77.95	446
43.90	609	57.00	2877	68.00	10304	78.95	3983
45.00	765	57.90	204	69.00	10592	79.90	1157
46.05	171	59.90	421	69.95	819	80.95	4233
47.00	1116	60.10	653	72.00	700	81.95	766
47.95	538	61.00	5254	73.00	4855	83.00	68
49.05	4080	62.05	5029	74.05	18239	85.85	205

Average of 12.847 to 12.859 min.: VN076446.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.00	4185	104.90	228	127.90	336	147.05	131
88.05	3637	105.80	141	128.90	273	147.80	110
90.90	452	106.05	333	130.00	425	148.00	87
92.00	3041	110.70	59	134.95	257	149.90	52
93.00	4454	111.90	53	136.95	171	155.00	63
94.05	12223	112.90	62	139.80	51	156.95	195
95.10	98592	114.90	51	141.00	971	158.70	61
96.05	6273	115.90	502	141.90	58	159.15	141
96.95	173	116.90	825	142.95	1589	160.75	128
97.20	51	117.90	529	145.00	401	171.20	51
103.90	538	118.95	722	145.85	159	172.05	1110

Average of 12.847 to 12.859 min.: VN076446.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
173.05	878						
174.00	77507						
175.00	5838						
176.00	75493						
177.05	5017						
178.00	85						

Instrument :

MSVOA_N

ClientSampleId :

BFB