


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN013024\
Data File : VN080804.D
Acq On : 30 Jan 2024 09:43
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012924W.M
Title : SW846 8260
Last Update : Mon Jan 29 12:54:23 2024

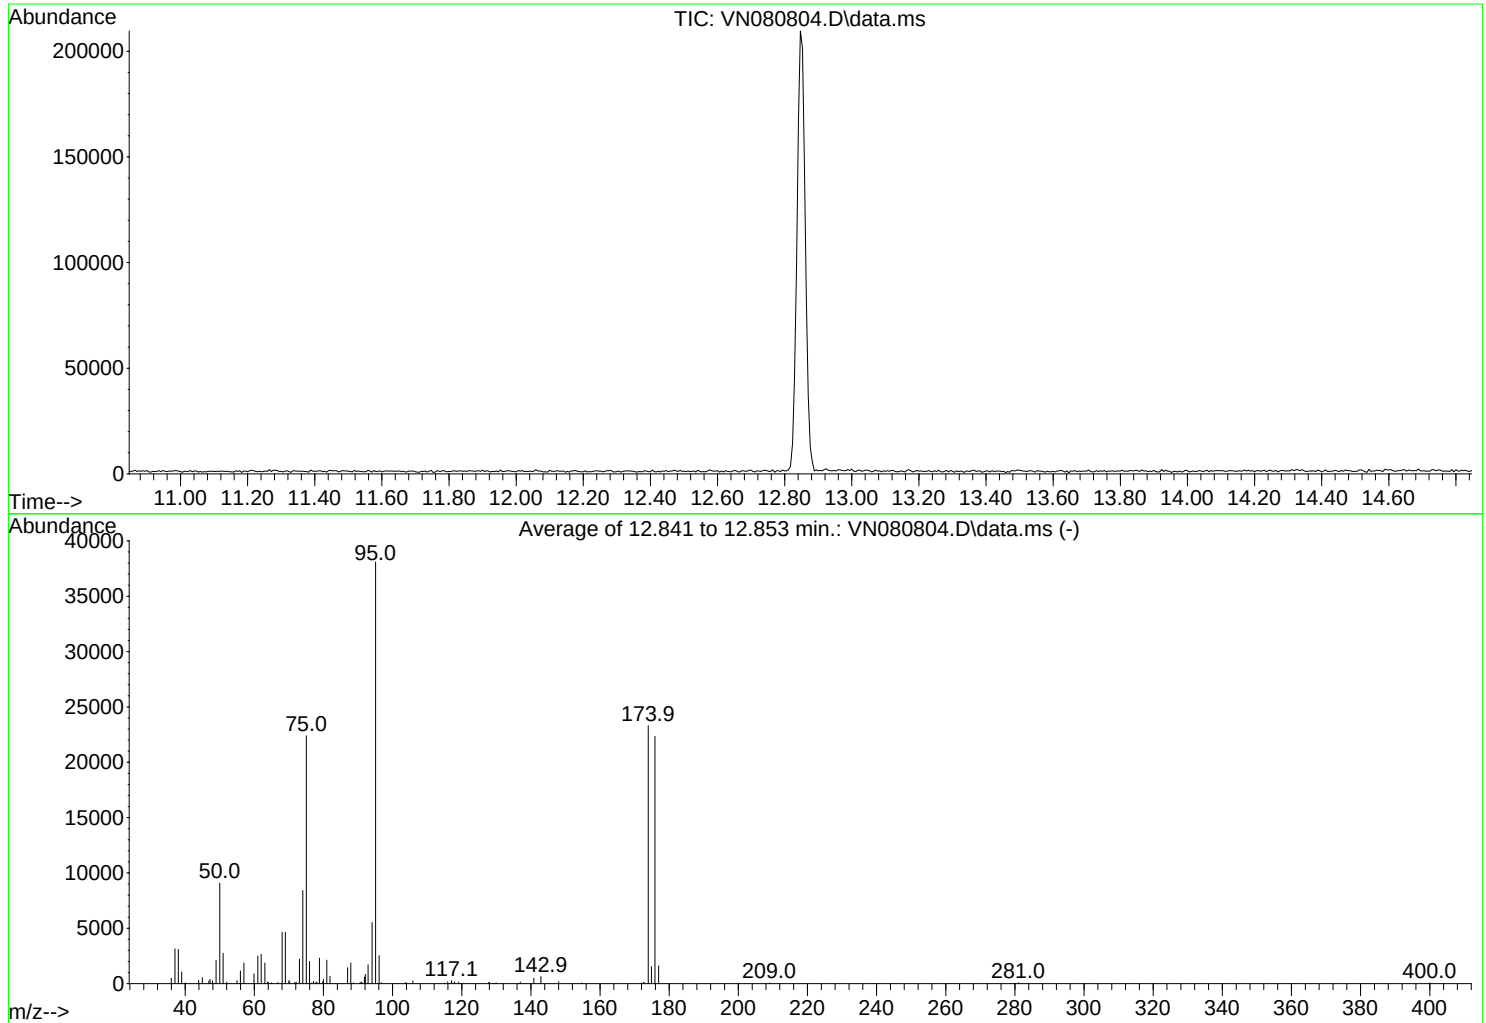

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.8	9083	PASS
75	95	30	60	58.8	22397	PASS
95	95	100	100	100.0	38107	PASS
96	95	5	9	6.6	2528	PASS
173	174	0.00	2	0.3	79	PASS
174	95	50	100	61.1	23301	PASS
175	174	5	9	6.6	1544	PASS
176	174	95	101	95.9	22336	PASS
177	176	5	9	7.2	1603	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	490	50.00	9083	64.10	101	75.05	2239
37.05	3151	50.95	2750	65.00	66	75.95	2011
38.00	3089	52.05	128	66.80	103	76.60	6
39.00	1051	55.00	281	68.05	4640	77.10	19
40.05	72	55.95	1139	68.95	4636	77.70	91
43.90	286	57.00	1866	70.00	280	78.10	163
44.95	538	59.90	885	70.20	183	78.85	2311
46.85	234	61.00	2482	71.75	128	79.80	166
47.15	387	62.00	2643	72.10	116	80.00	391
47.90	255	63.05	1873	73.05	2209	80.95	2121
48.95	2094	63.85	139	74.00	8413	81.90	671

Average of 12.841 to 12.853 min.: VN080804.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.95	1445	96.80	85	129.00	50	174.85	1544
87.90	1865	103.70	83	129.90	74	175.90	22336
88.70	67	103.90	75	136.90	142	176.95	1603
90.65	123	105.85	252	140.85	497	209.00	55
91.10	157	114.90	62	142.90	645	281.00	69
91.85	594	115.95	164	148.00	173	400.00	74
92.10	837	117.05	257	154.70	60		
92.90	1707	117.90	151	171.90	71		
94.05	5526	119.10	127	172.60	121		
95.05	38107	127.80	91	172.90	79		
96.10	2528	128.00	132	173.95	23301		

Instrument :

MSVOA_N

ClientSampleId :

BFB