
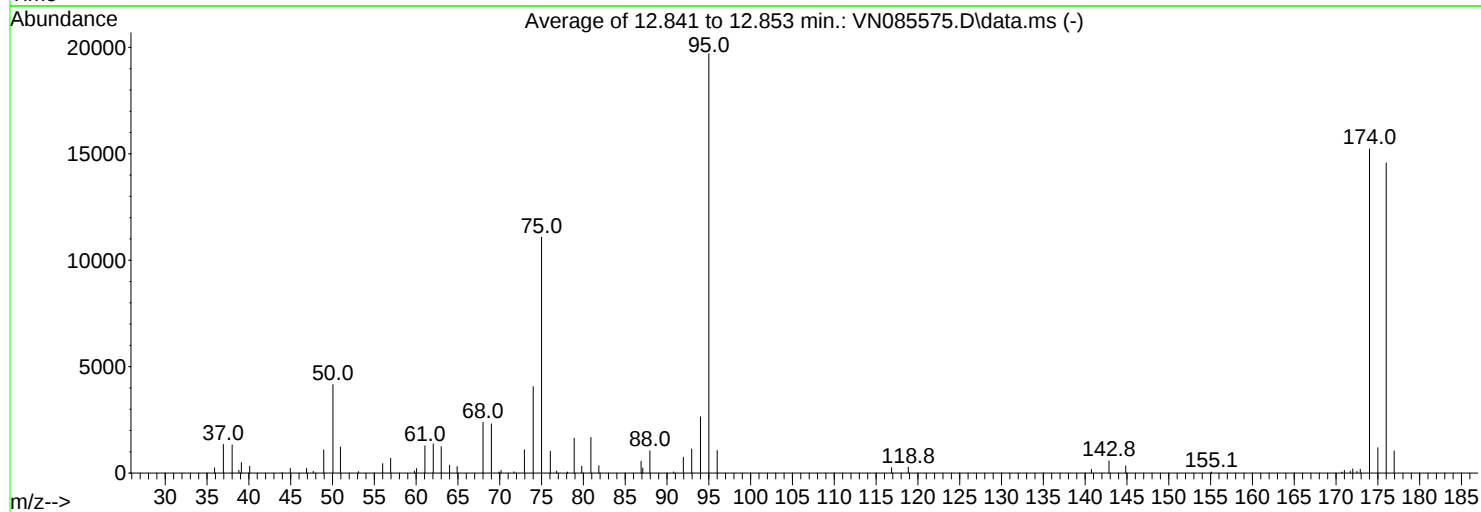


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN013025\
Data File : VN085575.D
Acq On : 30 Jan 2025 12:21
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
Title : SW846 8260
Last Update : Wed Jan 15 02:16:08 2025

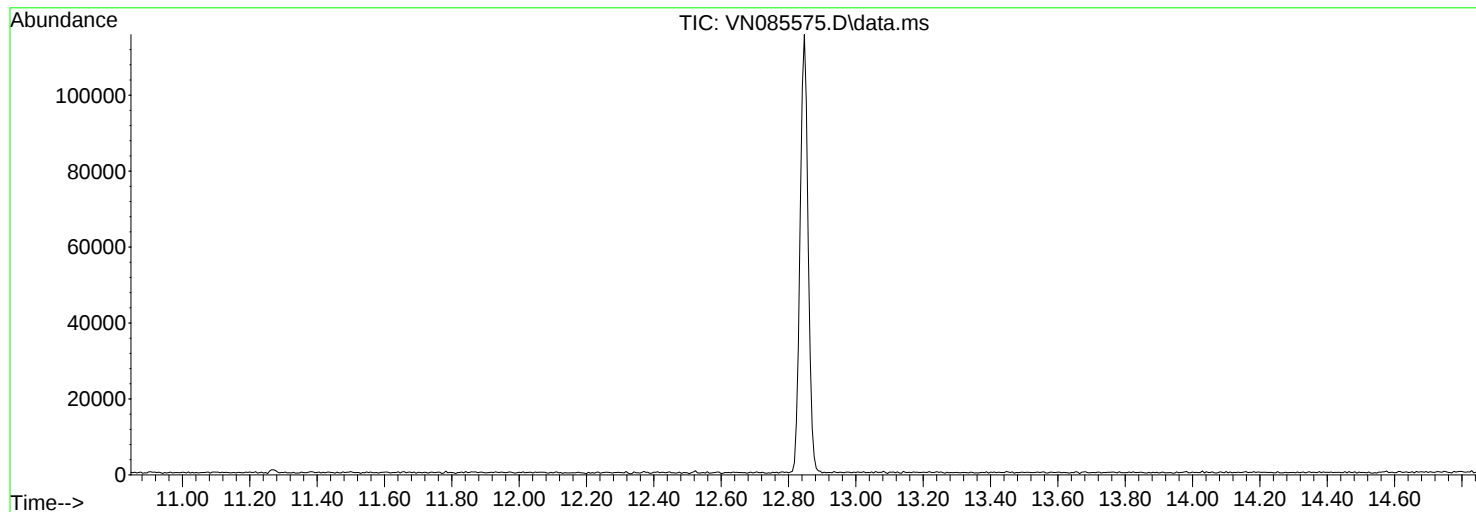

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	4154	PASS
75	95	30	60	56.3	11088	PASS
95	95	100	100	100.0	19701	PASS
96	95	5	9	5.4	1061	PASS
173	174	0.00	2	1.2	180	PASS
174	95	50	100	77.3	15228	PASS
175	174	5	9	7.8	1190	PASS
176	174	95	101	95.7	14566	PASS
177	176	5	9	7.1	1041	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	248	50.05	4154	64.90	307	78.10	53
36.95	1344	50.95	1224	68.00	2383	78.90	1642
38.00	1324	53.10	69	69.00	2313	79.80	322
38.80	132	56.00	445	69.90	52	80.90	1675
39.10	495	56.95	692	70.15	134	81.85	347
40.10	320	59.80	93	71.70	60	86.90	554
43.95	15	60.05	211	72.95	1091	87.10	240
44.95	227	61.05	1278	74.00	4064	87.95	1047
46.90	217	62.05	1373	75.00	11088	90.80	56
47.70	83	63.00	1242	76.05	1027	91.95	747
48.95	1090	64.00	367	76.80	97	92.95	1129

Average of 12.841 to 12.853 min.: VN085575.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.00	2647	171.70	87				
95.00	19701	172.00	201				
96.00	1061	172.50	78				
116.85	260	172.90	180				
118.85	277	174.00	15228				
140.75	178	175.00	1190				
142.85	573	176.00	14566				
144.85	340	176.95	1041				
155.10	52						
170.70	52						
171.00	125						

Instrument :

MSVOA_N

ClientSampleId :

BFB