


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN013120\
 Data File : VN059937.D
 Acq On : 31 Jan 2020 9:09
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N011320W.M
 Title : SW846 8260
 Last Update : Sat Jan 18 03:09:32 2020

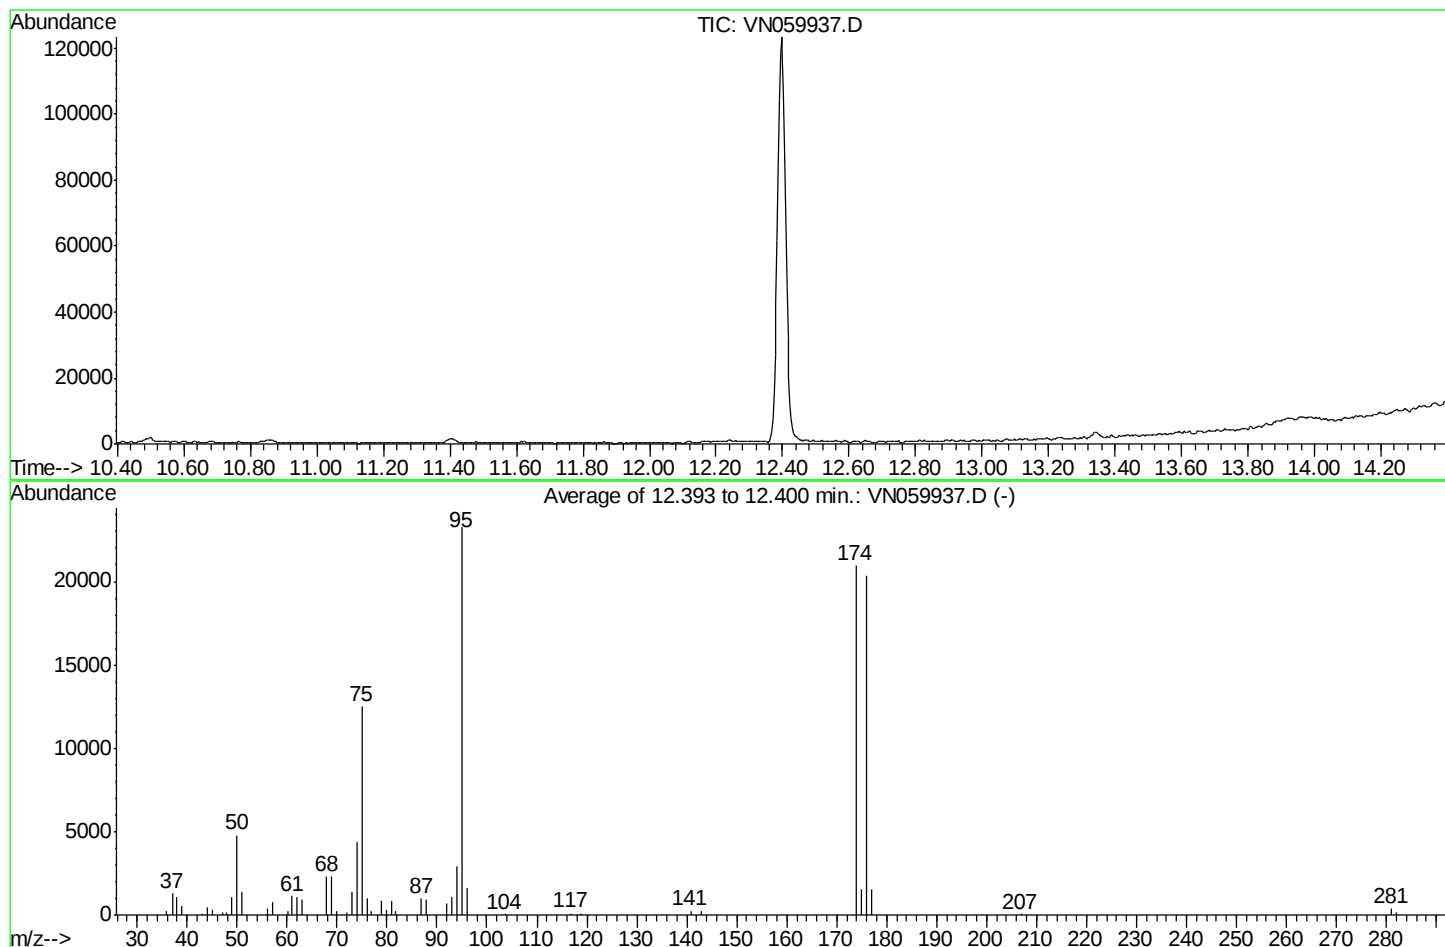

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	4768	PASS
75	95	30	60	53.8	12497	PASS
95	95	100	100	100.0	23250	PASS
96	95	5	9	6.9	1604	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.1	20954	PASS
175	174	5	9	7.2	1506	PASS
176	174	95	101	97.2	20370	PASS
177	176	5	9	7.4	1503	PASS