
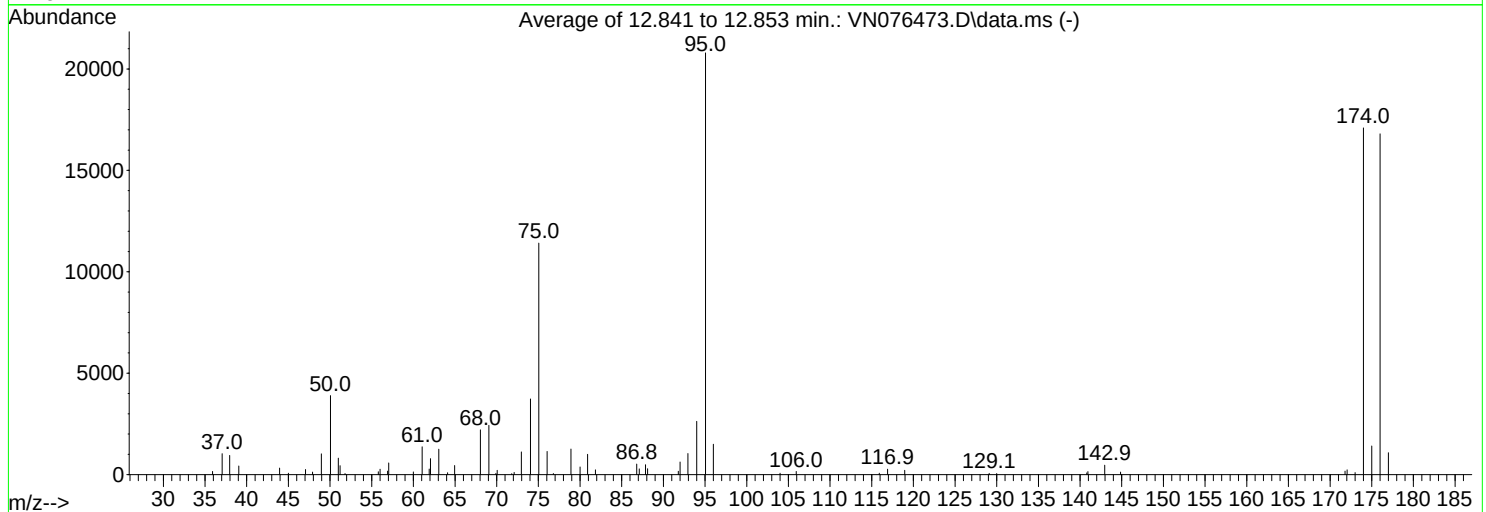


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN013123\
Data File : VN076473.D
Acq On : 31 Jan 2023 08:35
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011623W.M
Title : SW846 8260
Last Update : Tue Jan 17 03:59:22 2023

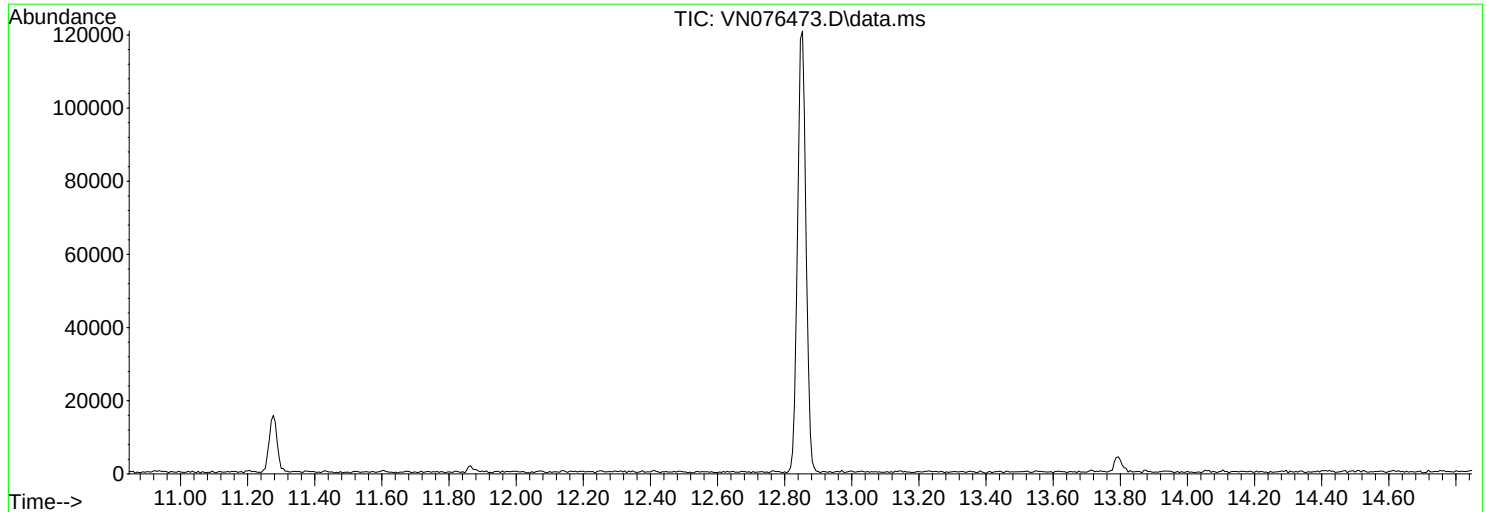

AutoFind: Scans 1834, 1835, 1836; Background Corrected with Scan 1827

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.7	3896	PASS
75	95	30	60	54.9	11416	PASS
95	95	100	100	100.0	20794	PASS
96	95	5	9	7.2	1498	PASS
173	174	0.00	2	0.6	104	PASS
174	95	50	100	82.2	17096	PASS
175	174	5	9	8.3	1416	PASS
176	174	95	101	98.3	16799	PASS
177	176	5	9	6.5	1084	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	156	51.20	440	64.10	95	76.05	114
37.05	1034	51.80	56	64.95	451	76.80	5
37.95	948	55.80	146	68.05	2210	78.90	126
39.05	424	56.00	268	69.05	2426	80.00	38
43.95	320	56.90	177	69.90	62	80.90	999
45.00	71	57.05	577	70.05	210	81.85	240
47.05	249	60.00	137	71.80	51	86.80	524
47.90	129	61.05	1373	72.10	107	87.10	281
48.95	1025	61.90	277	72.95	1122	87.85	492
50.05	3896	62.05	790	74.05	3730	88.10	292
51.00	812	63.05	1256	75.05	11416	91.80	162

Average of 12.841 to 12.853 min.: VN076473.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.00	627	130.00	52	177.00	1084		
92.95	1040	140.80	89				
94.00	2630	140.95	148				
95.05	20794	142.95	465				
96.00	1498	144.85	130				
104.00	69	171.80	175				
105.95	157	172.05	239				
115.90	71	173.00	104				
116.90	268	174.00	17096				
118.95	214	175.00	1416				
129.10	64	176.00	16799				

Instrument :

MSVOA_N

ClientSampleId :

BFB