
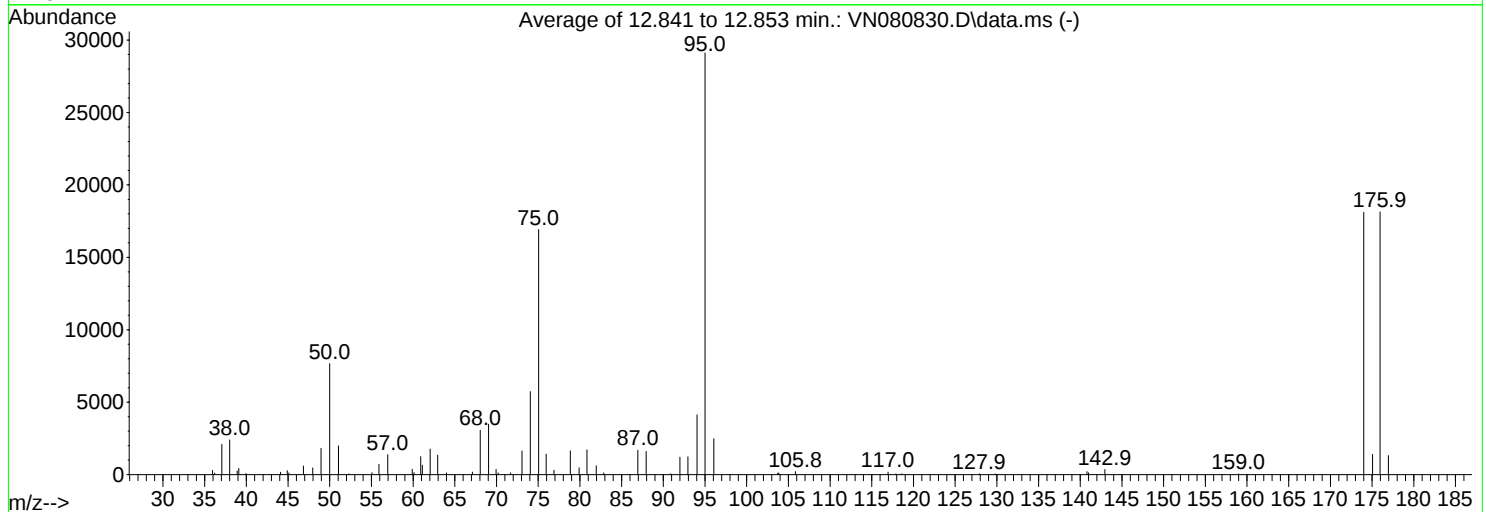


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN013124\
Data File : VN080830.D
Acq On : 31 Jan 2024 10:06
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012924W.M
Title : SW846 8260
Last Update : Mon Jan 29 12:54:23 2024

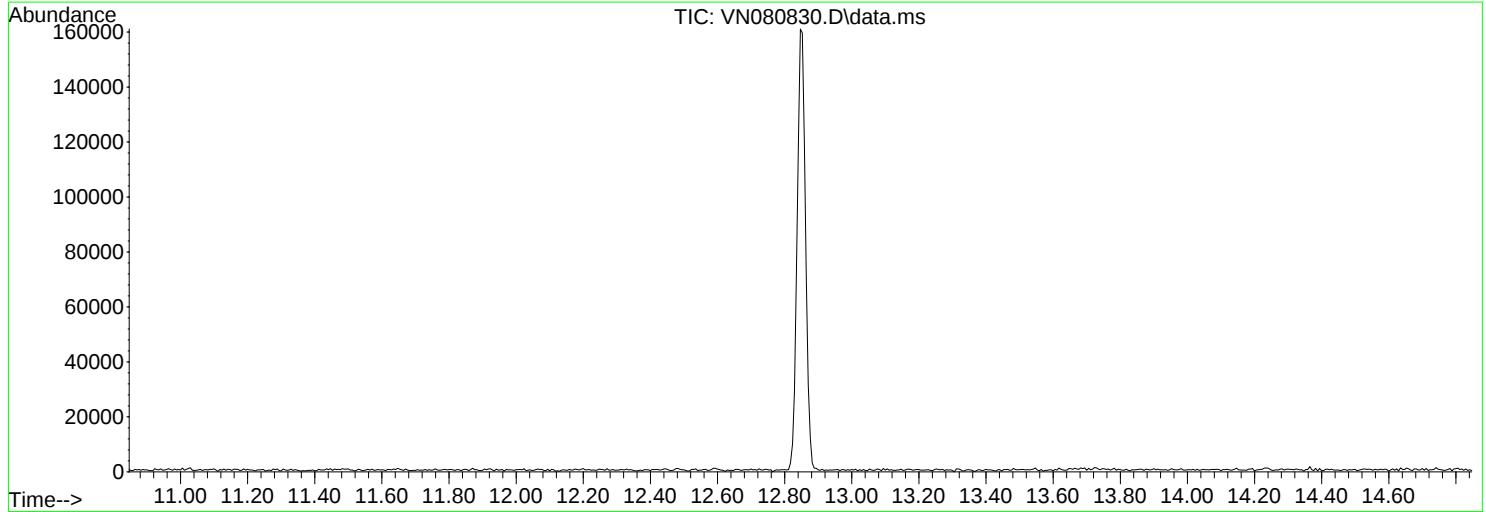

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.3	7665	PASS
75	95	30	60	58.1	16927	PASS
95	95	100	100	100.0	29117	PASS
96	95	5	9	8.5	2480	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	62.2	18112	PASS
175	174	5	9	7.8	1407	PASS
176	174	95	101	100.1	18131	PASS
177	176	5	9	7.3	1318	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	299	47.95	463	61.10	649	74.05	573
36.20	106	48.95	1815	62.05	1766	75.05	1692
37.05	2093	50.00	7665	62.95	1346	75.95	141
38.00	2393	51.05	1987	64.00	119	76.90	30
38.90	257	52.30	59	67.10	177	78.85	1643
39.10	430	55.05	129	68.05	3062	79.90	475
39.95	81	55.90	710	69.05	3484	80.85	1714
44.10	161	56.95	1379	69.95	361	81.95	620
44.90	278	59.90	374	70.20	121	82.85	117
45.10	121	60.10	147	71.70	120	86.95	1685
46.85	599	60.90	1248	73.05	1631	87.95	1605

Average of 12.841 to 12.853 min.: VN080830.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.90	54	118.60	61				
92.00	1207	127.90	59				
92.95	1234	129.80	55				
94.05	4129	140.80	214				
95.00	29117	141.00	135				
96.05	2480	142.95	352				
103.70	90	159.00	54				
103.85	118	174.00	18112				
105.85	206	175.05	1407				
116.95	179	175.95	18131				
117.90	58	176.95	1318				

Instrument :

MSVOA_N

ClientSampleId :

BFB